
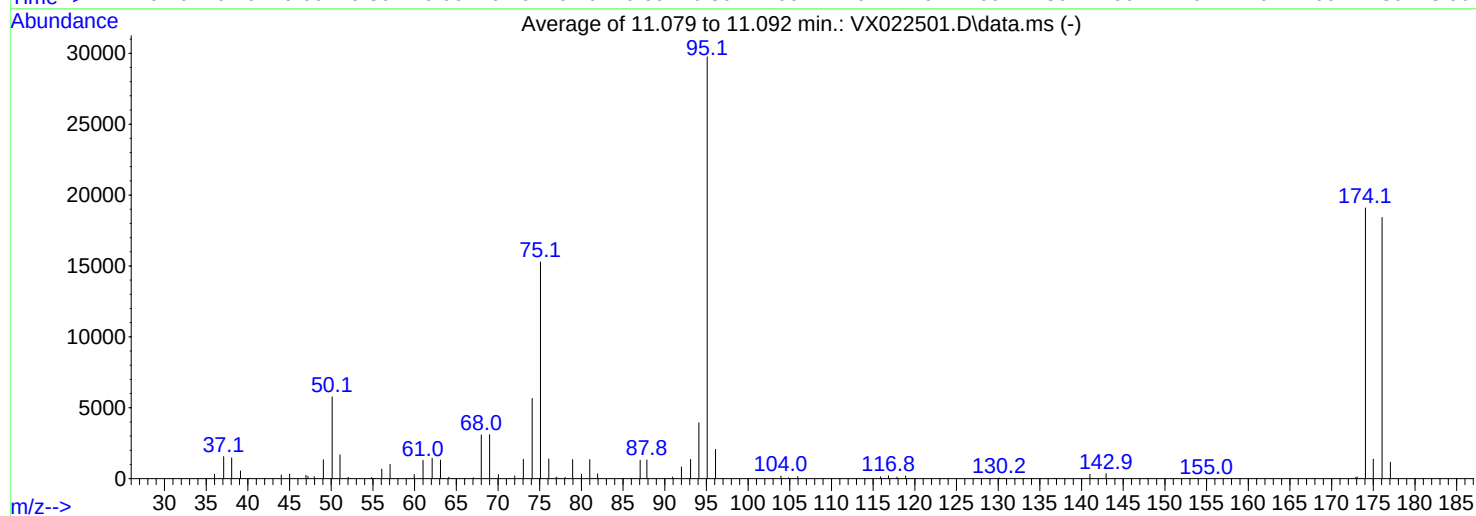


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060621\
 Data File : VX022501.D
 Acq On : 07 Jun 2021 00:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Title : SW846 8260
 Last Update : Wed May 19 14:23:10 2021

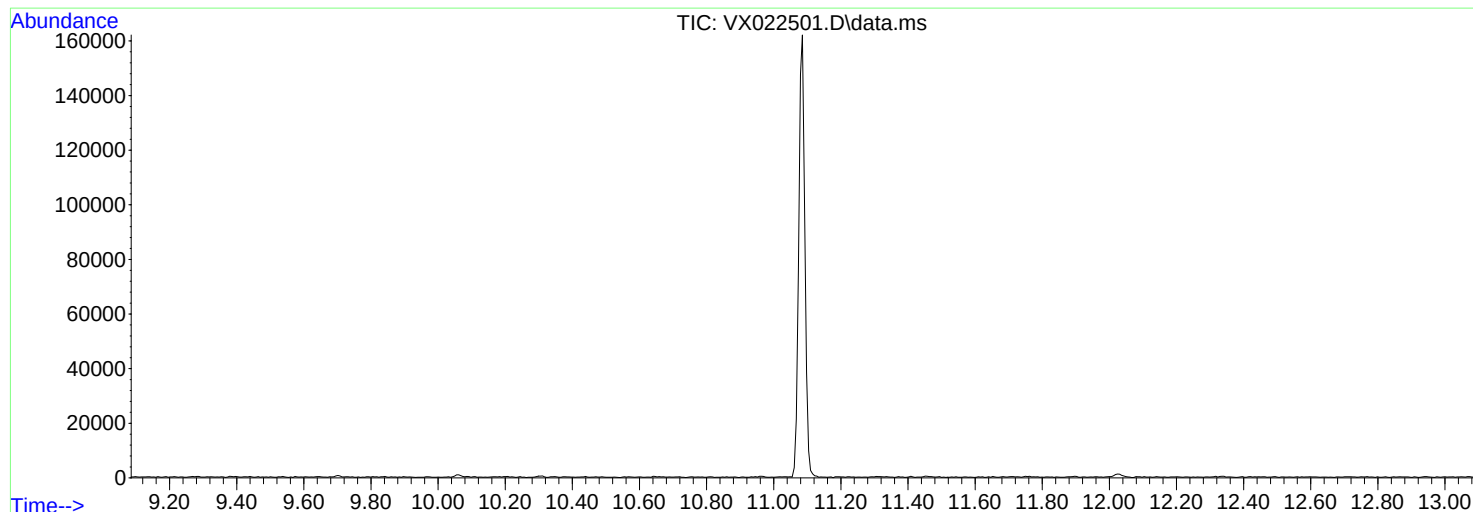

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	5764	PASS
75	95	30	60	51.4	15278	PASS
95	95	100	100	100.0	29749	PASS
96	95	5	9	6.9	2064	PASS
173	174	0.00	2	0.6	120	PASS
174	95	50	100	64.2	19095	PASS
175	174	5	9	7.2	1381	PASS
176	174	95	101	96.4	18416	PASS
177	176	5	9	6.3	1153	PASS