

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
 Data File : VX029232.D
 Acq On : 06 Jun 2022 12:23
 Operator : JC/MD
 Sample : VX0606WBS01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0606WBS01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
 Title : SW846 8260

Signal : TIC: VX029232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	10	13	20	rVB	106532	93006	3.83%	0.223%
2	1.288	30	33	43	rVB	94869	103481	4.26%	0.248%
3	1.374	43	47	51	rBV	95335	91941	3.79%	0.220%
4	1.605	79	85	94	rVB	80323	87355	3.60%	0.209%
5	1.685	94	98	106	rVB	59578	69211	2.85%	0.166%
6	1.886	126	131	140	rVB	141007	197776	8.15%	0.474%
7	2.130	165	171	183	rVB	91527	138595	5.71%	0.332%
8	2.233	183	188	196	rVB	38831	60232	2.48%	0.144%
9	2.325	196	203	208	rBV2	257673	483689	19.92%	1.160%
10	2.380	208	212	219	rVV	131552	221262	9.11%	0.530%
11	2.453	219	224	229	rVV	57635	94999	3.91%	0.228%
12	2.514	229	234	248	rVB	100963	158521	6.53%	0.380%
13	2.666	250	259	262	rBV2	123235	224903	9.26%	0.539%
14	2.703	262	265	272	rVV	68355	117835	4.85%	0.282%
15	2.788	272	279	293	rVB	132169	239125	9.85%	0.573%
16	2.971	299	309	318	rBV2	41969	135952	5.60%	0.326%
17	3.062	318	324	327	rBV	216014	425385	17.52%	1.020%
18	3.611	404	414	424	rBV2	90996	219297	9.03%	0.526%
19	3.721	424	432	459	rVB2	391082	1287872	53.04%	3.088%
20	4.483	541	557	564	rBV3	179533	545917	22.48%	1.309%
21	4.556	564	569	577	rVB	114100	279131	11.50%	0.669%
22	4.647	577	584	590	rBV2	75556	194366	8.01%	0.466%
23	4.721	590	596	597	rBV2	26714	43233	1.78%	0.104%
24	4.910	614	627	636	rBV4	111746	384862	15.85%	0.923%
25	5.007	636	643	651	rVV2	159844	487501	20.08%	1.169%
26	5.092	651	657	671	rVB2	90713	277225	11.42%	0.665%
27	5.385	693	705	713	rBV2	262435	789131	32.50%	1.892%
28	5.470	713	719	725	rVB2	92725	216323	8.91%	0.519%
29	5.550	725	732	739	rBV	244427	638904	26.31%	1.532%
30	5.690	747	755	768	rVB3	180649	568863	23.43%	1.364%
31	5.958	788	799	806	rBV	185728	483002	19.89%	1.158%
32	6.043	806	813	819	rBV	165642	441338	18.18%	1.058%
33	6.342	852	862	875	rBV	96118	246390	10.15%	0.591%
34	6.763	920	931	944	rBV	433647	1030108	42.43%	2.470%
35	7.129	983	991	1000	rBV	162761	356977	14.70%	0.856%
36	7.379	1023	1032	1037	rBV	209210	470504	19.38%	1.128%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
 Data File : VX029232.D
 Acq On : 06 Jun 2022 12:23
 Operator : JC/MD
 Sample : VX0606WBS01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0606WBS01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
 Title : SW846 8260

37	7.434	1037	1041	1051	rVB	139861	280050	11.53%	0.671%
38	7.586	1058	1066	1074	rBV	104005	207442	8.54%	0.497%
39	7.696	1074	1084	1095	rVB2	145929	325248	13.40%	0.780%
40	7.818	1095	1104	1112	rBV2	159606	445360	18.34%	1.068%
41	8.116	1146	1153	1163	rBV2	29708	52161	2.15%	0.125%
42	8.244	1167	1174	1185	rVV	543223	863261	35.56%	2.070%
43	8.366	1187	1194	1207	rVB	173518	278992	11.49%	0.669%
44	8.574	1221	1228	1235	rBV	800651	1229509	50.64%	2.948%
45	8.647	1235	1240	1247	rVV	896538	1442239	59.40%	3.458%
46	8.720	1247	1252	1262	rVB	418465	630415	25.96%	1.511%
47	8.982	1286	1295	1306	rBV	165569	253553	10.44%	0.608%
48	9.116	1311	1317	1320	rBV	205619	293062	12.07%	0.703%
49	9.153	1320	1323	1333	rVB	234565	337410	13.90%	0.809%
50	9.275	1336	1343	1346	rBV	325214	475152	19.57%	1.139%
51	9.311	1346	1349	1355	rVB	208278	279779	11.52%	0.671%
52	9.433	1363	1369	1378	rBV	683112	912482	37.58%	2.188%
53	9.525	1378	1384	1389	rVV	140842	208123	8.57%	0.499%
54	9.579	1389	1393	1396	rVV	212433	287538	11.84%	0.689%
55	9.610	1396	1398	1405	rVB	126947	157871	6.50%	0.378%
56	10.055	1465	1471	1483	rBV2	914365	1711159	70.48%	4.102%
57	10.165	1483	1489	1491	rVV	282451	389108	16.03%	0.933%
58	10.195	1491	1494	1505	rVV	517288	657910	27.10%	1.577%
59	10.305	1505	1512	1525	rVB	938001	1330896	54.82%	3.191%
60	10.652	1561	1569	1579	rBV2	709266	1249134	51.45%	2.995%
61	10.799	1588	1593	1597	rBV	119486	160976	6.63%	0.386%
62	10.841	1597	1600	1609	rVB	243882	309284	12.74%	0.741%
63	10.963	1614	1620	1625	rVV	576540	717780	29.56%	1.721%
64	11.018	1625	1629	1634	rVV	155044	197060	8.12%	0.472%
65	11.079	1634	1639	1651	rVV	731326	954361	39.31%	2.288%
66	11.201	1653	1659	1663	rVV2	381675	736729	30.34%	1.766%
67	11.238	1663	1665	1672	rVV2	257221	478665	19.71%	1.148%
68	11.305	1672	1676	1681	rVV	585334	694874	28.62%	1.666%
69	11.366	1681	1686	1691	rVV	477009	587129	24.18%	1.408%
70	11.451	1695	1700	1711	rVB	970726	1280230	52.73%	3.069%
71	11.719	1738	1744	1747	rBV2	719208	1052951	43.37%	2.524%
72	11.750	1747	1749	1756	rVB	557965	660173	27.19%	1.583%
73	11.890	1764	1772	1778	rBV	572706	698888	28.79%	1.675%
74	11.969	1780	1785	1788	rVV	424515	515186	21.22%	1.235%
75	12.018	1788	1793	1805	rVB4	1212825	2427949	100.00%	5.821%
76	12.335	1839	1845	1860	rBV	934060	1123290	46.26%	2.693%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
Data File : VX029232.D
Acq On : 06 Jun 2022 12:23
Operator : JC/MD
Sample : VX0606WBS01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0606WBS01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

77	12.542	1872	1879	1884	rBV	269987	351091	14.46%	0.842%
78	12.945	1933	1945	1957	rVB2	112521	160540	6.61%	0.385%
79	13.286	1996	2001	2010	rVB	552864	649662	26.76%	1.557%
80	13.591	2045	2051	2061	rVB	332140	431415	17.77%	1.034%
81	13.725	2067	2073	2077	rBV	247278	303325	12.49%	0.727%
82	13.774	2077	2081	2092	rVB	460700	579006	23.85%	1.388%
83	13.963	2106	2112	2119	rVB	350506	439641	18.11%	1.054%




Sum of corrected areas: 41712271

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
Data File : VX029232.D
Acq On : 06 Jun 2022 12:23
Operator : JC/MD
Sample : VX0606WBS01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0606WBS01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

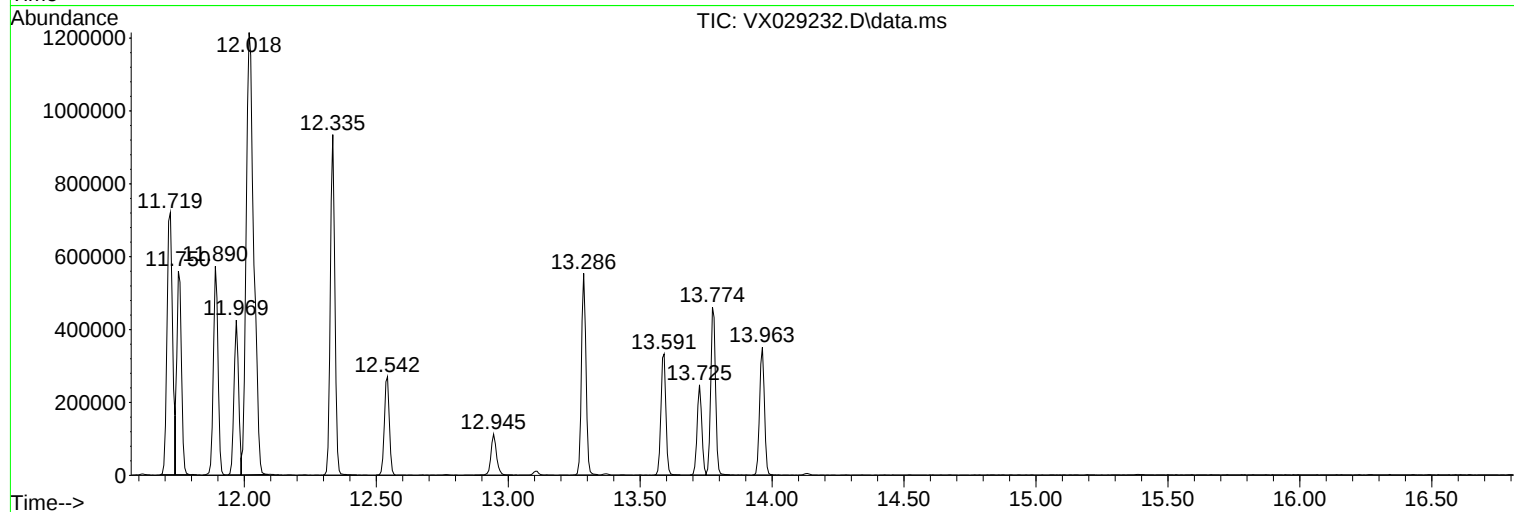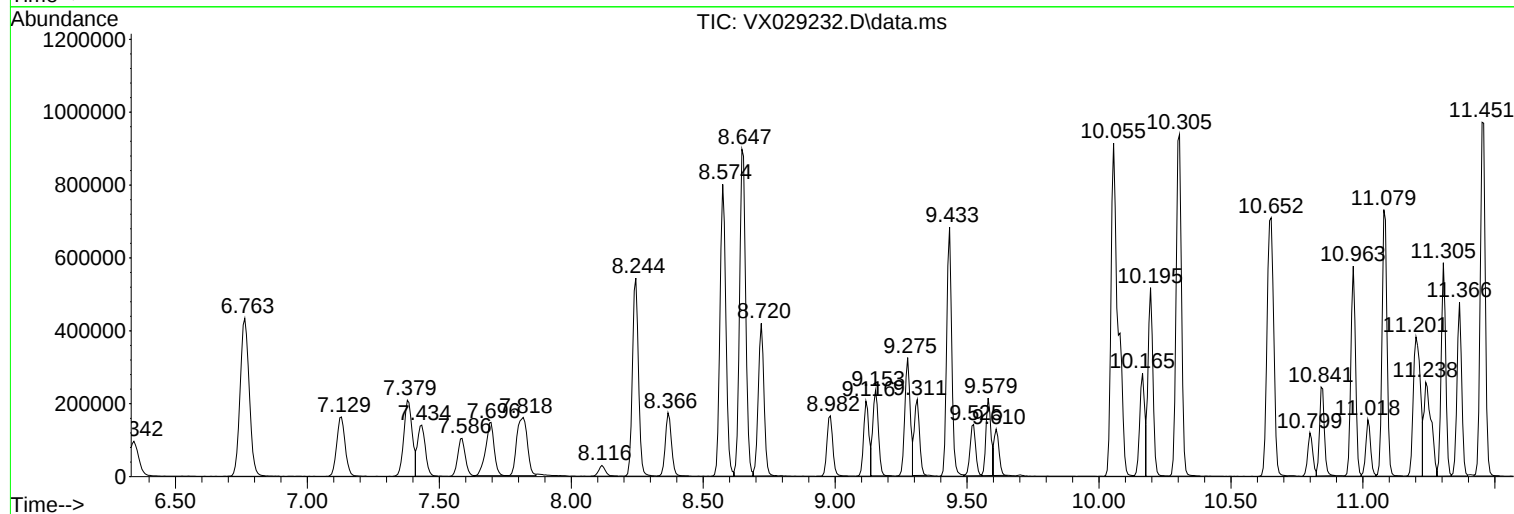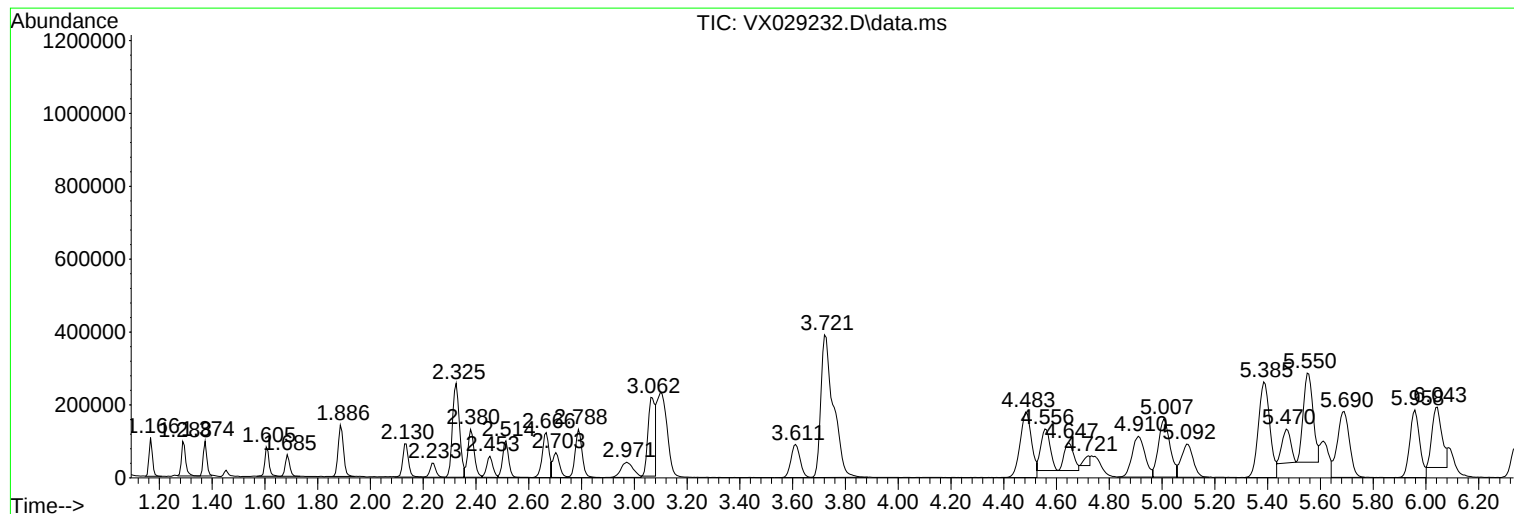

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
Data File : VX029232.D
Acq On : 06 Jun 2022 12:23
Operator : JC/MD
Sample : VX0606WBS01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0606WBS01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
Data File : VX029232.D
Acq On : 06 Jun 2022 12:23
Operator : JC/MD
Sample : VX0606WBS01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0606WBS01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc