

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
 Data File : VX029245.D
 Acq On : 06 Jun 2022 17:54
 Operator : JC/MD
 Sample : N3160-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	14	rVB	94349	79051	4.50%	0.768%
2	1.264	25	29	41	rBV3	22409	36173	2.06%	0.351%
3	1.368	41	46	53	rVB2	30118	44194	2.52%	0.429%
4	2.386	206	213	220	rVB	11306	20130	1.15%	0.195%
5	2.544	230	239	247	rBV	16530	34123	1.94%	0.331%
6	2.947	296	305	314	rBV	29954	71715	4.09%	0.696%
7	4.581	562	573	585	rBV2	13007	42691	2.43%	0.415%
8	5.099	646	658	675	rBV	97091	292855	16.69%	2.844%
9	5.391	693	706	722	rBV	212355	620422	35.35%	6.024%
10	5.556	722	733	748	rVB	330029	924150	52.66%	8.974%
11	5.958	789	799	821	rBV	215478	585948	33.39%	5.690%
12	6.763	921	931	946	rBV	544795	1290497	73.53%	12.531%
13	8.653	1233	1241	1248	rBV	1141688	1755004	100.00%	17.041%
14	10.055	1465	1471	1482	rBV	1218375	1615206	92.03%	15.684%
15	11.086	1634	1640	1654	rBV	950466	1255319	71.53%	12.189%
16	12.024	1788	1794	1803	rBV	1348124	1597488	91.02%	15.512%
17	12.853	1926	1930	1938	rBV	24032	33594	1.91%	0.326%




Sum of corrected areas: 10298560

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
Data File : VX029245.D
Acq On : 06 Jun 2022 17:54
Operator : JC/MD
Sample : N3160-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

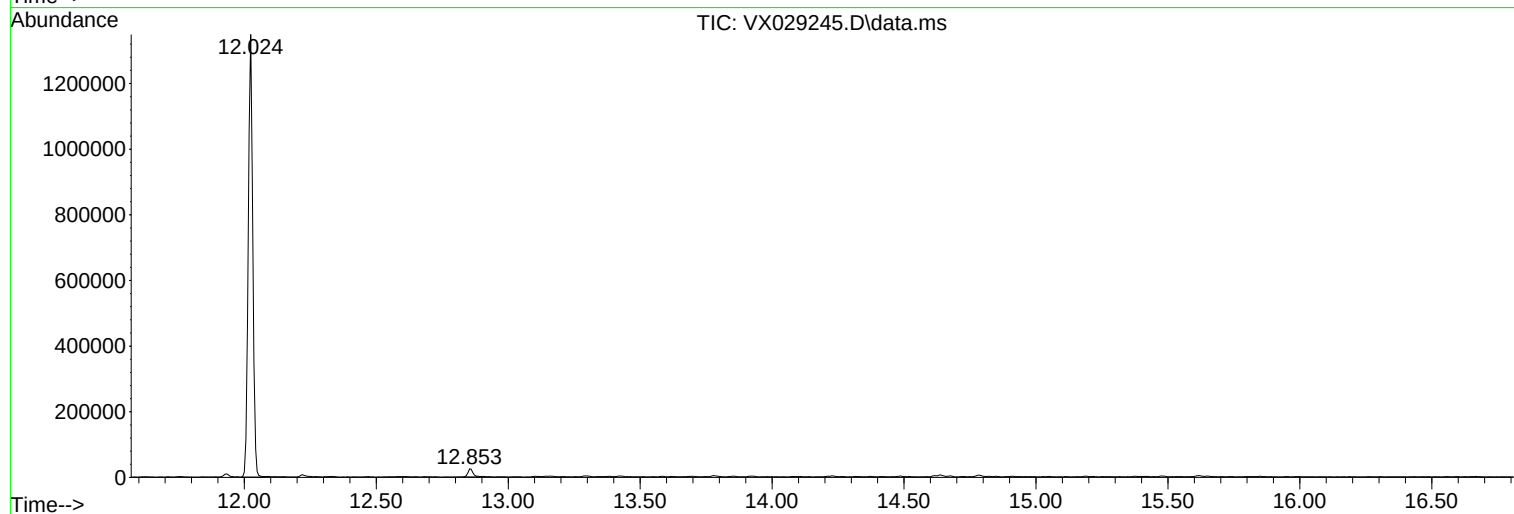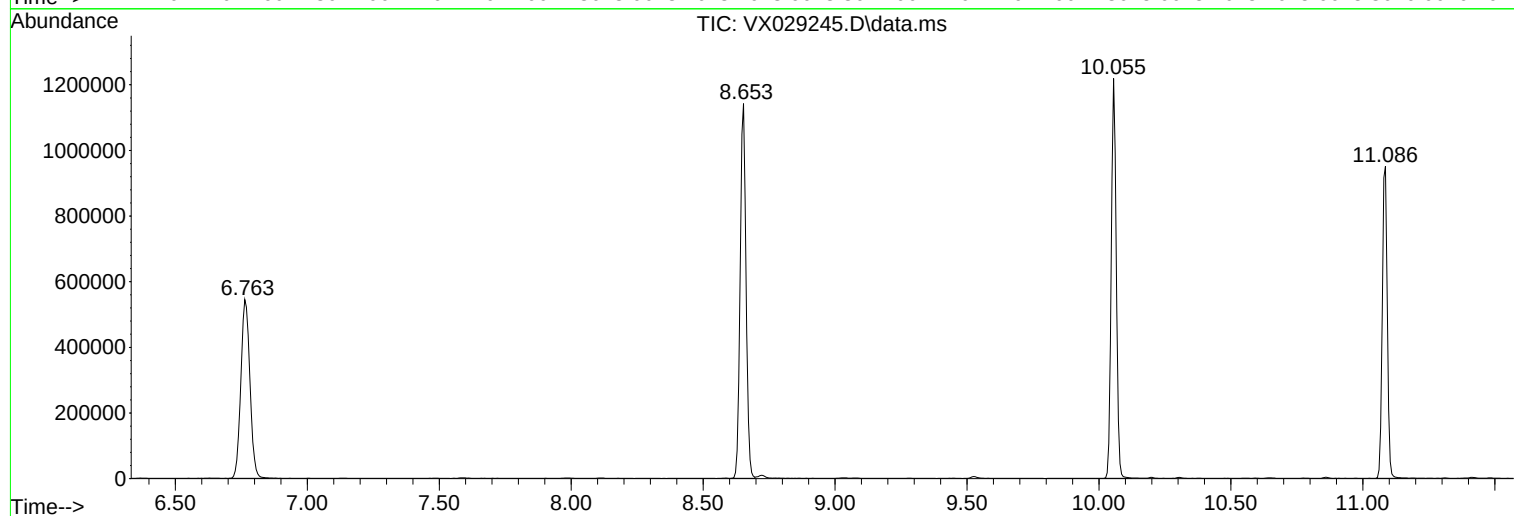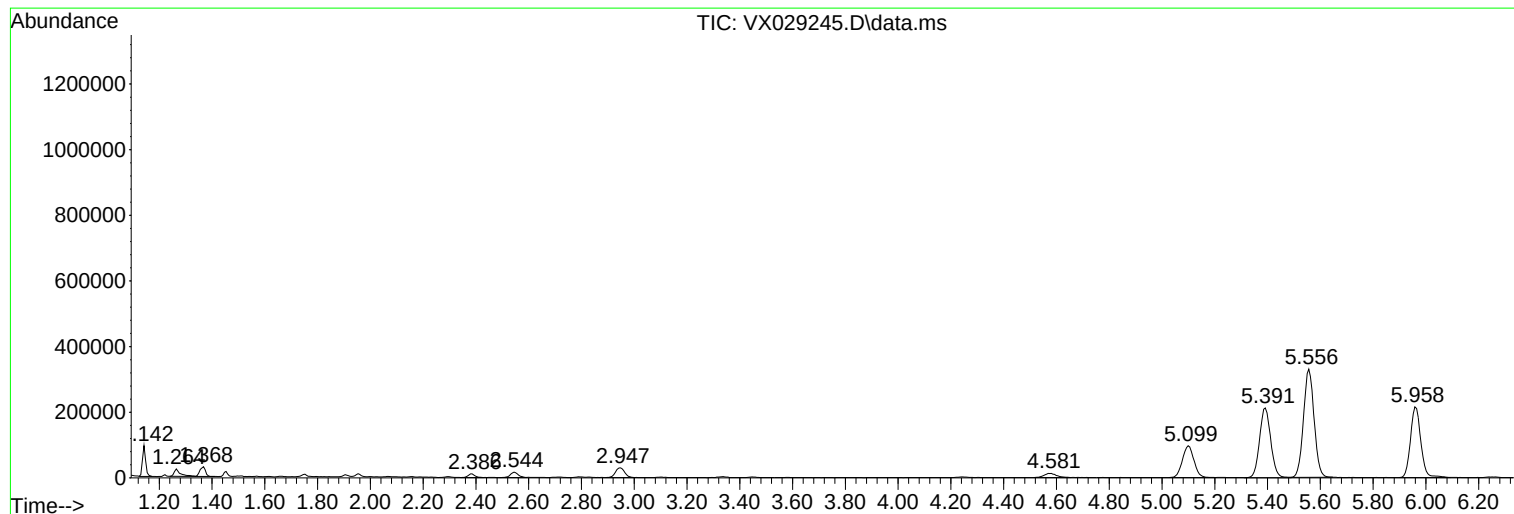

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
Data File : VX029245.D
Acq On : 06 Jun 2022 17:54
Operator : JC/MD
Sample : N3160-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060622\
Data File : VX029245.D
Acq On : 06 Jun 2022 17:54
Operator : JC/MD
Sample : N3160-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc