

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036028.D
 Acq On : 06 Jun 2023 13:27
 Operator : JC/MD
 Sample : 02991-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	7943	8489	0.73%	0.097%
2	1.264	26	29	31	rBV2	2301	2055	0.18%	0.024%
3	1.368	42	46	57	rBV	119255	150548	12.98%	1.727%
4	1.672	91	96	114	rBV	85537	146121	12.60%	1.676%
5	2.306	193	200	210	rBV	252804	391998	33.79%	4.497%
6	2.398	211	215	224	rVB3	2883	5551	0.48%	0.064%
7	2.471	224	227	228	rBV	557	348	0.03%	0.004%
8	2.508	230	233	237	rBV2	1488	2152	0.19%	0.025%
9	2.660	256	258	261	rBV	461	485	0.04%	0.006%
10	2.831	284	286	289	rBV	270	263	0.02%	0.003%
11	2.928	300	302	307	rVB2	300	454	0.04%	0.005%
12	3.087	325	328	333	rVB4	854	1304	0.11%	0.015%
13	3.227	348	351	353	rBV	277	252	0.02%	0.003%
14	3.264	353	357	359	rBV2	149	223	0.02%	0.003%
15	3.312	361	365	367	rBV	314	343	0.03%	0.004%
16	3.800	444	445	447	rBV	218	208	0.02%	0.002%
17	3.861	451	455	457	rVB	234	327	0.03%	0.004%
18	3.892	457	460	462	rBV2	257	280	0.02%	0.003%
19	4.001	475	478	479	rVB	301	266	0.02%	0.003%
20	4.020	479	481	485	rBV	280	225	0.02%	0.003%
21	4.074	488	490	495	rVB	325	332	0.03%	0.004%
22	4.343	531	534	535	rBV2	209	226	0.02%	0.003%
23	4.458	544	553	571	rBV	88907	271985	23.45%	3.120%
24	4.916	624	628	631	rBV2	232	347	0.03%	0.004%
25	5.056	637	651	668	rBV	142585	457217	39.41%	5.245%
26	5.214	675	677	682	rVB3	351	367	0.03%	0.004%
27	5.257	682	684	688	rVB2	190	236	0.02%	0.003%
28	5.385	699	705	710	rVB5	585	1448	0.12%	0.017%
29	5.964	787	800	816	rBV3	391766	1160081	100.00%	13.309%
30	6.141	827	829	832	rBV3	369	387	0.03%	0.004%
31	6.330	855	860	863	rBV2	190	343	0.03%	0.004%
32	6.757	920	930	942	rBV	287125	682367	58.82%	7.828%
33	7.123	983	990	995	rVB7	1817	4083	0.35%	0.047%
34	7.184	998	1000	1005	rBV2	230	289	0.02%	0.003%
35	7.306	1011	1020	1036	rBV	246705	538337	46.41%	6.176%
36	7.476	1044	1048	1052	rBV2	559	979	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036028.D
 Acq On : 06 Jun 2023 13:27
 Operator : JC/MD
 Sample : 02991-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.763	1092	1095	1096	rBV3	233	249	0.02%	0.003%
38	7.812	1100	1103	1105	rBV2	193	256	0.02%	0.003%
39	7.891	1112	1116	1119	rVB	194	234	0.02%	0.003%
40	7.927	1119	1122	1124	rBV3	426	574	0.05%	0.007%
41	8.324	1180	1187	1196	rBV	158483	253987	21.89%	2.914%
42	8.470	1209	1211	1217	rVB3	697	988	0.09%	0.011%
43	8.513	1217	1218	1220	rBV2	379	259	0.02%	0.003%
44	8.647	1233	1240	1249	rBV	595900	912121	78.63%	10.464%
45	8.878	1275	1278	1280	rBV2	341	433	0.04%	0.005%
46	8.945	1283	1289	1297	rBV	110335	169740	14.63%	1.947%
47	9.147	1321	1322	1326	rVB2	366	270	0.02%	0.003%
48	9.275	1339	1343	1349	rVB2	2708	3864	0.33%	0.044%
49	9.384	1355	1361	1378	rBV	404335	576942	49.73%	6.619%
50	9.519	1381	1383	1389	rVB4	1337	2083	0.18%	0.024%
51	9.890	1442	1444	1447	rVB2	280	247	0.02%	0.003%
52	10.055	1465	1471	1486	rVV	577351	813485	70.12%	9.332%
53	10.189	1491	1493	1499	rVV2	1182	1619	0.14%	0.019%
54	10.305	1508	1512	1515	rVB2	1299	1537	0.13%	0.018%
55	10.518	1543	1547	1549	rVV2	210	225	0.02%	0.003%
56	10.598	1557	1560	1562	rVB2	334	303	0.03%	0.003%
57	10.659	1564	1570	1573	rVB3	1098	1687	0.15%	0.019%
58	10.805	1591	1594	1597	rBV2	360	530	0.05%	0.006%
59	10.927	1611	1614	1615	rBV2	319	319	0.03%	0.004%
60	10.963	1617	1620	1624	rVB	626	792	0.07%	0.009%
61	11.018	1627	1629	1632	rVB2	274	228	0.02%	0.003%
62	11.085	1637	1640	1644	rVB	953	921	0.08%	0.011%
63	11.189	1652	1657	1668	rBV	431604	552023	47.58%	6.333%
64	11.305	1673	1676	1680	rBV3	579	823	0.07%	0.009%
65	11.451	1696	1700	1705	rVV2	810	1063	0.09%	0.012%
66	11.506	1708	1709	1712	rVV2	240	209	0.02%	0.002%
67	11.677	1735	1737	1740	rBV	305	429	0.04%	0.005%
68	11.707	1740	1742	1746	rVV2	281	330	0.03%	0.004%
69	11.756	1746	1750	1754	rVB4	1009	1325	0.11%	0.015%
70	11.927	1776	1778	1781	rBV	183	230	0.02%	0.003%
71	11.969	1782	1785	1788	rVV	1219	1377	0.12%	0.016%
72	12.018	1788	1793	1802	rVV	599156	778035	67.07%	8.926%
73	12.171	1816	1818	1820	rVB2	332	217	0.02%	0.002%
74	12.225	1823	1827	1831	rVB3	693	1088	0.09%	0.012%
75	12.317	1837	1842	1851	rBV	629228	787367	67.87%	9.033%
76	12.451	1863	1864	1865	rBV	449	259	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036028.D
 Acq On : 06 Jun 2023 13:27
 Operator : JC/MD
 Sample : 02991-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.536	1876	1878	1879	rBV	374	231	0.02%	0.003%
78	12.603	1886	1889	1893	rVB2	309	485	0.04%	0.006%
79	12.853	1927	1930	1935	rVB	1222	1409	0.12%	0.016%
80	13.115	1969	1973	1977	rVB3	1427	1852	0.16%	0.021%
81	13.341	2008	2010	2013	rVB3	349	409	0.04%	0.005%
82	13.365	2013	2014	2017	rBV2	282	350	0.03%	0.004%
83	13.561	2044	2046	2048	rBV2	244	217	0.02%	0.002%
84	13.591	2048	2051	2055	rVV2	1928	2334	0.20%	0.027%
85	13.689	2063	2067	2071	rVB2	969	1072	0.09%	0.012%
86	13.780	2078	2082	2088	rVV2	1411	2147	0.19%	0.025%
87	13.884	2095	2099	2100	rBV	352	351	0.03%	0.004%
88	13.963	2109	2112	2115	rVV2	1450	1661	0.14%	0.019%
89	14.127	2137	2139	2141	rVB2	293	210	0.02%	0.002%
90	14.176	2144	2147	2149	rBV2	229	239	0.02%	0.003%
91	14.335	2172	2173	2175	rBV	387	324	0.03%	0.004%
92	14.512	2198	2202	2204	rBV2	333	465	0.04%	0.005%
93	14.560	2208	2210	2211	rBV2	334	278	0.02%	0.003%
94	14.597	2214	2216	2218	rBV2	396	354	0.03%	0.004%
95	14.640	2221	2223	2228	rBV	451	457	0.04%	0.005%
96	14.676	2228	2229	2233	rBV3	315	254	0.02%	0.003%
97	15.207	2314	2316	2319	rVB	567	342	0.03%	0.004%
98	15.310	2331	2333	2335	rBV3	513	391	0.03%	0.004%
99	16.469	2521	2523	2526	rBV2	727	690	0.06%	0.008%
100	16.554	2535	2537	2540	rBV	709	698	0.06%	0.008%




Sum of corrected areas: 8716804

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036028.D
Acq On : 06 Jun 2023 13:27
Operator : JC/MD
Sample : 02991-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

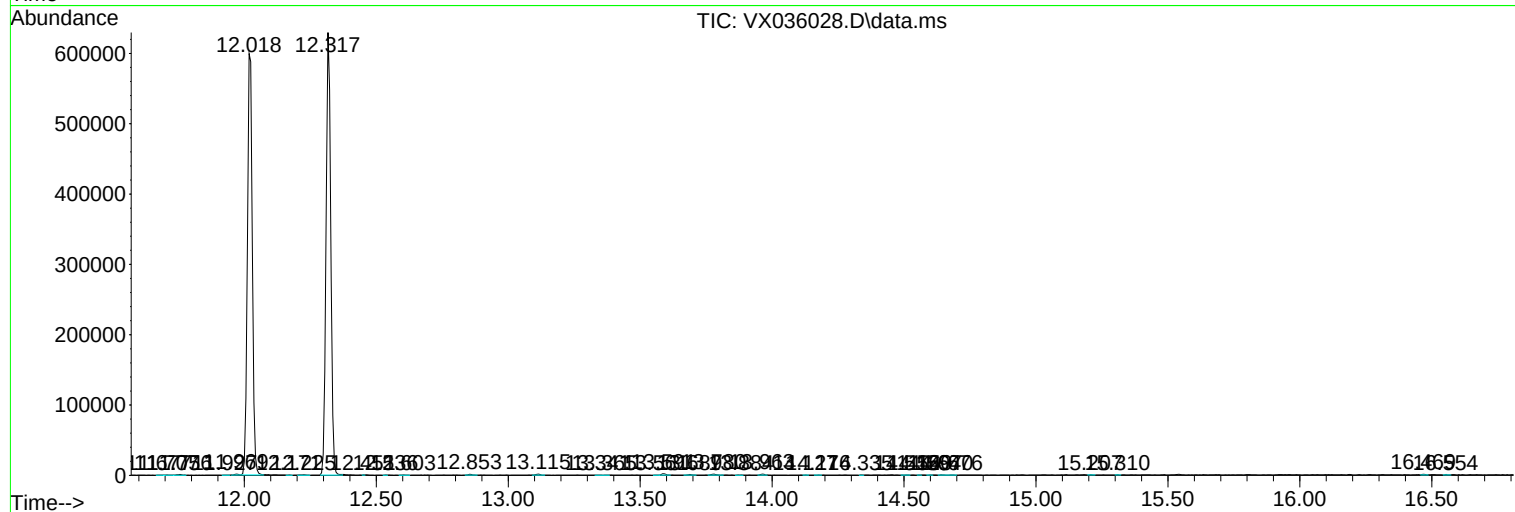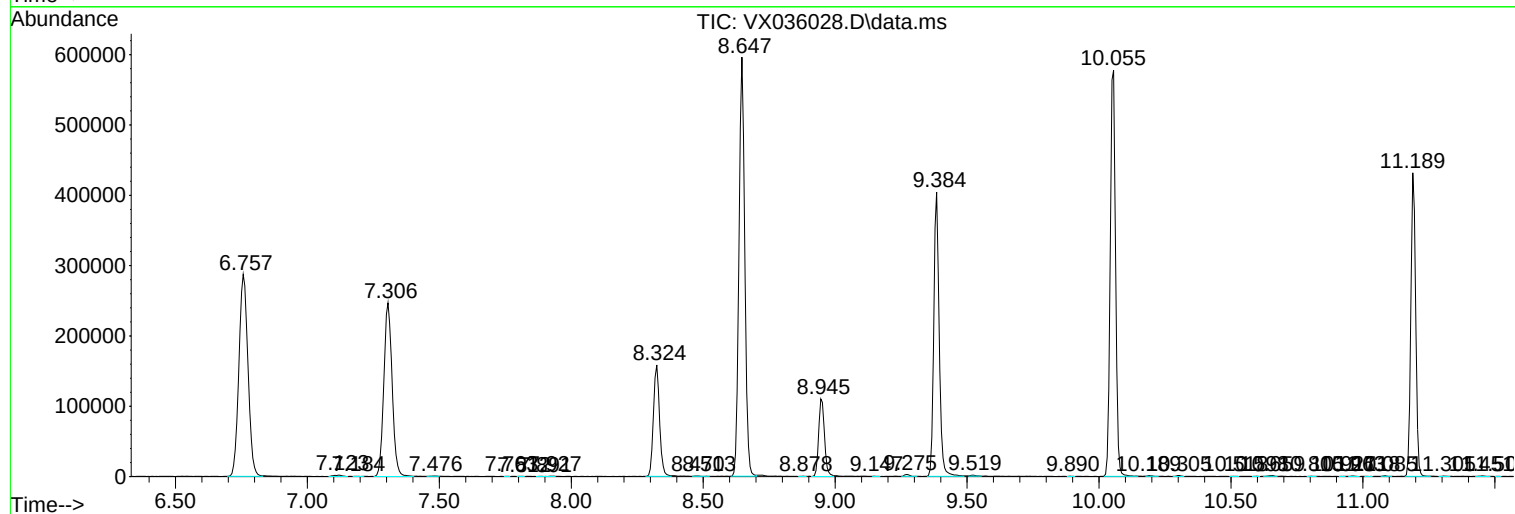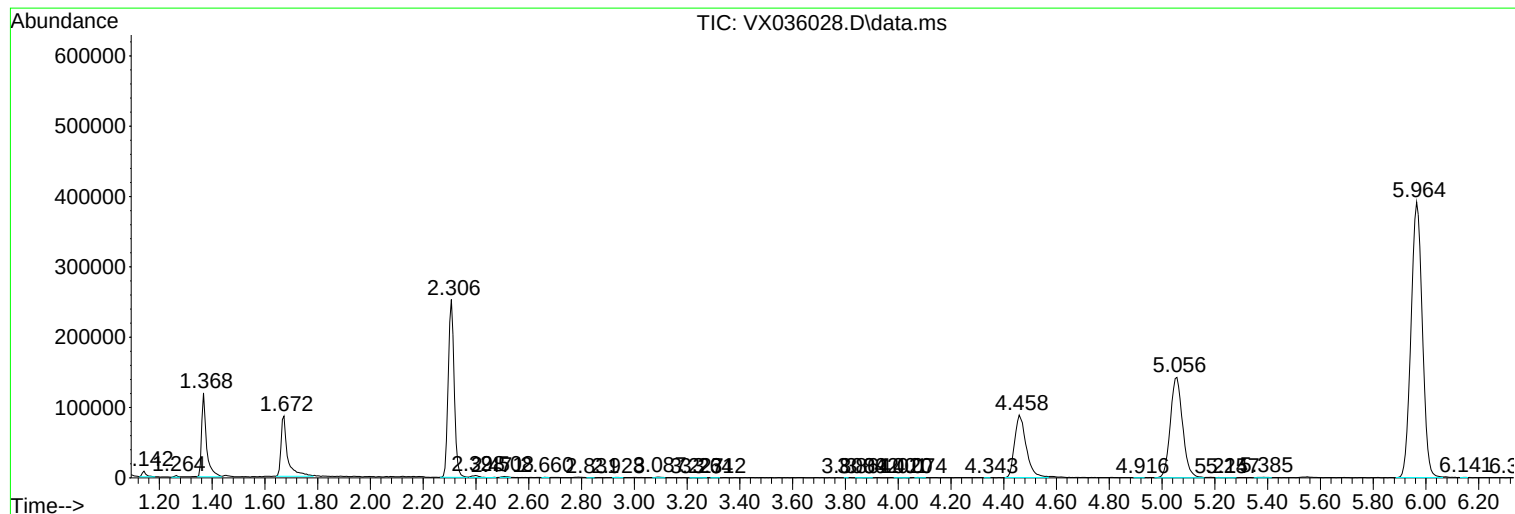

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036028.D
Acq On : 06 Jun 2023 13:27
Operator : JC/MD
Sample : 02991-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036028.D
Acq On : 06 Jun 2023 13:27
Operator : JC/MD
Sample : 02991-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc