

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036029.D
 Acq On : 06 Jun 2023 13:51
 Operator : JC/MD
 Sample : 02991-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	18	rBV	8232	8932	0.68%	0.092%
2	1.264	26	29	32	rBV3	1653	1949	0.15%	0.020%
3	1.368	42	46	63	rBV	141844	176650	13.44%	1.814%
4	1.673	91	96	107	rBV	105849	161400	12.28%	1.658%
5	2.307	194	200	211	rBV	292615	462134	35.16%	4.746%
6	2.514	231	234	238	rVB2	909	1238	0.09%	0.013%
7	2.703	263	265	268	rVB2	318	314	0.02%	0.003%
8	2.788	275	279	283	rBV4	1149	1635	0.12%	0.017%
9	2.935	298	303	306	rBV3	291	490	0.04%	0.005%
10	3.020	313	317	318	rVV2	346	455	0.03%	0.005%
11	3.044	318	321	322	rVV3	375	377	0.03%	0.004%
12	3.093	325	329	331	rBV	569	780	0.06%	0.008%
13	3.142	334	337	339	rVB2	306	281	0.02%	0.003%
14	3.172	339	342	344	rBV2	256	256	0.02%	0.003%
15	3.197	344	346	348	rVB	322	315	0.02%	0.003%
16	3.215	348	349	353	rBV2	182	251	0.02%	0.003%
17	3.294	359	362	364	rBV2	291	333	0.03%	0.003%
18	3.800	441	445	446	rBV3	189	237	0.02%	0.002%
19	3.977	471	474	478	rBV2	219	371	0.03%	0.004%
20	4.471	544	555	574	rBV	87622	288141	21.92%	2.959%
21	5.056	638	651	668	rBV	166988	522837	39.78%	5.369%
22	5.361	699	701	702	rBV	617	536	0.04%	0.006%
23	5.458	714	717	718	rBV2	353	304	0.02%	0.003%
24	5.550	725	732	733	rBV3	2058	3562	0.27%	0.037%
25	5.666	750	751	755	rVB2	303	226	0.02%	0.002%
26	5.971	788	801	819	rBV2	436462	1314371	100.00%	13.498%
27	6.458	880	881	884	rBV2	268	279	0.02%	0.003%
28	6.544	890	895	898	rVV3	274	377	0.03%	0.004%
29	6.757	919	930	942	rBV	310060	746024	56.76%	7.662%
30	7.111	983	988	995	rBV3	1705	3666	0.28%	0.038%
31	7.306	1010	1020	1037	rBV	270395	602372	45.83%	6.186%
32	7.470	1044	1047	1051	rBV4	573	1076	0.08%	0.011%
33	7.531	1052	1057	1066	rVB3	2751	5262	0.40%	0.054%
34	7.702	1083	1085	1089	rBV2	371	460	0.03%	0.005%
35	7.915	1118	1120	1126	rVB3	453	831	0.06%	0.009%
36	8.025	1137	1138	1142	rBV2	211	302	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036029.D
 Acq On : 06 Jun 2023 13:51
 Operator : JC/MD
 Sample : 02991-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	8.062	1142	1144	1147	rVB2	369	428	0.03%	0.004%
38	8.324	1180	1187	1203	rBV	174914	283470	21.57%	2.911%
39	8.470	1210	1211	1213	rBV2	443	294	0.02%	0.003%
40	8.647	1233	1240	1250	rBV	675301	1044738	79.49%	10.729%
41	8.836	1270	1271	1273	rBV	284	223	0.02%	0.002%
42	8.952	1284	1290	1298	rBV	123428	185300	14.10%	1.903%
43	9.214	1330	1333	1334	rVB	286	225	0.02%	0.002%
44	9.232	1334	1336	1337	rBV	393	263	0.02%	0.003%
45	9.269	1339	1342	1346	rVB4	1230	1818	0.14%	0.019%
46	9.385	1355	1361	1380	rBV	444801	641351	48.80%	6.587%
47	9.647	1402	1404	1408	rVB3	438	466	0.04%	0.005%
48	9.683	1408	1410	1414	rVB3	236	323	0.02%	0.003%
49	9.750	1420	1421	1424	rVB3	302	287	0.02%	0.003%
50	9.982	1458	1459	1464	rVB	437	484	0.04%	0.005%
51	10.055	1464	1471	1480	rBV	631691	886593	67.45%	9.105%
52	10.195	1491	1494	1497	rVB3	571	815	0.06%	0.008%
53	10.232	1499	1500	1504	rBV	298	365	0.03%	0.004%
54	10.299	1508	1511	1516	rVB3	930	1048	0.08%	0.011%
55	10.372	1521	1523	1525	rBV	278	218	0.02%	0.002%
56	10.720	1579	1580	1583	rBV2	284	260	0.02%	0.003%
57	10.744	1583	1584	1587	rBV2	364	342	0.03%	0.004%
58	10.781	1589	1590	1596	rVB3	288	385	0.03%	0.004%
59	10.842	1599	1600	1601	rBV	417	216	0.02%	0.002%
60	10.927	1611	1614	1616	rBV2	331	360	0.03%	0.004%
61	10.970	1618	1621	1623	rVV2	371	429	0.03%	0.004%
62	11.037	1630	1632	1635	rVB2	231	284	0.02%	0.003%
63	11.086	1635	1640	1643	rBV3	947	1259	0.10%	0.013%
64	11.189	1652	1657	1666	rBV	486868	610925	46.48%	6.274%
65	11.305	1675	1676	1678	rBV2	326	259	0.02%	0.003%
66	11.457	1696	1701	1705	rVB4	541	817	0.06%	0.008%
67	11.707	1739	1742	1745	rVB2	384	326	0.02%	0.003%
68	11.756	1747	1750	1754	rVB	688	569	0.04%	0.006%
69	11.823	1759	1761	1764	rVB	278	231	0.02%	0.002%
70	11.848	1764	1765	1767	rBV	338	275	0.02%	0.003%
71	11.970	1782	1785	1788	rBV2	909	1044	0.08%	0.011%
72	12.018	1788	1793	1802	rBV	683906	855103	65.06%	8.782%
73	12.256	1828	1832	1834	rBV2	265	389	0.03%	0.004%
74	12.317	1837	1842	1853	rBV	735301	891921	67.86%	9.160%
75	12.457	1863	1865	1867	rBV	270	218	0.02%	0.002%
76	12.610	1888	1890	1892	rVV2	345	333	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036029.D
 Acq On : 06 Jun 2023 13:51
 Operator : JC/MD
 Sample : 02991-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.646	1894	1896	1900	rVB2	204	240	0.02%	0.002%
78	12.811	1919	1923	1925	rBV	1950	2233	0.17%	0.023%
79	12.933	1942	1943	1947	rBV	284	350	0.03%	0.004%
80	12.969	1947	1949	1952	rVB2	362	353	0.03%	0.004%
81	13.030	1955	1959	1961	rBV2	423	544	0.04%	0.006%
82	13.110	1970	1972	1976	rVB3	692	768	0.06%	0.008%
83	13.146	1976	1978	1981	rVB	310	224	0.02%	0.002%
84	13.213	1986	1989	1992	rBV2	348	528	0.04%	0.005%
85	13.591	2046	2051	2053	rBV4	1076	1223	0.09%	0.013%
86	13.652	2058	2061	2062	rVB	388	267	0.02%	0.003%
87	13.701	2066	2069	2070	rBV2	306	305	0.02%	0.003%
88	13.780	2076	2082	2086	rBV3	1038	1506	0.11%	0.015%
89	14.006	2116	2119	2120	rBV2	307	299	0.02%	0.003%
90	14.024	2120	2122	2125	rVB2	348	298	0.02%	0.003%
91	14.122	2134	2138	2139	rVB2	390	446	0.03%	0.005%
92	14.286	2164	2165	2167	rBV	492	350	0.03%	0.004%
93	14.457	2190	2193	2195	rBV3	500	491	0.04%	0.005%
94	14.530	2204	2205	2207	rBV	333	263	0.02%	0.003%
95	15.140	2304	2305	2307	rVB2	625	272	0.02%	0.003%
96	15.176	2310	2311	2317	rVB4	471	595	0.05%	0.006%
97	15.414	2348	2350	2353	rBV3	542	426	0.03%	0.004%
98	15.542	2369	2371	2375	rVB4	729	764	0.06%	0.008%
99	16.097	2461	2462	2465	rBV2	564	564	0.04%	0.006%
100	16.578	2539	2541	2542	rBV	534	284	0.02%	0.003%




Sum of corrected areas: 9737271

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036029.D
Acq On : 06 Jun 2023 13:51
Operator : JC/MD
Sample : 02991-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

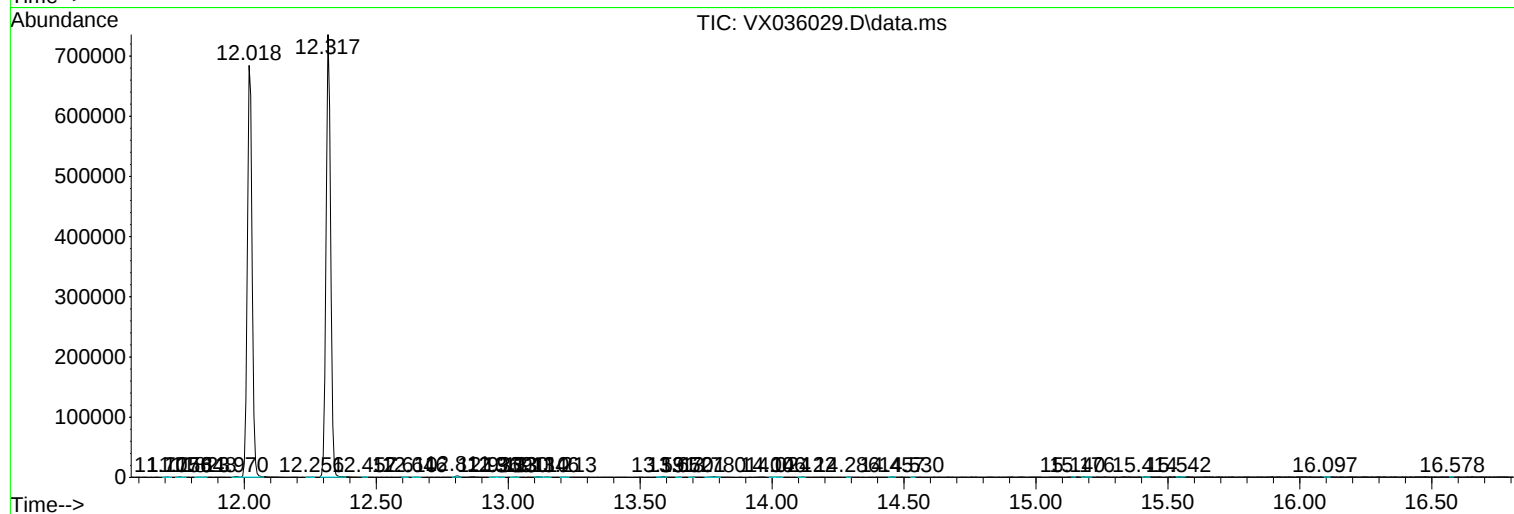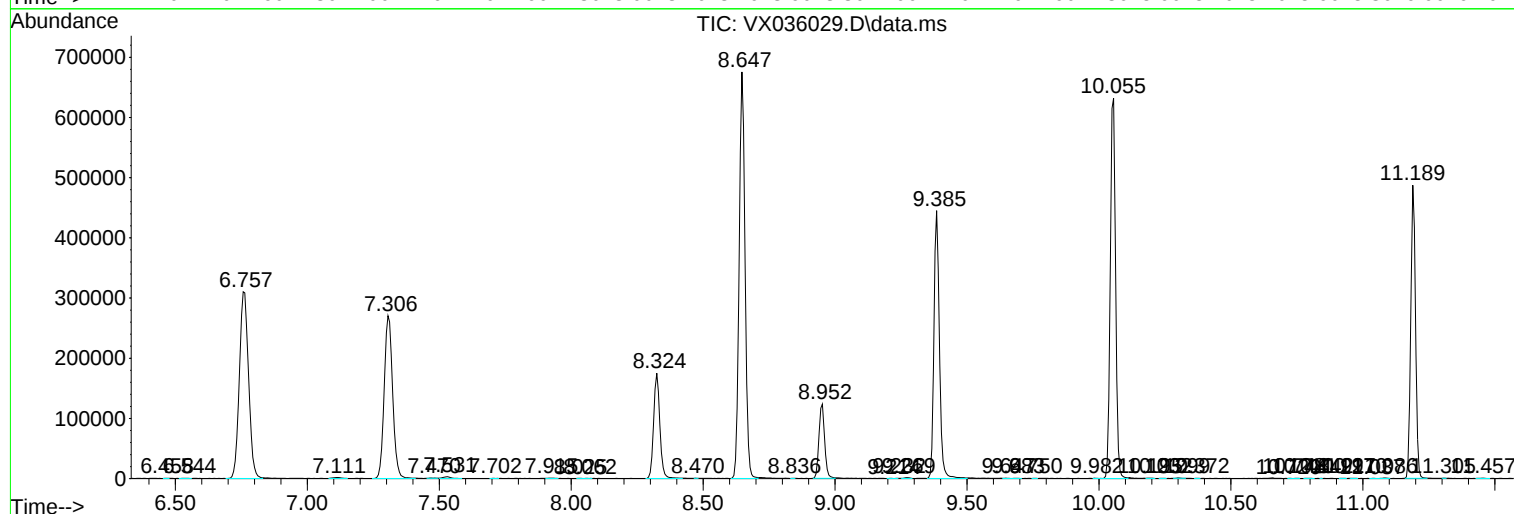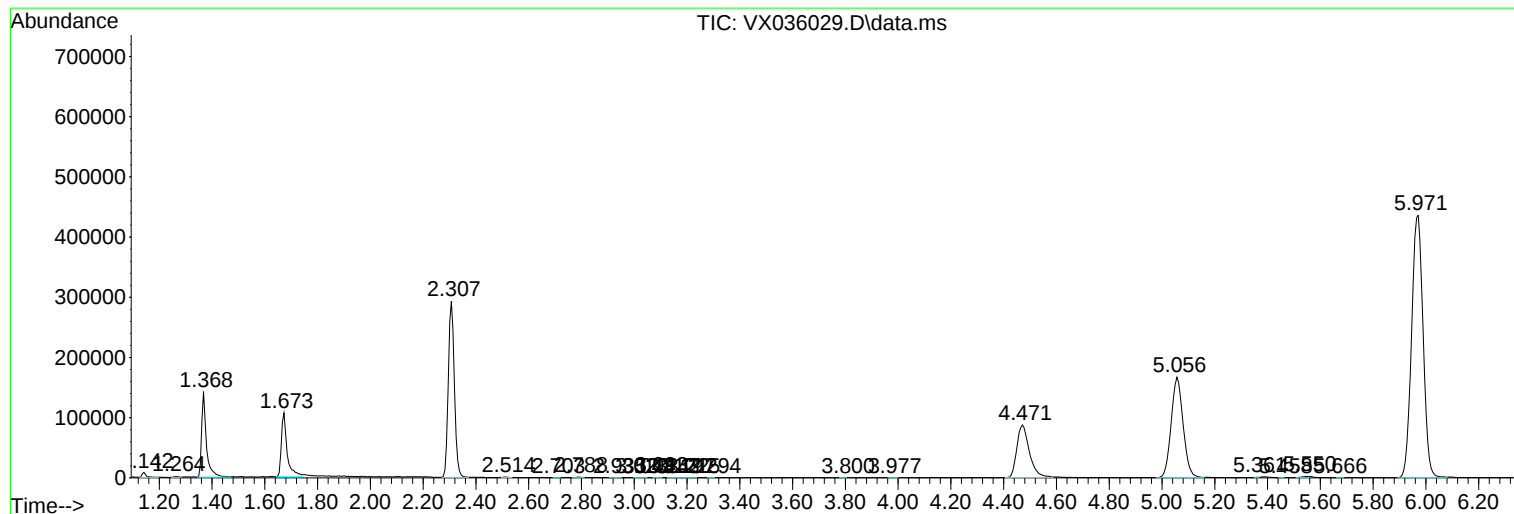

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036029.D
Acq On : 06 Jun 2023 13:51
Operator : JC/MD
Sample : 02991-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036029.D
Acq On : 06 Jun 2023 13:51
Operator : JC/MD
Sample : 02991-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------