

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036030.D
 Acq On : 06 Jun 2023 14:14
 Operator : JC/MD
 Sample : 02991-11 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M

Title : VOC Analysis

Signal : TIC: VX036030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	15	rVB	8794	9470	0.72%	0.087%
2	1.264	27	29	32	rBV2	1711	1050	0.08%	0.010%
3	1.368	42	46	64	rBV	142897	178349	13.50%	1.648%
4	1.672	91	96	106	rBV	104617	158751	12.02%	1.467%
5	2.306	194	200	210	rBV	297765	456171	34.54%	4.215%
6	2.514	228	234	242	rVB2	1367	2577	0.20%	0.024%
7	2.581	242	245	246	rBV	526	514	0.04%	0.005%
8	2.794	274	280	290	rVB5	2635	5754	0.44%	0.053%
9	2.867	290	292	296	rBV3	210	264	0.02%	0.002%
10	2.934	300	303	304	rBV	1603	1354	0.10%	0.013%
11	3.038	318	320	322	rVV	278	242	0.02%	0.002%
12	3.117	326	333	339	rVB5	2246	5597	0.42%	0.052%
13	3.276	356	359	361	rBV2	386	378	0.03%	0.003%
14	3.446	384	387	388	rBV2	228	217	0.02%	0.002%
15	3.477	391	392	394	rVB	234	169	0.01%	0.002%
16	3.501	394	396	397	rBV2	189	169	0.01%	0.002%
17	3.763	437	439	441	rBV	152	168	0.01%	0.002%
18	3.824	446	449	450	rVB2	257	217	0.02%	0.002%
19	3.855	450	454	457	rBV	150	262	0.02%	0.002%
20	3.910	461	463	467	rVB	255	299	0.02%	0.003%
21	3.959	470	471	474	rBV	239	247	0.02%	0.002%
22	4.471	544	555	569	rBV	95292	326961	24.76%	3.021%
23	5.056	639	651	669	rBV	165121	524912	39.74%	4.850%
24	5.397	698	707	714	rBV4	1146	3173	0.24%	0.029%
25	5.550	726	732	742	rVV4	2198	5537	0.42%	0.051%
26	5.678	751	753	757	rVB2	342	306	0.02%	0.003%
27	5.800	771	773	776	rBV2	190	260	0.02%	0.002%
28	5.970	788	801	818	rBV2	439980	1320749	100.00%	12.203%
29	6.245	843	846	848	rBV2	424	408	0.03%	0.004%
30	6.440	875	878	879	rBV2	197	198	0.01%	0.002%
31	6.556	896	897	901	rVB2	250	192	0.01%	0.002%
32	6.653	910	913	918	rBV2	260	456	0.03%	0.004%
33	6.757	920	930	945	rBV	323990	773858	58.59%	7.150%
34	7.049	976	978	979	rBV	239	166	0.01%	0.002%
35	7.123	982	990	1003	rVB	91153	204992	15.52%	1.894%
36	7.305	1010	1020	1035	rBV	272310	600999	45.50%	5.553%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036030.D
 Acq On : 06 Jun 2023 14:14
 Operator : JC/MD
 Sample : 02991-11 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.464	1044	1046	1047	rBV	530	359	0.03%	0.003%
38	7.537	1056	1058	1060	rVB2	299	253	0.02%	0.002%
39	7.708	1084	1086	1088	rVB2	277	204	0.02%	0.002%
40	7.885	1112	1115	1116	rVB2	246	238	0.02%	0.002%
41	7.933	1120	1123	1127	rVV4	818	798	0.06%	0.007%
42	8.061	1141	1144	1147	rBV2	290	285	0.02%	0.003%
43	8.214	1167	1169	1172	rBV	285	283	0.02%	0.003%
44	8.324	1180	1187	1202	rBV	175647	284235	21.52%	2.626%
45	8.470	1210	1211	1216	rVB3	498	572	0.04%	0.005%
46	8.525	1219	1220	1223	rBV2	258	189	0.01%	0.002%
47	8.647	1233	1240	1250	rBV	687910	1056138	79.97%	9.758%
48	8.824	1268	1269	1273	rBV2	362	463	0.04%	0.004%
49	8.952	1284	1290	1302	rBV	119969	184522	13.97%	1.705%
50	9.116	1314	1317	1319	rBV2	301	250	0.02%	0.002%
51	9.275	1336	1343	1355	rVB	516242	765516	57.96%	7.073%
52	9.384	1355	1361	1381	rBV	439142	633193	47.94%	5.850%
53	9.921	1448	1449	1451	rBV2	336	228	0.02%	0.002%
54	9.951	1451	1454	1456	rBV	234	221	0.02%	0.002%
55	9.976	1456	1458	1461	rBV3	141	176	0.01%	0.002%
56	10.055	1465	1471	1481	rBV	661607	902717	68.35%	8.341%
57	10.238	1499	1501	1503	rBV	270	171	0.01%	0.002%
58	10.378	1520	1524	1525	rVB2	218	220	0.02%	0.002%
59	10.396	1525	1527	1529	rBV	260	159	0.01%	0.001%
60	10.878	1604	1606	1607	rVV	285	208	0.02%	0.002%
61	10.915	1610	1612	1616	rBV2	202	281	0.02%	0.003%
62	11.085	1637	1640	1643	rBV4	753	806	0.06%	0.007%
63	11.189	1652	1657	1668	rVB	486300	612151	46.35%	5.656%
64	11.311	1676	1677	1679	rBV	516	329	0.02%	0.003%
65	11.384	1687	1689	1693	rBV2	225	360	0.03%	0.003%
66	11.713	1740	1743	1747	rVB3	561	648	0.05%	0.006%
67	11.762	1747	1751	1753	rBV3	338	389	0.03%	0.004%
68	11.969	1782	1785	1788	rBV2	609	792	0.06%	0.007%
69	12.018	1788	1793	1803	rBV	698968	877673	66.45%	8.109%
70	12.213	1823	1825	1830	rBV2	280	496	0.04%	0.005%
71	12.317	1836	1842	1849	rBV	707027	900008	68.14%	8.316%
72	12.445	1861	1863	1867	rBV3	389	531	0.04%	0.005%
73	12.792	1919	1920	1922	rVB2	277	161	0.01%	0.001%
74	12.859	1929	1931	1934	rVB2	428	251	0.02%	0.002%
75	12.902	1937	1938	1940	rBV	229	211	0.02%	0.002%
76	13.006	1954	1955	1959	rVB2	265	240	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036030.D
 Acq On : 06 Jun 2023 14:14
 Operator : JC/MD
 Sample : 02991-11 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M

Title : VOC Analysis

77	13.042	1959	1961	1963	rBV2	283	229	0.02%	0.002%
78	13.109	1970	1972	1978	rVB2	527	472	0.04%	0.004%
79	13.243	1993	1994	1998	rVB	289	199	0.02%	0.002%
80	13.402	2018	2020	2023	rBV2	251	332	0.03%	0.003%
81	13.499	2034	2036	2037	rBV	381	230	0.02%	0.002%
82	13.591	2046	2051	2054	rBV4	837	1012	0.08%	0.009%
83	13.688	2064	2067	2071	rBV3	681	816	0.06%	0.008%
84	13.774	2079	2081	2083	rBV	398	277	0.02%	0.003%
85	13.817	2085	2088	2089	rBV2	302	379	0.03%	0.004%
86	13.951	2107	2110	2111	rBV2	458	401	0.03%	0.004%
87	13.969	2111	2113	2116	rVB2	592	529	0.04%	0.005%
88	14.018	2119	2121	2124	rBV	278	302	0.02%	0.003%
89	14.085	2130	2132	2134	rBV2	204	229	0.02%	0.002%
90	14.127	2137	2139	2140	rBV	318	332	0.03%	0.003%
91	14.194	2145	2150	2154	rBV4	303	632	0.05%	0.006%
92	14.341	2171	2174	2176	rBV	284	339	0.03%	0.003%
93	14.408	2184	2185	2186	rBV	287	171	0.01%	0.002%
94	14.731	2236	2238	2239	rBV	360	222	0.02%	0.002%
95	14.816	2251	2252	2253	rBV	322	209	0.02%	0.002%
96	15.024	2285	2286	2288	rBV2	322	287	0.02%	0.003%
97	15.097	2296	2298	2300	rVB2	451	244	0.02%	0.002%
98	15.542	2368	2371	2378	rVB3	803	1320	0.10%	0.012%
99	15.883	2426	2427	2429	rBV2	568	469	0.04%	0.004%
100	16.475	2521	2524	2527	rBV4	784	1165	0.09%	0.011%




Sum of corrected areas: 10823108

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036030.D
Acq On : 06 Jun 2023 14:14
Operator : JC/MD
Sample : 02991-11 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

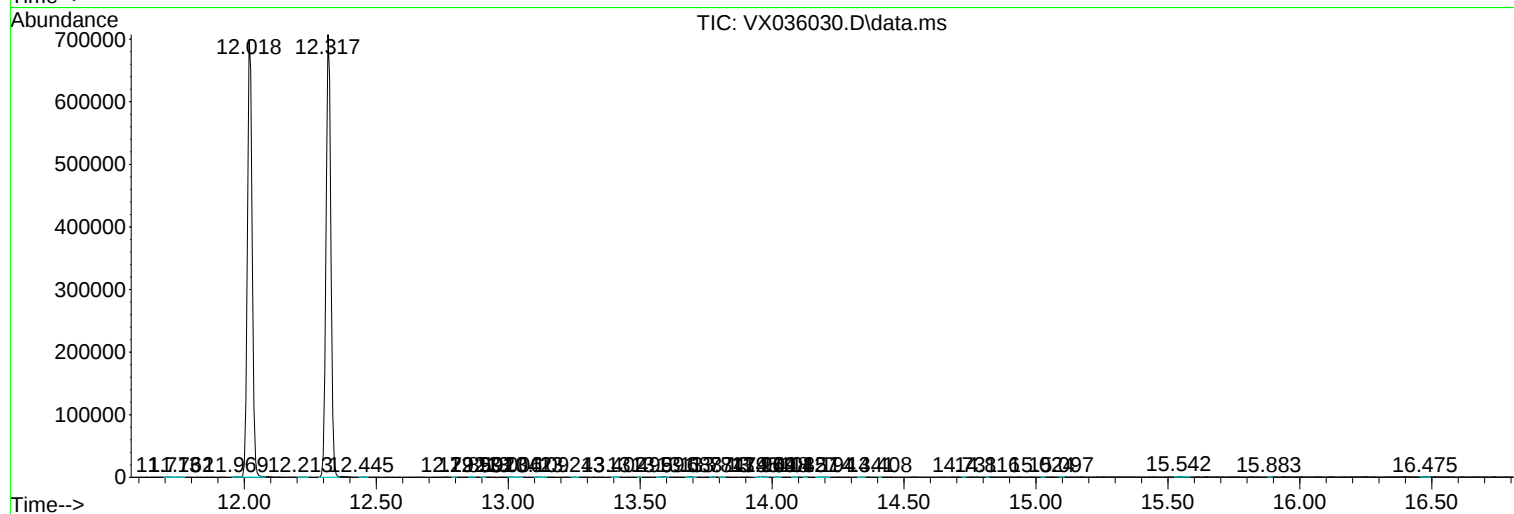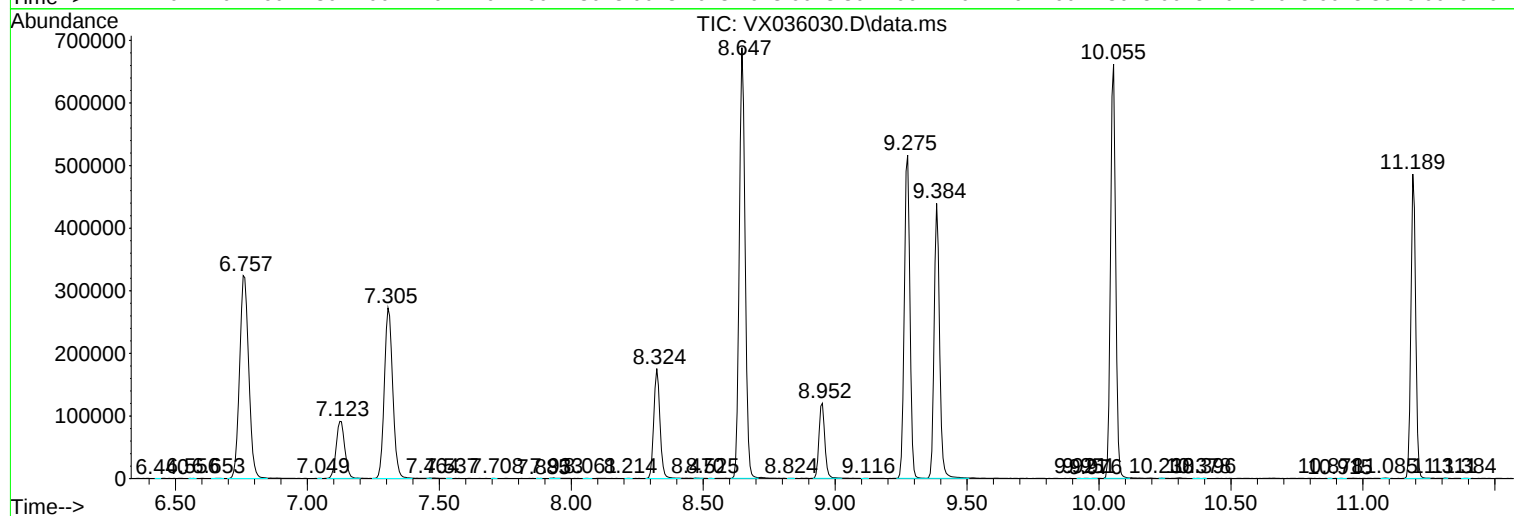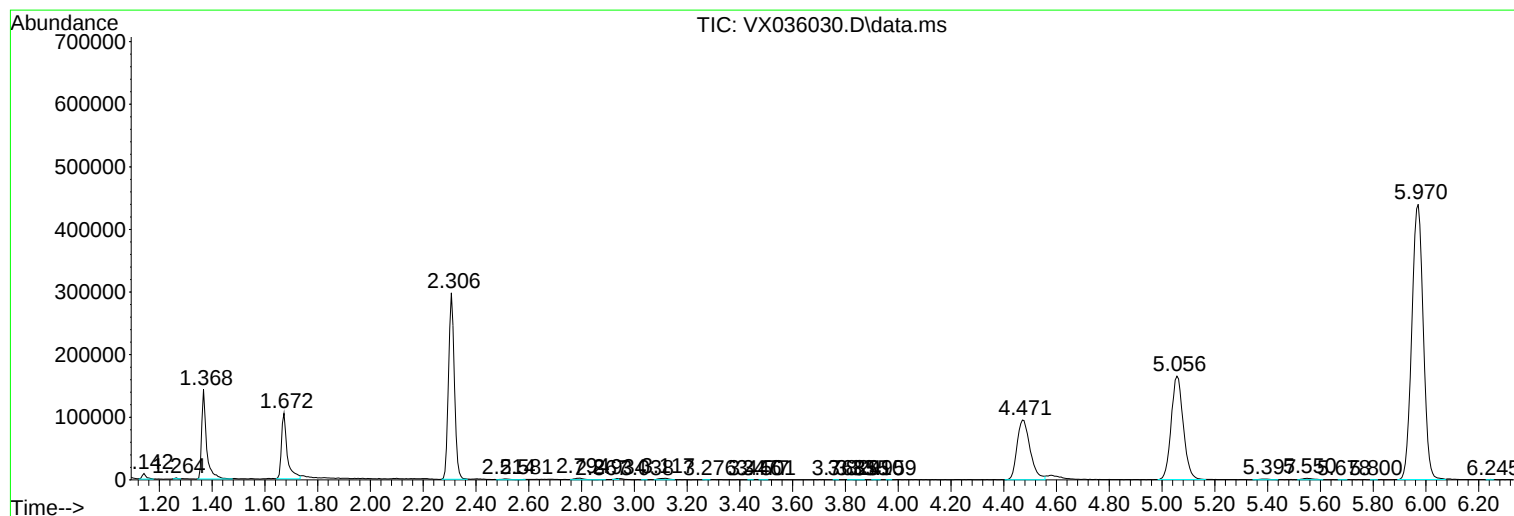

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036030.D
Acq On : 06 Jun 2023 14:14
Operator : JC/MD
Sample : 02991-11 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036030.D
Acq On : 06 Jun 2023 14:14
Operator : JC/MD
Sample : 02991-11 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc