

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036031.D
 Acq On : 06 Jun 2023 14:37
 Operator : JC/MD
 Sample : 02991-01 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M

Title : VOC Analysis

Signal : TIC: VX036031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	15	rVB	7952	8276	0.64%	0.078%
2	1.264	27	29	31	rVB2	1876	1317	0.10%	0.012%
3	1.368	42	46	59	rBV	138400	167677	12.92%	1.585%
4	1.673	91	96	117	rBV	103775	161930	12.48%	1.530%
5	2.307	194	200	212	rVB	289176	445041	34.29%	4.206%
6	2.508	229	233	238	rVB3	801	1197	0.09%	0.011%
7	2.788	275	279	287	rVB5	2279	4827	0.37%	0.046%
8	2.843	287	288	290	rBV2	304	207	0.02%	0.002%
9	2.867	290	292	293	rVV	299	184	0.01%	0.002%
10	2.886	293	295	298	rVV2	338	241	0.02%	0.002%
11	2.941	298	304	312	rVB3	1868	4302	0.33%	0.041%
12	3.056	321	323	325	rBV2	248	237	0.02%	0.002%
13	3.111	325	332	343	rVB2	5990	13954	1.08%	0.132%
14	3.264	355	357	362	rVB2	316	389	0.03%	0.004%
15	3.313	362	365	366	rBV	209	217	0.02%	0.002%
16	3.355	370	372	375	rBV	254	222	0.02%	0.002%
17	3.465	387	390	392	rBV	252	234	0.02%	0.002%
18	3.501	394	396	398	rBV	329	238	0.02%	0.002%
19	3.556	403	405	409	rVB3	377	378	0.03%	0.004%
20	3.593	409	411	415	rBV	259	264	0.02%	0.002%
21	3.654	418	421	423	rBV	246	290	0.02%	0.003%
22	3.739	428	435	437	rBV2	246	532	0.04%	0.005%
23	4.227	513	515	517	rVB	338	202	0.02%	0.002%
24	4.245	517	518	521	rBV2	189	184	0.01%	0.002%
25	4.477	544	556	567	rBV	92559	314367	24.22%	2.971%
26	5.056	639	651	668	rBV	165677	504164	38.84%	4.764%
27	5.379	698	704	705	rBV2	1139	1702	0.13%	0.016%
28	5.465	714	718	721	rBV3	423	695	0.05%	0.007%
29	5.550	724	732	742	rVV3	2890	7321	0.56%	0.069%
30	5.684	751	754	756	rBV2	185	203	0.02%	0.002%
31	5.745	762	764	767	rBV2	220	246	0.02%	0.002%
32	5.971	788	801	821	rBV2	431402	1297913	100.00%	12.265%
33	6.208	839	840	843	rBV2	303	291	0.02%	0.003%
34	6.233	843	844	847	rVB2	248	181	0.01%	0.002%
35	6.263	847	849	850	rBV2	294	225	0.02%	0.002%
36	6.342	861	862	864	rBV	215	189	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036031.D
 Acq On : 06 Jun 2023 14:37
 Operator : JC/MD
 Sample : 02991-01 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.452	878	880	883	rVB2	286	301	0.02%	0.003%
38	6.483	883	885	887	rBV2	267	262	0.02%	0.002%
39	6.623	905	908	911	rVB	185	205	0.02%	0.002%
40	6.696	918	920	921	rBV	218	216	0.02%	0.002%
41	6.757	921	930	949	rVV	311396	751324	57.89%	7.100%
42	7.019	970	973	974	rVB2	293	312	0.02%	0.003%
43	7.123	983	990	1002	rBV	75699	163105	12.57%	1.541%
44	7.306	1011	1020	1040	rBV	269760	597816	46.06%	5.649%
45	7.476	1044	1048	1053	rVV4	649	1143	0.09%	0.011%
46	7.611	1067	1070	1072	rVB2	220	252	0.02%	0.002%
47	7.647	1072	1076	1079	rBV2	328	534	0.04%	0.005%
48	7.934	1120	1123	1127	rBV2	448	522	0.04%	0.005%
49	8.074	1143	1146	1149	rVB2	186	233	0.02%	0.002%
50	8.324	1180	1187	1200	rBV	165080	276742	21.32%	2.615%
51	8.476	1210	1212	1213	rBV	458	372	0.03%	0.004%
52	8.647	1233	1240	1259	rBV	641319	1018132	78.44%	9.621%
53	8.952	1284	1290	1298	rBV	118100	181965	14.02%	1.720%
54	9.275	1336	1343	1355	rVV	570811	847226	65.28%	8.006%
55	9.385	1355	1361	1375	rBV	426627	607477	46.80%	5.741%
56	9.891	1442	1444	1448	rBV2	426	371	0.03%	0.004%
57	9.976	1456	1458	1462	rVB2	237	288	0.02%	0.003%
58	10.055	1465	1471	1484	rBV	636399	875450	67.45%	8.273%
59	10.189	1491	1493	1497	rVB4	746	841	0.06%	0.008%
60	10.250	1501	1503	1506	rVB	482	380	0.03%	0.004%
61	10.305	1508	1512	1518	rVB2	727	1359	0.10%	0.013%
62	10.397	1523	1527	1528	rBV	223	202	0.02%	0.002%
63	10.531	1547	1549	1552	rBV	214	251	0.02%	0.002%
64	10.598	1558	1560	1564	rVB2	327	340	0.03%	0.003%
65	10.640	1564	1567	1568	rBV2	502	533	0.04%	0.005%
66	10.842	1598	1600	1602	rBV2	197	187	0.01%	0.002%
67	10.957	1617	1619	1624	rVB2	405	423	0.03%	0.004%
68	11.092	1637	1641	1642	rVV4	794	951	0.07%	0.009%
69	11.189	1652	1657	1667	rBV	452431	590208	45.47%	5.577%
70	11.305	1673	1676	1677	rBV2	229	220	0.02%	0.002%
71	11.403	1689	1692	1693	rBV2	204	188	0.01%	0.002%
72	11.451	1697	1700	1703	rVV3	566	694	0.05%	0.007%
73	11.713	1741	1743	1744	rVB	428	231	0.02%	0.002%
74	11.750	1747	1749	1752	rBV3	322	331	0.03%	0.003%
75	11.915	1774	1776	1780	rVB	347	349	0.03%	0.003%
76	11.963	1782	1784	1788	rBV2	470	573	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036031.D
 Acq On : 06 Jun 2023 14:37
 Operator : JC/MD
 Sample : 02991-01 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1802	rBV	672736	842197	64.89%	7.959%
78	12.171	1816	1818	1820	rVV	270	187	0.01%	0.002%
79	12.219	1823	1826	1830	rVB3	559	736	0.06%	0.007%
80	12.317	1837	1842	1857	rBV	684641	869073	66.96%	8.213%
81	12.451	1862	1864	1865	rBV	482	272	0.02%	0.003%
82	12.628	1890	1893	1894	rBV	214	226	0.02%	0.002%
83	12.768	1914	1916	1918	rBV	257	297	0.02%	0.003%
84	12.945	1943	1945	1947	rBV	230	231	0.02%	0.002%
85	13.018	1954	1957	1958	rBV	237	206	0.02%	0.002%
86	13.110	1969	1972	1973	rBV	230	244	0.02%	0.002%
87	13.353	2010	2012	2014	rBV2	234	209	0.02%	0.002%
88	13.555	2044	2045	2048	rVV2	221	173	0.01%	0.002%
89	13.591	2048	2051	2056	rVB4	693	1048	0.08%	0.010%
90	13.689	2065	2067	2069	rBV	546	447	0.03%	0.004%
91	13.933	2106	2107	2110	rBV	340	303	0.02%	0.003%
92	14.036	2123	2124	2127	rBV2	412	413	0.03%	0.004%
93	14.109	2134	2136	2140	rBV3	262	362	0.03%	0.003%
94	14.250	2157	2159	2162	rVB2	327	327	0.03%	0.003%
95	14.311	2167	2169	2171	rVB2	303	245	0.02%	0.002%
96	14.341	2171	2174	2177	rBV2	439	606	0.05%	0.006%
97	14.487	2196	2198	2200	rBV2	419	298	0.02%	0.003%
98	15.786	2409	2411	2414	rVB2	705	525	0.04%	0.005%
99	15.999	2444	2446	2448	rBV2	397	286	0.02%	0.003%
100	16.426	2514	2516	2520	rBV2	577	693	0.05%	0.007%




Sum of corrected areas: 10582150

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036031.D
Acq On : 06 Jun 2023 14:37
Operator : JC/MD
Sample : 02991-01 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

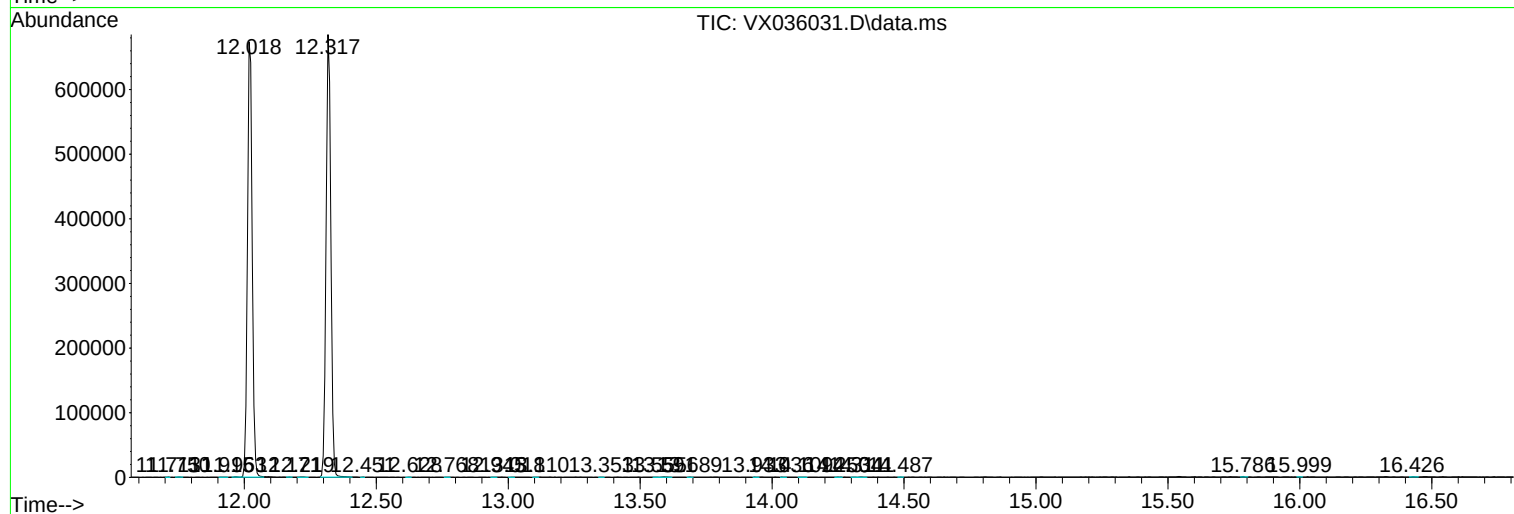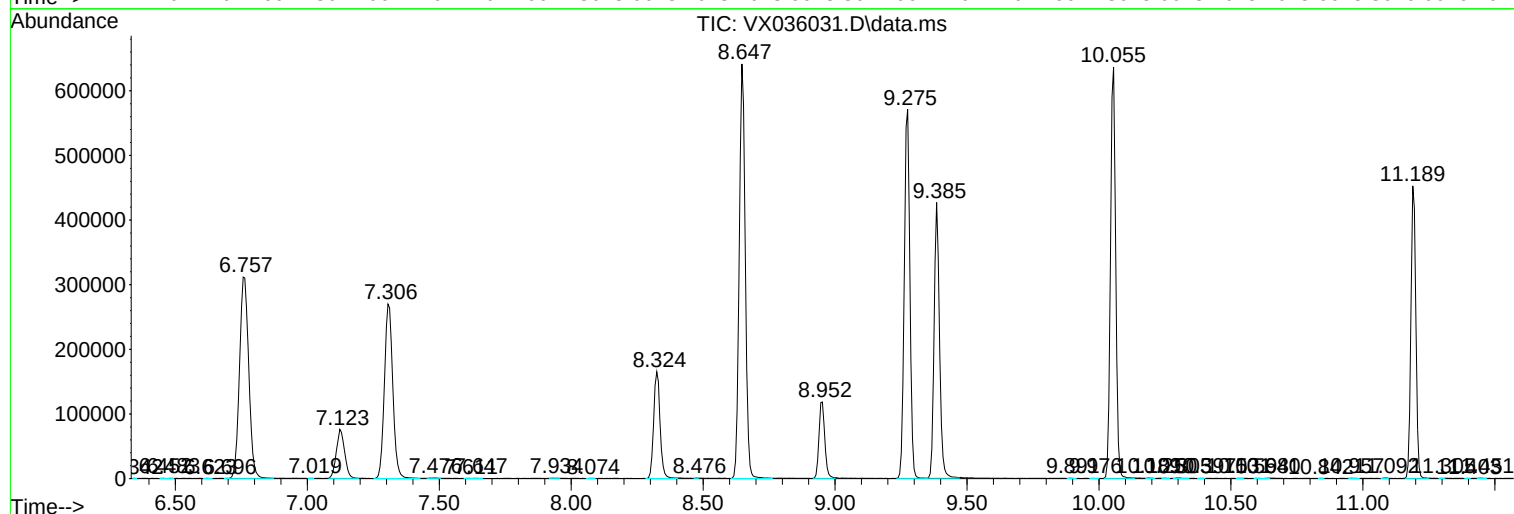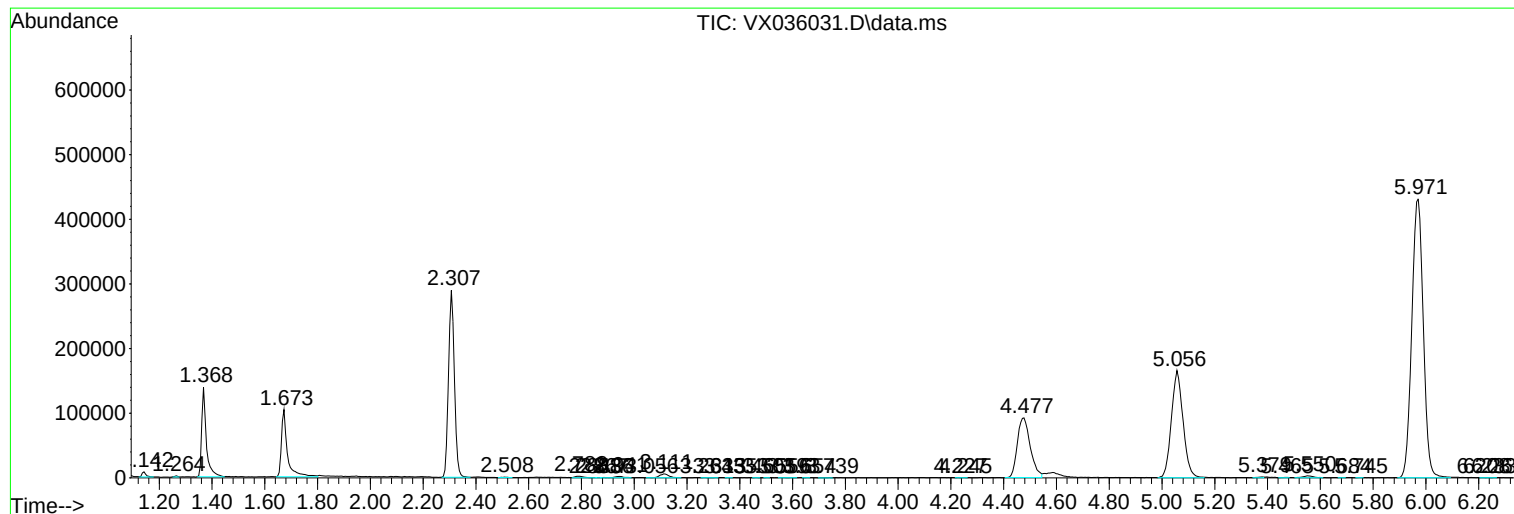

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036031.D
Acq On : 06 Jun 2023 14:37
Operator : JC/MD
Sample : 02991-01 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036031.D
Acq On : 06 Jun 2023 14:37
Operator : JC/MD
Sample : 02991-01 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
