

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036032.D
 Acq On : 06 Jun 2023 15:01
 Operator : JC/MD
 Sample : 02991-02 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	14	rVB2	8246	8613	0.67%	0.085%
2	1.264	26	29	32	rBV3	2076	2180	0.17%	0.021%
3	1.367	42	46	60	rBV	136652	166354	12.91%	1.633%
4	1.672	91	96	106	rBV	100119	148122	11.50%	1.454%
5	2.306	194	200	211	rBV	272252	428579	33.26%	4.208%
6	2.501	230	232	238	rBV2	708	985	0.08%	0.010%
7	2.751	271	273	275	rBV2	392	362	0.03%	0.004%
8	2.788	275	279	288	rVB4	2652	4814	0.37%	0.047%
9	2.867	288	292	295	rVB2	304	523	0.04%	0.005%
10	2.892	295	296	298	rBV2	305	257	0.02%	0.003%
11	2.946	298	305	312	rBV2	1997	4275	0.33%	0.042%
12	3.014	315	316	320	rBV3	484	539	0.04%	0.005%
13	3.111	325	332	340	rVB3	6159	14511	1.13%	0.142%
14	3.300	360	363	365	rBV2	212	209	0.02%	0.002%
15	3.611	410	414	416	rVB	275	307	0.02%	0.003%
16	3.684	423	426	427	rBV	207	187	0.01%	0.002%
17	3.763	438	439	443	rVB2	249	243	0.02%	0.002%
18	3.794	443	444	449	rBV2	244	303	0.02%	0.003%
19	3.855	453	454	456	rBV2	232	198	0.02%	0.002%
20	3.952	467	470	472	rBV2	238	256	0.02%	0.003%
21	3.983	472	475	478	rVV2	246	418	0.03%	0.004%
22	4.196	508	510	512	rBV2	221	245	0.02%	0.002%
23	4.312	528	529	533	rVV2	172	184	0.01%	0.002%
24	4.477	544	556	568	rBV	94658	326562	25.35%	3.207%
25	4.867	619	620	623	rVB3	293	217	0.02%	0.002%
26	5.056	638	651	670	rBV	157113	501509	38.93%	4.924%
27	5.214	675	677	681	rVB2	457	532	0.04%	0.005%
28	5.379	700	704	706	rBV2	512	856	0.07%	0.008%
29	5.550	725	732	733	rBV3	1217	2132	0.17%	0.021%
30	5.641	744	747	750	rVB2	179	199	0.02%	0.002%
31	5.794	769	772	774	rBV2	234	252	0.02%	0.002%
32	5.842	777	780	782	rBV2	226	238	0.02%	0.002%
33	5.867	782	784	787	rVB2	309	342	0.03%	0.003%
34	5.970	787	801	824	rBV2	431633	1288391	100.00%	12.651%
35	6.208	837	840	843	rBV2	350	466	0.04%	0.005%
36	6.300	851	855	857	rBV2	297	279	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036032.D
 Acq On : 06 Jun 2023 15:01
 Operator : JC/MD
 Sample : 02991-02 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.531	891	893	898	rBV2	283	461	0.04%	0.005%
38	6.757	921	930	943	rBV	276385	665255	51.63%	6.532%
39	7.123	982	990	1003	rBV2	71067	158897	12.33%	1.560%
40	7.305	1011	1020	1038	rBV	263898	585824	45.47%	5.752%
41	7.470	1042	1047	1048	rBV2	672	757	0.06%	0.007%
42	7.763	1092	1095	1098	rVB2	253	280	0.02%	0.003%
43	7.818	1102	1104	1106	rBV2	267	246	0.02%	0.002%
44	7.939	1117	1124	1126	rVB4	571	1022	0.08%	0.010%
45	8.086	1145	1148	1150	rVB	257	288	0.02%	0.003%
46	8.110	1150	1152	1154	rBV2	286	278	0.02%	0.003%
47	8.324	1180	1187	1200	rBV	168173	278932	21.65%	2.739%
48	8.574	1226	1228	1230	rVB	421	298	0.02%	0.003%
49	8.647	1234	1240	1253	rVV	652618	1004118	77.94%	9.860%
50	8.909	1279	1283	1284	rBV2	346	462	0.04%	0.005%
51	8.951	1284	1290	1307	rVV	124394	184348	14.31%	1.810%
52	9.208	1328	1332	1335	rBV2	301	535	0.04%	0.005%
53	9.275	1336	1343	1355	rBV	527468	782012	60.70%	7.679%
54	9.384	1356	1361	1377	rVV	442270	626581	48.63%	6.153%
55	9.689	1409	1411	1417	rVB4	220	237	0.02%	0.002%
56	9.805	1427	1430	1432	rBV2	253	231	0.02%	0.002%
57	9.890	1441	1444	1447	rVB2	353	454	0.04%	0.004%
58	10.000	1458	1462	1465	rBV2	232	443	0.03%	0.004%
59	10.055	1465	1471	1487	rVV	579366	781766	60.68%	7.676%
60	10.305	1508	1512	1517	rVB4	792	1313	0.10%	0.013%
61	10.348	1517	1519	1521	rBV	293	211	0.02%	0.002%
62	10.488	1538	1542	1546	rBV2	263	439	0.03%	0.004%
63	10.640	1564	1567	1574	rVB4	541	1162	0.09%	0.011%
64	10.701	1575	1577	1580	rVB2	322	302	0.02%	0.003%
65	10.963	1617	1620	1624	rVB2	543	761	0.06%	0.007%
66	11.000	1624	1626	1628	rBV	429	367	0.03%	0.004%
67	11.024	1628	1630	1633	rVB2	205	199	0.02%	0.002%
68	11.061	1633	1636	1637	rBV2	231	221	0.02%	0.002%
69	11.085	1637	1640	1644	rBV2	464	657	0.05%	0.006%
70	11.189	1652	1657	1668	rBV	460709	596473	46.30%	5.857%
71	11.311	1674	1677	1680	rBV4	562	607	0.05%	0.006%
72	11.707	1740	1742	1747	rBV	333	449	0.03%	0.004%
73	11.756	1747	1750	1751	rBV3	423	444	0.03%	0.004%
74	11.908	1773	1775	1778	rBV3	177	211	0.02%	0.002%
75	11.969	1783	1785	1788	rVB2	569	507	0.04%	0.005%
76	12.018	1788	1793	1803	rBV	561032	735184	57.06%	7.219%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036032.D
 Acq On : 06 Jun 2023 15:01
 Operator : JC/MD
 Sample : 02991-02 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.225	1826	1827	1830	rVB2	315	202	0.02%	0.002%
78	12.317	1837	1842	1852	rBV	675970	857834	66.58%	8.423%
79	12.457	1862	1865	1868	rVB3	536	695	0.05%	0.007%
80	12.786	1917	1919	1921	rBV	249	196	0.02%	0.002%
81	12.804	1921	1922	1924	rBV	291	193	0.01%	0.002%
82	12.853	1928	1930	1931	rBV2	332	292	0.02%	0.003%
83	13.121	1971	1974	1978	rBV2	543	714	0.06%	0.007%
84	13.225	1990	1991	1993	rVB	371	197	0.02%	0.002%
85	13.591	2048	2051	2053	rBV2	657	583	0.05%	0.006%
86	13.756	2073	2078	2079	rBV2	243	277	0.02%	0.003%
87	13.774	2079	2081	2086	rBV2	464	630	0.05%	0.006%
88	13.926	2101	2106	2109	rBV3	254	450	0.03%	0.004%
89	13.963	2109	2112	2113	rVV2	408	337	0.03%	0.003%
90	14.005	2117	2119	2121	rBV2	382	343	0.03%	0.003%
91	14.030	2121	2123	2124	rBV	354	189	0.01%	0.002%
92	14.121	2136	2138	2140	rBV	306	225	0.02%	0.002%
93	14.493	2198	2199	2201	rBV2	428	331	0.03%	0.003%
94	14.566	2206	2211	2212	rBV2	383	515	0.04%	0.005%
95	14.987	2278	2280	2282	rVB	451	193	0.01%	0.002%
96	15.024	2284	2286	2289	rBV3	301	318	0.02%	0.003%
97	16.042	2451	2453	2455	rBV	569	573	0.04%	0.006%
98	16.383	2508	2509	2510	rBV	491	227	0.02%	0.002%
99	16.542	2534	2535	2536	rBV	455	278	0.02%	0.003%
100	16.761	2569	2571	2573	rBV3	482	378	0.03%	0.004%




Sum of corrected areas: 10184041

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036032.D
Acq On : 06 Jun 2023 15:01
Operator : JC/MD
Sample : 02991-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

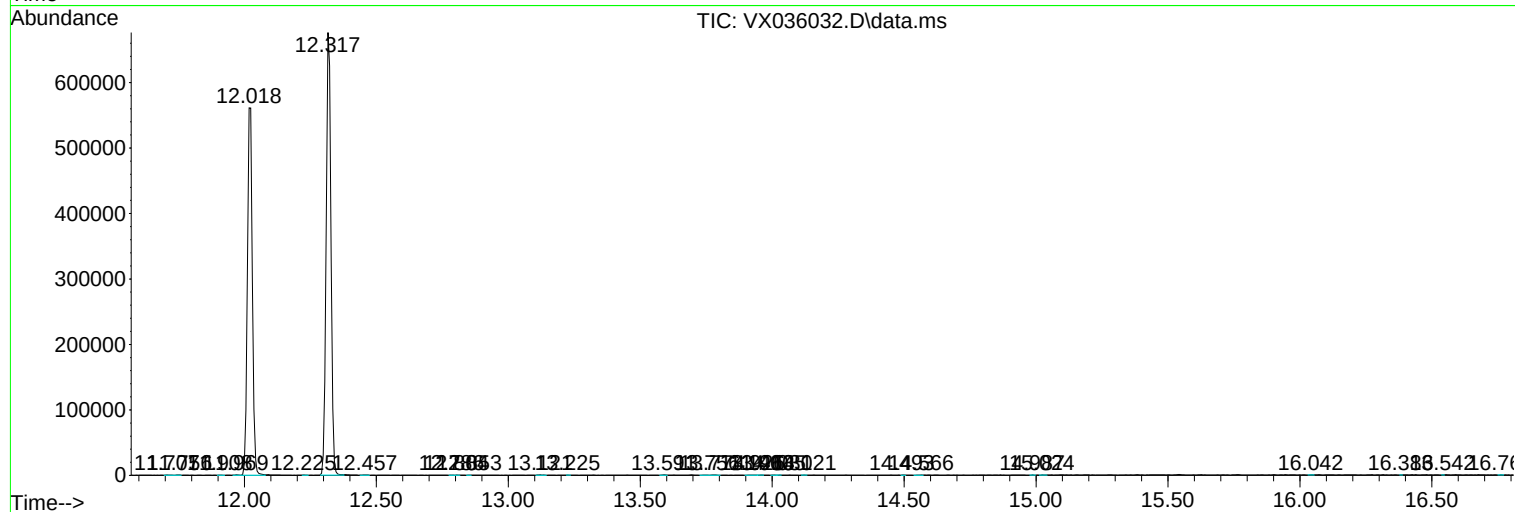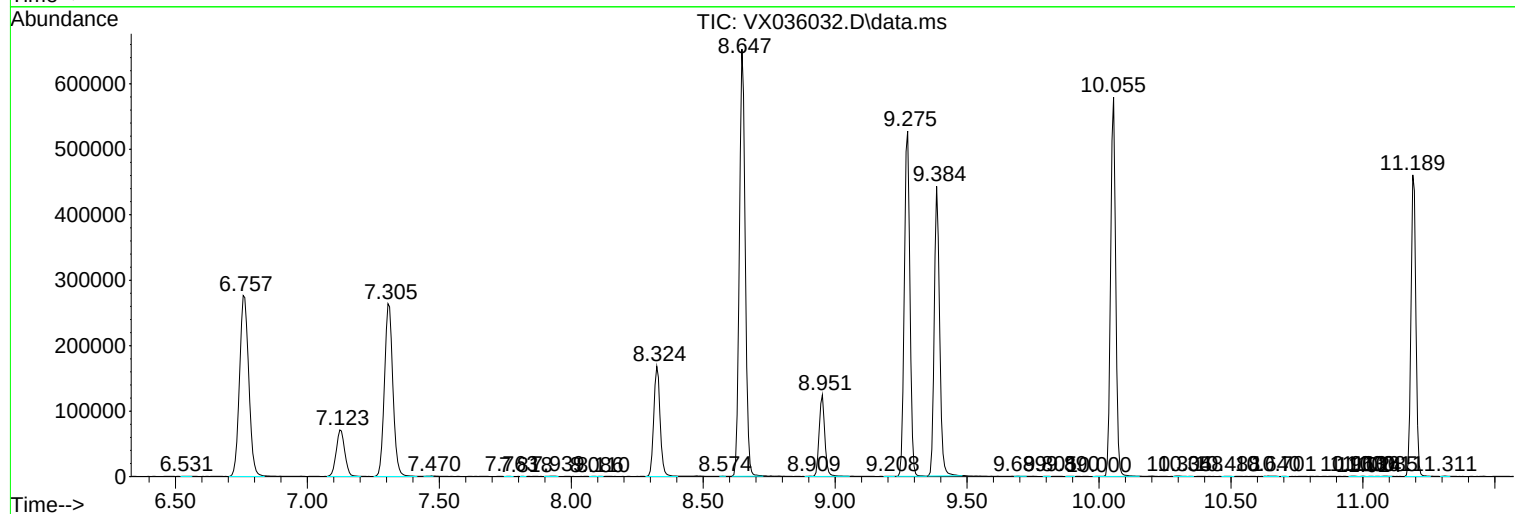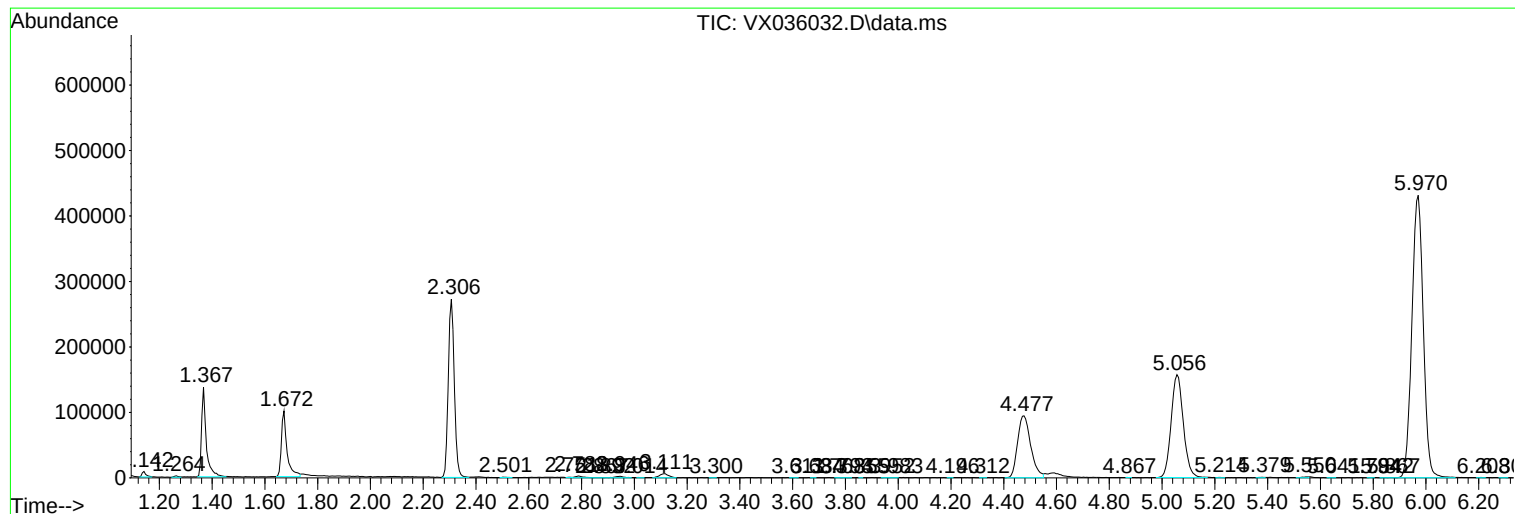

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036032.D
Acq On : 06 Jun 2023 15:01
Operator : JC/MD
Sample : 02991-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036032.D
Acq On : 06 Jun 2023 15:01
Operator : JC/MD
Sample : 02991-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------