

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036033.D
 Acq On : 06 Jun 2023 15:24
 Operator : JC/MD
 Sample : 02991-03 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M

Title : VOC Analysis

Signal : TIC: VX036033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rVB	8847	9260	0.85%	0.106%
2	1.264	26	29	32	rBV2	1505	1932	0.18%	0.022%
3	1.368	42	46	59	rBV	105733	135378	12.46%	1.552%
4	1.673	91	96	114	rBV	80952	132211	12.17%	1.516%
5	2.307	194	200	211	rVB	222955	348482	32.08%	3.996%
6	2.575	243	244	245	rBV	375	245	0.02%	0.003%
7	2.794	276	280	285	rVB4	1700	2702	0.25%	0.031%
8	2.941	297	304	311	rBV2	3661	7840	0.72%	0.090%
9	3.111	324	332	342	rBV2	25860	59845	5.51%	0.686%
10	3.245	352	354	356	rVB	312	277	0.03%	0.003%
11	3.270	356	358	360	rBV2	266	316	0.03%	0.004%
12	3.447	384	387	389	rVB3	302	312	0.03%	0.004%
13	3.550	400	404	405	rVV2	172	220	0.02%	0.003%
14	3.629	414	417	420	rBV	262	290	0.03%	0.003%
15	3.684	423	426	428	rBV	334	272	0.03%	0.003%
16	3.922	460	465	467	rBV	228	280	0.03%	0.003%
17	3.971	471	473	474	rBV2	264	252	0.02%	0.003%
18	4.087	490	492	496	rBV	250	268	0.02%	0.003%
19	4.209	510	512	514	rBV2	209	212	0.02%	0.002%
20	4.349	531	535	537	rBV	217	224	0.02%	0.003%
21	4.477	544	556	569	rBV2	106469	360420	33.18%	4.133%
22	5.056	638	651	669	rBV	138337	433184	39.88%	4.967%
23	5.391	700	706	708	rBV3	964	1705	0.16%	0.020%
24	5.458	715	717	718	rBV	351	266	0.02%	0.003%
25	5.556	726	733	739	rBV4	1959	5086	0.47%	0.058%
26	5.647	746	748	751	rBV	277	257	0.02%	0.003%
27	5.727	760	761	764	rBV2	317	313	0.03%	0.004%
28	5.757	764	766	769	rVV2	190	233	0.02%	0.003%
29	5.879	783	786	788	rBV2	242	250	0.02%	0.003%
30	5.971	788	801	818	rBV2	360404	1086324	100.00%	12.457%
31	6.446	876	879	881	rVB3	241	230	0.02%	0.003%
32	6.623	905	908	910	rBV2	378	455	0.04%	0.005%
33	6.757	919	930	943	rBV	239915	586066	53.95%	6.721%
34	6.909	953	955	959	rVB2	330	329	0.03%	0.004%
35	6.976	964	966	969	rVB2	338	318	0.03%	0.004%
36	7.025	972	974	976	rVB2	341	287	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036033.D
 Acq On : 06 Jun 2023 15:24
 Operator : JC/MD
 Sample : 02991-03 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.123	983	990	1001	rVB3	27245	61700	5.68%	0.708%
38	7.202	1001	1003	1006	rVB2	297	316	0.03%	0.004%
39	7.306	1010	1020	1037	rBV	230918	503257	46.33%	5.771%
40	7.482	1041	1049	1057	rVB5	894	2026	0.19%	0.023%
41	7.635	1072	1074	1078	rBV	179	245	0.02%	0.003%
42	7.915	1118	1120	1121	rBV	433	250	0.02%	0.003%
43	8.062	1143	1144	1147	rBV	211	257	0.02%	0.003%
44	8.098	1148	1150	1155	rVB3	468	624	0.06%	0.007%
45	8.238	1171	1173	1175	rBV2	235	271	0.02%	0.003%
46	8.324	1180	1187	1200	rBV	140184	227784	20.97%	2.612%
47	8.574	1227	1228	1233	rBV2	457	549	0.05%	0.006%
48	8.647	1233	1240	1256	rVV	529200	837432	77.09%	9.603%
49	8.879	1276	1278	1281	rVV2	188	215	0.02%	0.002%
50	8.952	1284	1290	1307	rVB	102099	152409	14.03%	1.748%
51	9.220	1332	1334	1336	rBV	369	264	0.02%	0.003%
52	9.269	1336	1342	1355	rVB	425010	643472	59.23%	7.379%
53	9.385	1355	1361	1374	rBV	405229	573391	52.78%	6.575%
54	9.580	1391	1393	1396	rVB3	618	604	0.06%	0.007%
55	9.720	1414	1416	1417	rBV	285	224	0.02%	0.003%
56	10.055	1465	1471	1488	rVB	502227	686120	63.16%	7.868%
57	10.305	1509	1512	1517	rVB2	1065	1440	0.13%	0.017%
58	10.762	1585	1587	1590	rBV2	225	239	0.02%	0.003%
59	10.964	1616	1620	1622	rBV3	336	368	0.03%	0.004%
60	11.012	1625	1628	1630	rBV3	325	305	0.03%	0.003%
61	11.085	1635	1640	1644	rBV4	737	1104	0.10%	0.013%
62	11.189	1652	1657	1669	rBV	409608	521622	48.02%	5.982%
63	11.305	1674	1676	1681	rVB3	463	539	0.05%	0.006%
64	11.354	1681	1684	1685	rBV	250	227	0.02%	0.003%
65	11.421	1693	1695	1698	rBV	275	227	0.02%	0.003%
66	11.451	1698	1700	1701	rVV	532	347	0.03%	0.004%
67	11.640	1729	1731	1733	rBV2	402	351	0.03%	0.004%
68	11.707	1740	1742	1746	rVB2	507	627	0.06%	0.007%
69	11.756	1746	1750	1753	rBV2	473	579	0.05%	0.007%
70	11.963	1782	1784	1788	rVB2	746	778	0.07%	0.009%
71	12.018	1788	1793	1805	rBV	490416	621976	57.26%	7.132%
72	12.140	1811	1813	1815	rVB2	504	278	0.03%	0.003%
73	12.232	1825	1828	1832	rVB2	299	248	0.02%	0.003%
74	12.317	1837	1842	1853	rVV	533863	688234	63.35%	7.892%
75	12.469	1863	1867	1872	rVB5	511	962	0.09%	0.011%
76	13.109	1970	1972	1975	rVB	445	464	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036033.D
 Acq On : 06 Jun 2023 15:24
 Operator : JC/MD
 Sample : 02991-03 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C06

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	13.201	1986	1987	1990	rVV	356	283	0.03%	0.003%
78	13.238	1990	1993	1997	rVB3	1417	1898	0.17%	0.022%
79	13.561	2043	2046	2048	rBV2	283	304	0.03%	0.003%
80	13.591	2048	2051	2053	rBV2	461	448	0.04%	0.005%
81	13.634	2056	2058	2061	rVB3	326	341	0.03%	0.004%
82	13.664	2061	2063	2066	rBV	193	253	0.02%	0.003%
83	13.689	2066	2067	2070	rVB3	488	381	0.04%	0.004%
84	13.780	2078	2082	2085	rBV2	506	622	0.06%	0.007%
85	14.054	2124	2127	2130	rBV2	232	303	0.03%	0.003%
86	14.091	2130	2133	2136	rBV2	295	384	0.04%	0.004%
87	14.207	2148	2152	2154	rBV2	248	295	0.03%	0.003%
88	14.243	2156	2158	2160	rBV	246	220	0.02%	0.003%
89	14.298	2166	2167	2169	rBV	419	272	0.03%	0.003%
90	14.426	2186	2188	2192	rVV	240	321	0.03%	0.004%
91	14.469	2192	2195	2197	rVB3	351	384	0.04%	0.004%
92	14.670	2227	2228	2229	rBV	387	258	0.02%	0.003%
93	15.079	2294	2295	2297	rBV	384	328	0.03%	0.004%
94	15.115	2299	2301	2302	rBV	454	323	0.03%	0.004%
95	15.170	2308	2310	2311	rBV	461	344	0.03%	0.004%
96	15.542	2369	2371	2376	rVB4	910	1375	0.13%	0.016%
97	15.963	2438	2440	2441	rBV	495	295	0.03%	0.003%
98	16.139	2467	2469	2470	rBV	667	434	0.04%	0.005%
99	16.188	2475	2477	2481	rVB3	583	691	0.06%	0.008%
100	16.615	2543	2547	2550	rBV3	634	941	0.09%	0.011%


Sum of corrected areas: 8720564

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036033.D
Acq On : 06 Jun 2023 15:24
Operator : JC/MD
Sample : 02991-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

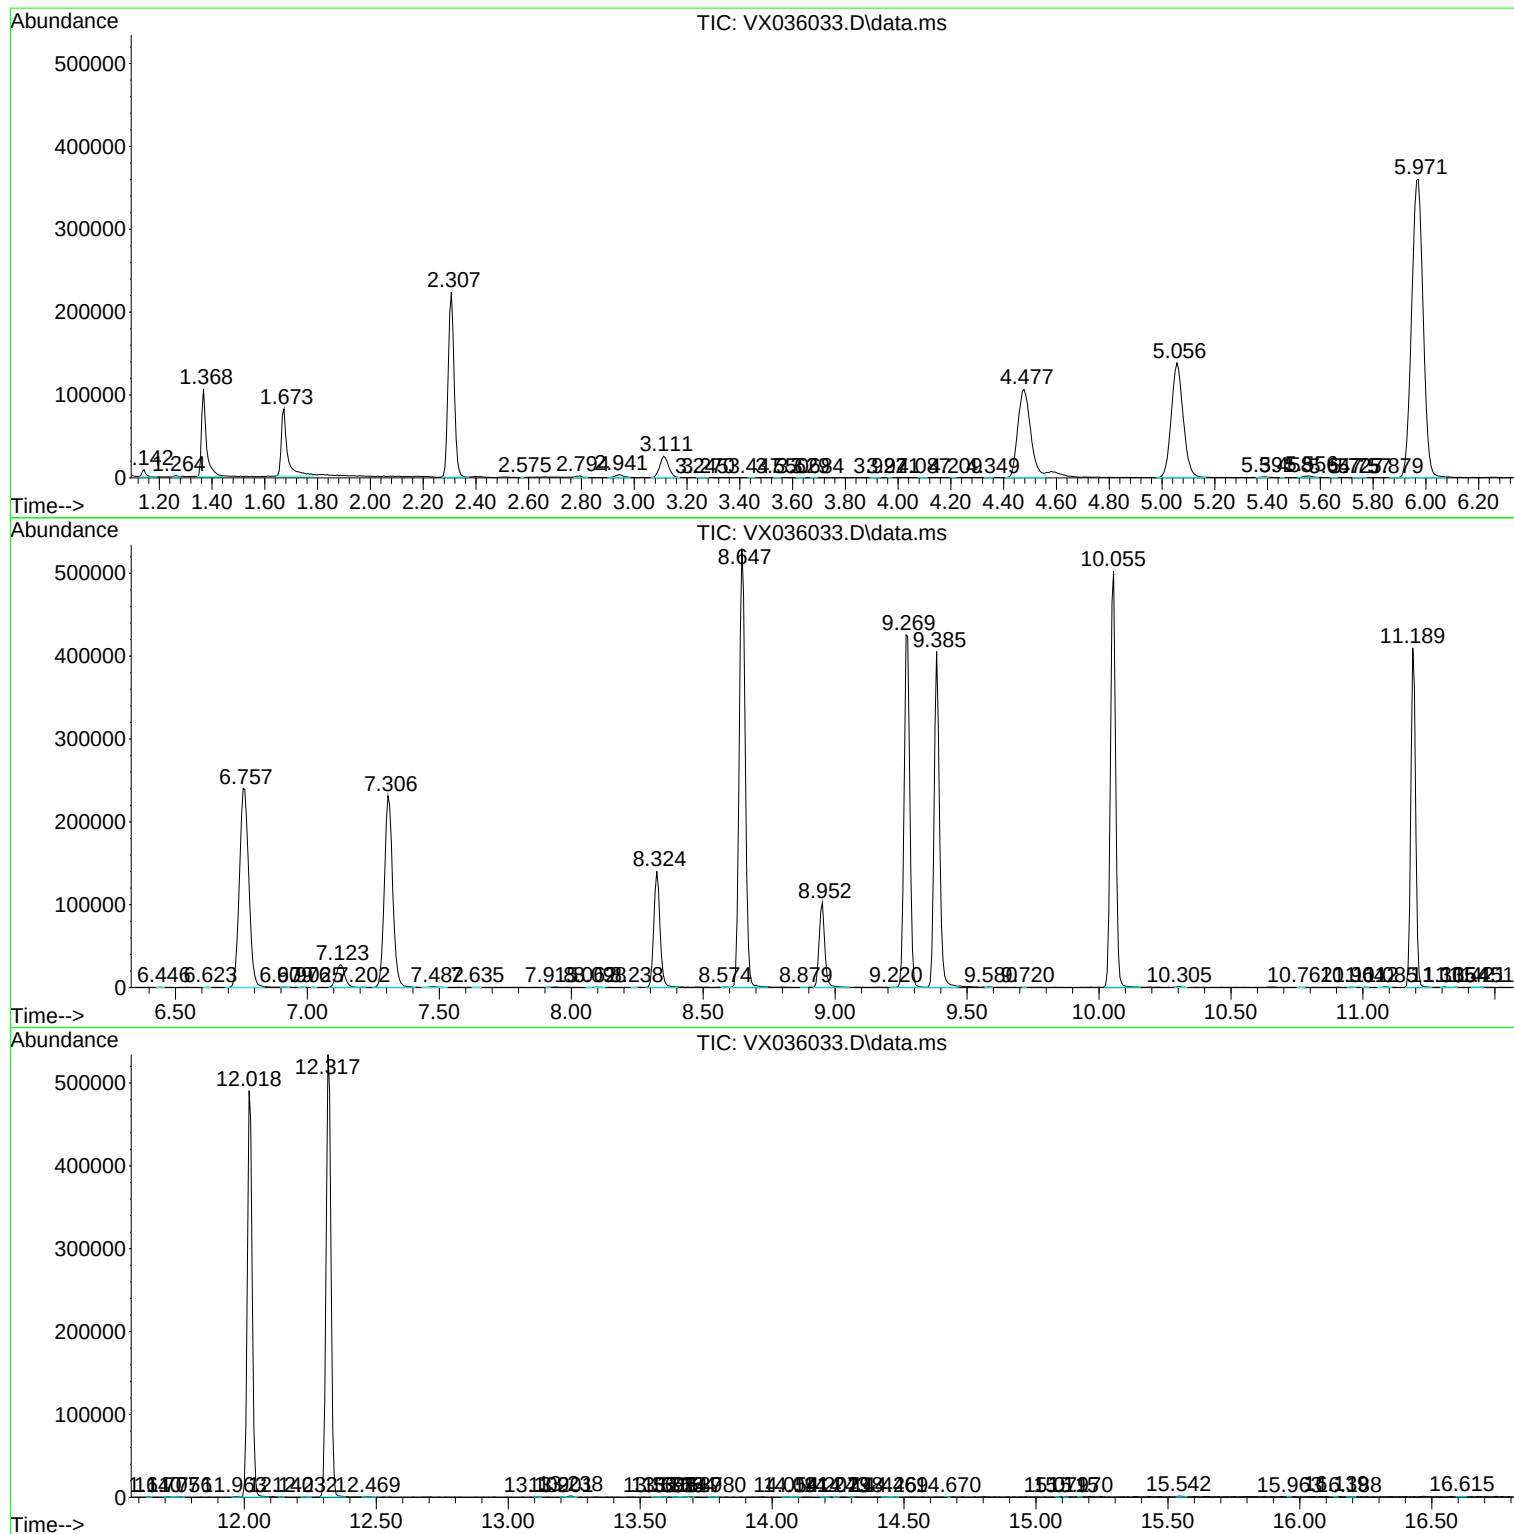

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036033.D
Acq On : 06 Jun 2023 15:24
Operator : JC/MD
Sample : 02991-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036033.D
Acq On : 06 Jun 2023 15:24
Operator : JC/MD
Sample : 02991-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------