

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036036.D
 Acq On : 06 Jun 2023 16:34
 Operator : JC/MD
 Sample : VIBLK628
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rVB2	9661	11348	0.81%	0.108%
2	1.264	27	29	32	rBV2	1742	2073	0.15%	0.020%
3	1.368	42	46	60	rBV	151089	188660	13.43%	1.801%
4	1.672	91	96	115	rBV	107689	177153	12.61%	1.691%
5	2.306	194	200	212	rVB	314680	495164	35.26%	4.728%
6	2.508	230	233	240	rVB	3567	5632	0.40%	0.054%
7	2.721	263	268	272	rBV3	934	1832	0.13%	0.017%
8	2.794	275	280	287	rVB2	3445	6031	0.43%	0.058%
9	2.873	292	293	298	rVB	361	341	0.02%	0.003%
10	2.947	298	305	311	rVB3	1274	3157	0.22%	0.030%
11	3.014	313	316	318	rBV3	217	307	0.02%	0.003%
12	3.099	323	330	341	rVB7	2890	8364	0.60%	0.080%
13	3.178	341	343	347	rBV3	292	380	0.03%	0.004%
14	3.599	410	412	415	rBV	449	576	0.04%	0.005%
15	3.757	436	438	442	rVB2	258	357	0.03%	0.003%
16	4.001	477	478	481	rVB	291	229	0.02%	0.002%
17	4.080	488	491	493	rBV2	286	346	0.02%	0.003%
18	4.391	540	542	544	rBV2	269	250	0.02%	0.002%
19	4.471	545	555	570	rBV	94974	304843	21.71%	2.910%
20	4.904	619	626	632	rBV3	891	2252	0.16%	0.022%
21	5.056	636	651	670	rVV	180746	553002	39.38%	5.280%
22	5.208	674	676	679	rVV2	271	242	0.02%	0.002%
23	5.391	697	706	713	rBV6	2351	6935	0.49%	0.066%
24	5.464	714	718	720	rBV2	1342	1735	0.12%	0.017%
25	5.550	727	732	743	rVB2	3936	9174	0.65%	0.088%
26	5.659	745	750	751	rBV	860	982	0.07%	0.009%
27	5.757	764	766	768	rBV2	280	221	0.02%	0.002%
28	5.842	778	780	781	rBV2	267	244	0.02%	0.002%
29	5.970	786	801	819	rBV2	473148	1404400	100.00%	13.408%
30	6.214	839	841	843	rBV2	211	222	0.02%	0.002%
31	6.757	919	930	948	rBV	321447	784997	55.90%	7.495%
32	6.989	966	968	970	rVB	276	254	0.02%	0.002%
33	7.056	977	979	981	rVB2	320	248	0.02%	0.002%
34	7.117	981	989	1001	rBV5	3497	9435	0.67%	0.090%
35	7.208	1001	1004	1007	rVB2	228	311	0.02%	0.003%
36	7.306	1011	1020	1030	rBV	287072	633820	45.13%	6.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036036.D
 Acq On : 06 Jun 2023 16:34
 Operator : JC/MD
 Sample : VIBLK628
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.769	1094	1096	1099	rBV2	194	236	0.02%	0.002%
38	7.830	1099	1106	1111	rVB3	1084	1902	0.14%	0.018%
39	7.891	1111	1116	1119	rBV2	289	391	0.03%	0.004%
40	7.927	1119	1122	1123	rBV	705	594	0.04%	0.006%
41	8.098	1149	1150	1152	rBV2	296	215	0.02%	0.002%
42	8.238	1170	1173	1174	rBV	291	231	0.02%	0.002%
43	8.324	1180	1187	1199	rBV	186627	307592	21.90%	2.937%
44	8.476	1208	1212	1220	rVB6	494	1290	0.09%	0.012%
45	8.580	1224	1229	1233	rVB4	2497	4081	0.29%	0.039%
46	8.647	1233	1240	1249	rBV	731214	1132049	80.61%	10.808%
47	8.952	1284	1290	1303	rBV	130232	199661	14.22%	1.906%
48	9.153	1319	1323	1328	rVB3	1783	2509	0.18%	0.024%
49	9.275	1338	1343	1348	rBV2	6001	9511	0.68%	0.091%
50	9.384	1355	1361	1377	rBV	479701	677260	48.22%	6.466%
51	9.567	1389	1391	1394	rVB3	476	376	0.03%	0.004%
52	9.616	1394	1399	1402	rVB4	1056	1729	0.12%	0.017%
53	9.695	1410	1412	1417	rBV4	975	1496	0.11%	0.014%
54	9.823	1428	1433	1434	rBV3	355	345	0.02%	0.003%
55	9.982	1458	1459	1465	rBV2	208	311	0.02%	0.003%
56	10.055	1465	1471	1485	rBV	671673	918492	65.40%	8.769%
57	10.153	1485	1487	1489	rVV2	417	361	0.03%	0.003%
58	10.195	1489	1494	1500	rVB2	5066	7075	0.50%	0.068%
59	10.305	1507	1512	1516	rBV2	5076	7000	0.50%	0.067%
60	10.427	1528	1532	1535	rBV3	233	361	0.03%	0.003%
61	10.463	1535	1538	1539	rBV2	196	228	0.02%	0.002%
62	10.652	1563	1569	1575	rVB3	6112	12613	0.90%	0.120%
63	10.799	1590	1593	1597	rVB3	711	742	0.05%	0.007%
64	10.896	1606	1609	1611	rBV2	318	283	0.02%	0.003%
65	10.933	1613	1615	1616	rVV	383	248	0.02%	0.002%
66	10.963	1616	1620	1628	rVB	5428	7038	0.50%	0.067%
67	11.085	1638	1640	1645	rVB	758	709	0.05%	0.007%
68	11.189	1651	1657	1663	rBV	498443	649906	46.28%	6.205%
69	11.317	1674	1678	1681	rVB3	346	629	0.04%	0.006%
70	11.451	1694	1700	1705	rBV2	5400	6993	0.50%	0.067%
71	11.591	1720	1723	1726	rBV3	259	446	0.03%	0.004%
72	11.707	1740	1742	1745	rVB3	642	677	0.05%	0.006%
73	11.750	1746	1749	1753	rBV2	5269	5736	0.41%	0.055%
74	11.921	1776	1777	1780	rBV2	289	292	0.02%	0.003%
75	11.969	1780	1785	1788	rBV	6124	7560	0.54%	0.072%
76	12.024	1788	1794	1804	rVB	681954	887975	63.23%	8.478%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036036.D
 Acq On : 06 Jun 2023 16:34
 Operator : JC/MD
 Sample : VIBLK628
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.207	1821	1824	1825	rBV2	242	250	0.02%	0.002%
78	12.250	1828	1831	1833	rBV2	226	217	0.02%	0.002%
79	12.317	1837	1842	1853	rVV	751597	956640	68.12%	9.133%
80	12.463	1864	1866	1869	rBV3	335	370	0.03%	0.004%
81	12.561	1880	1882	1885	rBV2	247	280	0.02%	0.003%
82	12.670	1896	1900	1903	rBV	210	380	0.03%	0.004%
83	12.939	1941	1944	1948	rBV4	768	980	0.07%	0.009%
84	13.109	1968	1972	1977	rBV3	6958	8243	0.59%	0.079%
85	13.152	1977	1979	1981	rVB	310	238	0.02%	0.002%
86	13.189	1981	1985	1987	rBV2	283	395	0.03%	0.004%
87	13.591	2046	2051	2058	rVB	7198	8878	0.63%	0.085%
88	13.689	2066	2067	2070	rVB	503	318	0.02%	0.003%
89	13.774	2077	2081	2085	rBV	6981	9057	0.64%	0.086%
90	13.963	2108	2112	2118	rBV	6528	8821	0.63%	0.084%
91	14.195	2147	2150	2151	rBV	317	280	0.02%	0.003%
92	14.292	2163	2166	2167	rBV2	412	399	0.03%	0.004%
93	14.329	2171	2172	2175	rBV	476	467	0.03%	0.004%
94	15.182	2310	2312	2318	rVB3	551	651	0.05%	0.006%
95	15.542	2367	2371	2376	rVB3	1303	2093	0.15%	0.020%
96	15.585	2376	2378	2379	rBV	527	341	0.02%	0.003%
97	15.932	2433	2435	2439	rBV3	538	800	0.06%	0.008%
98	16.383	2507	2509	2510	rBV	481	255	0.02%	0.002%
99	16.487	2524	2526	2527	rVB2	590	301	0.02%	0.003%
100	16.542	2533	2535	2538	rBV2	677	657	0.05%	0.006%




Sum of corrected areas: 10473971

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036036.D
Acq On : 06 Jun 2023 16:34
Operator : JC/MD
Sample : VIBLK628
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK628

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

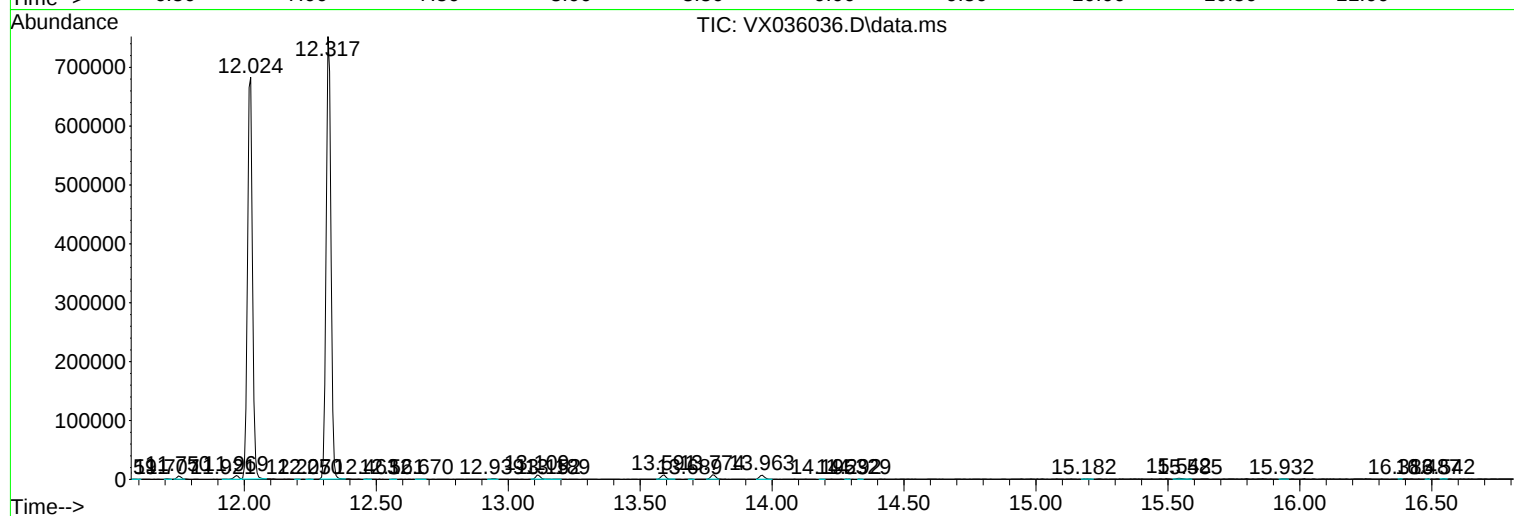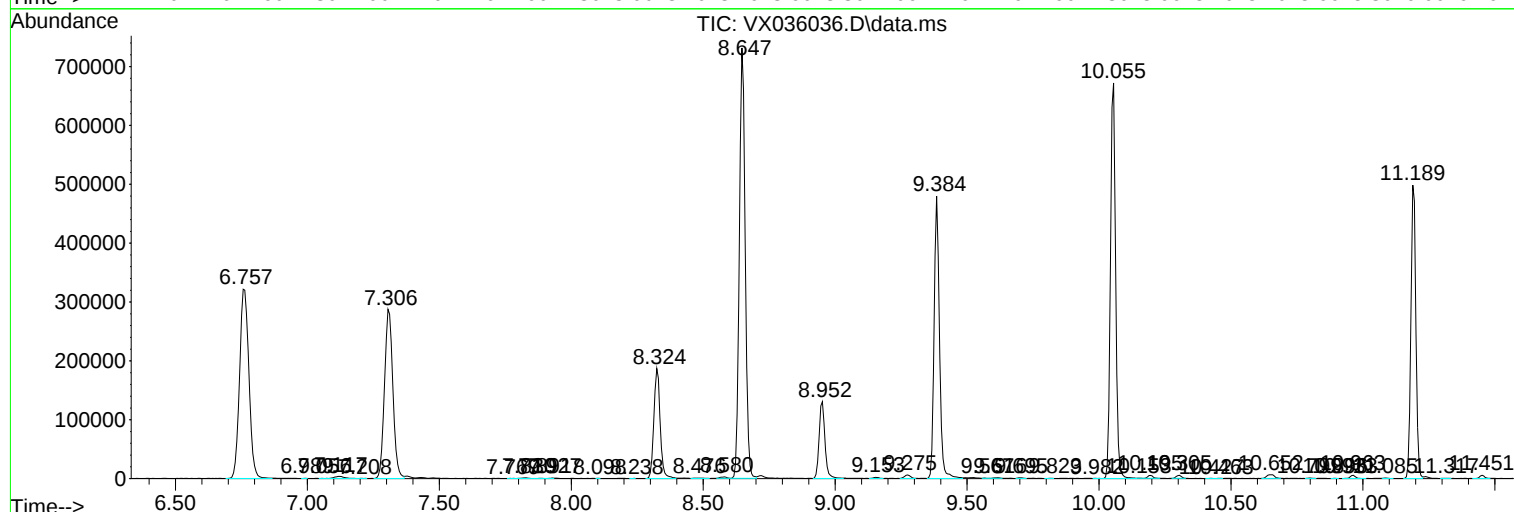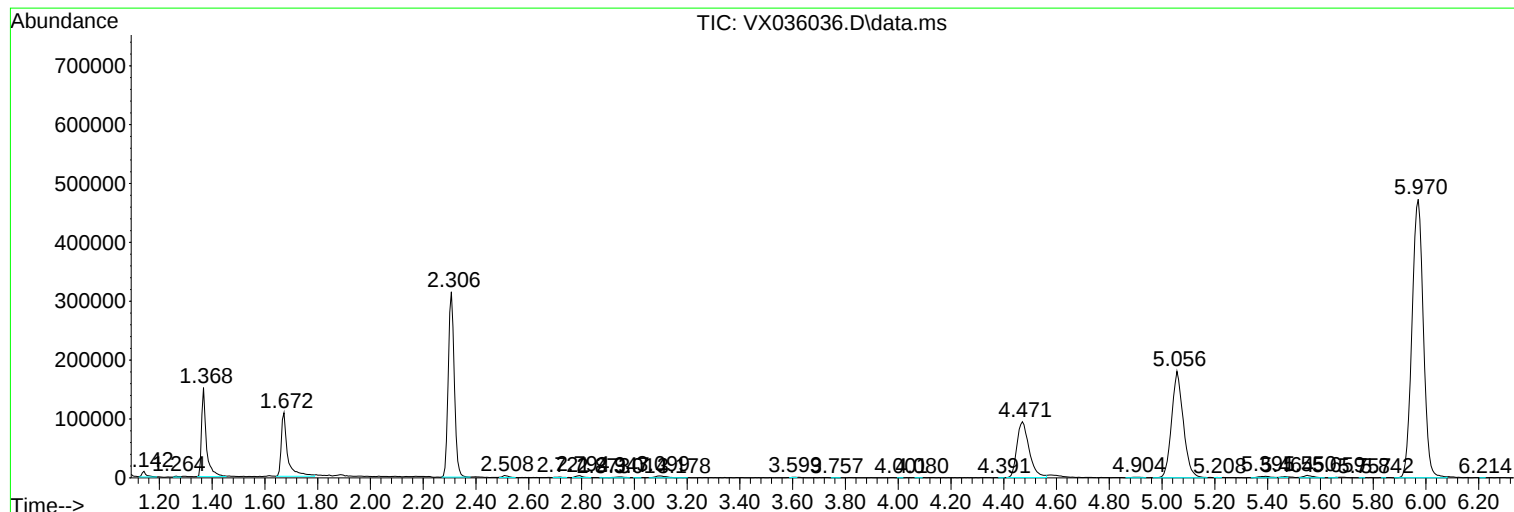

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036036.D
Acq On : 06 Jun 2023 16:34
Operator : JC/MD
Sample : VIBLK628
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK628

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036036.D
Acq On : 06 Jun 2023 16:34
Operator : JC/MD
Sample : VIBLK628
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK628

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------