

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036037.D
 Acq On : 06 Jun 2023 16:58
 Operator : JC/MD
 Sample : 02991-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	9284	10135	0.75%	0.102%
2	1.264	26	29	32	rBV2	1858	1976	0.15%	0.020%
3	1.368	42	46	61	rBV	140874	174253	12.83%	1.754%
4	1.611	84	86	88	rBV2	1189	1127	0.08%	0.011%
5	1.672	91	96	111	rBV	99714	158237	11.65%	1.593%
6	2.306	194	200	210	rBV	299778	466678	34.37%	4.699%
7	2.520	229	235	237	rBV2	1304	2323	0.17%	0.023%
8	2.709	262	266	268	rBV2	455	553	0.04%	0.006%
9	2.788	275	279	281	rBV3	1071	1552	0.11%	0.016%
10	2.947	302	305	309	rVB2	410	444	0.03%	0.004%
11	3.014	315	316	318	rBV	316	250	0.02%	0.003%
12	3.099	324	330	335	rBV3	766	1563	0.12%	0.016%
13	4.251	517	519	522	rVB	369	271	0.02%	0.003%
14	4.465	545	554	572	rBV2	90329	301440	22.20%	3.035%
15	4.940	628	632	634	rBV3	161	264	0.02%	0.003%
16	5.056	639	651	667	rBV	166939	539439	39.73%	5.431%
17	5.373	698	703	704	rBV	1347	1503	0.11%	0.015%
18	5.464	717	718	721	rVB	339	279	0.02%	0.003%
19	5.550	725	732	741	rVB4	2930	7780	0.57%	0.078%
20	5.660	748	750	752	rBV	320	212	0.02%	0.002%
21	5.781	766	770	771	rBV2	243	256	0.02%	0.003%
22	5.885	785	787	788	rVV	272	214	0.02%	0.002%
23	5.970	788	801	831	rVV2	449662	1357840	100.00%	13.672%
24	6.159	831	832	837	rVB3	419	511	0.04%	0.005%
25	6.239	844	845	848	rBV2	275	239	0.02%	0.002%
26	6.275	848	851	853	rBV2	354	294	0.02%	0.003%
27	6.464	877	882	885	rVB3	355	657	0.05%	0.007%
28	6.513	888	890	891	rBV2	330	217	0.02%	0.002%
29	6.763	919	931	948	rBV	319143	758125	55.83%	7.633%
30	7.050	977	978	982	rVB	273	265	0.02%	0.003%
31	7.117	982	989	997	rBV6	2041	4821	0.36%	0.049%
32	7.312	1009	1021	1042	rBV	281170	630071	46.40%	6.344%
33	7.482	1044	1049	1054	rVV5	845	1229	0.09%	0.012%
34	7.586	1062	1066	1067	rBV3	221	246	0.02%	0.002%
35	7.818	1102	1104	1109	rVB2	364	406	0.03%	0.004%
36	7.927	1119	1122	1128	rVB3	657	1052	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036037.D
 Acq On : 06 Jun 2023 16:58
 Operator : JC/MD
 Sample : 02991-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	8.281	1178	1180	1181	rBV	281	233	0.02%	0.002%
38	8.324	1181	1187	1201	rVV	175439	290476	21.39%	2.925%
39	8.470	1208	1211	1212	rBV2	394	423	0.03%	0.004%
40	8.647	1233	1240	1256	rBV	675463	1064264	78.38%	10.716%
41	8.878	1277	1278	1280	rVB	522	297	0.02%	0.003%
42	8.909	1280	1283	1284	rVB	407	354	0.03%	0.004%
43	8.952	1284	1290	1301	rBV	131463	193770	14.27%	1.951%
44	9.183	1327	1328	1330	rBV2	313	235	0.02%	0.002%
45	9.275	1339	1343	1347	rVB3	2421	2970	0.22%	0.030%
46	9.384	1355	1361	1378	rBV	478112	666661	49.10%	6.712%
47	9.701	1410	1413	1417	rBV3	1759	1981	0.15%	0.020%
48	9.756	1421	1422	1428	rVB3	499	515	0.04%	0.005%
49	9.817	1430	1432	1434	rBV2	354	364	0.03%	0.004%
50	9.890	1442	1444	1447	rVB2	196	210	0.02%	0.002%
51	10.055	1465	1471	1488	rBV	651226	879701	64.79%	8.857%
52	10.244	1499	1502	1506	rVB2	580	904	0.07%	0.009%
53	10.305	1508	1512	1517	rVV2	1212	1724	0.13%	0.017%
54	10.378	1523	1524	1529	rBV2	228	310	0.02%	0.003%
55	10.415	1529	1530	1534	rBV2	279	292	0.02%	0.003%
56	10.659	1562	1570	1575	rBV4	1393	2595	0.19%	0.026%
57	10.793	1591	1592	1595	rBV2	242	217	0.02%	0.002%
58	10.848	1599	1601	1604	rVV2	199	202	0.01%	0.002%
59	10.890	1606	1608	1612	rBV2	300	290	0.02%	0.003%
60	10.921	1612	1613	1617	rBV2	221	226	0.02%	0.002%
61	10.963	1617	1620	1624	rBV3	860	1040	0.08%	0.010%
62	11.031	1629	1631	1634	rVV2	216	260	0.02%	0.003%
63	11.061	1634	1636	1637	rVV	283	243	0.02%	0.002%
64	11.085	1637	1640	1644	rVB3	684	988	0.07%	0.010%
65	11.189	1652	1657	1668	rBV	494429	633938	46.69%	6.383%
66	11.311	1676	1677	1679	rBV2	278	230	0.02%	0.002%
67	11.451	1697	1700	1705	rVB2	788	982	0.07%	0.010%
68	11.494	1705	1707	1711	rVB2	287	256	0.02%	0.003%
69	11.701	1739	1741	1744	rVV2	456	477	0.04%	0.005%
70	11.756	1747	1750	1754	rVV3	1019	1153	0.08%	0.012%
71	11.969	1781	1785	1788	rBV4	1703	1841	0.14%	0.019%
72	12.024	1788	1794	1804	rVV	642527	840742	61.92%	8.465%
73	12.116	1807	1809	1812	rVB2	431	445	0.03%	0.004%
74	12.201	1821	1823	1825	rBV2	391	340	0.03%	0.003%
75	12.317	1837	1842	1849	rBV	707177	897523	66.10%	9.037%
76	12.609	1887	1890	1892	rVB2	232	258	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036037.D
 Acq On : 06 Jun 2023 16:58
 Operator : JC/MD
 Sample : 02991-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.640	1892	1895	1896	rBV	235	293	0.02%	0.003%
78	13.006	1953	1955	1959	rVB3	329	383	0.03%	0.004%
79	13.115	1970	1973	1977	rBV3	1214	1477	0.11%	0.015%
80	13.341	2008	2010	2013	rVB3	327	239	0.02%	0.002%
81	13.585	2047	2050	2054	rVB4	1663	2248	0.17%	0.023%
82	13.622	2054	2056	2060	rBV2	264	241	0.02%	0.002%
83	13.780	2079	2082	2087	rVB2	1191	1239	0.09%	0.012%
84	13.963	2109	2112	2116	rVB2	1478	1675	0.12%	0.017%
85	14.237	2155	2157	2161	rVB	469	528	0.04%	0.005%
86	14.280	2161	2164	2169	rBV2	488	679	0.05%	0.007%
87	14.323	2169	2171	2174	rVB2	402	331	0.02%	0.003%
88	14.390	2180	2182	2185	rVB2	339	248	0.02%	0.002%
89	14.463	2192	2194	2197	rVB	463	298	0.02%	0.003%
90	14.536	2203	2206	2207	rBV	388	335	0.02%	0.003%
91	14.554	2207	2209	2211	rVV2	296	229	0.02%	0.002%
92	15.066	2291	2293	2296	rBV3	457	429	0.03%	0.004%
93	15.097	2296	2298	2299	rBV2	416	282	0.02%	0.003%
94	15.274	2326	2327	2329	rBV	404	407	0.03%	0.004%
95	15.548	2369	2372	2377	rVB6	893	1279	0.09%	0.013%
96	15.798	2410	2413	2415	rBV	927	866	0.06%	0.009%
97	15.938	2434	2436	2438	rBV2	488	402	0.03%	0.004%
98	15.999	2444	2446	2449	rBV2	433	501	0.04%	0.005%
99	16.566	2537	2539	2540	rBV	419	232	0.02%	0.002%
100	16.603	2544	2545	2546	rBV	565	316	0.02%	0.003%




Sum of corrected areas: 9931809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036037.D
Acq On : 06 Jun 2023 16:58
Operator : JC/MD
Sample : 02991-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

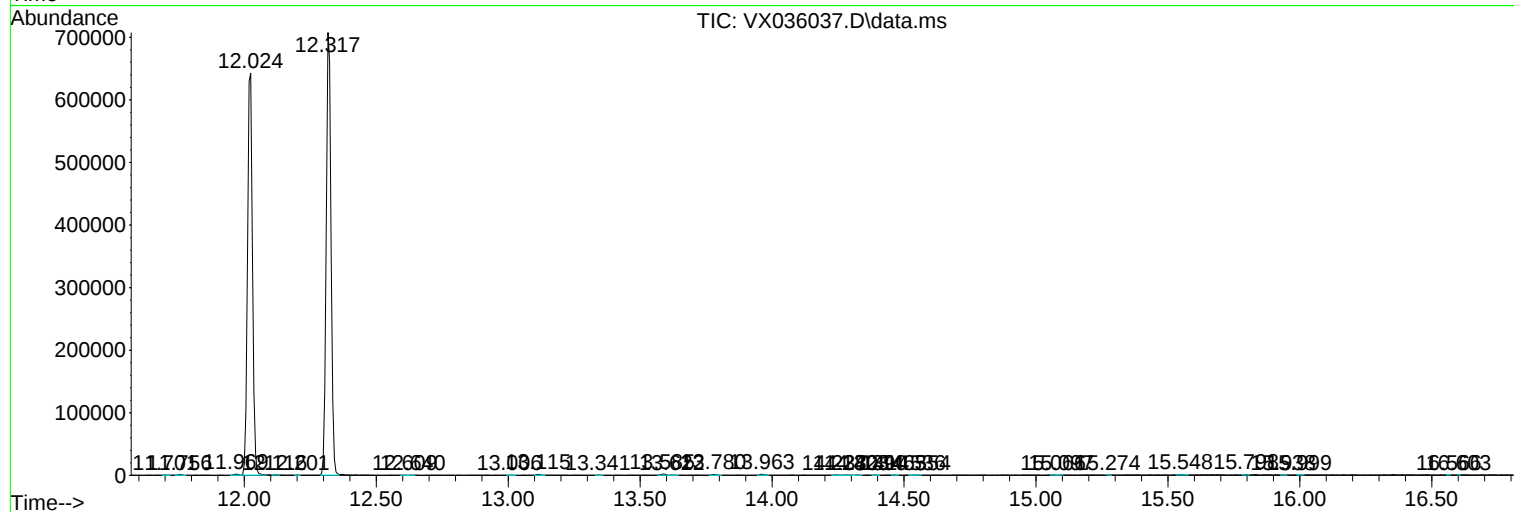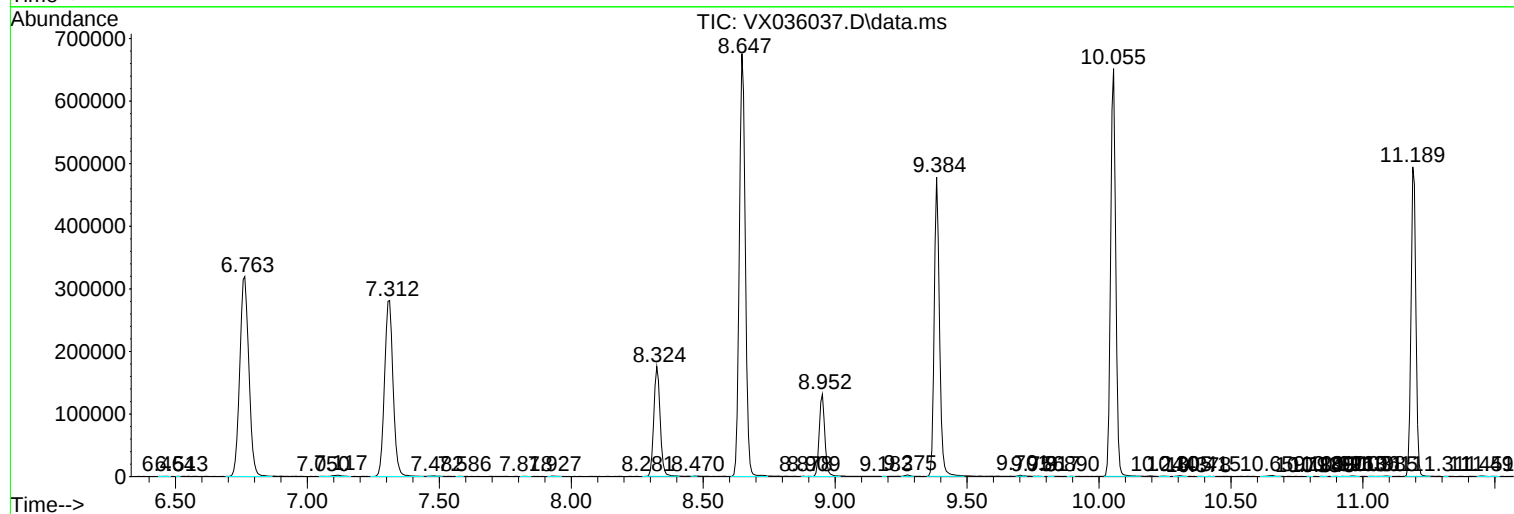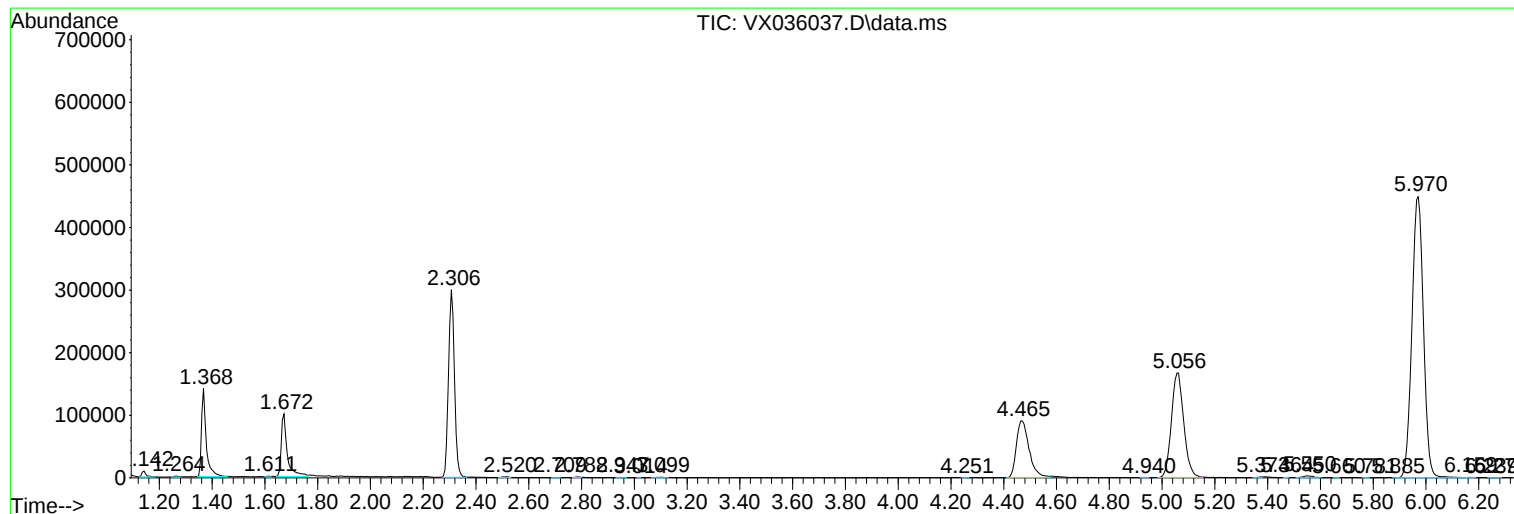

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036037.D
Acq On : 06 Jun 2023 16:58
Operator : JC/MD
Sample : 02991-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036037.D
Acq On : 06 Jun 2023 16:58
Operator : JC/MD
Sample : 02991-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------