

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036038.D
 Acq On : 06 Jun 2023 17:21
 Operator : JC/MD
 Sample : 02992-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB2	8852	10584	0.80%	0.104%
2	1.264	26	29	32	rBV2	2158	1992	0.15%	0.020%
3	1.368	42	46	59	rBV	123389	154616	11.66%	1.516%
4	1.672	91	96	115	rBV	93560	152570	11.50%	1.496%
5	2.307	193	200	211	rBV	257555	405444	30.56%	3.977%
6	2.514	229	234	238	rVB	2083	2979	0.22%	0.029%
7	2.788	274	279	289	rVB4	2478	5044	0.38%	0.049%
8	2.916	298	300	301	rBV2	231	208	0.02%	0.002%
9	2.947	301	305	307	rVV4	451	781	0.06%	0.008%
10	3.093	324	329	330	rBV2	3821	4677	0.35%	0.046%
11	3.215	347	349	352	rBV3	284	353	0.03%	0.003%
12	3.264	356	357	361	rVV2	348	349	0.03%	0.003%
13	3.294	361	362	365	rVB2	310	260	0.02%	0.003%
14	3.508	393	397	399	rVB2	200	242	0.02%	0.002%
15	3.611	408	414	420	rVB4	987	1999	0.15%	0.020%
16	3.739	433	435	440	rVV2	267	368	0.03%	0.004%
17	3.849	450	453	456	rBV2	184	270	0.02%	0.003%
18	3.904	459	462	464	rBV3	162	239	0.02%	0.002%
19	4.001	477	478	481	rBV	229	213	0.02%	0.002%
20	4.135	497	500	504	rBV2	274	297	0.02%	0.003%
21	4.178	504	507	510	rVV2	206	213	0.02%	0.002%
22	4.263	518	521	523	rBV	318	353	0.03%	0.003%
23	4.318	527	530	531	rBV2	281	302	0.02%	0.003%
24	4.471	545	555	583	rBV	98633	325931	24.57%	3.197%
25	4.904	619	626	631	rBV5	715	1742	0.13%	0.017%
26	5.056	638	651	667	rBV	163225	515140	38.83%	5.053%
27	5.391	699	706	711	rBV3	1291	2938	0.22%	0.029%
28	5.477	712	720	726	rVB5	1506	3790	0.29%	0.037%
29	5.556	726	733	734	rBV3	958	1845	0.14%	0.018%
30	5.684	750	754	759	rVB4	883	1492	0.11%	0.015%
31	5.970	788	801	825	rVV2	439512	1326519	100.00%	13.011%
32	6.147	829	830	834	rVV3	567	552	0.04%	0.005%
33	6.178	834	835	838	rVV	369	294	0.02%	0.003%
34	6.531	892	893	897	rVV2	350	258	0.02%	0.003%
35	6.562	897	898	901	rVV2	274	208	0.02%	0.002%
36	6.592	901	903	905	rVB	323	228	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036038.D
 Acq On : 06 Jun 2023 17:21
 Operator : JC/MD
 Sample : 02992-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.653	910	913	914	rBV2	319	247	0.02%	0.002%
38	6.763	920	931	949	rBV	314995	762429	57.48%	7.478%
39	7.123	981	990	1001	rBV2	59911	130570	9.84%	1.281%
40	7.306	1011	1020	1031	rBV	279529	612379	46.16%	6.006%
41	7.428	1038	1040	1045	rVB3	1405	1983	0.15%	0.019%
42	7.574	1062	1064	1067	rVB	310	211	0.02%	0.002%
43	7.775	1095	1097	1099	rVB	293	211	0.02%	0.002%
44	7.824	1101	1105	1109	rBV4	967	1902	0.14%	0.019%
45	7.927	1119	1122	1123	rBV	495	666	0.05%	0.007%
46	8.025	1136	1138	1141	rVV2	195	189	0.01%	0.002%
47	8.098	1149	1150	1153	rVB2	235	204	0.02%	0.002%
48	8.190	1163	1165	1170	rBV2	232	354	0.03%	0.003%
49	8.324	1180	1187	1199	rBV	178469	289691	21.84%	2.841%
50	8.580	1224	1229	1233	rBV3	3091	5223	0.39%	0.051%
51	8.647	1234	1240	1249	rVV	653659	1020688	76.94%	10.011%
52	8.720	1249	1252	1258	rVB3	5116	7854	0.59%	0.077%
53	8.952	1284	1290	1305	rVB	120010	189566	14.29%	1.859%
54	9.098	1311	1314	1317	rBV3	339	324	0.02%	0.003%
55	9.153	1319	1323	1329	rVV3	2762	3662	0.28%	0.036%
56	9.275	1333	1343	1350	rBV	97725	142120	10.71%	1.394%
57	9.385	1355	1361	1373	rBV	474532	662937	49.98%	6.502%
58	9.610	1393	1398	1403	rBV4	1339	2197	0.17%	0.022%
59	9.897	1443	1445	1447	rBV	382	365	0.03%	0.004%
60	10.055	1465	1471	1483	rBV	676198	935796	70.55%	9.178%
61	10.195	1490	1494	1499	rVB	5428	6857	0.52%	0.067%
62	10.269	1503	1506	1507	rBV	351	290	0.02%	0.003%
63	10.299	1507	1511	1518	rBV	5580	8070	0.61%	0.079%
64	10.390	1524	1526	1530	rBV2	307	367	0.03%	0.004%
65	10.640	1563	1567	1575	rVB4	5613	7751	0.58%	0.076%
66	10.793	1588	1592	1599	rBV5	1251	2176	0.16%	0.021%
67	10.964	1615	1620	1626	rVB2	4997	7019	0.53%	0.069%
68	11.012	1626	1628	1630	rBV	330	268	0.02%	0.003%
69	11.085	1636	1640	1645	rVB5	1042	1536	0.12%	0.015%
70	11.189	1652	1657	1664	rBV	484087	638862	48.16%	6.266%
71	11.305	1674	1676	1677	rBV	248	191	0.01%	0.002%
72	11.451	1696	1700	1706	rVB2	4958	6500	0.49%	0.064%
73	11.506	1706	1709	1711	rBV2	264	358	0.03%	0.004%
74	11.677	1735	1737	1739	rBV	331	264	0.02%	0.003%
75	11.713	1740	1743	1745	rVB2	850	594	0.04%	0.006%
76	11.756	1745	1750	1755	rBV	4009	5630	0.42%	0.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036038.D
 Acq On : 06 Jun 2023 17:21
 Operator : JC/MD
 Sample : 02992-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.969	1781	1785	1788	rBV	5073	5458	0.41%	0.054%
78	12.018	1788	1793	1805	rVV	685229	888812	67.00%	8.718%
79	12.189	1819	1821	1823	rBV	256	236	0.02%	0.002%
80	12.219	1823	1826	1831	rVB2	1152	1275	0.10%	0.013%
81	12.317	1837	1842	1850	rBV	663296	889703	67.07%	8.726%
82	12.463	1863	1866	1869	rVB2	336	402	0.03%	0.004%
83	12.622	1888	1892	1894	rBV2	352	422	0.03%	0.004%
84	12.756	1912	1914	1918	rVB2	310	424	0.03%	0.004%
85	12.860	1929	1931	1934	rVB2	523	450	0.03%	0.004%
86	12.939	1942	1944	1949	rVB4	807	1028	0.08%	0.010%
87	13.116	1969	1973	1978	rVB2	3945	5059	0.38%	0.050%
88	13.591	2047	2051	2054	rBV3	3737	4489	0.34%	0.044%
89	13.689	2062	2067	2070	rBV3	464	712	0.05%	0.007%
90	13.780	2078	2082	2086	rBV2	3880	4760	0.36%	0.047%
91	13.878	2095	2098	2102	rBV3	342	509	0.04%	0.005%
92	13.908	2102	2103	2106	rVV2	300	234	0.02%	0.002%
93	13.963	2108	2112	2115	rVB2	3901	4629	0.35%	0.045%
94	14.061	2125	2128	2129	rBV3	436	420	0.03%	0.004%
95	14.152	2141	2143	2147	rBV2	280	362	0.03%	0.004%
96	14.201	2150	2151	2155	rVB2	330	365	0.03%	0.004%
97	14.249	2157	2159	2161	rBV	668	452	0.03%	0.004%
98	14.762	2241	2243	2244	rBV2	325	234	0.02%	0.002%
99	14.969	2276	2277	2279	rBV	368	308	0.02%	0.003%
100	15.536	2368	2370	2375	rBV4	818	1079	0.08%	0.011%




Sum of corrected areas: 10195613

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036038.D
Acq On : 06 Jun 2023 17:21
Operator : JC/MD
Sample : 02992-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

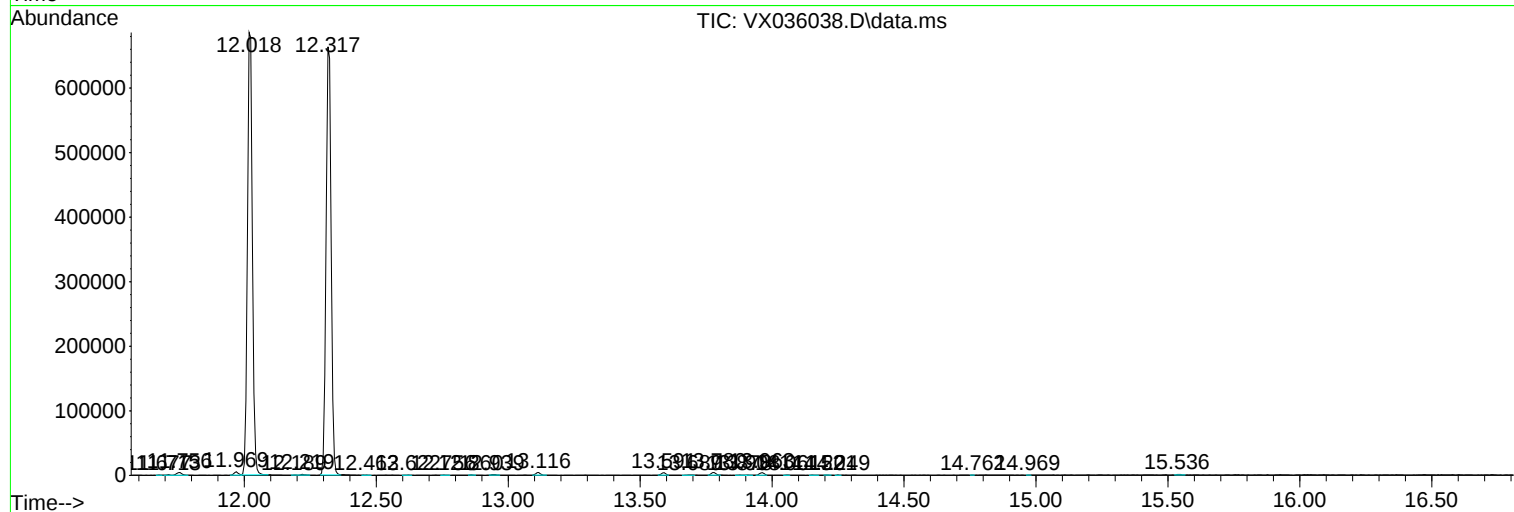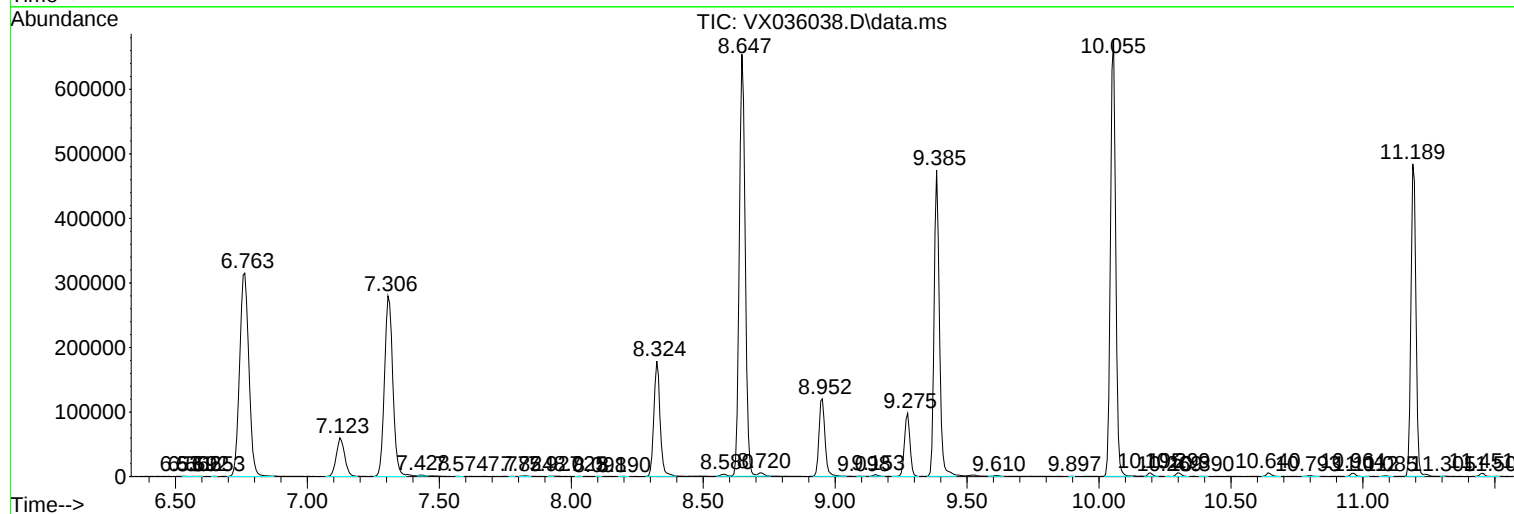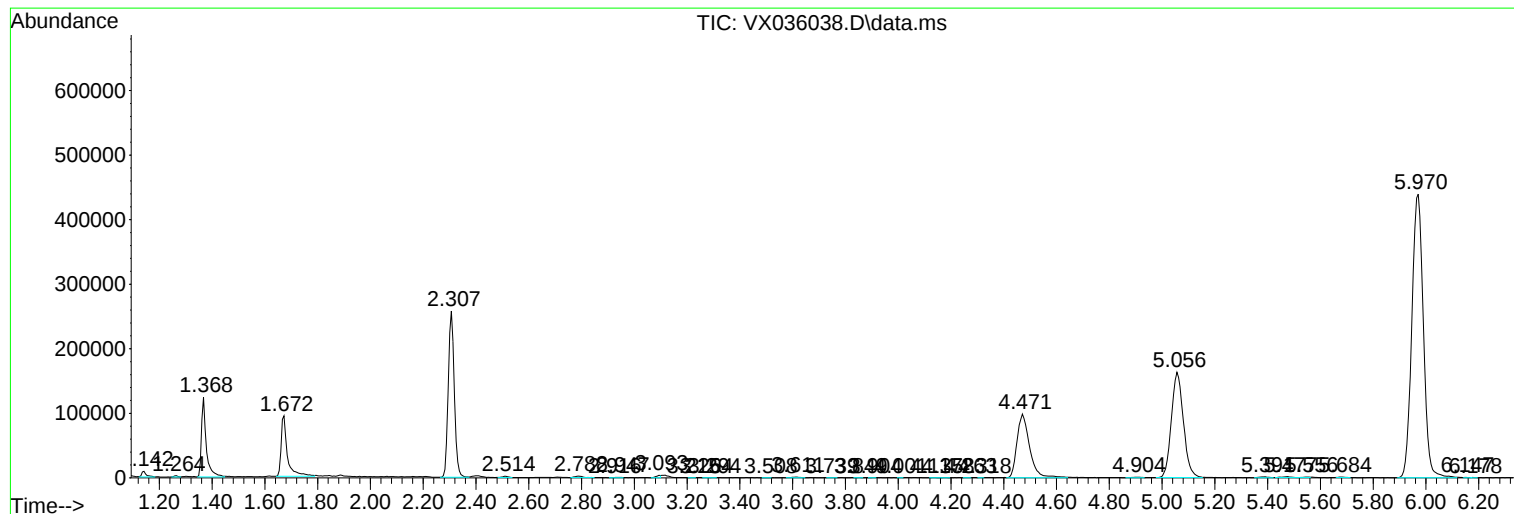

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036038.D
Acq On : 06 Jun 2023 17:21
Operator : JC/MD
Sample : 02992-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036038.D
Acq On : 06 Jun 2023 17:21
Operator : JC/MD
Sample : 02992-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc