

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036039.D
 Acq On : 06 Jun 2023 17:45
 Operator : JC/MD
 Sample : 02992-09 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M

Title : VOC Analysis

Signal : TIC: VX036039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	18	rVB	9601	10633	0.84%	0.105%
2	1.264	26	29	32	rBV2	2261	2580	0.20%	0.026%
3	1.367	42	46	59	rBV	126885	157740	12.42%	1.565%
4	1.672	91	96	109	rBV	97758	151613	11.94%	1.504%
5	2.306	194	200	210	rBV	270962	422473	33.26%	4.191%
6	2.391	210	214	218	rBV4	1090	1787	0.14%	0.018%
7	2.507	229	233	242	rVB	1991	3567	0.28%	0.035%
8	2.605	247	249	250	rVV	329	167	0.01%	0.002%
9	2.623	250	252	253	rVB	578	346	0.03%	0.003%
10	2.647	253	256	257	rBV2	613	615	0.05%	0.006%
11	2.788	274	279	285	rVB4	2399	4238	0.33%	0.042%
12	2.940	299	304	311	rVB3	1897	4168	0.33%	0.041%
13	3.032	316	319	321	rBV2	213	217	0.02%	0.002%
14	3.105	325	331	333	rBV6	1654	3129	0.25%	0.031%
15	3.336	367	369	372	rVB2	269	196	0.02%	0.002%
16	3.434	383	385	389	rVB2	302	368	0.03%	0.004%
17	3.538	400	402	404	rVB	209	167	0.01%	0.002%
18	3.568	404	407	409	rBV2	273	300	0.02%	0.003%
19	3.586	409	410	412	rVB	419	187	0.01%	0.002%
20	3.690	423	427	430	rBV2	197	288	0.02%	0.003%
21	3.824	448	449	451	rBV	294	185	0.01%	0.002%
22	3.995	476	477	480	rBV	198	176	0.01%	0.002%
23	4.086	489	492	494	rVB2	199	181	0.01%	0.002%
24	4.476	545	556	569	rBV2	89716	304453	23.97%	3.020%
25	4.824	612	613	615	rVB2	307	197	0.02%	0.002%
26	5.056	638	651	671	rBV	161152	511044	40.23%	5.069%
27	5.226	678	679	681	rBV	299	230	0.02%	0.002%
28	5.275	685	687	689	rBV2	192	178	0.01%	0.002%
29	5.537	727	730	732	rBV2	603	690	0.05%	0.007%
30	5.647	745	748	749	rBV2	217	194	0.02%	0.002%
31	5.757	763	766	767	rBV2	296	273	0.02%	0.003%
32	5.824	775	777	778	rBV	263	173	0.01%	0.002%
33	5.970	788	801	818	rBV2	427123	1270291	100.00%	12.601%
34	6.513	889	890	892	rBV	297	195	0.02%	0.002%
35	6.628	907	909	911	rBV	138	187	0.01%	0.002%
36	6.763	921	931	944	rBV	295130	714592	56.25%	7.089%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036039.D
 Acq On : 06 Jun 2023 17:45
 Operator : JC/MD
 Sample : 02992-09 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.909	953	955	959	rVB3	342	347	0.03%	0.003%
38	7.128	982	991	1003	rBV	56285	127002	10.00%	1.260%
39	7.305	1011	1020	1039	rBV	265278	589923	46.44%	5.852%
40	7.476	1045	1048	1053	rBV3	774	1365	0.11%	0.014%
41	7.567	1061	1063	1068	rBV2	248	209	0.02%	0.002%
42	7.610	1068	1070	1071	rBV	251	199	0.02%	0.002%
43	7.799	1099	1101	1104	rVB	194	182	0.01%	0.002%
44	7.927	1119	1122	1123	rBV2	363	320	0.03%	0.003%
45	8.110	1150	1152	1155	rBV	193	282	0.02%	0.003%
46	8.183	1161	1164	1166	rBV2	194	200	0.02%	0.002%
47	8.323	1180	1187	1199	rBV	163901	271492	21.37%	2.693%
48	8.646	1233	1240	1256	rBV	644650	1000696	78.78%	9.927%
49	8.841	1271	1272	1274	rVB2	438	252	0.02%	0.002%
50	8.890	1278	1280	1281	rBV	270	178	0.01%	0.002%
51	8.951	1284	1290	1302	rVV	117004	178779	14.07%	1.773%
52	9.079	1308	1311	1314	rBV2	389	461	0.04%	0.005%
53	9.207	1331	1332	1335	rVB2	306	200	0.02%	0.002%
54	9.274	1336	1343	1352	rVV	399822	577335	45.45%	5.727%
55	9.384	1355	1361	1380	rBV	439446	623492	49.08%	6.185%
56	9.665	1405	1407	1409	rBV	269	172	0.01%	0.002%
57	9.732	1417	1418	1423	rBV3	332	268	0.02%	0.003%
58	9.866	1438	1440	1443	rBV2	295	331	0.03%	0.003%
59	9.975	1455	1458	1459	rBV2	229	258	0.02%	0.003%
60	10.055	1465	1471	1482	rBV	634395	854258	67.25%	8.474%
61	10.189	1491	1493	1495	rBV2	454	516	0.04%	0.005%
62	10.305	1507	1512	1516	rVB4	1207	1848	0.15%	0.018%
63	10.366	1521	1522	1525	rBV2	250	217	0.02%	0.002%
64	10.518	1545	1547	1551	rBV2	131	170	0.01%	0.002%
65	10.737	1581	1583	1584	rBV	299	183	0.01%	0.002%
66	10.859	1602	1603	1607	rBV2	278	386	0.03%	0.004%
67	10.957	1618	1619	1623	rVB2	353	363	0.03%	0.004%
68	11.091	1637	1641	1645	rVB	441	535	0.04%	0.005%
69	11.189	1652	1657	1665	rBV	458608	595814	46.90%	5.910%
70	11.317	1674	1678	1684	rVB	814	1250	0.10%	0.012%
71	11.457	1697	1701	1704	rVV3	369	438	0.03%	0.004%
72	11.561	1716	1718	1720	rVB2	288	211	0.02%	0.002%
73	11.585	1720	1722	1725	rBV2	169	173	0.01%	0.002%
74	11.628	1725	1729	1731	rBV2	300	427	0.03%	0.004%
75	11.707	1741	1742	1744	rVV	478	227	0.02%	0.002%
76	11.756	1747	1750	1755	rVB3	418	689	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036039.D
 Acq On : 06 Jun 2023 17:45
 Operator : JC/MD
 Sample : 02992-09 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.969	1779	1785	1788	rBV3	708	945	0.07%	0.009%
78	12.024	1788	1794	1807	rBV	619909	807144	63.54%	8.007%
79	12.316	1837	1842	1858	rVB	669152	862946	67.93%	8.560%
80	12.463	1863	1866	1869	rBV3	365	444	0.03%	0.004%
81	12.902	1937	1938	1941	rBV	305	241	0.02%	0.002%
82	13.115	1969	1973	1975	rBV3	722	786	0.06%	0.008%
83	13.304	2003	2004	2006	rBV	321	204	0.02%	0.002%
84	13.585	2046	2050	2054	rVV4	737	1053	0.08%	0.010%
85	13.688	2066	2067	2072	rVV3	294	351	0.03%	0.003%
86	13.725	2072	2073	2075	rVB	502	245	0.02%	0.002%
87	13.774	2078	2081	2086	rVB3	562	787	0.06%	0.008%
88	13.835	2088	2091	2093	rBV2	306	345	0.03%	0.003%
89	13.853	2093	2094	2097	rBV2	264	185	0.01%	0.002%
90	13.969	2108	2113	2114	rBV4	351	495	0.04%	0.005%
91	14.231	2154	2156	2159	rBV	559	435	0.03%	0.004%
92	14.462	2190	2194	2197	rBV2	363	514	0.04%	0.005%
93	14.536	2204	2206	2208	rVB	355	213	0.02%	0.002%
94	14.597	2214	2216	2218	rBV	279	213	0.02%	0.002%
95	14.755	2240	2242	2244	rBV2	442	418	0.03%	0.004%
96	15.103	2298	2299	2300	rBV	601	304	0.02%	0.003%
97	15.353	2338	2340	2343	rBV4	491	466	0.04%	0.005%
98	15.542	2367	2371	2374	rBV5	962	1234	0.10%	0.012%
99	16.365	2505	2506	2509	rVB2	872	694	0.05%	0.007%
100	16.505	2527	2529	2531	rBV2	474	446	0.04%	0.004%


Sum of corrected areas: 10080774

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036039.D
Acq On : 06 Jun 2023 17:45
Operator : JC/MD
Sample : 02992-09 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

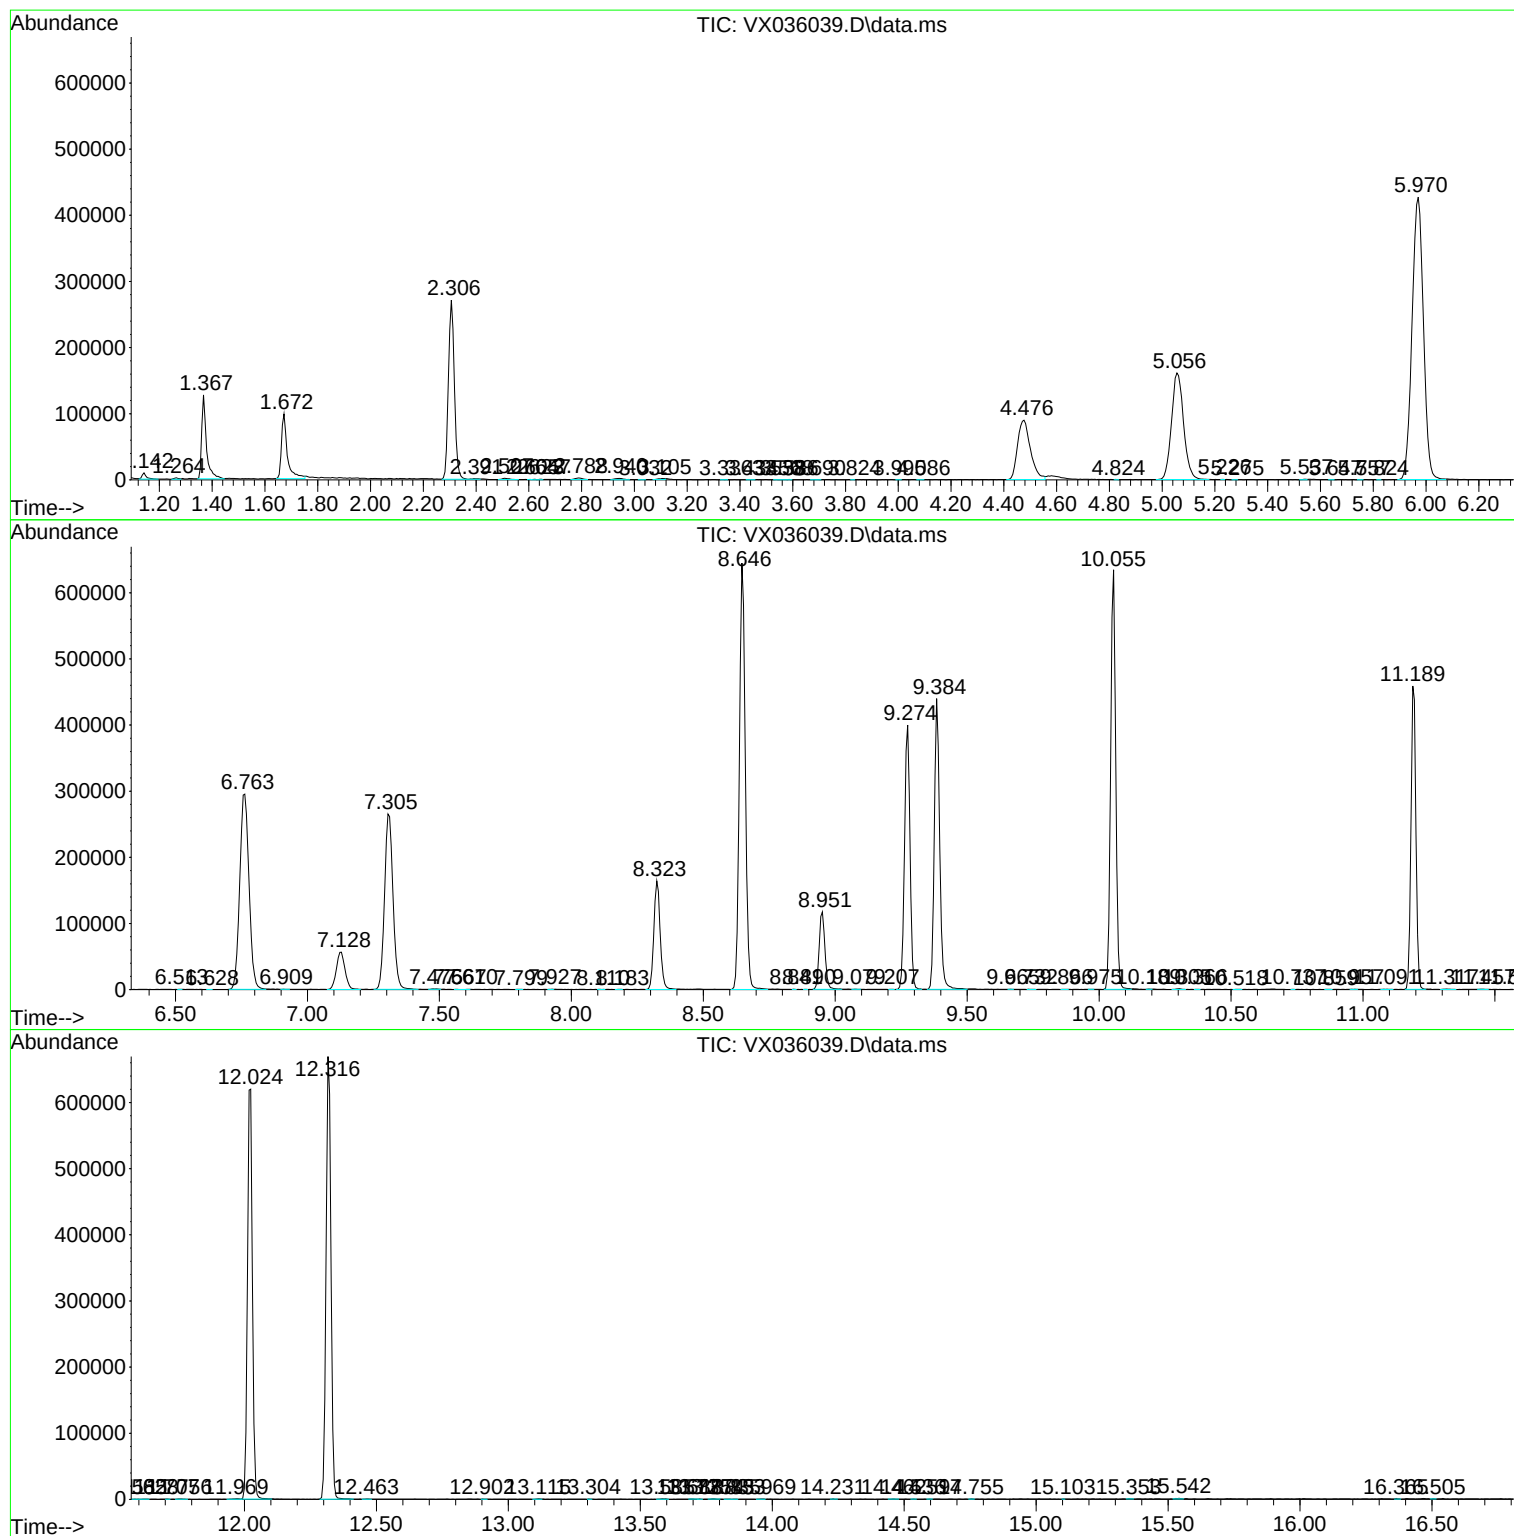

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036039.D
Acq On : 06 Jun 2023 17:45
Operator : JC/MD
Sample : 02992-09 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036039.D
Acq On : 06 Jun 2023 17:45
Operator : JC/MD
Sample : 02992-09 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------