

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036040.D
 Acq On : 06 Jun 2023 18:08
 Operator : JC/MD
 Sample : 02992-10 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	9029	9434	0.75%	0.093%
2	1.264	27	29	33	rBV	1608	1456	0.12%	0.014%
3	1.368	42	46	59	rBV	133233	160902	12.79%	1.578%
4	1.672	91	96	113	rBV	96826	153019	12.17%	1.500%
5	2.306	194	200	212	rBV	262383	409428	32.56%	4.015%
6	2.508	230	233	238	rVB2	818	1323	0.11%	0.013%
7	2.599	245	248	250	rBV2	371	504	0.04%	0.005%
8	2.672	259	260	263	rBV3	376	352	0.03%	0.003%
9	2.758	272	274	275	rBV	312	193	0.02%	0.002%
10	2.788	275	279	287	rVB3	2842	4194	0.33%	0.041%
11	2.843	287	288	290	rVB	346	224	0.02%	0.002%
12	2.947	298	305	311	rBV3	1642	4046	0.32%	0.040%
13	2.995	311	313	315	rVV3	246	194	0.02%	0.002%
14	3.081	326	327	328	rBV	343	240	0.02%	0.002%
15	3.166	339	341	343	rBV	202	192	0.02%	0.002%
16	3.257	354	356	359	rBV2	211	207	0.02%	0.002%
17	3.288	359	361	363	rBV	218	194	0.02%	0.002%
18	3.434	382	385	389	rVB2	285	420	0.03%	0.004%
19	3.465	389	390	392	rBV2	219	183	0.01%	0.002%
20	3.520	396	399	402	rBV2	264	372	0.03%	0.004%
21	3.623	413	416	418	rBV	186	190	0.02%	0.002%
22	3.745	434	436	438	rVB2	225	193	0.02%	0.002%
23	3.885	457	459	463	rBV2	184	253	0.02%	0.002%
24	3.971	469	473	475	rBV	261	265	0.02%	0.003%
25	3.995	475	477	481	rVB2	217	222	0.02%	0.002%
26	4.245	516	518	523	rBV2	274	346	0.03%	0.003%
27	4.306	526	528	531	rBV	199	253	0.02%	0.002%
28	4.471	544	555	570	rBV	92845	313203	24.90%	3.071%
29	4.867	618	620	623	rVB2	250	224	0.02%	0.002%
30	5.056	639	651	668	rBV	158216	505760	40.22%	4.959%
31	5.330	695	696	699	rVB2	218	185	0.01%	0.002%
32	5.385	703	705	708	rBV3	315	323	0.03%	0.003%
33	5.464	716	718	720	rBV2	270	335	0.03%	0.003%
34	5.720	758	760	762	rBV	290	191	0.02%	0.002%
35	5.800	771	773	774	rBV	241	189	0.02%	0.002%
36	5.836	776	779	781	rVB2	236	187	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036040.D
 Acq On : 06 Jun 2023 18:08
 Operator : JC/MD
 Sample : 02992-10 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	5.970	788	801	818	rBV2	418471	1257635	100.00%	12.331%
38	6.220	840	842	847	rVB2	376	521	0.04%	0.005%
39	6.281	847	852	854	rBV2	215	349	0.03%	0.003%
40	6.300	854	855	858	rBV	232	205	0.02%	0.002%
41	6.641	909	911	912	rVV	366	217	0.02%	0.002%
42	6.678	916	917	920	rVB	530	262	0.02%	0.003%
43	6.757	920	930	944	rBV	307005	736744	58.58%	7.224%
44	7.123	981	990	1006	rBV	157354	358622	28.52%	3.516%
45	7.305	1010	1020	1038	rBV	261557	576413	45.83%	5.652%
46	7.427	1038	1040	1044	rVB2	233	247	0.02%	0.002%
47	7.470	1044	1047	1052	rVB4	648	1112	0.09%	0.011%
48	7.513	1052	1054	1056	rBV2	378	282	0.02%	0.003%
49	7.659	1077	1078	1081	rBV2	251	277	0.02%	0.003%
50	7.921	1120	1121	1124	rBV	286	388	0.03%	0.004%
51	7.982	1128	1131	1132	rBV2	290	192	0.02%	0.002%
52	8.141	1154	1157	1160	rBV	321	482	0.04%	0.005%
53	8.324	1180	1187	1198	rBV	161682	262031	20.84%	2.569%
54	8.549	1221	1224	1226	rBV2	267	280	0.02%	0.003%
55	8.647	1233	1240	1254	rBV	631714	996409	79.23%	9.770%
56	8.952	1283	1290	1303	rBV	112525	172857	13.74%	1.695%
57	9.201	1329	1331	1333	rVB3	362	262	0.02%	0.003%
58	9.275	1336	1343	1352	rVB	314752	460724	36.63%	4.518%
59	9.384	1355	1361	1380	rBV	435703	622461	49.49%	6.103%
60	9.945	1451	1453	1456	rVB2	862	623	0.05%	0.006%
61	10.055	1465	1471	1482	rBV	635194	872098	69.34%	8.551%
62	10.201	1491	1495	1497	rBV2	720	637	0.05%	0.006%
63	10.305	1510	1512	1516	rVB2	1022	938	0.07%	0.009%
64	10.415	1527	1530	1532	rBV	361	337	0.03%	0.003%
65	10.646	1564	1568	1569	rBV2	554	629	0.05%	0.006%
66	11.189	1652	1657	1669	rBV	458545	593398	47.18%	5.818%
67	11.311	1674	1677	1680	rBV	296	408	0.03%	0.004%
68	11.610	1725	1726	1729	rBV2	223	249	0.02%	0.002%
69	11.762	1746	1751	1754	rBV3	563	1008	0.08%	0.010%
70	11.811	1758	1759	1761	rVB	336	183	0.01%	0.002%
71	11.969	1782	1785	1788	rBV3	933	1060	0.08%	0.010%
72	12.018	1788	1793	1803	rBV	649513	841688	66.93%	8.253%
73	12.164	1813	1817	1818	rBV2	236	275	0.02%	0.003%
74	12.213	1823	1825	1827	rVB	488	298	0.02%	0.003%
75	12.317	1837	1842	1853	rBV	681684	856589	68.11%	8.399%
76	12.536	1873	1878	1879	rBV2	295	408	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036040.D
 Acq On : 06 Jun 2023 18:08
 Operator : JC/MD
 Sample : 02992-10 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.567	1882	1883	1885	rBV2	325	239	0.02%	0.002%
78	12.652	1895	1897	1899	rBV2	267	261	0.02%	0.003%
79	12.713	1906	1907	1910	rBV2	191	225	0.02%	0.002%
80	13.103	1969	1971	1972	rBV	272	232	0.02%	0.002%
81	13.390	2016	2018	2020	rBV2	323	258	0.02%	0.003%
82	13.481	2031	2033	2034	rBV	387	204	0.02%	0.002%
83	13.542	2041	2043	2047	rBV3	256	309	0.02%	0.003%
84	13.591	2047	2051	2056	rBV2	637	1015	0.08%	0.010%
85	13.682	2065	2066	2070	rBV2	427	429	0.03%	0.004%
86	13.780	2079	2082	2086	rBV	763	811	0.06%	0.008%
87	13.963	2109	2112	2115	rVB3	399	572	0.05%	0.006%
88	14.134	2138	2140	2142	rVB2	444	359	0.03%	0.004%
89	14.158	2142	2144	2147	rBV2	241	273	0.02%	0.003%
90	14.255	2159	2160	2163	rBV2	324	406	0.03%	0.004%
91	14.438	2188	2190	2192	rBV2	341	304	0.02%	0.003%
92	14.493	2197	2199	2202	rBV2	267	263	0.02%	0.003%
93	14.591	2214	2215	2217	rBV2	255	181	0.01%	0.002%
94	15.097	2296	2298	2300	rBV3	401	379	0.03%	0.004%
95	15.249	2321	2323	2324	rVB2	396	186	0.01%	0.002%
96	15.536	2369	2370	2373	rBV2	621	636	0.05%	0.006%
97	15.664	2389	2391	2395	rBV3	499	437	0.03%	0.004%
98	15.731	2400	2402	2405	rBV3	494	719	0.06%	0.007%
99	15.804	2412	2414	2416	rVB2	648	357	0.03%	0.004%
100	16.371	2505	2507	2510	rVB2	574	398	0.03%	0.004%


Sum of corrected areas: 10198647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036040.D
Acq On : 06 Jun 2023 18:08
Operator : JC/MD
Sample : 02992-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

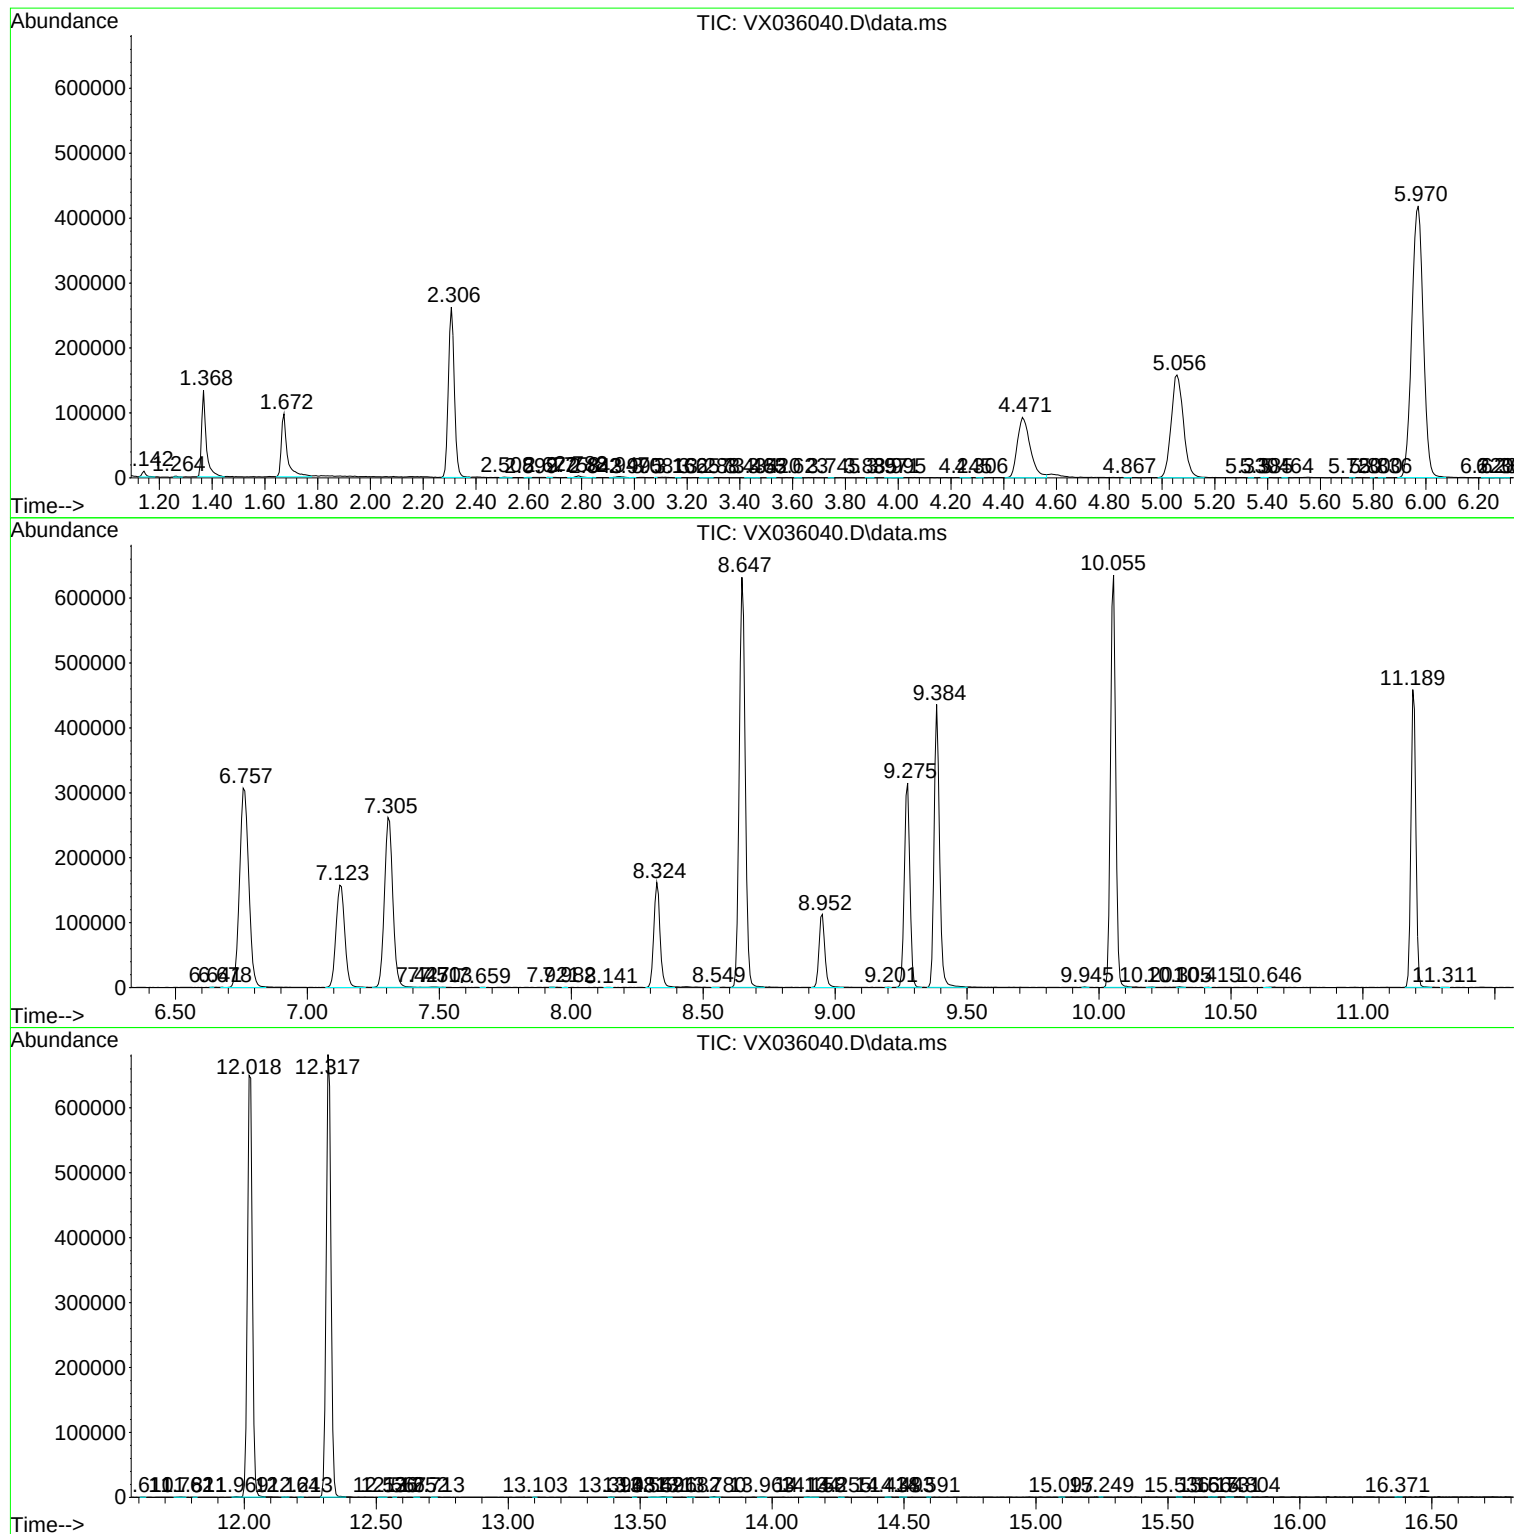

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036040.D
Acq On : 06 Jun 2023 18:08
Operator : JC/MD
Sample : 02992-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036040.D
Acq On : 06 Jun 2023 18:08
Operator : JC/MD
Sample : 02992-10 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------