

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036041.D
 Acq On : 06 Jun 2023 18:31
 Operator : JC/MD
 Sample : 02992-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	12	rBV2	7882	7181	0.55%	0.068%
2	1.264	26	29	32	rBV3	2415	2384	0.18%	0.023%
3	1.367	42	46	58	rBV	131505	159415	12.10%	1.506%
4	1.672	91	96	108	rBV	103297	151704	11.52%	1.434%
5	2.306	193	200	210	rBV	272145	421168	31.97%	3.980%
6	2.514	230	234	238	rBV2	661	1098	0.08%	0.010%
7	2.721	266	268	269	rVB	433	210	0.02%	0.002%
8	2.788	275	279	284	rVB4	934	1925	0.15%	0.018%
9	2.934	301	303	306	rBV3	233	395	0.03%	0.004%
10	3.014	315	316	320	rBV	136	175	0.01%	0.002%
11	3.056	320	323	324	rVV3	198	245	0.02%	0.002%
12	3.111	324	332	342	rVB3	8083	20283	1.54%	0.192%
13	3.245	352	354	356	rVV2	268	181	0.01%	0.002%
14	3.276	356	359	362	rVB	269	248	0.02%	0.002%
15	3.373	372	375	379	rBV	292	600	0.05%	0.006%
16	3.410	379	381	382	rVB	333	188	0.01%	0.002%
17	3.452	387	388	391	rVV	312	214	0.02%	0.002%
18	3.678	424	425	427	rBV	322	202	0.02%	0.002%
19	4.044	484	485	489	rVV2	250	285	0.02%	0.003%
20	4.074	489	490	492	rVB	270	189	0.01%	0.002%
21	4.471	545	555	574	rBV2	106799	368695	27.99%	3.484%
22	4.867	618	620	625	rVB2	213	219	0.02%	0.002%
23	5.056	638	651	668	rBV2	165143	527267	40.03%	4.982%
24	5.312	691	693	696	rBV2	206	283	0.02%	0.003%
25	5.678	751	753	754	rBV	371	191	0.01%	0.002%
26	5.751	762	765	766	rBV2	224	183	0.01%	0.002%
27	5.861	780	783	785	rBV2	173	226	0.02%	0.002%
28	5.970	787	801	817	rBV2	439634	1317225	100.00%	12.447%
29	6.275	849	851	852	rBV	299	198	0.02%	0.002%
30	6.495	886	887	891	rVB2	287	249	0.02%	0.002%
31	6.635	907	910	911	rBV2	261	213	0.02%	0.002%
32	6.763	920	931	946	rBV	323013	774599	58.81%	7.320%
33	6.976	964	966	968	rBV	433	281	0.02%	0.003%
34	7.123	982	990	1002	rBV	80829	184129	13.98%	1.740%
35	7.305	1011	1020	1041	rVB	278330	606641	46.05%	5.733%
36	7.488	1041	1050	1053	rBV4	893	2008	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036041.D
 Acq On : 06 Jun 2023 18:31
 Operator : JC/MD
 Sample : 02992-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.592	1064	1067	1068	rVV	364	323	0.02%	0.003%
38	7.653	1074	1077	1080	rBV2	236	307	0.02%	0.003%
39	8.324	1180	1187	1202	rBV	170202	277050	21.03%	2.618%
40	8.439	1202	1206	1210	rVB3	1110	2035	0.15%	0.019%
41	8.647	1233	1240	1258	rBV	669482	1042959	79.18%	9.856%
42	8.951	1284	1290	1303	rBV	118936	179142	13.60%	1.693%
43	9.177	1324	1327	1330	rBV3	276	413	0.03%	0.004%
44	9.201	1330	1331	1333	rBV	277	180	0.01%	0.002%
45	9.275	1336	1343	1350	rBV	372436	532537	40.43%	5.032%
46	9.384	1355	1361	1374	rBV	452069	635515	48.25%	6.005%
47	9.659	1404	1406	1408	rVB2	400	324	0.02%	0.003%
48	9.762	1421	1423	1426	rVB2	212	199	0.02%	0.002%
49	9.909	1445	1447	1448	rBV2	297	205	0.02%	0.002%
50	9.927	1448	1450	1451	rBV	313	220	0.02%	0.002%
51	10.055	1465	1471	1481	rBV	680624	934351	70.93%	8.829%
52	10.183	1490	1492	1493	rBV	335	273	0.02%	0.003%
53	10.305	1509	1512	1517	rVB2	881	1187	0.09%	0.011%
54	10.372	1521	1523	1526	rBV2	297	345	0.03%	0.003%
55	10.409	1526	1529	1530	rBV2	254	217	0.02%	0.002%
56	10.640	1565	1567	1572	rVB2	376	464	0.04%	0.004%
57	10.695	1572	1576	1577	rBV2	246	202	0.02%	0.002%
58	10.823	1593	1597	1599	rVB2	268	357	0.03%	0.003%
59	10.957	1618	1619	1622	rBV2	378	242	0.02%	0.002%
60	11.079	1637	1639	1643	rVB2	437	516	0.04%	0.005%
61	11.189	1652	1657	1667	rBV	476402	621900	47.21%	5.877%
62	11.317	1673	1678	1681	rVV4	1115	1577	0.12%	0.015%
63	11.451	1698	1700	1703	rVB2	534	501	0.04%	0.005%
64	11.512	1708	1710	1712	rVV2	404	338	0.03%	0.003%
65	11.536	1712	1714	1718	rVB2	292	208	0.02%	0.002%
66	11.701	1739	1741	1742	rVB2	376	239	0.02%	0.002%
67	11.750	1748	1749	1753	rVV3	264	345	0.03%	0.003%
68	11.860	1765	1767	1769	rVB2	216	197	0.01%	0.002%
69	11.884	1769	1771	1773	rBV2	277	310	0.02%	0.003%
70	12.024	1788	1794	1803	rBV	713926	894622	67.92%	8.454%
71	12.116	1807	1809	1811	rVB2	605	535	0.04%	0.005%
72	12.152	1813	1815	1817	rBV	291	222	0.02%	0.002%
73	12.213	1823	1825	1832	rBV4	652	1225	0.09%	0.012%
74	12.317	1837	1842	1850	rBV	703511	888303	67.44%	8.394%
75	12.463	1864	1866	1869	rVB	595	527	0.04%	0.005%
76	12.524	1872	1876	1879	rBV2	303	431	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036041.D
 Acq On : 06 Jun 2023 18:31
 Operator : JC/MD
 Sample : 02992-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.622	1889	1892	1893	rBV2	229	236	0.02%	0.002%
78	12.658	1897	1898	1901	rBV2	303	265	0.02%	0.003%
79	12.731	1908	1910	1912	rBV2	280	334	0.03%	0.003%
80	12.804	1920	1922	1923	rBV2	246	227	0.02%	0.002%
81	12.835	1925	1927	1928	rBV	247	201	0.02%	0.002%
82	12.896	1935	1937	1940	rBV2	406	420	0.03%	0.004%
83	12.945	1943	1945	1950	rVV3	722	890	0.07%	0.008%
84	13.067	1961	1965	1968	rBV2	257	355	0.03%	0.003%
85	13.115	1971	1973	1976	rVB2	380	338	0.03%	0.003%
86	13.164	1979	1981	1982	rBV	261	208	0.02%	0.002%
87	13.384	2015	2017	2019	rBV2	323	359	0.03%	0.003%
88	13.493	2034	2035	2039	rBV2	199	233	0.02%	0.002%
89	13.591	2048	2051	2055	rVB3	613	818	0.06%	0.008%
90	13.780	2077	2082	2083	rBV3	507	752	0.06%	0.007%
91	13.908	2100	2103	2106	rBV2	219	336	0.03%	0.003%
92	14.127	2137	2139	2141	rBV	441	264	0.02%	0.002%
93	14.170	2144	2146	2149	rBV	441	553	0.04%	0.005%
94	14.255	2157	2160	2161	rBV	363	478	0.04%	0.005%
95	14.457	2187	2193	2195	rBV3	517	901	0.07%	0.009%
96	14.761	2241	2243	2244	rBV2	442	329	0.02%	0.003%
97	15.109	2299	2300	2305	rBV2	359	503	0.04%	0.005%
98	15.243	2320	2322	2325	rVB	878	773	0.06%	0.007%
99	15.621	2382	2384	2385	rBV2	448	219	0.02%	0.002%
100	15.926	2433	2434	2437	rBV2	492	491	0.04%	0.005%




Sum of corrected areas: 10582423

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036041.D
Acq On : 06 Jun 2023 18:31
Operator : JC/MD
Sample : 02992-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

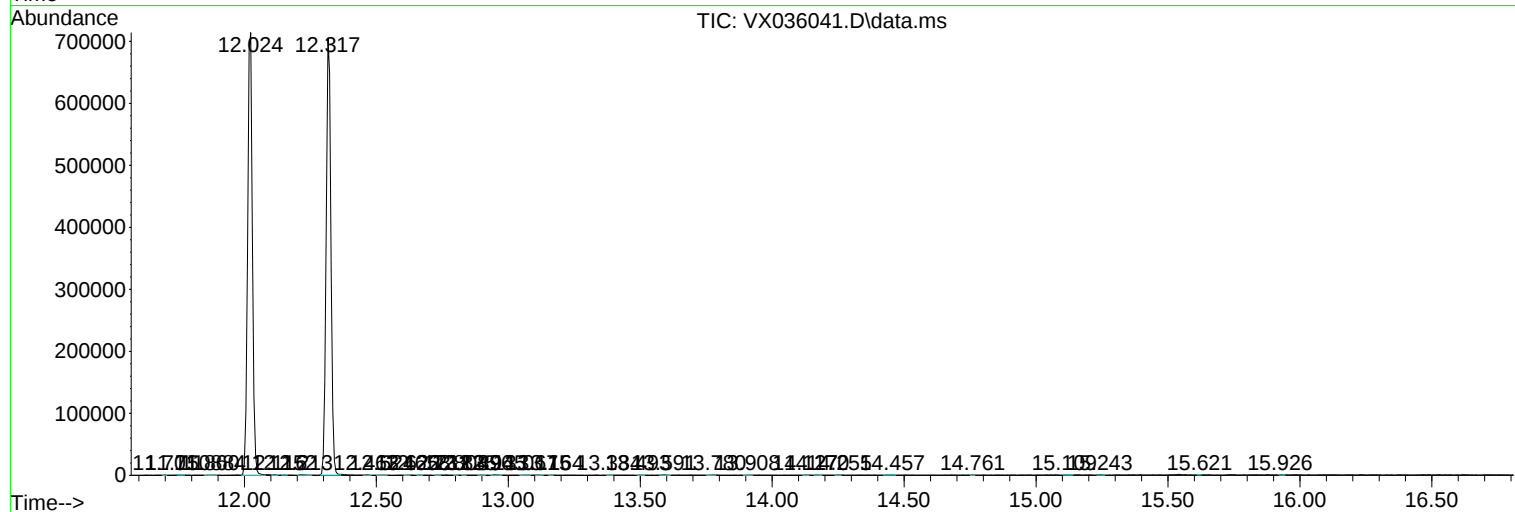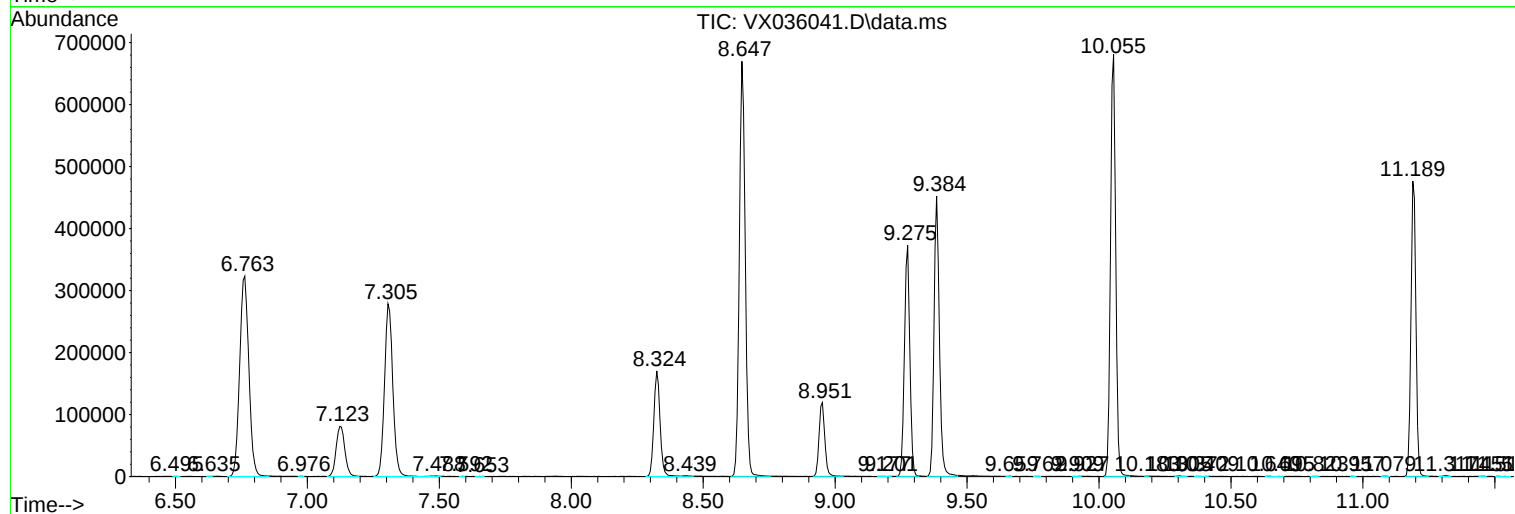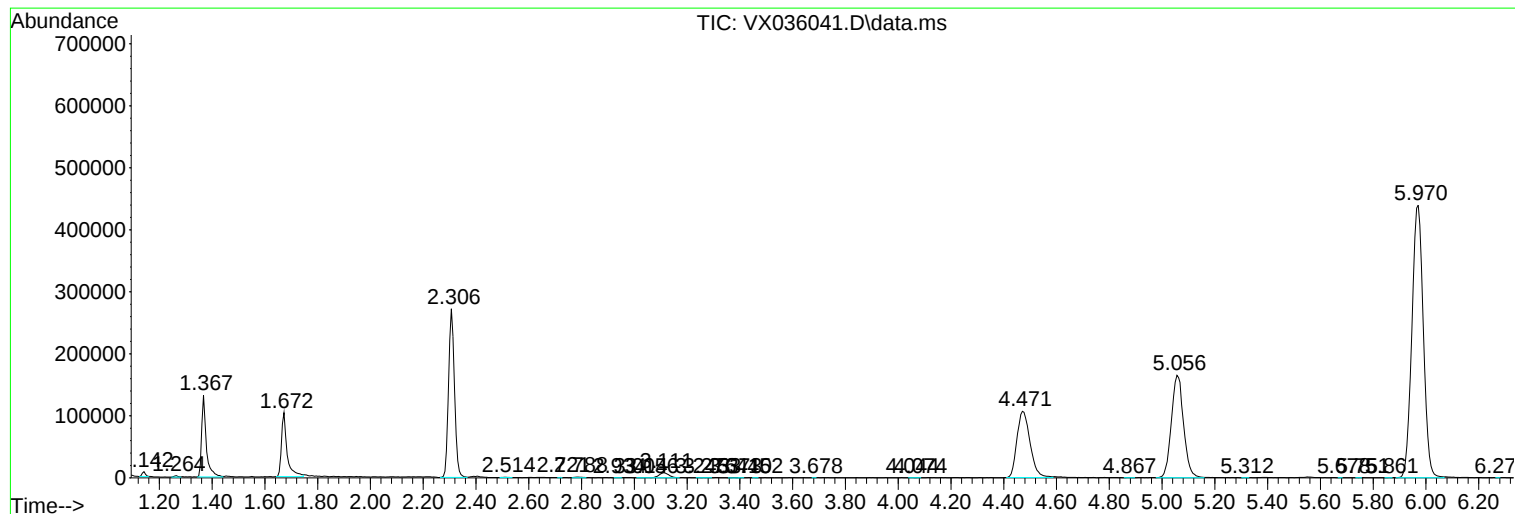

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036041.D
Acq On : 06 Jun 2023 18:31
Operator : JC/MD
Sample : 02992-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036041.D
Acq On : 06 Jun 2023 18:31
Operator : JC/MD
Sample : 02992-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------