

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036042.D
 Acq On : 06 Jun 2023 18:55
 Operator : JC/MD
 Sample : 02992-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	14	rVB2	8648	8602	0.65%	0.086%
2	1.264	26	29	33	rBV3	2538	2988	0.23%	0.030%
3	1.368	42	46	57	rBV	135897	165527	12.47%	1.655%
4	1.459	57	61	67	rVB	6591	9693	0.73%	0.097%
5	1.673	91	96	115	rBV	104488	156314	11.78%	1.563%
6	2.307	194	200	209	rBV	276148	430931	32.47%	4.308%
7	2.618	249	251	253	rBV2	377	257	0.02%	0.003%
8	2.788	275	279	284	rVB5	1040	1970	0.15%	0.020%
9	2.928	300	302	304	rBV2	305	270	0.02%	0.003%
10	3.008	313	315	316	rBV2	440	264	0.02%	0.003%
11	3.111	325	332	333	rBV4	3140	5437	0.41%	0.054%
12	3.270	357	358	363	rVB2	234	315	0.02%	0.003%
13	3.398	376	379	381	rBV2	243	250	0.02%	0.002%
14	3.532	397	401	403	rBV2	136	235	0.02%	0.002%
15	3.636	416	418	420	rBV	359	368	0.03%	0.004%
16	3.672	420	424	426	rVB2	313	323	0.02%	0.003%
17	4.050	485	486	490	rVB	312	241	0.02%	0.002%
18	4.270	520	522	524	rBV	207	225	0.02%	0.002%
19	4.465	544	554	580	rBV	89915	298229	22.47%	2.981%
20	4.727	596	597	600	rBV2	261	287	0.02%	0.003%
21	4.763	601	603	605	rVB2	327	199	0.01%	0.002%
22	4.879	620	622	625	rVB2	264	244	0.02%	0.002%
23	5.056	638	651	667	rBV	166208	531192	40.02%	5.310%
24	5.208	675	676	680	rBV2	315	346	0.03%	0.003%
25	5.391	700	706	714	rBV2	1006	2035	0.15%	0.020%
26	5.544	726	731	733	rBV	1389	2116	0.16%	0.021%
27	5.617	741	743	745	rBV2	192	202	0.02%	0.002%
28	5.830	774	778	783	rBV2	253	390	0.03%	0.004%
29	5.971	787	801	816	rBV2	440606	1327157	100.00%	13.267%
30	6.391	868	870	874	rBV2	280	475	0.04%	0.005%
31	6.470	881	883	887	rVB2	264	240	0.02%	0.002%
32	6.653	910	913	915	rVB2	249	204	0.02%	0.002%
33	6.763	921	931	948	rBV	331282	794462	59.86%	7.942%
34	7.037	972	976	978	rBV2	231	346	0.03%	0.003%
35	7.123	983	990	999	rBV5	6199	15824	1.19%	0.158%
36	7.239	1008	1009	1011	rBV	219	231	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036042.D
 Acq On : 06 Jun 2023 18:55
 Operator : JC/MD
 Sample : 02992-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.306	1011	1020	1043	rVB	280449	614082	46.27%	6.139%
38	7.482	1043	1049	1057	rBV4	862	2076	0.16%	0.021%
39	7.598	1063	1068	1073	rBV2	258	537	0.04%	0.005%
40	7.720	1085	1088	1090	rVB3	246	316	0.02%	0.003%
41	7.751	1090	1093	1096	rBV2	242	317	0.02%	0.003%
42	7.934	1119	1123	1125	rVV2	708	821	0.06%	0.008%
43	7.976	1128	1130	1131	rVB	495	309	0.02%	0.003%
44	7.988	1131	1132	1136	rBV2	247	303	0.02%	0.003%
45	8.324	1180	1187	1197	rBV	177134	282117	21.26%	2.820%
46	8.647	1233	1240	1249	rBV	674973	1038273	78.23%	10.379%
47	8.830	1268	1270	1272	rBV2	265	292	0.02%	0.003%
48	8.952	1284	1290	1299	rBV	119347	184859	13.93%	1.848%
49	9.275	1336	1343	1351	rBV	67187	103145	7.77%	1.031%
50	9.385	1355	1361	1378	rVV	444014	631441	47.58%	6.312%
51	9.519	1381	1383	1388	rVB5	1379	1686	0.13%	0.017%
52	9.726	1413	1417	1419	rBV2	241	293	0.02%	0.003%
53	9.884	1440	1443	1446	rBV2	354	502	0.04%	0.005%
54	9.945	1450	1453	1454	rVB2	278	232	0.02%	0.002%
55	10.055	1465	1471	1484	rBV	674301	936583	70.57%	9.363%
56	10.275	1504	1507	1509	rBV2	246	256	0.02%	0.003%
57	10.299	1509	1511	1514	rVV2	868	944	0.07%	0.009%
58	10.391	1524	1526	1529	rBV2	255	260	0.02%	0.003%
59	10.573	1555	1556	1558	rBV	273	214	0.02%	0.002%
60	10.640	1565	1567	1571	rVB3	417	530	0.04%	0.005%
61	10.762	1585	1587	1590	rBV2	301	335	0.03%	0.003%
62	10.951	1616	1618	1619	rVV	243	223	0.02%	0.002%
63	11.043	1632	1633	1636	rBV2	222	232	0.02%	0.002%
64	11.092	1637	1641	1642	rVV2	453	471	0.04%	0.005%
65	11.134	1645	1648	1652	rVB3	357	404	0.03%	0.004%
66	11.189	1652	1657	1666	rBV	494212	624462	47.05%	6.243%
67	11.311	1675	1677	1681	rVB4	1262	1392	0.10%	0.014%
68	11.531	1710	1713	1714	rBV	356	286	0.02%	0.003%
69	11.561	1716	1718	1721	rVV2	336	264	0.02%	0.003%
70	11.610	1724	1726	1728	rBV	342	229	0.02%	0.002%
71	11.640	1728	1731	1733	rBV	274	249	0.02%	0.002%
72	11.707	1741	1742	1744	rVV	336	255	0.02%	0.003%
73	11.756	1747	1750	1751	rVB2	268	256	0.02%	0.003%
74	12.018	1788	1793	1803	rBV	728013	903597	68.09%	9.033%
75	12.219	1823	1826	1832	rVB4	1673	2526	0.19%	0.025%
76	12.317	1837	1842	1851	rBV	711597	898782	67.72%	8.985%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036042.D
 Acq On : 06 Jun 2023 18:55
 Operator : JC/MD
 Sample : 02992-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.860	1928	1931	1935	rVB3	830	790	0.06%	0.008%
78	12.988	1950	1952	1954	rBV2	242	228	0.02%	0.002%
79	13.103	1969	1971	1976	rVB3	513	746	0.06%	0.007%
80	13.219	1987	1990	1991	rBV	346	286	0.02%	0.003%
81	13.244	1991	1994	1996	rVB2	250	262	0.02%	0.003%
82	13.329	2006	2008	2011	rVB3	269	247	0.02%	0.002%
83	13.488	2030	2034	2035	rBV	213	232	0.02%	0.002%
84	13.689	2061	2067	2071	rBV3	553	1193	0.09%	0.012%
85	13.792	2083	2084	2086	rVB	531	276	0.02%	0.003%
86	13.981	2114	2115	2119	rBV2	326	257	0.02%	0.003%
87	14.189	2147	2149	2153	rBV2	278	285	0.02%	0.003%
88	14.292	2164	2166	2167	rBV	344	211	0.02%	0.002%
89	14.378	2178	2180	2185	rBV2	309	470	0.04%	0.005%
90	14.512	2198	2202	2203	rBV3	294	281	0.02%	0.003%
91	14.603	2216	2217	2219	rVB2	368	218	0.02%	0.002%
92	14.695	2230	2232	2234	rBV3	419	419	0.03%	0.004%
93	14.896	2263	2265	2266	rBV	386	242	0.02%	0.002%
94	15.115	2299	2301	2303	rBV	337	351	0.03%	0.004%
95	15.542	2368	2371	2376	rBV6	959	1463	0.11%	0.015%
96	15.877	2424	2426	2431	rVB2	595	553	0.04%	0.006%
97	16.267	2488	2490	2491	rBV	469	384	0.03%	0.004%
98	16.383	2508	2509	2511	rVB2	497	284	0.02%	0.003%
99	16.408	2511	2513	2516	rBV4	588	542	0.04%	0.005%
100	16.456	2520	2521	2522	rBV	550	244	0.02%	0.002%


Sum of corrected areas: 10003204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036042.D
Acq On : 06 Jun 2023 18:55
Operator : JC/MD
Sample : 02992-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

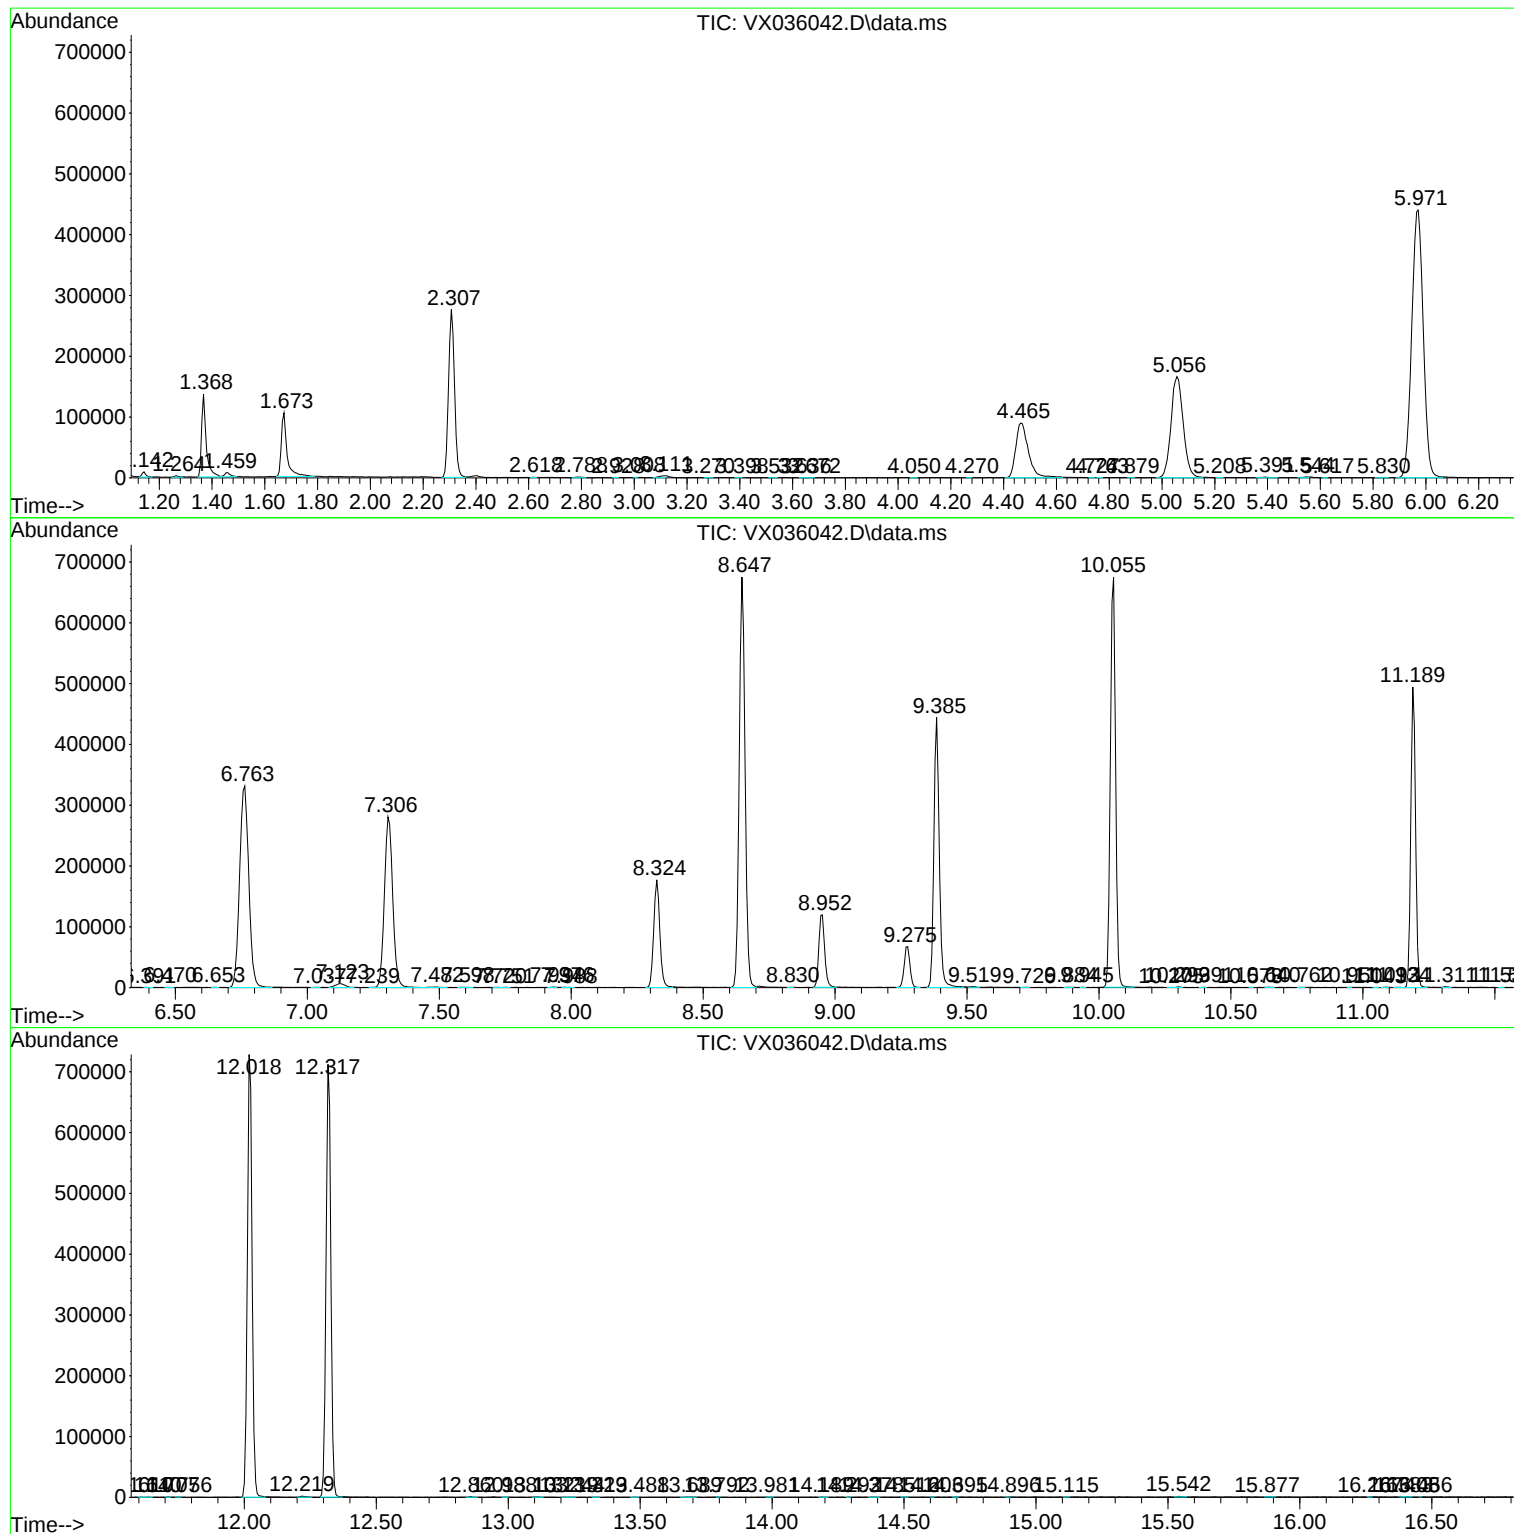

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036042.D
Acq On : 06 Jun 2023 18:55
Operator : JC/MD
Sample : 02992-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036042.D
Acq On : 06 Jun 2023 18:55
Operator : JC/MD
Sample : 02992-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc