

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036043.D
 Acq On : 06 Jun 2023 19:18
 Operator : JC/MD
 Sample : 02992-13 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M

Title : VOC Analysis

Signal : TIC: VX036043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB2	9367	9567	0.76%	0.104%
2	1.264	26	29	32	rBV4	1370	1397	0.11%	0.015%
3	1.368	42	46	59	rBV	133914	164262	13.13%	1.778%
4	1.672	91	96	107	rBV	103640	150375	12.02%	1.628%
5	2.306	193	200	210	rBV	270447	417619	33.38%	4.521%
6	2.794	276	280	289	rVB4	2114	4601	0.37%	0.050%
7	2.940	299	304	312	rVB2	2428	5461	0.44%	0.059%
8	3.087	326	328	331	rVB2	212	237	0.02%	0.003%
9	3.142	336	337	339	rBV2	464	266	0.02%	0.003%
10	3.172	341	342	344	rBV	256	185	0.01%	0.002%
11	3.203	344	347	349	rVB2	286	262	0.02%	0.003%
12	3.581	407	409	410	rBV	325	197	0.02%	0.002%
13	3.709	428	430	432	rBV	189	248	0.02%	0.003%
14	3.879	456	458	461	rBV2	281	276	0.02%	0.003%
15	3.934	462	467	469	rVB2	234	284	0.02%	0.003%
16	3.971	469	473	474	rBV2	173	248	0.02%	0.003%
17	4.038	482	484	488	rBV2	163	245	0.02%	0.003%
18	4.148	500	502	503	rVB	344	208	0.02%	0.002%
19	4.172	503	506	507	rBV	183	202	0.02%	0.002%
20	4.276	522	523	527	rVB2	227	249	0.02%	0.003%
21	4.324	527	531	534	rBV2	298	481	0.04%	0.005%
22	4.471	544	555	568	rBV2	78851	272458	21.78%	2.949%
23	5.056	639	651	669	rVB	156258	490372	39.20%	5.308%
24	5.263	683	685	687	rVB2	282	210	0.02%	0.002%
25	5.324	692	695	696	rBV2	353	276	0.02%	0.003%
26	5.544	726	731	734	rBV4	1347	2652	0.21%	0.029%
27	5.970	788	801	821	rBV2	417732	1251085	100.00%	13.542%
28	6.129	825	827	829	rVB2	390	247	0.02%	0.003%
29	6.312	856	857	859	rBV	283	199	0.02%	0.002%
30	6.385	867	869	874	rVB2	270	397	0.03%	0.004%
31	6.434	874	877	878	rBV2	328	321	0.03%	0.003%
32	6.507	886	889	892	rBV2	215	250	0.02%	0.003%
33	6.678	914	917	918	rBV2	251	238	0.02%	0.003%
34	6.763	920	931	943	rBV	303941	737317	58.93%	7.981%
35	6.989	966	968	970	rBV3	261	240	0.02%	0.003%
36	7.117	983	989	993	rBV6	1330	2695	0.22%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036043.D
 Acq On : 06 Jun 2023 19:18
 Operator : JC/MD
 Sample : 02992-13 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.178	998	999	1004	rBV2	266	237	0.02%	0.003%
38	7.306	1010	1020	1034	rBV	262884	569160	45.49%	6.161%
39	7.482	1045	1049	1050	rBV3	739	903	0.07%	0.010%
40	7.604	1067	1069	1074	rVB2	151	220	0.02%	0.002%
41	7.702	1083	1085	1088	rVB	265	230	0.02%	0.002%
42	7.738	1088	1091	1092	rBV2	249	190	0.02%	0.002%
43	7.866	1110	1112	1114	rBV	240	228	0.02%	0.002%
44	7.933	1119	1123	1130	rVB3	527	911	0.07%	0.010%
45	8.025	1136	1138	1140	rVB2	286	174	0.01%	0.002%
46	8.055	1140	1143	1144	rBV2	193	188	0.02%	0.002%
47	8.208	1165	1168	1169	rBV	249	208	0.02%	0.002%
48	8.324	1181	1187	1202	rBV	159364	260209	20.80%	2.817%
49	8.574	1224	1228	1233	rBV4	668	1122	0.09%	0.012%
50	8.647	1234	1240	1259	rVB	612179	968721	77.43%	10.486%
51	8.952	1283	1290	1304	rBV	110003	168848	13.50%	1.828%
52	9.244	1335	1338	1339	rBV	297	365	0.03%	0.004%
53	9.275	1339	1343	1349	rVB3	2086	3048	0.24%	0.033%
54	9.323	1349	1351	1355	rVB2	278	254	0.02%	0.003%
55	9.384	1355	1361	1378	rBV	438781	619972	49.55%	6.711%
56	9.519	1382	1383	1386	rVV3	715	701	0.06%	0.008%
57	9.567	1390	1391	1393	rBV2	363	286	0.02%	0.003%
58	9.653	1403	1405	1406	rBV	373	288	0.02%	0.003%
59	9.756	1420	1422	1428	rVB2	264	362	0.03%	0.004%
60	9.921	1447	1449	1452	rBV2	210	329	0.03%	0.004%
61	10.055	1465	1471	1481	rBV	642083	863258	69.00%	9.344%
62	10.305	1509	1512	1515	rVB3	864	927	0.07%	0.010%
63	10.464	1536	1538	1541	rBV2	261	277	0.02%	0.003%
64	10.500	1541	1544	1545	rBV2	245	197	0.02%	0.002%
65	10.531	1548	1549	1553	rBV	202	245	0.02%	0.003%
66	10.604	1559	1561	1565	rBV2	194	254	0.02%	0.003%
67	10.640	1565	1567	1568	rBV	245	179	0.01%	0.002%
68	10.872	1602	1605	1607	rBV2	282	244	0.02%	0.003%
69	11.012	1626	1628	1630	rVV2	228	220	0.02%	0.002%
70	11.189	1652	1657	1671	rBV	473089	592519	47.36%	6.414%
71	11.378	1682	1688	1690	rVB2	417	680	0.05%	0.007%
72	11.408	1690	1693	1696	rBV	282	482	0.04%	0.005%
73	11.555	1715	1717	1719	rBV	218	178	0.01%	0.002%
74	11.854	1763	1766	1769	rVB	271	325	0.03%	0.004%
75	11.921	1775	1777	1780	rBV2	290	225	0.02%	0.002%
76	11.969	1783	1785	1788	rBV2	239	176	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
 Data File : VX036043.D
 Acq On : 06 Jun 2023 19:18
 Operator : JC/MD
 Sample : 02992-13 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F6C19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1806	rBV	628721	824869	65.93%	8.929%
78	12.207	1822	1824	1826	rBV2	260	199	0.02%	0.002%
79	12.317	1837	1842	1850	rBV	643430	833978	66.66%	9.027%
80	12.628	1891	1893	1897	rVV	299	255	0.02%	0.003%
81	12.756	1912	1914	1917	rBV2	269	282	0.02%	0.003%
82	12.853	1928	1930	1935	rVB2	264	466	0.04%	0.005%
83	12.920	1939	1941	1943	rBV	247	273	0.02%	0.003%
84	13.048	1960	1962	1964	rVB2	223	173	0.01%	0.002%
85	13.073	1964	1966	1968	rBV2	217	235	0.02%	0.003%
86	13.237	1991	1993	1995	rBV2	364	331	0.03%	0.004%
87	13.329	2006	2008	2011	rBV2	294	378	0.03%	0.004%
88	13.591	2049	2051	2054	rVB2	457	358	0.03%	0.004%
89	13.926	2103	2106	2107	rBV2	356	288	0.02%	0.003%
90	14.121	2136	2138	2140	rBV2	290	337	0.03%	0.004%
91	14.195	2148	2150	2151	rVB	350	184	0.01%	0.002%
92	14.493	2197	2199	2200	rBV	341	229	0.02%	0.002%
93	14.560	2208	2210	2211	rBV2	303	187	0.01%	0.002%
94	14.743	2238	2240	2243	rBV2	300	216	0.02%	0.002%
95	14.999	2281	2282	2287	rVB2	388	359	0.03%	0.004%
96	15.042	2287	2289	2290	rBV	443	250	0.02%	0.003%
97	15.889	2426	2428	2430	rBV2	473	354	0.03%	0.004%
98	16.115	2463	2465	2466	rBV	503	275	0.02%	0.003%
99	16.255	2486	2488	2490	rBV	409	222	0.02%	0.002%
100	16.438	2516	2518	2519	rBV2	440	199	0.02%	0.002%




Sum of corrected areas: 9238264

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036043.D
Acq On : 06 Jun 2023 19:18
Operator : JC/MD
Sample : 02992-13 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

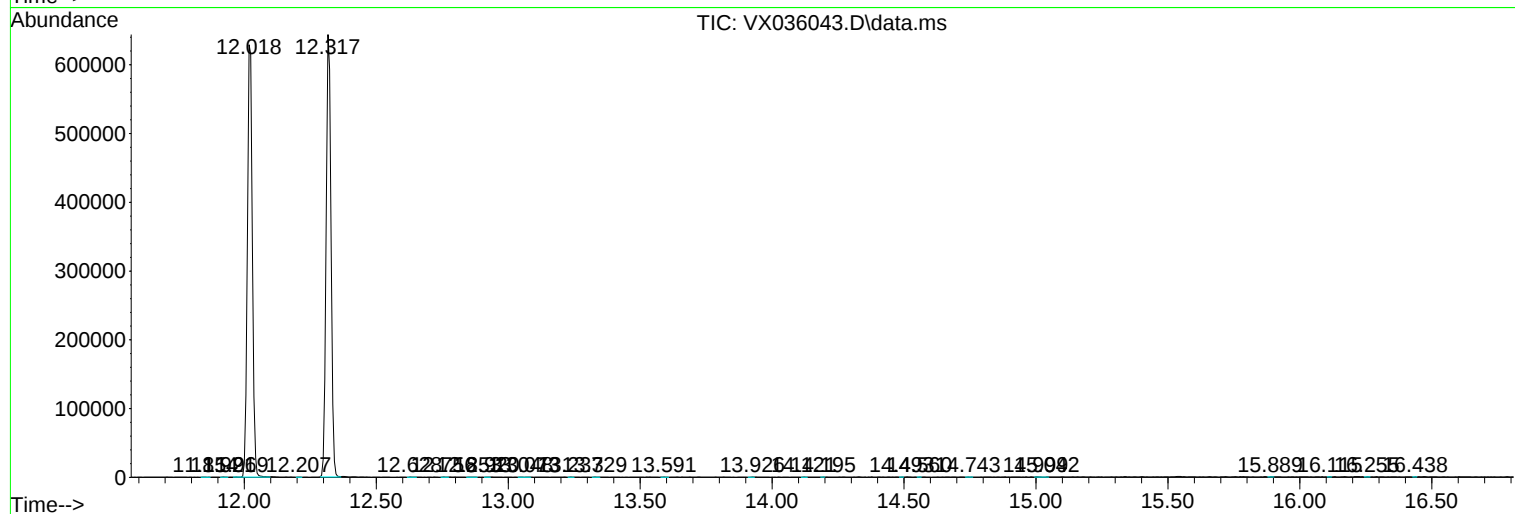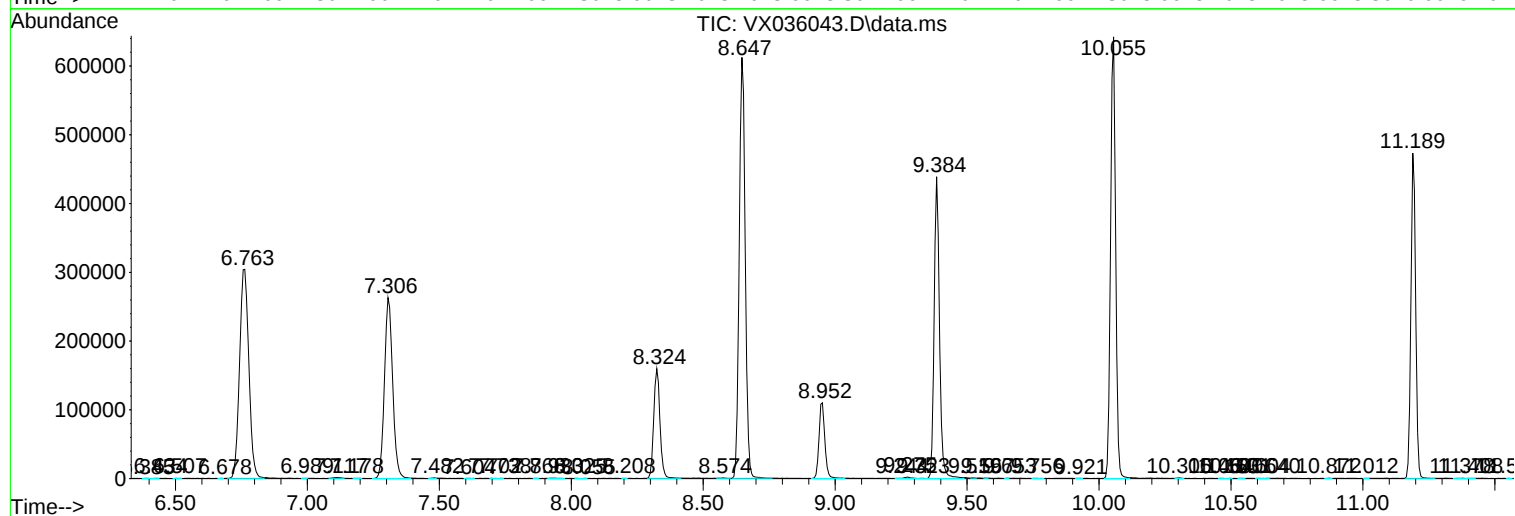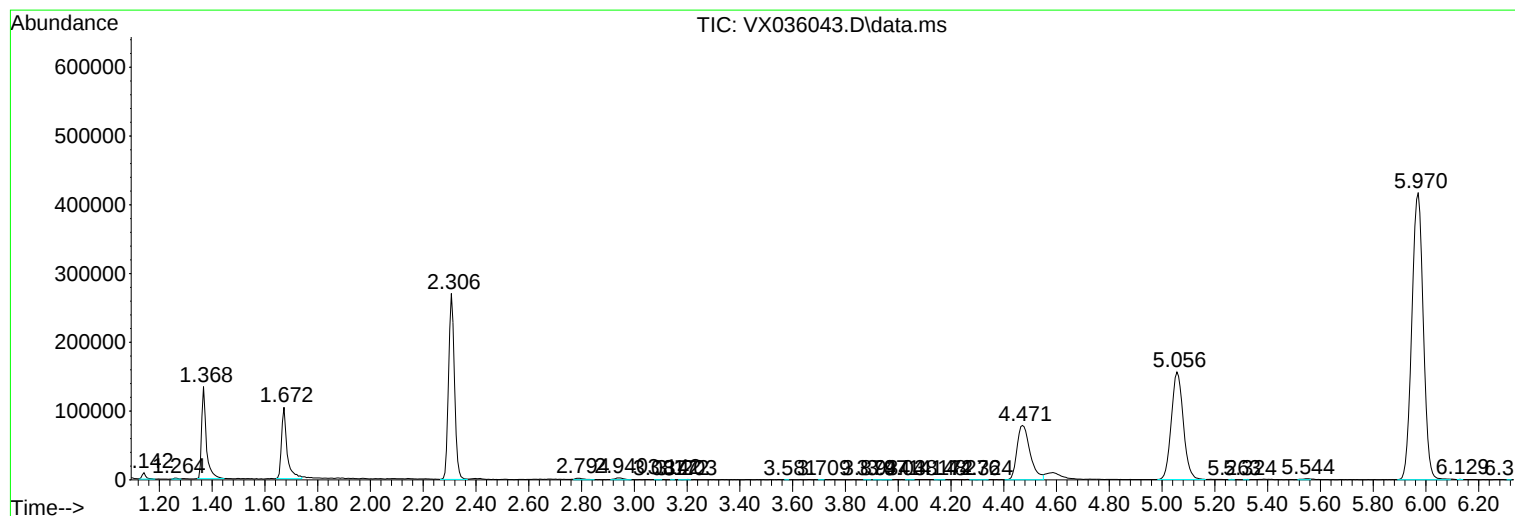

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036043.D
Acq On : 06 Jun 2023 19:18
Operator : JC/MD
Sample : 02992-13 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036043.D
Acq On : 06 Jun 2023 19:18
Operator : JC/MD
Sample : 02992-13 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F6C19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------