
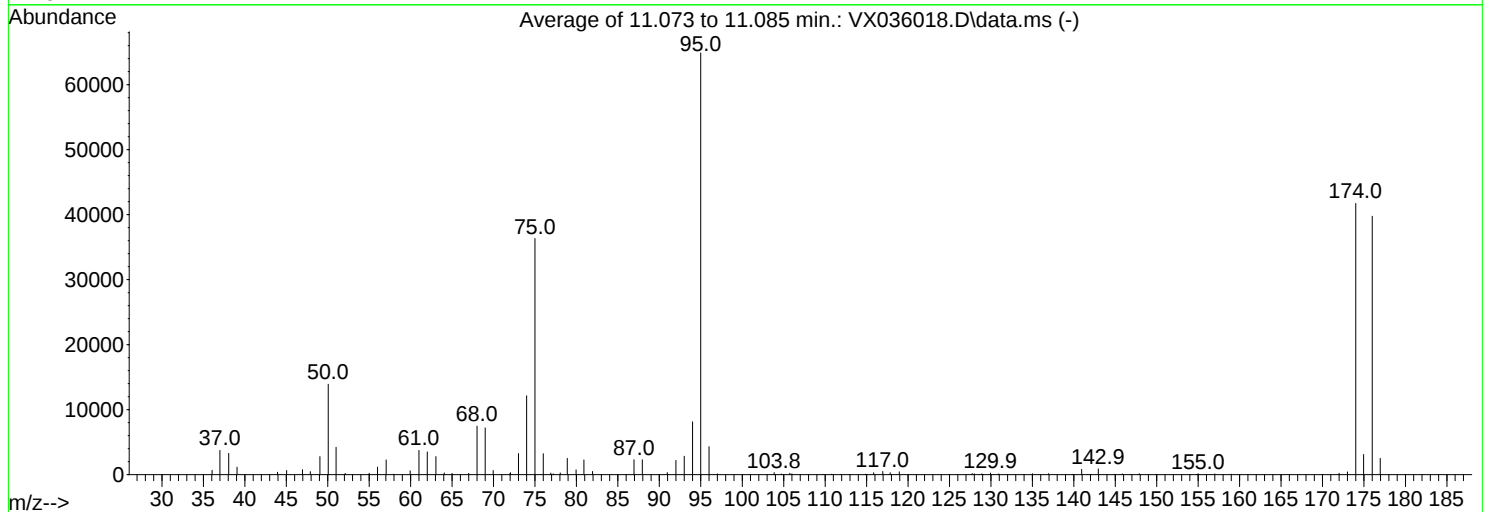


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060623\
Data File : VX036018.D
Acq On : 06 Jun 2023 08:46
Operator : JC/MD
Sample : BFB628
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB628

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM060623WMA.M
Title : VOC Analysis
Last Update : Wed Jun 07 05:37:48 2023

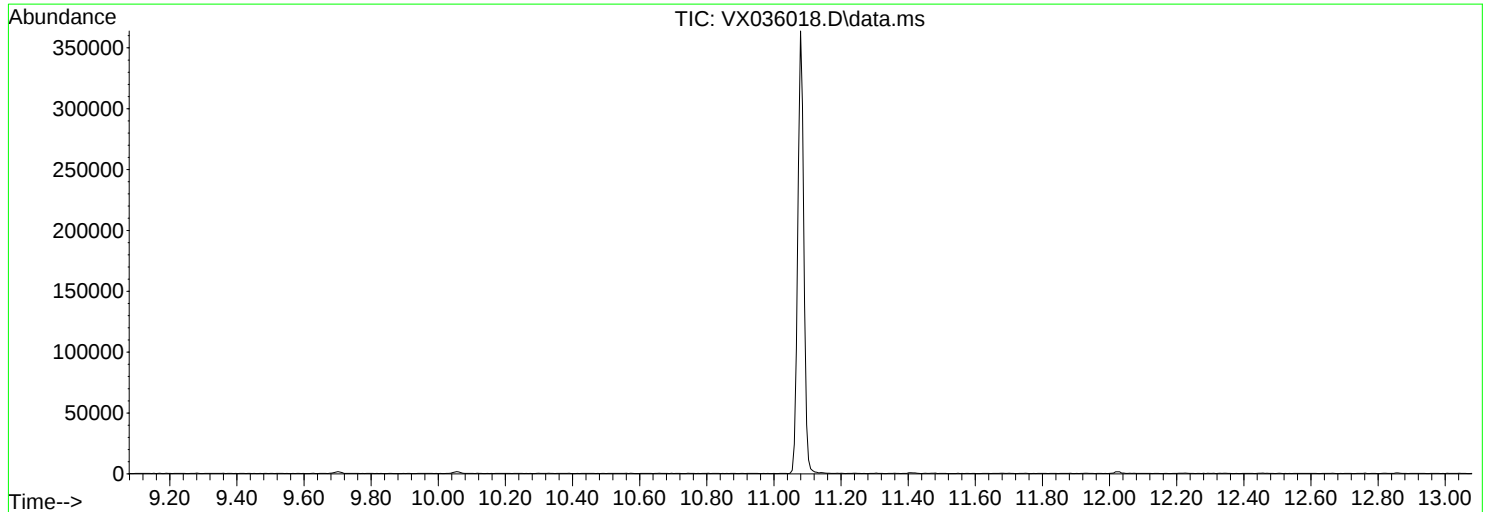

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.4	13915	PASS
75	95	30	80	56.0	36347	PASS
95	95	100	100	100.0	64891	PASS
96	95	5	9	6.6	4307	PASS
173	174	0.00	2	1.0	424	PASS
174	95	50	120	64.3	41733	PASS
175	174	5	9	7.4	3099	PASS
176	174	95	101	95.3	39763	PASS
177	176	5	9	6.3	2502	PASS

m/z	Abundance
40.00	206.0
44.00	226.0

Instrument :
MSVOA_X
ClientSampleId :
BFB628

m/z	Abundance
36.10	618.0
37.00	3565.0
38.00	2986.0
39.00	1184.0
39.90	109.0
43.00	56.0
44.00	544.0
45.00	636.0
47.00	601.0
47.90	355.0
49.10	2342.0
50.10	12427.0
51.00	3622.0
52.00	169.0
55.10	186.0
56.00	1088.0
57.00	1995.0
58.00	57.0
60.00	468.0
61.00	3542.0
62.00	3144.0
63.00	2541.0
64.00	156.0
65.00	135.0
66.90	209.0
68.00	6379.0
69.00	6405.0
70.00	700.0
71.90	414.0
73.00	2603.0
74.00	10546.0
75.00	31784.0
76.00	2896.0
76.90	354.0
78.10	241.0
78.90	2445.0
79.90	575.0
80.90	2115.0
81.90	396.0
86.90	1602.0
88.00	1806.0
90.90	308.0
92.00	1703.0
93.00	2454.0
94.00	6979.0
95.00	55600.0
96.00	3984.0
97.00	134.0
104.00	243.0
104.70	123.0
105.80	335.0
109.70	67.0
110.80	75.0
113.00	54.0
115.00	70.0
116.00	174.0
116.90	425.0
117.90	231.0
119.00	303.0
128.00	212.0
128.90	183.0
129.90	195.0
131.00	144.0
135.00	107.0
136.90	157.0
141.00	596.0
142.00	117.0
142.90	643.0
145.00	63.0
145.80	99.0
147.70	95.0
154.80	55.0
157.00	122.0
159.00	73.0
172.00	210.0
174.00	29936.0
175.00	2226.0
176.00	29696.0
176.90	1736.0

Instrument :
MSVOA_X
ClientSampleId :
BFB628

m/z	Abundance
36.10	797.0
37.00	4644.0
38.10	4004.0
39.10	1265.0
40.00	208.0
43.00	93.0
44.00	583.0
45.10	702.0
46.00	68.0
47.00	968.0
47.90	725.0
49.00	3433.0
50.00	16720.0
51.00	5113.0
52.10	254.0
55.00	340.0
56.00	1297.0
57.00	2717.0
57.90	95.0
60.00	626.0
61.00	4292.0
62.00	4276.0
63.00	3616.0
64.10	406.0
65.10	251.0
67.00	233.0
68.00	8916.0
69.00	8428.0
70.00	605.0
72.10	446.0
73.00	4186.0
74.00	14701.0
75.00	43128.0
76.00	3998.0
77.20	343.0
78.10	298.0
78.90	2796.0
80.00	879.0
80.90	2702.0
81.90	661.0
83.00	96.0
86.00	70.0
86.90	2426.0
88.00	2967.0
91.00	435.0
92.00	2669.0
93.00	3264.0
94.00	9887.0
95.00	76112.0
96.00	4649.0
97.00	174.0
103.80	308.0
104.80	133.0
106.00	384.0
109.70	82.0
110.80	81.0
111.90	60.0
112.90	53.0
114.80	84.0
115.80	295.0
116.90	573.0
117.90	302.0
118.90	613.0
127.70	327.0
128.90	218.0
129.90	267.0
130.90	87.0
134.00	69.0
135.00	173.0
136.90	146.0
139.80	72.0
141.00	1012.0
142.10	60.0
143.00	1010.0
145.00	109.0
145.90	171.0
146.80	81.0
147.90	236.0
155.00	223.0
157.00	182.0
159.00	106.0
171.90	256.0
173.00	753.0
174.00	49888.0
175.00	3884.0
176.00	45920.0
177.00	3007.0
178.00	61.0

Instrument :
MSVOA_X
ClientSampleId :
BFB628

m/z	Abundance
36.00	573.0
37.00	3044.0
38.10	2826.0
39.10	1030.0
40.00	131.0
43.90	650.0
45.00	611.0
46.00	63.0
46.90	711.0
47.90	356.0
49.00	2557.0
50.00	12599.0
51.00	3920.0
52.20	161.0
54.90	148.0
56.00	1078.0
57.10	2111.0
57.90	62.0
59.90	684.0
61.00	3399.0
62.00	3065.0
63.10	2203.0
64.00	272.0
64.90	191.0
67.10	133.0
68.00	7058.0
69.00	6774.0
69.90	595.0
72.00	414.0
73.00	2989.0
74.00	11187.0
75.00	34128.0
76.00	2822.0
76.90	366.0
77.90	255.0
78.90	2319.0
79.90	735.0
80.90	2008.0
82.00	465.0
86.00	65.0
87.00	2841.0
87.90	2087.0
90.90	229.0
92.00	2219.0
93.00	2787.0
94.00	7523.0
95.00	62960.0
96.00	4289.0
97.00	108.0
103.80	387.0
104.70	75.0
105.70	357.0
110.80	58.0
111.90	73.0
114.80	90.0
115.80	418.0
117.00	480.0
117.80	357.0
118.90	389.0
127.80	173.0
128.00	173.0
129.10	98.0
130.00	313.0
131.00	120.0
135.00	144.0
137.00	129.0
139.80	98.0
140.90	856.0
141.70	87.0
142.90	1041.0
144.90	62.0
145.90	135.0
146.90	97.0
147.90	240.0
149.90	77.0
154.10	66.0
155.00	232.0
157.00	57.0
159.00	71.0
172.10	233.0
173.00	519.0
174.00	45376.0
174.90	3187.0
176.00	43672.0
177.00	2763.0

Instrument :
MSVOA_X
ClientSampleId :
BFB628