

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060624\
 Data File : VX041764.D
 Acq On : 06 Jun 2024 10:00
 Operator : JC/MD
 Sample : VX0606MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0606MBL01

Quant Time: Jun 07 00:55:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 30 07:36:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	147974	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	230477	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	227452	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	111865	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	86819	47.838	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.680%
35) Dibromofluoromethane	5.385	113	72746	45.652	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.300%
50) Toluene-d8	8.647	98	272906	49.014	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.020%
62) 4-Bromofluorobenzene	11.079	95	102271	49.767	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060624\
Data File : VX041764.D
Acq On : 06 Jun 2024 10:00
Operator : JC/MD
Sample : VX0606MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0606MBL01

Quant Time: Jun 07 00:55:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260
QLast Update : Thu May 30 07:36:24 2024
Response via : Initial Calibration




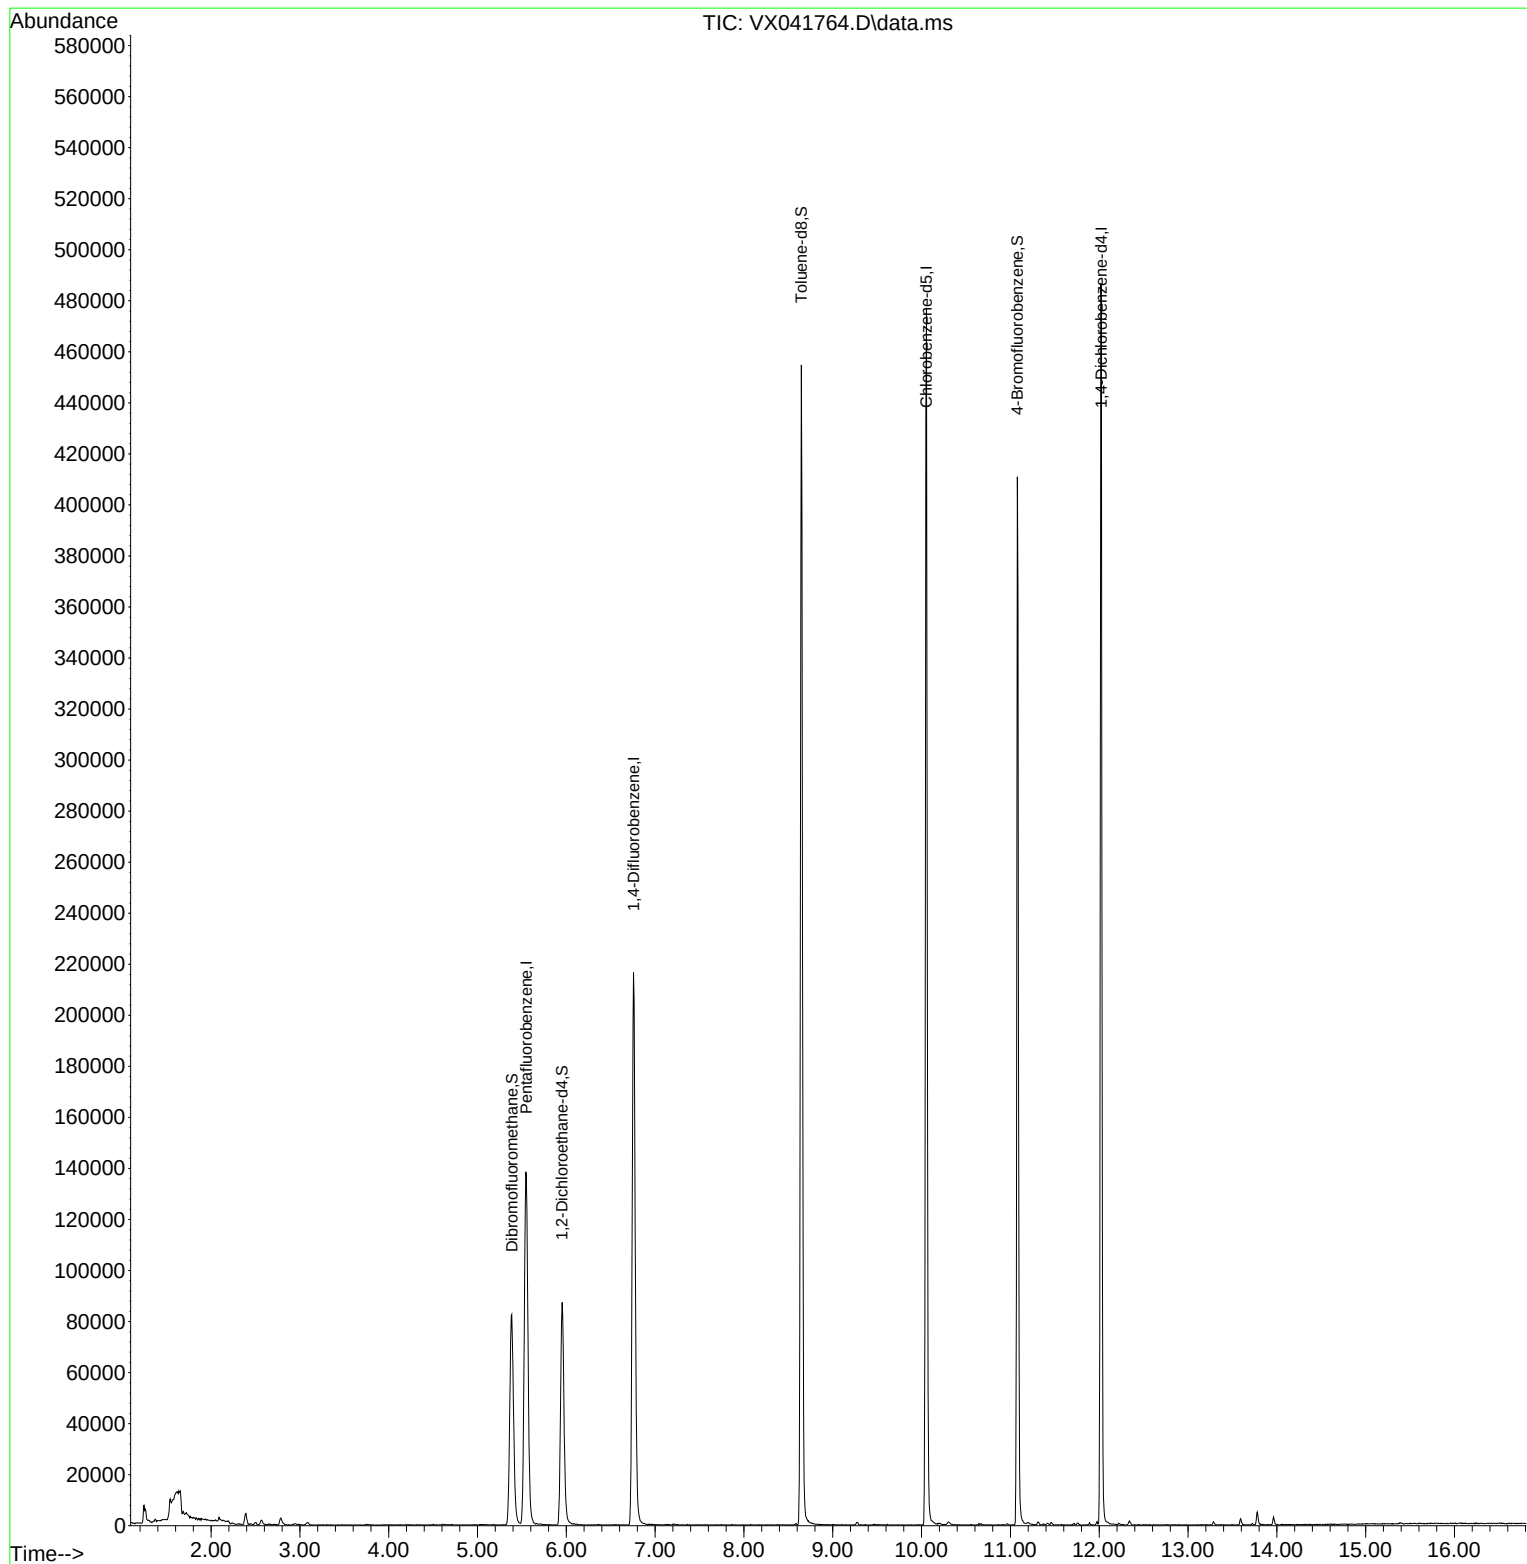


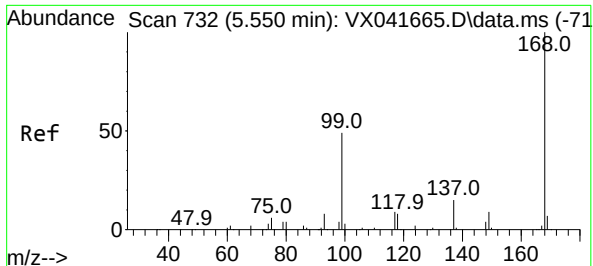

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX041764.D
Acq: 06 Jun 2024 10:00




Instrument :
MSVOA_X
ClientSampleId :
VX0606MBL01


Tgt Ion:168 Resp: 147974
Ion Ratio Lower Upper
168 100
99 49.8 56.6 85.0#

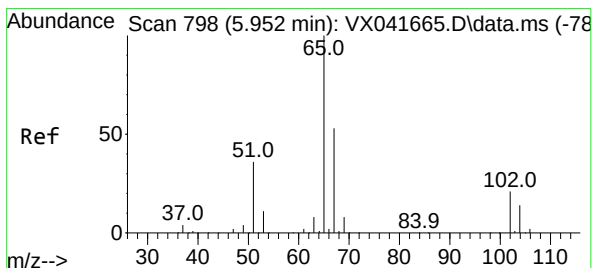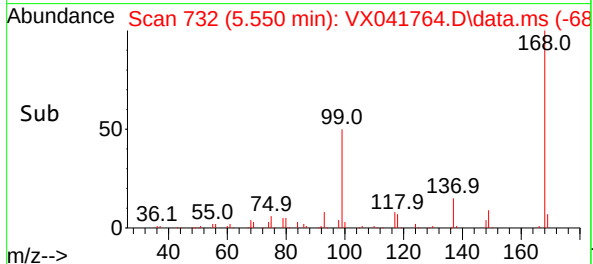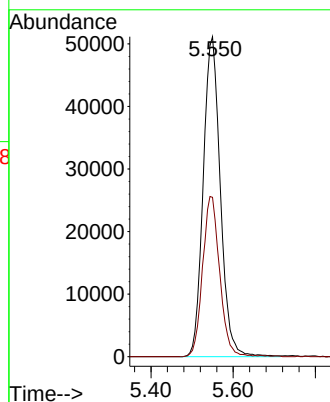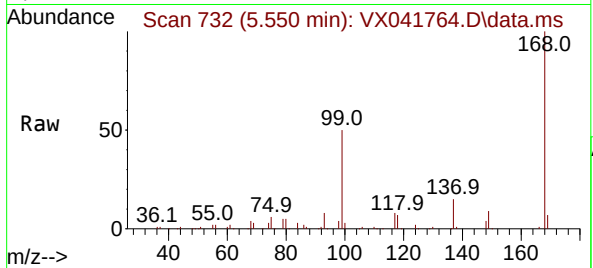

#33
1,2-Dichloroethane-d4
Concen: 47.838 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX041764.D
Acq: 06 Jun 2024 10:00

Tgt Ion: 65 Resp: 86819
Ion Ratio Lower Upper
65 100
67 50.8 0.0 100.2


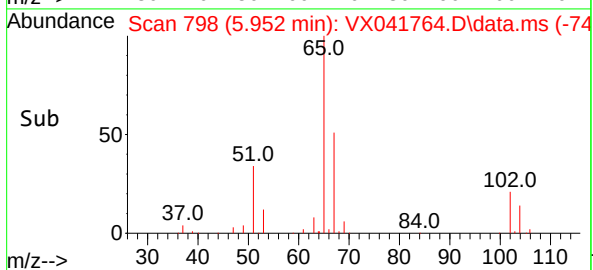
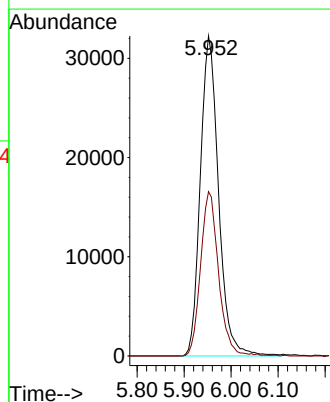
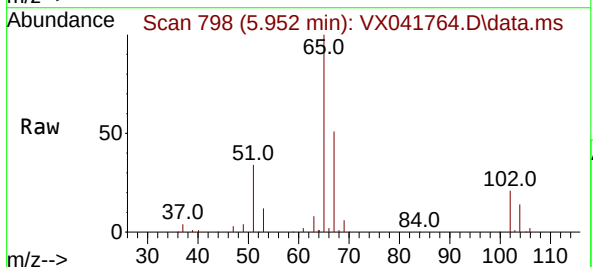


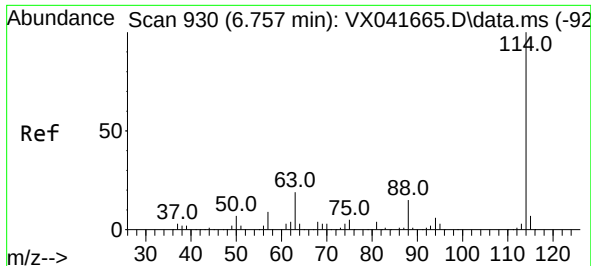

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX041764.D
Acq: 06 Jun 2024 10:00




Instrument :
MSVOA_X
ClientSampleId :
VX0606MBL01


Tgt Ion:114 Resp: 230477
Ion Ratio Lower Upper
114 100
63 20.3 0.0 45.0
88 14.9 0.0 36.6

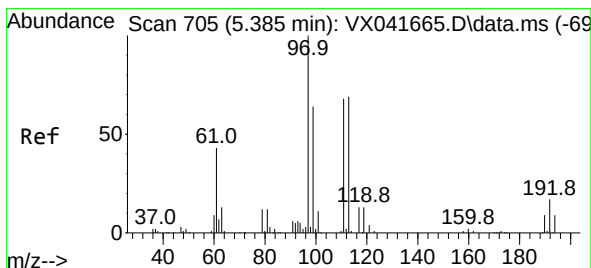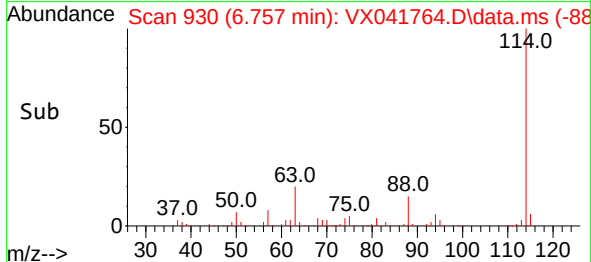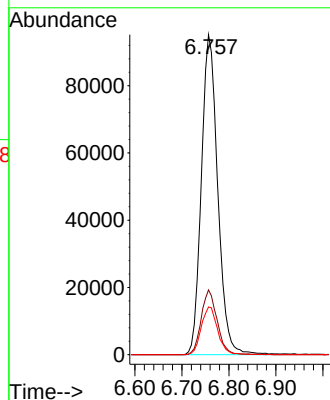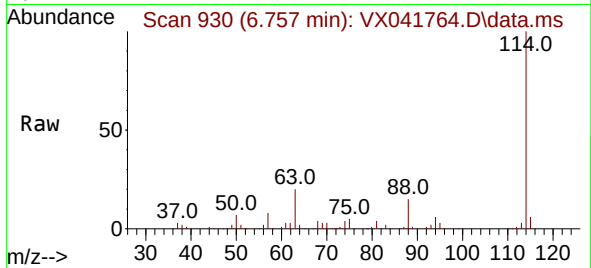

#35
Dibromofluoromethane
Concen: 45.652 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX041764.D
Acq: 06 Jun 2024 10:00

Tgt Ion:113 Resp: 72746
Ion Ratio Lower Upper
113 100
111 101.1 82.9 124.3
192 24.2 13.3 19.9#


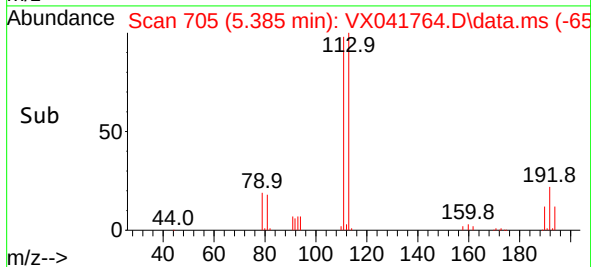
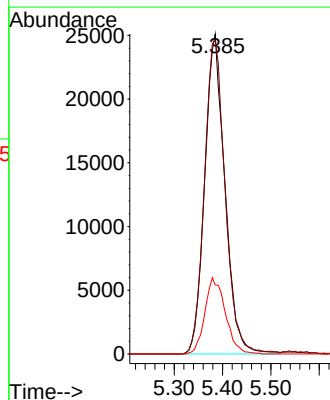
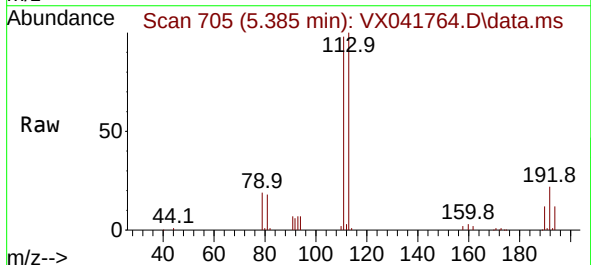


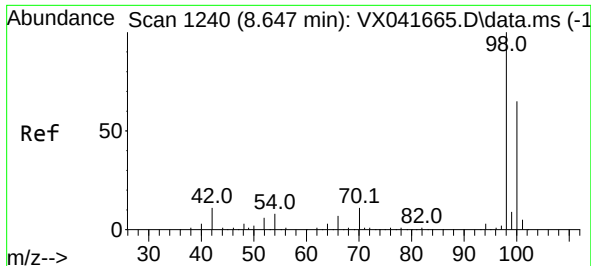

#50
Toluene-d8
Concen: 49.014 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX041764.D
Acq: 06 Jun 2024 10:00




Instrument :
MSVOA_X
ClientSampleId :
VX0606MBL01


Tgt Ion: 98 Resp: 272906
Ion Ratio Lower Upper
98 100
100 66.1 53.1 79.7

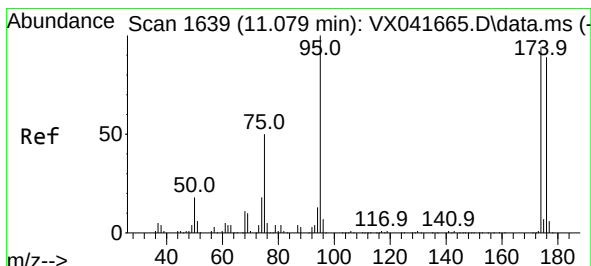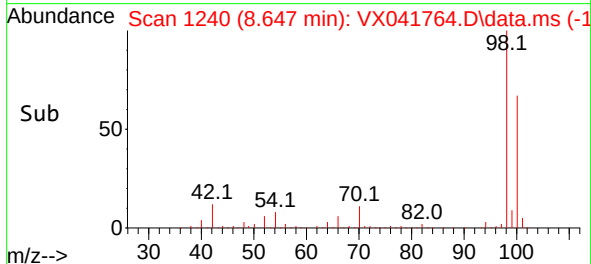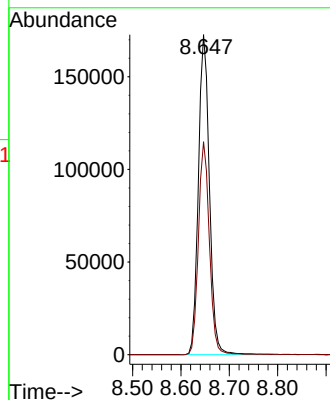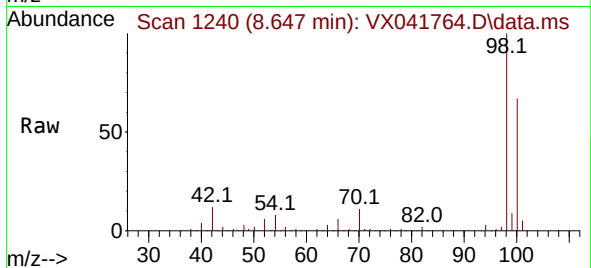

#62
4-Bromofluorobenzene
Concen: 49.767 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX041764.D
Acq: 06 Jun 2024 10:00

Tgt Ion: 95 Resp: 102271
Ion Ratio Lower Upper
95 100
174 95.8 0.0 135.6
176 91.9 0.0 131.0


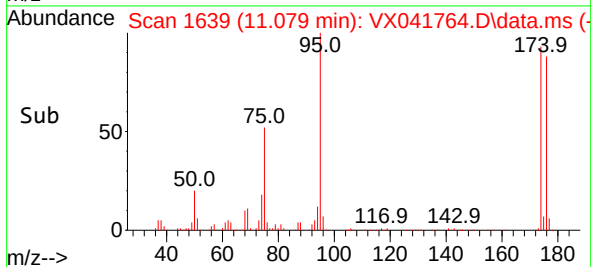
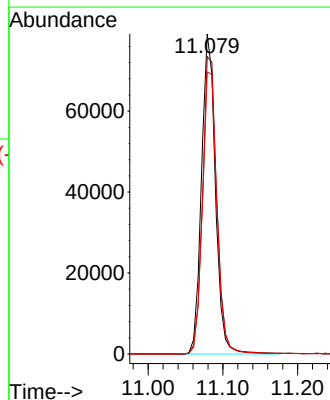
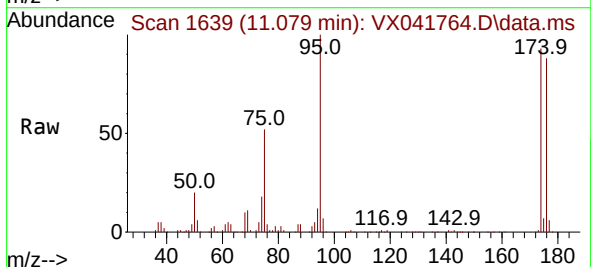


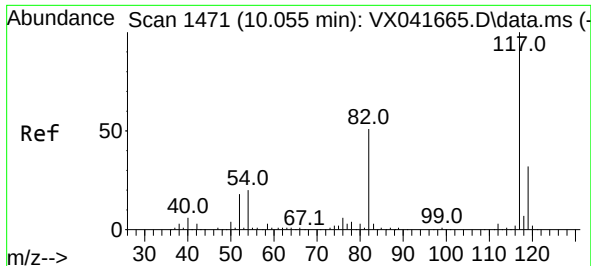

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX041764.D
Acq: 06 Jun 2024 10:00

Instrument :
MSVOA_X
ClientSampleId :
VX0606MBL01

Tgt Ion:117 Resp: 227452
Ion Ratio Lower Upper
117 100
82 51.0 46.2 69.4
119 32.1 25.5 38.3

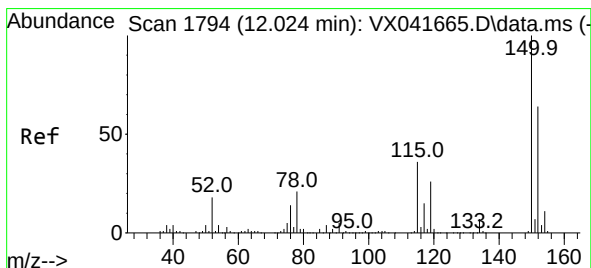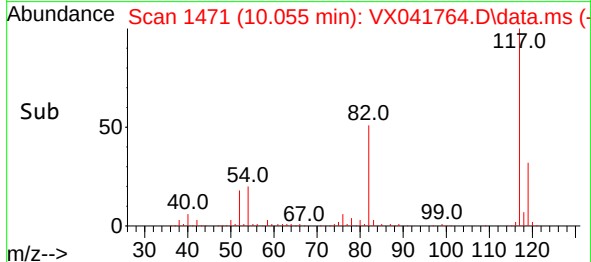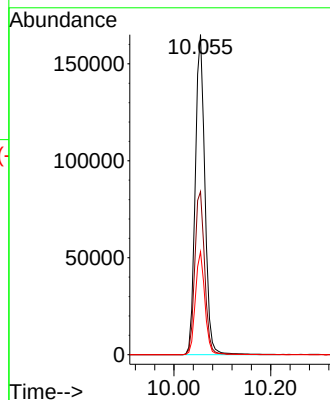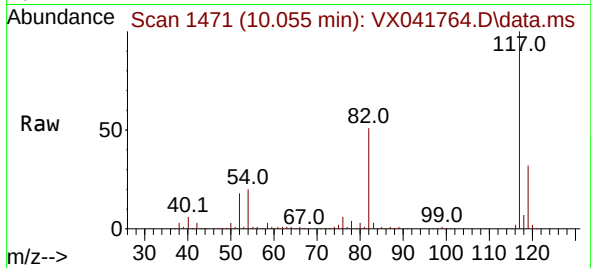

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX041764.D
Acq: 06 Jun 2024 10:00

Tgt Ion:152 Resp: 111865
Ion Ratio Lower Upper
152 100
115 54.0 43.3 129.9
150 155.3 0.0 345.0

