

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060624\
 Data File : VX041772.D
 Acq On : 06 Jun 2024 13:10
 Operator : JC/MD
 Sample : P2749-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SY-12I

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
 Title : SW846 8260

Signal : TIC: VX041772.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	7349	8357	1.21%	0.197%
2	1.551	69	76	79	rBV2	7375	14481	2.10%	0.341%
3	2.947	297	305	311	rBV	8907	20666	2.99%	0.486%
4	3.605	404	413	425	rVB	9688	22709	3.29%	0.534%
5	4.495	549	559	570	rBV2	11377	32412	4.69%	0.763%
6	5.032	640	647	658	rBV4	3217	10606	1.53%	0.250%
7	5.385	695	705	721	rBV2	70624	209335	30.28%	4.927%
8	5.550	721	732	760	rVB	119482	343557	49.70%	8.086%
9	5.958	789	799	809	rBV	76139	205110	29.67%	4.828%
10	6.763	921	931	950	rBV	183839	447008	64.67%	10.521%
11	8.647	1234	1240	1251	rBV	386775	606819	87.79%	14.282%
12	9.275	1338	1343	1349	rVB2	5702	8440	1.22%	0.199%
13	10.055	1465	1471	1473	rBV	410687	591147	85.52%	13.913%
14	10.080	1473	1475	1490	rVB	284293	342628	49.57%	8.064%
15	10.293	1499	1510	1518	rVB	19860	31307	4.53%	0.737%
16	10.866	1595	1604	1613	rBV4	4710	8705	1.26%	0.205%
17	11.079	1634	1639	1653	rBV	339981	446401	64.58%	10.507%
18	11.366	1679	1686	1692	rBV	7994	11694	1.69%	0.275%
19	11.969	1781	1785	1789	rBV	32362	42694	6.18%	1.005%
20	12.024	1789	1794	1808	rVV2	409245	691217	100.00%	16.269%
21	12.152	1808	1815	1820	rVV5	6728	10904	1.58%	0.257%
22	12.335	1839	1845	1857	rVB	62429	82376	11.92%	1.939%
23	12.524	1867	1876	1879	rBV5	4207	9137	1.32%	0.215%
24	12.561	1879	1882	1891	rVB2	10670	18318	2.65%	0.431%
25	12.664	1891	1899	1903	rBV6	4479	9568	1.38%	0.225%
26	13.122	1969	1974	1980	rBV3	8784	13416	1.94%	0.316%
27	13.939	2103	2108	2117	rBV4	5779	9736	1.41%	0.229%




Sum of corrected areas: 4248748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060624\
Data File : VX041772.D
Acq On : 06 Jun 2024 13:10
Operator : JC/MD
Sample : P2749-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SY-12I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

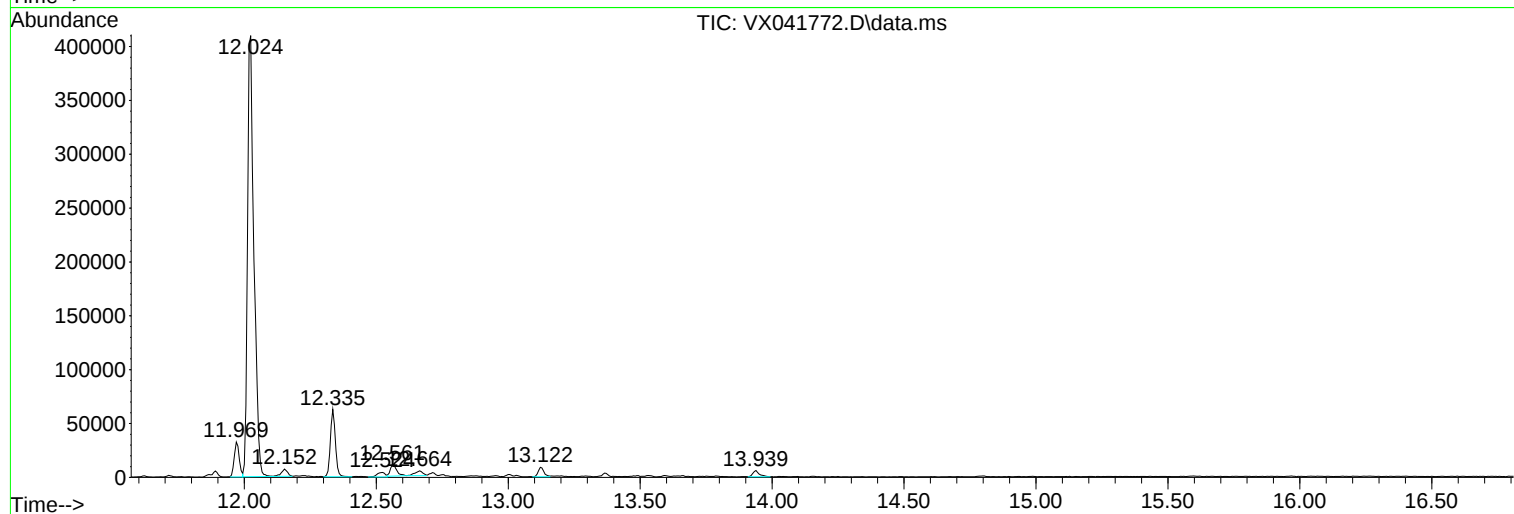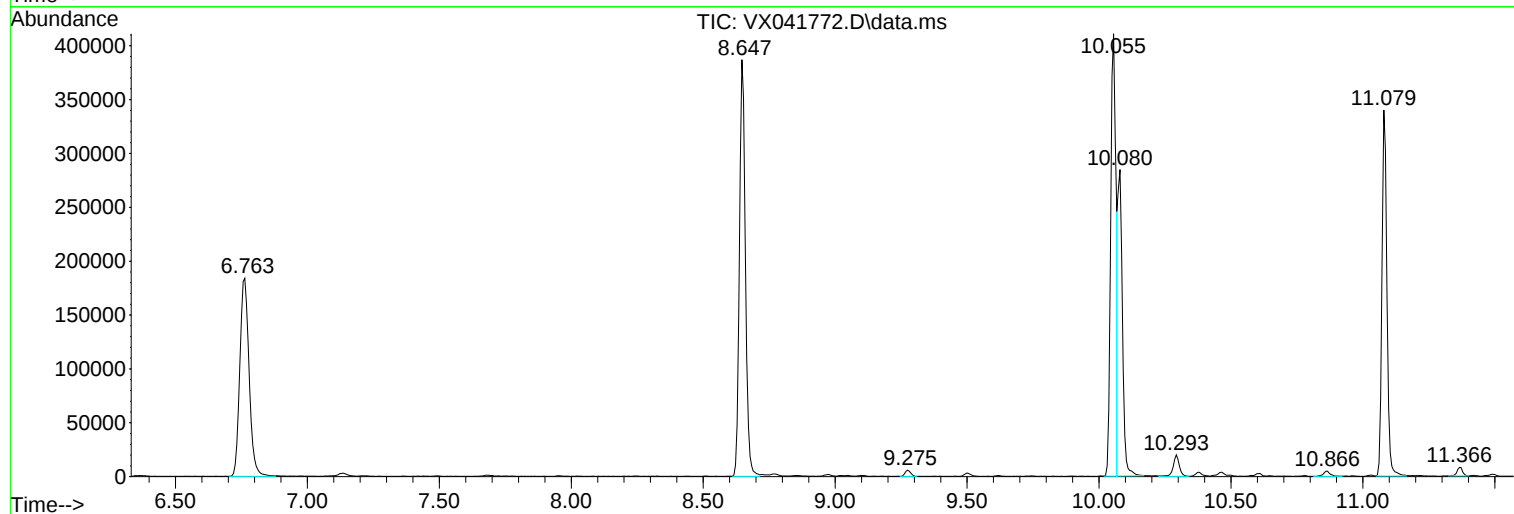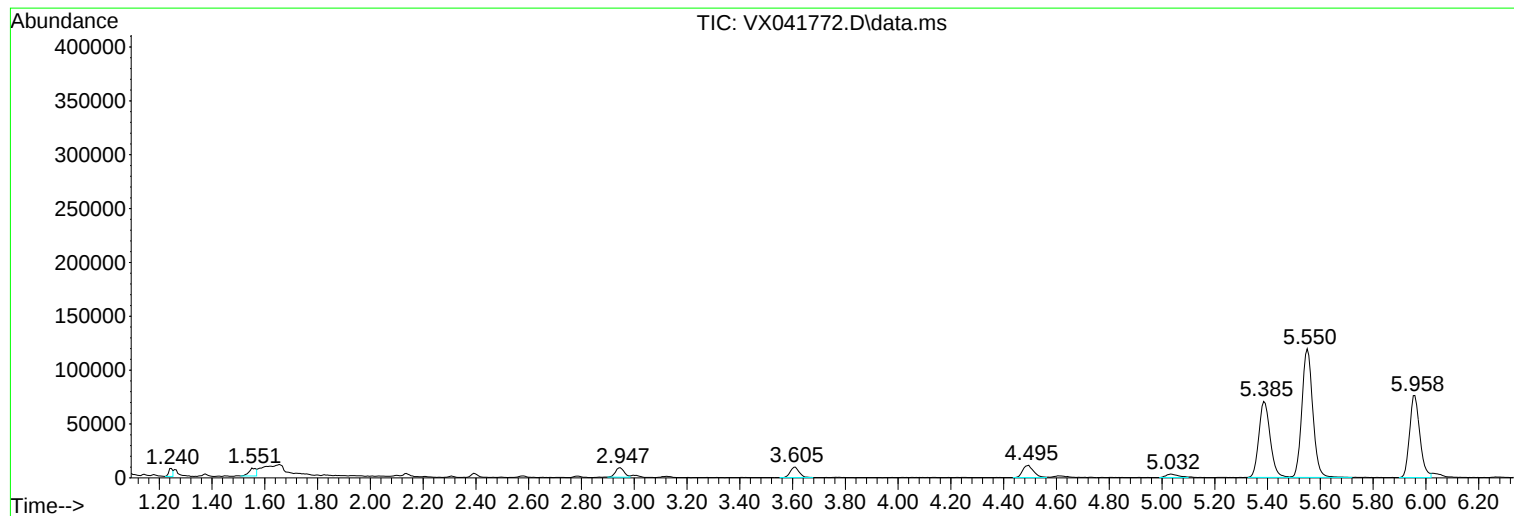

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060624\
Data File : VX041772.D
Acq On : 06 Jun 2024 13:10
Operator : JC/MD
Sample : P2749-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SY-12I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060624\
Data File : VX041772.D
Acq On : 06 Jun 2024 13:10
Operator : JC/MD
Sample : P2749-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SY-12I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc