

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\WX060625\
 Data File : VX046555.D
 Acq On : 07 Jun 2025 04:31
 Operator : JC/MD
 Sample : Q2236-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-A2-07-G

Quant Time: Jun 07 05:25:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	119993	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.775	114	228870	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	241518	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	121477	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	101404	47.501	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	95.000%
35) Dibromofluoromethane	5.403	113	58738	34.899	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	69.800%#
50) Toluene-d8	8.653	98	293116	52.823	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	105.640%
62) 4-Bromofluorobenzene	11.079	95	133450	58.126	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	116.260%
Target Compounds						
					Qvalue	
8) Diethyl Ether	2.148	74	27604	31.239	ug/l	93
11) Tert butyl alcohol	2.965	59	322	1.359	ug/l #	72
13) Acrolein	2.257	56	147	30.457	ug/l	84
16) Acetone	2.391	43	52524	66.097	ug/l	99
17) Carbon Disulfide	2.538	76	762	0.453	ug/l #	76
20) Methylene Chloride	2.812	84	2744	1.602	ug/l #	79
25) 2-Butanone	4.604	43	2876	2.420	ug/l	94
31) Cyclohexane	5.574	56	2951	1.189	ug/l #	21
36) 1,1-Dichloropropene	5.562	75	10974	4.565	ug/l #	52
38) Carbon Tetrachloride	5.562	117	14062	5.222	ug/l #	16
40) Benzene	6.049	78	425637	62.888	ug/l	99
42) 1,2-Dichloroethane	6.049	62	4380	1.556	ug/l #	78
48) Methyl methacrylate	7.628	41	681	0.324	ug/l #	24
51) 4-Methyl-2-Pentanone	8.579	43	1740	0.669	ug/l	97
52) Toluene	8.720	92	177358	42.654	ug/l	99
53) t-1,3-Dichloropropene	8.720	75	2373	0.979	ug/l #	1
55) 1,1,2-Trichloroethane	9.018	97	2568	1.538	ug/l #	18
59) 2-Hexanone	9.457	43	489	0.262	ug/l	77
67) Ethyl Benzene	10.195	91	960531	96.864	ug/l	98
68) m/p-Xylenes	10.299	106	164878	45.836	ug/l	100
69) o-Xylene	10.640	106	114888	33.020	ug/l	99
70) Styrene	10.652	104	22278	3.741	ug/l #	19
73) Isopropylbenzene	10.963	105	45915	4.808	ug/l	100
76) 1,2,3-Trichloropropane	11.378	75	2782	1.081	ug/l #	1
78) n-propylbenzene	11.304	91	11028	0.954	ug/l #	54
79) 2-Chlorotoluene	11.378	91	35485	5.091	ug/l #	45
80) 1,3,5-Trimethylbenzene	11.451	105	43065	5.412	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	72526	81.309	ug/l #	1
82) 4-Chlorotoluene	11.451	91	5224	0.632	ug/l #	48
83) tert-Butylbenzene	11.750	119	17378	2.145	ug/l #	41
84) 1,2,4-Trimethylbenzene	11.750	105	151023	18.761	ug/l	98
85) sec-Butylbenzene	11.750	105	151023	14.509	ug/l #	57
86) p-Isopropyltoluene	12.012	119	6183	0.713	ug/l #	69
89) n-Butylbenzene	12.243	91	237138	27.829	ug/l #	44
90) Hexachloroethane	12.408	117	60780	39.410	ug/l #	19
92) 1,2-Dibromo-3-Chloropr...	12.963	75	643	0.939	ug/l #	10

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046555.D
Acq On : 07 Jun 2025 04:31
Operator : JC/MD
Sample : Q2236-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G

Quant Time: Jun 07 05:25:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
95) Naphthalene	13.786	128	9909635	1102.595	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046555.D
Acq On : 07 Jun 2025 04:31
Operator : JC/MD
Sample : Q2236-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Quant Time: Jun 07 05:25:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

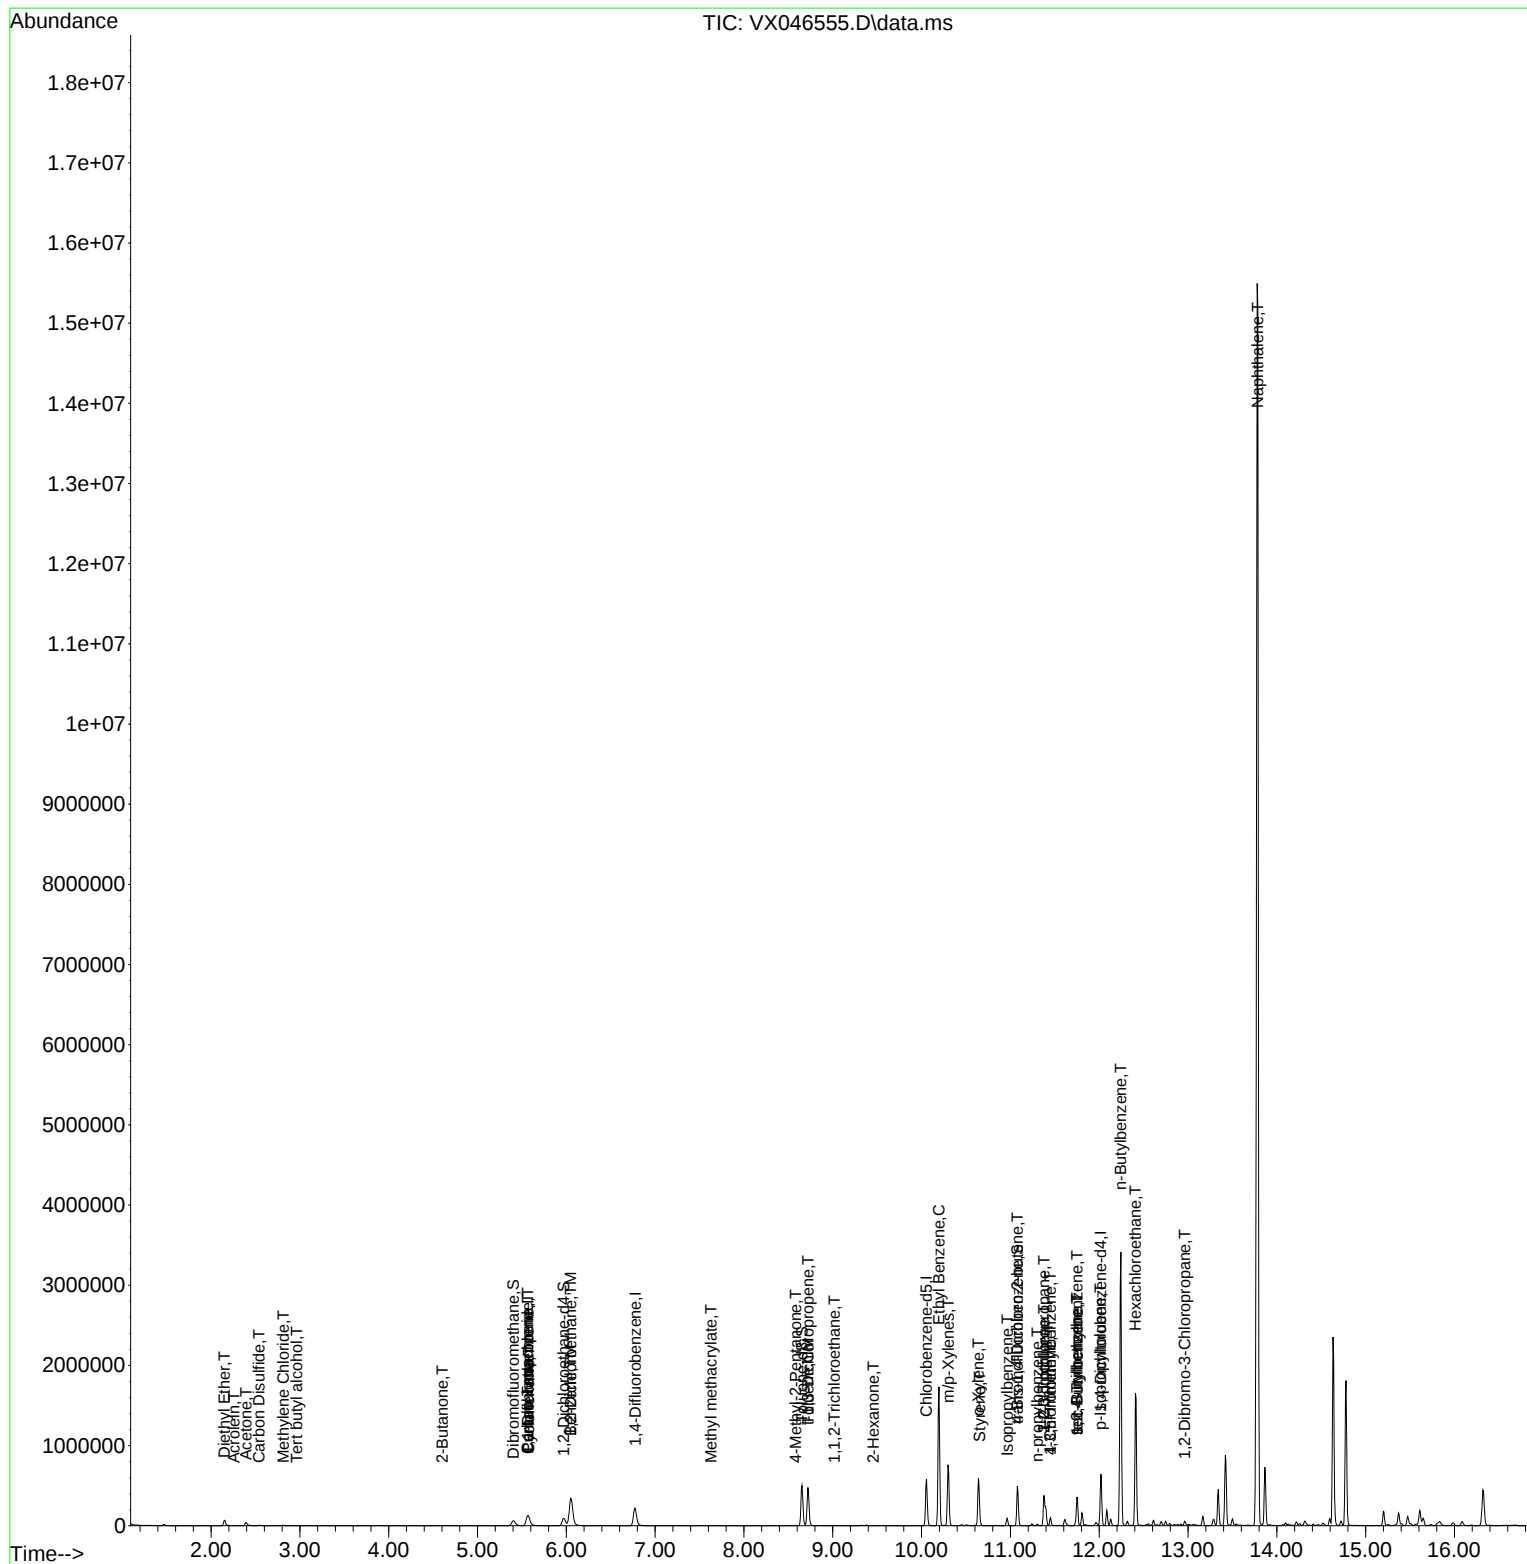



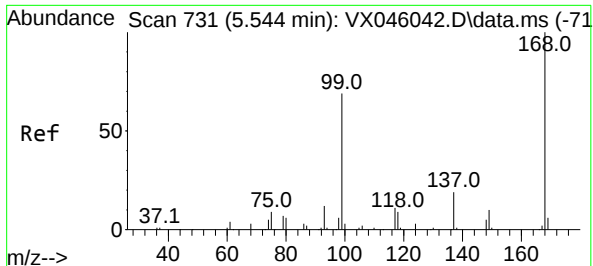


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.568 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G



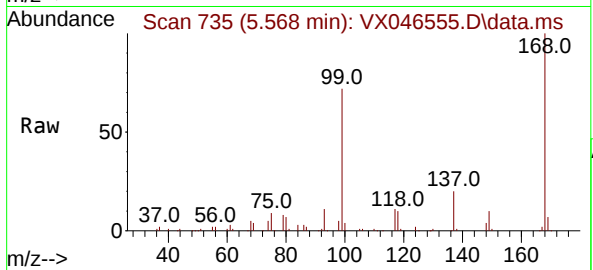



Tgt Ion:168 Resp: 119993
Ion Ratio Lower Upper
168 100
99 71.9 54.9 82.3

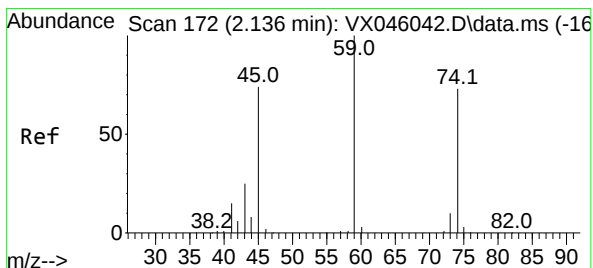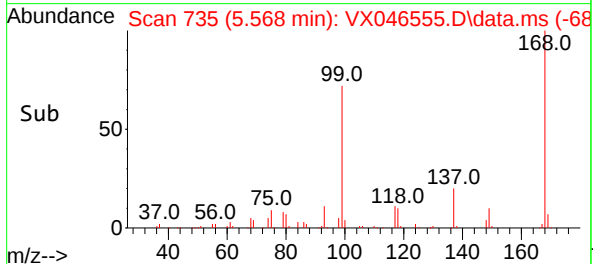

#8
Diethyl Ether
Concen: 31.239 ug/l
RT: 2.148 min Scan# 174
Delta R.T. -0.006 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 74 Resp: 27604
Ion Ratio Lower Upper
74 100
45 102.9 54.9 164.8


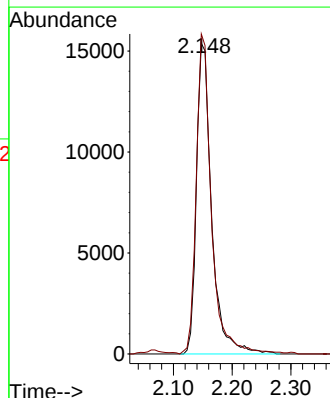
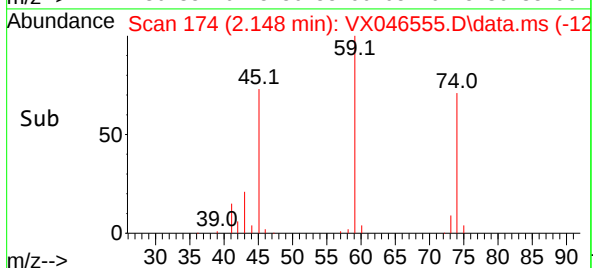
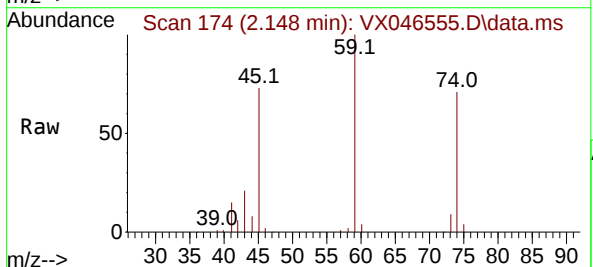


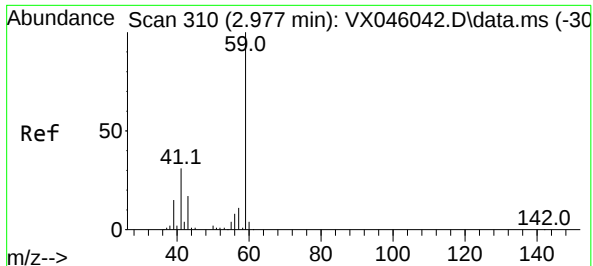

#11
Tert butyl alcohol
Concen: 1.359 ug/l
RT: 2.965 min Scan# 30
Delta R.T. -0.006 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion: 59 Resp: 322
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#

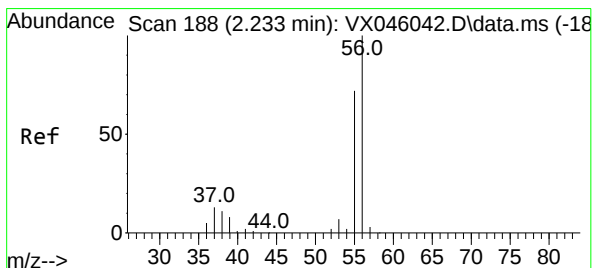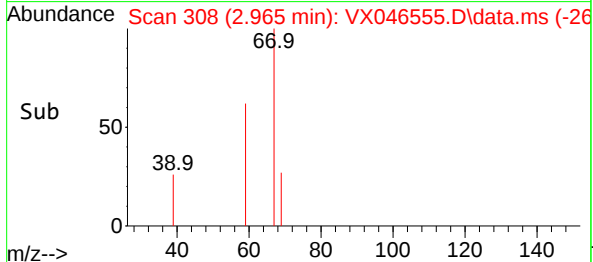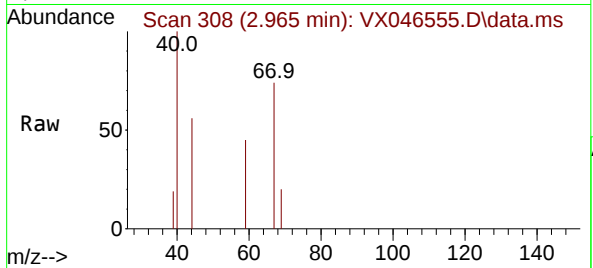

#13
Acrolein
Concen: 30.457 ug/l
RT: 2.257 min Scan# 192
Delta R.T. 0.006 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 56 Resp: 147
Ion Ratio Lower Upper
56 100
55 57.1 56.2 84.4


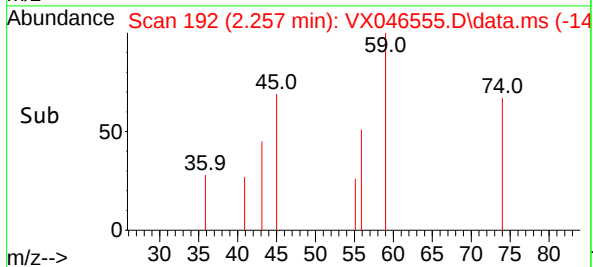

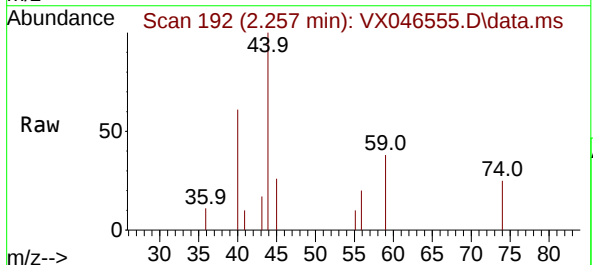




#16
Acetone
Concen: 66.097 ug/l
RT: 2.391 min Scan# 214
Delta R.T. -0.001 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion: 43 Resp: 52524
Ion Ratio Lower Upper
43 100
58 27.2 21.2 31.8

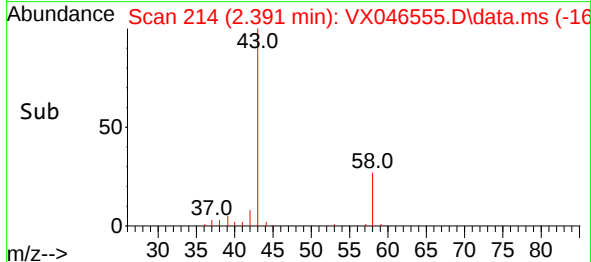

#17
Carbon Disulfide
Concen: 0.453 ug/l
RT: 2.538 min Scan# 238
Delta R.T. 0.006 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 76 Resp: 762
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.4#


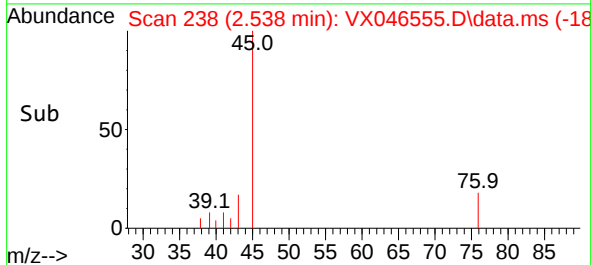






#20
Methylene Chloride
Concen: 1.602 ug/l
RT: 2.812 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion:	84	Resp:	2744
Ion	Ratio	Lower	Upper
84	100		
49	116.9	113.9	170.9
51	32.2	33.5	50.3#
86	46.8	53.8	80.8#

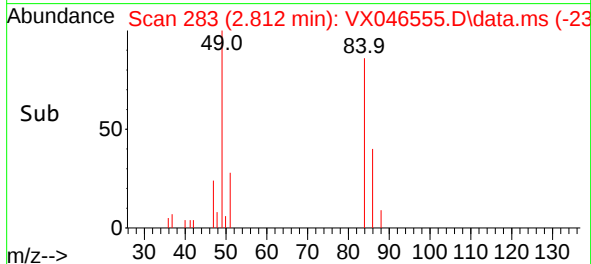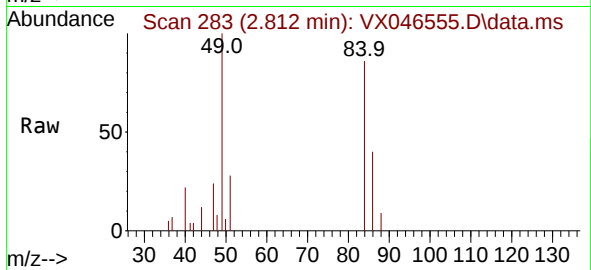

#25
2-Butanone
Concen: 2.420 ug/l
RT: 4.604 min Scan# 577
Delta R.T. 0.030 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion:	43	Resp:	2876
Ion	Ratio	Lower	Upper
43	100		
72	20.2	18.4	27.6


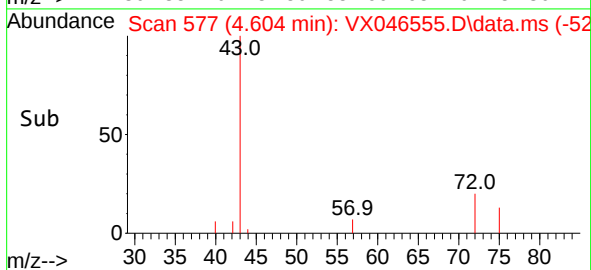




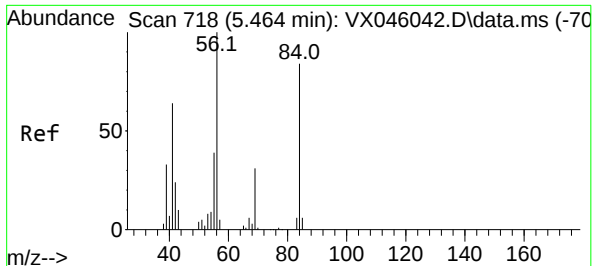

#31
Cyclohexane
Concen: 1.189 ug/l
RT: 5.574 min Scan# 718
Delta R.T. 0.085 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion: 56 Resp: 2951
Ion Ratio Lower Upper
56 100
69 153.9 24.4 36.6#
84 106.3 66.9 100.3#

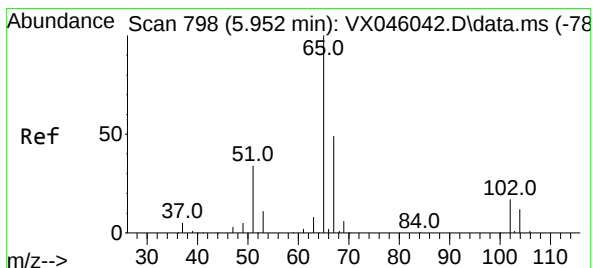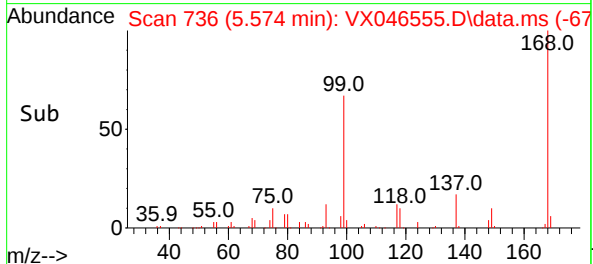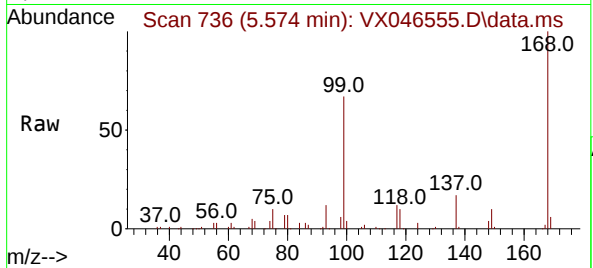

#33
1,2-Dichloroethane-d4
Concen: 47.501 ug/l
RT: 5.970 min Scan# 801
Delta R.T. 0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 65 Resp: 101404
Ion Ratio Lower Upper
65 100
67 50.4 0.0 99.0


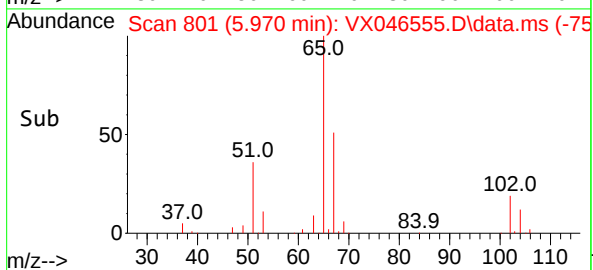

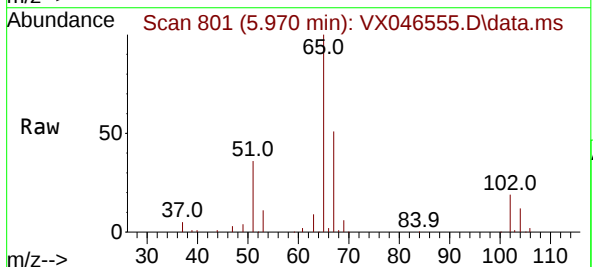




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.775 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion:114 Resp: 228870
Ion Ratio Lower Upper
114 100
63 22.9 0.0 49.2
88 18.0 0.0 33.6

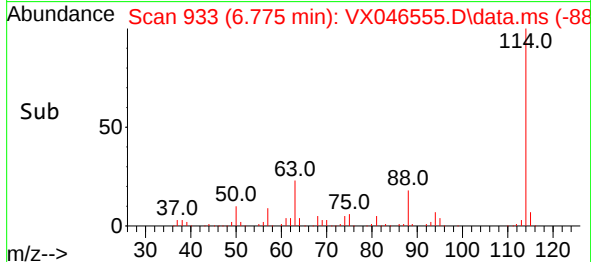

#35
Dibromofluoromethane
Concen: 34.899 ug/l
RT: 5.403 min Scan# 708
Delta R.T. 0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion:113 Resp: 58738
Ion Ratio Lower Upper
113 100
111 102.0 83.1 124.7
192 16.7 13.3 19.9




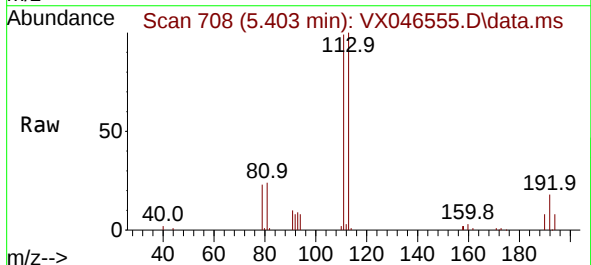




#36
 1,1-Dichloropropene
 Concen: 4.565 ug/l
 RT: 5.562 min Scan# 714
 Delta R.T. -0.152 min
 Lab File: VX046555.D
 Acq: 07 Jun 2025 04:31




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-A2-07-G


Tgt Ion: 75 Resp: 10974
 Ion Ratio Lower Upper
 75 100
 110 9.5 16.3 48.9#
 77 0.0 24.3 36.5#

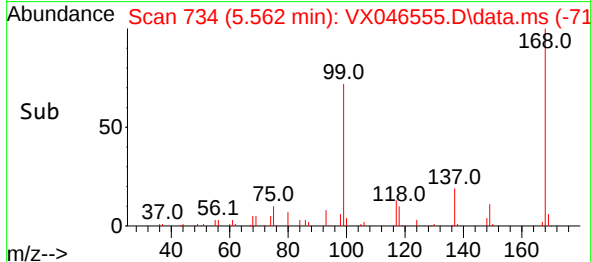

#38
 Carbon Tetrachloride
 Concen: 5.222 ug/l
 RT: 5.562 min Scan# 734
 Delta R.T. -0.134 min
 Lab File: VX046555.D
 Acq: 07 Jun 2025 04:31

Tgt Ion: 117 Resp: 14062
 Ion Ratio Lower Upper
 117 100
 119 3.9 75.2 112.8#
 121 0.0 24.2 36.4#

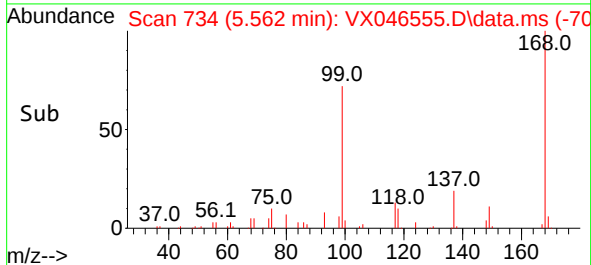



#40

Benzene

Concen: 62.888 ug/l

RT: 6.049 min Scan# 814

Delta R.T. -0.007 min

Lab File: VX046555.D

Acq: 07 Jun 2025 04:31

Instrument :

MSVOA_X

ClientSampleId :





WC-A2-07-G

Tgt Ion: 78 Resp: 425637

Ion Ratio Lower Upper

78 100

77 24.3 19.0 28.4

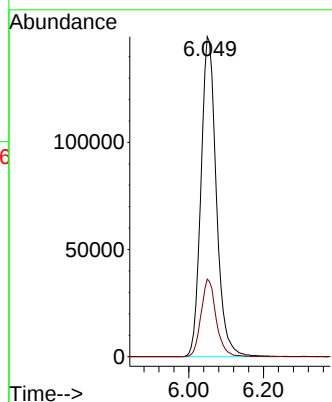

#42

1,2-Dichloroethane

Concen: 1.556 ug/l

RT: 6.049 min Scan# 814

Delta R.T. -0.049 min

Lab File: VX046555.D




Acq: 07 Jun 2025 04:31


Tgt Ion: 62 Resp: 4380

Ion Ratio Lower Upper

62 100

98 0.0 0.0 15.2

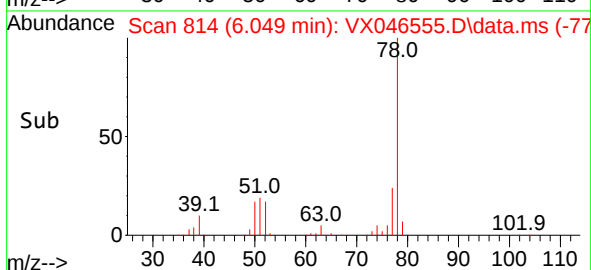



#48

Methyl methacrylate

Concen: 0.324 ug/l

RT: 7.628 min Scan# 1

Delta R.T. -0.074 min

Lab File: VX046555.D

Acq: 07 Jun 2025 04:31

Instrument :

MSVOA_X

ClientSampleId :

WC-A2-07-G





Tgt Ion: 41 Resp: 681

Ion Ratio Lower Upper

41 100

69 0.0 58.5 87.7#

39 14.0 51.7 77.5#

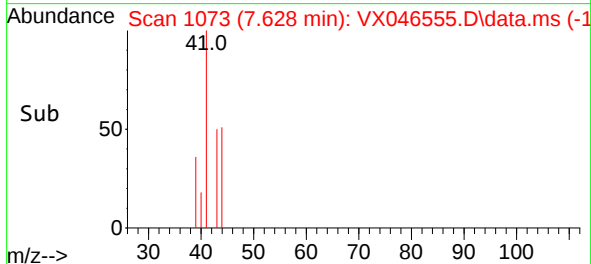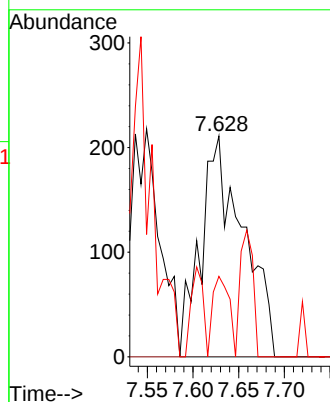

#50

Toluene-d8

Concen: 52.823 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX046555.D




Acq: 07 Jun 2025 04:31


Tgt Ion: 98 Resp: 293116

Ion Ratio Lower Upper

98 100

100 65.9 53.5 80.3







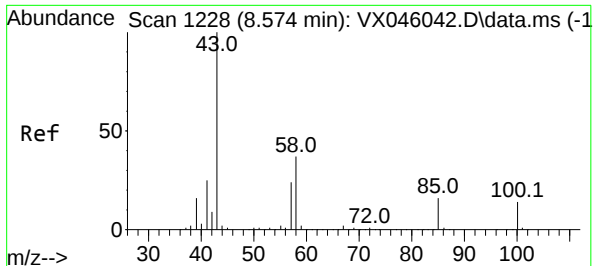

#51
4-Methyl-2-Pentanone
Concen: 0.669 ug/l
RT: 8.579 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion: 43 Resp: 1740
Ion Ratio Lower Upper
43 100
58 37.7 28.9 43.3

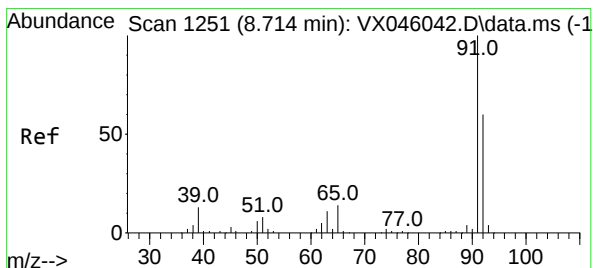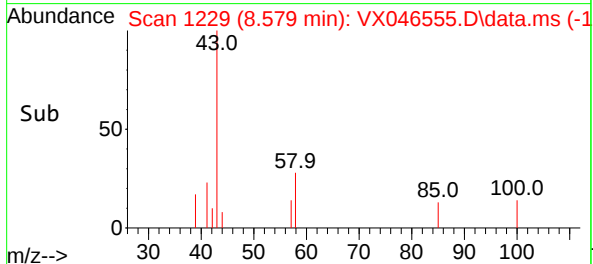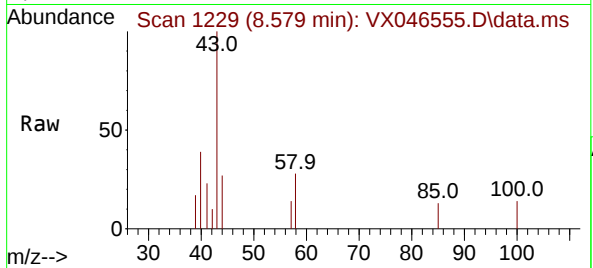

#52
Toluene
Concen: 42.654 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 92 Resp: 177358
Ion Ratio Lower Upper
92 100
91 169.0 136.6 205.0

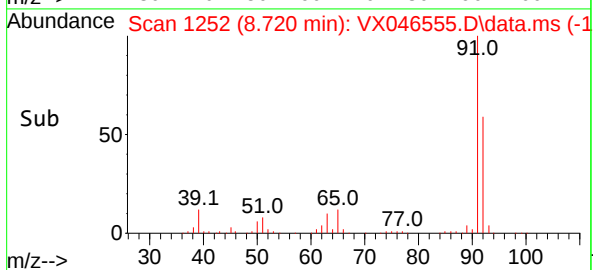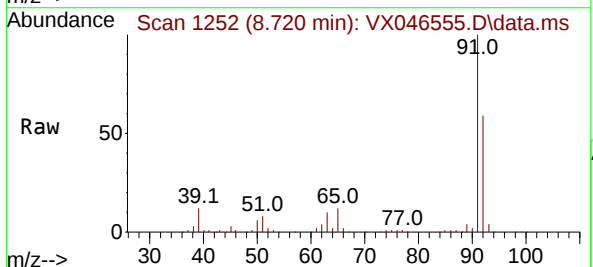



#53

t-1,3-Dichloropropene

Concen: 0.979 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX046555.D

Acq: 07 Jun 2025 04:31

Instrument :

MSVOA_X

ClientSampleId :





WC-A2-07-G

Tgt Ion: 75 Resp: 2373

Ion Ratio Lower Upper

75 100

77 176.0 25.0 37.6#

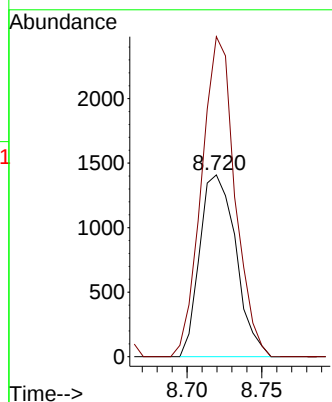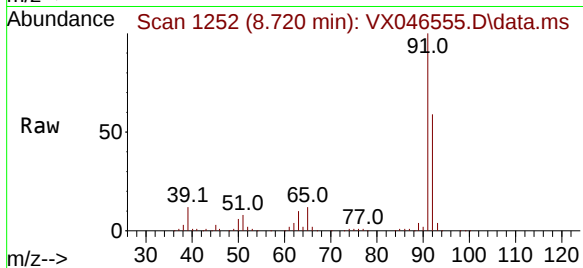

#55

1,1,2-Trichloroethane

Concen: 1.538 ug/l

RT: 9.018 min Scan# 1301

Delta R.T. -0.135 min

Lab File: VX046555.D

Acq: 07 Jun 2025 04:31

Tgt Ion: 97 Resp: 2568




Ion Ratio Lower Upper


97 100

83 0.0 69.0 103.6#

85 0.0 44.3 66.5#

99 7.8 47.8 71.6#


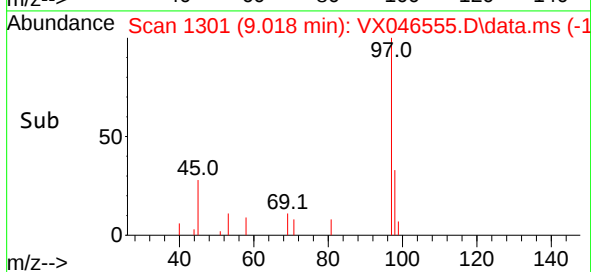

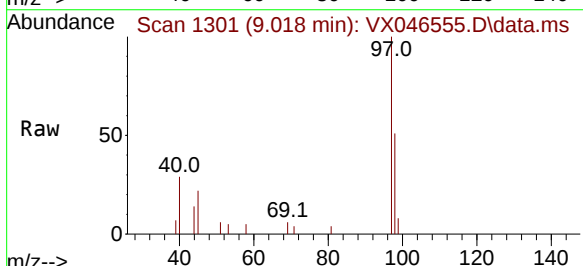




#59
2-Hexanone
Concen: 0.262 ug/l
RT: 9.457 min Scan# 11
Delta R.T. 0.024 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion: 43 Resp: 489
Ion Ratio Lower Upper
43 100
58 33.7 24.9 74.6

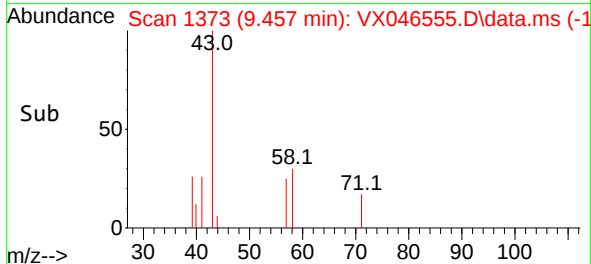

#62
4-Bromofluorobenzene
Concen: 58.126 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 95 Resp: 133450
Ion Ratio Lower Upper
95 100
174 67.5 0.0 135.8
176 65.9 0.0 131.4


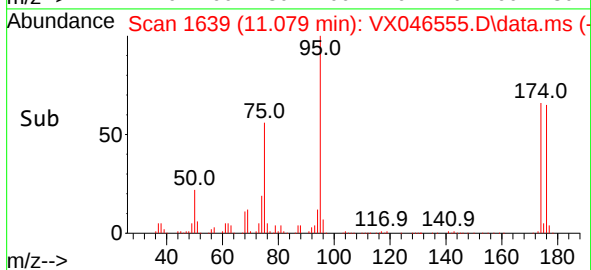






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion:117 Resp: 241518
Ion Ratio Lower Upper
117 100
82 61.0 50.6 76.0
119 33.4 25.8 38.6

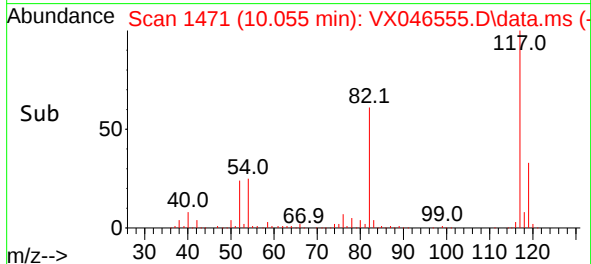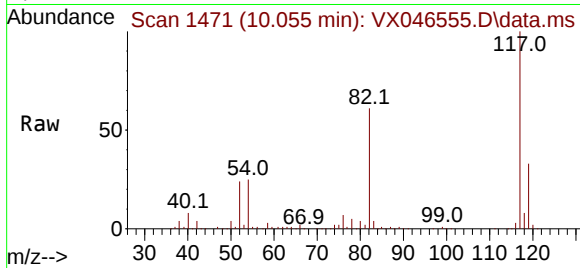

#67
Ethyl Benzene
Concen: 96.864 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 91 Resp: 960531
Ion Ratio Lower Upper
91 100
106 30.3 23.4 35.2



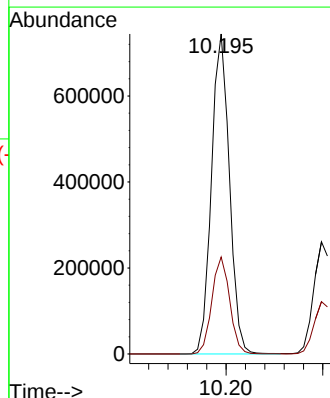
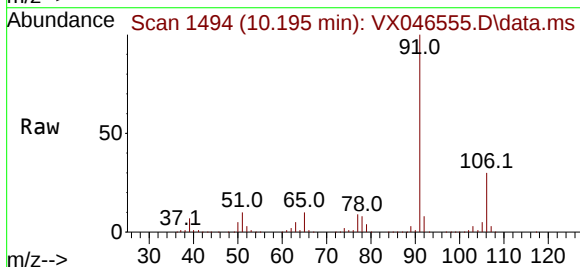




#68
m/p-Xylenes
Concen: 45.836 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion:106 Resp: 164878
Ion Ratio Lower Upper
106 100
91 213.6 171.2 256.8

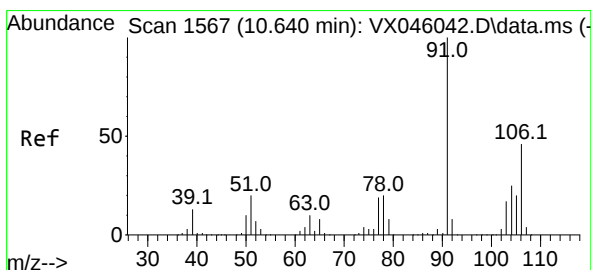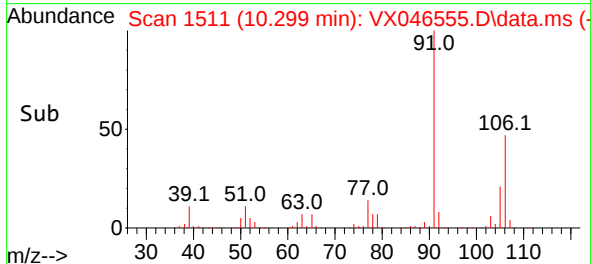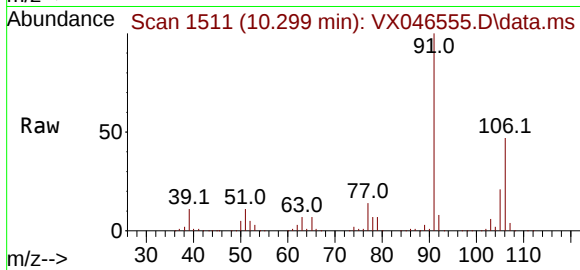

#69
o-Xylene
Concen: 33.020 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion:106 Resp: 114888
Ion Ratio Lower Upper
106 100
91 227.8 112.7 338.1

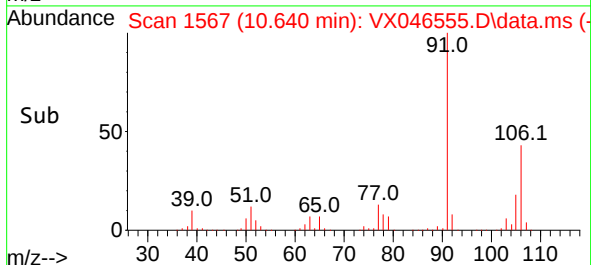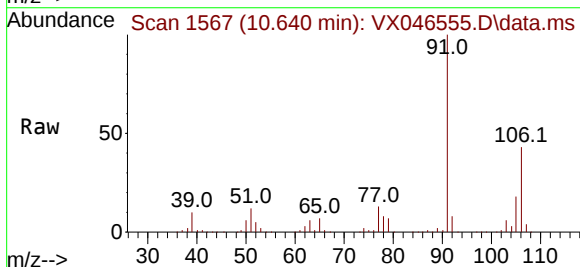



#70

Styrene

Concen: 3.741 ug/l

RT: 10.652 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX046555.D

Acq: 07 Jun 2025 04:31

Instrument :

MSVOA_X

ClientSampleId :

WC-A2-07-G





Tgt Ion:104 Resp: 22278

Ion Ratio Lower Upper

104 100

78 123.6 45.7 68.5#

103 106.0 43.7 65.5#

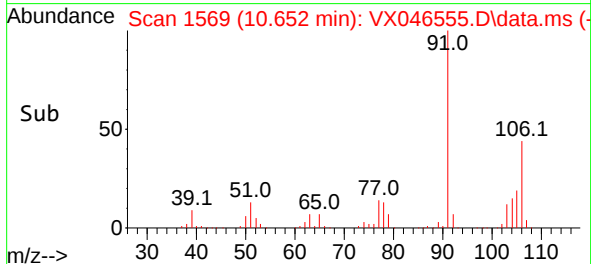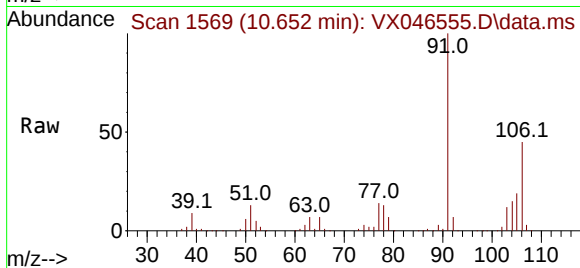

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX046555.D

Acq: 07 Jun 2025 04:31




Tgt Ion:152 Resp: 121477


Ion Ratio Lower Upper

152 100

115 65.2 46.9 140.7

150 157.9 0.0 351.0


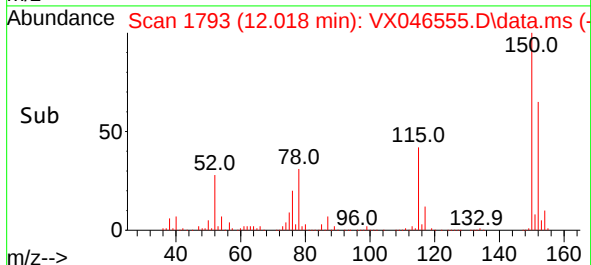






#73
Isopropylbenzene
Concen: 4.808 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion:105 Resp: 45915
Ion Ratio Lower Upper
105 100
120 25.4 12.8 38.4

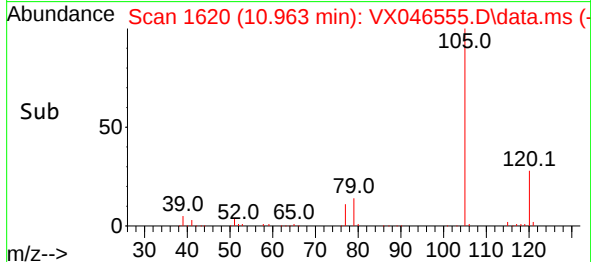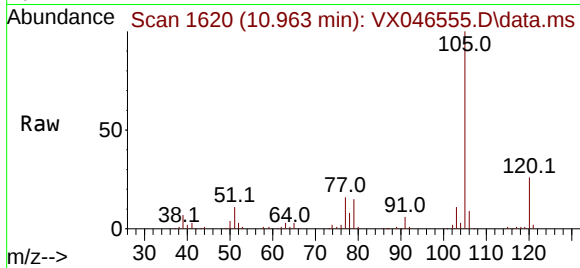

#76
1,2,3-Trichloropropane
Concen: 1.081 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.140 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 75 Resp: 2782
Ion Ratio Lower Upper
75 100
77 1244.9 20.5 61.5#




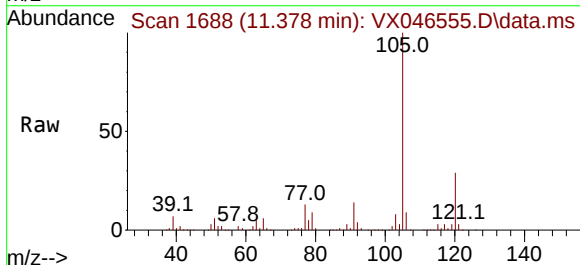




#78
n-propylbenzene
Concen: 0.954 ug/l
RT: 11.304 min Scan# 1676
Delta R.T. -0.001 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion: 91 Resp: 11028
Ion Ratio Lower Upper
91 100
120 0.0 10.8 32.4#

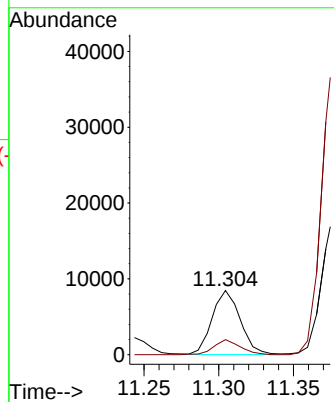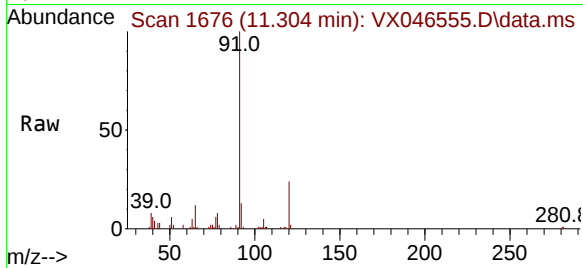

#79
2-Chlorotoluene
Concen: 5.091 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 91 Resp: 35485
Ion Ratio Lower Upper
91 100
126 1.0 15.6 46.7#



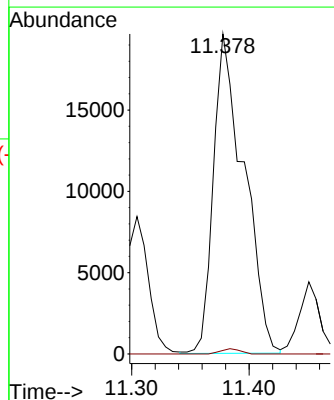
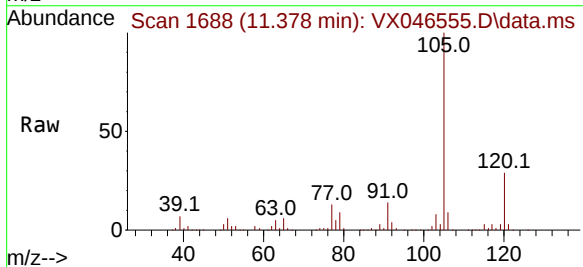




#80
1,3,5-Trimethylbenzene
Concen: 5.412 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion:105 Resp: 43065
Ion Ratio Lower Upper
105 100
120 47.1 23.1 69.2

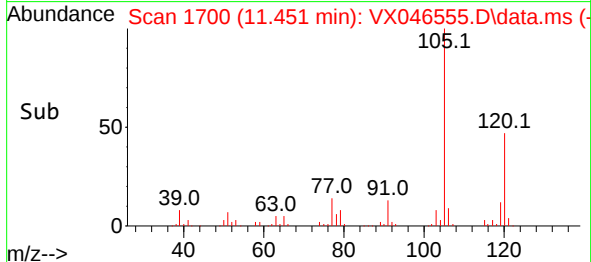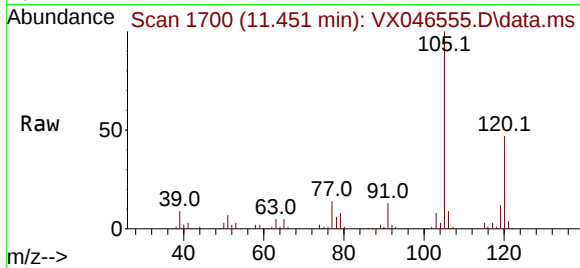

#81
trans-1,4-Dichloro-2-butene
Concen: 81.309 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 75 Resp: 72526
Ion Ratio Lower Upper
75 100
53 0.0 100.5 150.7#
89 0.0 37.0 55.6#




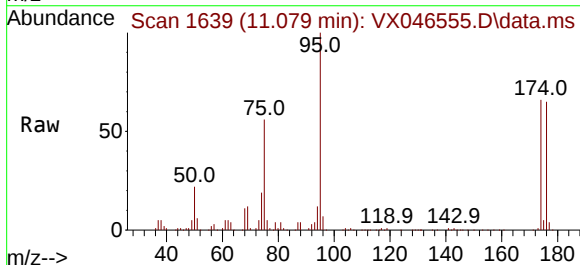




#82
4-Chlorotoluene
Concen: 0.632 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion: 91 Resp: 5224
Ion Ratio Lower Upper
91 100
126 0.0 13.3 39.8#

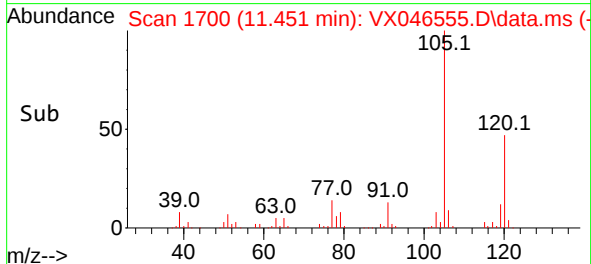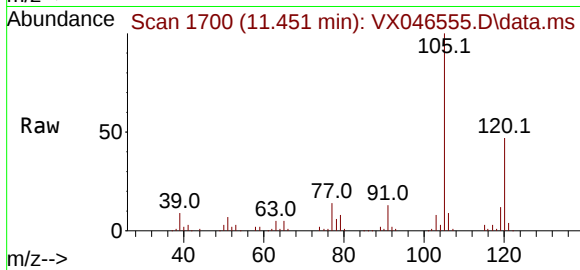

#83
tert-Butylbenzene
Concen: 2.145 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.037 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 119 Resp: 17378
Ion Ratio Lower Upper
119 100
91 116.2 32.9 98.7#
134 0.0 11.4 34.1#


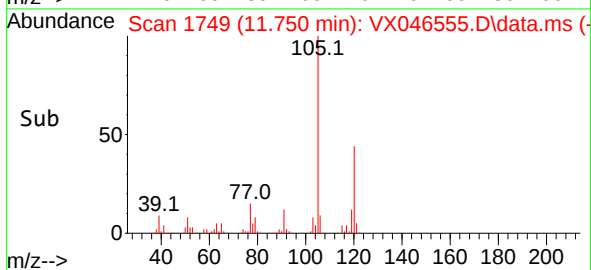

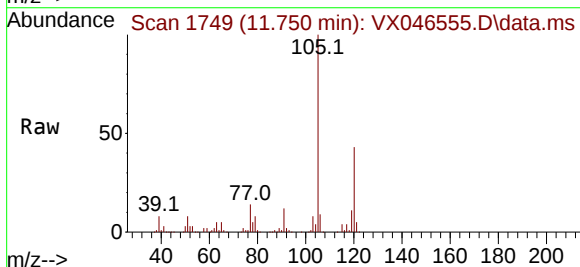




#84
1,2,4-Trimethylbenzene
Concen: 18.761 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion:105 Resp: 151023
Ion Ratio Lower Upper
105 100
120 43.4 21.2 63.6

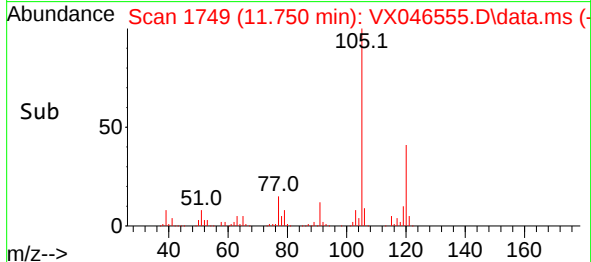

#85
sec-Butylbenzene
Concen: 14.509 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion:105 Resp: 151023
Ion Ratio Lower Upper
105 100
134 0.0 9.7 29.1#









#86
p-Isopropyltoluene
Concen: 0.713 ug/l
RT: 12.012 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion:119 Resp: 6183
Ion Ratio Lower Upper
119 100
134 28.1 12.5 37.5
91 0.0 13.8 41.4#

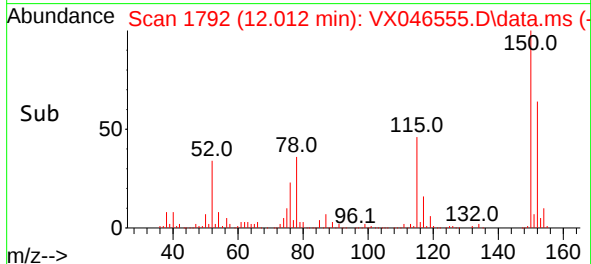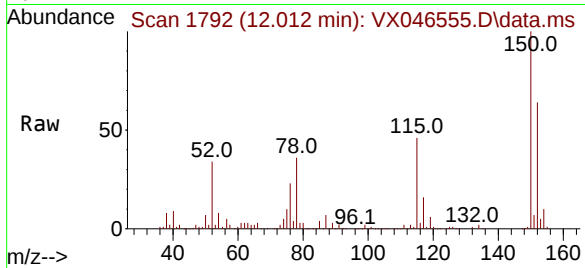

#89
n-Butylbenzene
Concen: 27.829 ug/l
RT: 12.243 min Scan# 1830
Delta R.T. -0.086 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Tgt Ion: 91 Resp: 237138
Ion Ratio Lower Upper
91 100
92 9.9 26.9 80.7#
134 2.5 11.8 35.3#


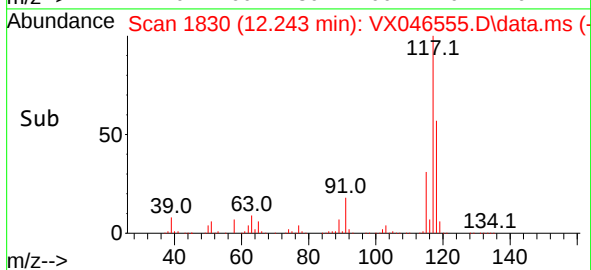

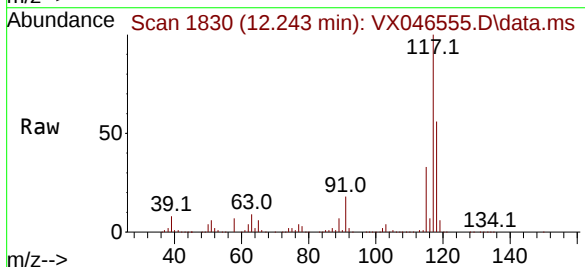




#90
Hexachloroethane
Concen: 39.410 ug/l
RT: 12.408 min Scan# 117
Delta R.T. -0.128 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31




Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G


Tgt Ion:117 Resp: 60780
Ion Ratio Lower Upper
117 100
201 0.0 31.6 94.7#

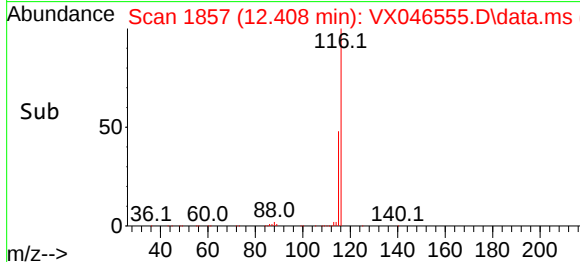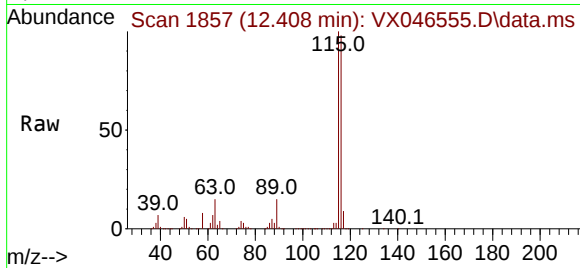

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.939 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.024 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31


Tgt Ion: 75 Resp: 643
Ion Ratio Lower Upper
75 100
155 0.0 34.9 104.8#
157 0.0 43.8 131.4#

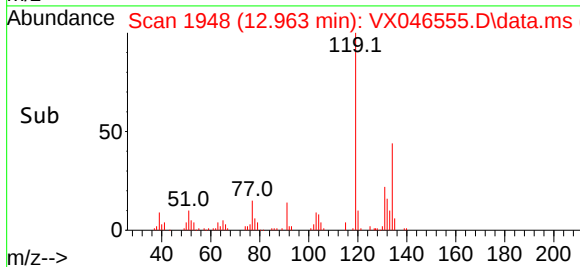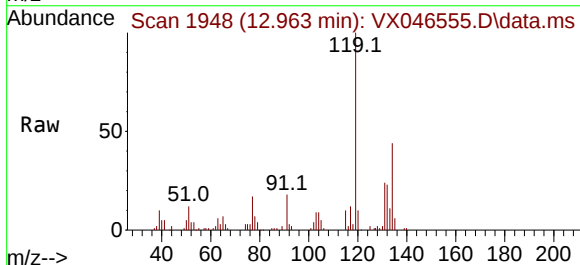



#95
Naphthalene
Concen: 1102.595 ug/l
RT: 13.786 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX046555.D
Acq: 07 Jun 2025 04:31

Instrument :
MSVOA_X
ClientSampleId :
WC-A2-07-G

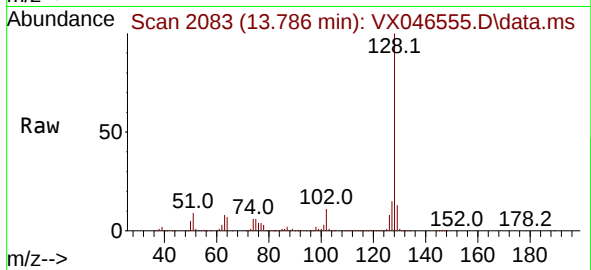

Tgt Ion:128 Resp: 9909635
Ion Ratio Lower Upper
128 100
127 14.0 10.4 15.6
129 12.5 8.6 13.0

