

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060719\
 Data File : VX010130.D
 Acq On : 07 Jun 2019 23:41
 Operator : JC/SP
 Sample : K3221-04 10X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPS1-TT-MW309D-20190605

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	34	rVB	84148	109867	8.61%	1.562%
2	1.635	66	79	81	rBV	12638	41920	3.28%	0.596%
3	3.013	299	305	316	rVB	18800	47025	3.68%	0.668%
4	4.714	575	584	595	rBV2	4268	15957	1.25%	0.227%
5	5.494	701	712	725	rBV	154859	443743	34.76%	6.308%
6	5.659	728	739	757	rVB	267536	748641	58.64%	10.642%
7	6.061	794	805	821	rBV	146703	383136	30.01%	5.446%
8	6.854	926	935	948	rBV	386481	917888	71.90%	13.048%
9	8.713	1233	1240	1254	rBV	827155	1276582	100.00%	18.146%
10	10.109	1463	1469	1479	rBV	800023	1095171	85.79%	15.568%
11	11.134	1628	1637	1649	rBV	695995	896610	70.24%	12.745%
12	12.079	1785	1792	1804	rBV	811860	1058424	82.91%	15.045%


Sum of corrected areas: 7034964

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060719\
Data File : VX010130.D
Acq On : 07 Jun 2019 23:41
Operator : JC/SP
Sample : K3221-04 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW309D-20190605

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

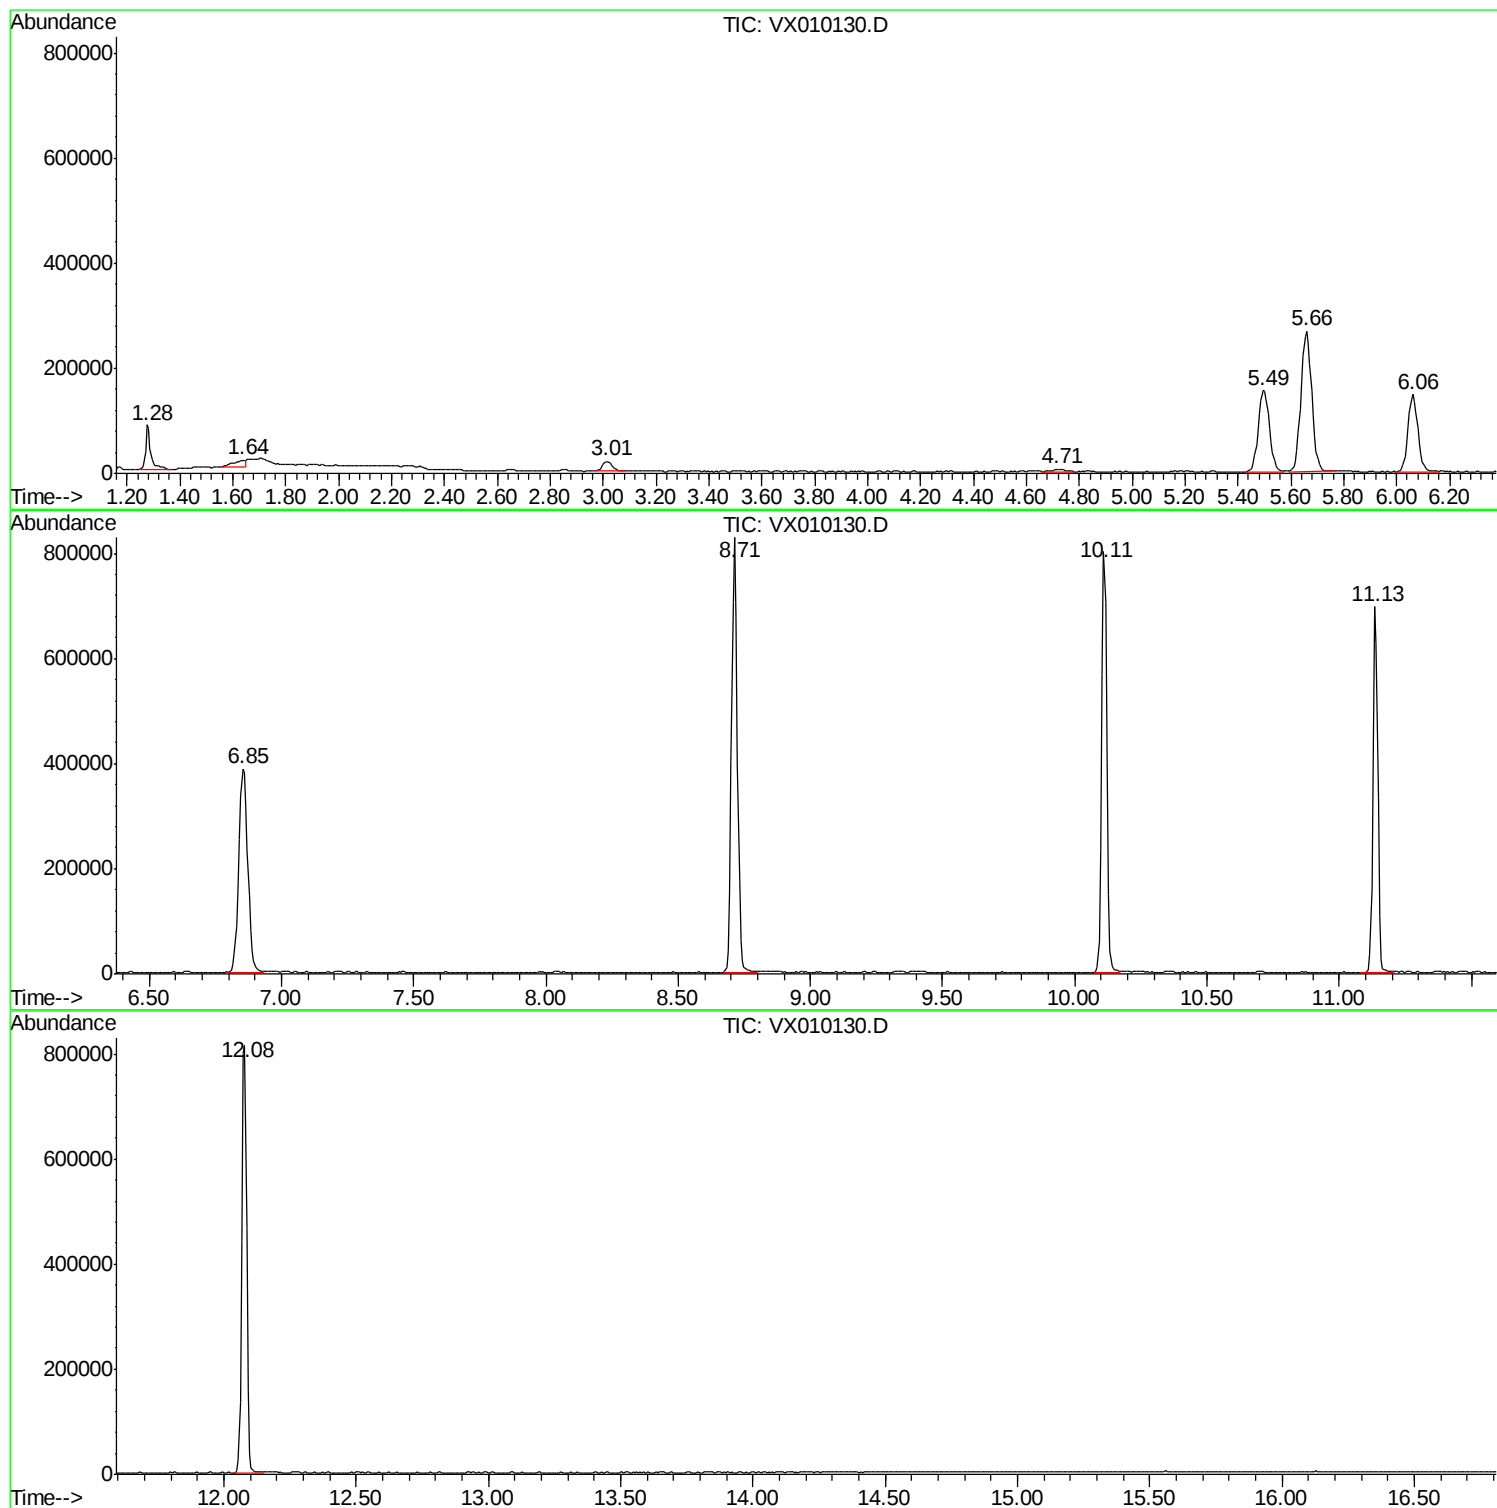

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX060719\
Data File : VX010130.D
Acq On : 07 Jun 2019 23:41
Operator : JC/SP
Sample : K3221-04 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW309D-20190605

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX060719\
Data File : VX010130.D
Acq On : 07 Jun 2019 23:41
Operator : JC/SP
Sample : K3221-04 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW309D-20190605

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc