


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060719\
 Data File : VX010100.D
 Acq On : 07 Jun 2019 10:59
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
 Title : SW846 8260
 Last Update : Sat Jun 08 02:12:13 2019

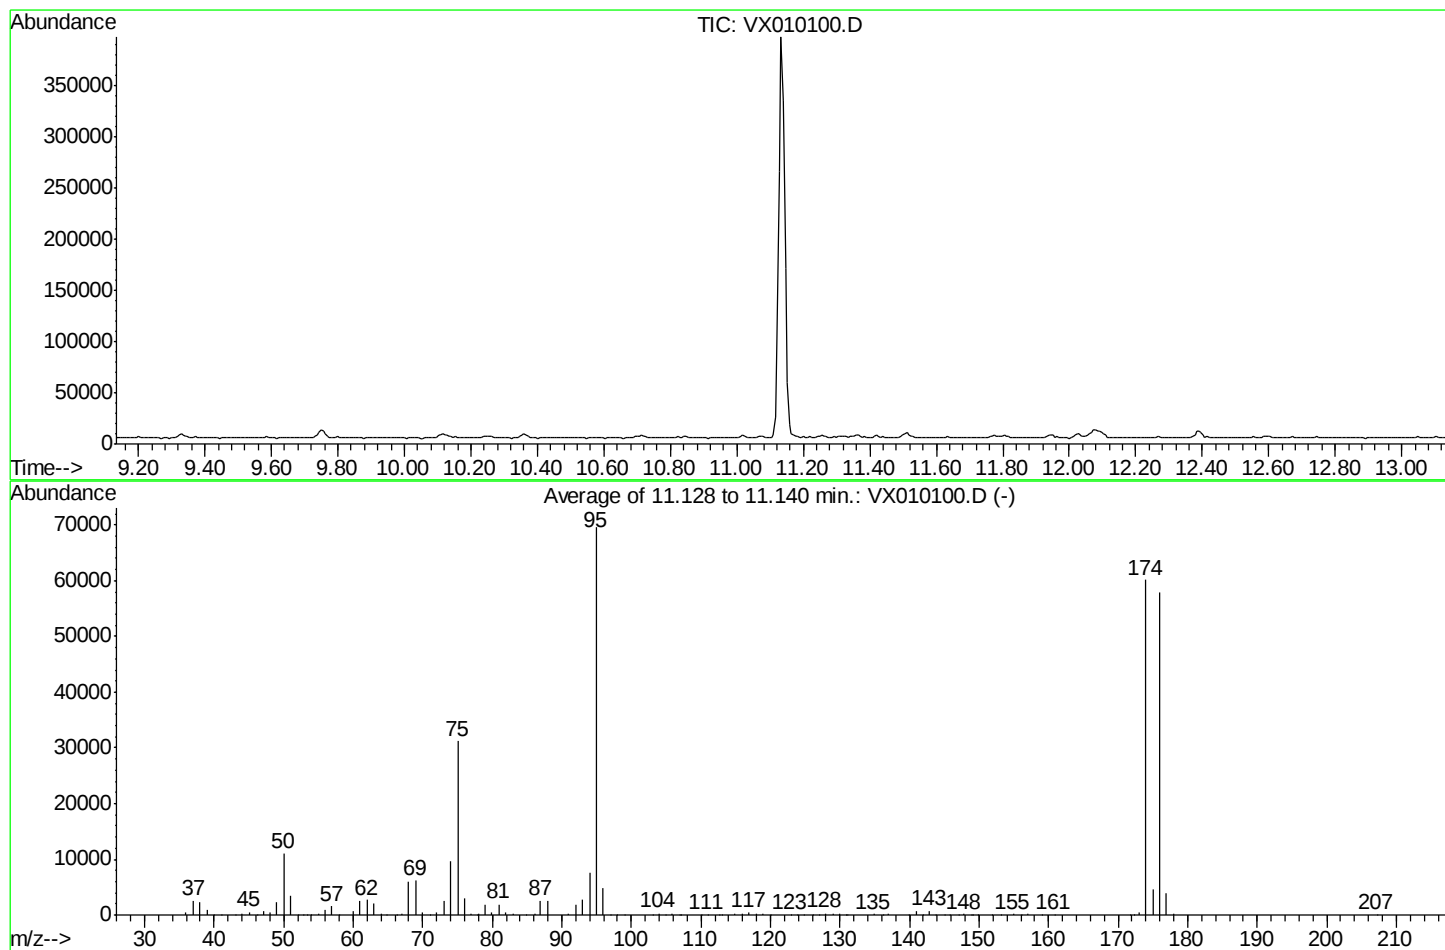

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	10940	PASS
75	95	30	60	44.8	31202	PASS
95	95	100	100	100.0	69587	PASS
96	95	5	9	6.8	4728	PASS
173	174	0.00	2	0.9	542	PASS
174	95	50	100	86.5	60170	PASS
175	174	5	9	7.7	4620	PASS
176	174	95	101	96.2	57880	PASS
177	176	5	9	6.6	3849	PASS