


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060719\
Data File : VX010108.D
Acq On : 07 Jun 2019 14:24
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Title : SW846 8260
Last Update : Sat Jun 08 02:12:13 2019

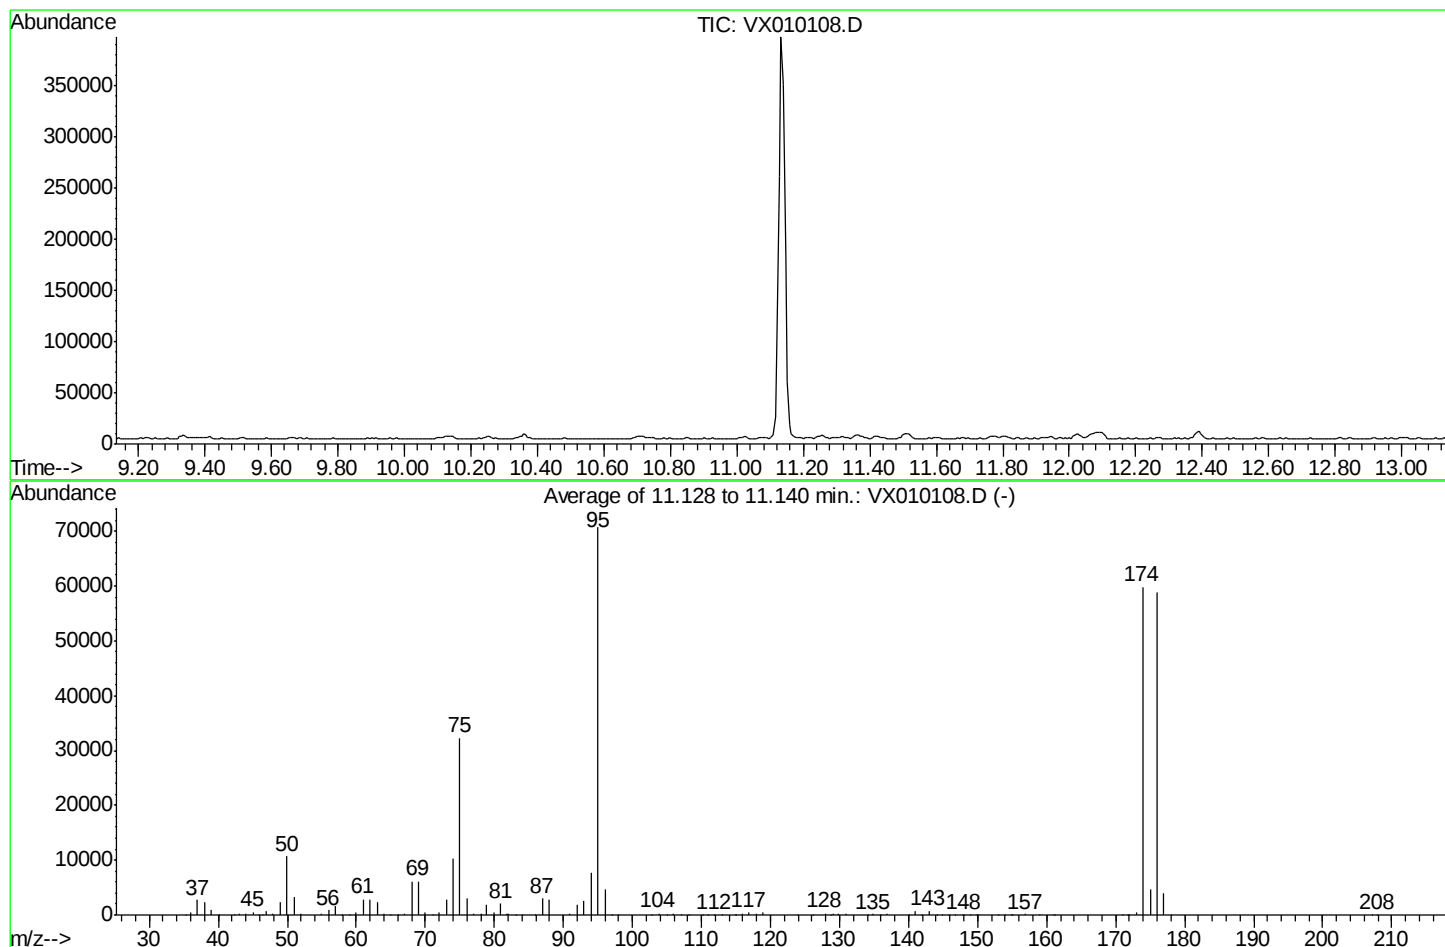

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	10731	PASS
75	95	30	60	45.6	32217	PASS
95	95	100	100	100.0	70699	PASS
96	95	5	9	6.6	4664	PASS
173	174	0.00	2	0.9	509	PASS
174	95	50	100	84.5	59765	PASS
175	174	5	9	7.7	4629	PASS
176	174	95	101	98.4	58786	PASS
177	176	5	9	6.7	3934	PASS