

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060721\
 Data File : VX022537.D
 Acq On : 07 Jun 2021 16:33
 Operator : JC/MD
 Sample : M2583-04DL 50X
 Misc : 4.99g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 40955DL


Quant Time: Jun 07 17:24:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 07 14:27:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	60359	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.775	114	122604	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	105747	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	39132	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	49667	46.287	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	92.580%		
35) Dibromofluoromethane	5.397	113	36535	47.628	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.260%		
50) Toluene-d8	8.653	98	149872	48.966	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	97.940%		
62) 4-Bromofluorobenzene	11.085	95	50350	44.257	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	88.520%		
Target Compounds			Qvalue			
5) Bromomethane	1.605	94	287	0.658	ug/l #	80
10) Methyl Iodide	2.465	142	186	0.213	ug/l #	72
11) Tert butyl alcohol	2.977	59	118	0.490	ug/l #	73
13) Acrolein	2.087	56	29	3.369	ug/l #	1
14) Allyl chloride	2.386	41	2517	1.793	ug/l #	1
16) Acetone	2.386	43	134807	279.590	ug/l	93
17) Carbon Disulfide	2.520	76	262	3.511	ug/l #	75
20) Methylene Chloride	2.800	84	290	0.288	ug/l #	63
31) Cyclohexane	5.513	56	608	0.479	ug/l #	32
36) 1,1-Dichloropropene	5.568	75	5965	5.029	ug/l #	49
38) Carbon Tetrachloride	5.562	117	6983	8.157	ug/l #	12
39) Methylcyclohexane	7.397	83	1136	2.667	ug/l #	86
51) 4-Methyl-2-Pentanone	8.580	43	501	0.326	ug/l #	58
52) Toluene	8.726	92	70944	30.861	ug/l	99
53) t-1,3-Dichloropropene	8.726	75	790	3.747	ug/l #	1
56) Ethyl methacrylate	9.031	69	38	2.723	ug/l #	1
67) Ethyl Benzene	10.195	91	5030	1.244	ug/l	100
68) m/p-Xylenes	10.305	106	7714	5.249	ug/l	91
69) o-Xylene	10.646	106	4205	2.926	ug/l	99
73) Isopropylbenzene	10.963	105	1456	0.457	ug/l	92
76) 1,2,3-Trichloropropane	11.085	75	27316	26.945	ug/l #	39
78) n-propylbenzene	11.305	91	7503	1.938	ug/l	98
79) 2-Chlorotoluene	11.384	91	4065	1.765	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.457	105	10939	4.014	ug/l	92
81) trans-1,4-Dichloro-2-b...	11.085	75	27316	66.227	ug/l #	12
82) 4-Chlorotoluene	11.457	91	1559	0.585	ug/l #	45
83) tert-Butylbenzene	11.975	119	2563	1.056	ug/l	90
84) 1,2,4-Trimethylbenzene	11.756	105	46422	16.938	ug/l	97
85) sec-Butylbenzene	11.890	105	2246	0.695	ug/l	79
86) p-Isopropyltoluene	12.012	119	7468	2.797	ug/l	95
89) n-Butylbenzene	12.329	91	5237	2.043	ug/l #	44
90) Hexachloroethane	12.530	117	637	4.667	ug/l #	9
95) Naphthalene	13.780	128	3239	1.061	ug/l #	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed





Instrument :
MSVOA_X
ClientSampleId :
40955DL



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampleId :
40955DL


Tgt Ion:168 Resp: 60359
Ion Ratio Lower Upper
168 100
99 76.9 45.8 68.6#

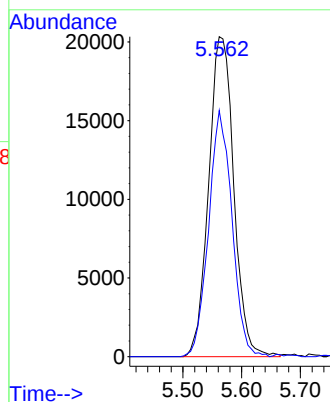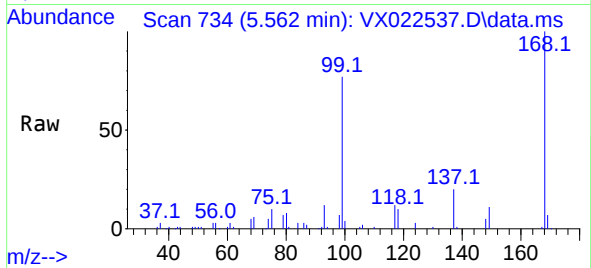

#5
Bromomethane
Concen: 0.658 ug/l
RT: 1.605 min Scan# 85
Delta R.T. 0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 94 Resp: 287
Ion Ratio Lower Upper
94 100
96 76.3 76.4 114.6#


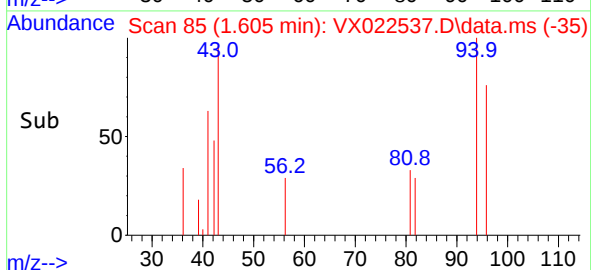






#10
Methyl Iodide
Concen: 0.213 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampleID :
40955DL


Tgt Ion:142 Resp: 186
Ion Ratio Lower Upper
142 100
127 25.8 33.3 49.9#
141 0.0 11.4 17.0#

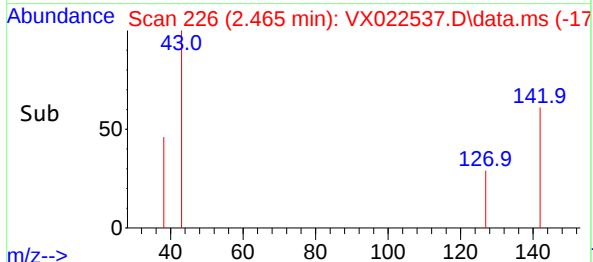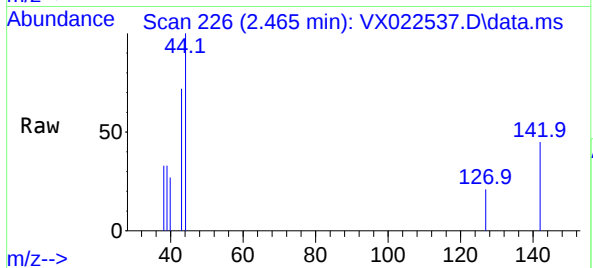

#11
Tert butyl alcohol
Concen: 0.490 ug/l
RT: 2.977 min Scan# 310
Delta R.T. -0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 59 Resp: 118
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


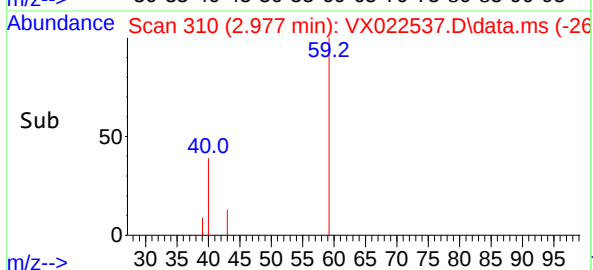






#13
Acrolein
Concen: 3.369 ug/l
RT: 2.087 min Scan# 164
Delta R.T. -0.152 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampleID :
40955DL


Tgt Ion: 56 Resp: 29
Ion Ratio Lower Upper
56 100
55 237.9 56.4 84.6#



#14
Allyl chloride
Concen: 1.793 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.280 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 41 Resp: 2517
Ion Ratio Lower Upper
41 100
39 162.1 51.6 77.4#
76 0.0 30.5 45.7#


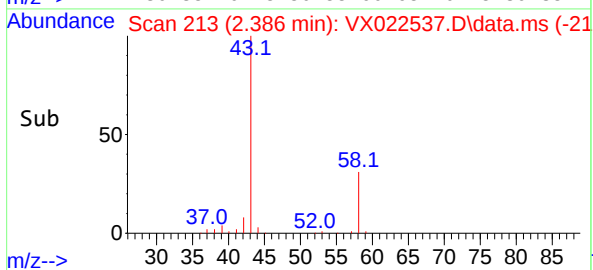






#16
Acetone
Concen: 279.590 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampled :
40955DL


Tgt Ion: 43 Resp: 134807
Ion Ratio Lower Upper
43 100
58 30.7 27.8 41.8

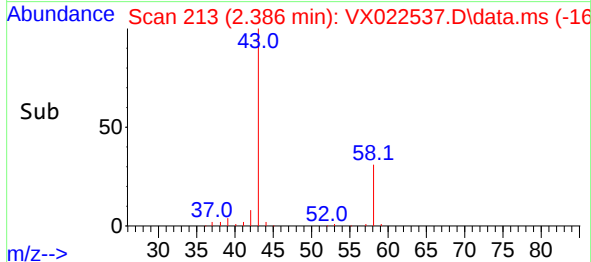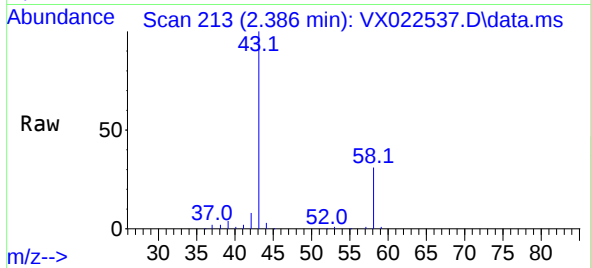

#17
Carbon Disulfide
Concen: 3.511 ug/l
RT: 2.520 min Scan# 235
Delta R.T. 0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 76 Resp: 262
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

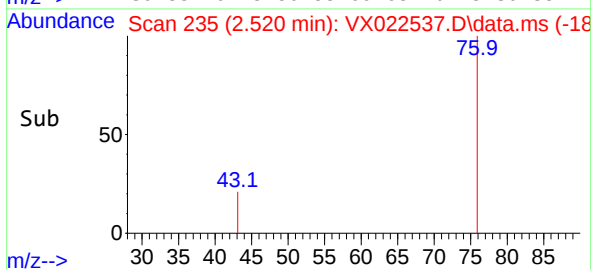







#20
Methylene Chloride
Concen: 0.288 ug/l
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Instrument :
MSVOA_X
ClientSampled :
40955DL

Tgt Ion: 84 Resp: 290




Ion	Ratio	Lower	Upper
84	100		
49	53.1	88.6	132.8#
51	33.7	27.0	40.6
86	41.8	50.3	75.5#

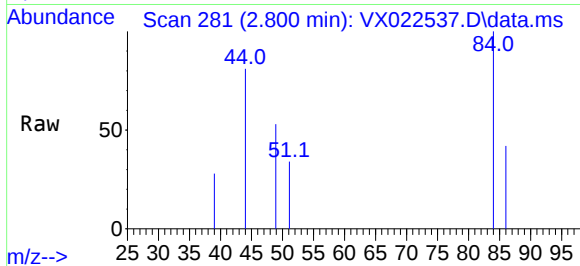


#31
Cyclohexane
Concen: 0.479 ug/l
RT: 5.513 min Scan# 726
Delta R.T. 0.036 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 56 Resp: 608

Ion	Ratio	Lower	Upper
56	100		
69	0.0	25.3	37.9#
84	21.2	71.4	107.0#

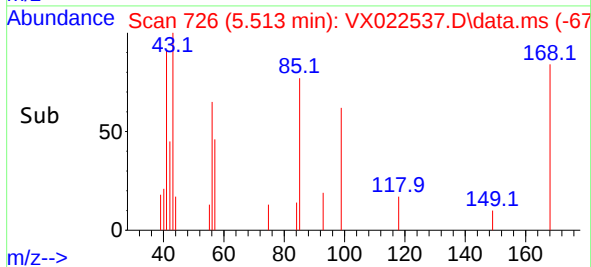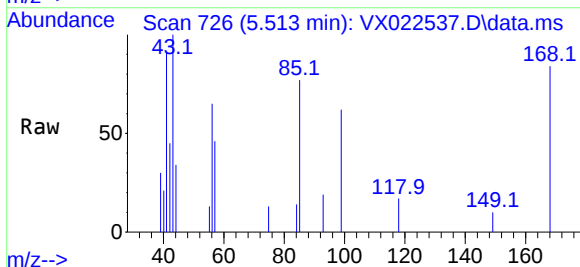







#33

1,2-Dichloroethane-d4
Concen: 46.287 ug/l
RT: 5.970 min Scan# 801
Delta R.T. 0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Instrument :
MSVOA_X
ClientSampled :
40955DL




Tgt Ion: 65 Resp: 49667
Ion Ratio Lower Upper
65 100
67 52.4 0.0 105.4




#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.775 min Scan# 933
Delta R.T. 0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 114 Resp: 122604
Ion Ratio Lower Upper
114 100
63 21.2 0.0 40.8
88 15.1 0.0 32.8


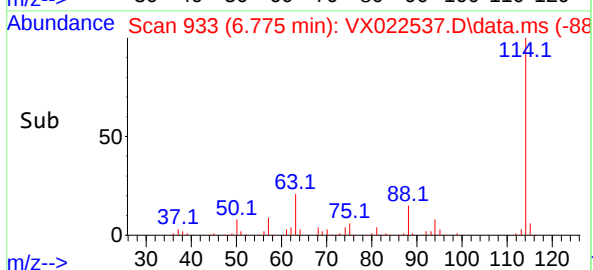




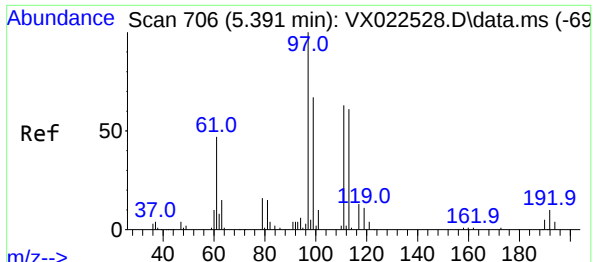

#35
Dibromofluoromethane
Concen: 47.628 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampled :
40955DL


Tgt Ion:113 Resp: 36535
Ion Ratio Lower Upper
113 100
111 103.6 81.9 122.9
192 14.3 16.7 25.1#

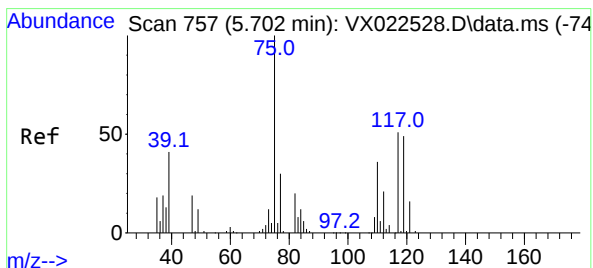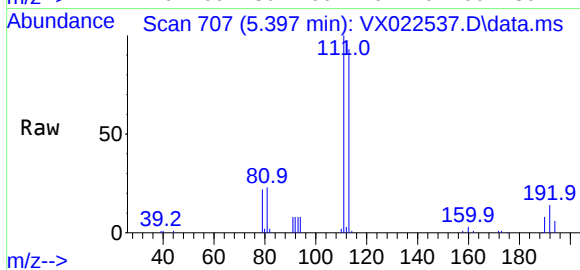

#36
1,1-Dichloropropene
Concen: 5.029 ug/l
RT: 5.568 min Scan# 735
Delta R.T. -0.134 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 75 Resp: 5965
Ion Ratio Lower Upper
75 100
110 9.3 18.1 54.4#
77 0.0 25.3 37.9#


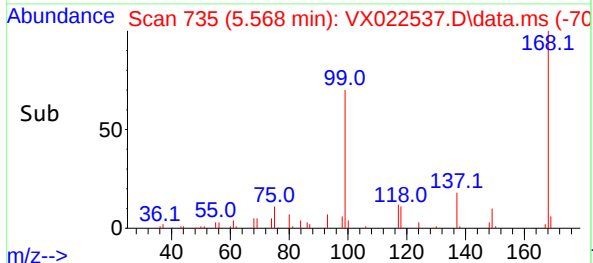
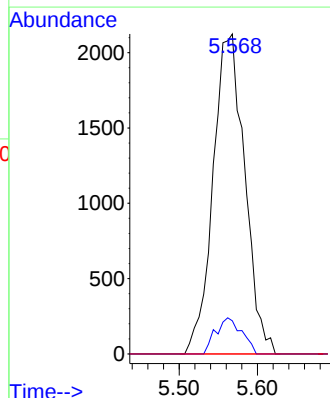
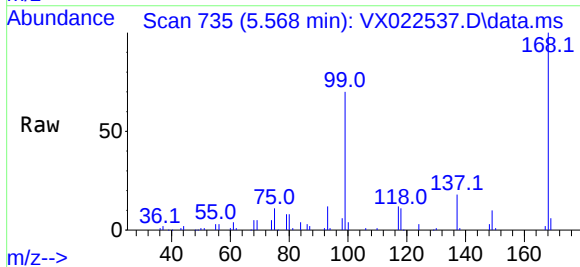


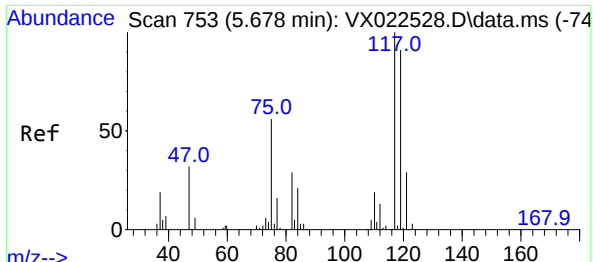

#38
Carbon Tetrachloride
Concen: 8.157 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.116 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampleID :
40955DL


Tgt Ion:117 Resp: 6983
Ion Ratio Lower Upper
117 100
119 0.0 76.2 114.2#
121 0.0 24.8 37.2#

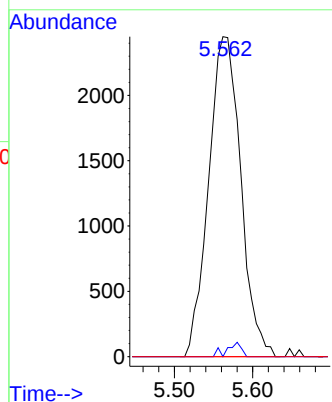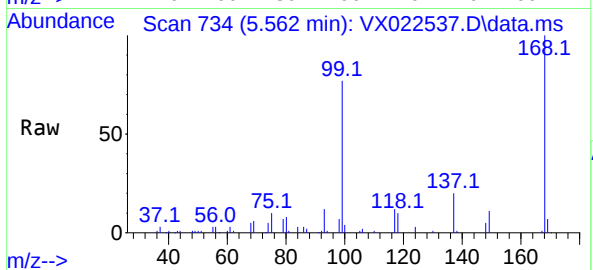

#39
Methylcyclohexane
Concen: 2.667 ug/l
RT: 7.397 min Scan# 1035
Delta R.T. 0.012 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 83 Resp: 1136
Ion Ratio Lower Upper
83 100
55 57.7 58.9 88.3#
98 43.8 38.1 57.1


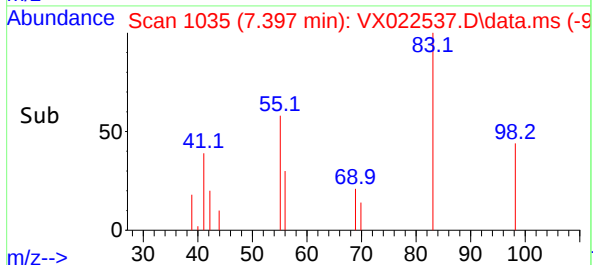

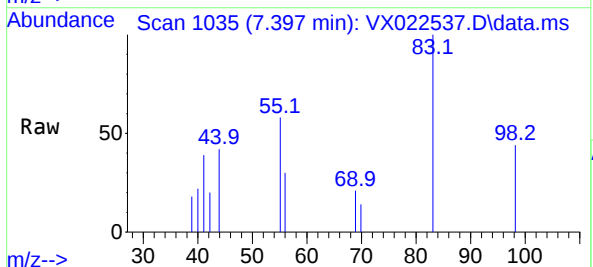




#50
Toluene-d8
Concen: 48.966 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampleID :
40955DL


Tgt Ion: 98 Resp: 149872
Ion Ratio Lower Upper
98 100
100 65.3 51.9 77.9

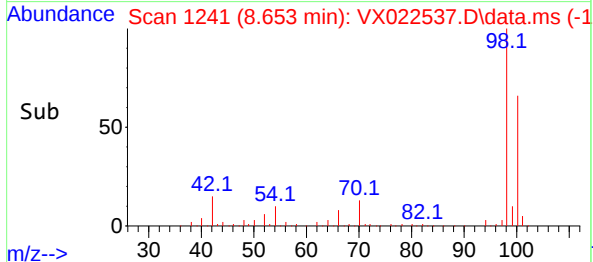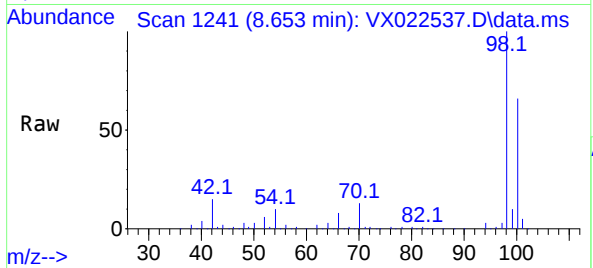

#51
4-Methyl-2-Pentanone
Concen: 0.326 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. -0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 43 Resp: 501
Ion Ratio Lower Upper
43 100
58 17.2 35.4 53.0#

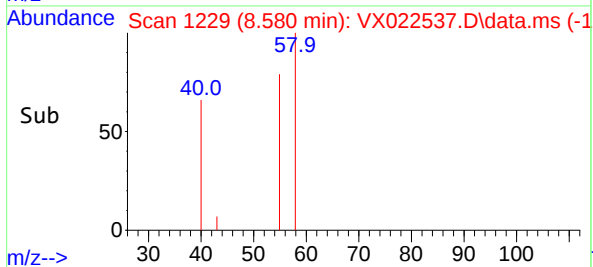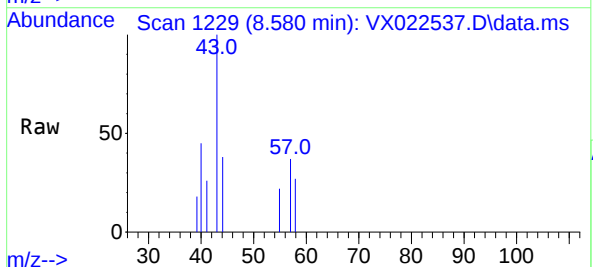



#52

Toluene

Concen: 30.861 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. 0.006 min

Lab File: VX022537.D


Acq: 07 Jun 2021 16:33

Tgt Ion: 92 Resp: 70944




Ion Ratio Lower Upper

92 100

91 170.4 137.1 205.7

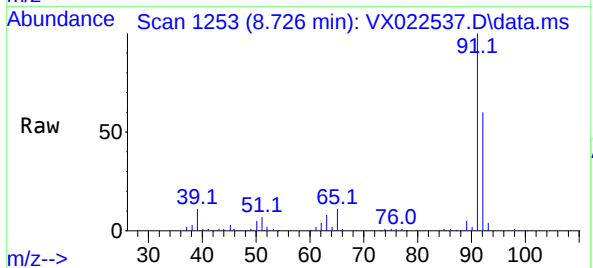

Abundance

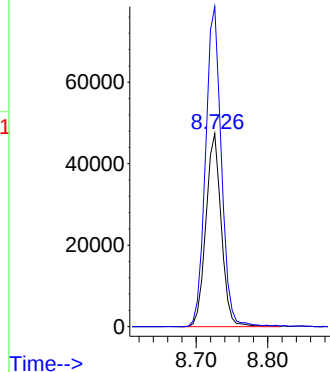

#53

t-1,3-Dichloropropene

Concen: 3.747 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. -0.256 min

Lab File: VX022537.D


Acq: 07 Jun 2021 16:33

Tgt Ion: 75 Resp: 790



Ion Ratio Lower Upper


75 100

77 153.6 24.9 37.3#

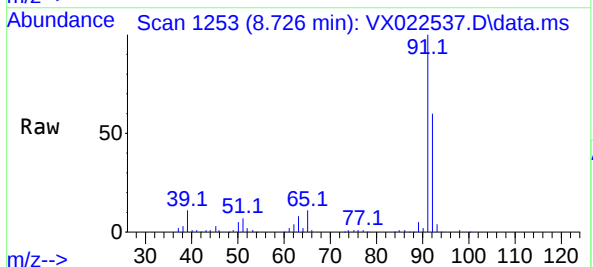

Abundance



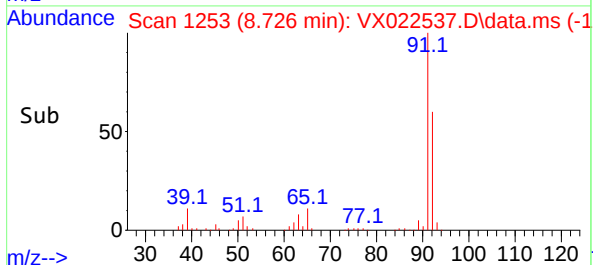
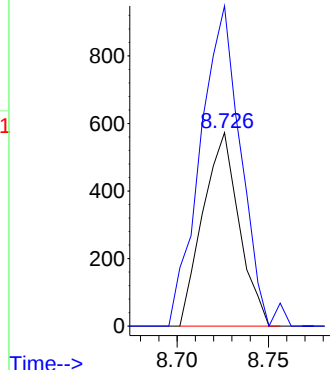




#56
Ethyl methacrylate
Concen: 2.723 ug/l
RT: 9.031 min Scan# 1303
Delta R.T. -0.091 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampled :
40955DL


Tgt Ion: 69 Resp: 38
Ion Ratio Lower Upper
69 100
41 76.3 46.8 70.2#
39 544.7 24.7 37.1#

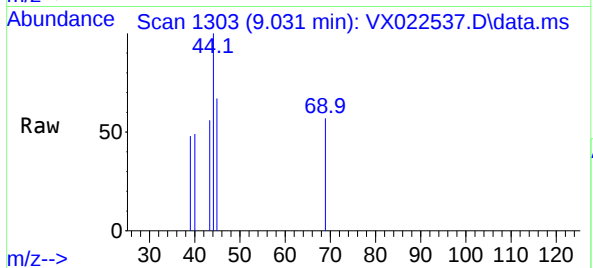

#62
4-Bromofluorobenzene
Concen: 44.257 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 95 Resp: 50350
Ion Ratio Lower Upper
95 100
174 62.8 0.0 154.6
176 60.3 0.0 155.8


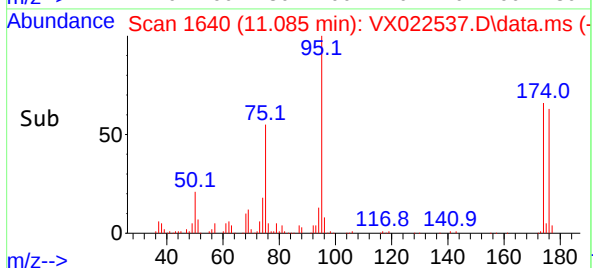
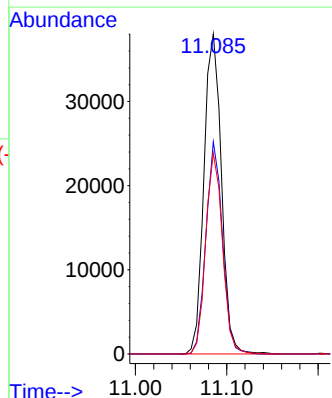





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampled :
40955DL


Tgt Ion:117 Resp: 105747
Ion Ratio Lower Upper
117 100
82 59.4 47.4 71.2
119 35.0 26.6 39.8

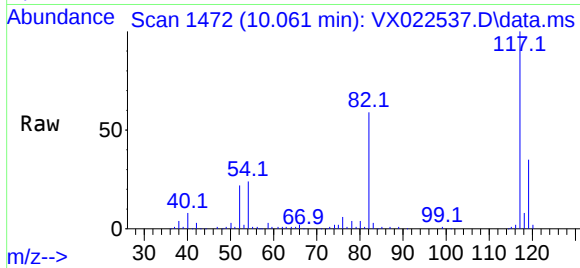

#67
Ethyl Benzene
Concen: 1.244 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 91 Resp: 5030
Ion Ratio Lower Upper
91 100
106 31.0 24.6 37.0


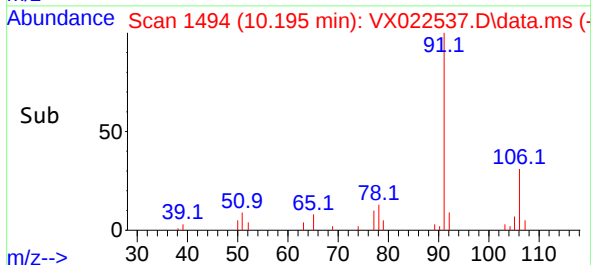
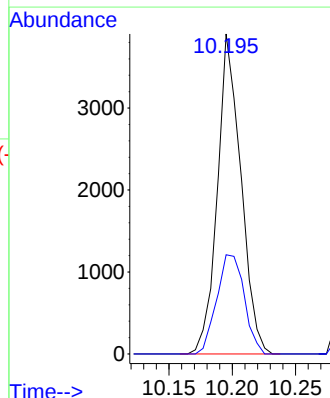
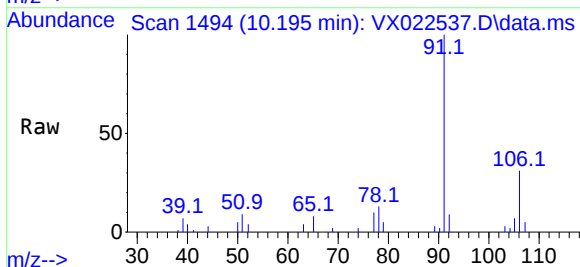




#68
m/p-Xylenes
Concen: 5.249 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampleID :
40955DL


Tgt Ion:106 Resp: 7714
Ion Ratio Lower Upper
106 100
91 217.7 162.8 244.2

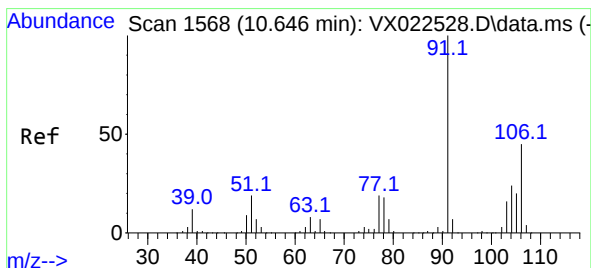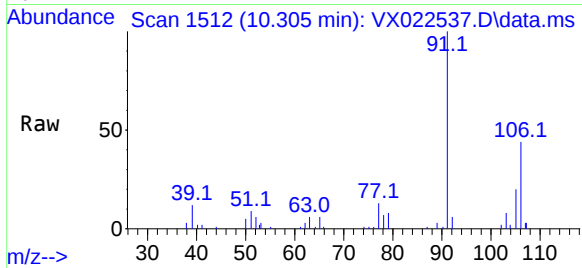

#69
o-Xylene
Concen: 2.926 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion:106 Resp: 4205
Ion Ratio Lower Upper
106 100
91 214.4 108.1 324.2


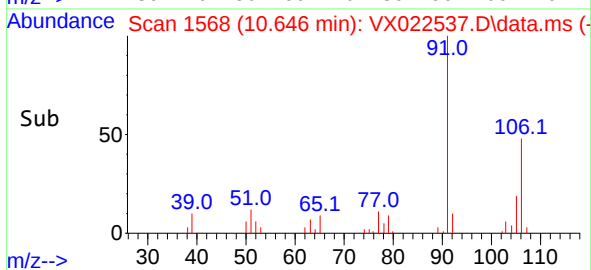

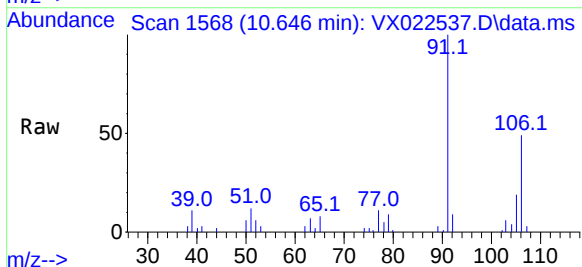




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampleID :
40955DL


Tgt Ion:152 Resp: 39132
Ion Ratio Lower Upper
152 100
115 69.8 41.1 123.3
150 158.7 0.0 349.0

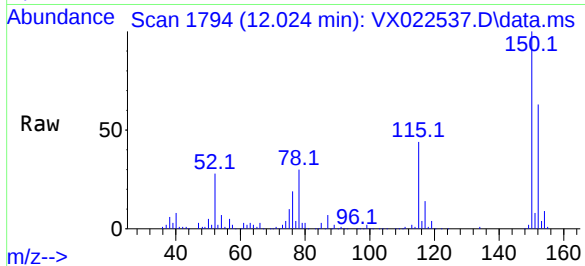

#73
Isopropylbenzene
Concen: 0.457 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion:105 Resp: 1456
Ion Ratio Lower Upper
105 100
120 22.5 13.2 39.6


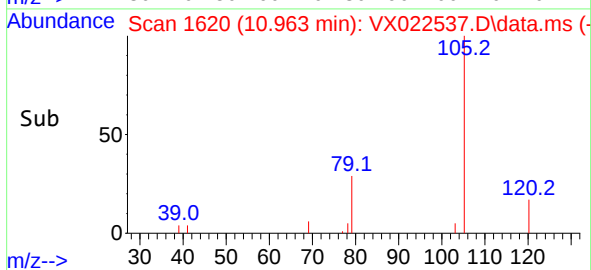

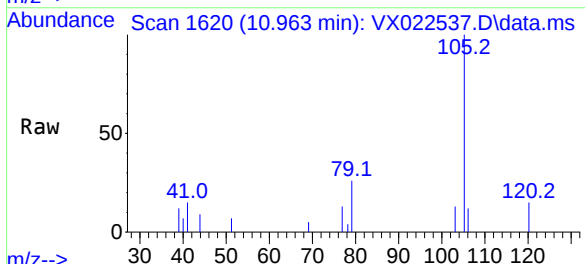




#76
1,2,3-Trichloropropane
Concen: 26.945 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampled :
40955DL


Tgt Ion: 75 Resp: 27316
Ion Ratio Lower Upper
75 100
77 1.4 19.1 57.5#

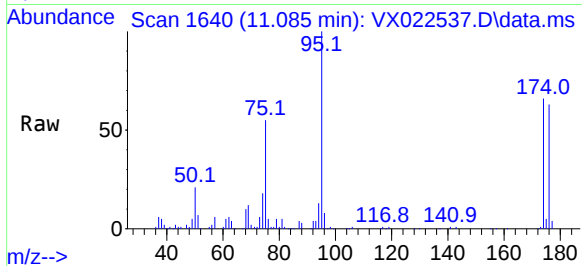

#78
n-propylbenzene
Concen: 1.938 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 91 Resp: 7503
Ion Ratio Lower Upper
91 100
120 22.0 11.5 34.5


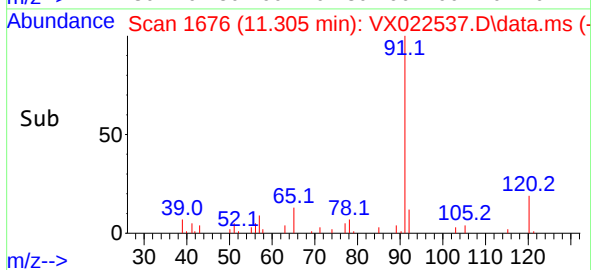

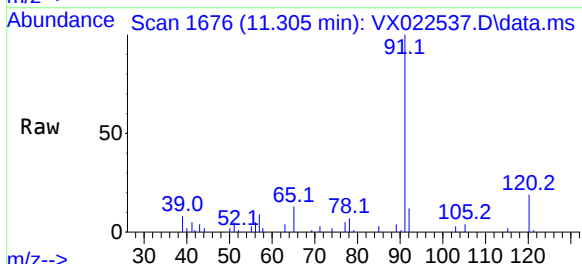




#79
2-Chlorotoluene
Concen: 1.765 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.018 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampled :
40955DL


Tgt Ion: 91 Resp: 4065
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#

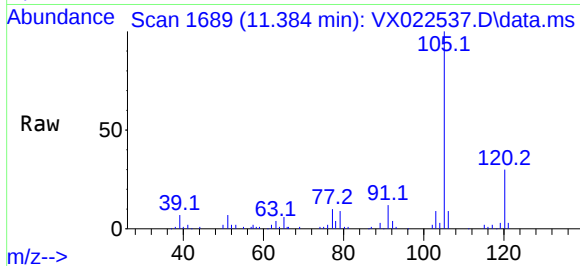

#80
1,3,5-Trimethylbenzene
Concen: 4.014 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 105 Resp: 10939
Ion Ratio Lower Upper
105 100
120 52.8 23.8 71.5


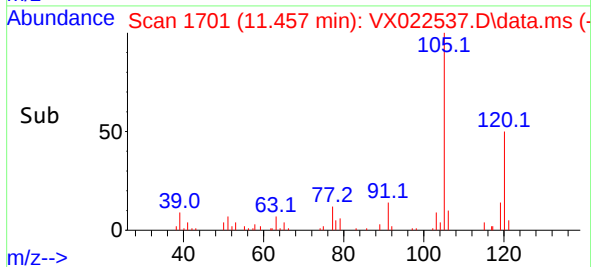

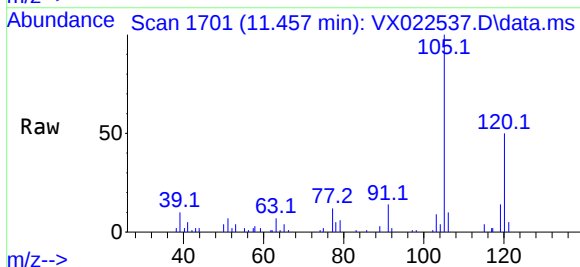




#81
trans-1,4-Dichloro-2-butene
Concen: 66.227 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampleId :
40955DL


Tgt Ion: 75 Resp: 27316
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

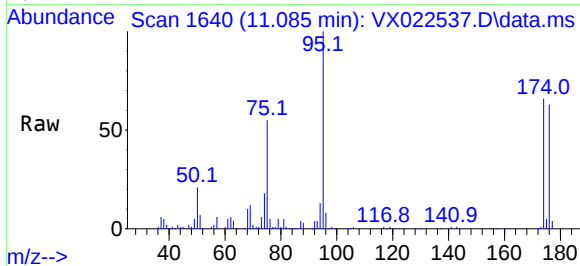

#82
4-Chlorotoluene
Concen: 0.585 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion: 91 Resp: 1559
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

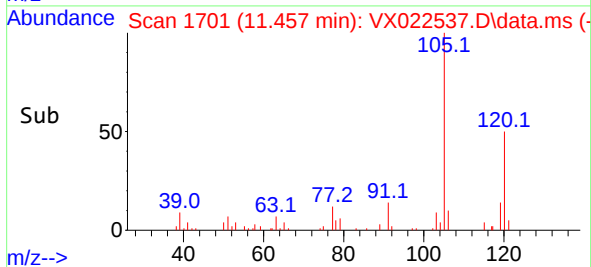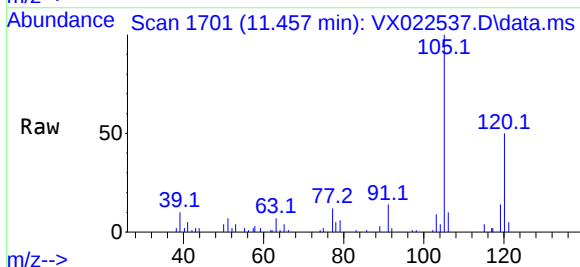







#83
tert-Butylbenzene
Concen: 1.056 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.256 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Instrument :
MSVOA_X
ClientSampled :
40955DL

Tgt Ion:119 Resp: 2563




Ion	Ratio	Lower	Upper
119	100		
91	48.2	27.9	83.7
134	27.5	11.3	33.9

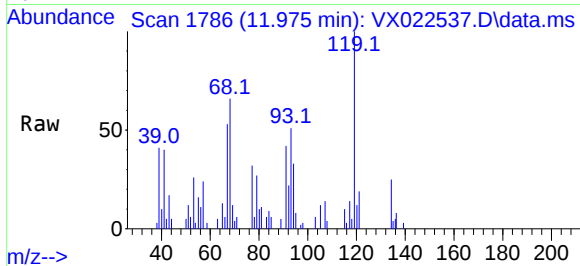


#84
1,2,4-Trimethylbenzene
Concen: 16.938 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Tgt Ion:105 Resp: 46422

Ion	Ratio	Lower	Upper
105	100		
120	42.7	22.4	67.3


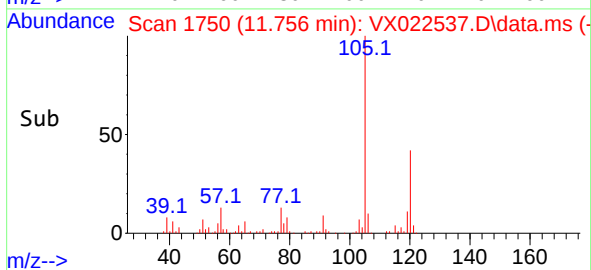

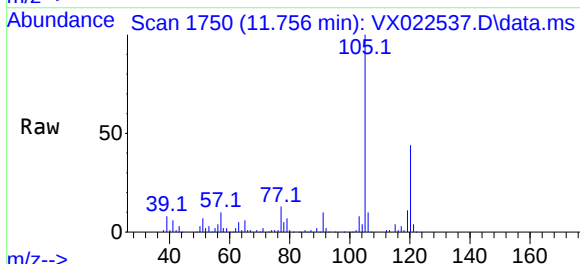




#85
 sec-Butylbenzene
 Concen: 0.695 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. -0.006 min
 Lab File: VX022537.D
 Acq: 07 Jun 2021 16:33




Instrument :
 MSVOA_X
 ClientSampleID :
 40955DL


Tgt Ion:105 Resp: 2246
 Ion Ratio Lower Upper
 105 100
 134 29.6 10.0 29.8

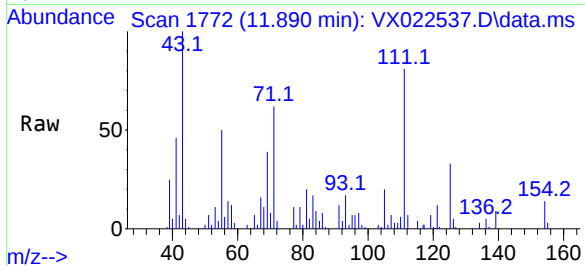

#86
 p-Isopropyltoluene
 Concen: 2.797 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. -0.000 min
 Lab File: VX022537.D
 Acq: 07 Jun 2021 16:33

Tgt Ion:119 Resp: 7468
 Ion Ratio Lower Upper
 119 100
 134 24.8 12.9 38.7
 91 27.6 11.7 35.0


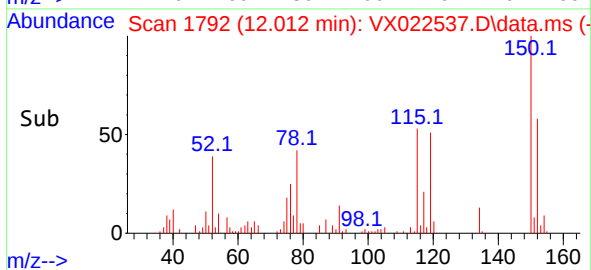

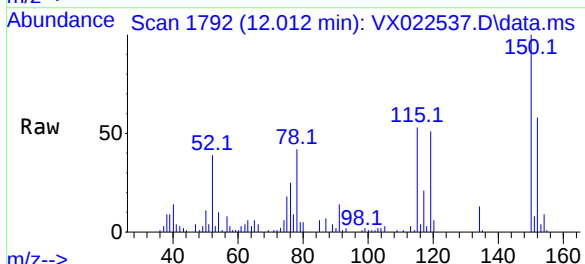




#89
n-Butylbenzene
Concen: 2.043 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33




Instrument :
MSVOA_X
ClientSampled :
40955DL


Tgt Ion: 91 Resp: 5237
Ion Ratio Lower Upper
91 100
92 35.9 27.4 82.0
134 86.8 13.2 39.5#

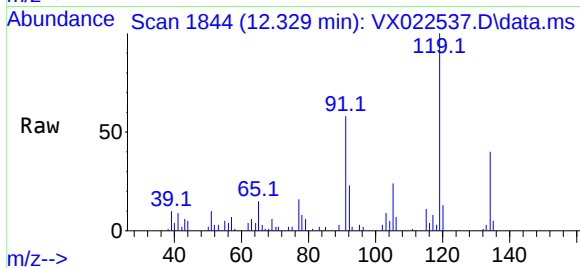

#90
Hexachloroethane
Concen: 4.667 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.012 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33


Tgt Ion: 117 Resp: 637
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

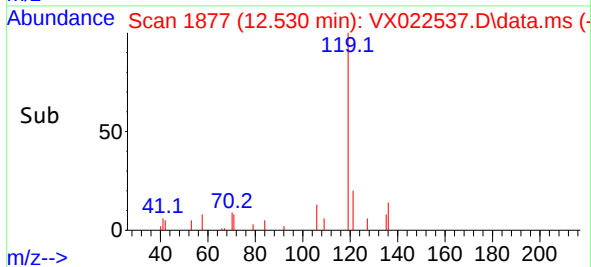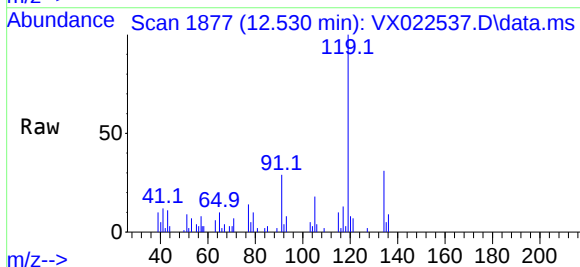



#95
Naphthalene
Concen: 1.061 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022537.D
Acq: 07 Jun 2021 16:33

Instrument :
MSVOA_X
ClientSampleId :
40955DL

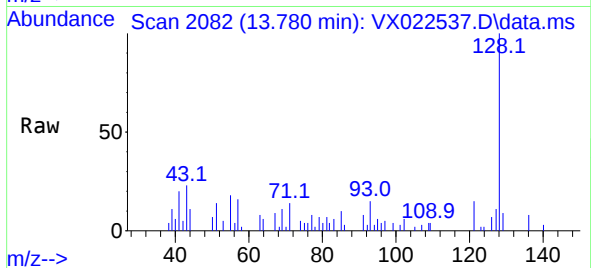

Tgt Ion:128 Resp: 3239
Ion Ratio Lower Upper
128 100
127 15.5 10.3 15.5#
129 12.5 8.8 13.2

