


Acrolein

Response Ratio

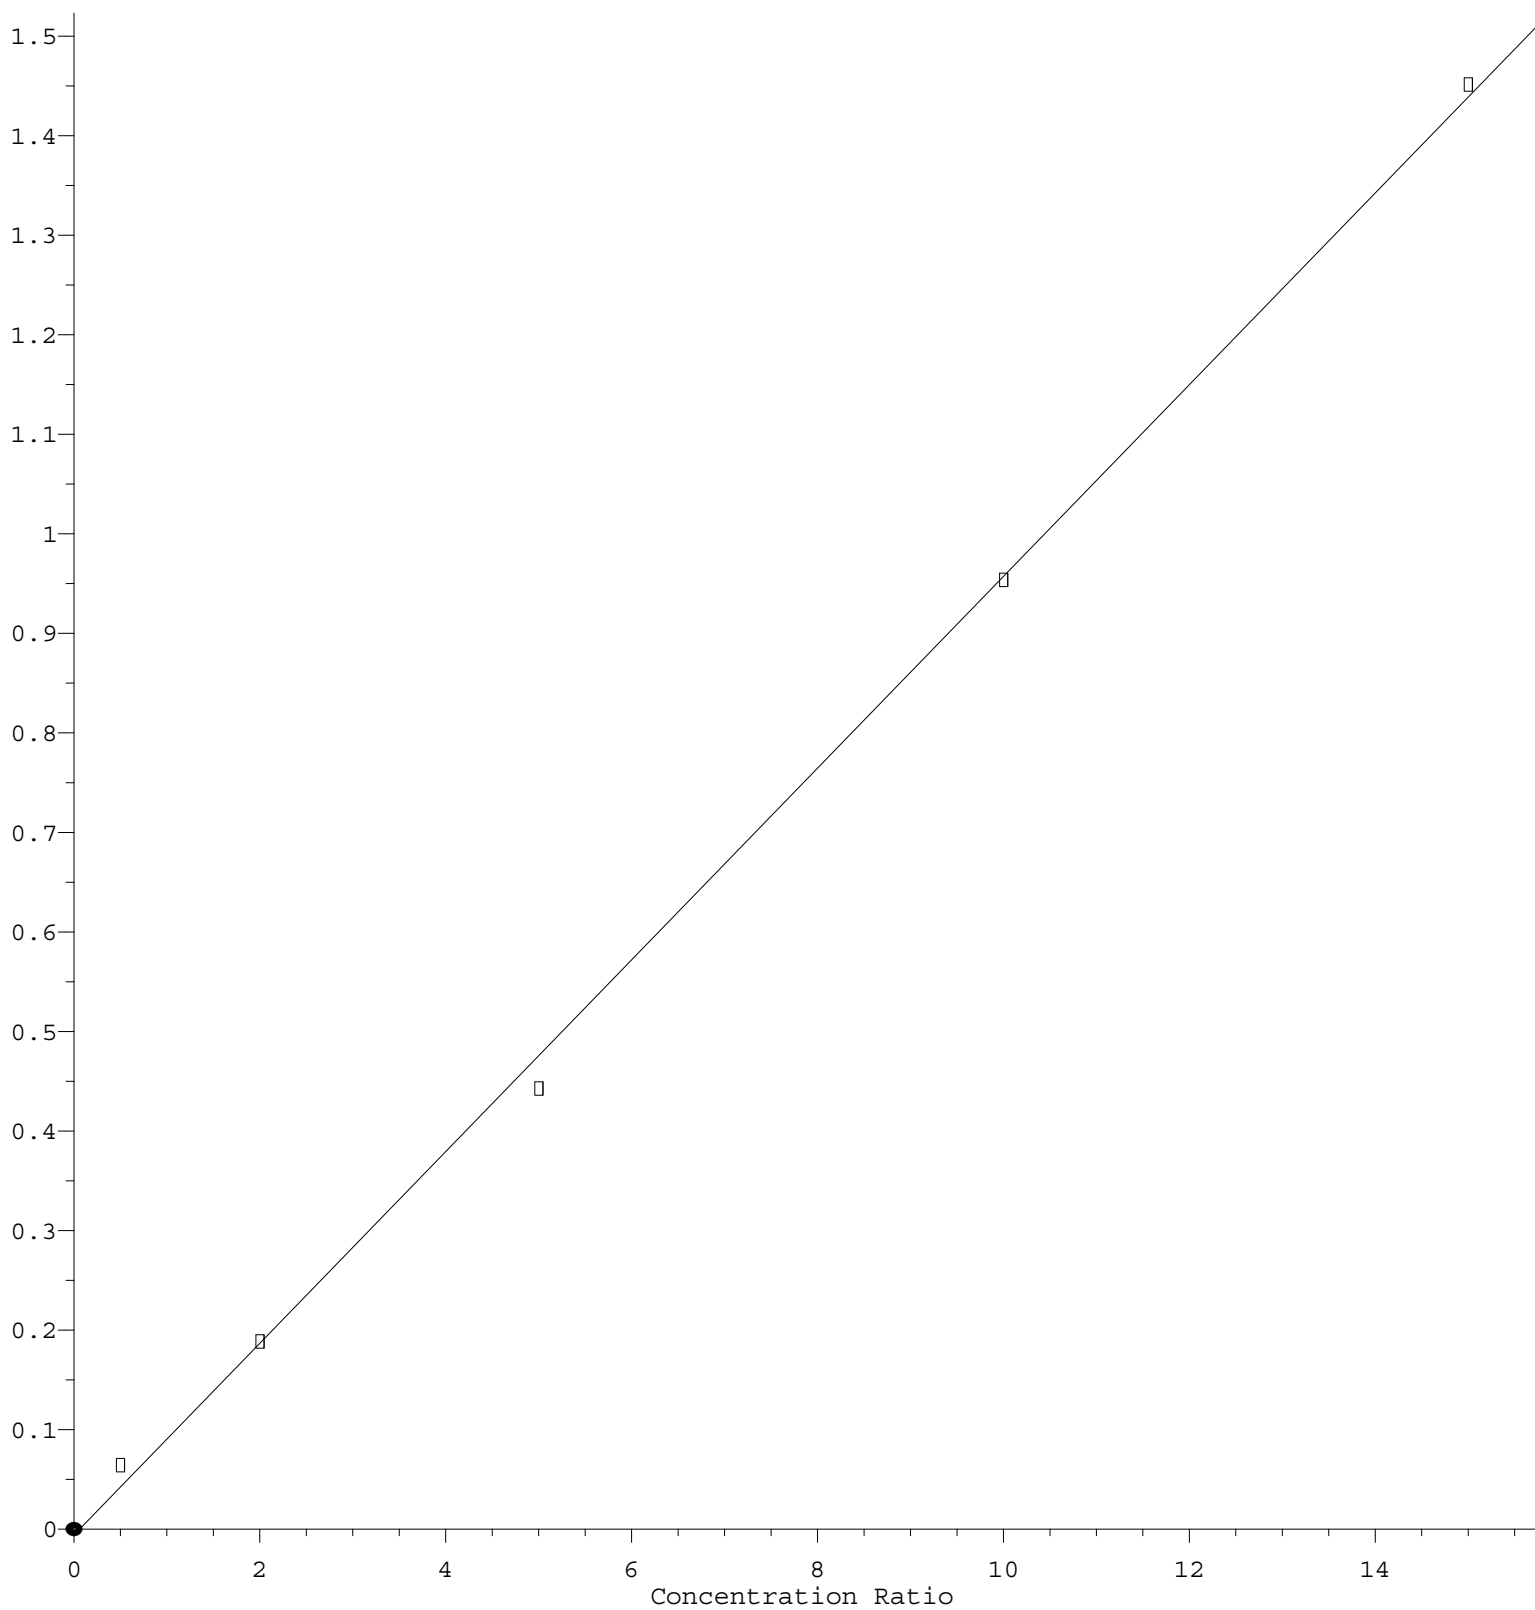

$$\text{Response} = 9.633 \times 10^{-2} \times \text{Amt} - 6.010 \times 10^{-3}$$


Coef of Det (r^2) = 0.998688 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

1,1,1,2-Tetrachloroethane

Response Ratio

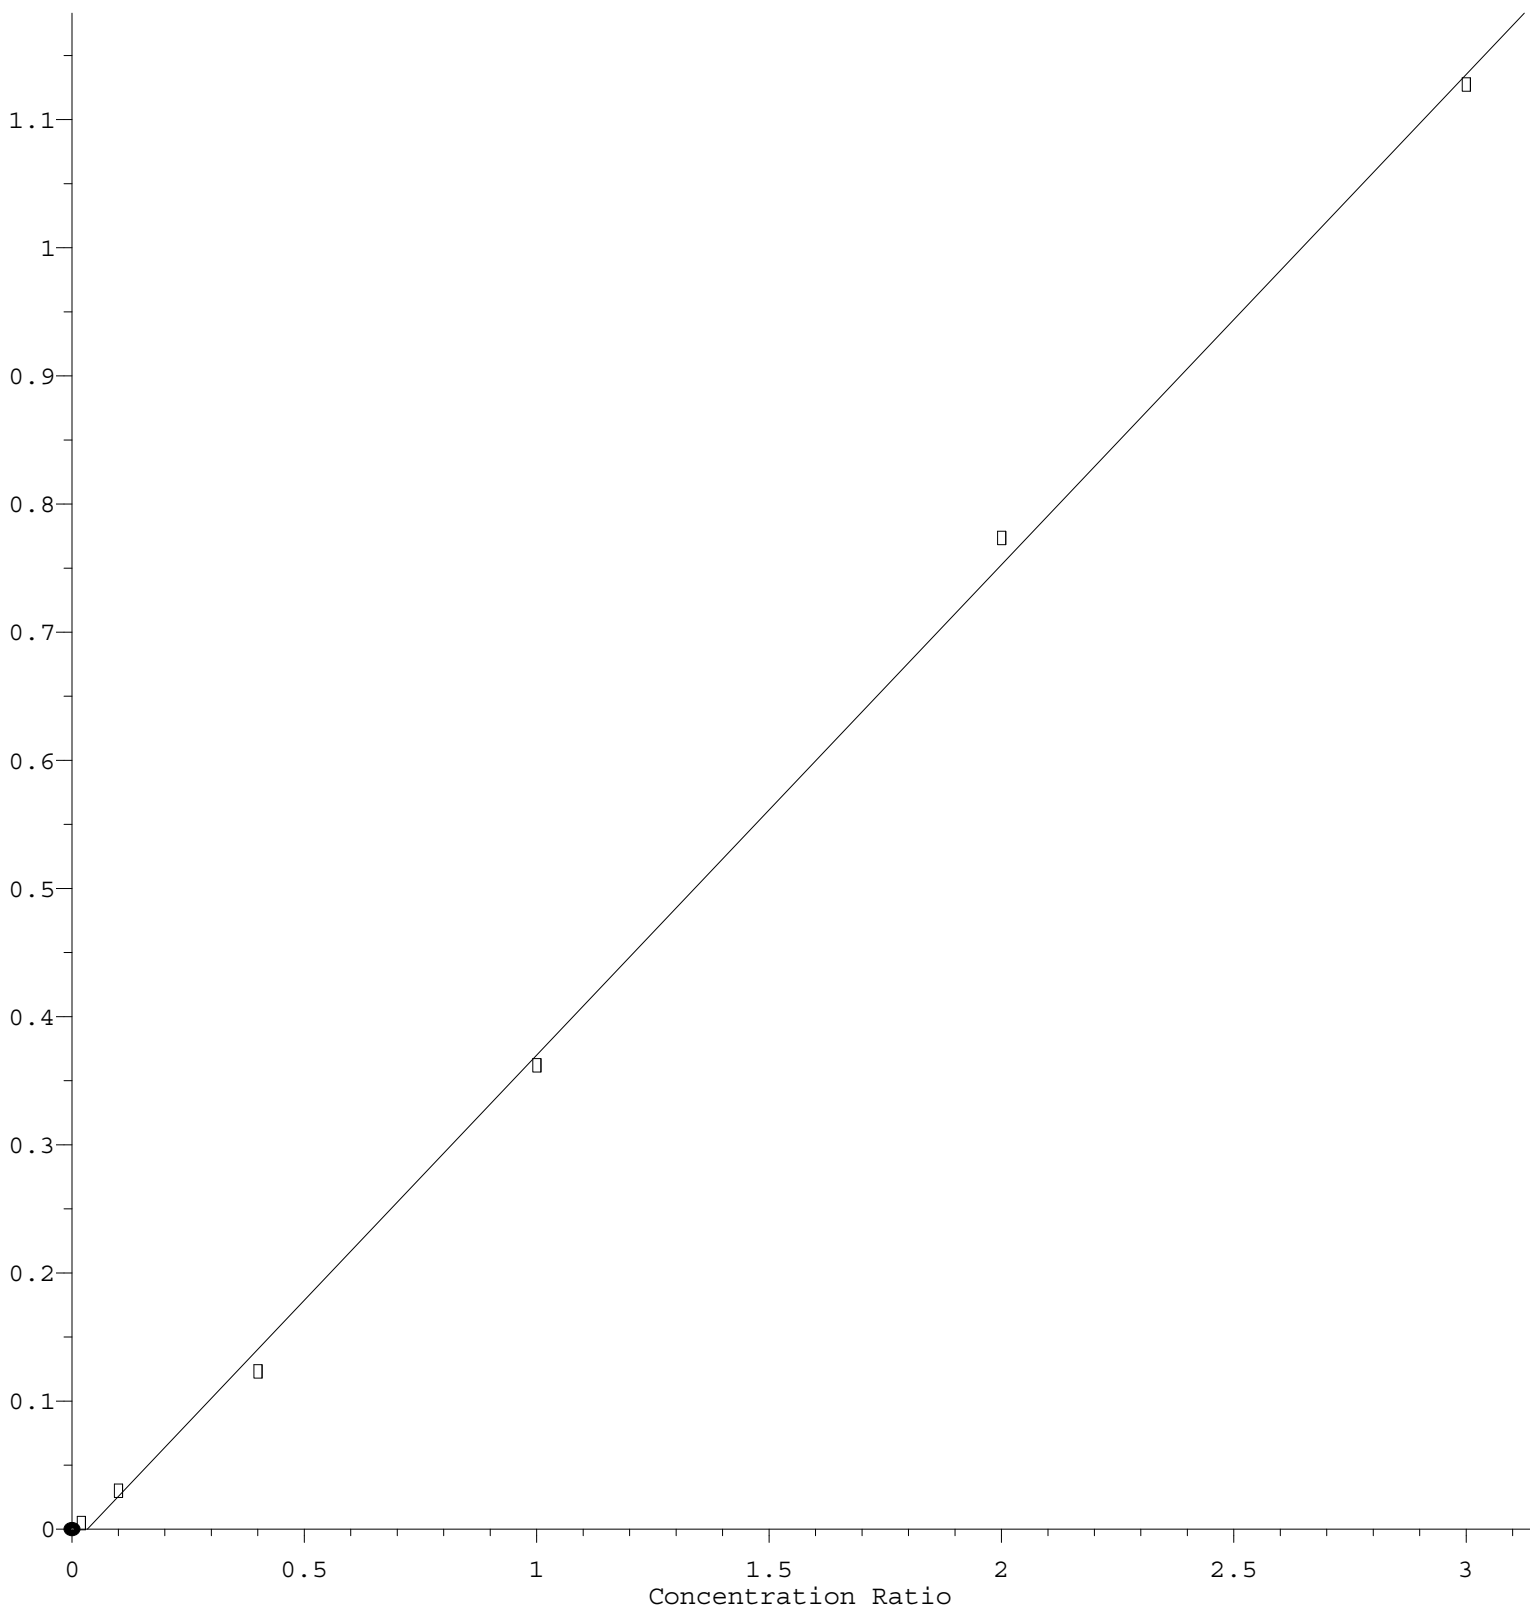


$$\text{Response} = 3.829\text{e-}001 * \text{Amt} - 1.265\text{e-}002$$

Coef of Det (r^2) = 0.999065 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021


Bromoform

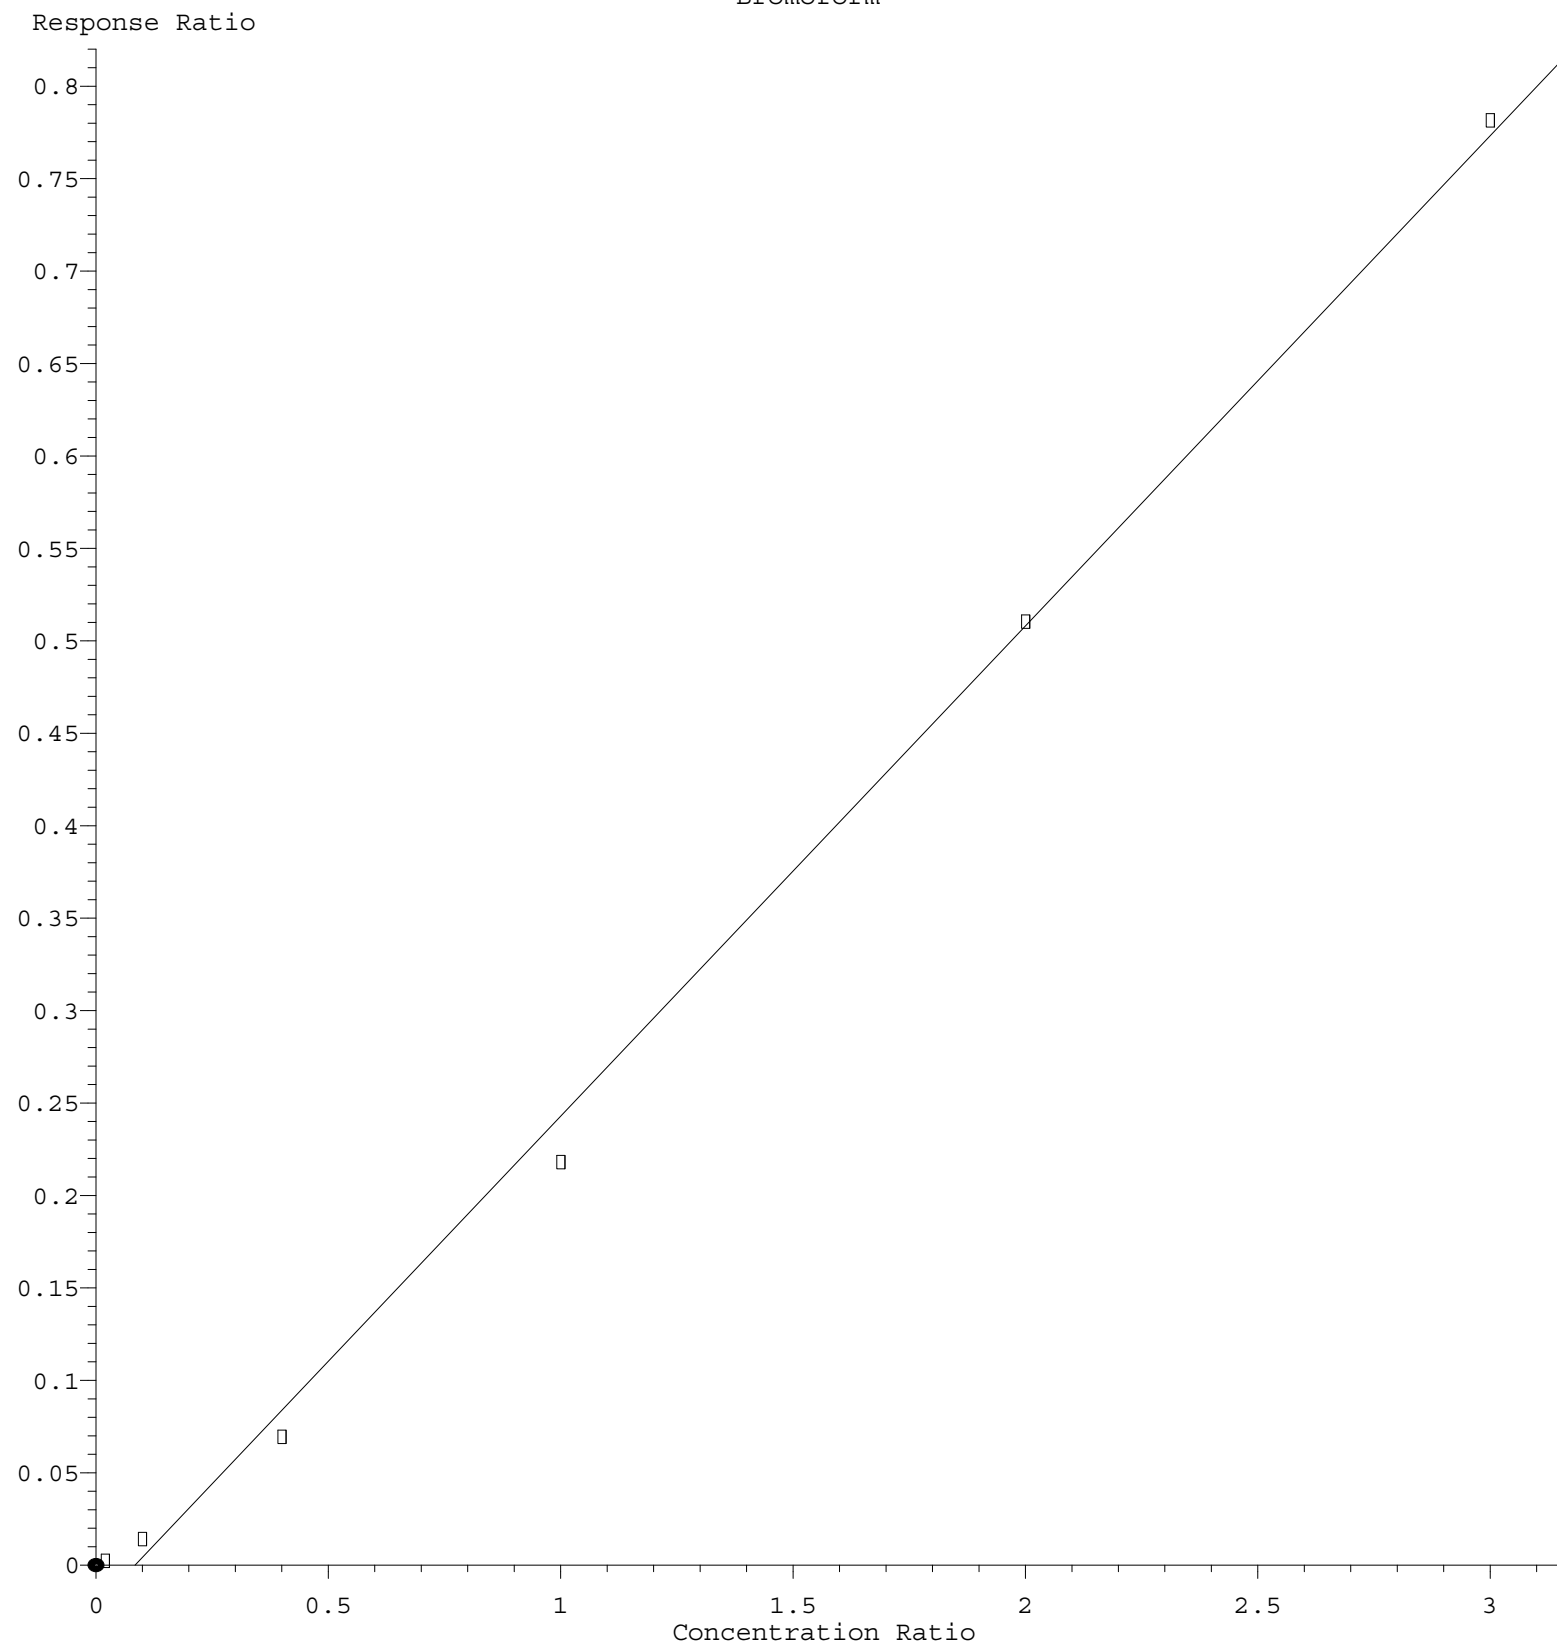

Response = $2.651e-001 * Amt - 2.214e-002$
 Coef of Det (r^2) = 0.997261 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M
 Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

trans-1,4-Dichloro-2-butene

Response Ratio

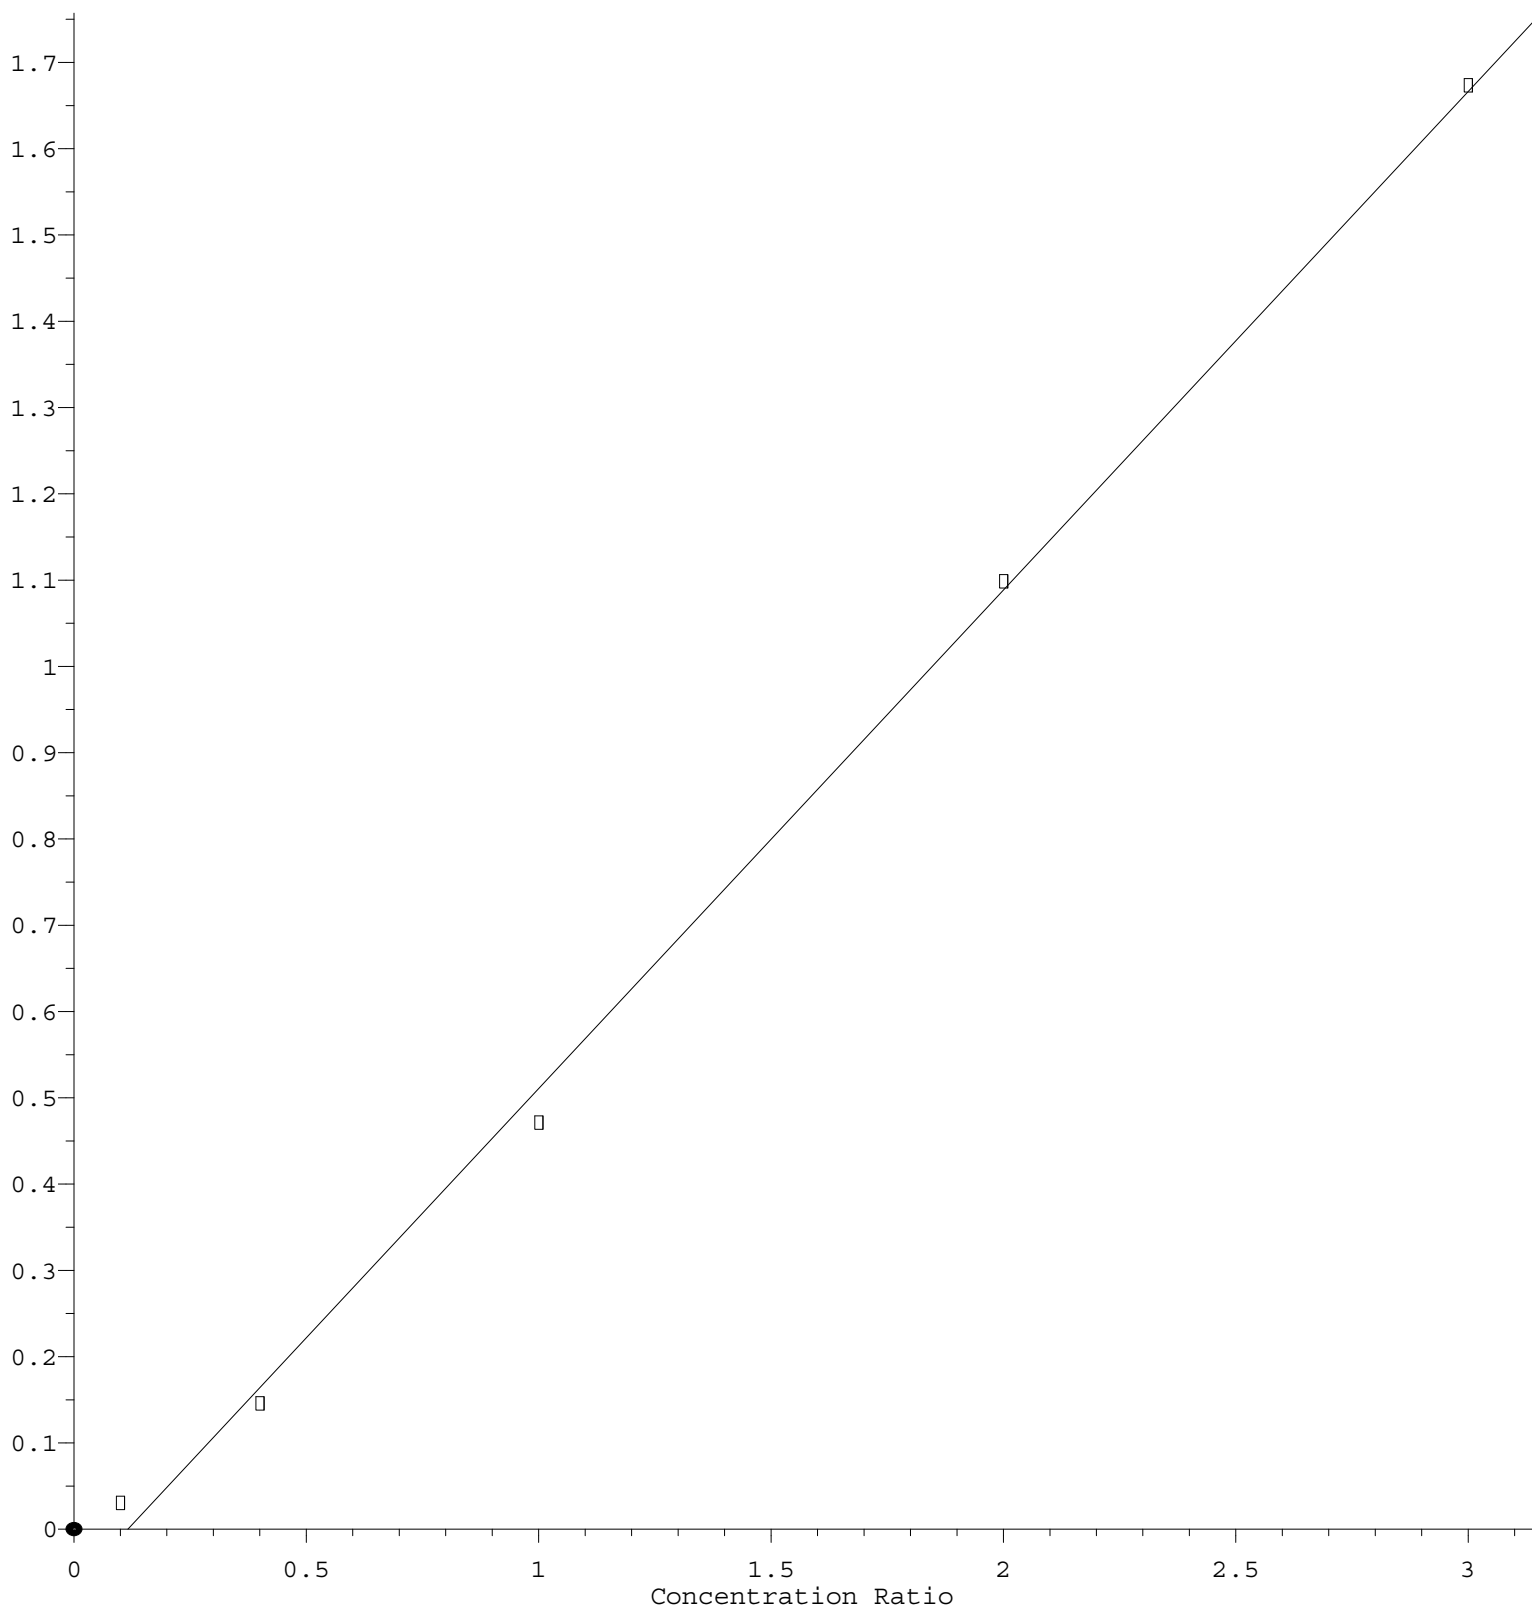

$$\text{Response} = 5.777\text{e-}001 * \text{Amt} - 6.720\text{e-}002$$


Coef of Det (r^2) = 0.998112 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

Hexachloroethane

Response Ratio

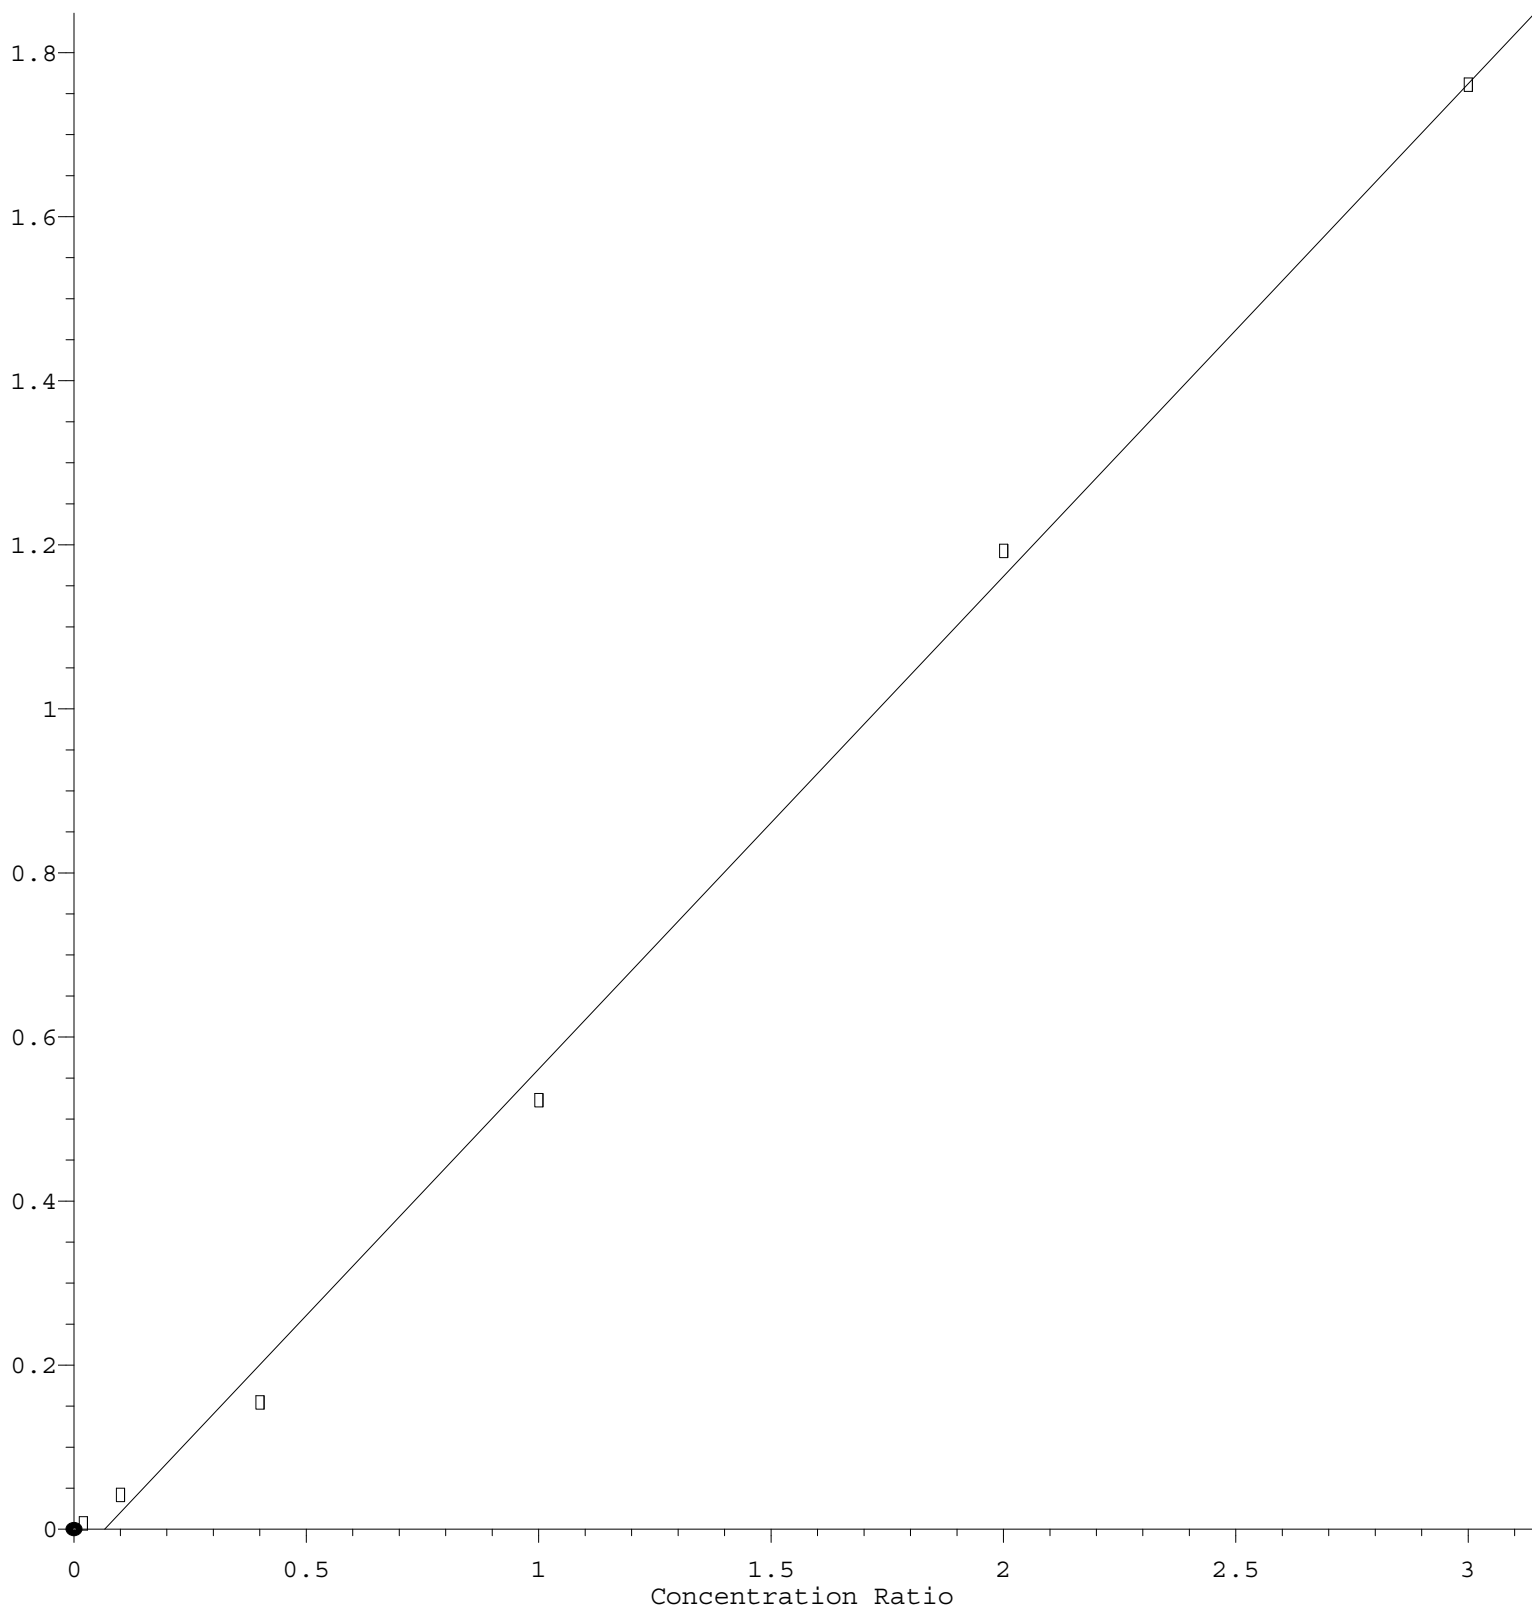

$$\text{Response} = 6.010\text{e-}001 * \text{Amt} - 3.981\text{e-}002$$


Coef of Det (r^2) = 0.997594 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

1,2-Dibromo-3-Chloropropane

Response Ratio

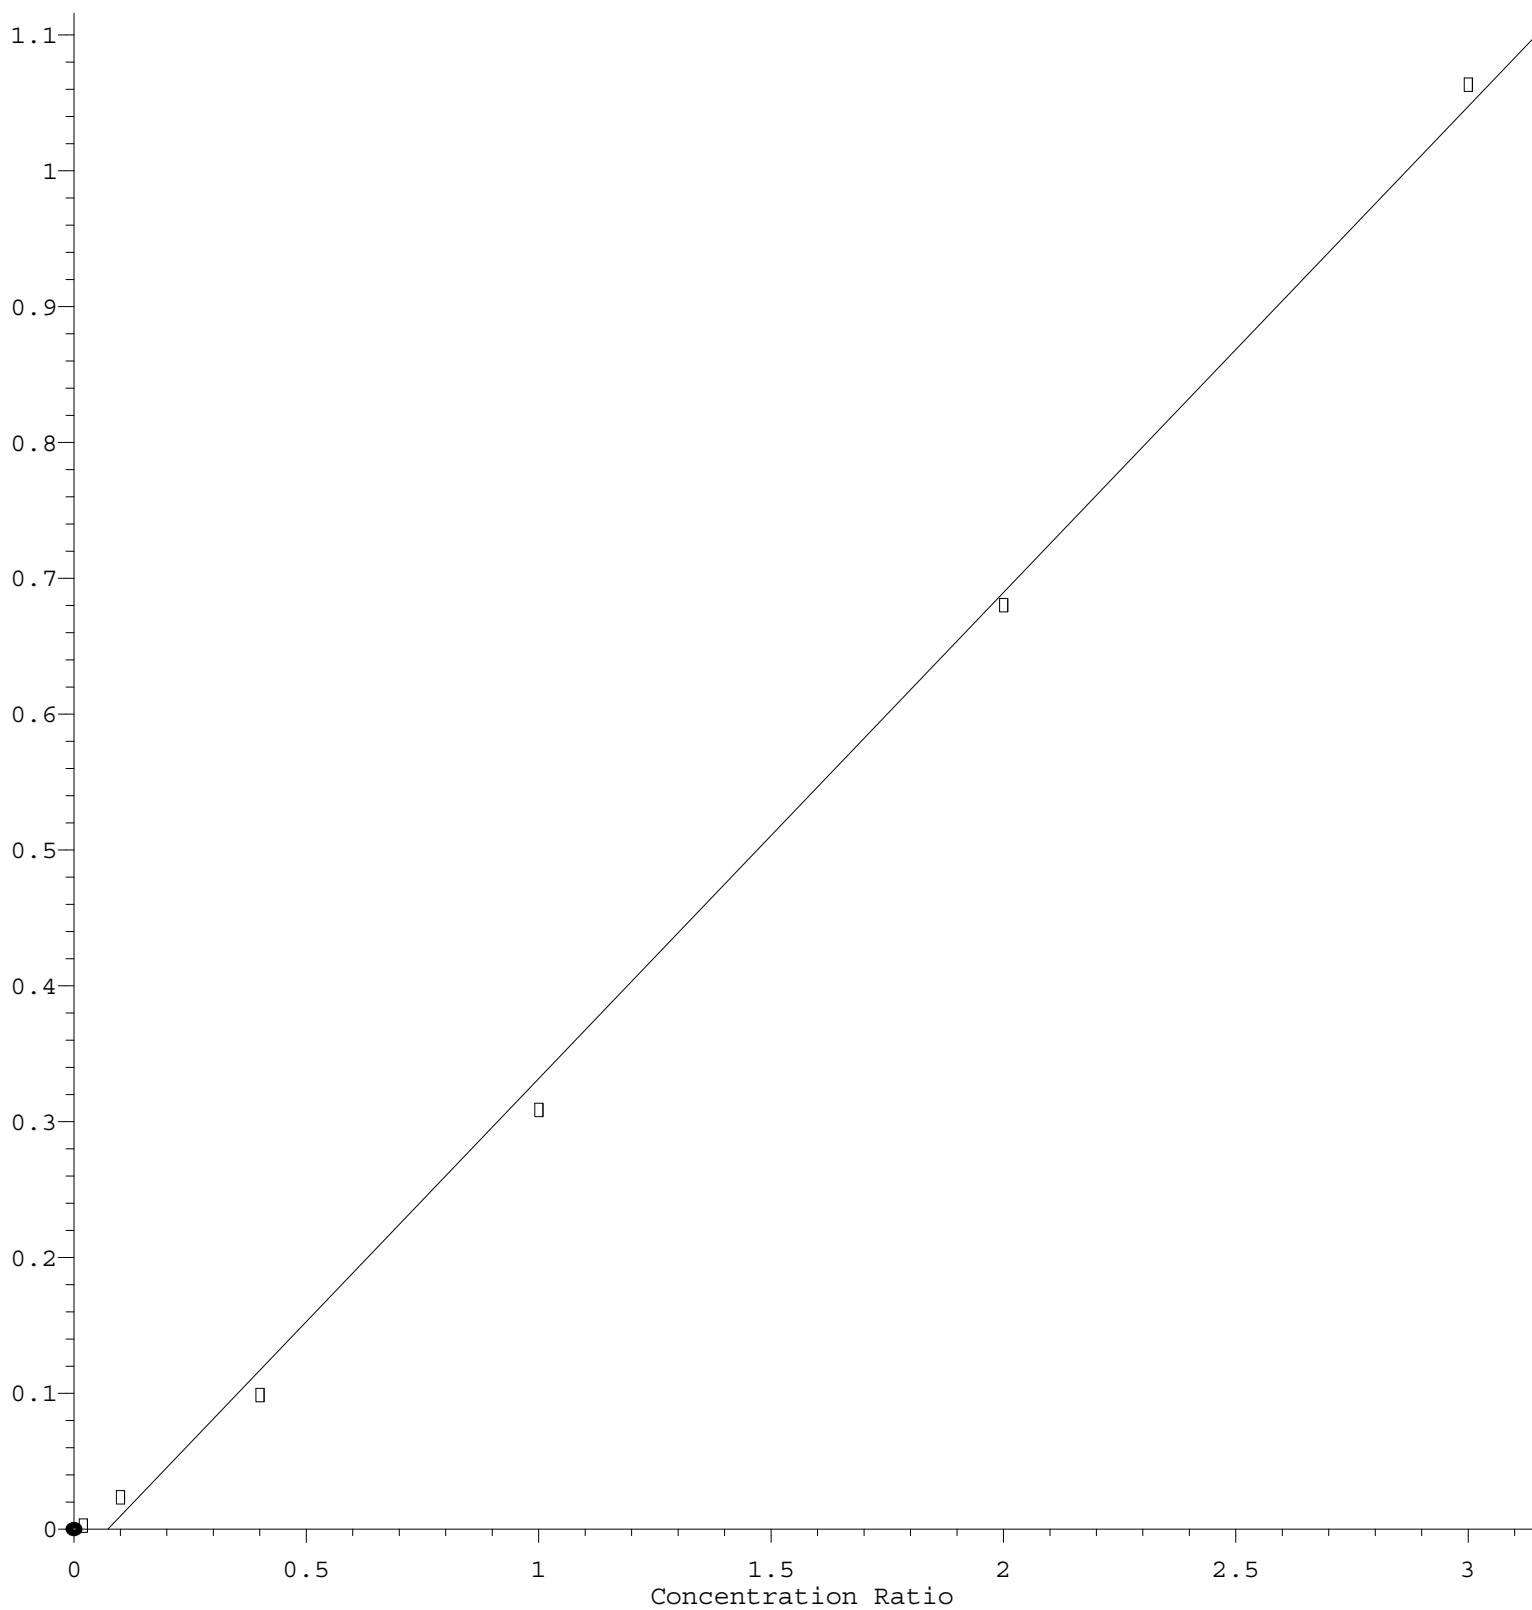

$$\text{Response} = 3.578\text{e-}001 * \text{Amt} - 2.602\text{e-}002$$


Coef of Det (r^2) = 0.997949 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

Carbon Disulfide

Response Ratio

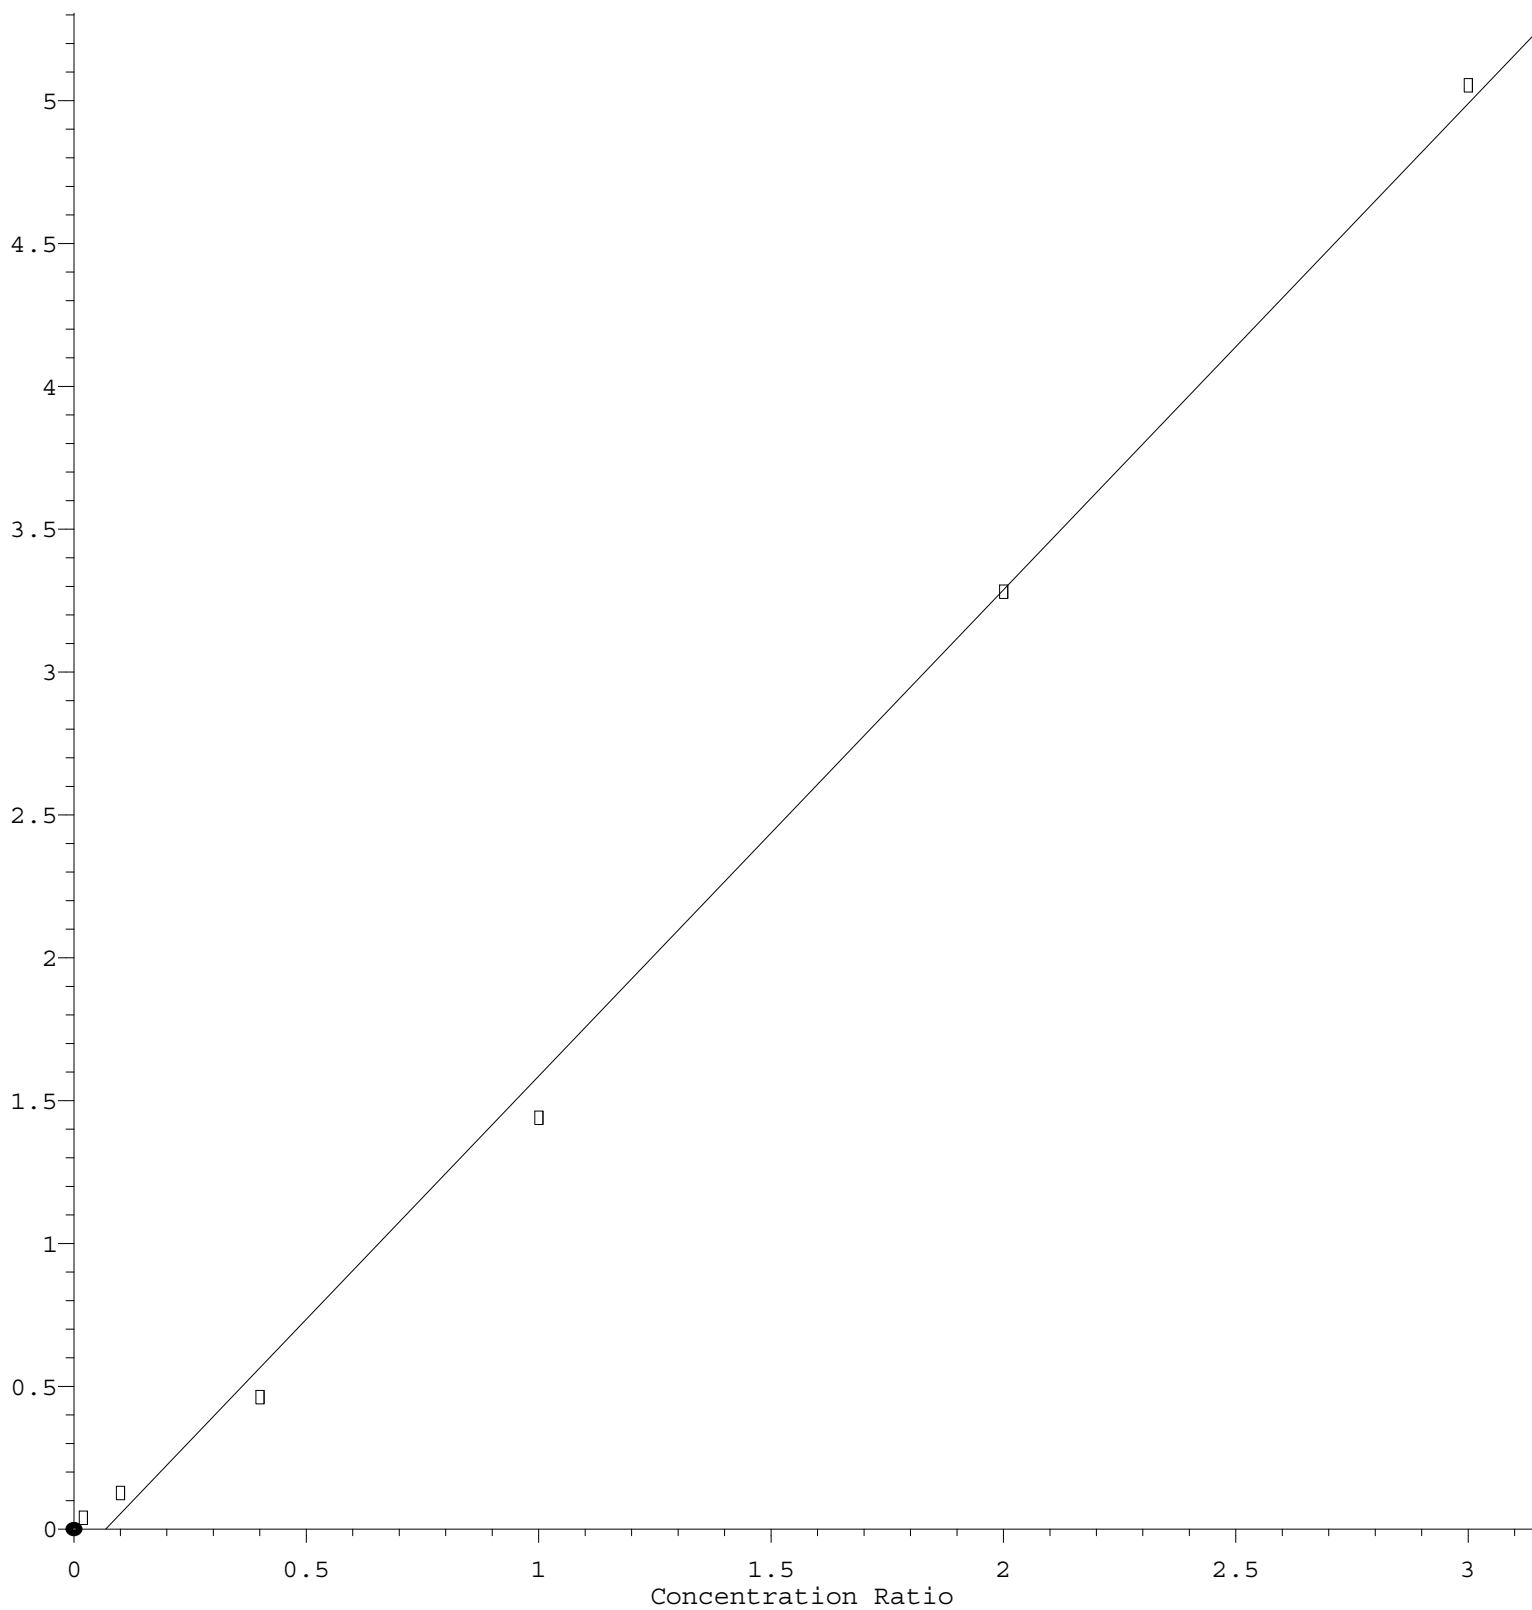

$$\text{Response} = 1.701\text{e}+000 * \text{Amt} - 1.152\text{e}-001$$


Coef of Det (r^2) = 0.997269 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

Carbon Tetrachloride

Response Ratio

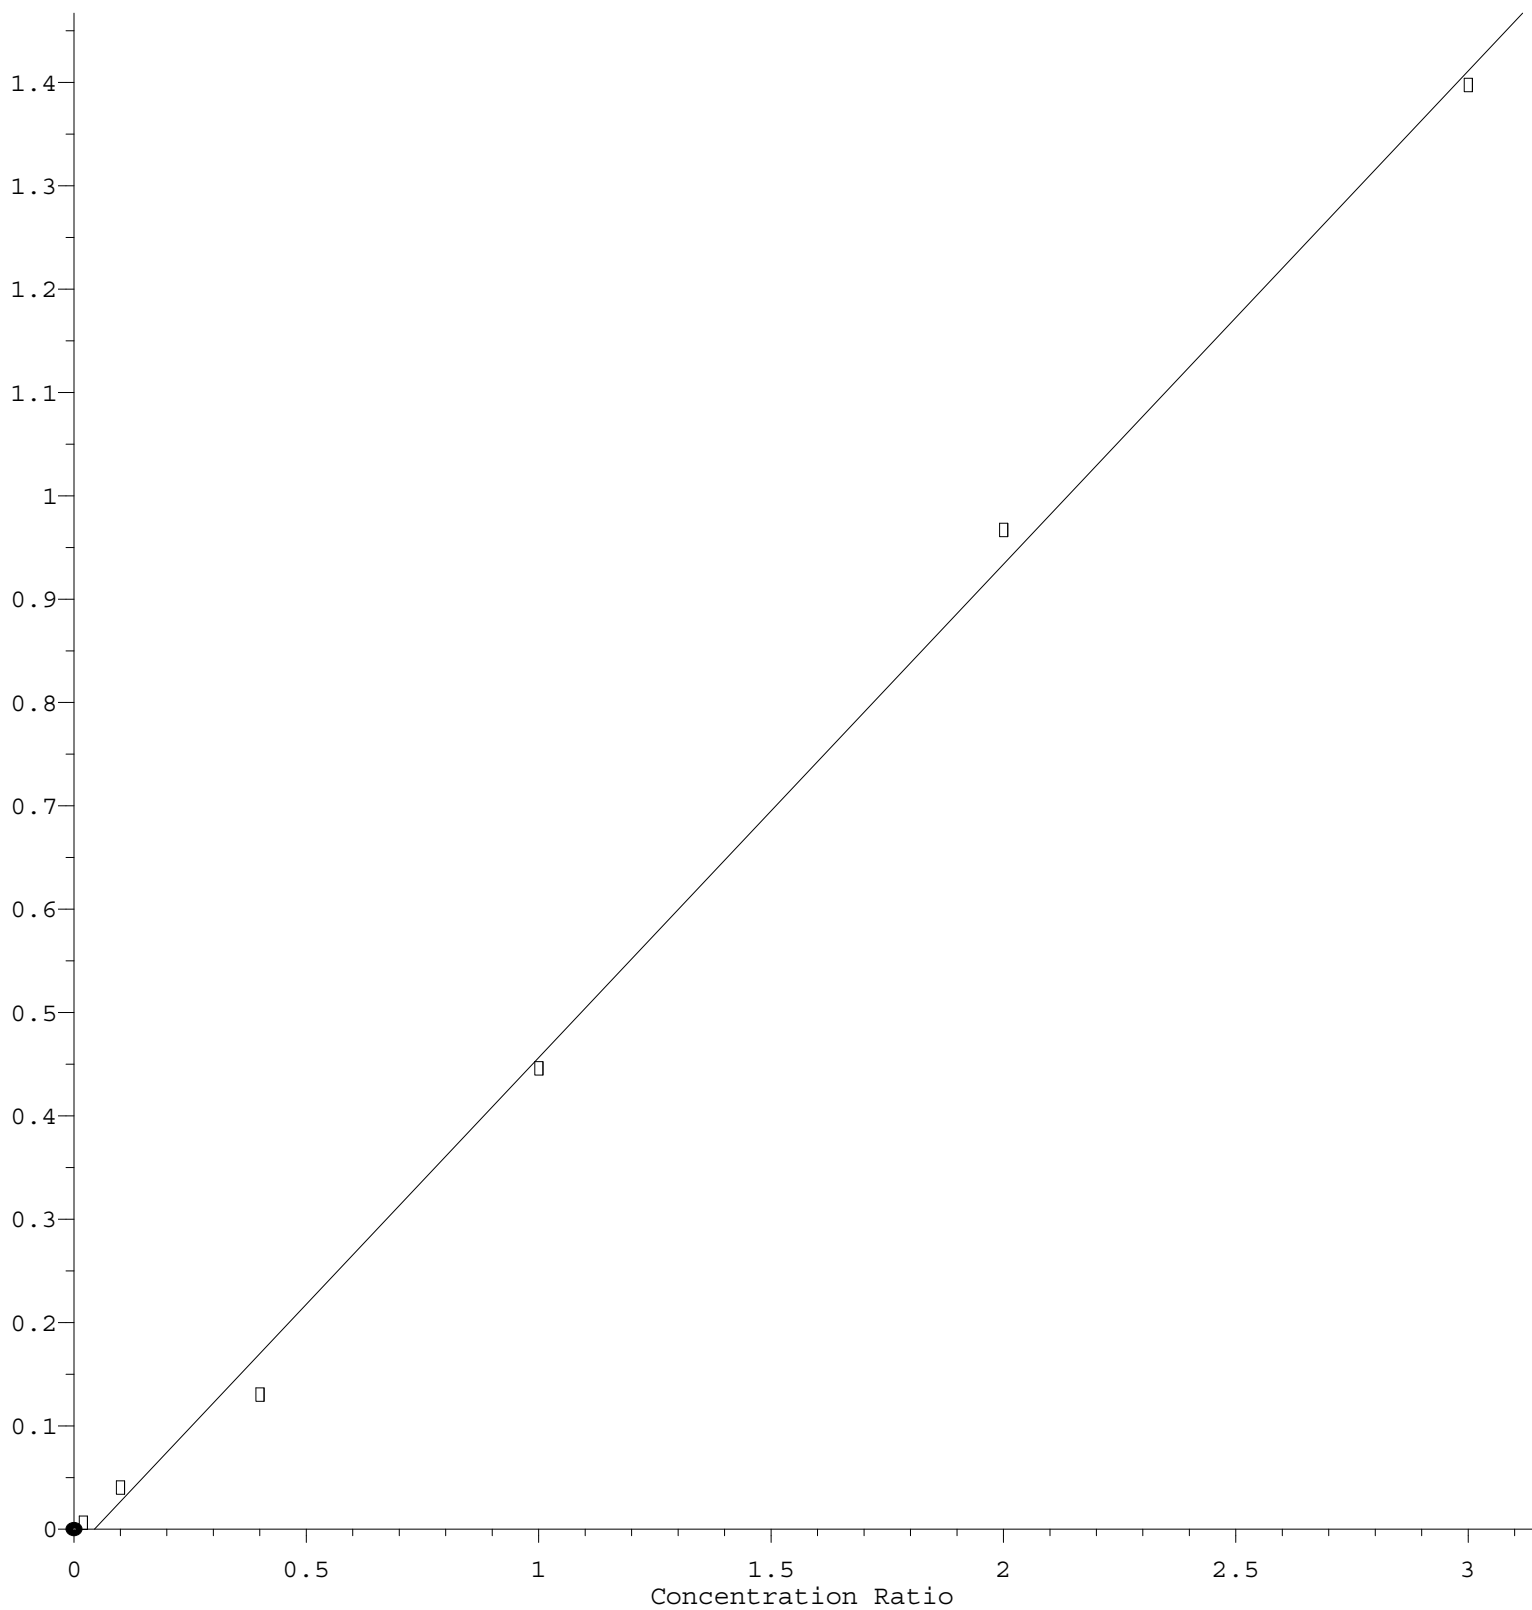

$$\text{Response} = 4.774\text{e-}001 * \text{Amt} - 2.093\text{e-}002$$


Coef of Det (r^2) = 0.997850 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

Methylcyclohexane

Response Ratio

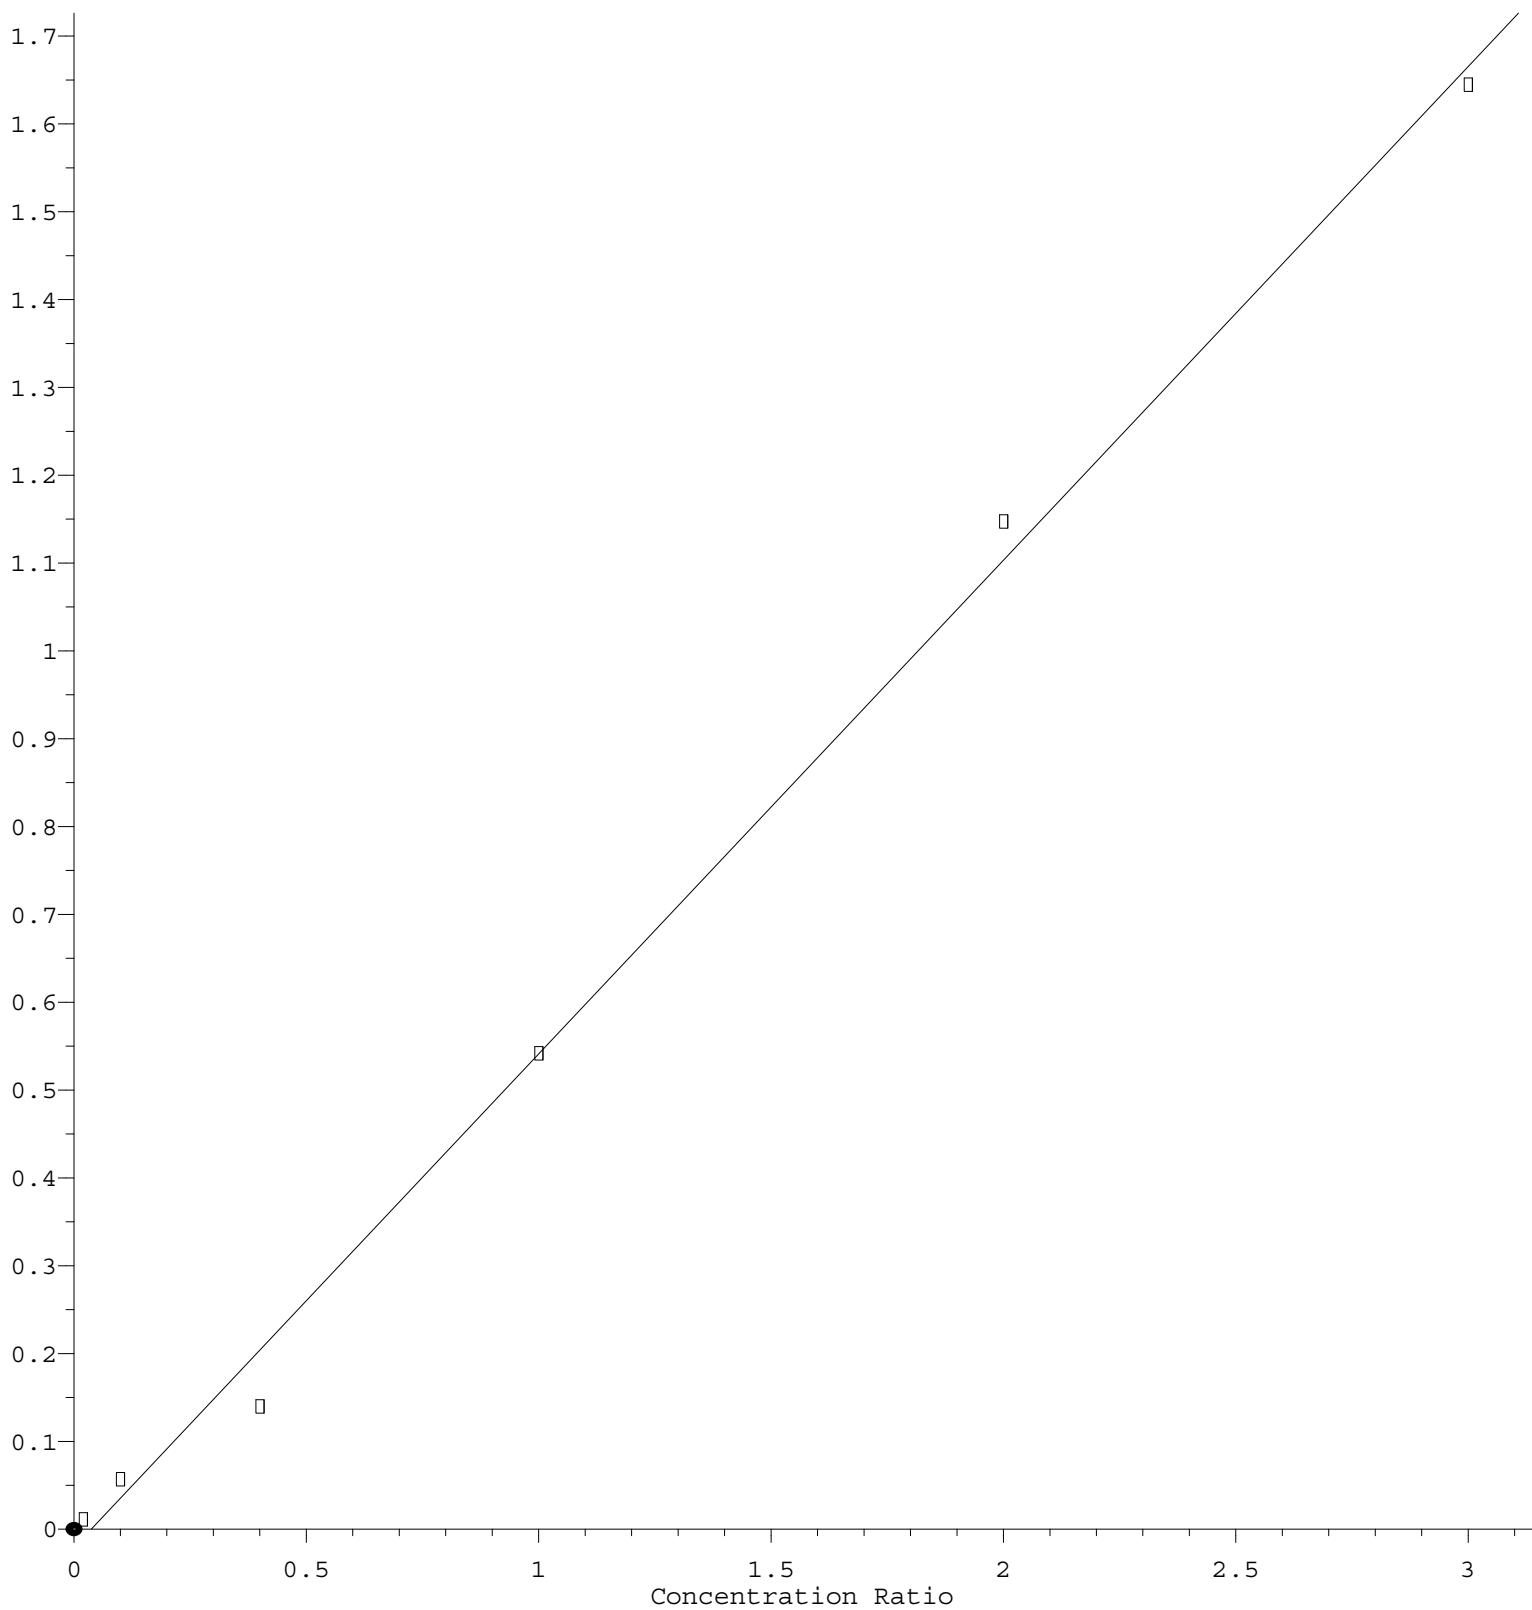

$$\text{Response} = 5.622\text{e-}001 * \text{Amt} - 2.072\text{e-}002$$


Coef of Det (r^2) = 0.996721 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

Bromodichloromethane

Response Ratio

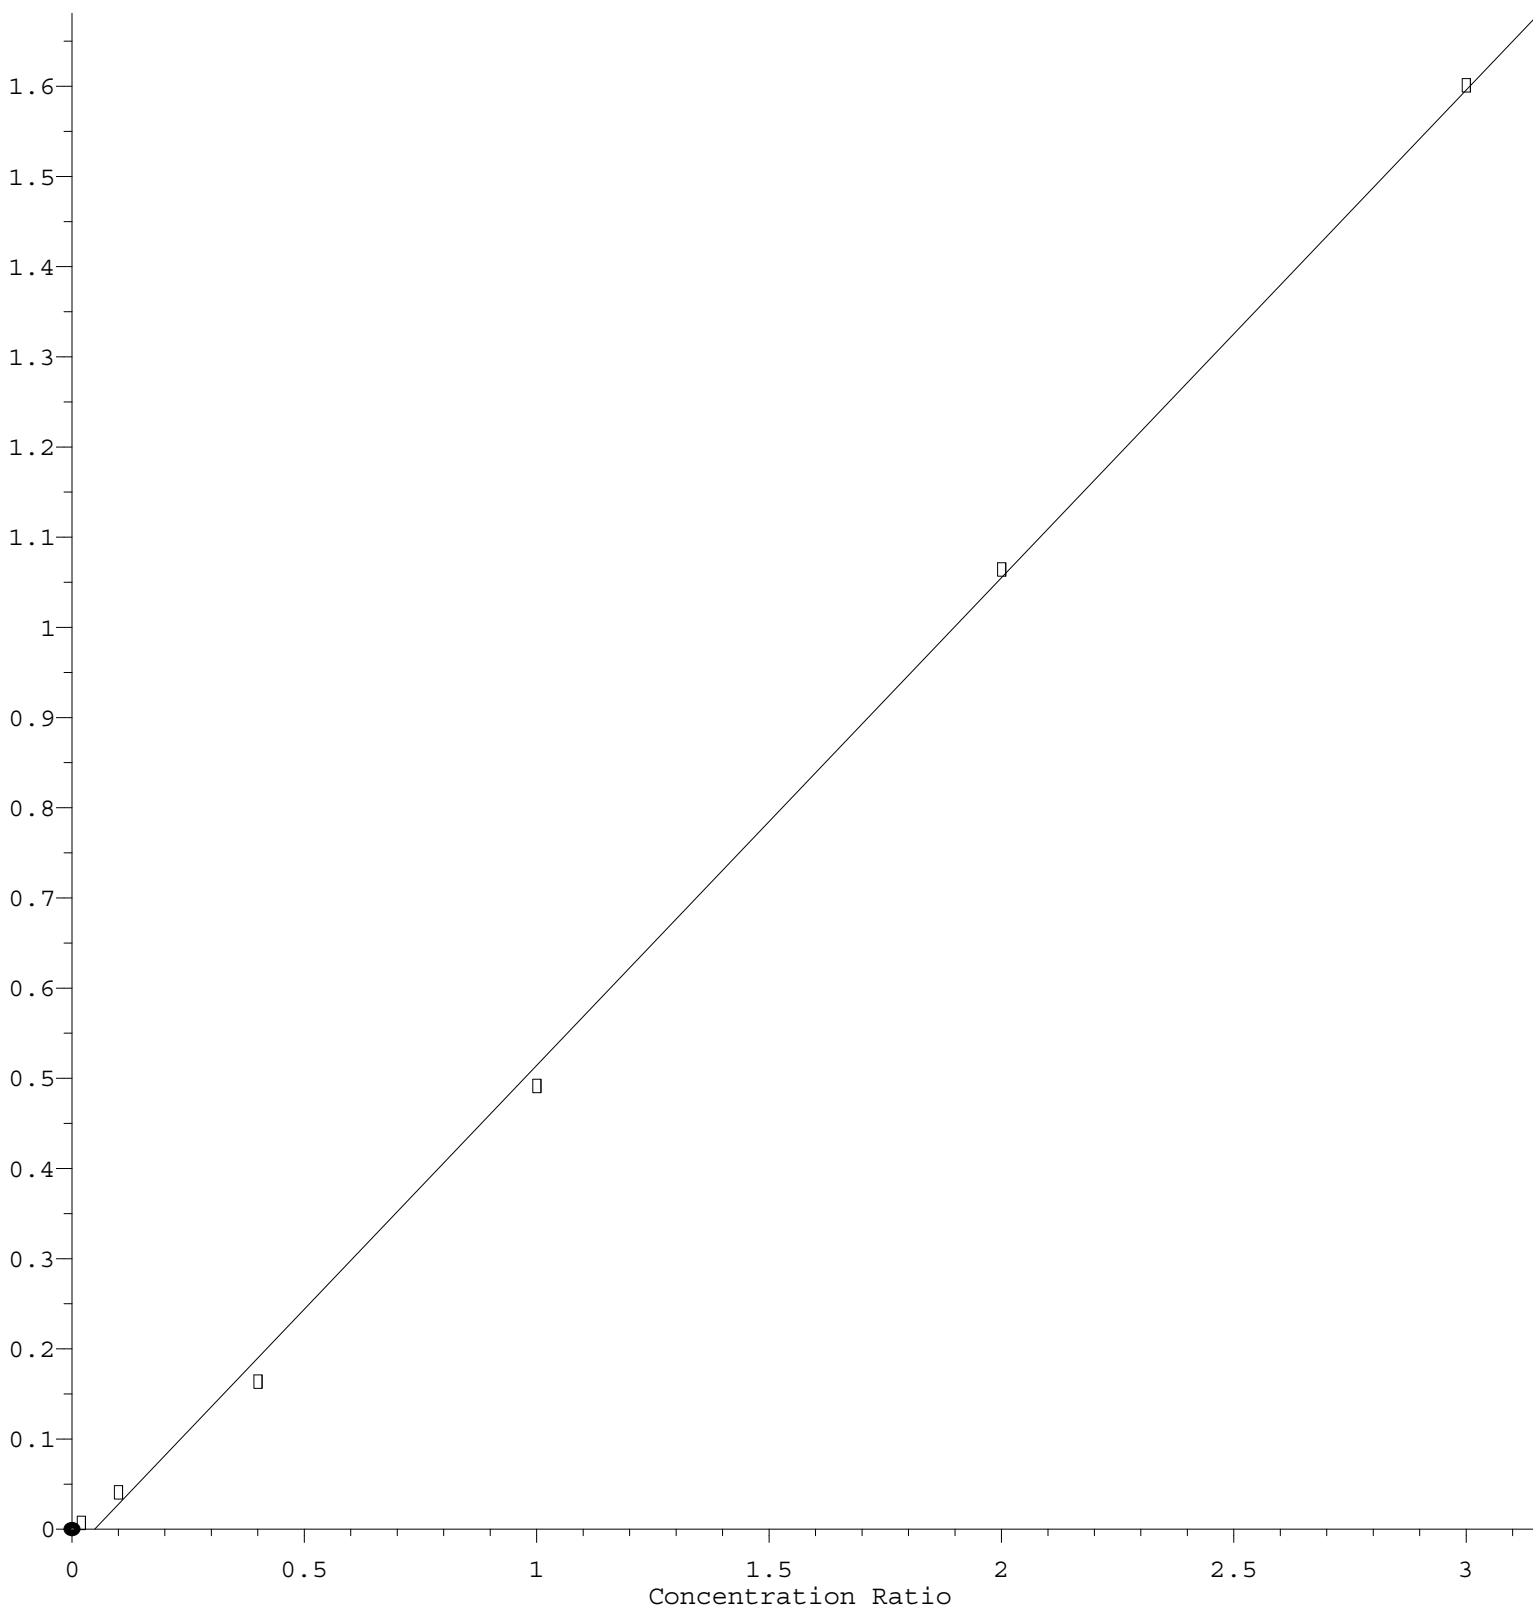

$$\text{Response} = 5.409\text{e-}001 * \text{Amt} - 2.650\text{e-}002$$


Coef of Det (r^2) = 0.999033 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

t-1,3-Dichloropropene

Response Ratio

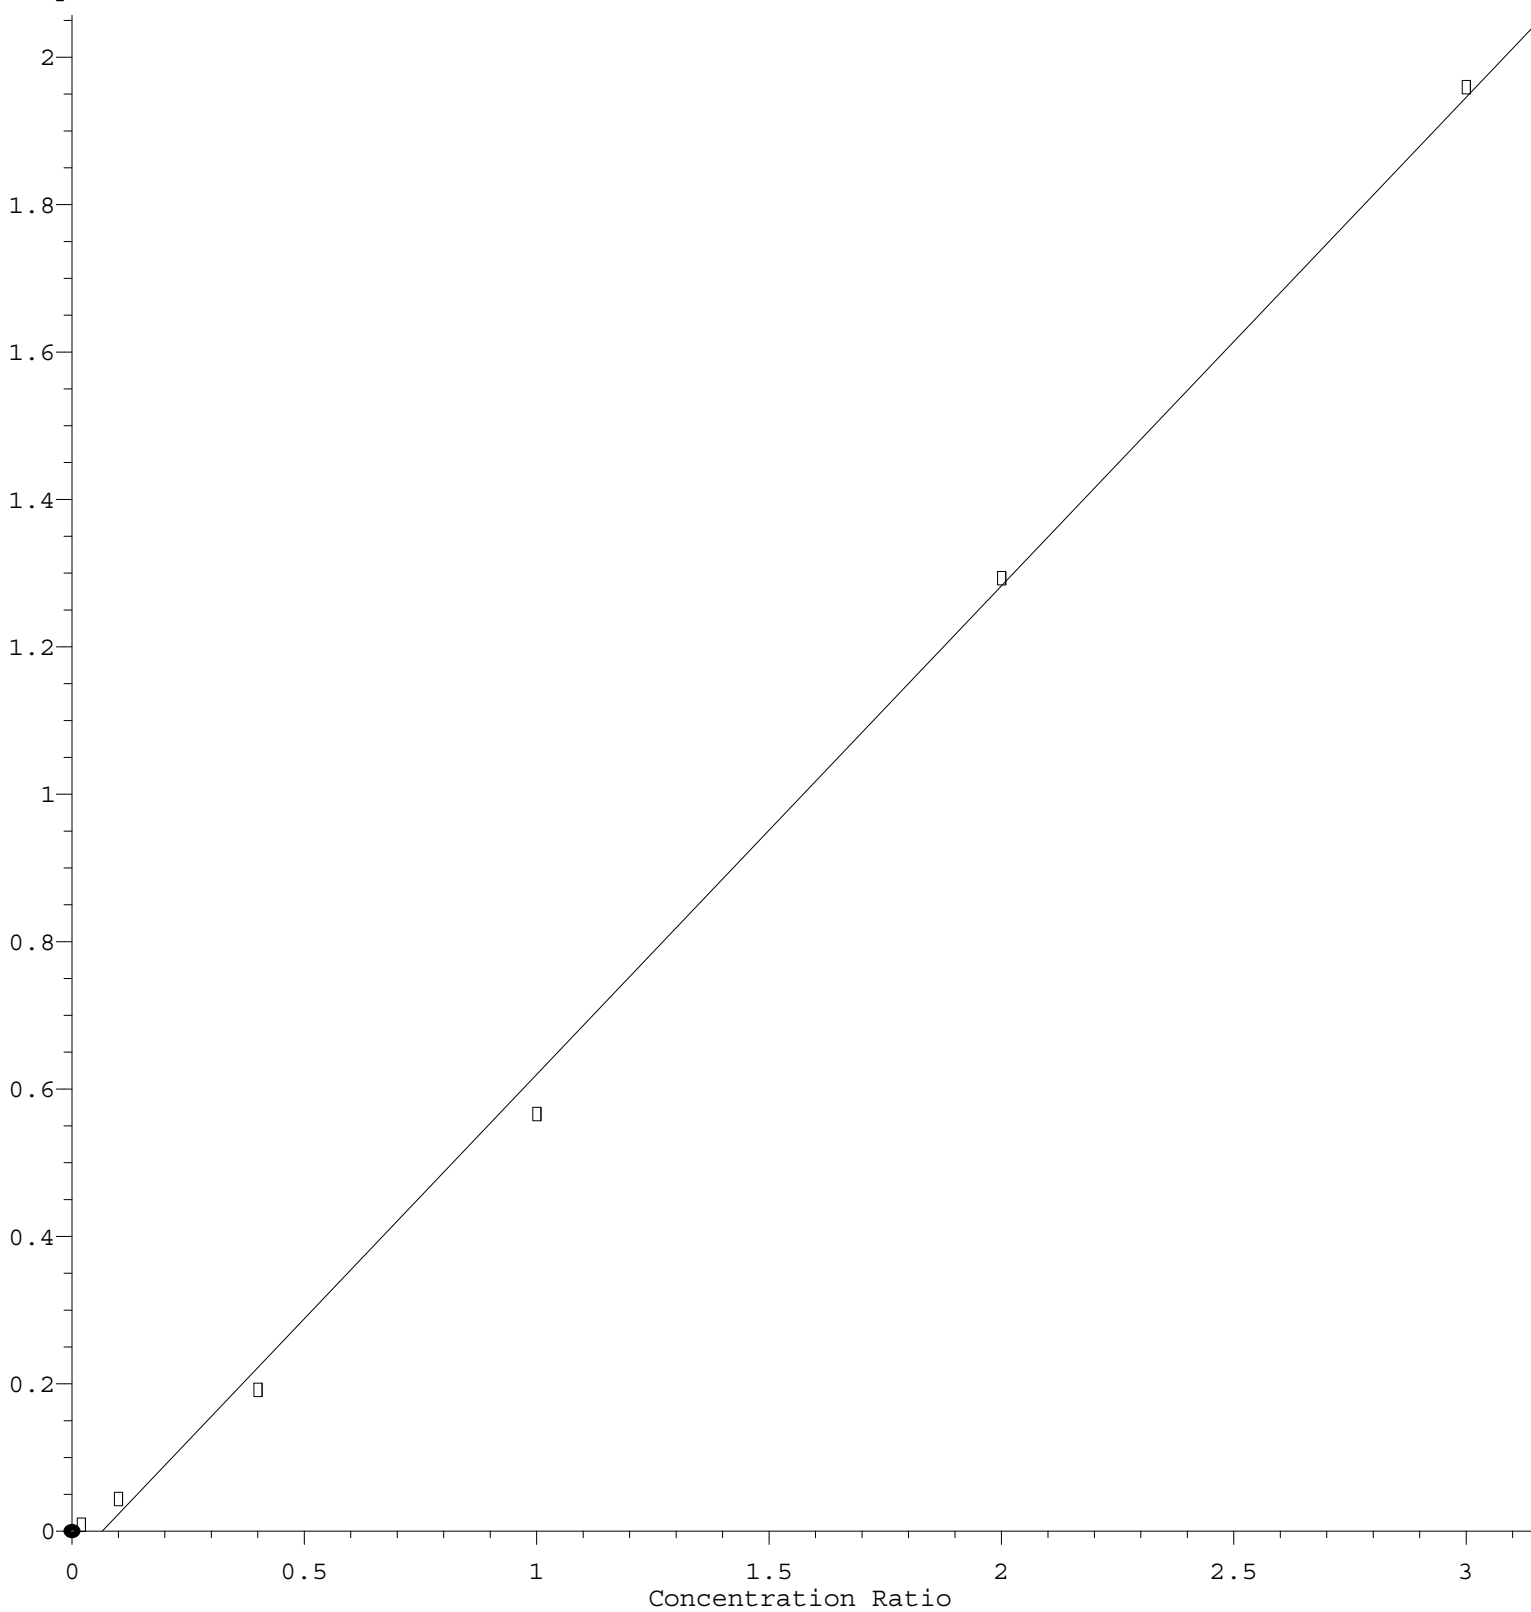

$$\text{Response} = 6.629\text{e-}001 * \text{Amt} - 4.324\text{e-}002$$


Coef of Det (r^2) = 0.998075 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

cis-1,3-Dichloropropene

Response Ratio

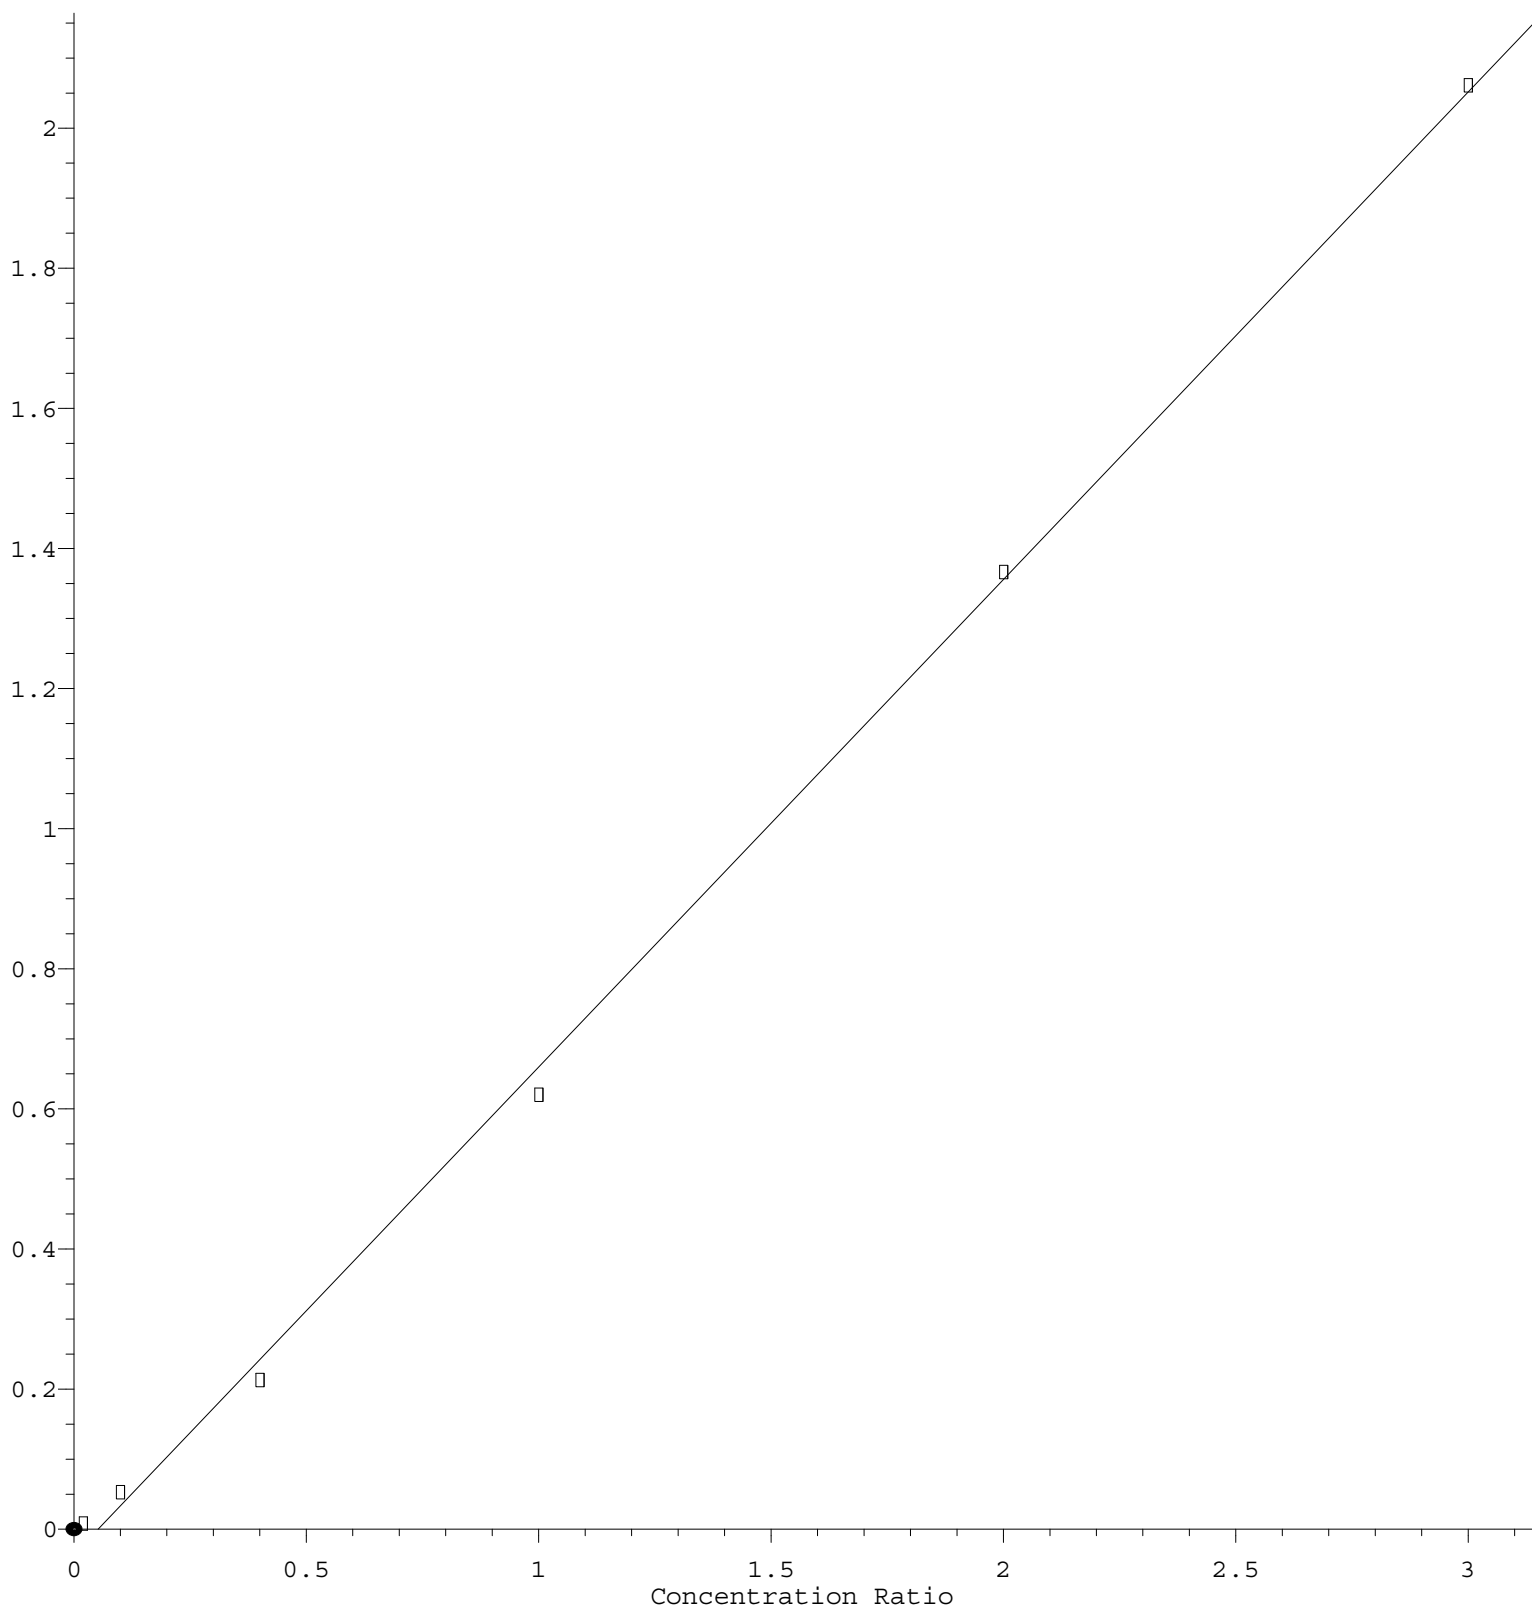

$$\text{Response} = 6.959\text{e-}001 * \text{Amt} - 3.603\text{e-}002$$


Coef of Det (r^2) = 0.998858 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

Ethyl methacrylate

Response Ratio

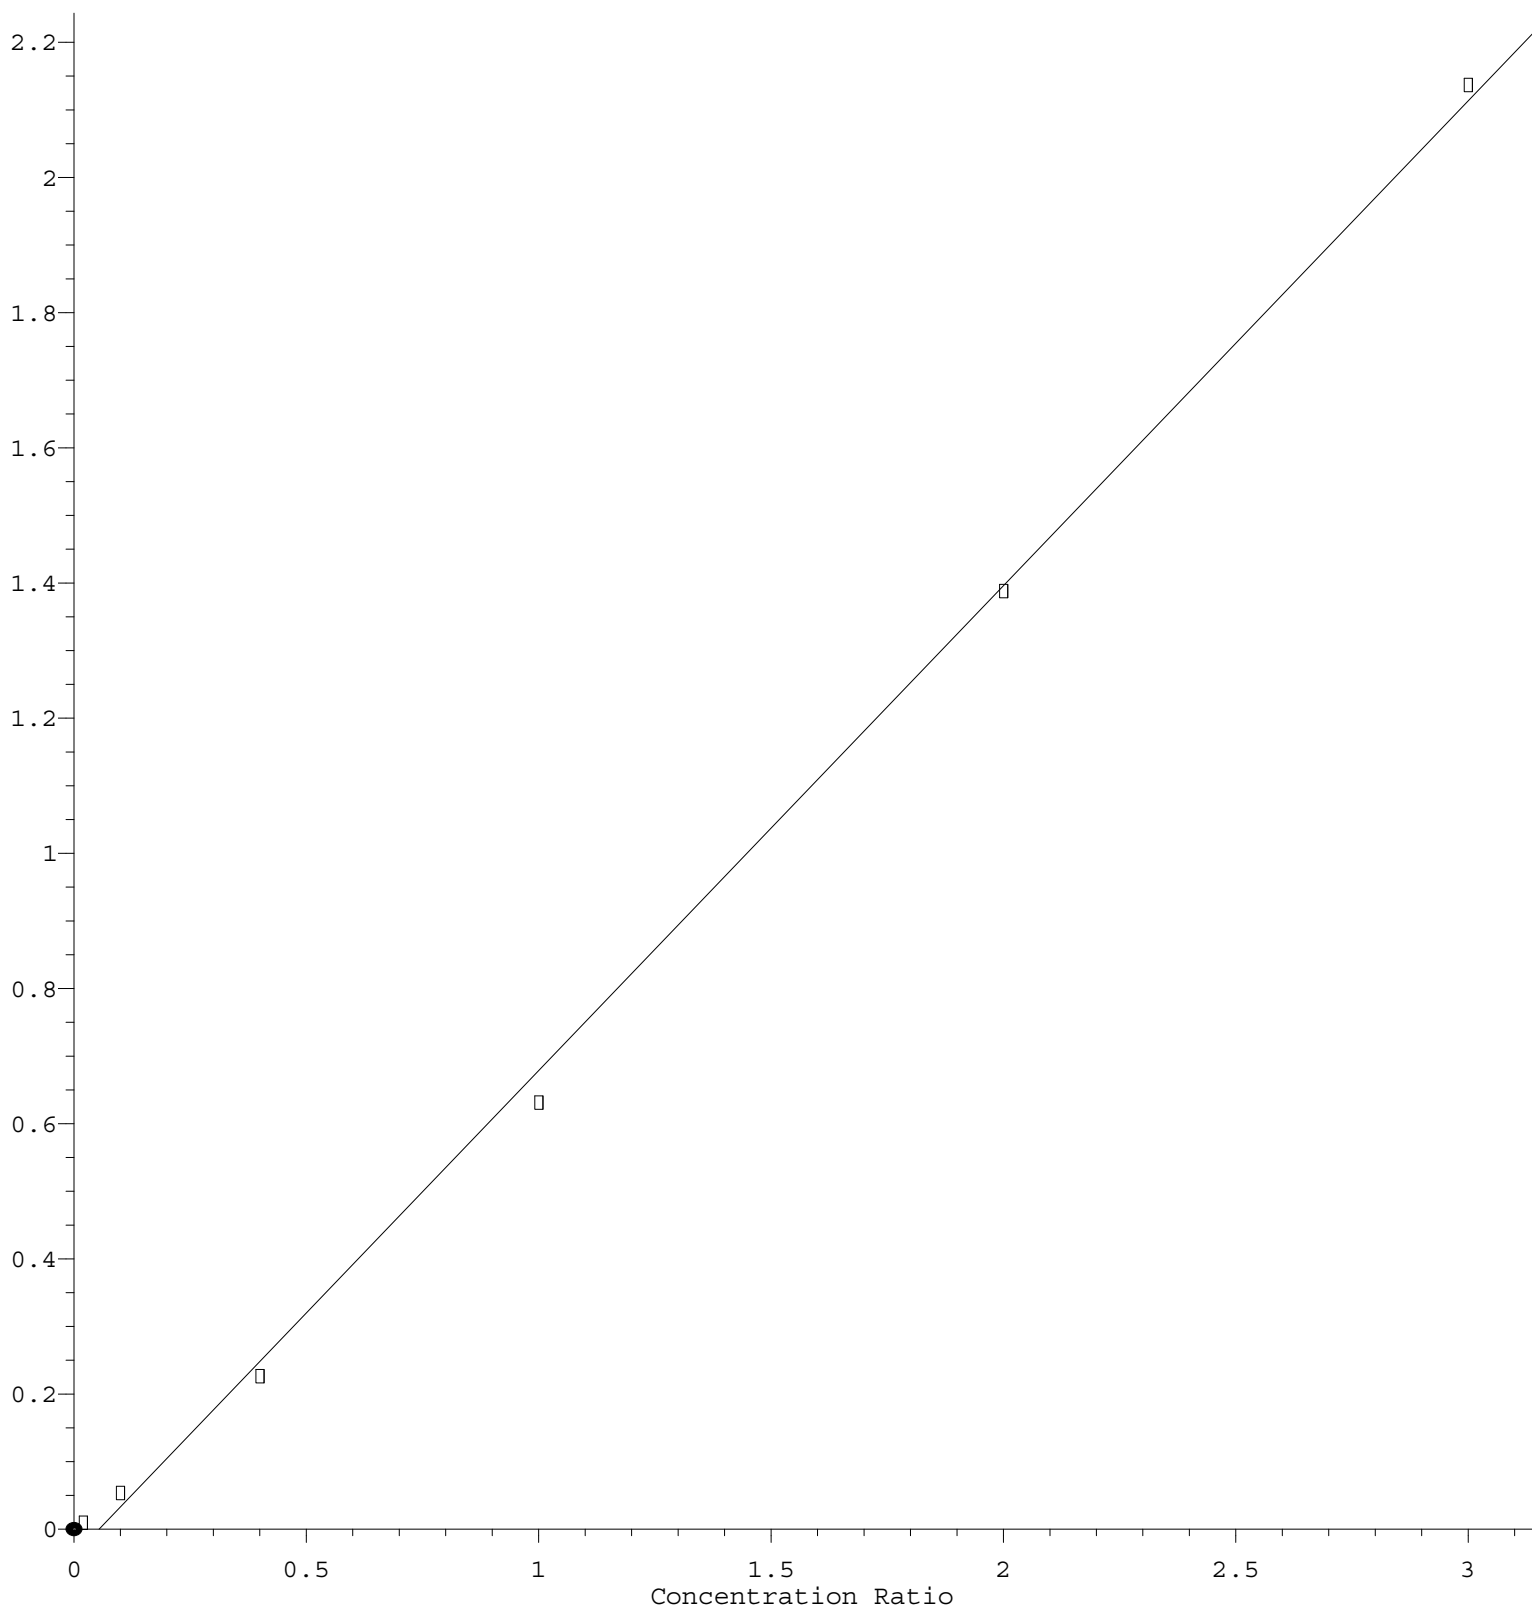

$$\text{Response} = 7.174\text{e-}001 * \text{Amt} - 3.875\text{e-}002$$


Coef of Det (r^2) = 0.998649 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021

Dibromochloromethane

Response Ratio

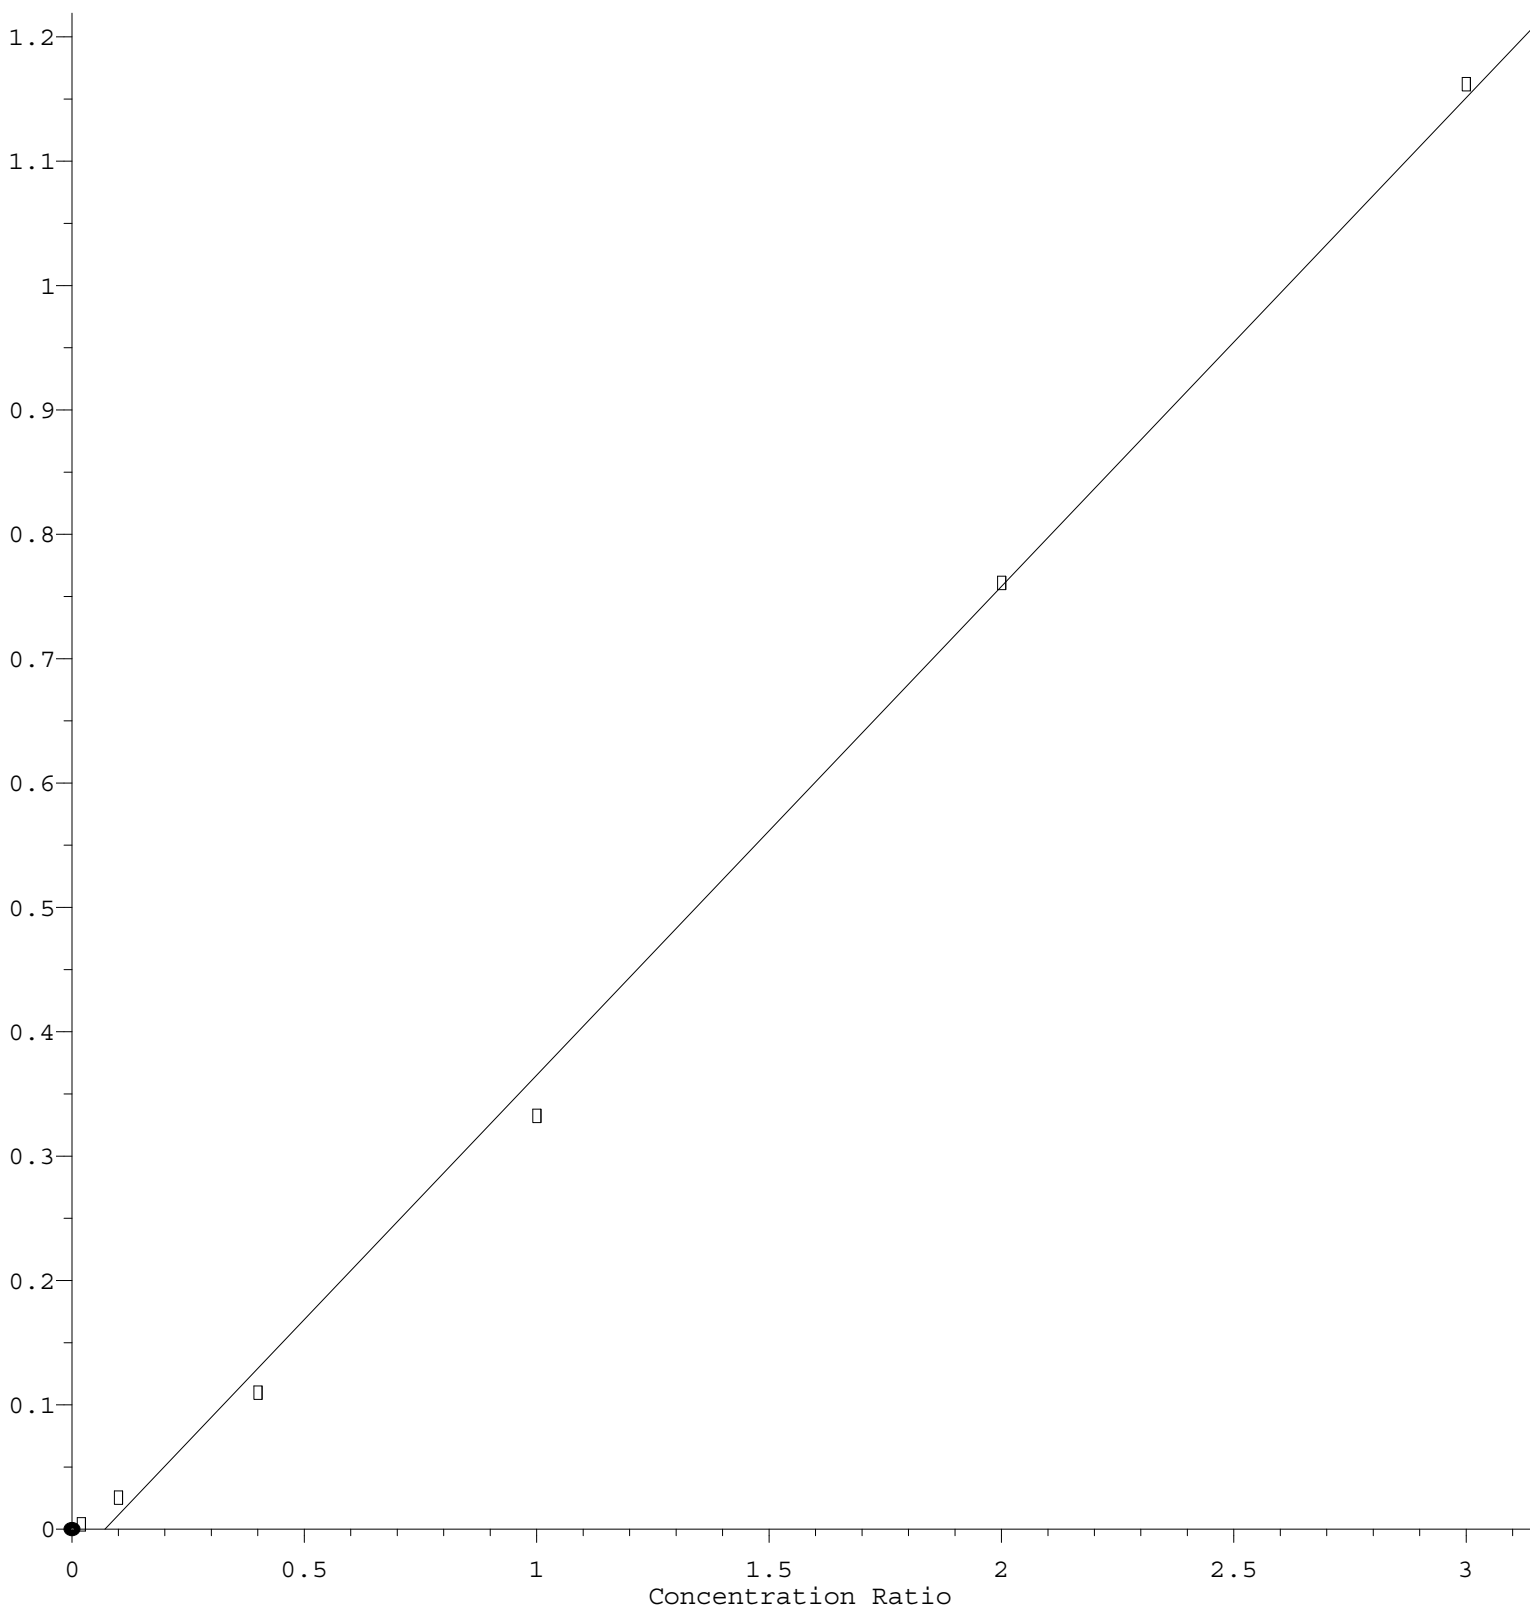

$$\text{Response} = 3.930\text{e-}001 * \text{Amt} - 2.808\text{e-}002$$

Coef of Det (r^2) = 0.997858 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060721W.M

Calibration Table Last Updated: Mon Jun 07 14:27:50 2021