


Chloroethane


Response Ratio

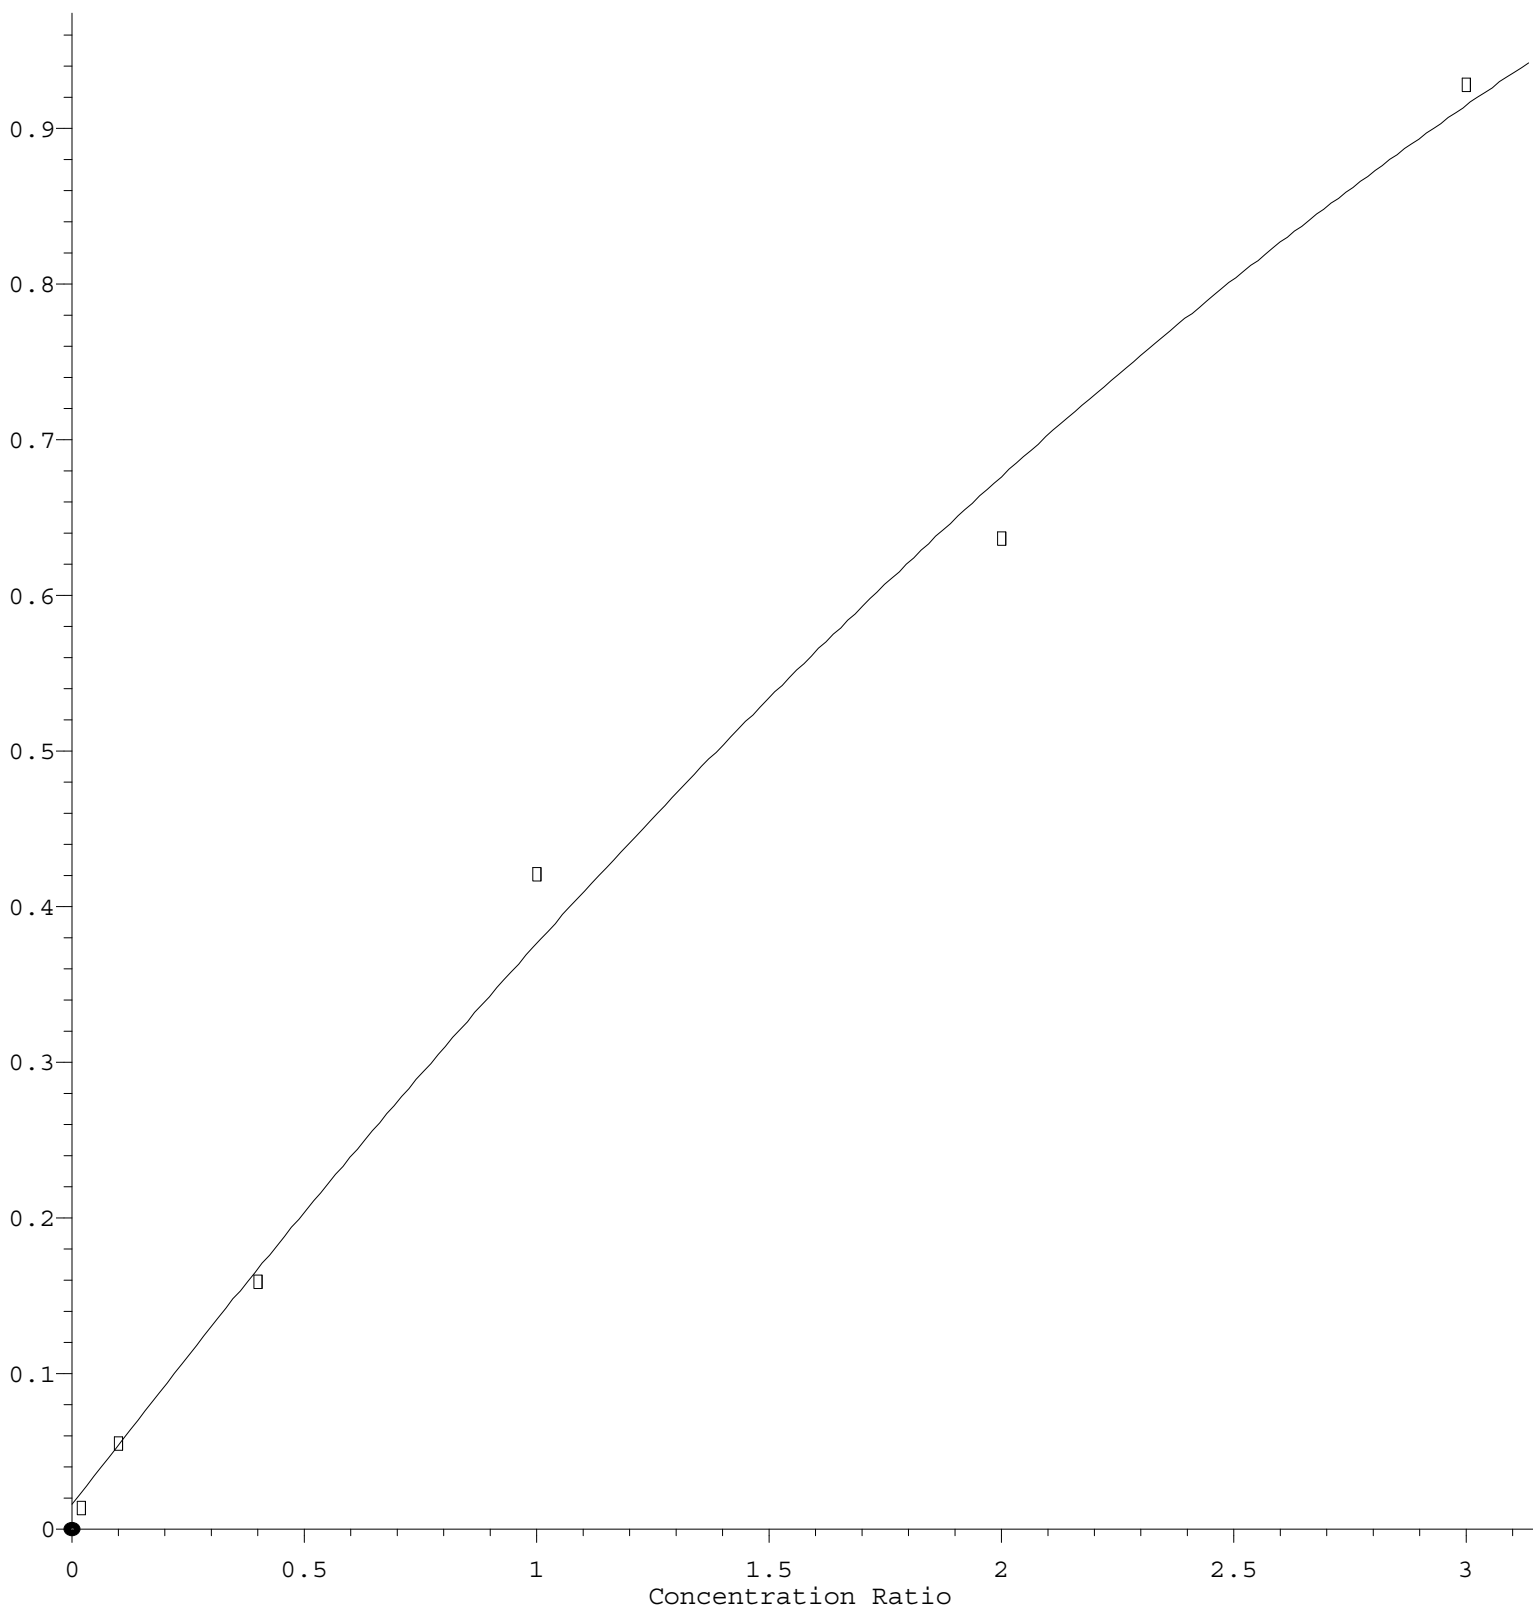

$R = -3.055e-002 A^2 + 3.915e-001 A + 1.554e-002$
 Coef of Det (r^2) = 0.994079 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060722W.M
 Calibration Table Last Updated: Wed Jun 08 03:00:38 2022

Methyl Iodide

Response Ratio

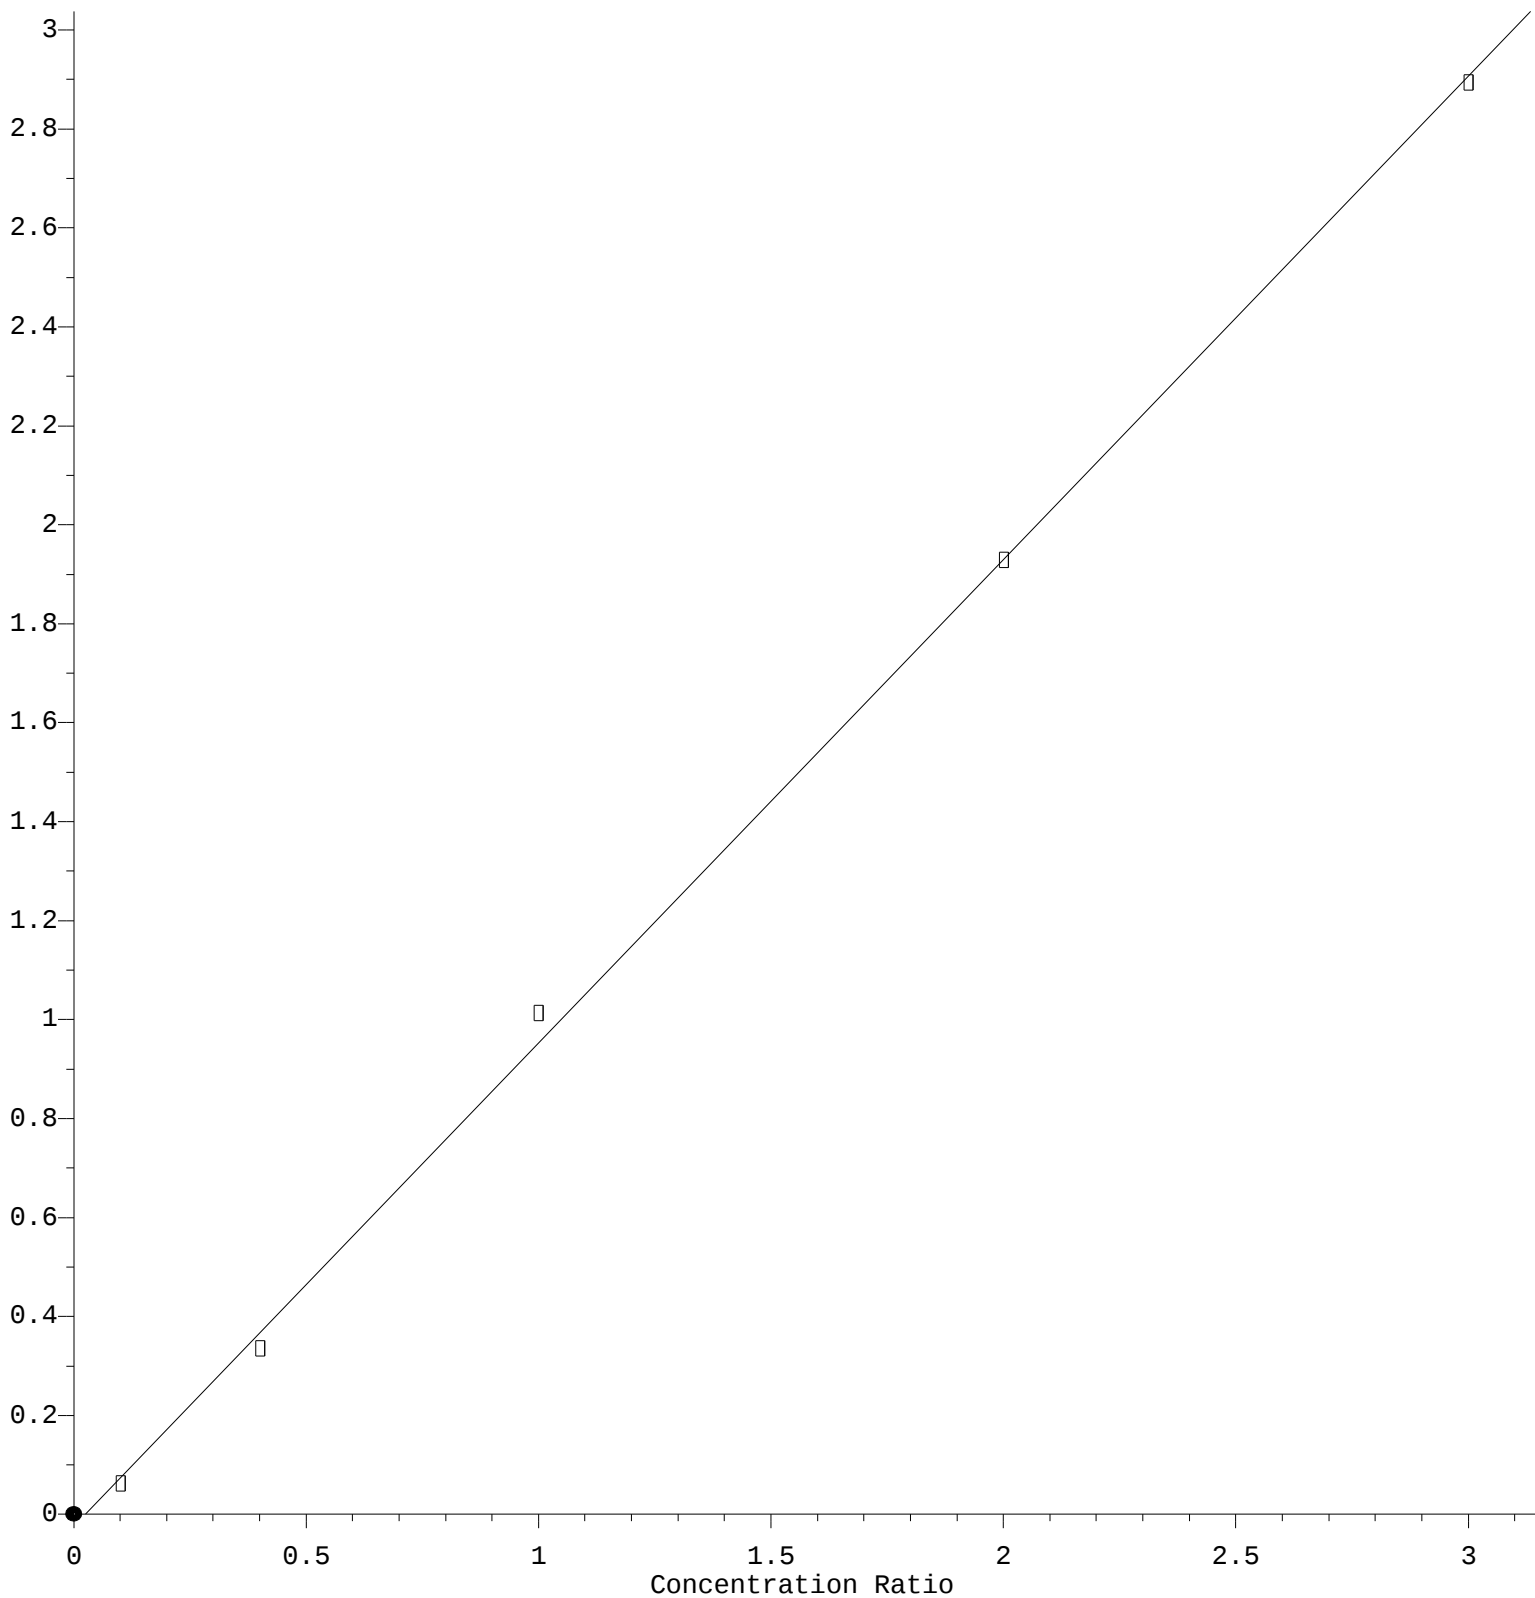

$$\text{Response} = 9.771\text{e-}001 * \text{Amt} - 2.414\text{e-}002$$


Coef of Det (r^2) = 0.999110 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M

Calibration Table Last Updated: Wed Jun 08 03:00:38 2022

Tert butyl alcohol

Response Ratio

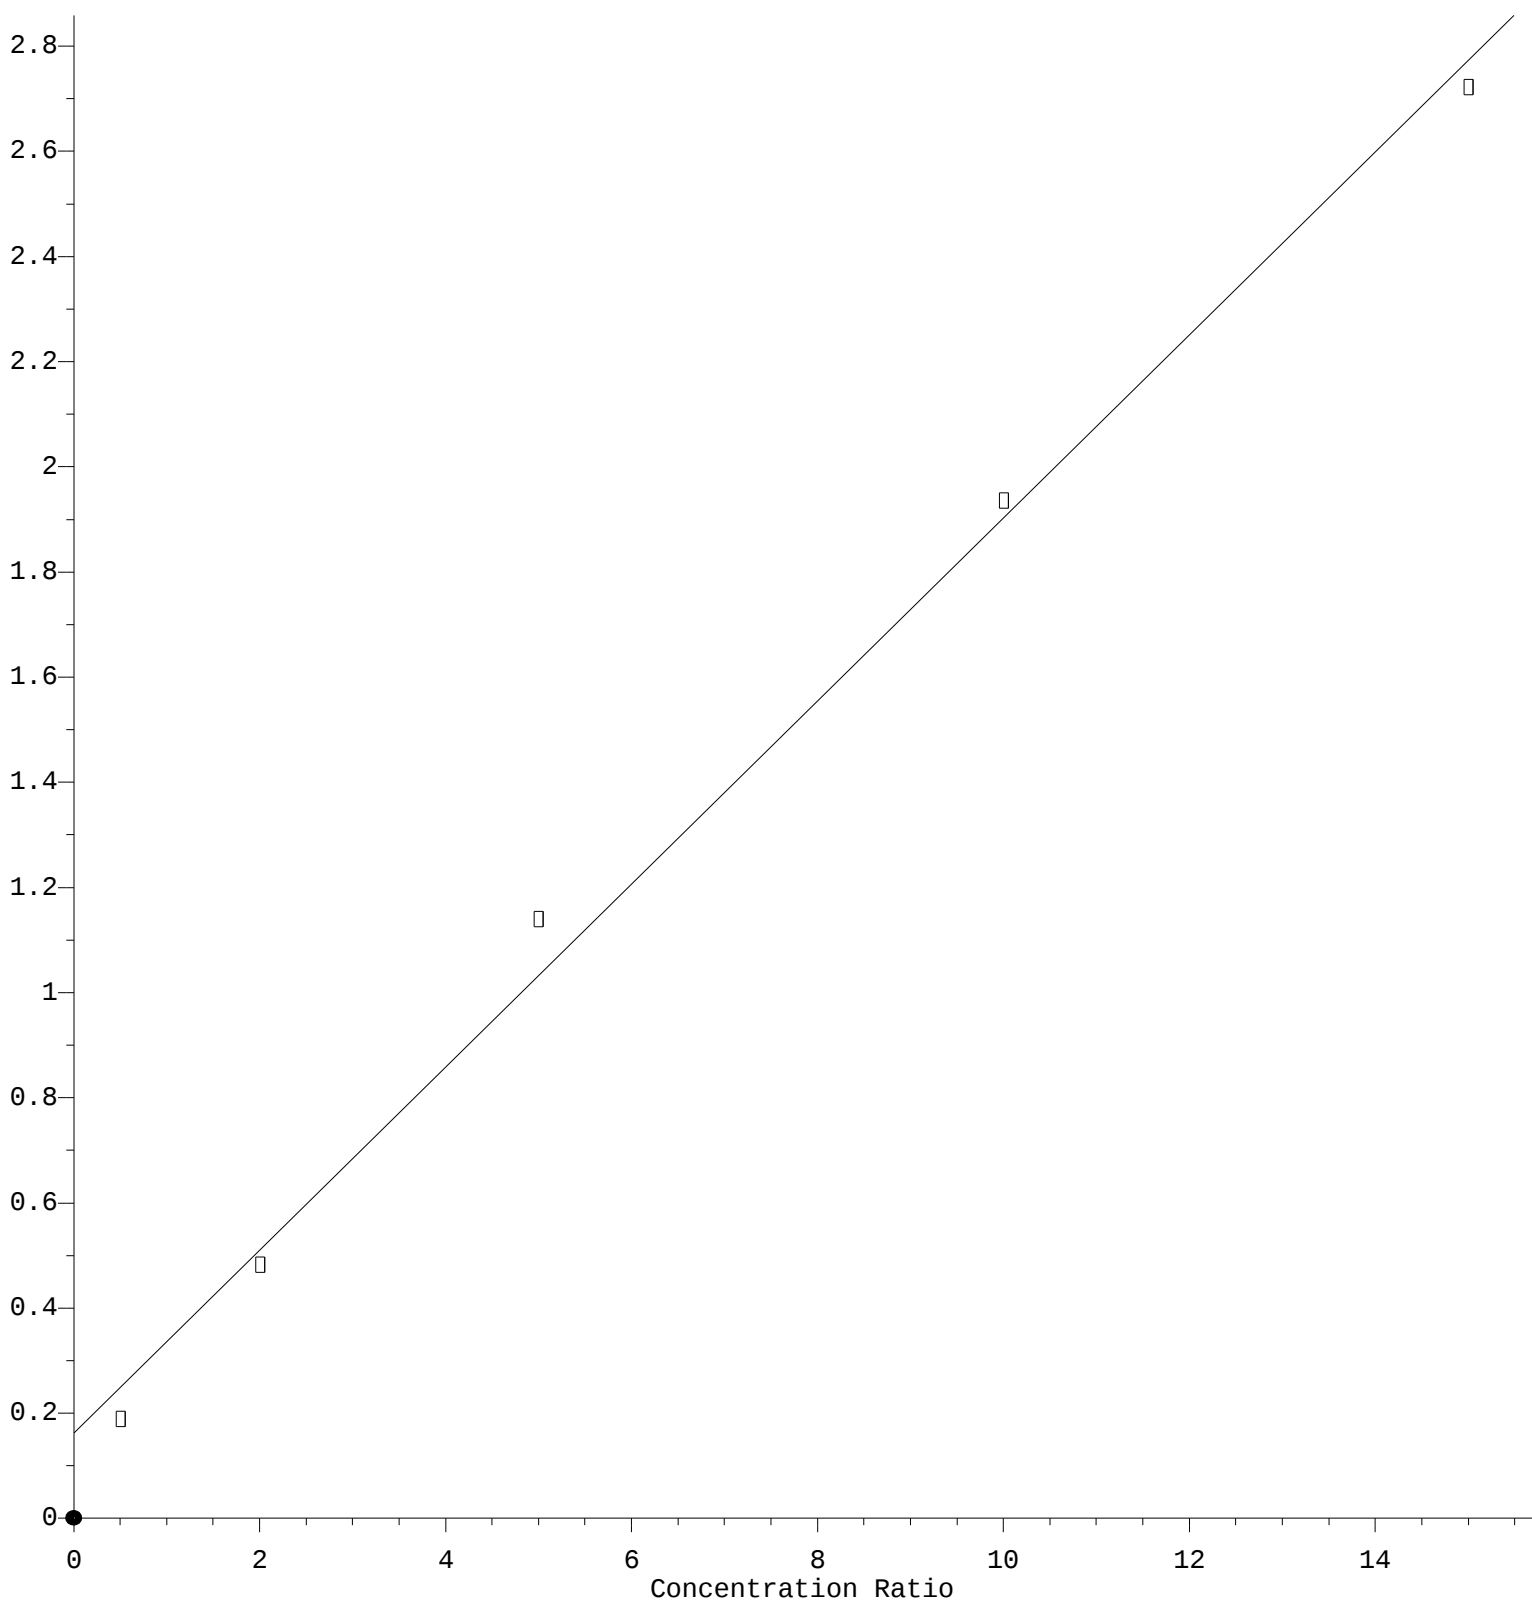

$$\text{Response} = 1.741\text{e-}001 * \text{Amt} + 1.618\text{e-}001$$


Coef of Det (r^2) = 0.995539 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M

Calibration Table Last Updated: Wed Jun 08 03:00:38 2022

1,2-Dichloroethane-d4

Response Ratio

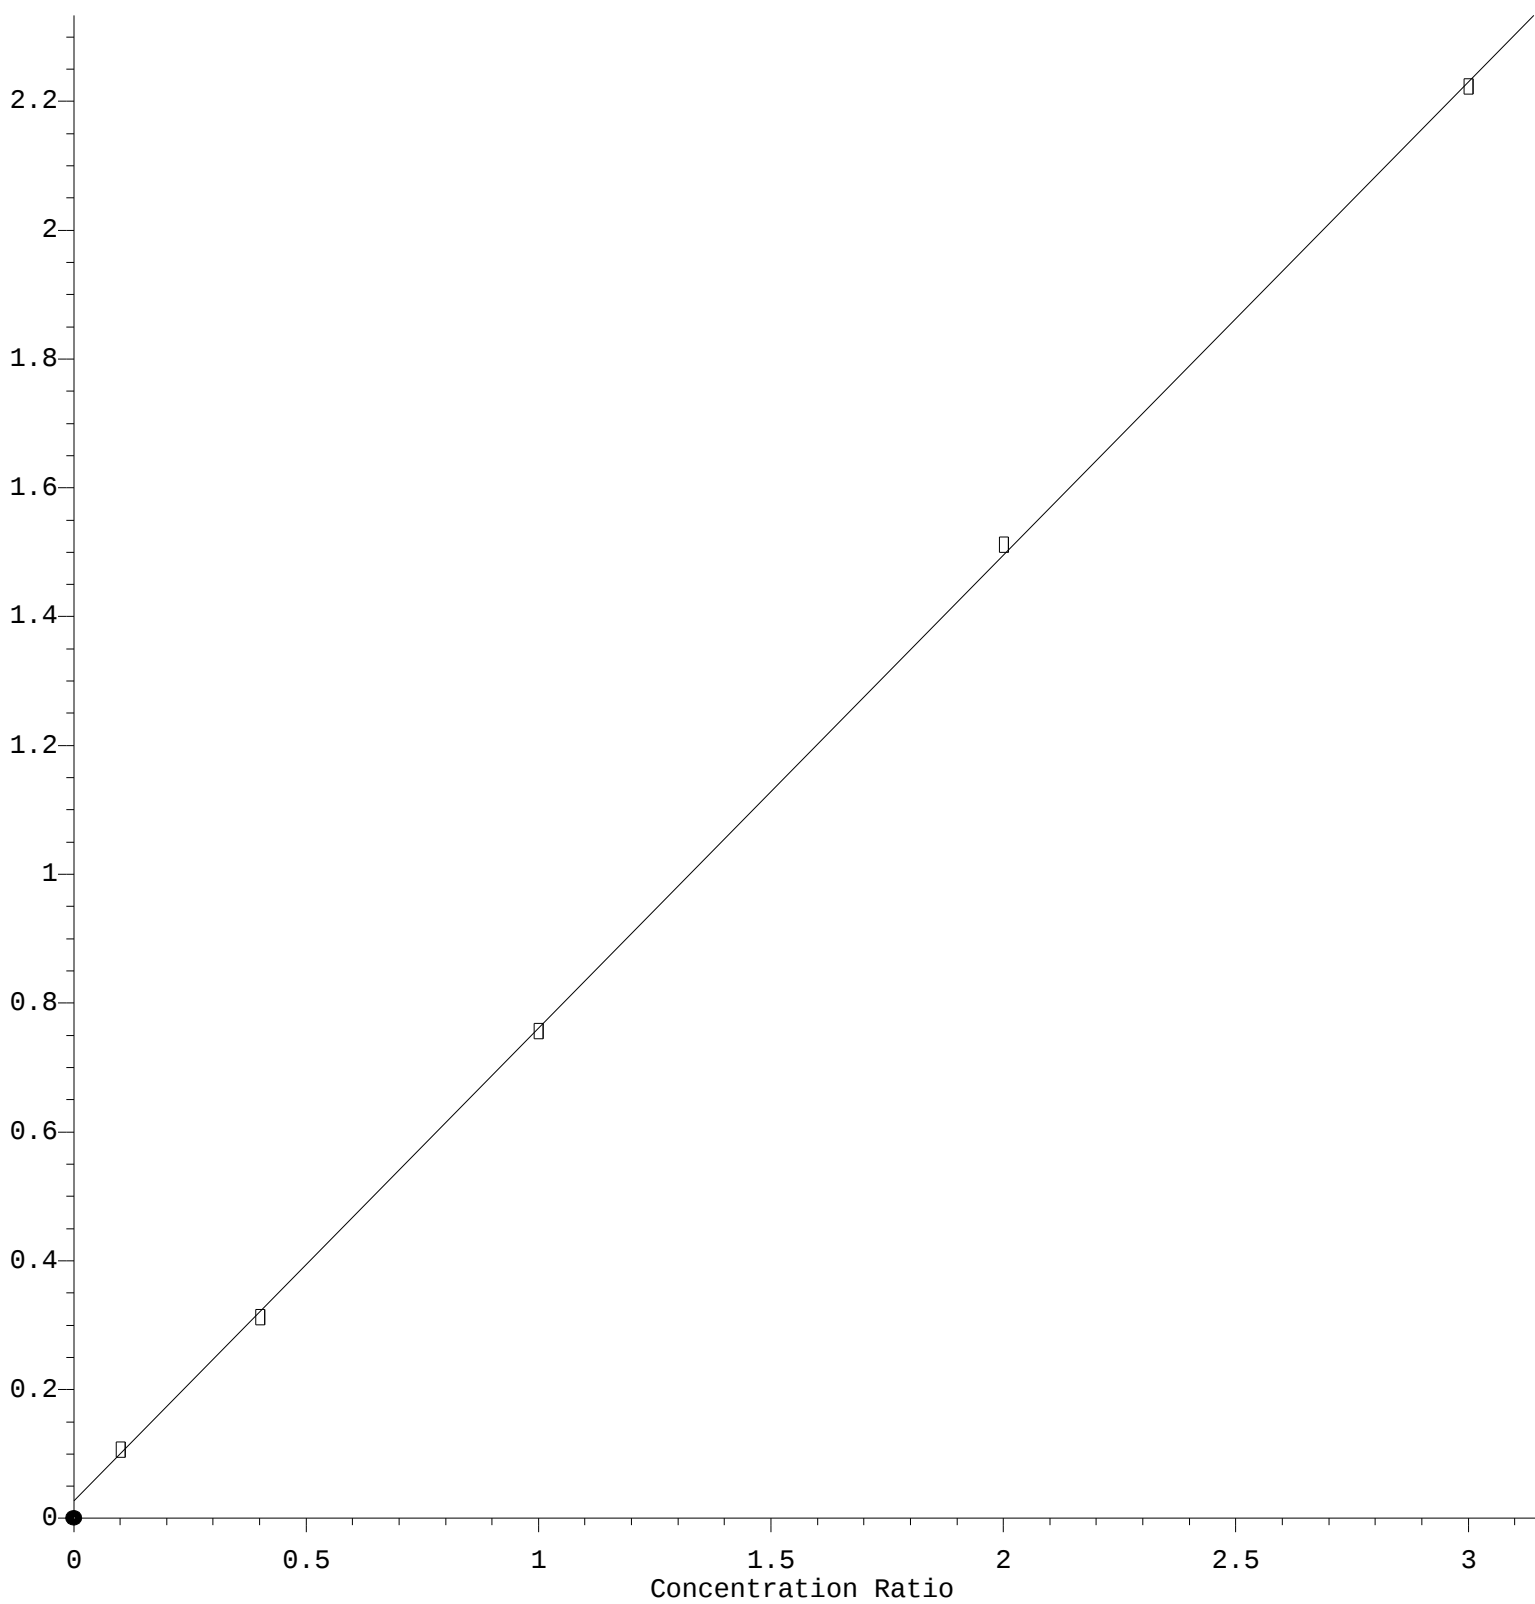

$$\text{Response} = 7.344\text{e-}001 * \text{Amt} + 2.670\text{e-}002$$


Coef of Det (r^2) = 0.999859 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M

Calibration Table Last Updated: Wed Jun 08 03:00:38 2022

Methacrylonitrile

Response Ratio

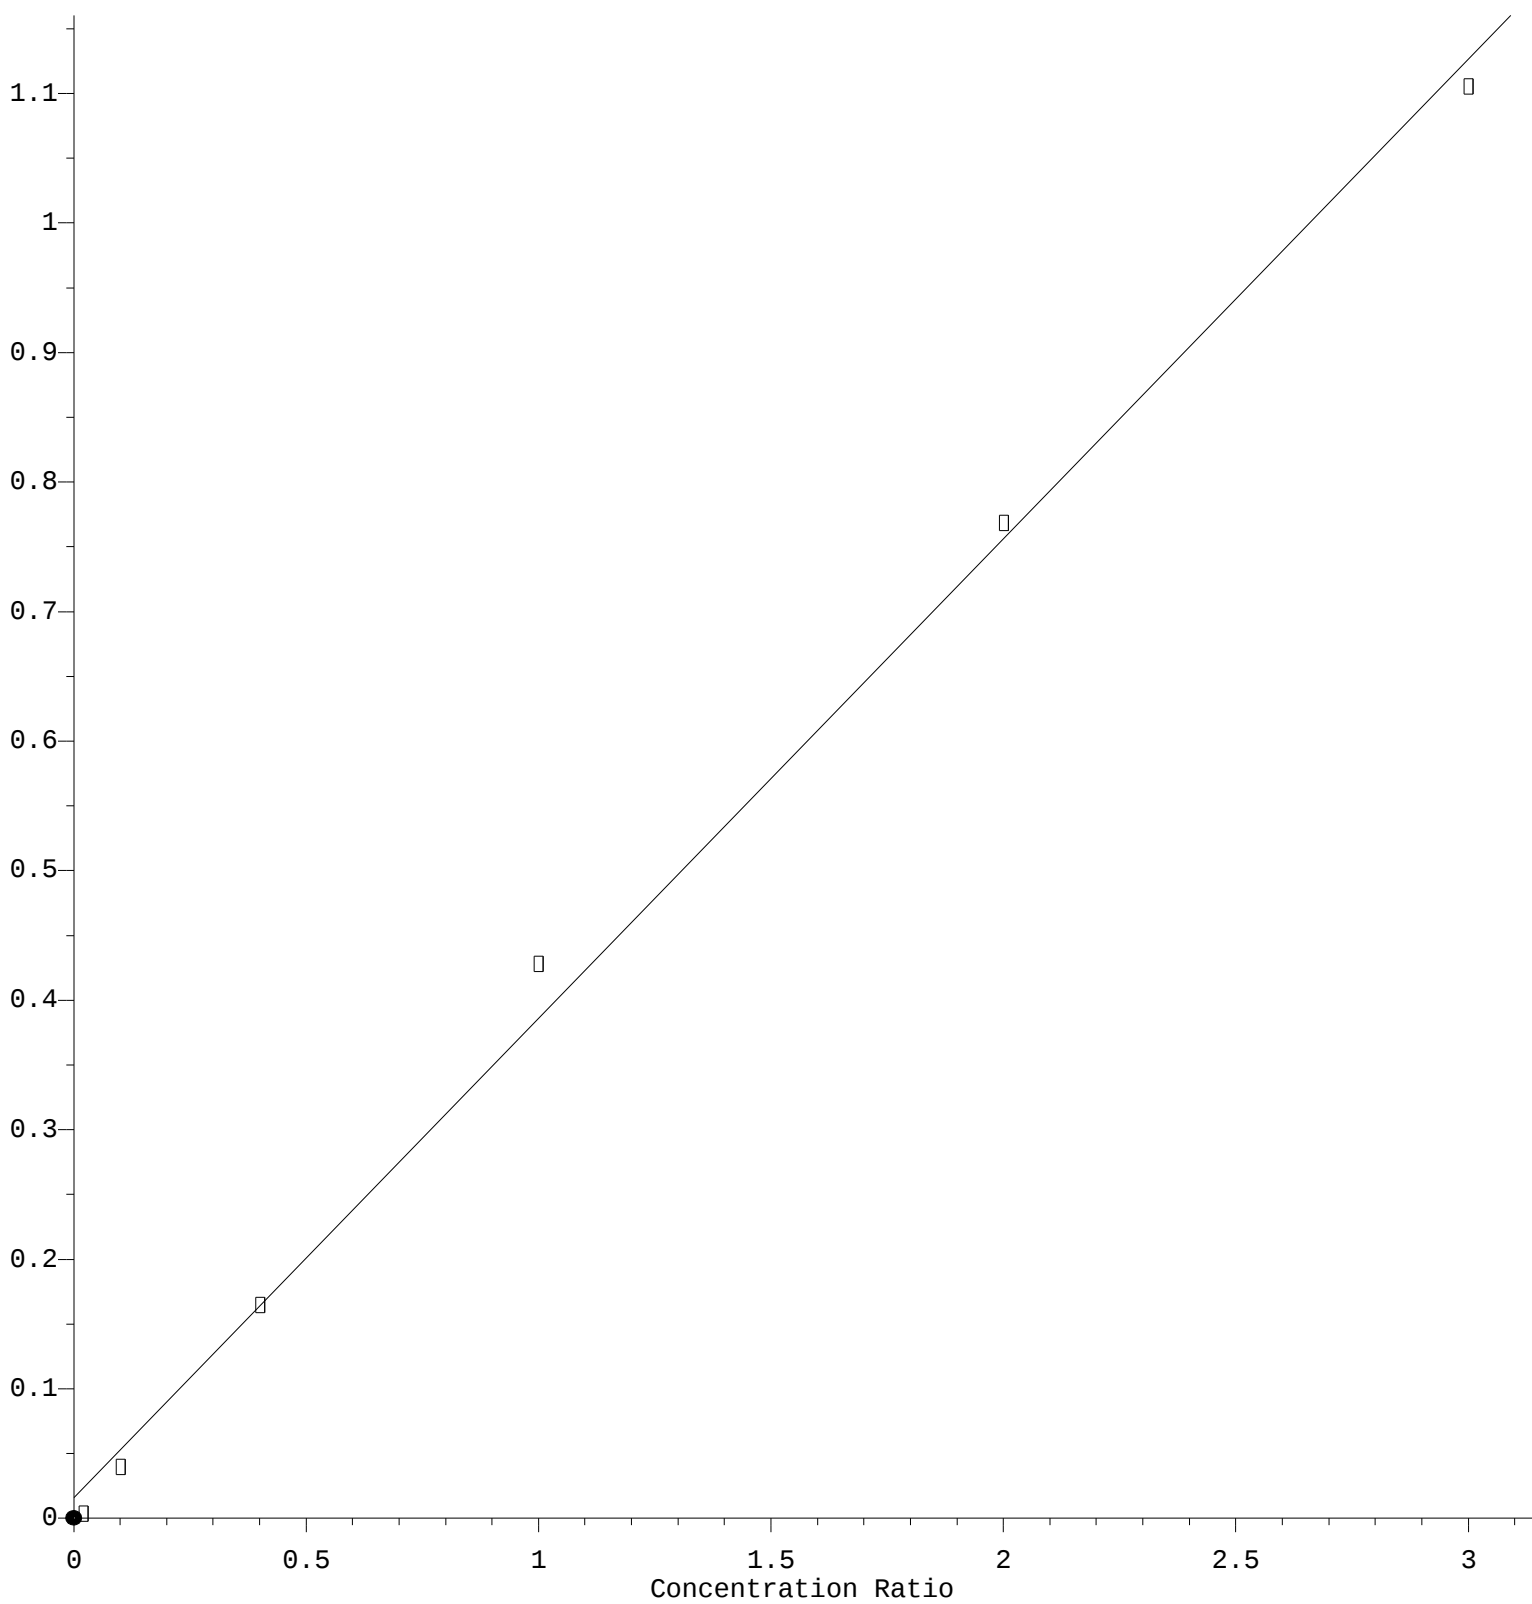

$$\text{Response} = 3.702\text{e-}001 * \text{Amt} + 1.578\text{e-}002$$


Coef of Det (r^2) = 0.996982 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M

Calibration Table Last Updated: Wed Jun 08 03:00:38 2022

t-1,3-Dichloropropene

Response Ratio

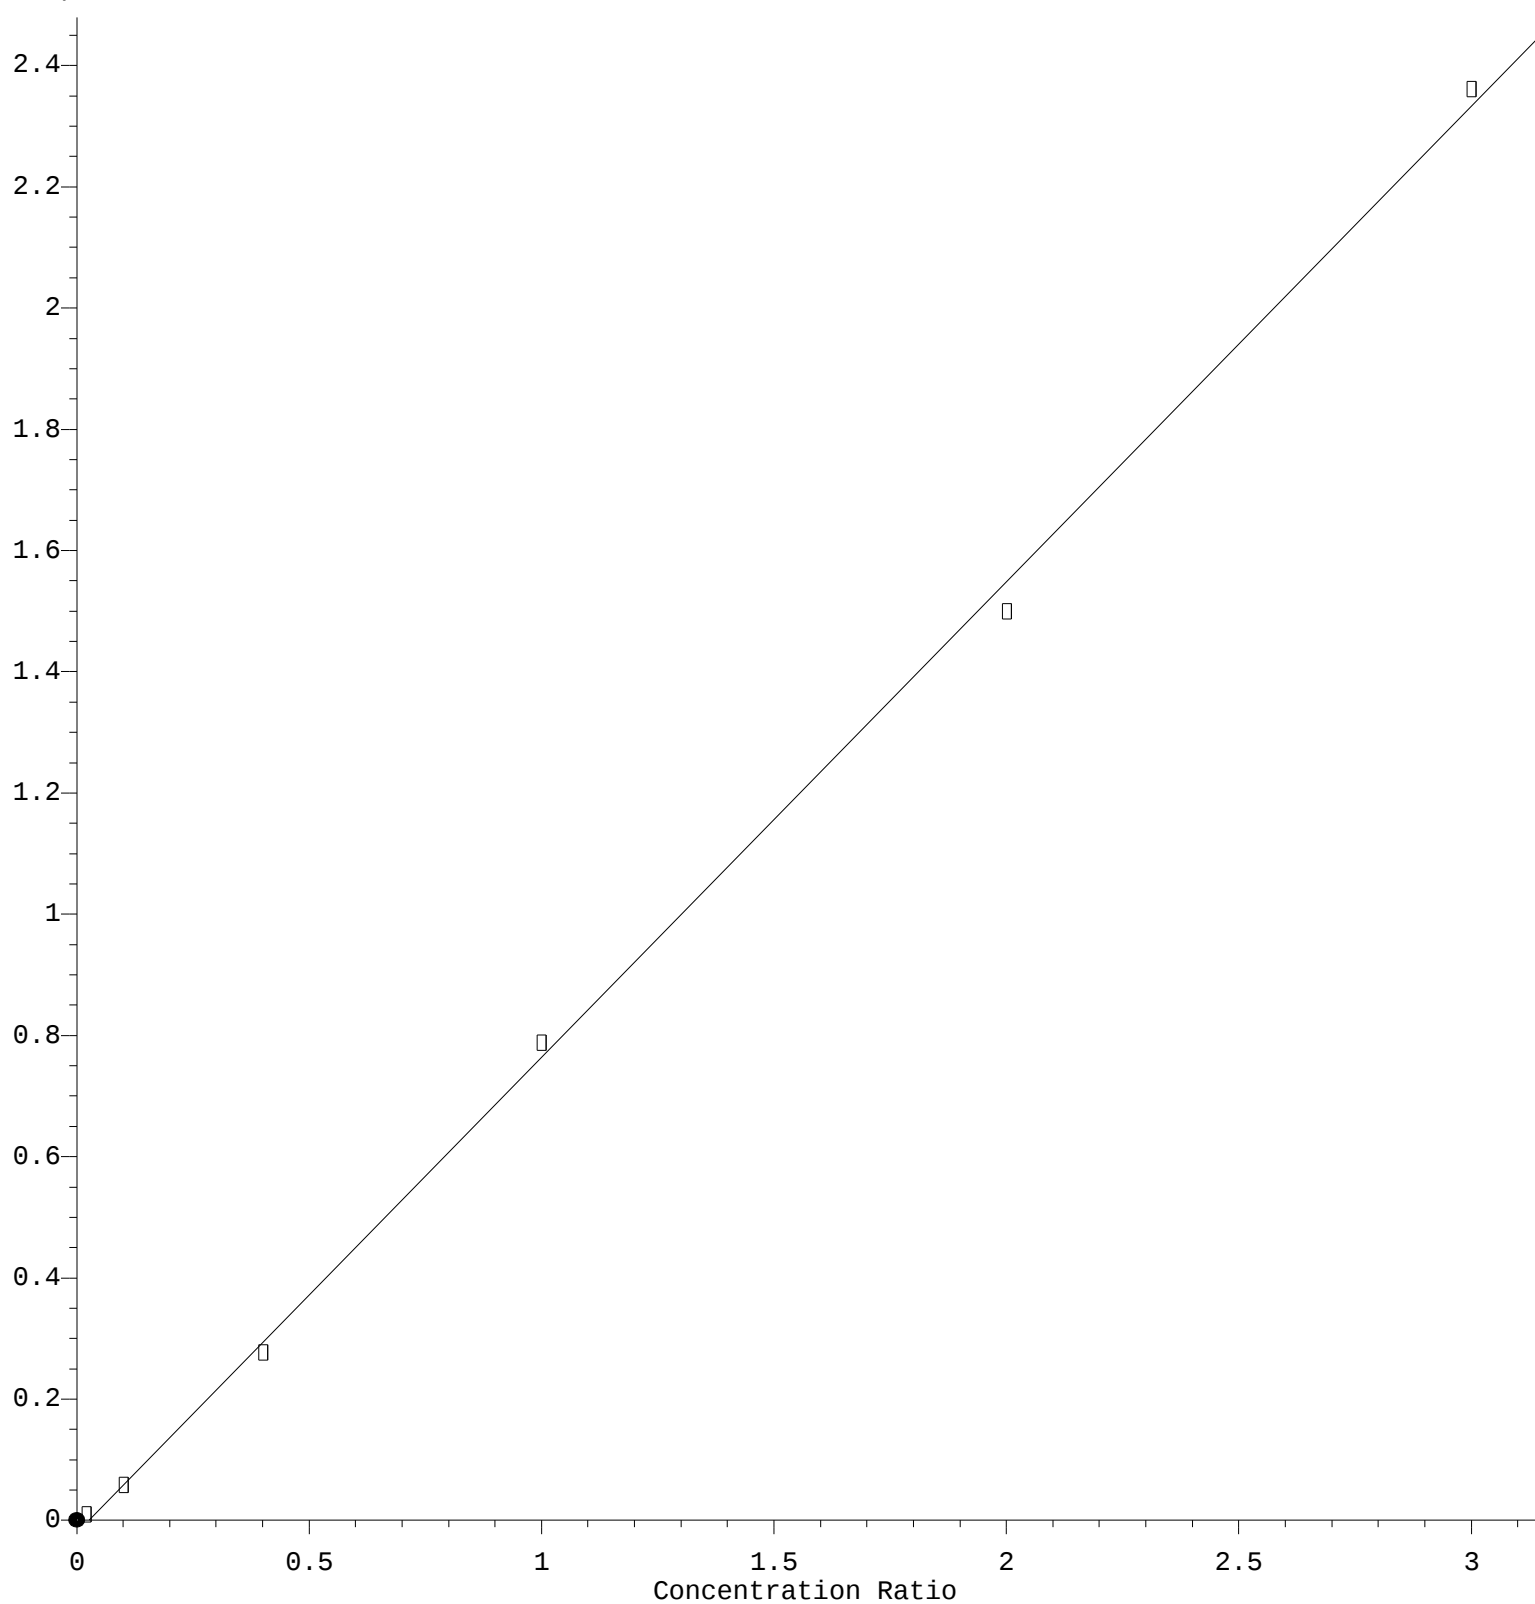

$$\text{Response} = 7.847\text{e-}001 * \text{Amt} - 2.066\text{e-}002$$


Coef of Det (r^2) = 0.999016 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M

Calibration Table Last Updated: Wed Jun 08 03:00:38 2022

trans-1,4-Dichloro-2-butene

Response Ratio

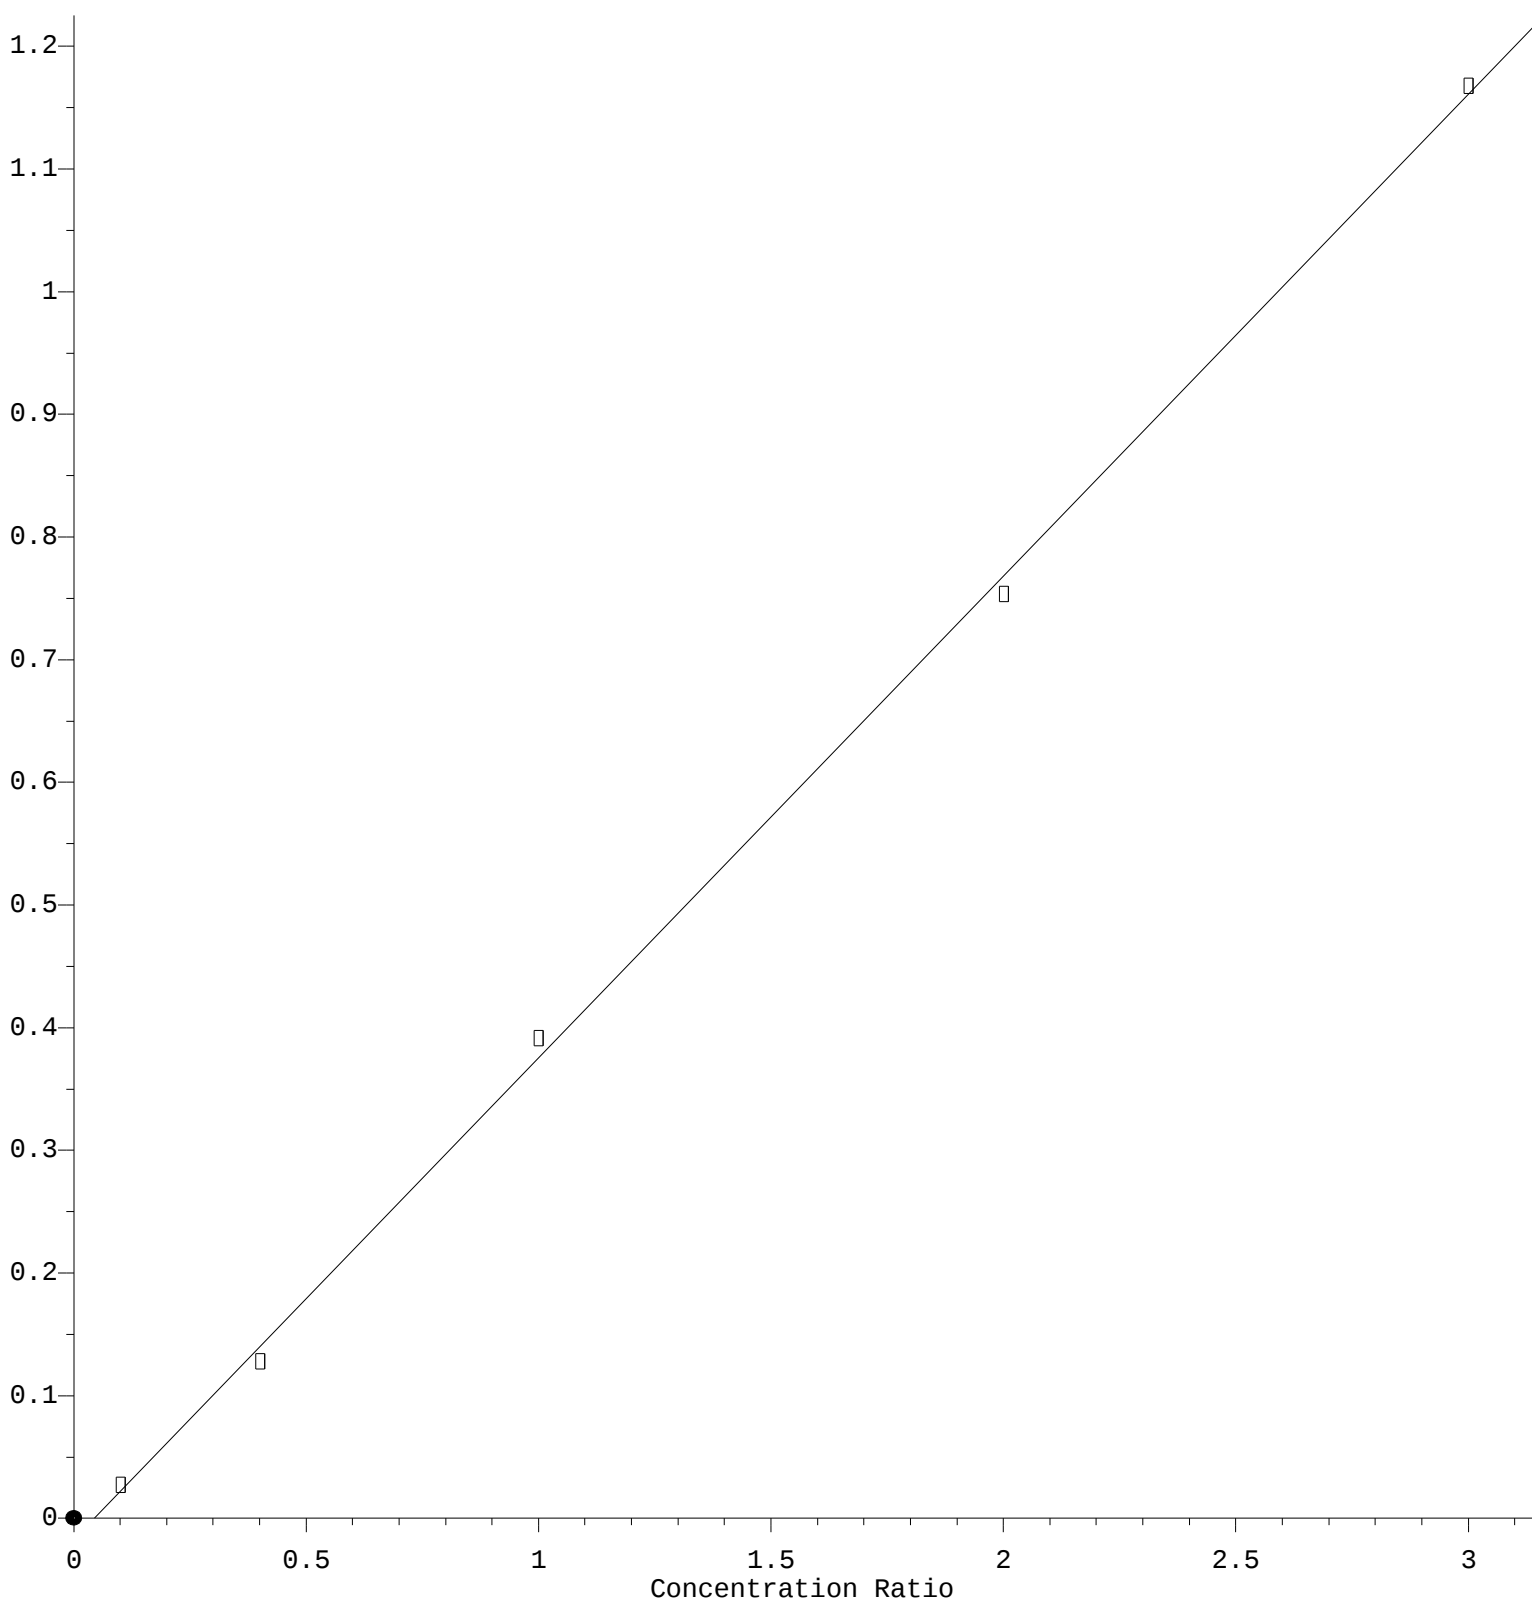

$$\text{Response} = 3.928\text{e-}001 * \text{Amt} - 1.730\text{e-}002$$

Coef of Det (r^2) = 0.999216 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M

Calibration Table Last Updated: Wed Jun 08 03:00:38 2022