

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060723\
 Data File : VX036054.D
 Acq On : 07 Jun 2023 12:36
 Operator : JC/MD
 Sample : VX0607WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0607WBL01

Quant Time: Jun 08 07:22:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Tue May 23 11:36:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	4.903	128	40924	30.000	ug/l	0.01
28) 1,4-Difluorobenzene	6.757	114	231968	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	204142	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.952	65	108561	31.926	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	106.433%
60) 4-Bromofluorobenzene	11.079	95	104803	30.595	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	102.000%
63) Toluene-d8	8.647	98	271752	30.112	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	100.367%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060723\
Data File : VX036054.D
Acq On : 07 Jun 2023 12:36
Operator : JC/MD
Sample : VX0607WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0607WBL01

Quant Time: Jun 08 07:22:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X052323W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Tue May 23 11:36:37 2023
Response via : Initial Calibration




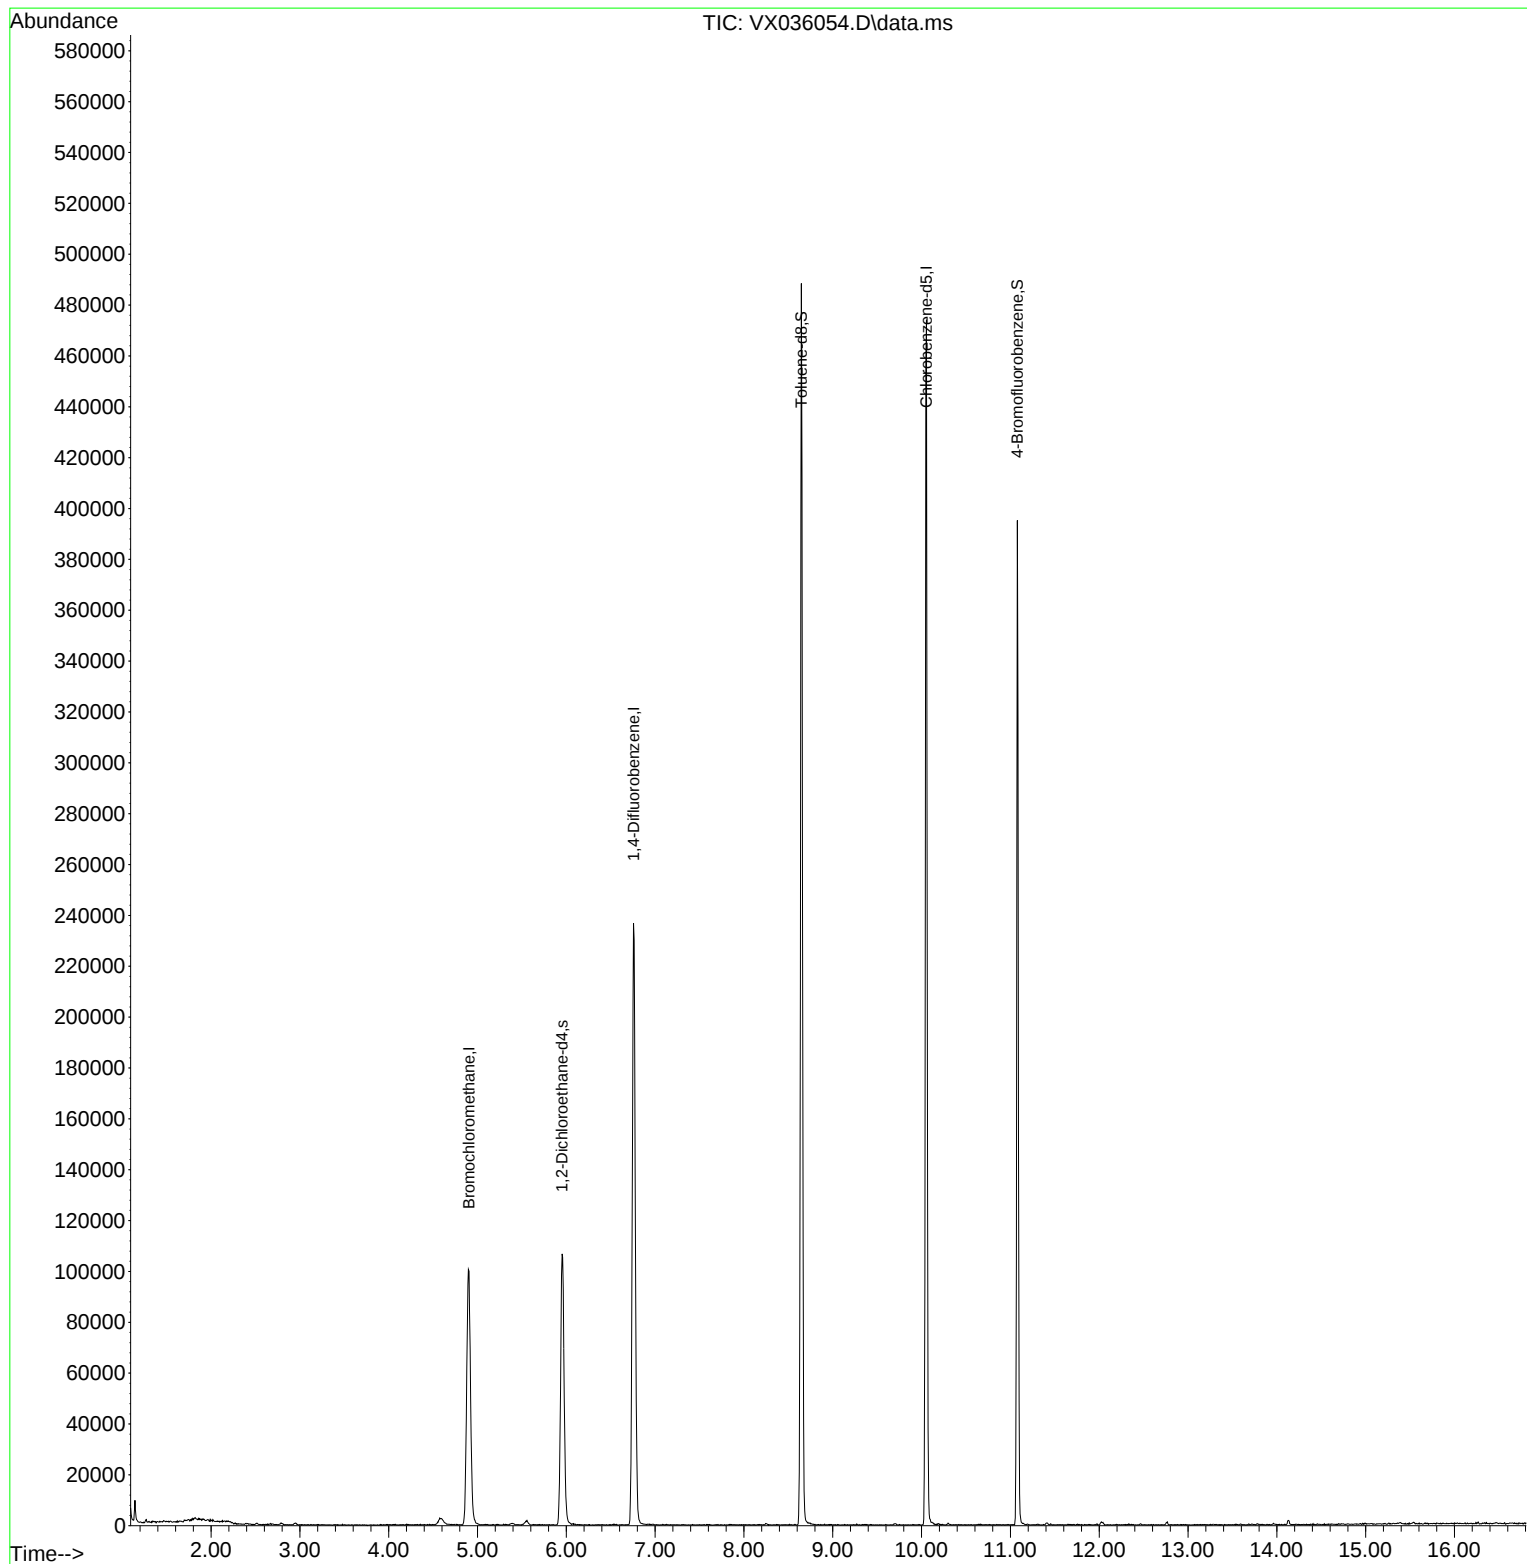


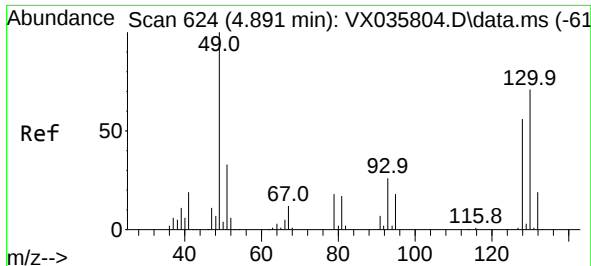

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.903 min Scan# 61
Delta R.T. 0.012 min
Lab File: VX036054.D
Acq: 07 Jun 2023 12:36




Instrument :
MSVOA_X
ClientSampleId :
VX0607WBL01


Tgt Ion:128 Resp: 40924
Ion Ratio Lower Upper
128 100
49 175.7 0.0 428.8
130 128.2 0.0 310.8

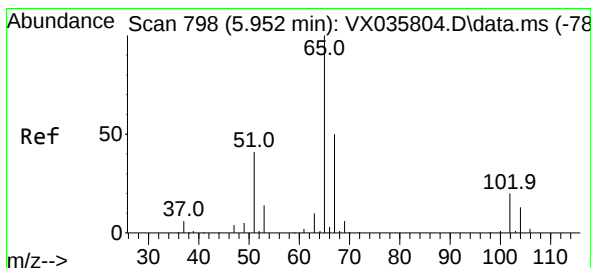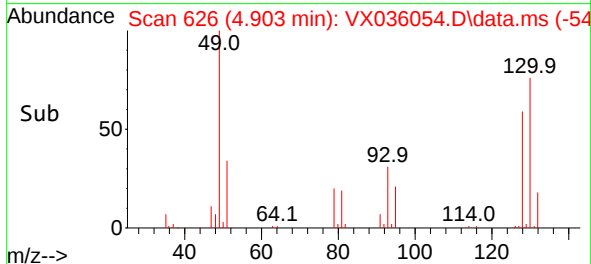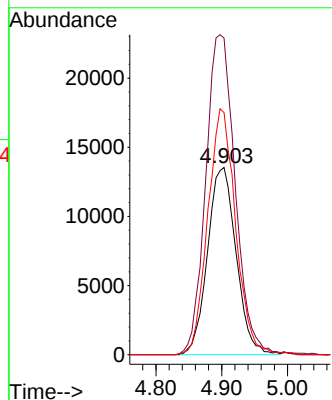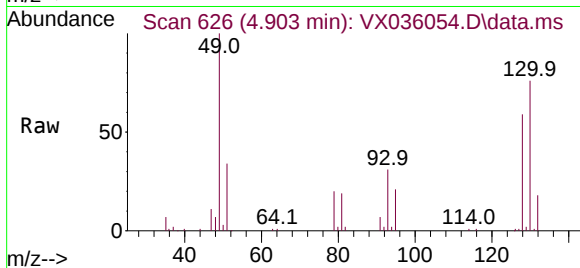

#27
1,2-Dichloroethane-d4
Concen: 31.926 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX036054.D
Acq: 07 Jun 2023 12:36

Tgt Ion: 65 Resp: 108561
Ion Ratio Lower Upper
65 100
67 50.8 40.9 61.3

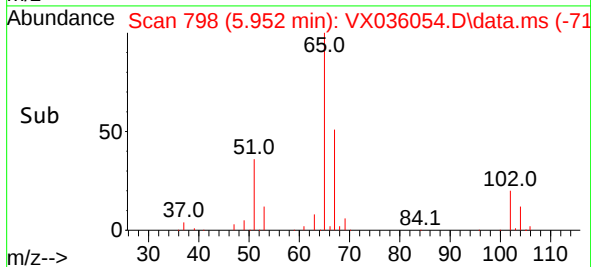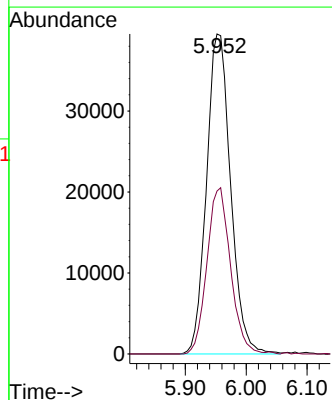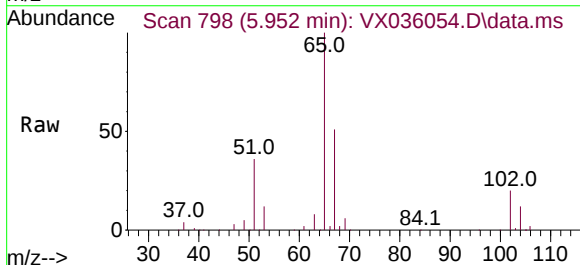




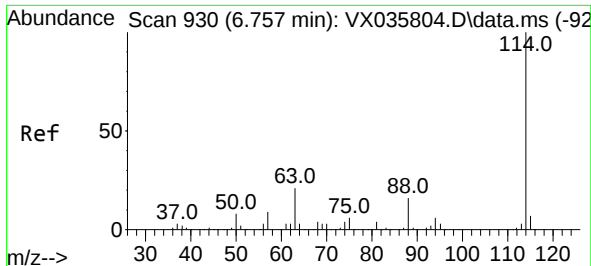


#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 6.757 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: VX036054.D
 Acq: 07 Jun 2023 12:36

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0607WBL01

Tgt Ion:114 Resp: 231968




Ion	Ratio	Lower	Upper
114	100		
63	22.1	18.0	27.0
88	17.2	13.3	19.9

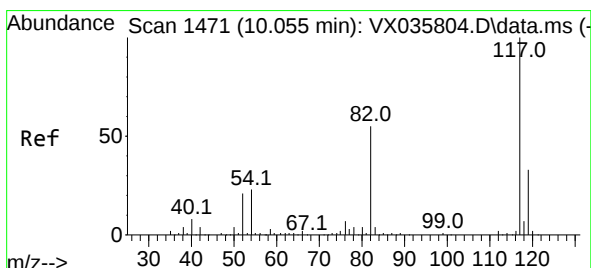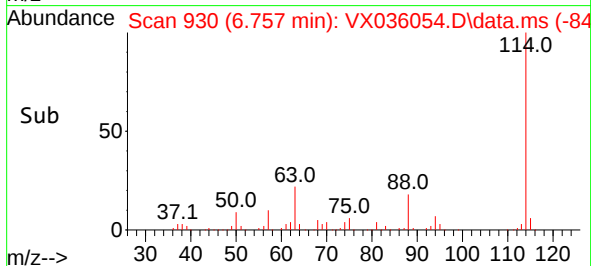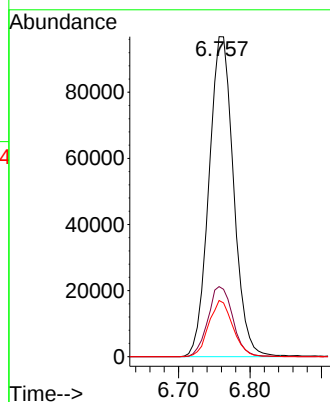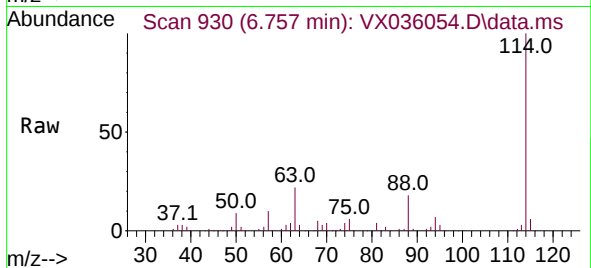


#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 10.055 min Scan# 1471
 Delta R.T. -0.000 min
 Lab File: VX036054.D
 Acq: 07 Jun 2023 12:36

Tgt Ion:117 Resp: 204142

Ion	Ratio	Lower	Upper
117	100		
82	59.8	45.8	68.8
119	31.6	25.4	38.0


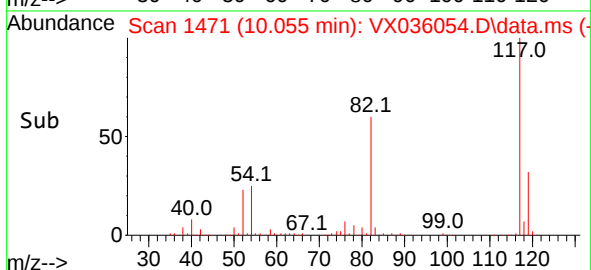
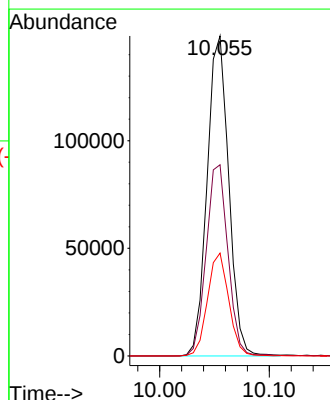
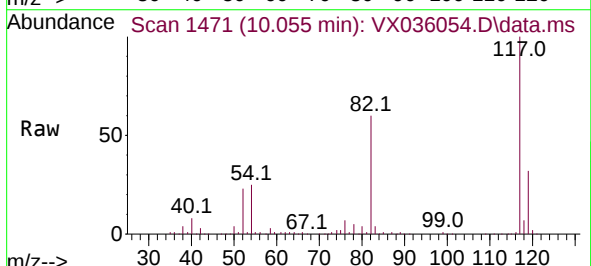


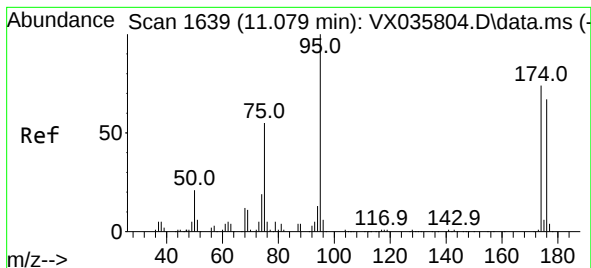

#60
4-Bromofluorobenzene
Concen: 30.595 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX036054.D
Acq: 07 Jun 2023 12:36

Instrument :
MSVOA_X
ClientSampleId :
VX0607WBL01

Tgt Ion: 95 Resp: 104803
Ion Ratio Lower Upper
95 100
174 65.7 0.2 0.4#
176 63.3 0.2 0.2#

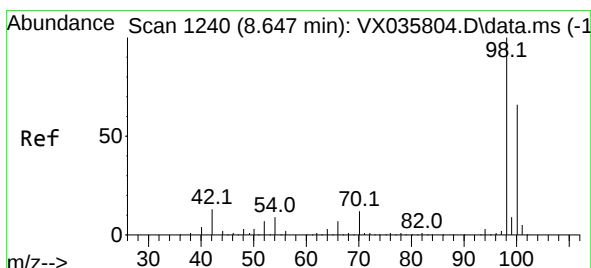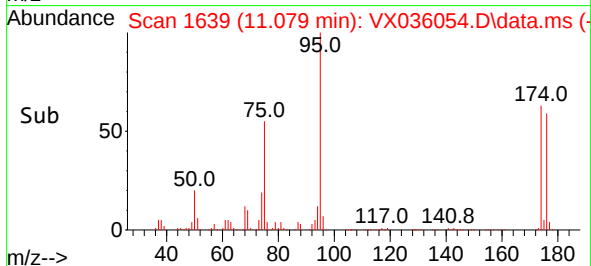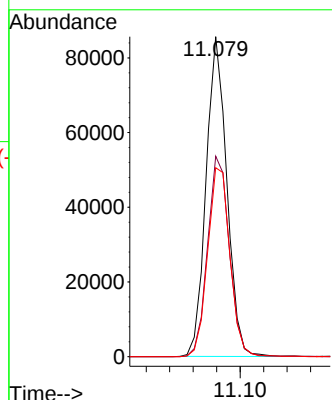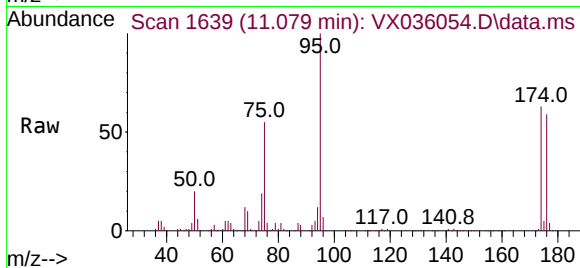

#63
Toluene-d8
Concen: 30.112 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX036054.D
Acq: 07 Jun 2023 12:36

Tgt Ion: 98 Resp: 271752
Ion Ratio Lower Upper
98 100
100 66.5 52.1 78.1

