
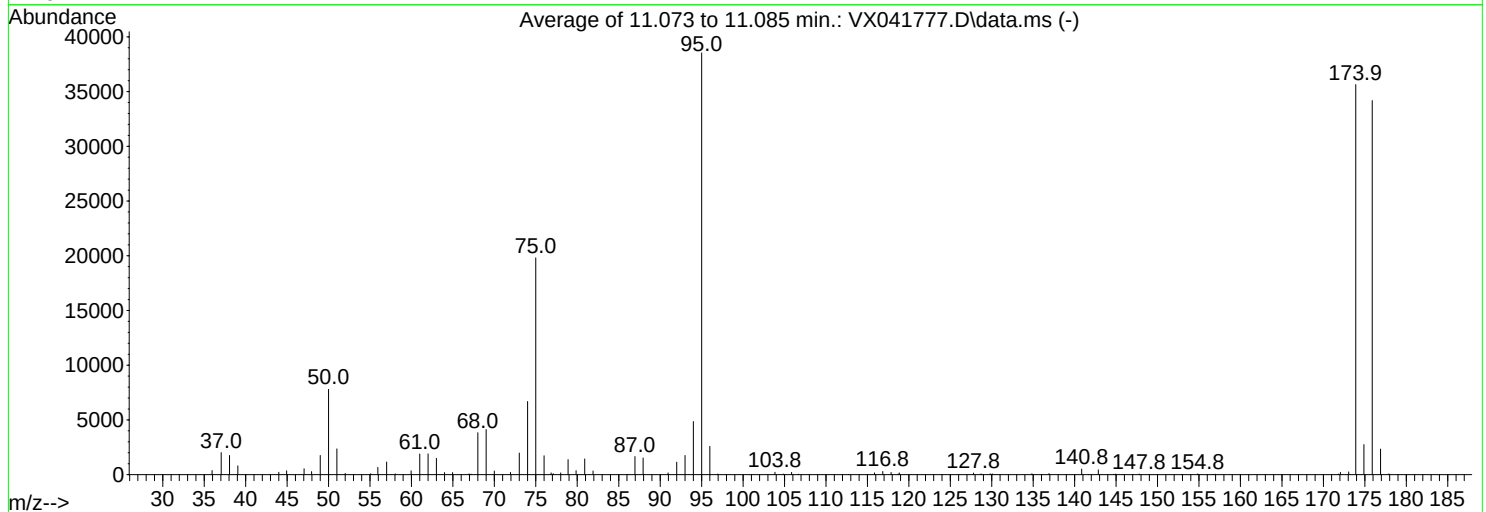


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060724\
Data File : VX041777.D
Acq On : 07 Jun 2024 09:24
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051524W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu May 16 05:13:13 2024

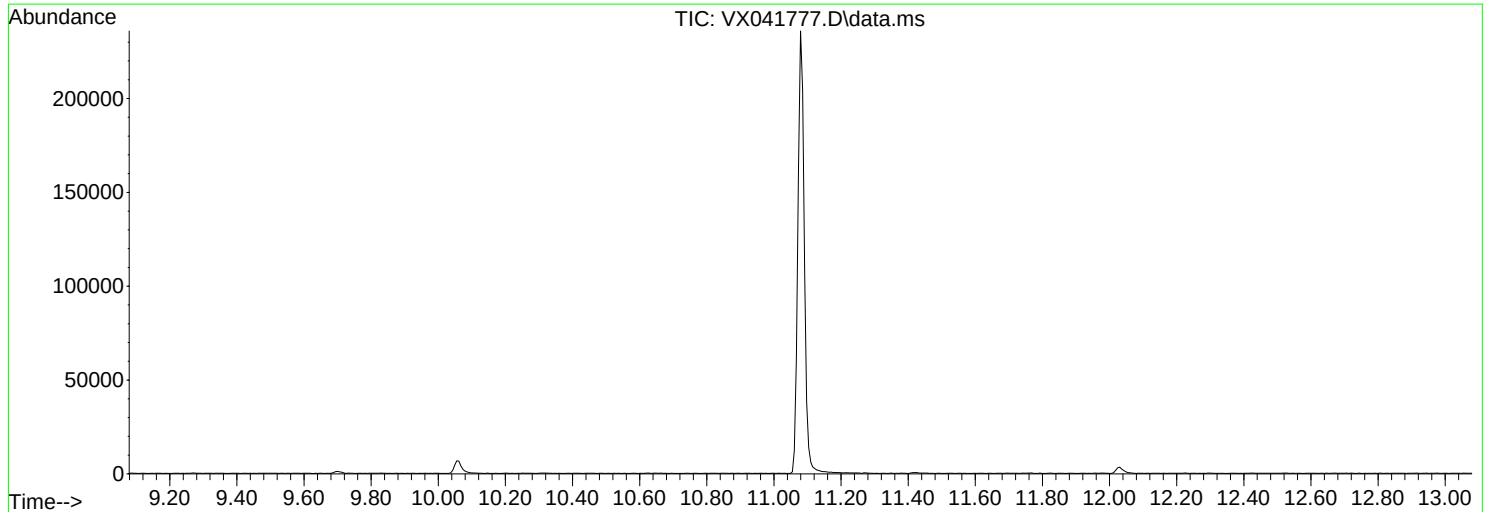

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	7795	PASS
75	95	30	60	51.4	19813	PASS
95	95	100	100	100.0	38541	PASS
96	95	5	9	6.7	2582	PASS
173	174	0.00	2	0.7	250	PASS
174	95	50	100	92.5	35643	PASS
175	174	5	9	7.7	2745	PASS
176	174	95	101	95.9	34189	PASS
177	176	5	9	6.8	2334	PASS