

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060819\
 Data File : VX010150.D
 Acq On : 08 Jun 2019 19:50
 Operator : JC/SP
 Sample : K3249-20
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPS1-TT-MW303S-20190606

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	17	21	26	rBV	16324	24326	1.87%	0.351%
2	2.611	234	239	246	rVB	7300	14295	1.10%	0.206%
3	3.019	298	306	316	rVB2	4937	13495	1.04%	0.195%
4	4.696	574	581	592	rVB	4483	13012	1.00%	0.188%
5	5.501	698	713	725	rBV2	158679	454421	34.98%	6.554%
6	5.659	729	739	756	rVB	266329	756043	58.19%	10.905%
7	6.062	795	805	819	rBV	142700	377388	29.05%	5.443%
8	6.860	925	936	951	rBV	395531	928366	71.46%	13.390%
9	8.714	1232	1240	1255	rBV	834766	1299180	100.00%	18.738%
10	10.110	1462	1469	1482	rBV	818960	1105480	85.09%	15.945%
11	11.134	1631	1637	1650	rBV	711967	890823	68.57%	12.849%
12	12.073	1786	1791	1803	rVB	824245	1056394	81.31%	15.237%


Sum of corrected areas: 6933223

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060819\
Data File : VX010150.D
Acq On : 08 Jun 2019 19:50
Operator : JC/SP
Sample : K3249-20
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW303S-20190606

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

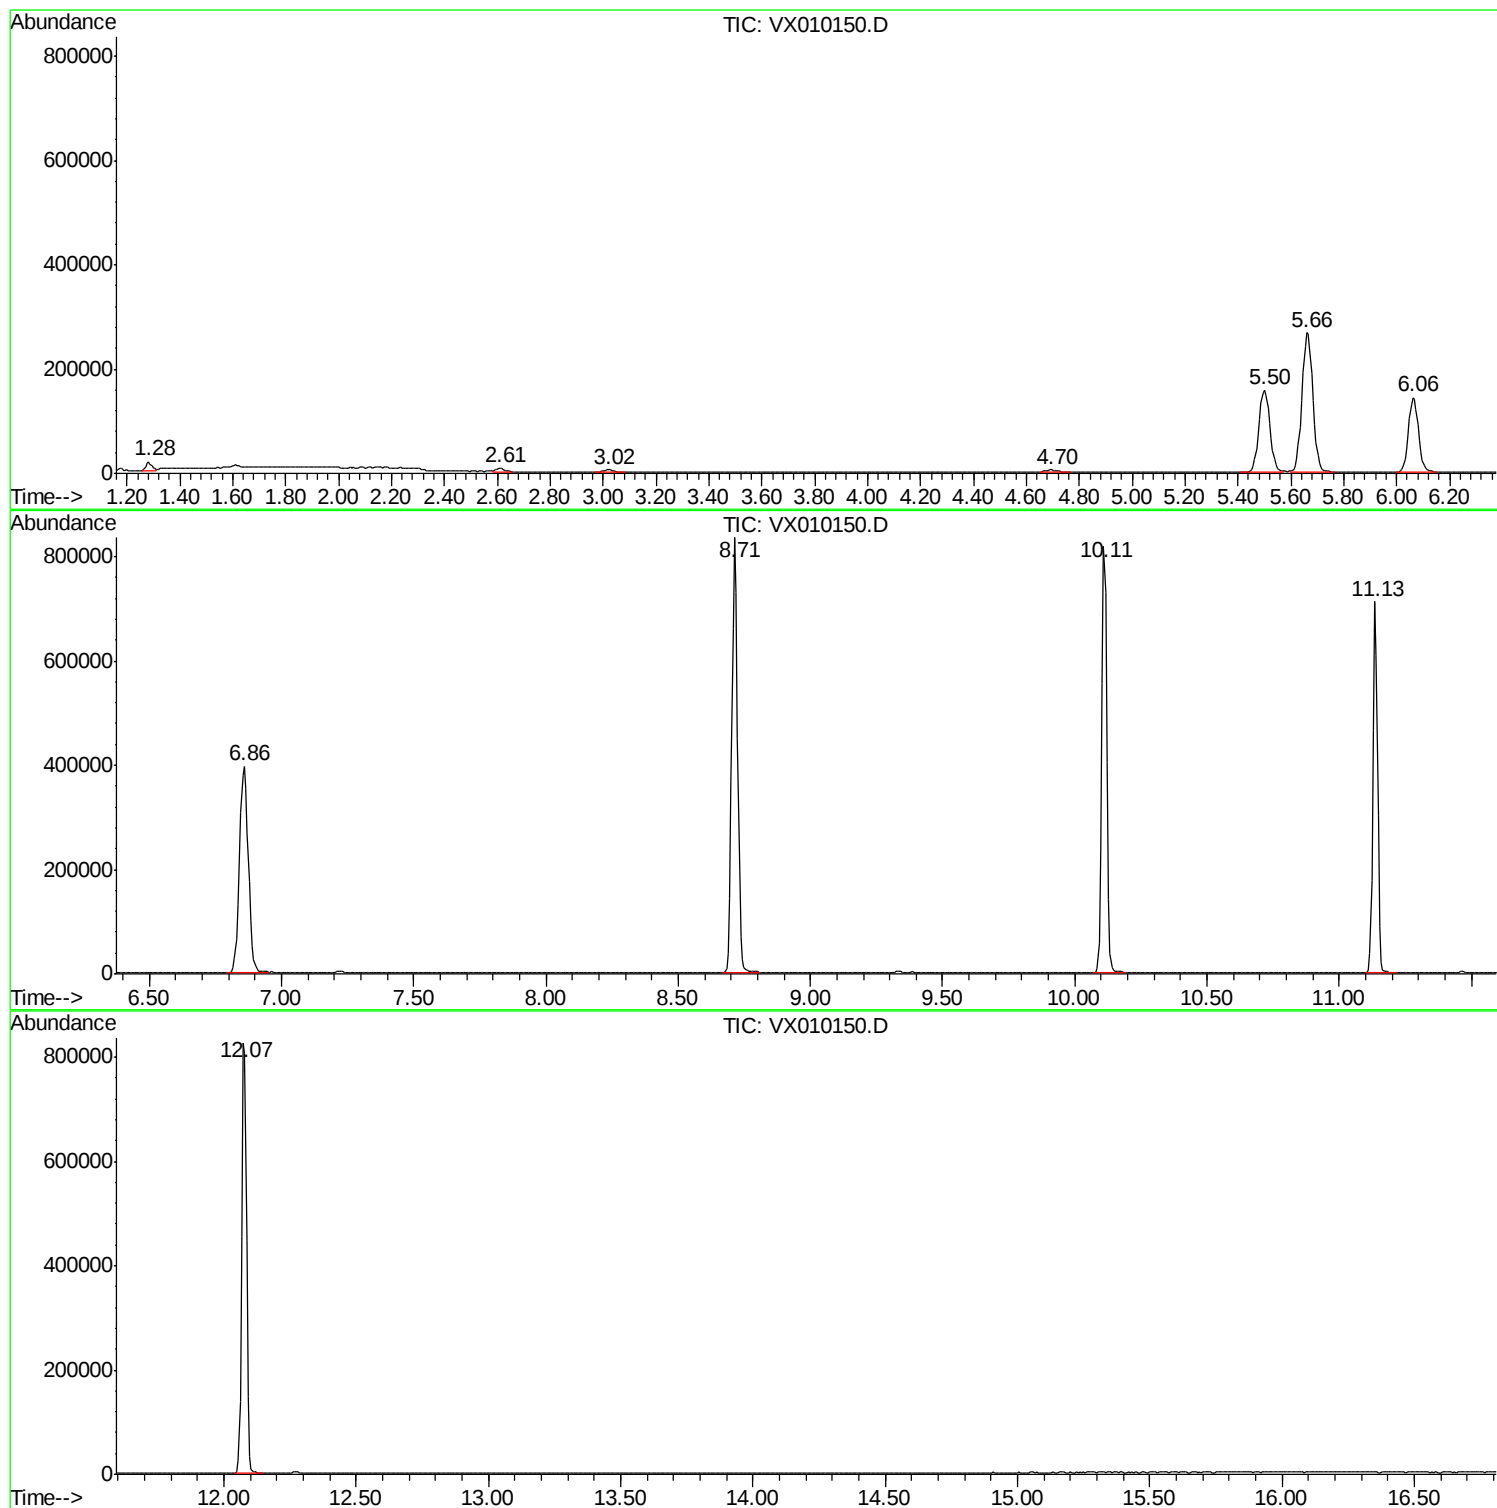

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX060819\
Data File : VX010150.D
Acq On : 08 Jun 2019 19:50
Operator : JC/SP
Sample : K3249-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW303S-20190606

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX060819\
Data File : VX010150.D
Acq On : 08 Jun 2019 19:50
Operator : JC/SP
Sample : K3249-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPS1-TT-MW303S-20190606

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc