


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX060819\
Data File : VX010136.D
Acq On : 08 Jun 2019 14:03
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060719W.M
Title : SW846 8260
Last Update : Sat Jun 08 02:12:13 2019

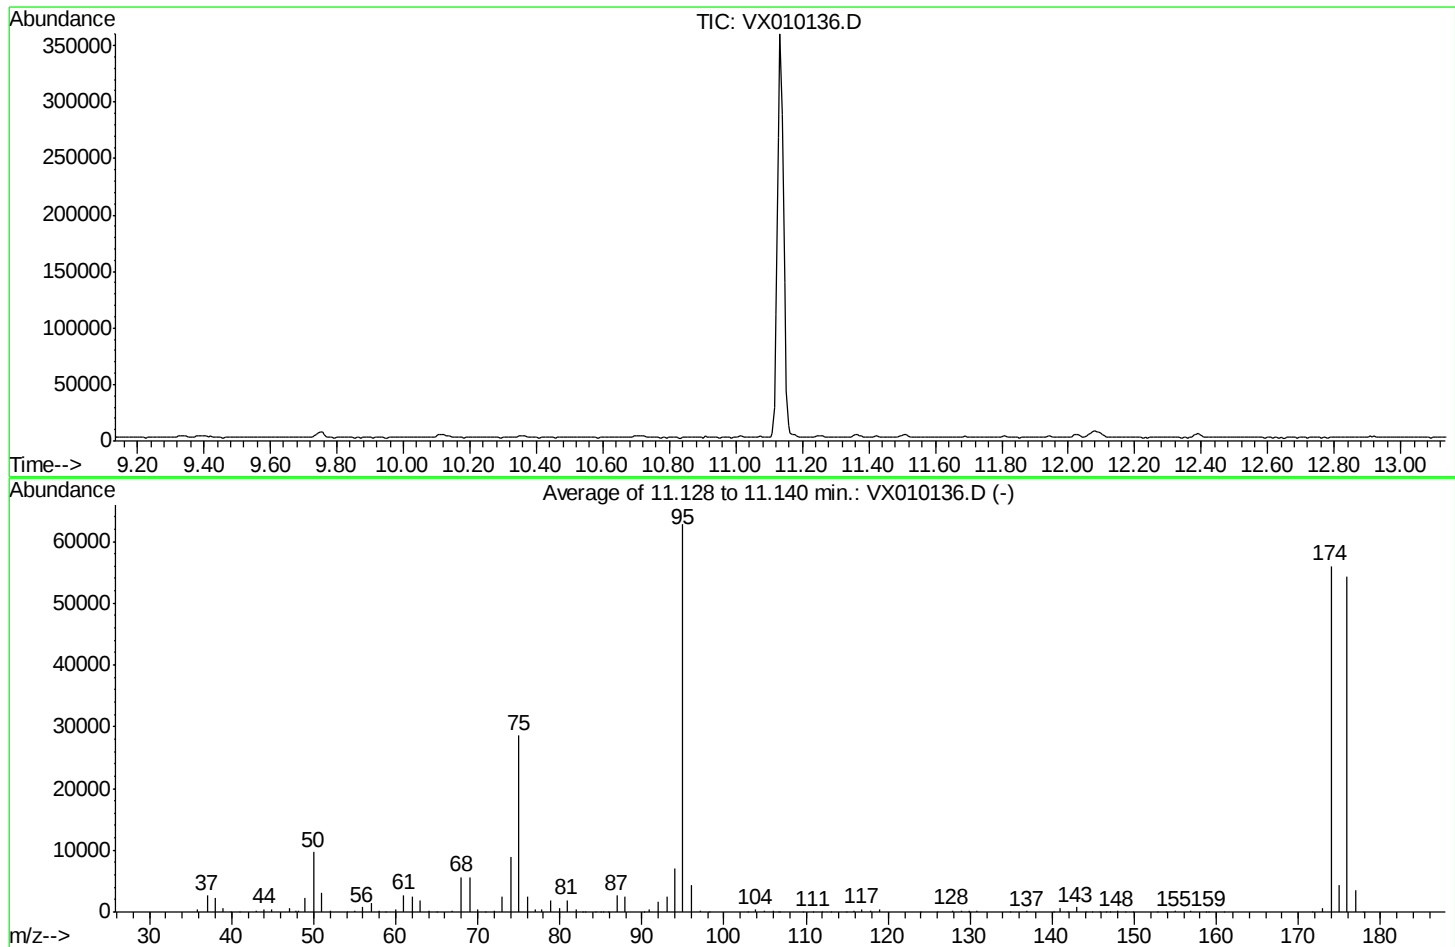

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	9678	PASS
75	95	30	60	45.5	28575	PASS
95	95	100	100	100.0	62770	PASS
96	95	5	9	6.9	4331	PASS
173	174	0.00	2	0.9	530	PASS
174	95	50	100	89.2	55978	PASS
175	174	5	9	7.7	4323	PASS
176	174	95	101	97.2	54394	PASS
177	176	5	9	6.5	3515	PASS