

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060820\
 Data File : VX016631.D
 Acq On : 08 Jun 2020 12:27
 Operator : JC/SP
 Sample : L2894-12DL 10X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LF012RW164-200601DL

Quant Time: Jun 09 06:40:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 27 16:31:05 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	218104	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	350872	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	345074	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	189906	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	129246	47.72	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.44%	
35) Dibromofluoromethane	5.46	113	108523	50.23	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.46%	
50) Toluene-d8	8.70	98	422012	50.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.38%	
62) 4-Bromofluorobenzene	11.12	95	176969	54.46	ug/l	0.00
Spiked Amount 50.000			Recovery	=	108.92%	
Target Compounds						
27) cis-1,2-Dichloroethene	4.56	96	190745	71.029	ug/l	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060820\
Data File : VX016631.D
Acq On : 08 Jun 2020 12:27
Operator : JC/SP
Sample : L2894-12DL 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF012RW164-200601DL

Quant Time: Jun 09 06:40:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260
QLast Update : Wed May 27 16:31:05 2020
Response via : Initial Calibration

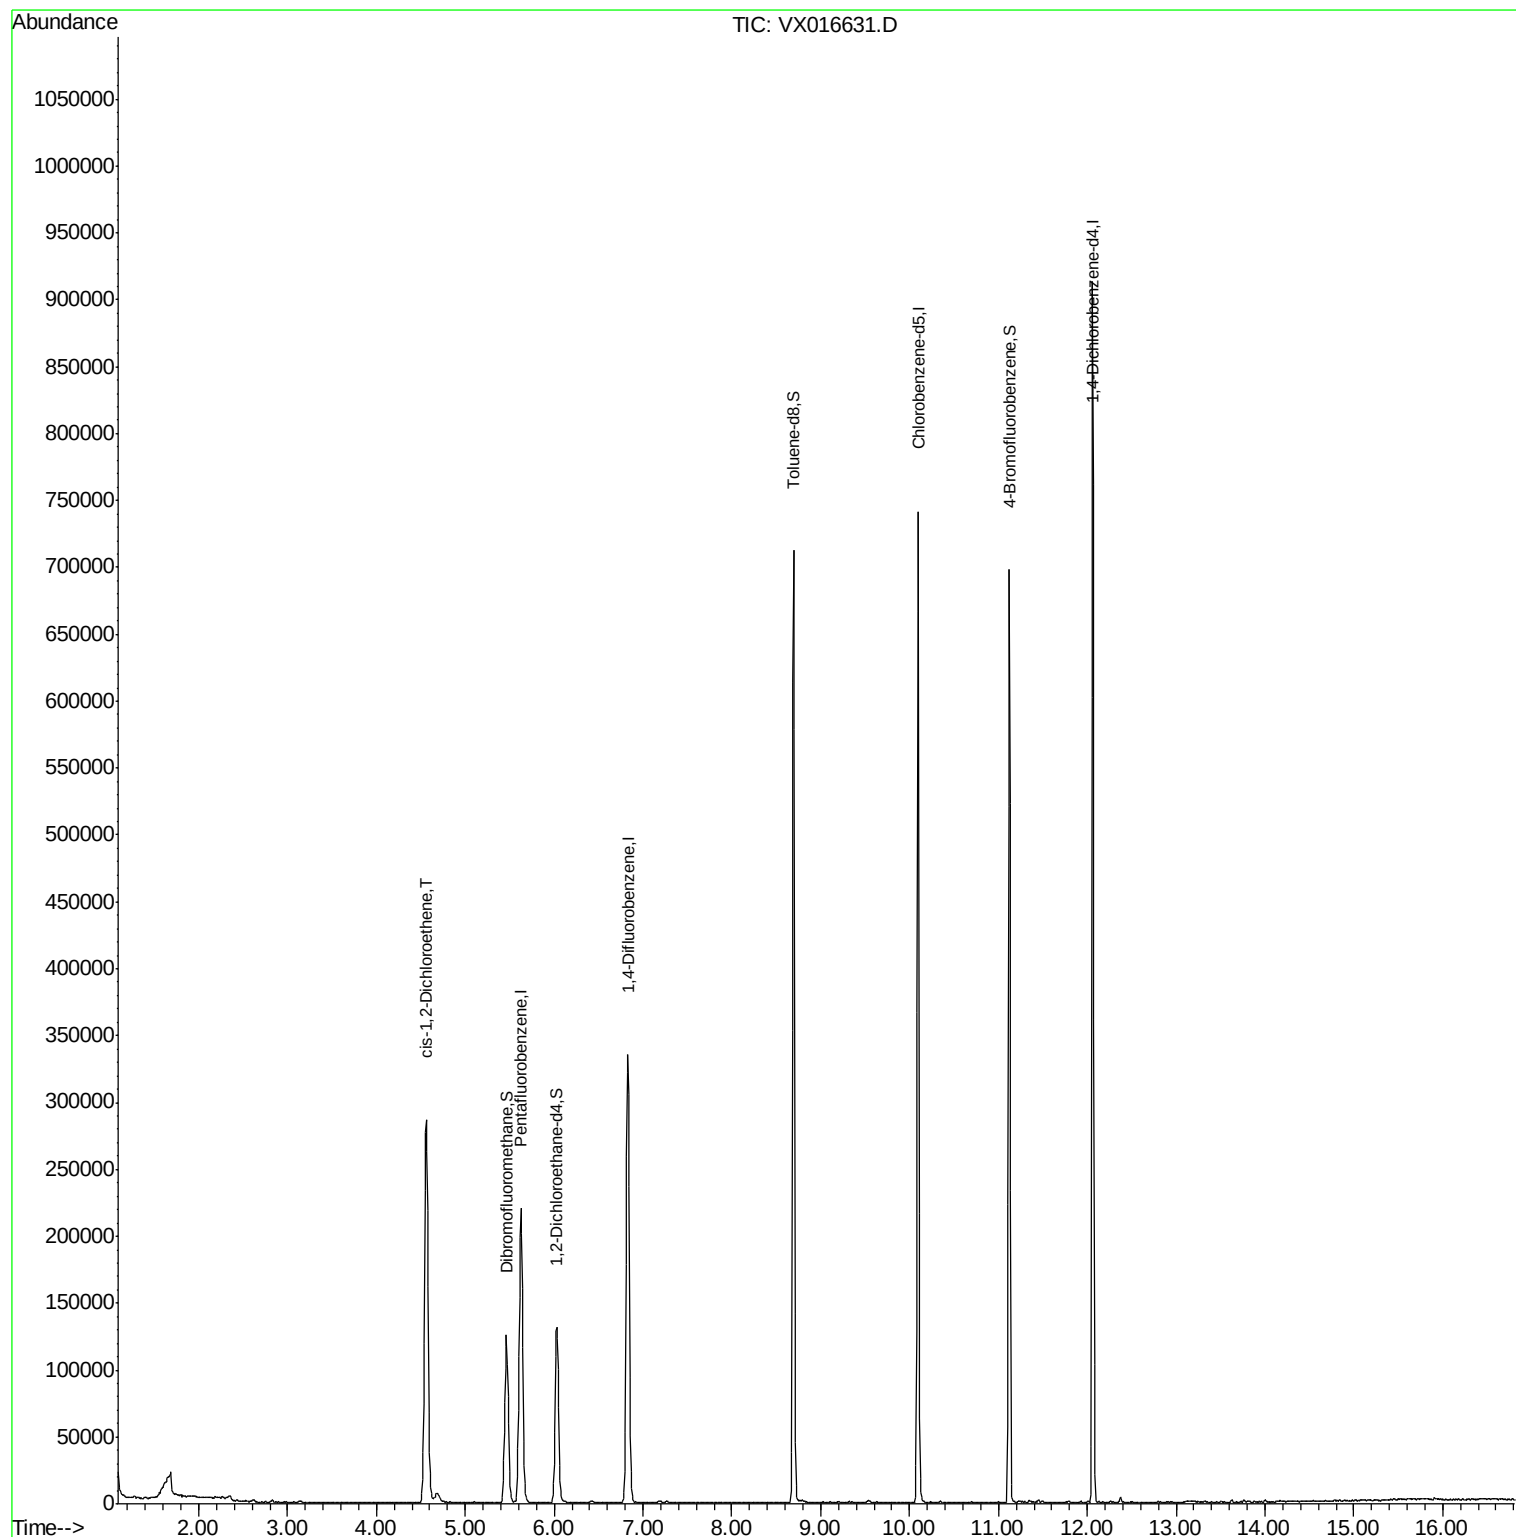

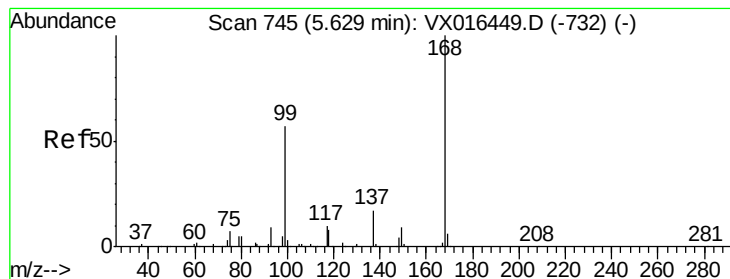

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX016631.D

Acq: 08 Jun 2020 12:27

Instrument :

MSVOA_X

ClientSampleId :


LF012RW164-200601DL

Tot Ion:168 Resp: 218104

Ion Ratio Lower Upper




168 100

99 57.3 45.2 67.8

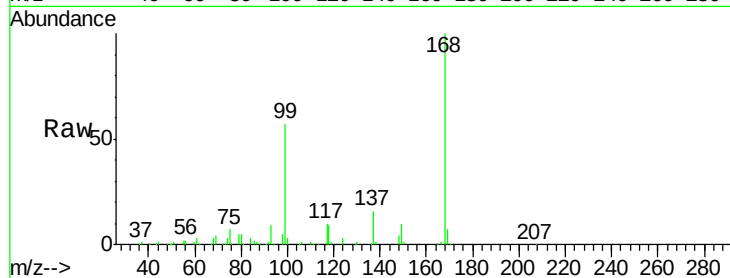

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

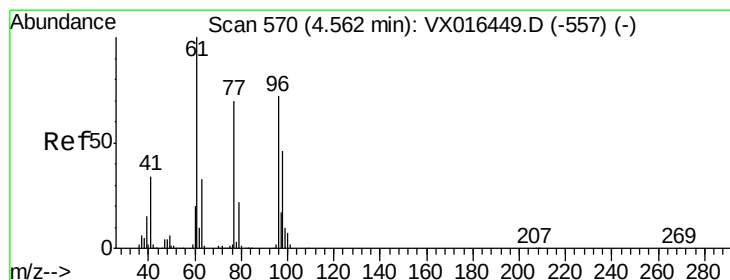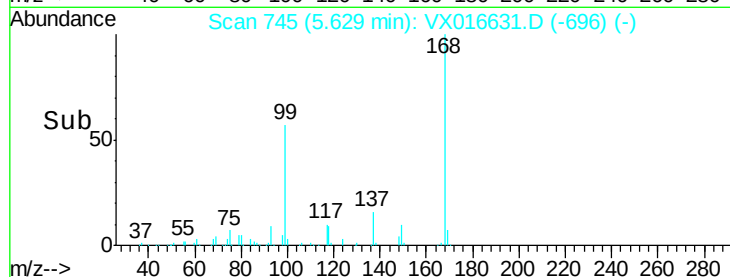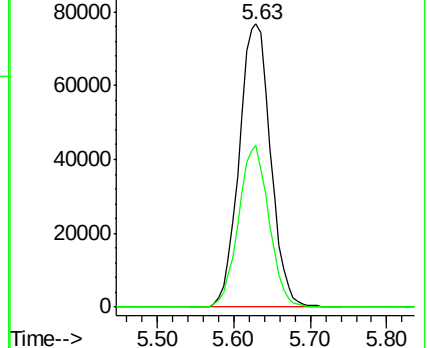

#27

cis-1,2-Dichloroethene

Concen: 71.029 ug/l

RT: 4.56 min Scan# 570

Delta R.T. -0.00 min

Lab File: VX016631.D

Acq: 08 Jun 2020 12:27


Tgt Ion: 96 Resp: 190745

Ion Ratio Lower Upper

96 100

61 122.1 0.0 284.6



98 64.5 0.0 127.2

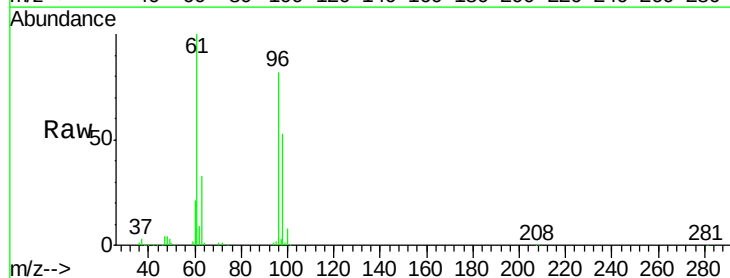


Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0



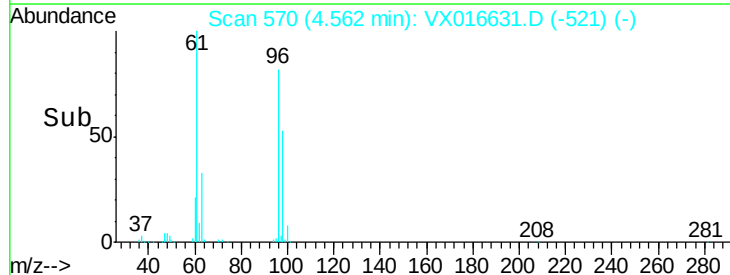
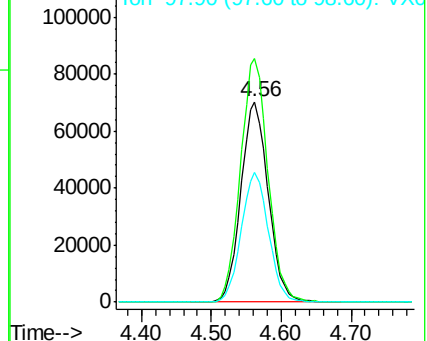


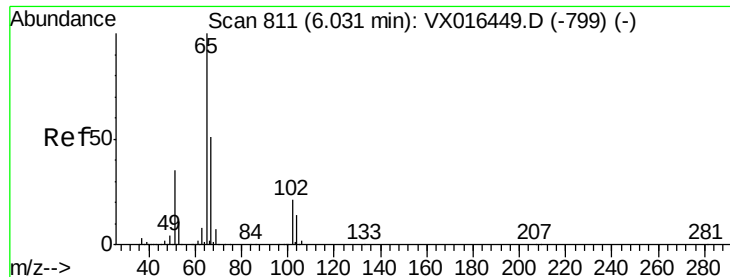

#33
 1,2-Dichloroethane-d4
 Concen: 47.717 ug/l
 RT: 6.03 min Scan# 811
 Delta R.T. -0.00 min
 Lab File: VX016631.D
 Acq: 08 Jun 2020 12:27




Instrument :
 MSVOA_X
 ClientSampleId :
 LF012RW164-200601DL


Tot Ion: 65 Resp: 129246
 Ion Ratio Lower Upper
 65 100
 67 52.6 0.0 104.8

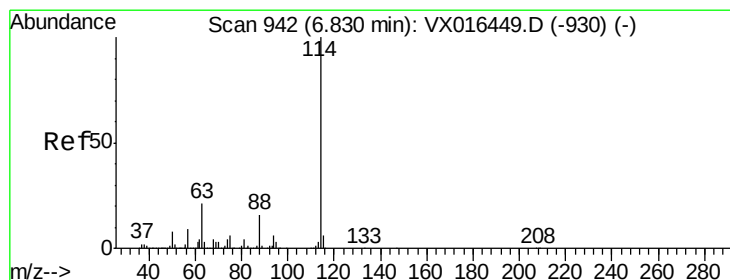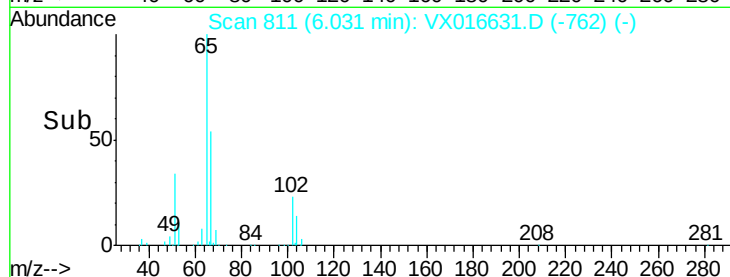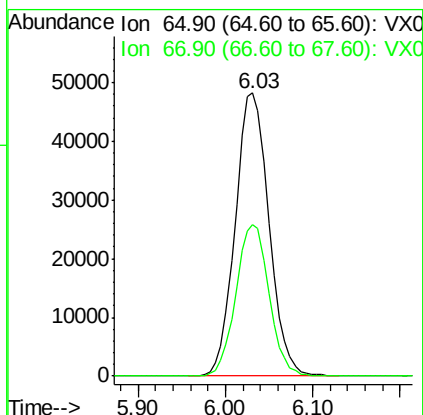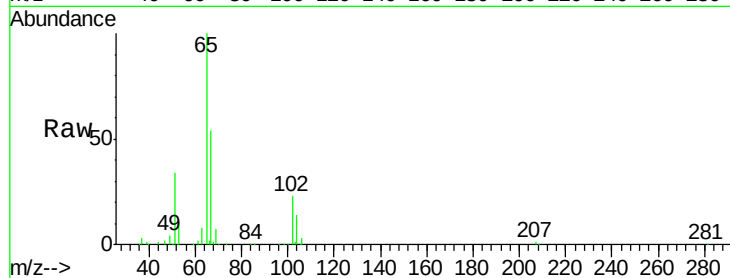

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. -0.00 min
 Lab File: VX016631.D
 Acq: 08 Jun 2020 12:27

Tgt Ion: 114 Resp: 350872
 Ion Ratio Lower Upper
 114 100
 63 19.1 0.0 42.6
 88 16.5 0.0 32.8

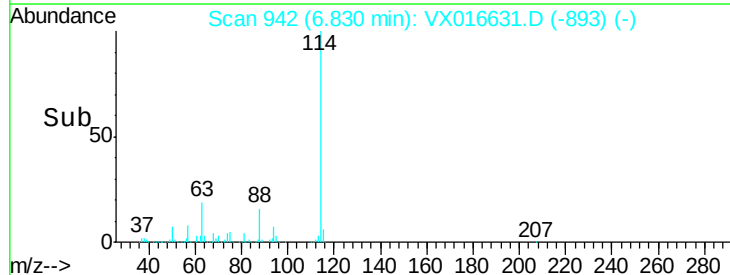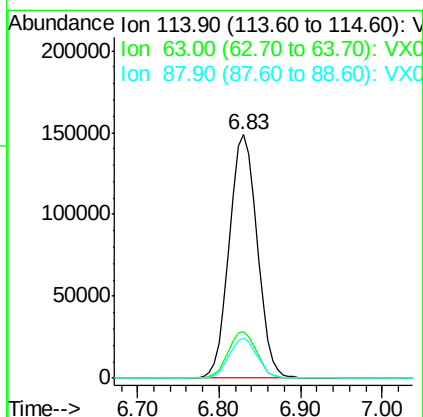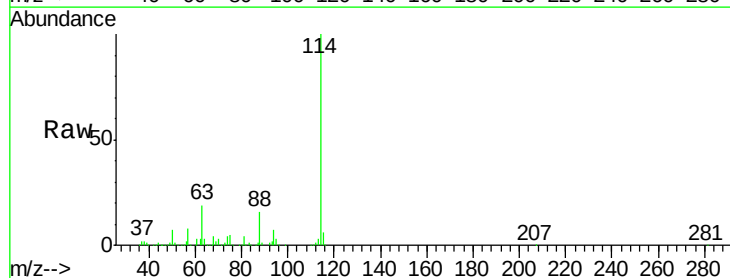

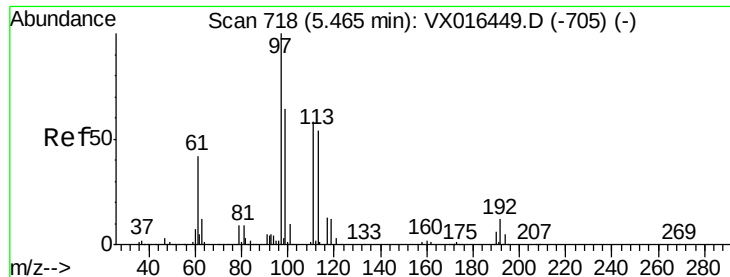

#35

Dibromofluoromethane

Concen: 50.231 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX016631.D

Acq: 08 Jun 2020 12:27

Instrument :

MSVOA_X

ClientSampleId :

LF012RW164-200601DL


Tot Ion:113 Resp: 108523

Ion Ratio Lower Upper

113 100

111 102.6 83.0 124.6




192 22.7 17.7 26.5

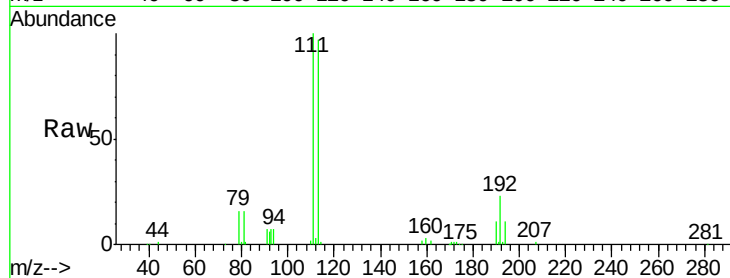

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

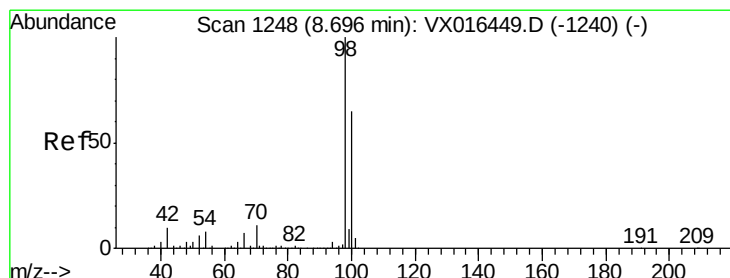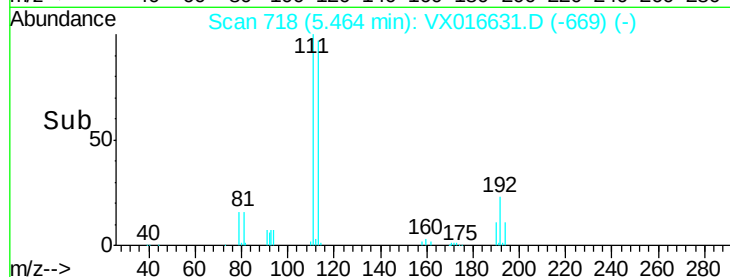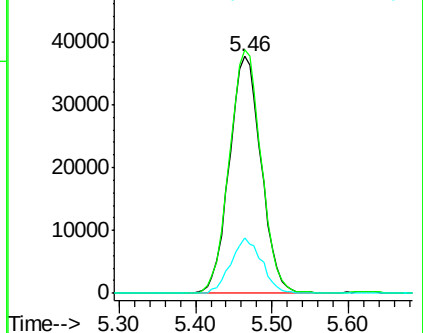

#50

Toluene-d8

Concen: 50.185 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX016631.D


Acq: 08 Jun 2020 12:27

Tgt Ion: 98 Resp: 422012

Ion Ratio Lower Upper



98 100


100 66.7 53.8 80.6

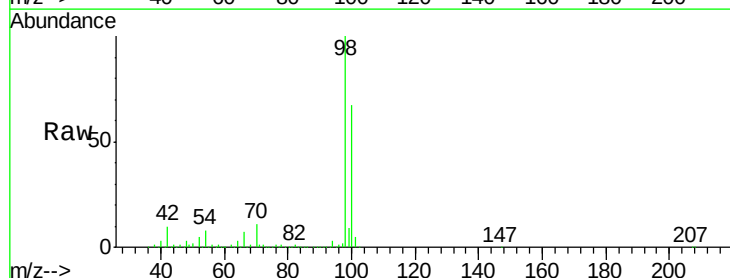

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

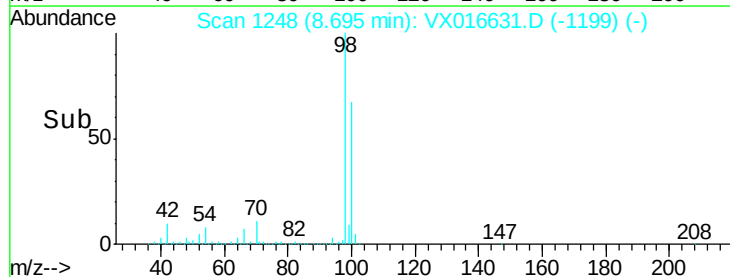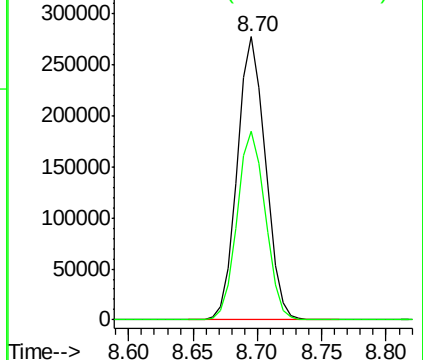

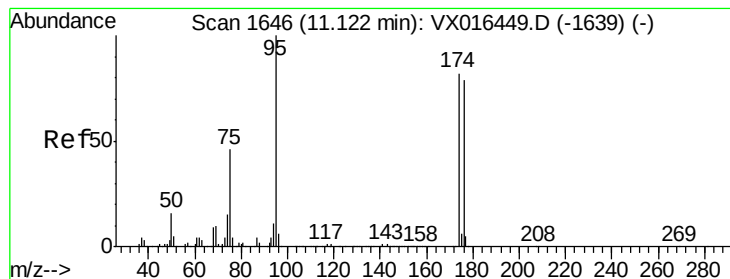

#62

4-Bromofluorobenzene

Concen: 54.465 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX016631.D

Acq: 08 Jun 2020 12:27

Instrument :

MSVOA_X

ClientSampleId :

LF012RW164-200601DL


Tot Ion: 95 Resp: 176969

Ion Ratio Lower Upper

95 100

174 86.6 0.0 163.0




176 84.1 0.0 156.8

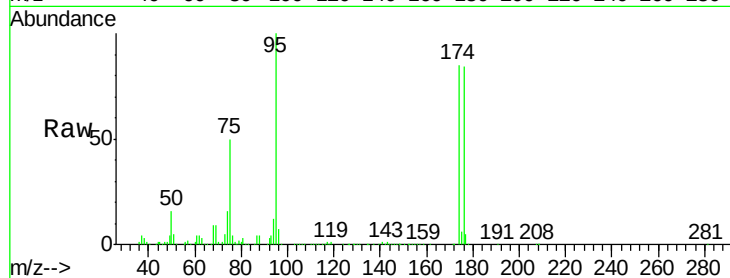

Abundance Ion 94.90 (94.60 to 95.60): VX016631.D (-1597) (-)

Ion 173.80 (173.50 to 174.50): VX016631.D (-1597) (-)

Ion 175.80 (175.50 to 176.50): VX016631.D (-1597) (-)

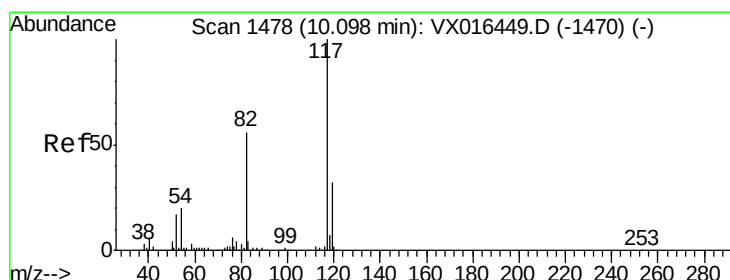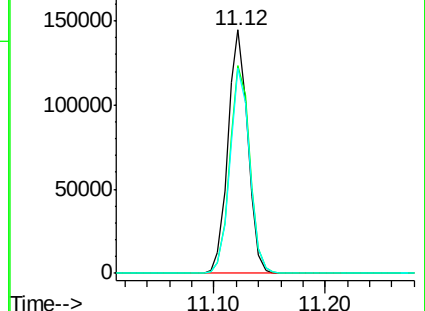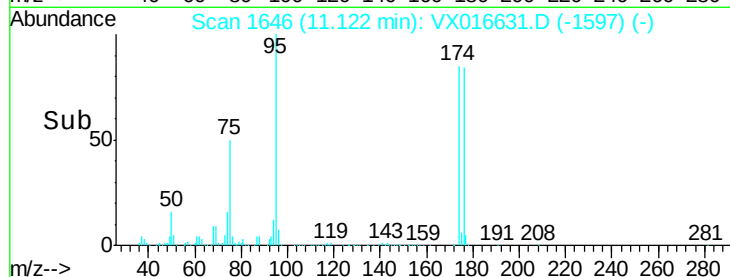

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX016631.D

Acq: 08 Jun 2020 12:27


Tgt Ion: 117 Resp: 345074

Ion Ratio Lower Upper

117 100

82 54.6 45.0 67.6



119 32.3 25.8 38.8

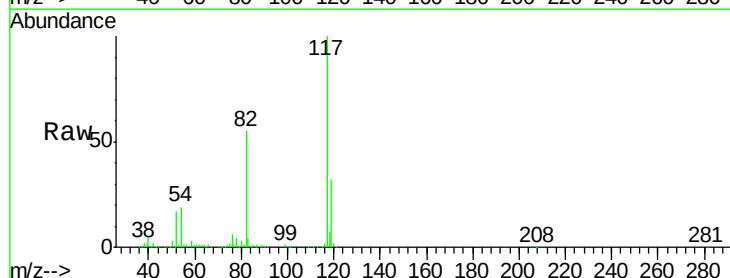


Abundance Ion 116.90 (116.60 to 117.60): VX016631.D (-1429) (-)

Ion 82.00 (81.70 to 82.70): VX016631.D (-1429) (-)

Ion 118.90 (118.60 to 119.60): VX016631.D (-1429) (-)

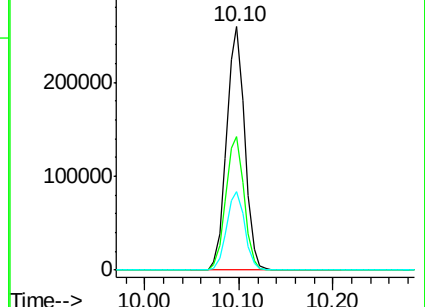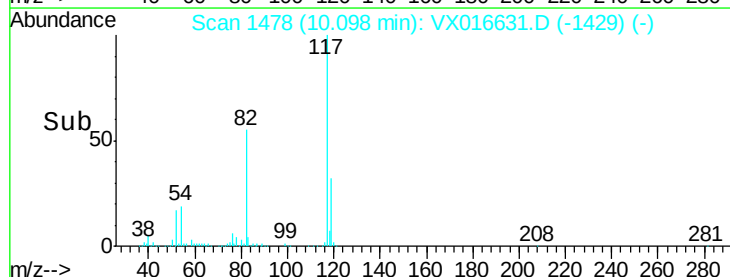

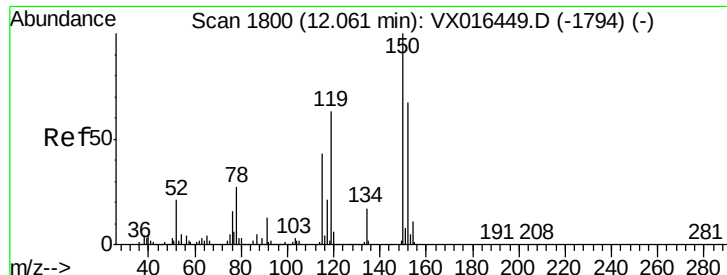

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX016631.D

Acq: 08 Jun 2020 12:27

Instrument :

MSVOA_X

ClientSampleId :

LF012RW164-200601DL


Tot Ion:152 Resp: 189906

Ion Ratio Lower Upper

152 100

115 57.7 39.9 119.6

150 156.9 0.0 341.0

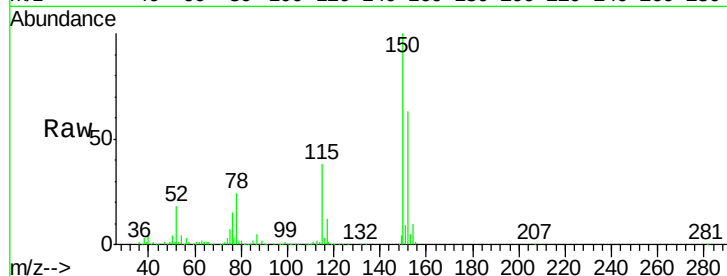

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

