

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060822\
 Data File : VX029324.D
 Acq On : 08 Jun 2022 16:23
 Operator : JC/MD
 Sample : N3203-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 09 07:00:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 08 03:00:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	274194	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	461253	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	397758	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	175947	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	259888	62.712	ug/l	0.00
Spiked Amount 50.000	Range	61 - 141	Recovery	=	125.420%	
35) Dibromofluoromethane	5.391	113	52400	13.363	ug/l	0.00
Spiked Amount 50.000	Range	69 - 133	Recovery	=	26.720%#	
50) Toluene-d8	8.653	98	769940	55.517	ug/l	0.00
Spiked Amount 50.000	Range	65 - 126	Recovery	=	111.040%	
62) 4-Bromofluorobenzene	11.085	95	291322	53.678	ug/l	0.00
Spiked Amount 50.000	Range	58 - 135	Recovery	=	107.360%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.618	94	706	0.273	ug/l	93
6) Chloroethane	1.685	64	341	Below Cal	#	43
10) Methyl Iodide	2.453	142	487	1.326	ug/l #	75
11) Tert butyl alcohol	2.953	59	11219	Below Cal	#	76
13) Acrolein	2.239	56	358	0.707	ug/l #	76
14) Allyl chloride	2.556	41	3406	0.515	ug/l #	59
16) Acetone	2.380	43	2253376	1015.887	ug/l	97
18) Methyl Acetate	2.556	43	10970	1.867	ug/l #	46
20) Methylene Chloride	2.788	84	10987	2.218	ug/l	95
23) Vinyl Acetate	3.873	43	4045	0.365	ug/l #	66
25) 2-Butanone	4.568	43	13204	3.763	ug/l	94
29) Tetrahydrofuran	5.038	42	649	0.284	ug/l #	32
31) Cyclohexane	5.556	56	5672	0.763	ug/l #	1
36) 1,1-Dichloropropene	5.562	75	22087	3.410	ug/l #	50
37) Ethyl Acetate	4.568	43	13204	1.975	ug/l #	65
38) Carbon Tetrachloride	5.556	117	30264	4.571	ug/l #	15
40) Benzene	6.044	78	81241	4.213	ug/l	96
41) Methacrylonitrile	5.019	41	406	Below Cal	#	34
48) Methyl methacrylate	7.604	41	8418	1.666	ug/l #	15
51) 4-Methyl-2-Pentanone	8.580	43	7487	1.139	ug/l	90
52) Toluene	8.720	92	27676	2.236	ug/l	99
53) t-1,3-Dichloropropene	8.726	75	317	1.360	ug/l #	1
59) 2-Hexanone	9.439	43	1620	0.324	ug/l	84
67) Ethyl Benzene	10.195	91	45489	2.361	ug/l	99
68) m/p-Xylenes	10.299	106	40269	5.401	ug/l	94
69) o-Xylene	10.646	106	23382	3.227	ug/l	94
73) Isopropylbenzene	10.963	105	3766	0.272	ug/l	99
76) 1,2,3-Trichloropropane	11.085	75	147289	35.840	ug/l #	38
80) 1,3,5-Trimethylbenzene	11.451	105	5454	0.464	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.085	75	147289	108.752	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.756	105	23333	2.010	ug/l	96
85) sec-Butylbenzene	11.756	105	23333	1.665	ug/l #	56
89) n-Butylbenzene	12.244	91	27912	2.818	ug/l #	41
90) Hexachloroethane	12.414	117	10199	5.461	ug/l #	10
95) Naphthalene	13.780	128	5051680	394.016	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060822\
Data File : VX029324.D
Acq On : 08 Jun 2022 16:23
Operator : JC/MD
Sample : N3203-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 09 07:00:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 08 03:00:38 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060822\
Data File : VX029324.D
Acq On : 08 Jun 2022 16:23
Operator : JC/MD
Sample : N3203-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 09 07:00:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 08 03:00:38 2022
Response via : Initial Calibration




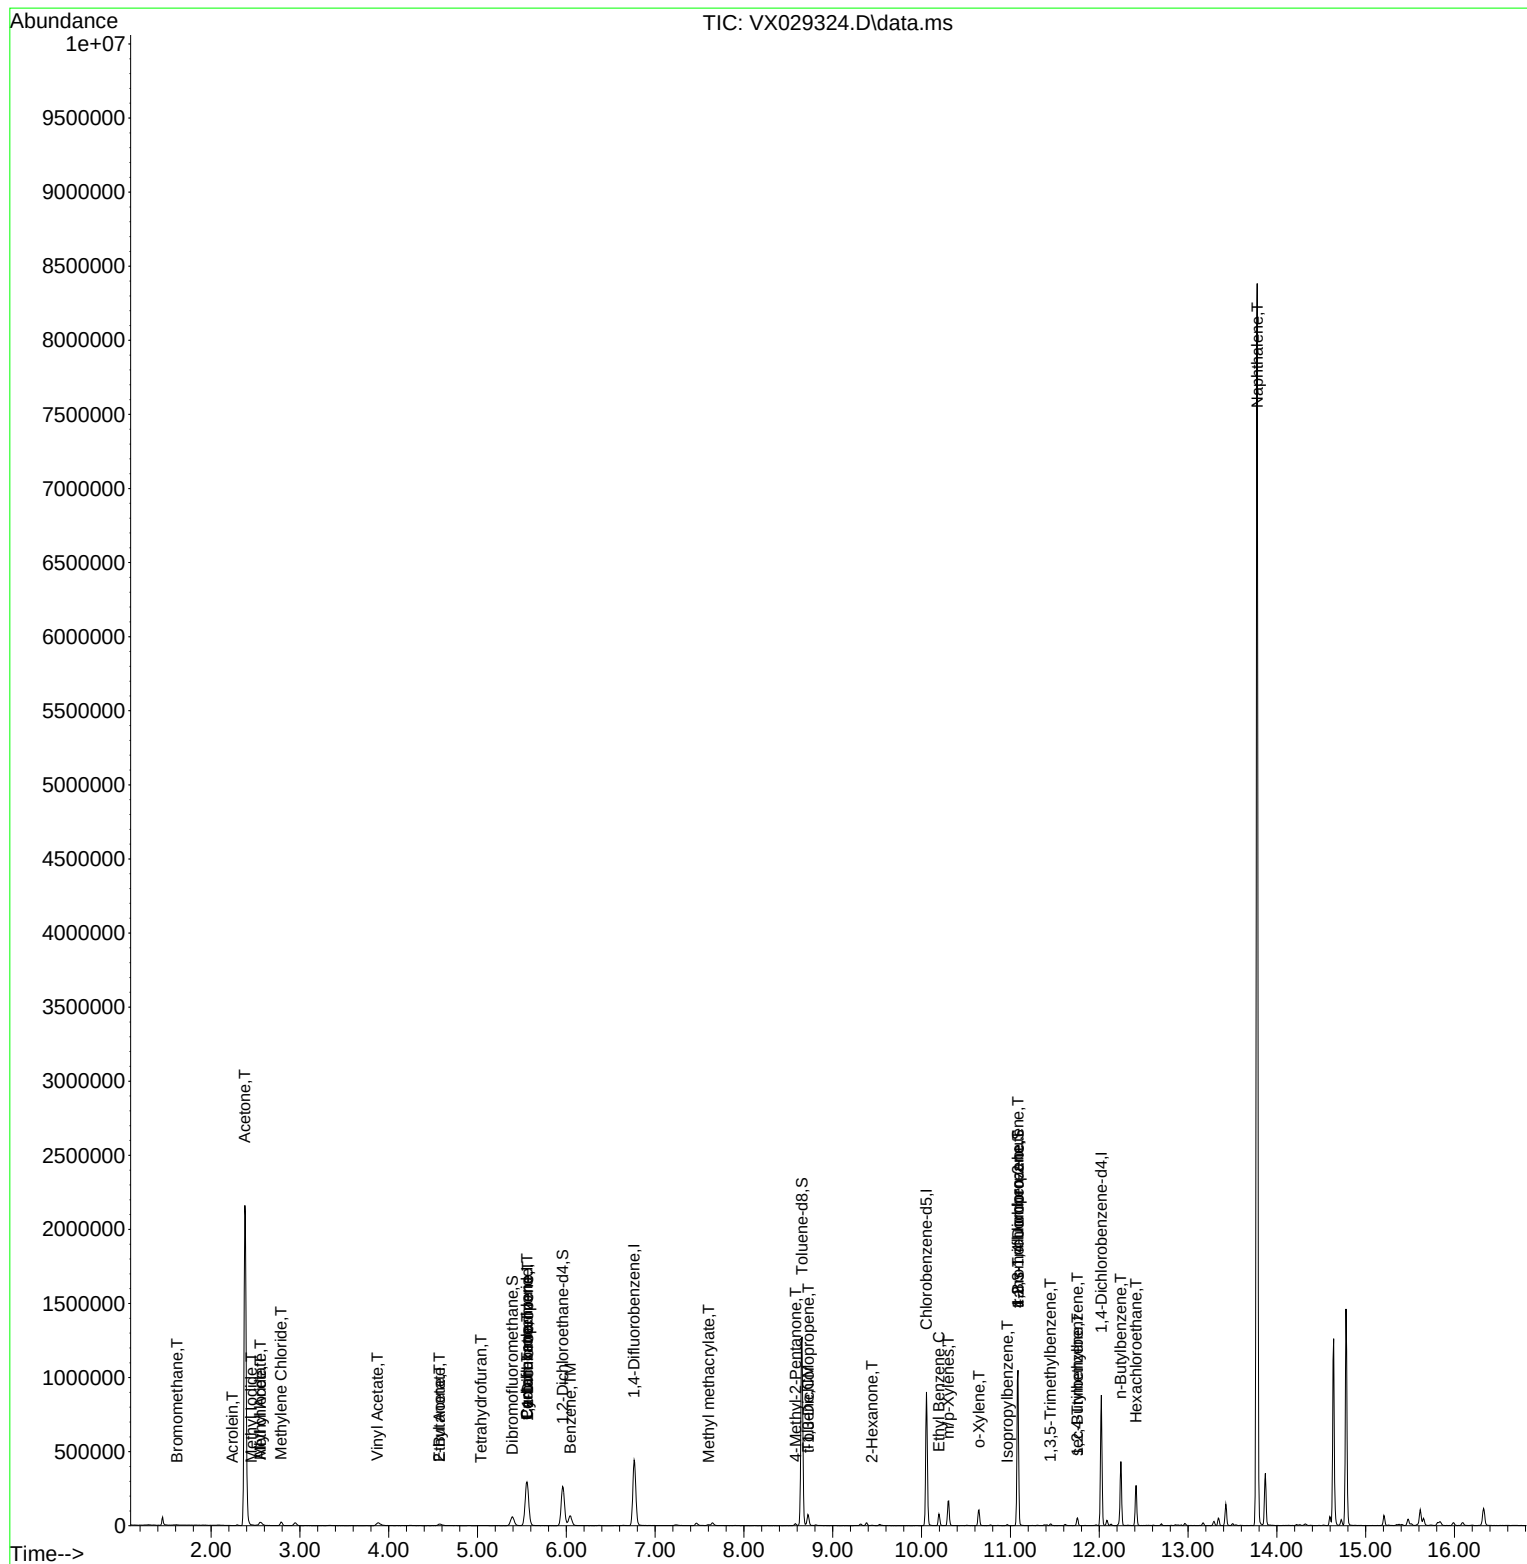




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 274194
Ion Ratio Lower Upper
168 100
99 61.5 41.7 62.5

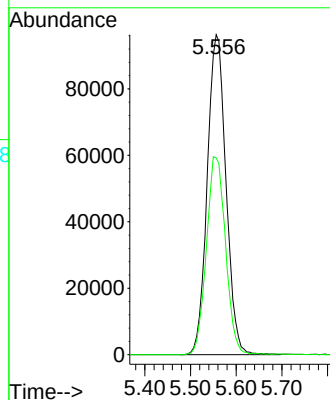

#5
Bromomethane
Concen: 0.273 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23


Tgt Ion: 94 Resp: 706
Ion Ratio Lower Upper
94 100
96 87.5 75.3 112.9

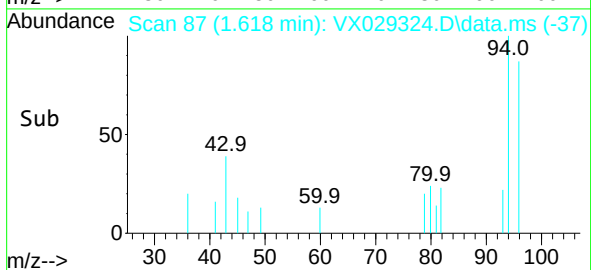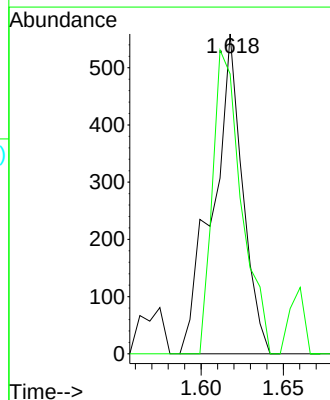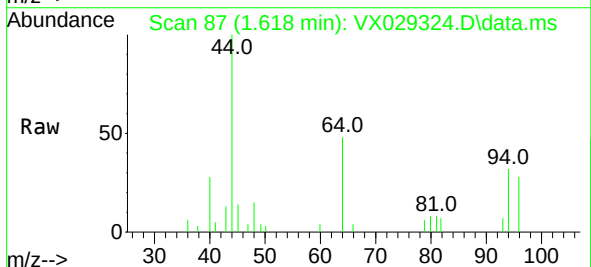



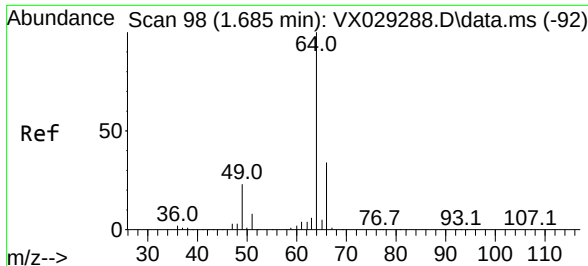


#6
Chloroethane
Concen: Below Cal
RT: 1.685 min Scan# 98
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Instrument :
MSVOA_X
ClientSampleId :



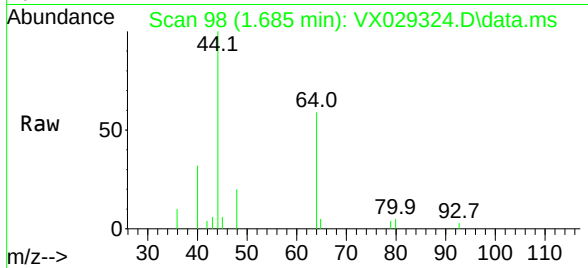



Tgt Ion: 64 Resp: 341
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#

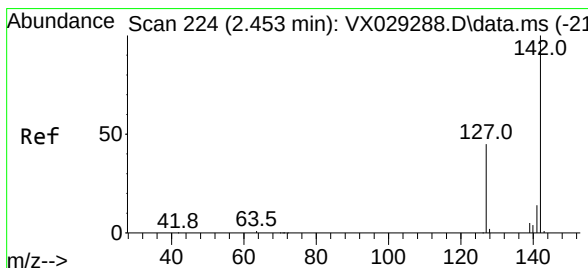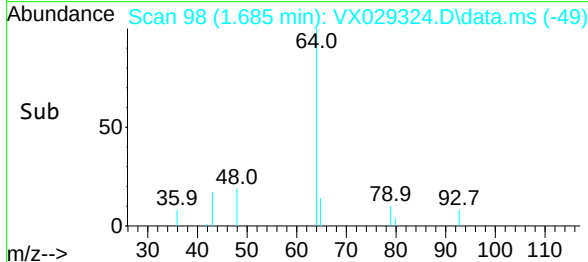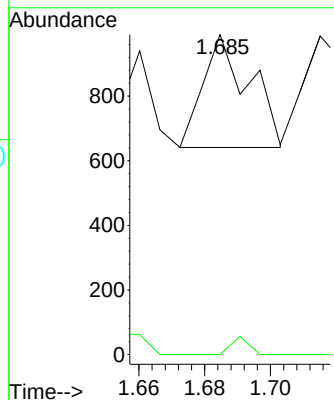

#10
Methyl Iodide
Concen: 1.326 ug/l
RT: 2.453 min Scan# 224
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion: 142 Resp: 487
Ion Ratio Lower Upper
142 100
127 29.0 33.9 50.9#
141 0.0 11.4 17.2#


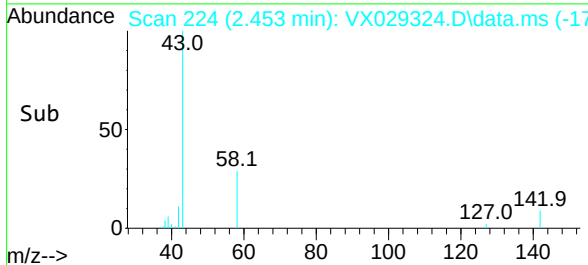
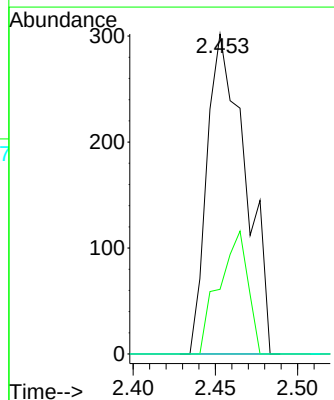
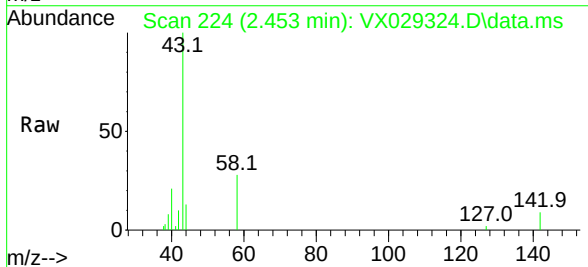




#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.953 min Scan# 306
Delta R.T. -0.042 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 59 Resp: 11219
Ion Ratio Lower Upper
59 100
57 1.6 8.3 12.5#

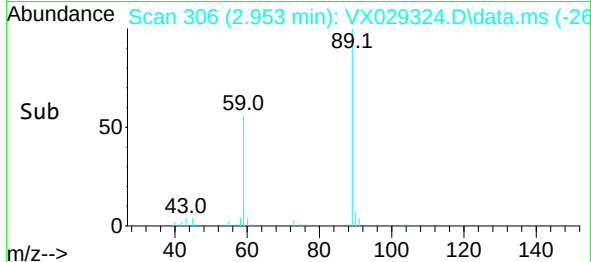

#13
Acrolein
Concen: 0.707 ug/l
RT: 2.239 min Scan# 189
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23


Tgt Ion: 56 Resp: 358
Ion Ratio Lower Upper
56 100
55 88.0 55.0 82.6#

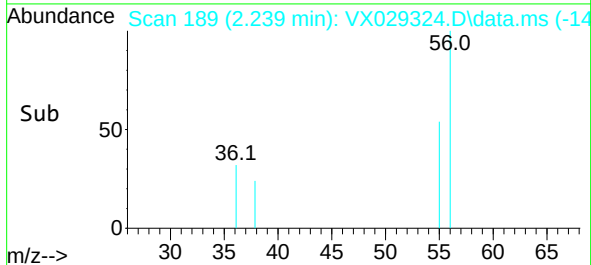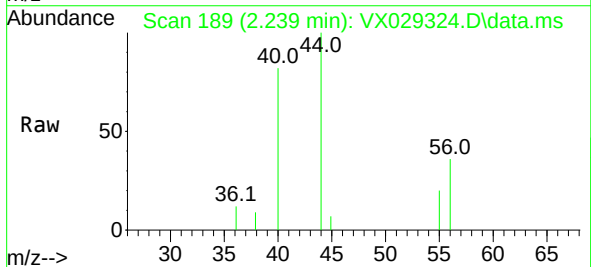






#14
 Allyl chloride
 Concen: 0.515 ug/l
 RT: 2.556 min Scan# 241
 Delta R.T. -0.110 min
 Lab File: VX029324.D
 Acq: 08 Jun 2022 16:23

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion: 41 Resp: 3406
 Ion Ratio Lower Upper
 41 100
 39 82.3 50.4 75.6#
 76 0.0 32.7 49.1#

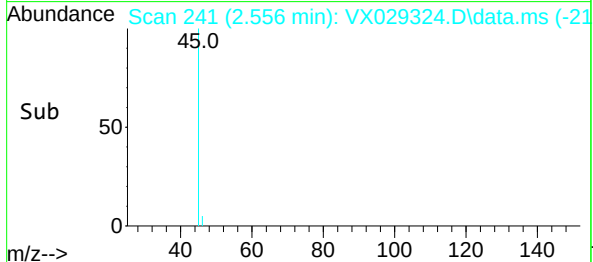

#16
 Acetone
 Concen: 1015.887 ug/l
 RT: 2.380 min Scan# 212
 Delta R.T. -0.012 min
 Lab File: VX029324.D
 Acq: 08 Jun 2022 16:23

Tgt Ion: 43 Resp: 2253376
 Ion Ratio Lower Upper
 43 100
 58 34.2 28.8 43.2


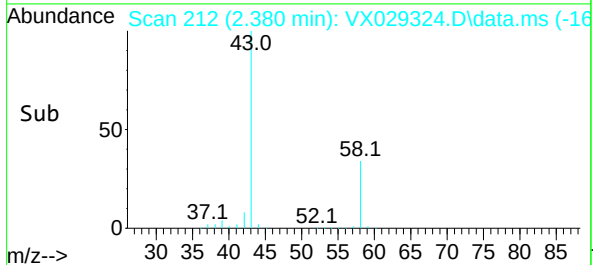

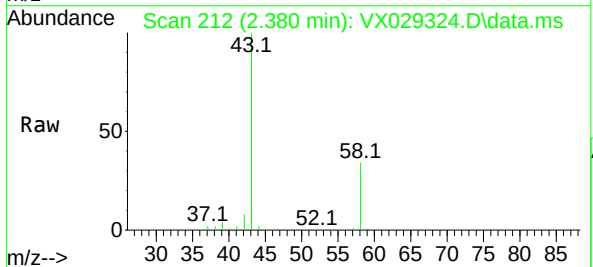




#18
Methyl Acetate
Concen: 1.867 ug/l
RT: 2.556 min Scan# 241
Delta R.T. -0.153 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 10970
Ion Ratio Lower Upper
43 100
74 0.0 22.8 34.2#

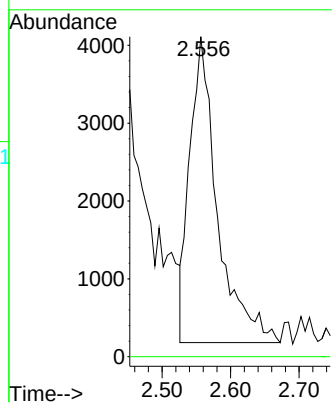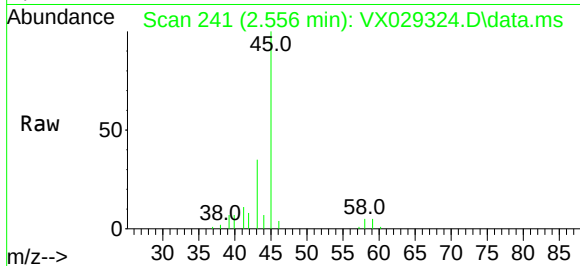

#20
Methylene Chloride
Concen: 2.218 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion: 84 Resp: 10987
Ion Ratio Lower Upper
84 100
49 113.1 85.5 128.3
51 37.4 26.6 39.8
86 65.9 51.5 77.3


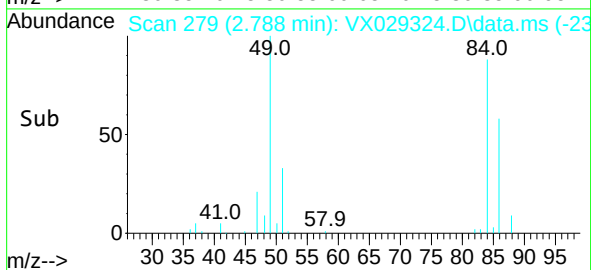

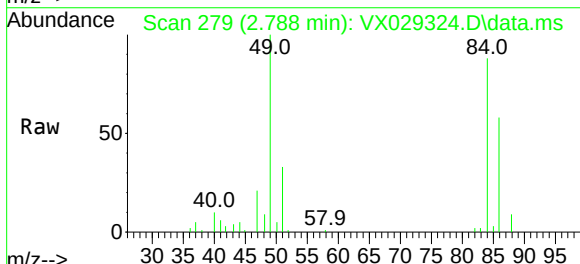




#23
 Vinyl Acetate
 Concen: 0.365 ug/l
 RT: 3.873 min Scan# 41
 Delta R.T. 0.146 min
 Lab File: VX029324.D
 Acq: 08 Jun 2022 16:23




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 43 Resp: 4045
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.8 16.2#

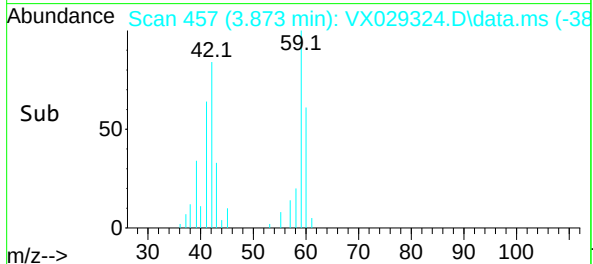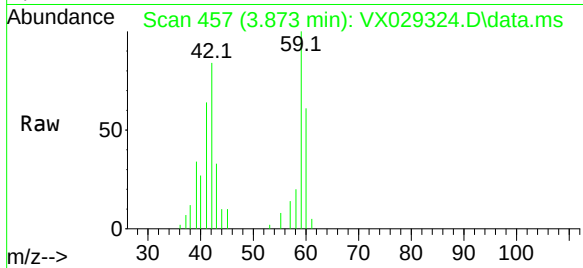

#25
 2-Butanone
 Concen: 3.763 ug/l
 RT: 4.568 min Scan# 571
 Delta R.T. 0.006 min
 Lab File: VX029324.D
 Acq: 08 Jun 2022 16:23

Tgt Ion: 43 Resp: 13204
 Ion Ratio Lower Upper
 43 100
 72 27.2 24.4 36.6

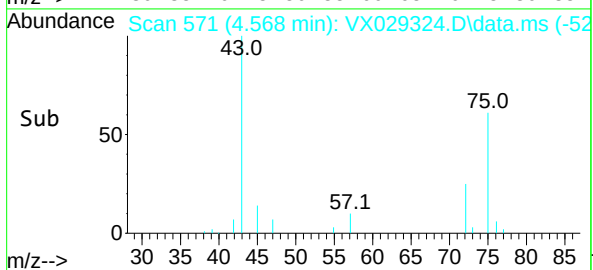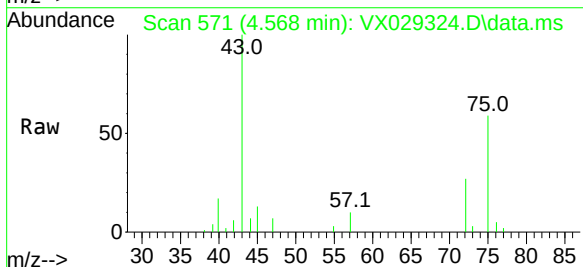



#29

Tetrahydrofuran

Concen: 0.284 ug/l

RT: 5.038 min Scan# 64

Delta R.T. 0.024 min

Lab File: VX029324.D





Acq: 08 Jun 2022 16:23

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:	42	Resp:	649
Ion	Ratio	Lower	Upper
42	100		
72	0.0	44.1	66.1#
71	9.6	40.5	60.7#

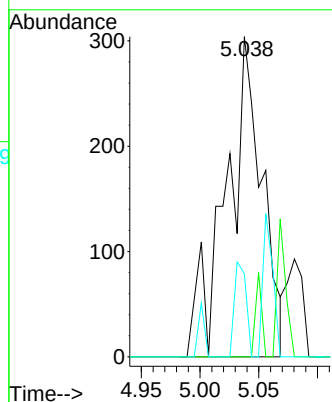

#31

Cyclohexane

Concen: 0.763 ug/l




RT: 5.556 min Scan# 733


Delta R.T. 0.079 min

Lab File: VX029324.D

Acq: 08 Jun 2022 16:23

Tgt Ion:	56	Resp:	5672
Ion	Ratio	Lower	Upper
56	100		
69	191.0	26.7	40.1#
84	145.4	77.2	115.8#

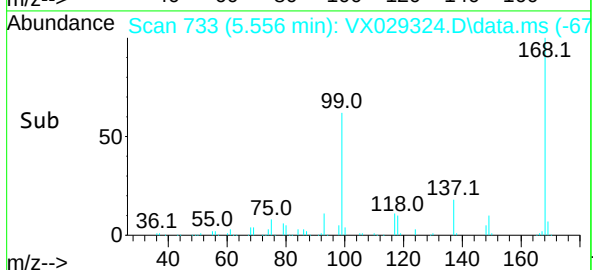



#33

1,2-Dichloroethane-d4

Concen: 62.712 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029324.D

Acq: 08 Jun 2022 16:23

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 259888

Ion Ratio Lower Upper

65 100

67 52.0 0.0 107.4

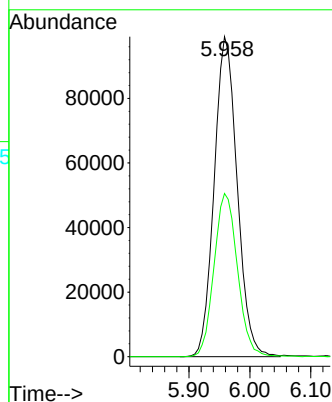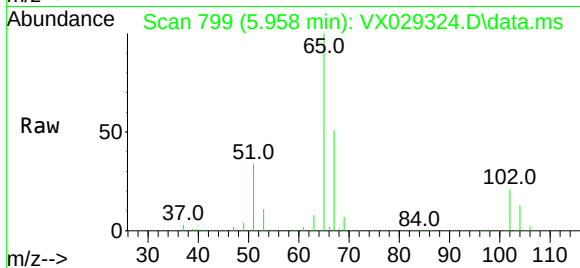

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX029324.D

Acq: 08 Jun 2022 16:23




Tgt Ion: 114 Resp: 461253


Ion Ratio Lower Upper

114 100

63 19.5 0.0 36.8

88 16.0 0.0 32.4

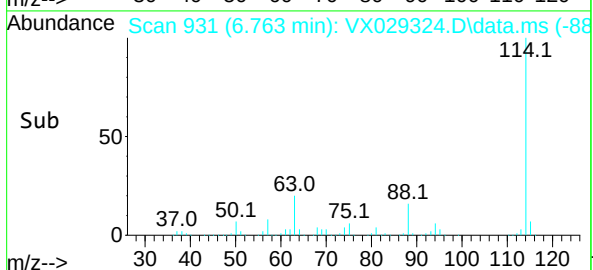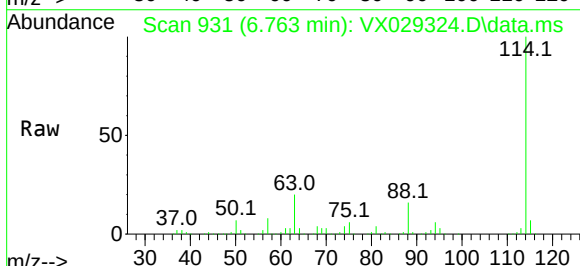



#35

Dibromofluoromethane

Concen: 13.363 ug/l

RT: 5.391 min Scan# 706

Delta R.T. -0.000 min


Lab File: VX029324.D

Acq: 08 Jun 2022 16:23

Instrument :

MSVOA_X

ClientSampleId :

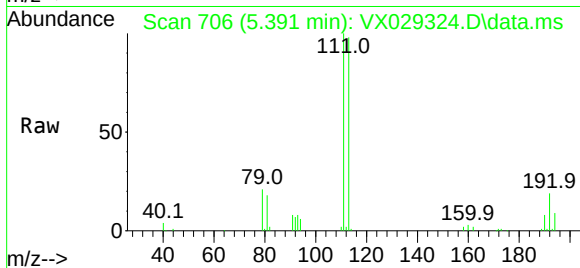




Tgt Ion:113 Resp: 52400

Ion Ratio Lower Upper

113 100

111 104.5 82.8 124.2

192 18.2 16.9 25.3

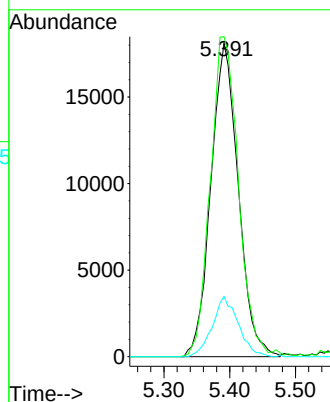

#36

1,1-Dichloropropene

Concen: 3.410 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.134 min

Lab File: VX029324.D

Acq: 08 Jun 2022 16:23




Tgt Ion: 75 Resp: 22087


Ion Ratio Lower Upper

75 100

110 10.0 18.3 54.8#

77 0.0 24.8 37.2#


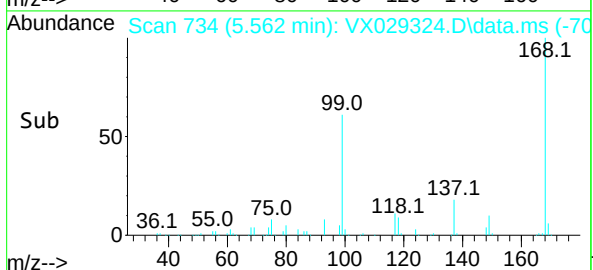
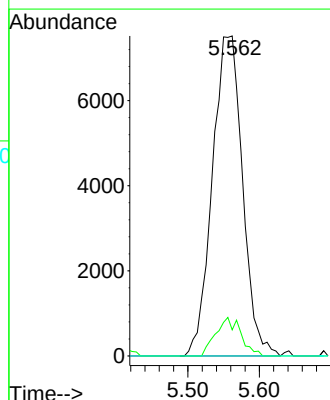
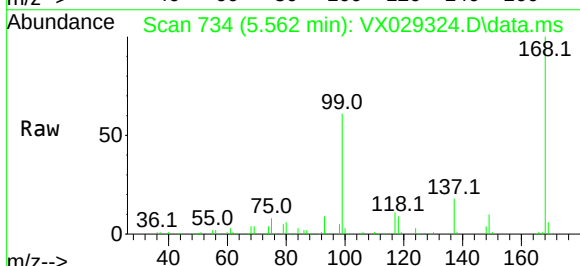




#37
Ethyl Acetate
Concen: 1.975 ug/l
RT: 4.568 min Scan# 51
Delta R.T. -0.153 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 13204
Ion Ratio Lower Upper
43 100
61 0.0 12.6 19.0#
70 0.0 10.2 15.2#

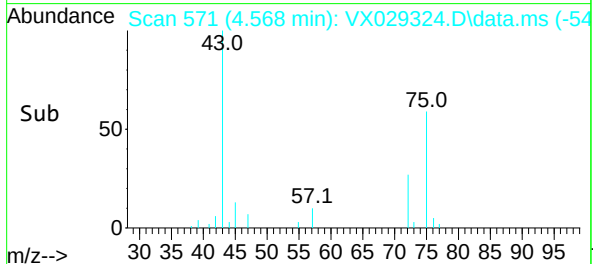

#38
Carbon Tetrachloride
Concen: 4.571 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion: 117 Resp: 30264
Ion Ratio Lower Upper
117 100
119 4.7 77.3 115.9#
121 0.0 24.2 36.2#


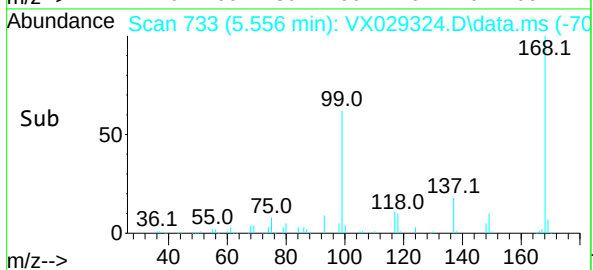

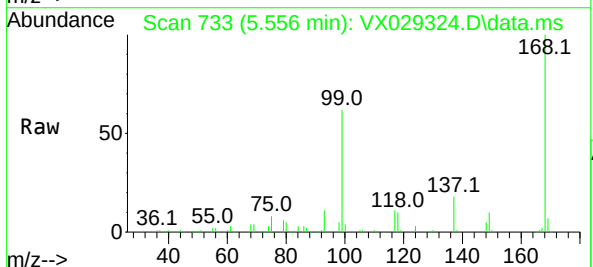




#40
Benzene
Concen: 4.213 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 78 Resp: 81241
Ion Ratio Lower Upper
78 100
77 22.0 19.3 28.9

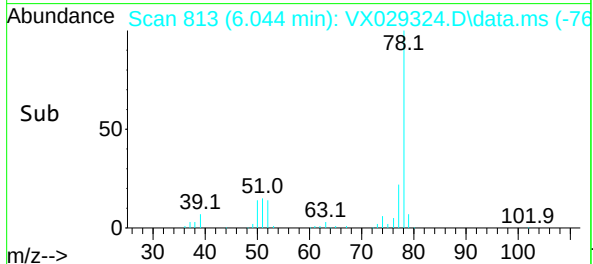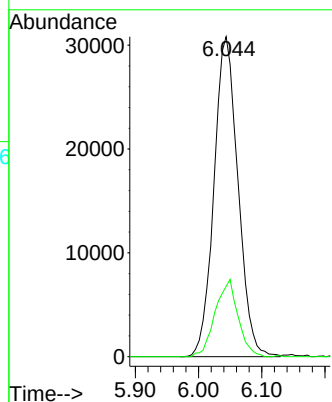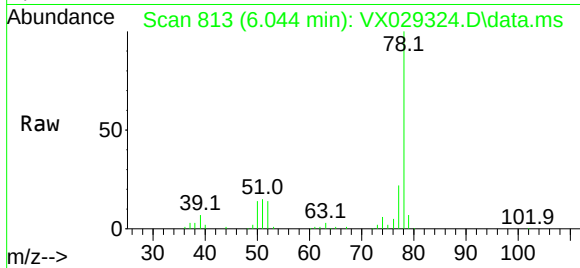

#41
Methacrylonitrile
Concen: Below Cal
RT: 5.019 min Scan# 645
Delta R.T. 0.091 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion: 41 Resp: 406
Ion Ratio Lower Upper
41 100
39 35.5 43.0 64.4#
67 0.0 70.2 105.4#
52 0.0 26.0 39.0#


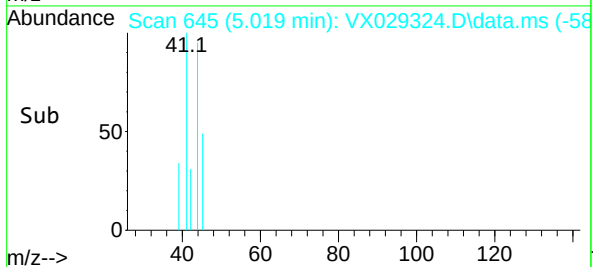

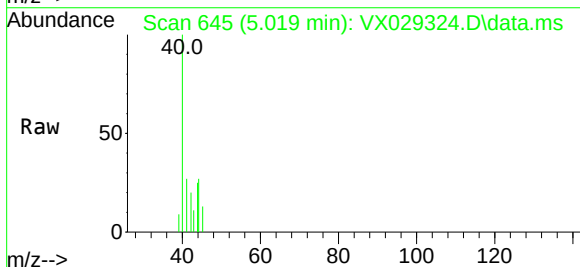




#48
Methyl methacrylate
Concen: 1.666 ug/l
RT: 7.604 min Scan# 1069
Delta R.T. -0.092 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 41 Resp: 8418
Ion Ratio Lower Upper
41 100
69 0.0 82.5 123.7#
39 16.4 43.8 65.8#

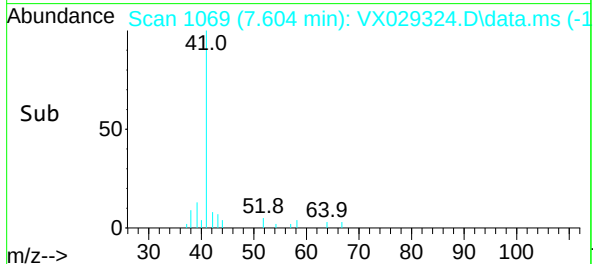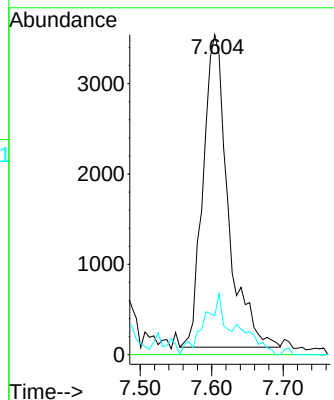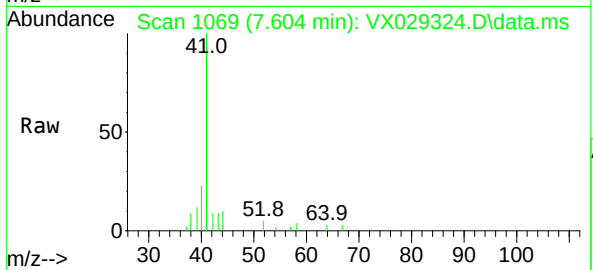

#50
Toluene-d8
Concen: 55.517 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion: 98 Resp: 769940
Ion Ratio Lower Upper
98 100
100 66.5 52.6 78.8



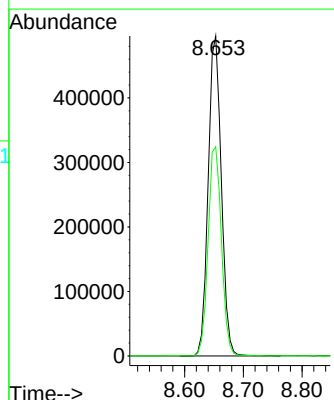
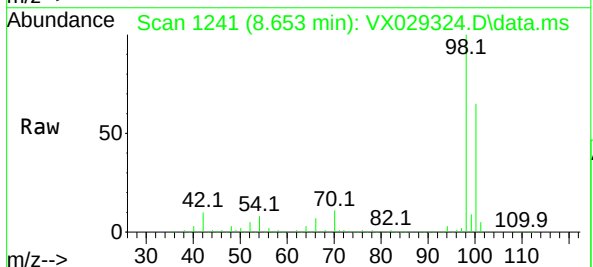




#51
4-Methyl-2-Pentanone
Concen: 1.139 ug/l
RT: 8.580 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 7487
Ion Ratio Lower Upper
43 100
58 38.7 36.1 54.1



#52
Toluene
Concen: 2.236 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion: 92 Resp: 27676
Ion Ratio Lower Upper
92 100
91 172.9 137.5 206.3

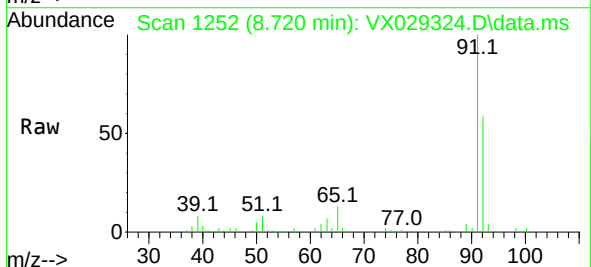



#53

t-1,3-Dichloropropene

Concen: 1.360 ug/l

RT: 8.726 min Scan# 11

Delta R.T. -0.256 min

Lab File: VX029324.D

Acq: 08 Jun 2022 16:23

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 317

Ion Ratio Lower Upper

75 100

77 112.8 25.4 38.0#

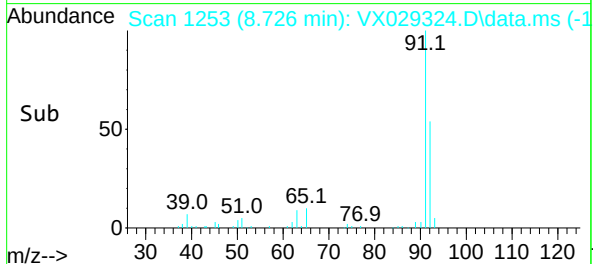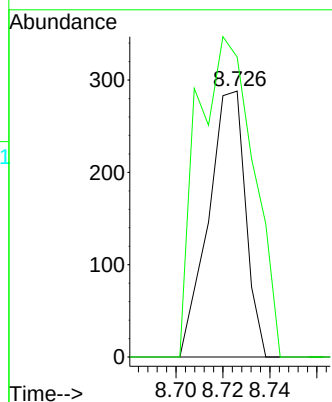

#59

2-Hexanone

Concen: 0.324 ug/l

RT: 9.439 min Scan# 1370

Delta R.T. 0.006 min

Lab File: VX029324.D




Acq: 08 Jun 2022 16:23


Tgt Ion: 43 Resp: 1620

Ion Ratio Lower Upper

43 100

58 51.4 31.9 95.7


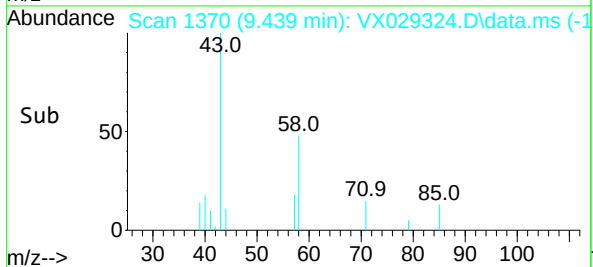
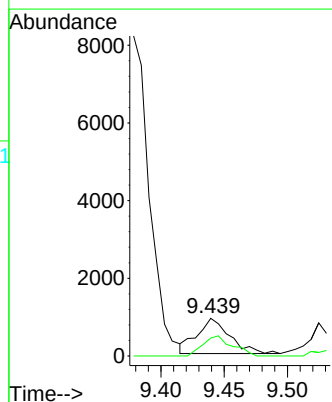
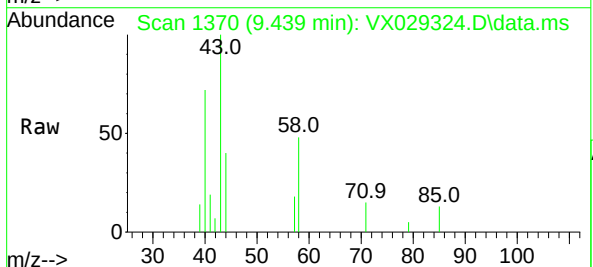




#62
4-Bromofluorobenzene
Concen: 53.678 ug/l
RT: 11.085 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 291322
Ion Ratio Lower Upper
95 100
174 72.2 0.0 163.0
176 69.6 0.0 155.0

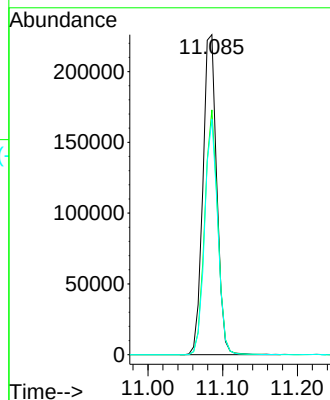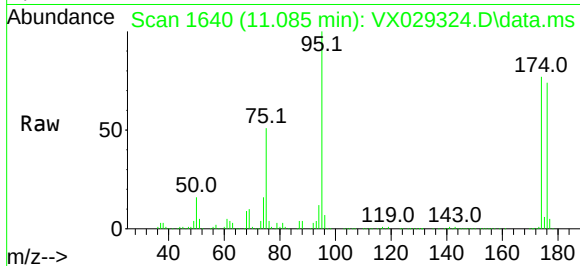

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion:117 Resp: 397758
Ion Ratio Lower Upper
117 100
82 58.2 41.8 62.8
119 32.7 24.8 37.2


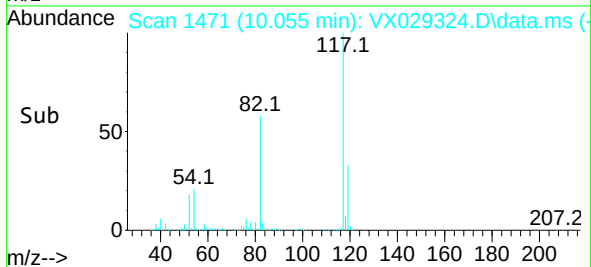
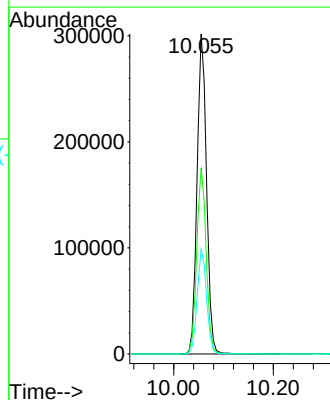
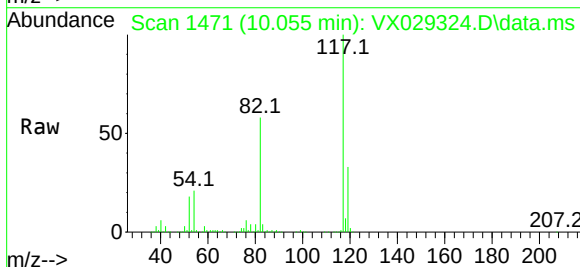




#67
Ethyl Benzene
Concen: 2.361 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 45489
Ion Ratio Lower Upper
91 100
106 31.0 24.6 36.8

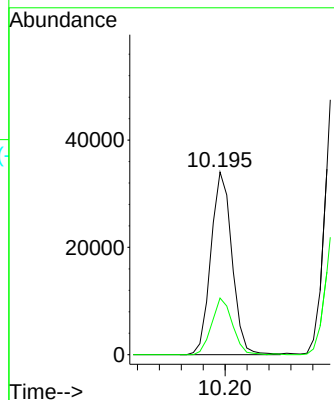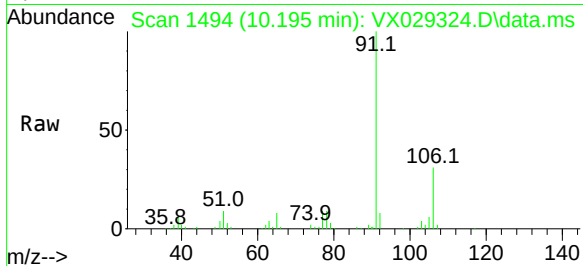

#68
m/p-Xylenes
Concen: 5.401 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion: 106 Resp: 40269
Ion Ratio Lower Upper
106 100
91 209.2 160.4 240.6



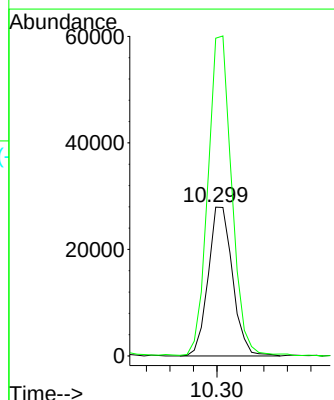
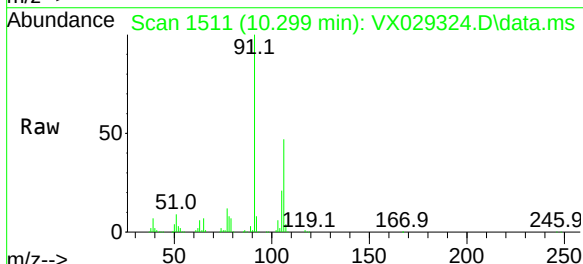




#69
o-Xylene
Concen: 3.227 ug/l
RT: 10.646 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 23382
Ion Ratio Lower Upper
106 100
91 221.0 106.1 318.1

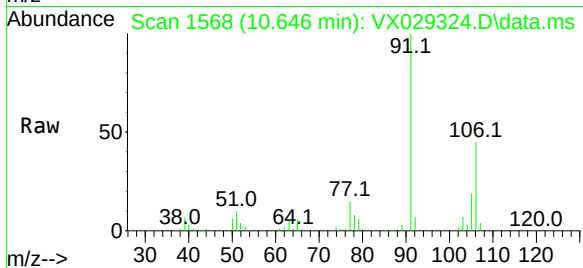

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion:152 Resp: 175947
Ion Ratio Lower Upper
152 100
115 63.1 37.5 112.7
150 157.2 0.0 338.2


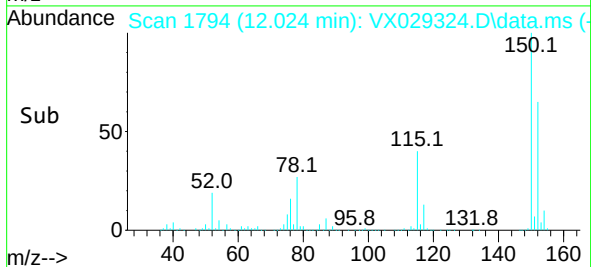

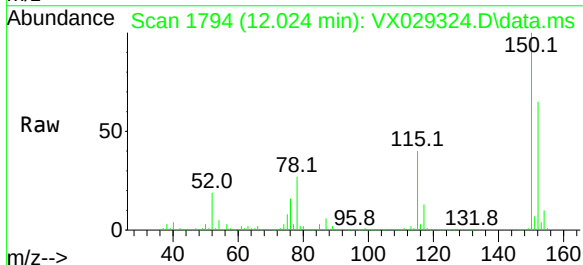




#73
Isopropylbenzene
Concen: 0.272 ug/l
RT: 10.963 min Scan# 1640
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 3766
Ion Ratio Lower Upper
105 100
120 26.5 13.5 40.5

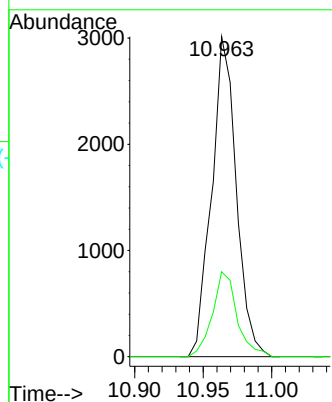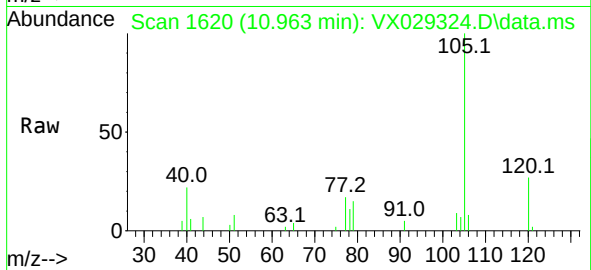

#76
1,2,3-Trichloropropane
Concen: 35.840 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23


Tgt Ion: 75 Resp: 147289
Ion Ratio Lower Upper
75 100
77 1.1 19.4 58.2#

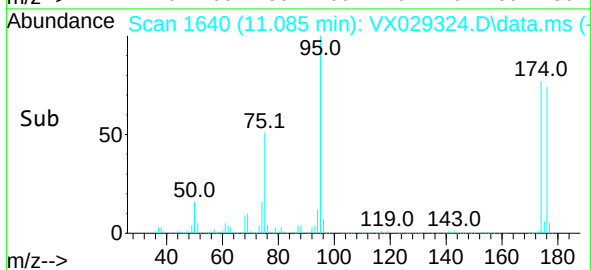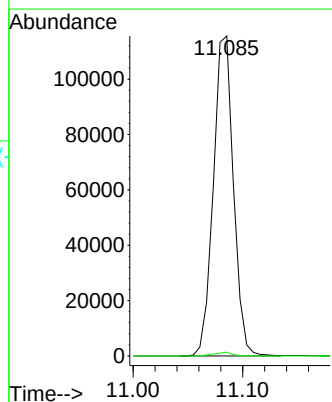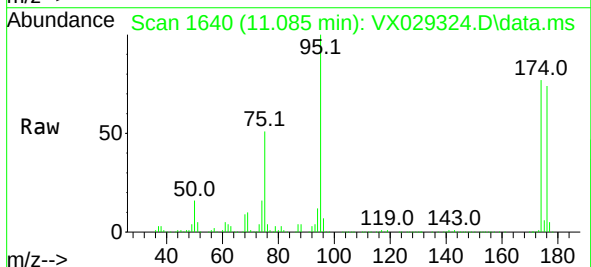






#80
1,3,5-Trimethylbenzene
Concen: 0.464 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23


Instrument :
MSVOA_X
ClientSampleId :

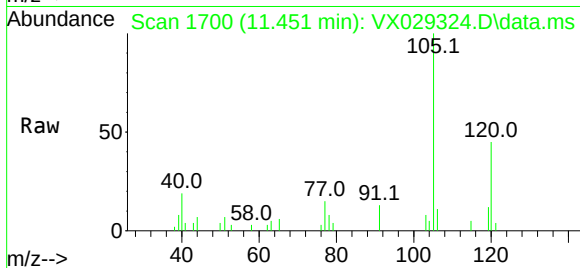



Tgt Ion:105 Resp: 5454
Ion Ratio Lower Upper
105 100
120 48.1 24.3 72.9




#81
trans-1,4-Dichloro-2-butene
Concen: 108.752 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

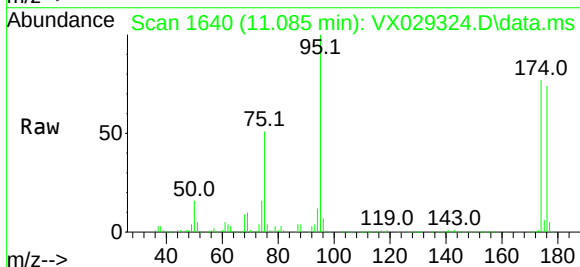

Tgt Ion: 75 Resp: 147289
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#



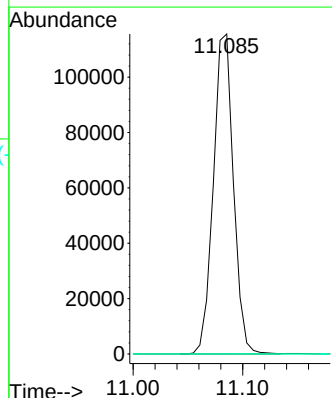
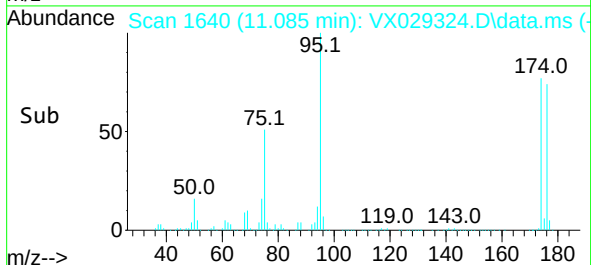




#84
1,2,4-Trimethylbenzene
Concen: 2.010 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 23333
Ion Ratio Lower Upper
105 100
120 42.8 22.6 67.8

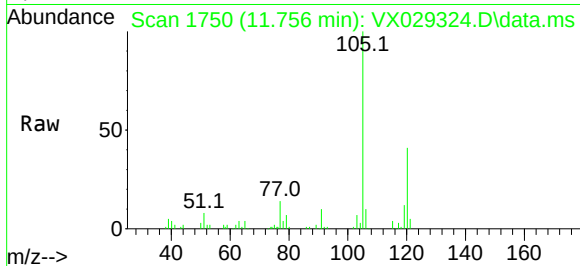

#85
sec-Butylbenzene
Concen: 1.665 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Tgt Ion:105 Resp: 23333
Ion Ratio Lower Upper
105 100
134 0.0 10.2 30.4#

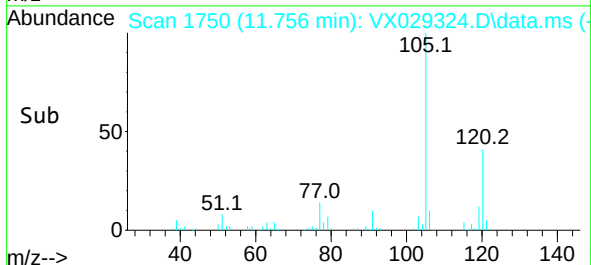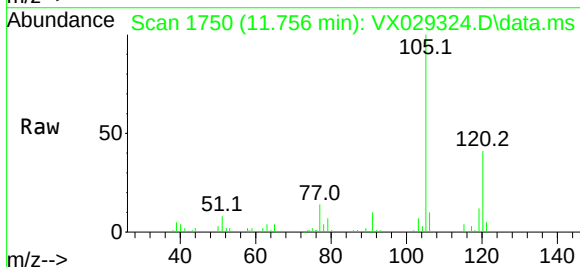



#89

n-Butylbenzene

Concen: 2.818 ug/l

RT: 12.244 min Scan# 11

Delta R.T. -0.092 min

Lab File: VX029324.D





Acq: 08 Jun 2022 16:23

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 91	Resp: 27912
Ion Ratio	Lower Upper
91	100
92	9.5 27.8 83.3#
134	0.2 13.3 39.8#

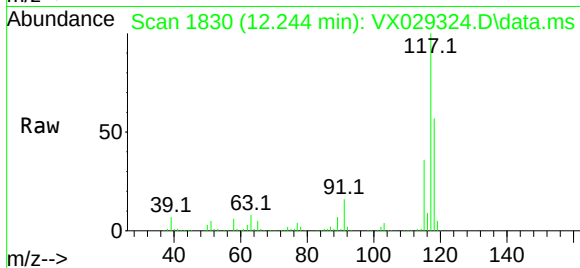

#90

Hexachloroethane

Concen: 5.461 ug/l




RT: 12.414 min Scan# 1858


Delta R.T. -0.128 min

Lab File: VX029324.D

Acq: 08 Jun 2022 16:23


Tgt Ion: 117	Resp: 10199
Ion Ratio	Lower Upper
117	100
201	0.0 39.5 118.5#

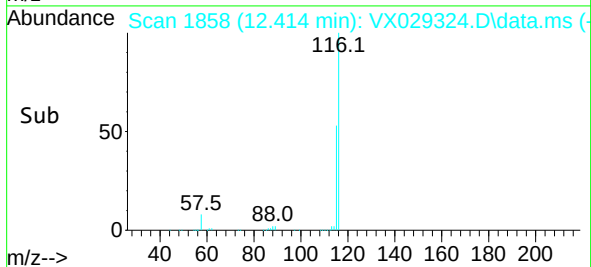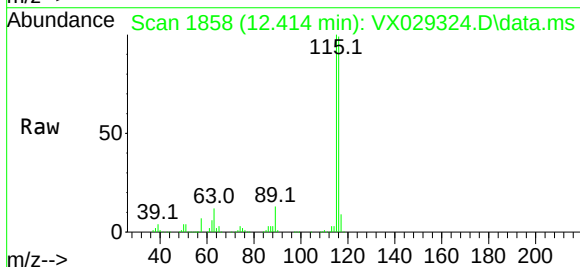

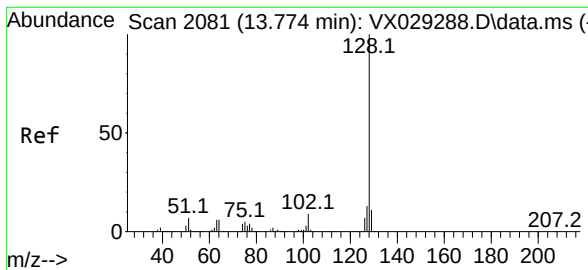

#95
Naphthalene
Concen: 394.016 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX029324.D
Acq: 08 Jun 2022 16:23

Instrument :
MSVOA_X
ClientSampleId :

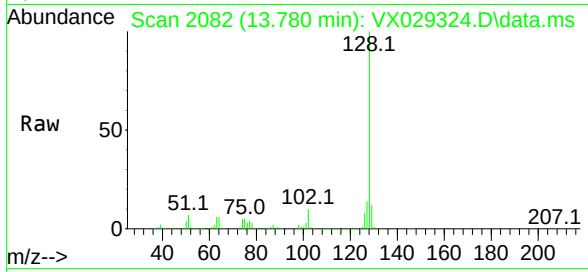

Tgt Ion:128 Resp: 5051680
Ion Ratio Lower Upper
128 100
127 13.7 10.2 15.4
129 11.9 8.7 13.1

