

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060822\
 Data File : VX029335.D
 Acq On : 08 Jun 2022 20:40
 Operator : JC/MD
 Sample : N3175-21 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-1713

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M

Title : SW846 8260

Signal : TIC: VX029335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	25	28	32	rBV	50822	43607	2.07%	0.444%
2	2.946	296	305	315	rBV	55722	131702	6.27%	1.341%
3	4.580	561	573	586	rBV2	12485	43876	2.09%	0.447%
4	5.391	693	706	720	rBV	242578	696068	33.11%	7.086%
5	5.556	722	733	747	rVV	322499	906155	43.11%	9.225%
6	5.958	789	799	817	rBV	267111	712180	33.88%	7.250%
7	6.763	922	931	942	rBV	473855	1137614	54.12%	11.581%
8	6.879	944	950	963	rVB2	51147	127715	6.08%	1.300%
9	7.214	998	1005	1014	rBV	34236	72952	3.47%	0.743%
10	8.653	1234	1241	1258	rBV	1335588	2102022	100.00%	21.400%
11	9.567	1386	1391	1406	rBV2	9037	30780	1.46%	0.313%
12	10.055	1465	1471	1483	rBV	963467	1273984	60.61%	12.970%
13	11.085	1634	1640	1654	rVB	1070257	1375281	65.43%	14.001%
14	12.024	1781	1794	1802	rBV	941691	1137710	54.12%	11.582%
15	12.219	1820	1826	1834	rBV	20439	31096	1.48%	0.317%




Sum of corrected areas: 9822742

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060822\
Data File : VX029335.D
Acq On : 08 Jun 2022 20:40
Operator : JC/MD
Sample : N3175-21 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1713

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

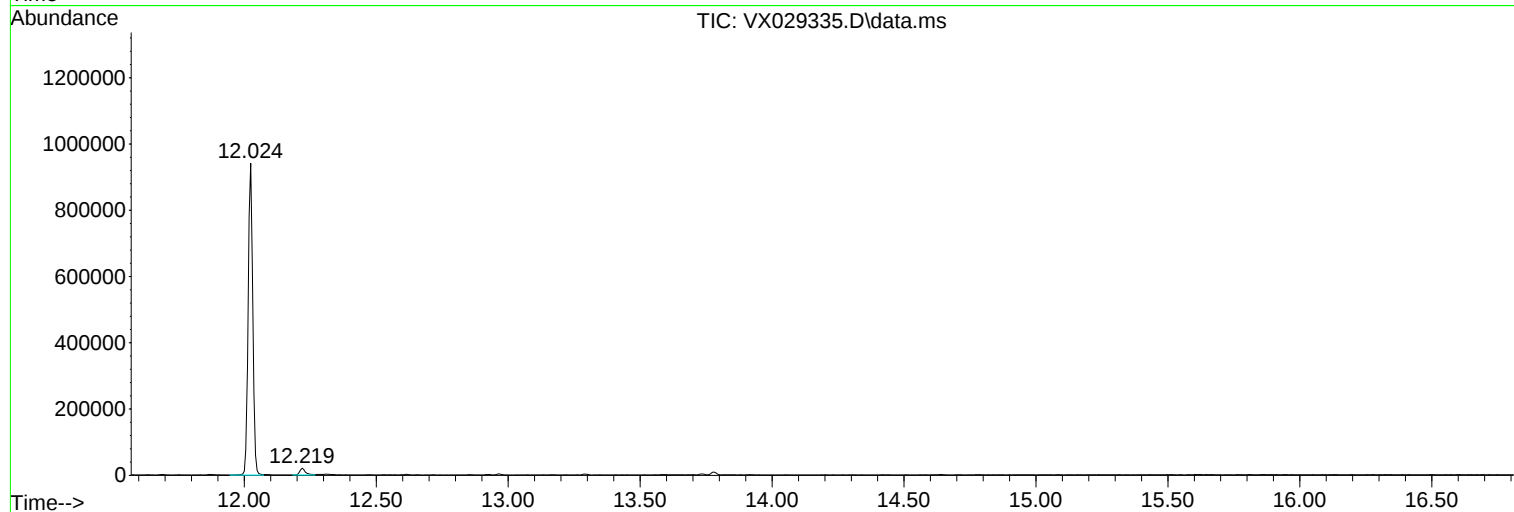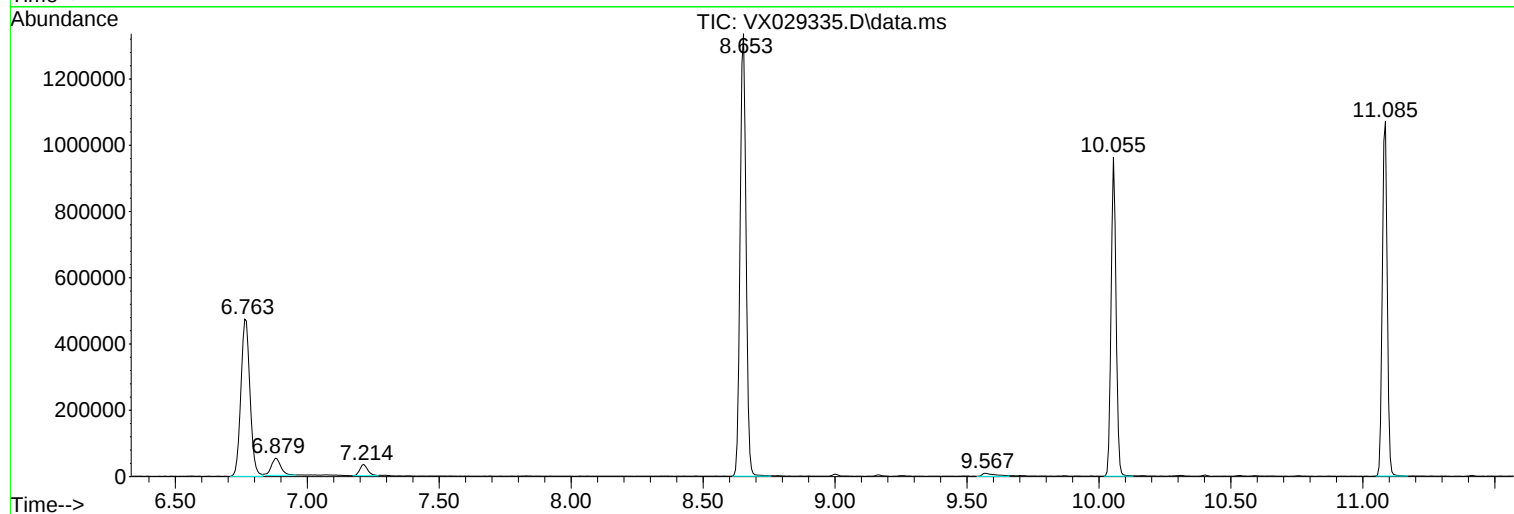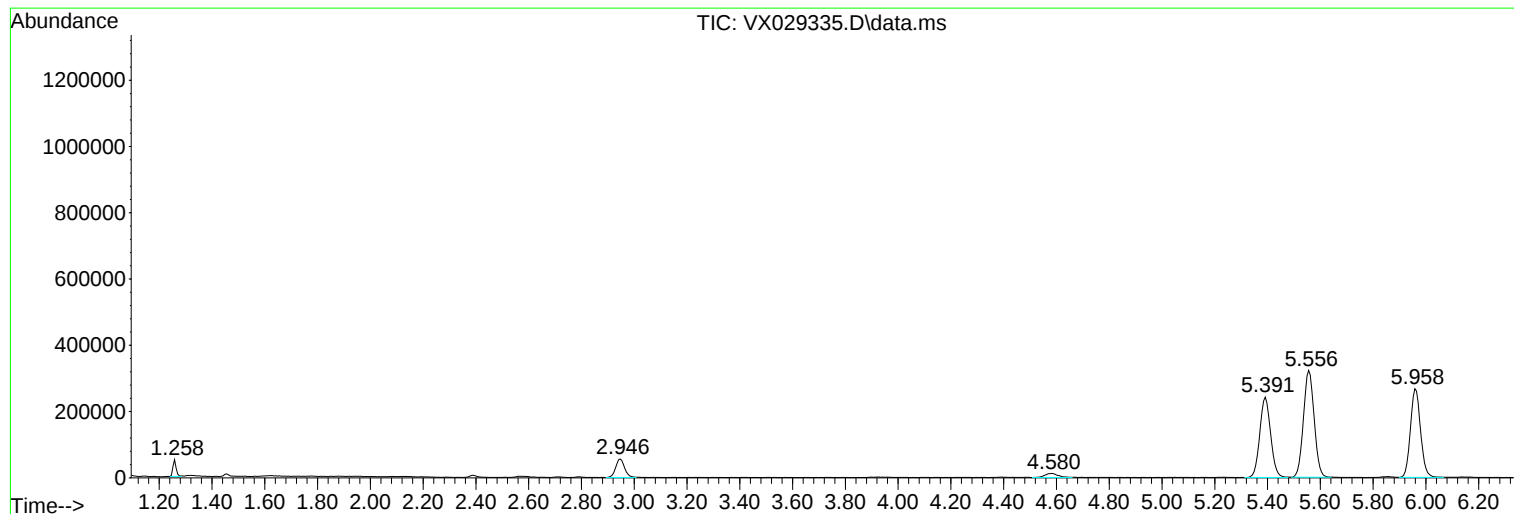

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060822\
Data File : VX029335.D
Acq On : 08 Jun 2022 20:40
Operator : JC/MD
Sample : N3175-21 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1713










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1,3-Dioxane, 2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.879	5.61 ug/l	127715	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Dioxane, 2-methyl-	102	C5H10O2	000626-68-6	50
2			2-(2-Methoxyethoxy)ethyl acetate	162	C7H14O4	1000351-95-4	42
3			Oxirane, (propoxymethyl)-	116	C6H12O2	003126-95-2	32
4			1,3-Dioxolane, 4-methyl-2-propyl-	130	C7H14O2	004352-99-2	28
5			2H-1,2-Oxazine,tetrahydro-	87	C4H9NO	036652-42-3	17

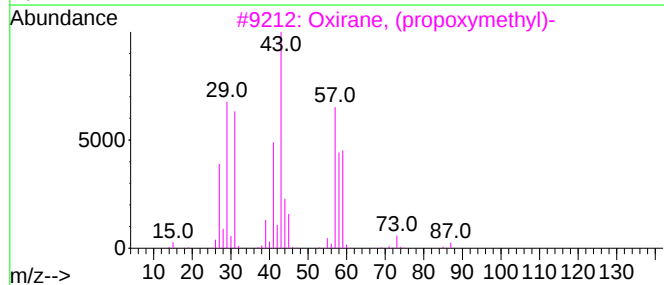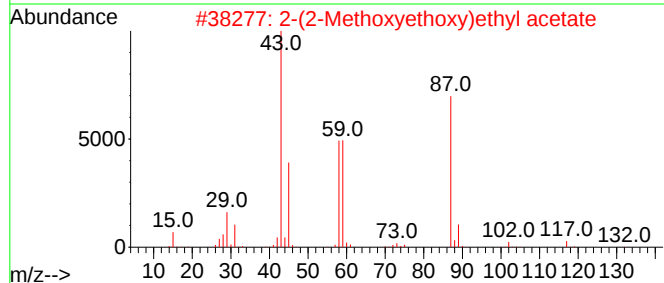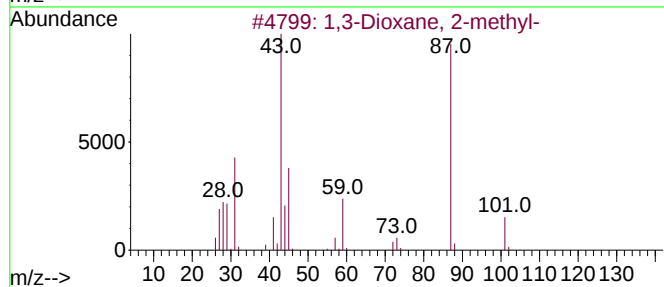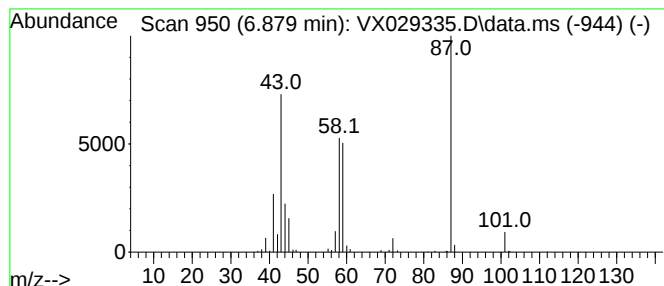

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060822\
Data File : VX029335.D
Acq On : 08 Jun 2022 20:40
Operator : JC/MD
Sample : N3175-21 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1713

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,3-Dioxane, 2-...	6.879	5.6	ug/l	127715	2	6.763	1137610	50.0