


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060822\
 Data File : VX029312.D
 Acq On : 08 Jun 2022 10:10
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
 Title : SW846 8260
 Last Update : Wed Jun 08 03:00:38 2022

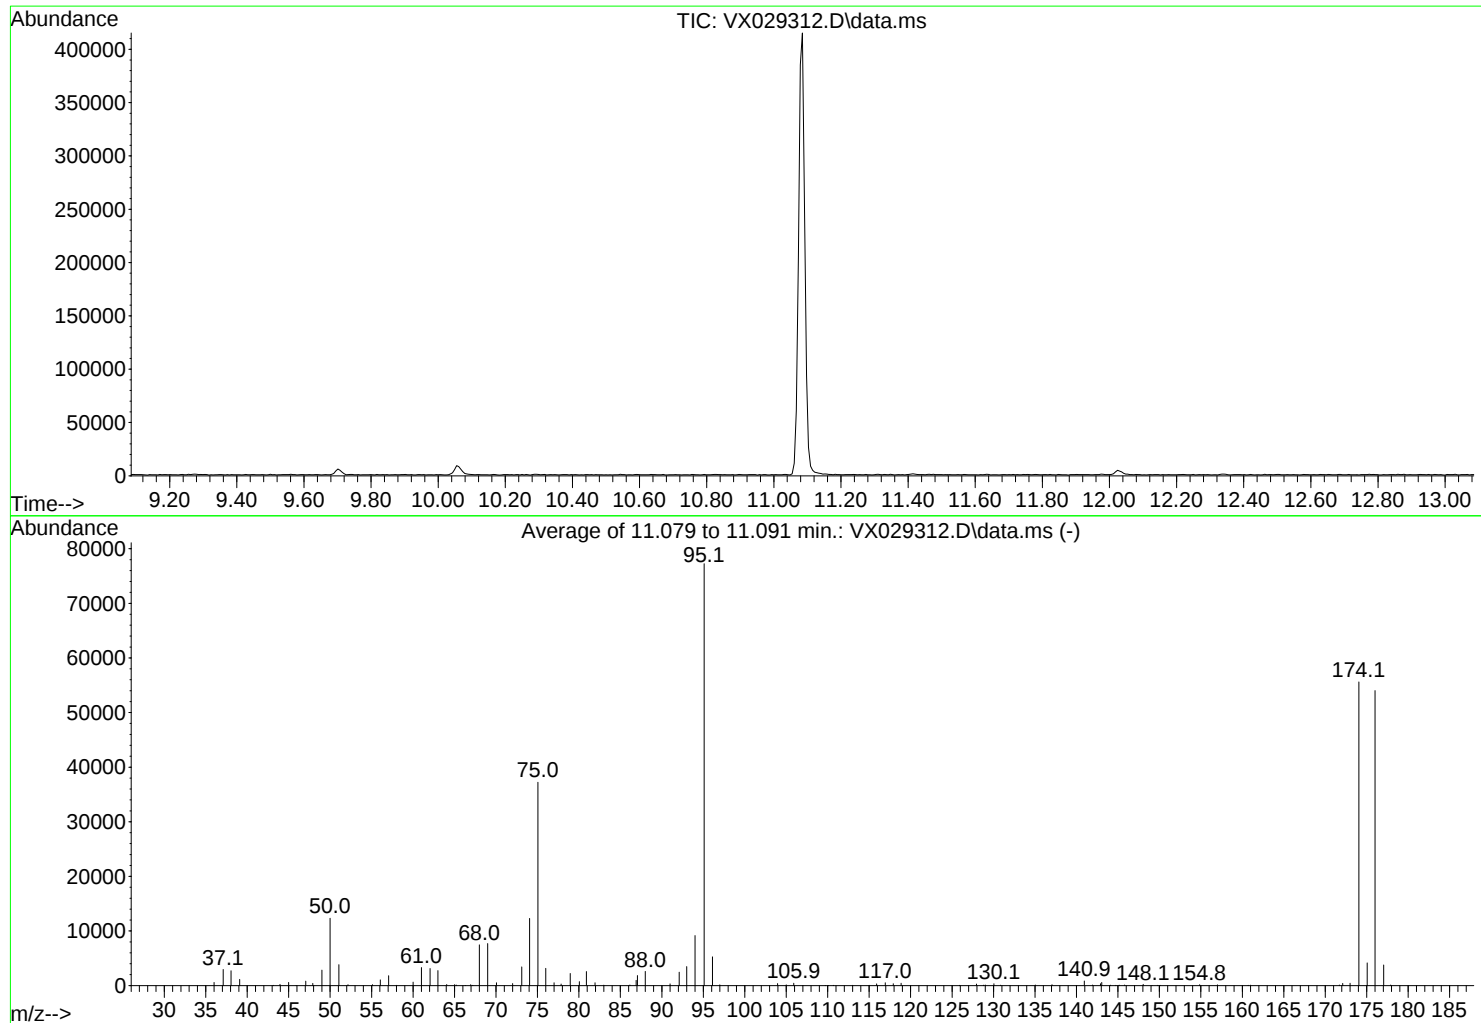

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	12338	PASS
75	95	30	60	48.2	37221	PASS
95	95	100	100	100.0	77251	PASS
96	95	5	9	6.8	5271	PASS
173	174	0.00	2	0.8	440	PASS
174	95	50	100	72.0	55595	PASS
175	174	5	9	7.5	4158	PASS
176	174	95	101	97.2	54029	PASS
177	176	5	9	6.9	3755	PASS