

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036074.D
 Acq On : 08 Jun 2023 16:42
 Operator : JC/MD
 Sample : 03097-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZER3

Quant Time: Jun 09 02:23:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 07 05:37:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	312028	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	282922	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	130388	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	98486	46.457	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.920%
7) Chloroethane-d5	1.672	69	78959	48.564	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.120%
11) 1,1-Dichloroethene-d2	2.306	65	50786	47.249	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.500%
21) 2-Butanone-d5	4.471	46	166333	95.722	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.720%
24) Chloroform-d	5.056	84	204907	46.352	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.700%
26) 1,2-Dichloroethane-d4	5.958	65	158031	48.991	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.980%
32) Benzene-d6	5.970	84	414197	48.666	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.340%
36) 1,2-Dichloropropane-d6	7.306	67	129322	48.886	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.780%
41) Toluene-d8	8.647	98	369989	47.232	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.460%
43) trans-1,3-Dichloroprop...	8.952	79	55257	43.515	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.020%
47) 2-Hexanone-d5	9.384	63	114434	97.146	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.150%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	167513	46.359	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.720%
66) 1,2-Dichlorobenzene-d4	12.317	152	126701	50.050	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.100%
Target Compounds						
13) Acetone	2.410	43	9451	5.148	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036074.D
Acq On : 08 Jun 2023 16:42
Operator : JC/MD
Sample : 03097-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZER3

Quant Time: Jun 09 02:23:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 07 05:37:48 2023
Response via : Initial Calibration

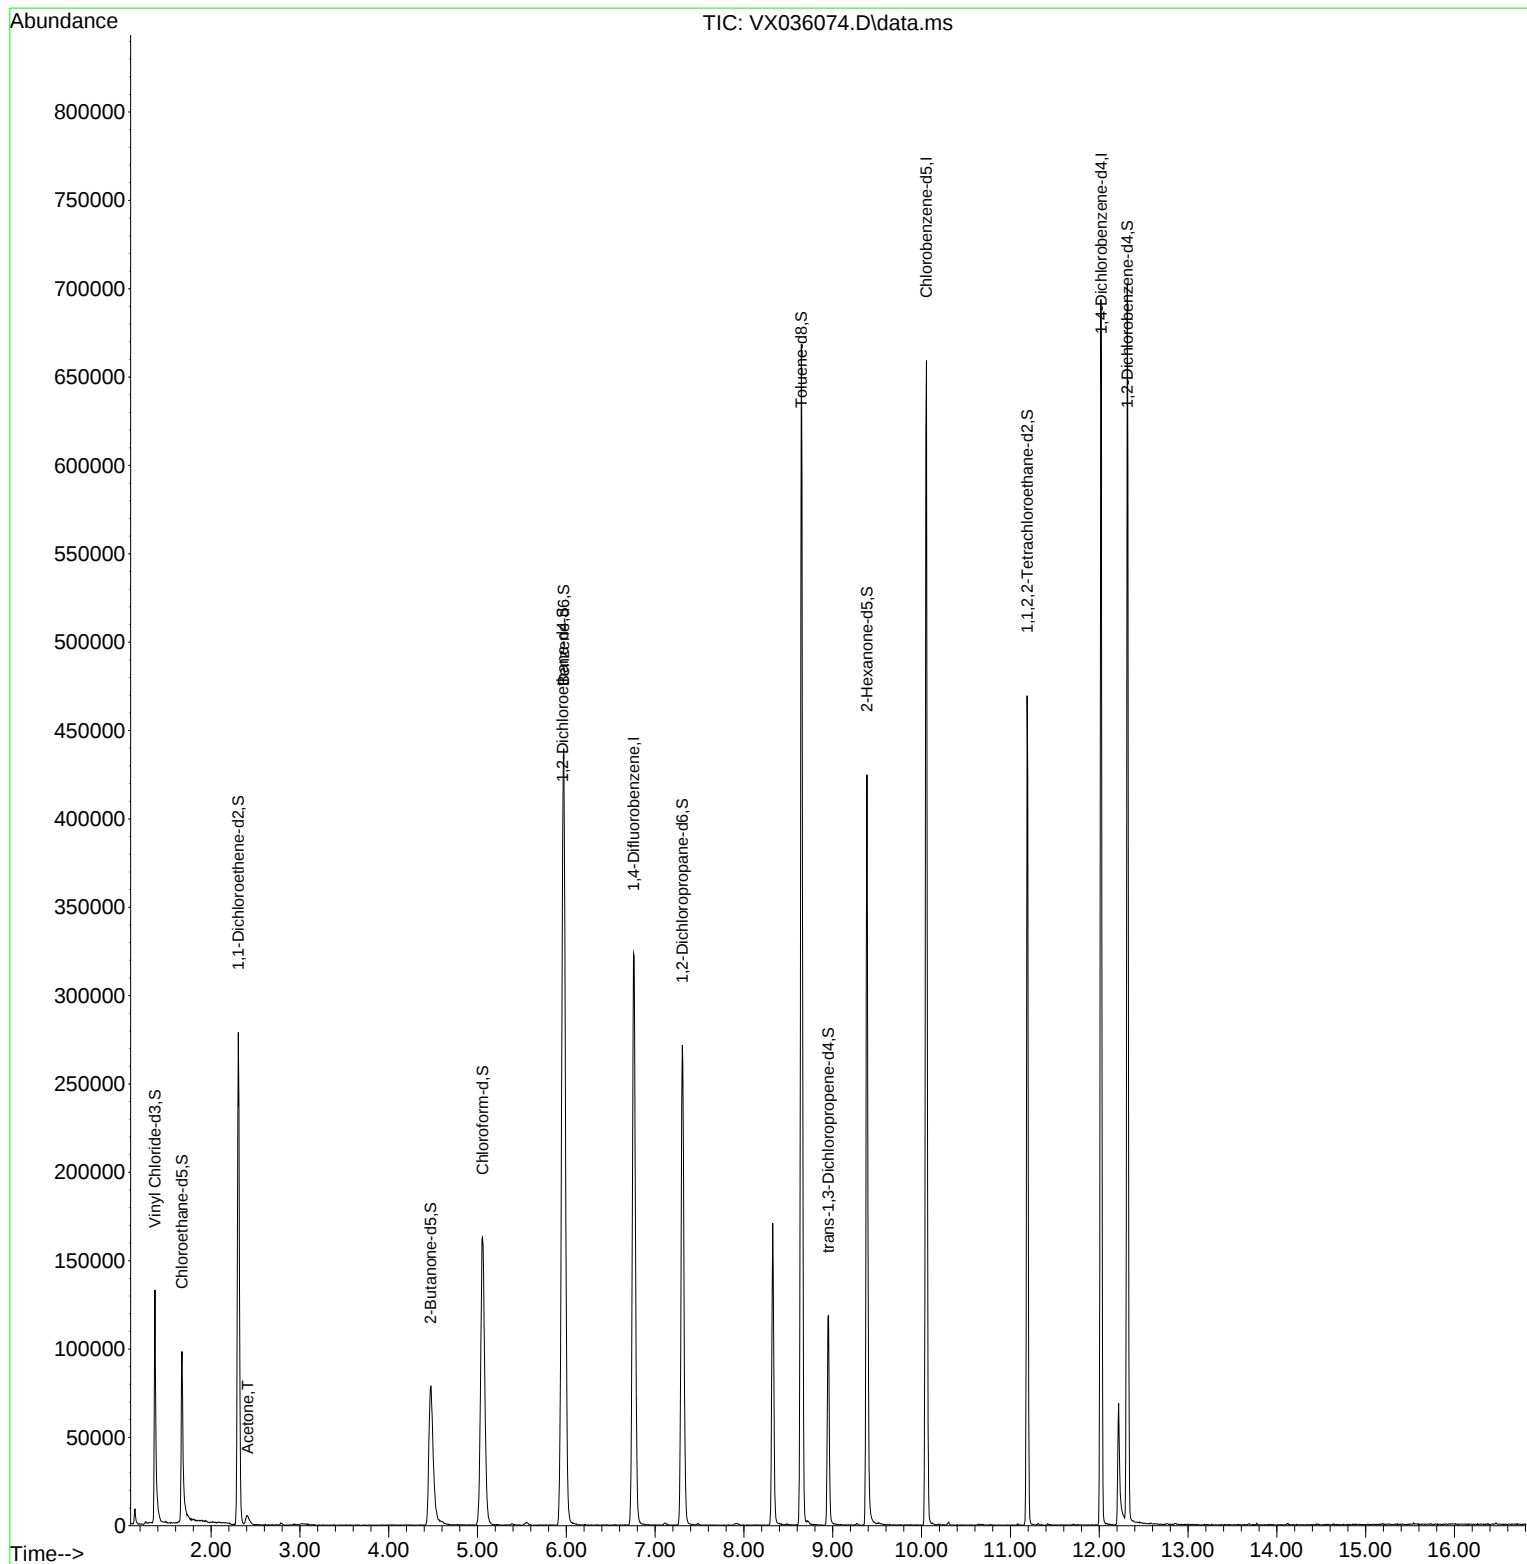

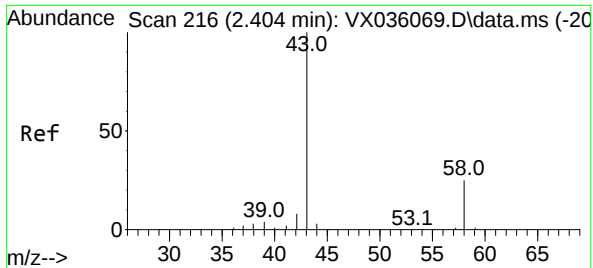

#13
 Acetone
 Concen: 5.148 ug/L
 RT: 2.410 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX036074.D
 Acq: 08 Jun 2023 16:42

Instrument :
 MSVOA_X
 ClientSampleId :
 EZER3

Tgt Ion: 43 Resp: 9451
 Ion Ratio Lower Upper
 43 100
 58 26.3 0.0 55.4

