

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036075.D
 Acq On : 08 Jun 2023 17:05
 Operator : JC/MD
 Sample : 03097-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZER4

Quant Time: Jun 09 02:23:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 07 05:37:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	334810	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	301165	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	130814	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	100436	44.153	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.300%		
7) Chloroethane-d5	1.673	69	80924	46.386	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.780%		
11) 1,1-Dichloroethene-d2	2.307	65	53104	46.044	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.080%		
21) 2-Butanone-d5	4.471	46	168684	90.470	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.470%		
24) Chloroform-d	5.056	84	212997	44.904	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.800%		
26) 1,2-Dichloroethane-d4	5.958	65	163838	47.335	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.680%		
32) Benzene-d6	5.971	84	431642	47.644	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.280%		
36) 1,2-Dichloropropane-d6	7.306	67	134619	47.805	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.620%		
41) Toluene-d8	8.647	98	386797	46.387	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.780%		
43) trans-1,3-Dichloroprop...	8.946	79	56812	42.029	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.060%		
47) 2-Hexanone-d5	9.385	63	114261	91.123	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.120%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	167456	43.536	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.080%		
66) 1,2-Dichlorobenzene-d4	12.317	152	123440	48.603	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.200%		
Target Compounds					Qvalue	
13) Acetone	2.416	43	6793	3.448	ug/L	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036075.D
Acq On : 08 Jun 2023 17:05
Operator : JC/MD
Sample : 03097-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZER4

Quant Time: Jun 09 02:23:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 07 05:37:48 2023
Response via : Initial Calibration

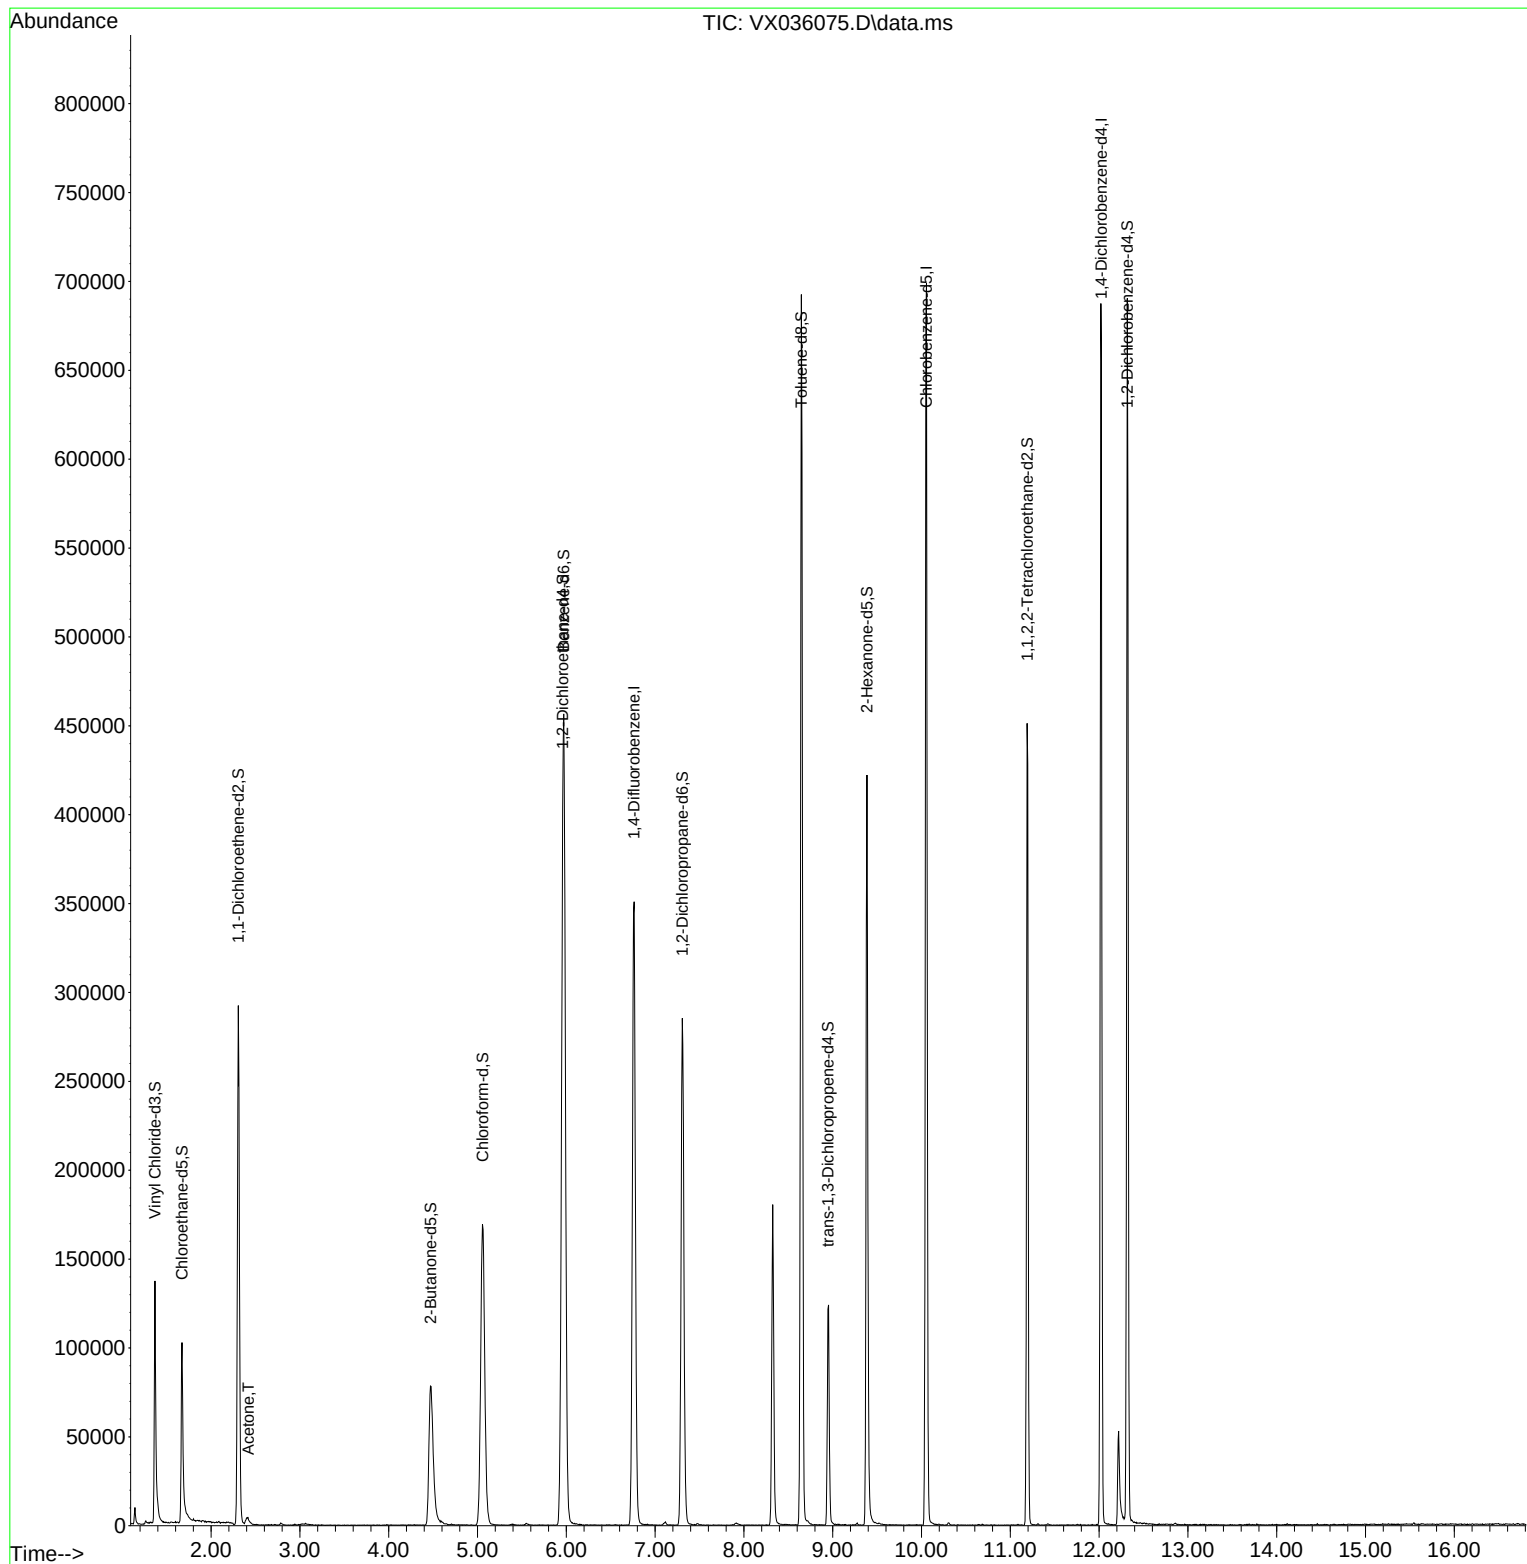

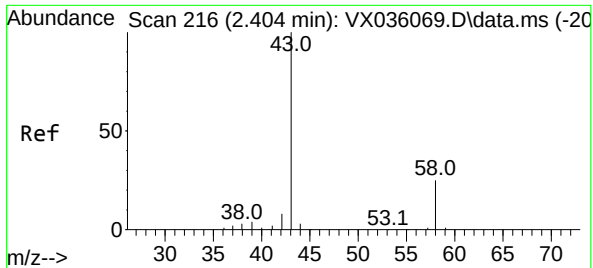

#13
 Acetone
 Concen: 3.448 ug/L
 RT: 2.416 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX036075.D
 Acq: 08 Jun 2023 17:05

Instrument :
 MSVOA_X
 ClientSampleId :
 EZER4

Tgt Ion: 43 Resp: 6793
 Ion Ratio Lower Upper
 43 100
 58 5.4 0.0 55.4

