

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036076.D
 Acq On : 08 Jun 2023 17:28
 Operator : JC/MD
 Sample : 03097-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZES1

Quant Time: Jun 09 02:23:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 07 05:37:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	320023	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	289983	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	130911	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	102015	46.919	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.840%
7) Chloroethane-d5	1.673	69	82697	49.593	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.180%
11) 1,1-Dichloroethene-d2	2.307	65	54009	48.992	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.980%
21) 2-Butanone-d5	4.471	46	167874	94.195	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.200%
24) Chloroform-d	5.056	84	215610	47.555	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.100%
26) 1,2-Dichloroethane-d4	5.958	65	164805	49.814	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.620%
32) Benzene-d6	5.971	84	431751	49.494	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.980%
36) 1,2-Dichloropropane-d6	7.306	67	135347	49.917	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.840%
41) Toluene-d8	8.647	98	390265	48.608	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.220%
43) trans-1,3-Dichloroprop...	8.952	79	56669	43.540	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.080%
47) 2-Hexanone-d5	9.385	63	116080	96.144	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.140%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	170733	46.100	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	12.317	152	129237	50.848	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.700%
Target Compounds						
					Qvalue	
13) Acetone	2.410	43	7055	3.747	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036076.D
Acq On : 08 Jun 2023 17:28
Operator : JC/MD
Sample : 03097-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZES1

Quant Time: Jun 09 02:23:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 07 05:37:48 2023
Response via : Initial Calibration

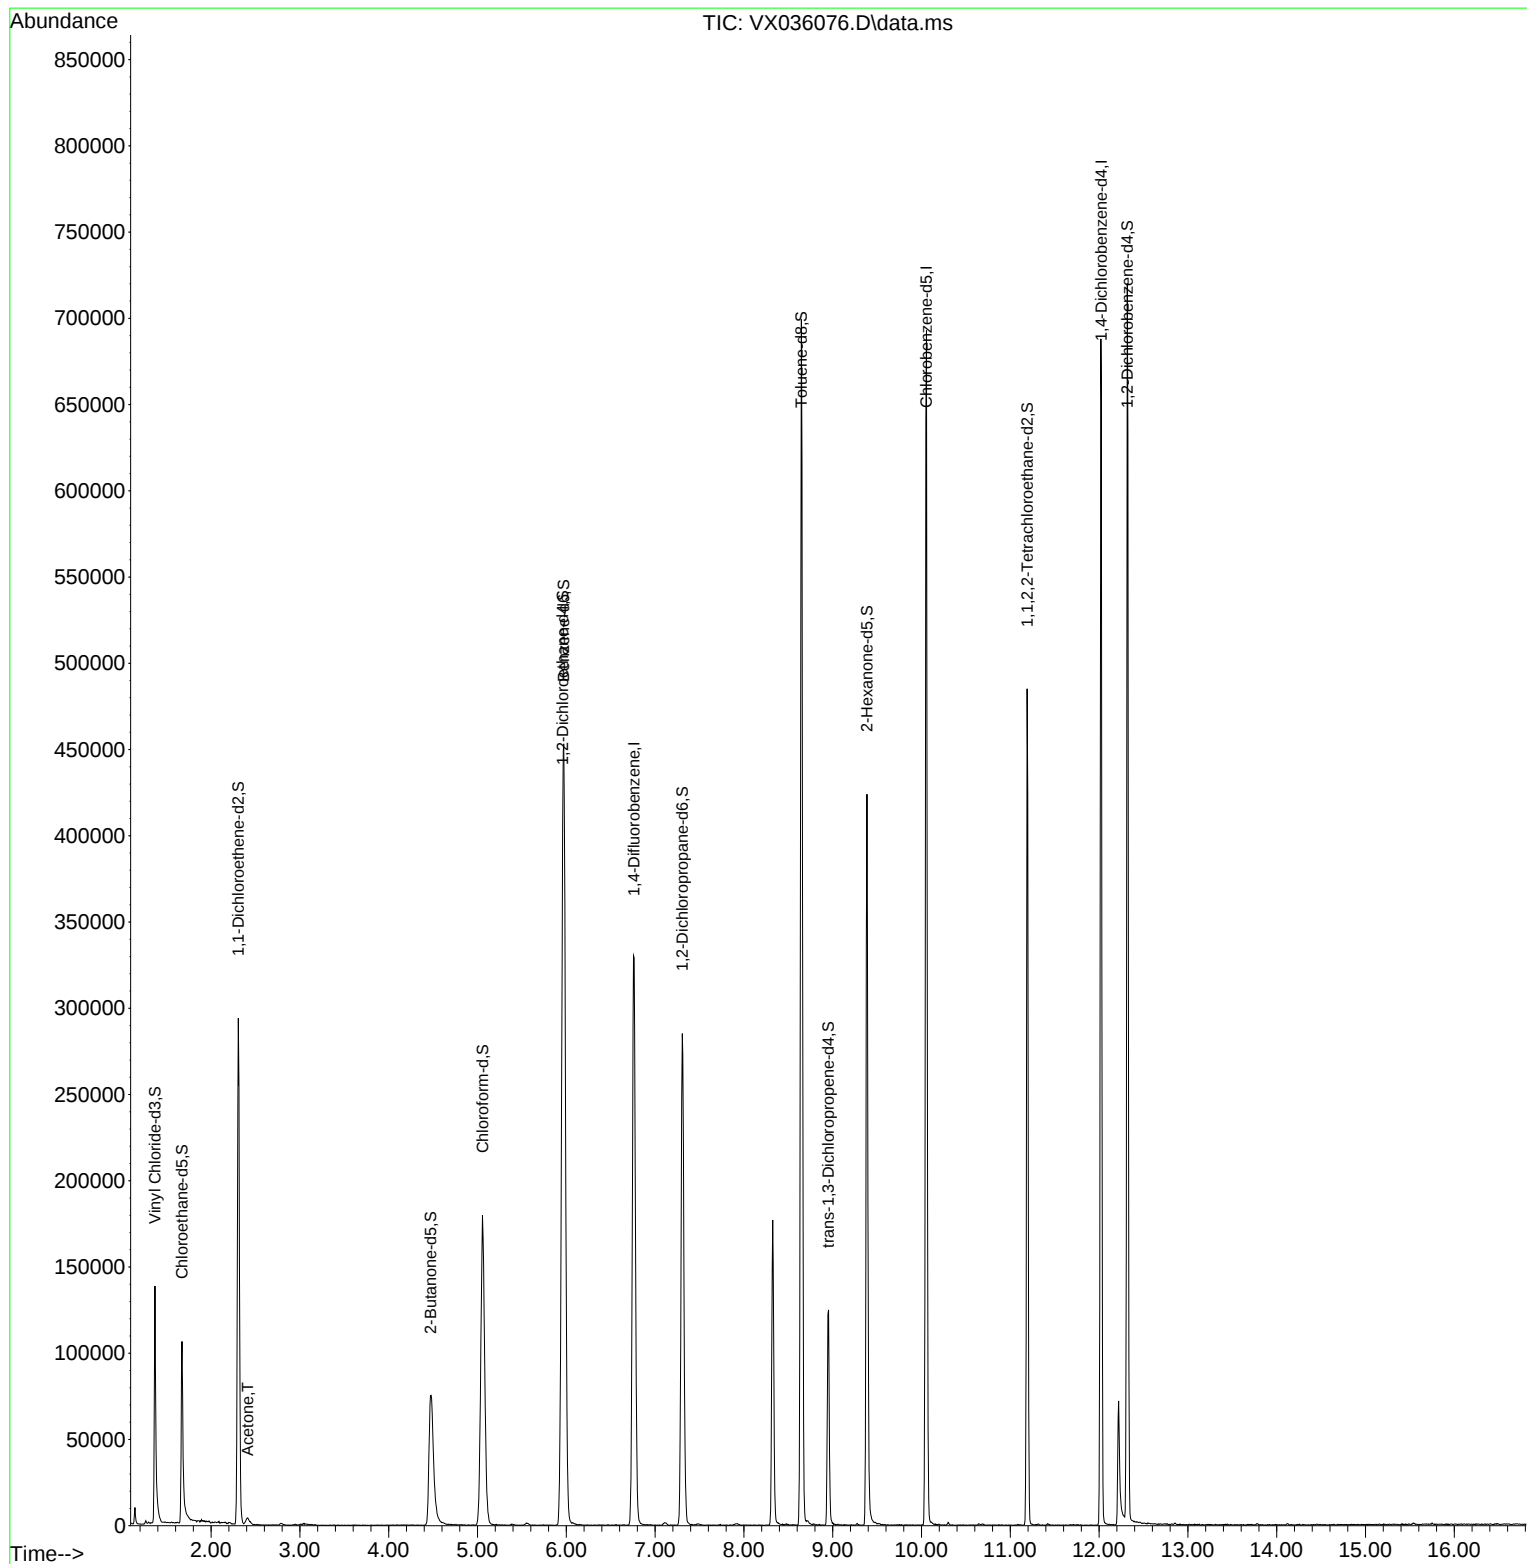

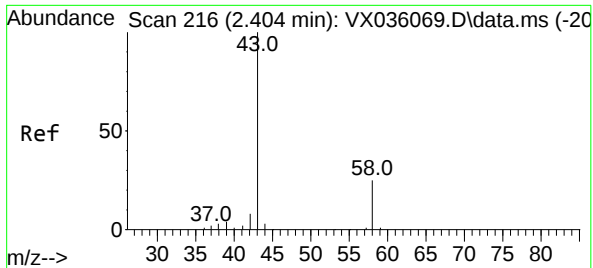

#13
 Acetone
 Concen: 3.747 ug/L
 RT: 2.410 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX036076.D
 Acq: 08 Jun 2023 17:28

Instrument :
 MSVOA_X
 ClientSampleId :
 EZES1

Tgt Ion: 43 Resp: 7055
 Ion Ratio Lower Upper
 43 100
 58 21.8 0.0 55.4

