

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036077.D
 Acq On : 08 Jun 2023 17:52
 Operator : JC/MD
 Sample : 03097-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZER8

Quant Time: Jun 09 02:24:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 07 05:37:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	316864	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	290058	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	130308	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	102784	47.744	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	95.480%	
7) Chloroethane-d5	1.672	69	84330	51.076	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	102.160%	
11) 1,1-Dichloroethene-d2	2.306	65	54297	49.744	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	99.480%	
21) 2-Butanone-d5	4.471	46	171750	97.331	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	97.330%	
24) Chloroform-d	5.056	84	216076	48.133	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.260%	
26) 1,2-Dichloroethane-d4	5.952	65	164858	50.327	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.660%	
32) Benzene-d6	5.976	84	436182	49.989	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.980%	
36) 1,2-Dichloropropane-d6	7.306	67	135620	50.005	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	100.020%	
41) Toluene-d8	8.647	98	391555	48.756	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	97.520%	
43) trans-1,3-Dichloroprop...	8.952	79	58761	45.136	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	90.280%	
47) 2-Hexanone-d5	9.384	63	118777	98.352	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	98.350%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	172680	46.614	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	93.220%	
66) 1,2-Dichlorobenzene-d4	12.317	152	130939	51.756	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	103.520%	
Target Compounds					Qvalue	
13) Acetone	2.410	43	6954	3.730	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036077.D
Acq On : 08 Jun 2023 17:52
Operator : JC/MD
Sample : 03097-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZER8

Quant Time: Jun 09 02:24:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 07 05:37:48 2023
Response via : Initial Calibration

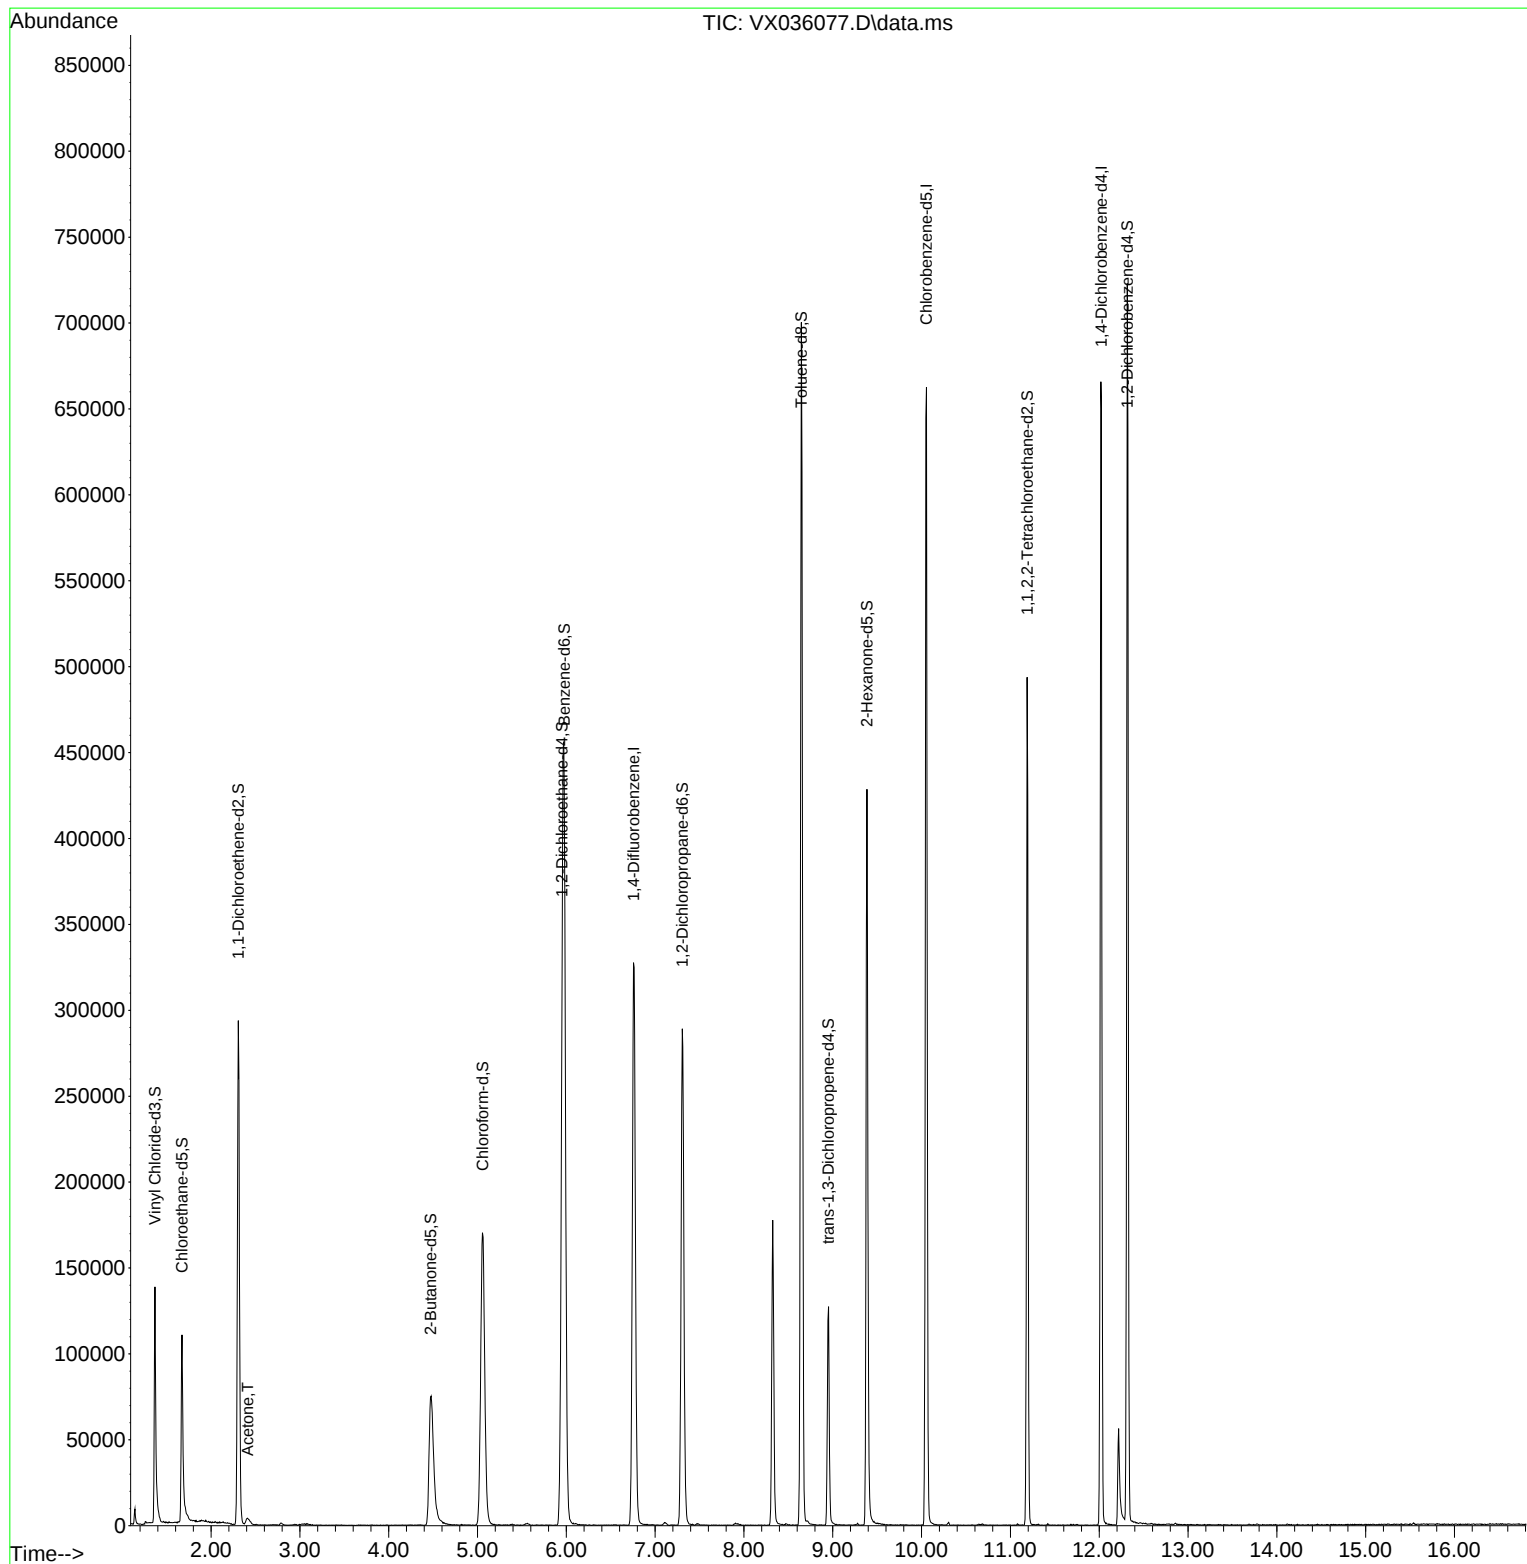

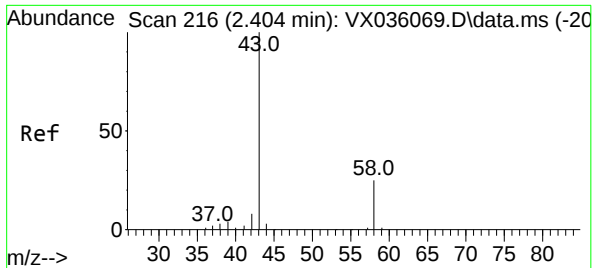

#13
 Acetone
 Concen: 3.730 ug/L
 RT: 2.410 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX036077.D
 Acq: 08 Jun 2023 17:52

Instrument :
 MSVOA_X
 ClientSampleId :
 EZER8

Tgt Ion: 43 Resp: 6954
 Ion Ratio Lower Upper
 43 100
 58 27.4 0.0 55.4

