

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036082.D
 Acq On : 08 Jun 2023 19:49
 Operator : JC/MD
 Sample : 03097-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEP5

Quant Time: Jun 09 02:24:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 07 05:37:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	305336	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	278603	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	127296	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	95252	45.916	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.840%
7) Chloroethane-d5	1.673	69	75812	47.651	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.300%
11) 1,1-Dichloroethene-d2	2.307	65	50260	47.784	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.560%
21) 2-Butanone-d5	4.477	46	161525	94.993	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.990%
24) Chloroform-d	5.056	84	200317	46.307	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.620%
26) 1,2-Dichloroethane-d4	5.952	65	153028	48.480	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.960%
32) Benzene-d6	5.971	84	406692	48.525	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.060%
36) 1,2-Dichloropropane-d6	7.306	67	127214	48.834	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.660%
41) Toluene-d8	8.647	98	363973	47.185	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.360%
43) trans-1,3-Dichloroprop...	8.952	79	52737	42.174	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.340%
47) 2-Hexanone-d5	9.385	63	110231	95.028	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.030%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	162965	45.800	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.600%
66) 1,2-Dichlorobenzene-d4	12.317	152	123431	49.942	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.880%
Target Compounds						
					Qvalue	
13) Acetone	2.410	43	7562	4.209	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036082.D
Acq On : 08 Jun 2023 19:49
Operator : JC/MD
Sample : 03097-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEP5

Quant Time: Jun 09 02:24:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 07 05:37:48 2023
Response via : Initial Calibration

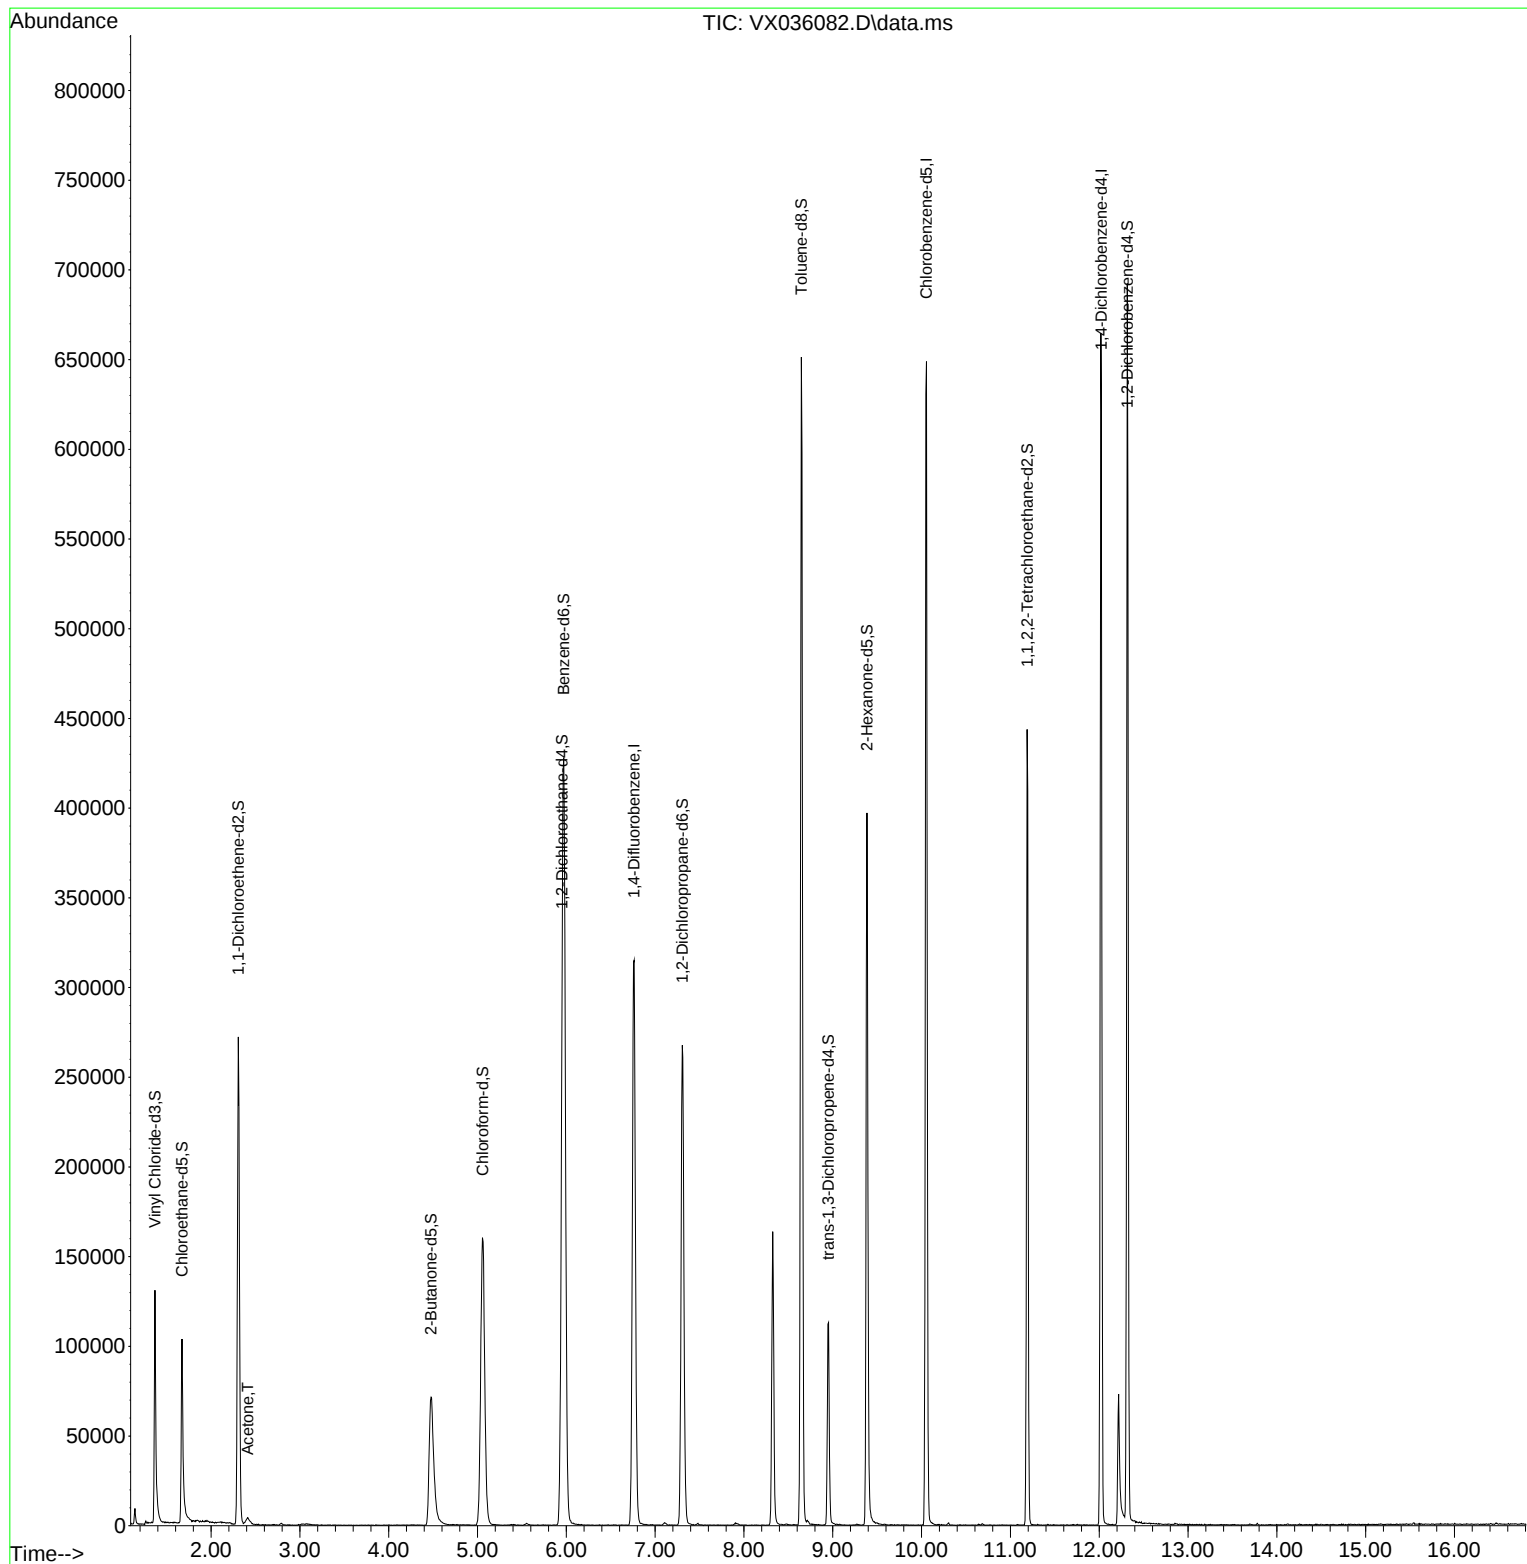

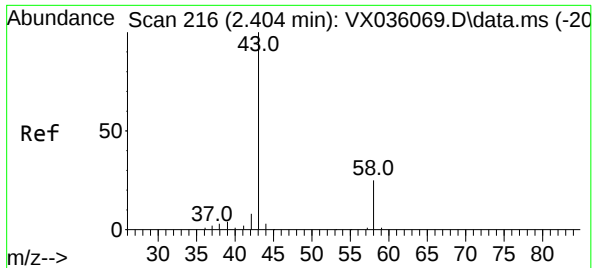

#13
 Acetone
 Concen: 4.209 ug/L
 RT: 2.410 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX036082.D
 Acq: 08 Jun 2023 19:49

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEP5

Tgt Ion: 43 Resp: 7562
 Ion Ratio Lower Upper
 43 100
 58 20.9 0.0 55.4

