

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036071.D
 Acq On : 08 Jun 2023 15:32
 Operator : JC/MD
 Sample : 03097-01 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	9093	9148	0.71%	0.098%
2	1.264	27	29	32	rVB	1556	1217	0.09%	0.013%
3	1.367	42	46	62	rBV	137504	162147	12.54%	1.728%
4	1.672	91	96	111	rBV	98453	150821	11.67%	1.608%
5	2.306	194	200	212	rVB	277686	434154	33.58%	4.628%
6	2.398	212	215	216	rBV3	696	699	0.05%	0.007%
7	2.453	223	224	226	rBV	303	246	0.02%	0.003%
8	2.514	230	234	236	rBV2	458	659	0.05%	0.007%
9	2.575	243	244	248	rVB2	343	211	0.02%	0.002%
10	2.690	260	263	264	rBV2	336	249	0.02%	0.003%
11	2.788	273	279	284	rBV5	2571	4829	0.37%	0.051%
12	2.940	298	304	313	rVB4	2370	5915	0.46%	0.063%
13	3.062	323	324	326	rBV	322	242	0.02%	0.003%
14	3.129	333	335	338	rVV3	208	259	0.02%	0.003%
15	3.276	353	359	361	rVB2	278	446	0.03%	0.005%
16	3.337	367	369	371	rBV2	206	215	0.02%	0.002%
17	3.477	390	392	396	rVV	231	284	0.02%	0.003%
18	3.507	396	397	401	rVV3	256	243	0.02%	0.003%
19	3.605	411	413	416	rBV2	172	248	0.02%	0.003%
20	3.751	434	437	439	rBV2	166	223	0.02%	0.002%
21	4.294	522	526	529	rVB2	255	314	0.02%	0.003%
22	4.324	529	531	533	rBV	235	211	0.02%	0.002%
23	4.471	545	555	570	rBV	79919	269440	20.84%	2.872%
24	4.958	632	635	639	rBV2	207	235	0.02%	0.003%
25	5.056	639	651	670	rBV2	161081	519975	40.22%	5.543%
26	5.379	699	704	706	rBV4	622	1021	0.08%	0.011%
27	5.519	724	727	728	rBV3	345	359	0.03%	0.004%
28	5.531	728	729	730	rBV3	581	413	0.03%	0.004%
29	5.964	787	800	816	rBV2	431800	1292911	100.00%	13.782%
30	6.190	835	837	839	rVB	388	220	0.02%	0.002%
31	6.287	851	853	854	rVB2	298	199	0.02%	0.002%
32	6.312	856	857	860	rVB	382	247	0.02%	0.003%
33	6.348	860	863	866	rBV	258	298	0.02%	0.003%
34	6.446	876	879	880	rBV	228	248	0.02%	0.003%
35	6.464	880	882	889	rVB3	426	612	0.05%	0.007%
36	6.537	891	894	896	rBV3	246	226	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036071.D
 Acq On : 08 Jun 2023 15:32
 Operator : JC/MD
 Sample : 03097-01 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.757	919	930	945	rVV	288852	696712	53.89%	7.427%
38	7.037	973	976	978	rBV2	166	218	0.02%	0.002%
39	7.104	982	987	995	rVB4	1772	3403	0.26%	0.036%
40	7.208	1001	1004	1005	rBV	355	237	0.02%	0.003%
41	7.305	1011	1020	1036	rBV	271968	592020	45.79%	6.311%
42	7.433	1039	1041	1043	rVB2	326	244	0.02%	0.003%
43	7.482	1043	1049	1052	rBV2	1173	1744	0.13%	0.019%
44	7.659	1077	1078	1081	rVB	290	198	0.02%	0.002%
45	7.933	1118	1123	1125	rBV2	705	911	0.07%	0.010%
46	8.092	1147	1149	1153	rVB2	196	267	0.02%	0.003%
47	8.244	1169	1174	1180	rBV2	8707	14131	1.09%	0.151%
48	8.324	1180	1187	1200	rBV	167535	278638	21.55%	2.970%
49	8.470	1209	1211	1217	rVB3	628	939	0.07%	0.010%
50	8.580	1227	1229	1233	rVB	321	337	0.03%	0.004%
51	8.647	1233	1240	1257	rBV	671504	1029586	79.63%	10.975%
52	8.945	1283	1289	1302	rBV	119265	183386	14.18%	1.955%
53	9.275	1340	1343	1345	rVB3	376	450	0.03%	0.005%
54	9.311	1347	1349	1353	rVB3	252	254	0.02%	0.003%
55	9.384	1355	1361	1373	rBV	423852	595341	46.05%	6.346%
56	9.604	1395	1397	1399	rVB	464	346	0.03%	0.004%
57	9.628	1399	1401	1408	rVB	232	260	0.02%	0.003%
58	9.695	1408	1412	1421	rVB2	2377	3743	0.29%	0.040%
59	9.774	1421	1425	1429	rBV2	311	523	0.04%	0.006%
60	9.927	1447	1450	1452	rBV2	325	404	0.03%	0.004%
61	10.055	1465	1471	1487	rBV	587706	826517	63.93%	8.810%
62	10.268	1505	1506	1509	rBV	361	308	0.02%	0.003%
63	10.311	1509	1513	1515	rVB2	371	538	0.04%	0.006%
64	10.555	1551	1553	1555	rBV	362	345	0.03%	0.004%
65	10.573	1555	1556	1560	rVB	270	268	0.02%	0.003%
66	10.610	1560	1562	1564	rBV2	283	367	0.03%	0.004%
67	10.665	1566	1571	1573	rBV2	429	681	0.05%	0.007%
68	10.774	1587	1589	1592	rVB2	293	215	0.02%	0.002%
69	10.811	1594	1595	1599	rVB	207	246	0.02%	0.003%
70	10.927	1611	1614	1617	rBV2	202	336	0.03%	0.004%
71	11.079	1636	1639	1645	rBV3	716	977	0.08%	0.010%
72	11.189	1652	1657	1667	rBV	466677	586691	45.38%	6.254%
73	11.305	1674	1676	1679	rVB2	407	356	0.03%	0.004%
74	11.341	1679	1682	1685	rVB2	248	324	0.03%	0.003%
75	11.402	1691	1692	1696	rVB2	227	277	0.02%	0.003%
76	11.683	1736	1738	1740	rBV	249	200	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036071.D
 Acq On : 08 Jun 2023 15:32
 Operator : JC/MD
 Sample : 03097-01 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.707	1740	1742	1744	rVB2	292	242	0.02%	0.003%
78	11.872	1767	1769	1771	rVB2	334	240	0.02%	0.003%
79	12.018	1788	1793	1804	rBV	628418	801552	62.00%	8.544%
80	12.244	1828	1830	1833	rVB2	261	321	0.02%	0.003%
81	12.317	1837	1842	1850	rBV	711291	890274	68.86%	9.490%
82	12.445	1861	1863	1866	rBV2	261	255	0.02%	0.003%
83	12.518	1873	1875	1878	rBV3	191	261	0.02%	0.003%
84	12.573	1883	1884	1887	rBV	345	255	0.02%	0.003%
85	12.634	1893	1894	1896	rBV	209	196	0.02%	0.002%
86	12.847	1925	1929	1932	rBV3	382	587	0.05%	0.006%
87	12.920	1938	1941	1942	rVB2	302	281	0.02%	0.003%
88	12.932	1942	1943	1947	rBV2	247	295	0.02%	0.003%
89	13.073	1965	1966	1968	rBV	313	298	0.02%	0.003%
90	13.280	1998	2000	2003	rVB2	204	205	0.02%	0.002%
91	13.512	2036	2038	2040	rBV	265	271	0.02%	0.003%
92	13.670	2062	2064	2067	rVB	237	198	0.02%	0.002%
93	13.774	2079	2081	2086	rBV3	337	408	0.03%	0.004%
94	14.414	2184	2186	2188	rVB2	250	206	0.02%	0.002%
95	14.615	2218	2219	2221	rBV2	216	226	0.02%	0.002%
96	15.072	2292	2294	2296	rBV2	528	397	0.03%	0.004%
97	15.304	2329	2332	2335	rBV3	432	566	0.04%	0.006%
98	15.828	2416	2418	2421	rBV2	317	357	0.03%	0.004%
99	16.060	2454	2456	2457	rBV	369	265	0.02%	0.003%
100	16.493	2525	2527	2530	rVB3	713	804	0.06%	0.009%




Sum of corrected areas: 9381282

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036071.D
Acq On : 08 Jun 2023 15:32
Operator : JC/MD
Sample : 03097-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

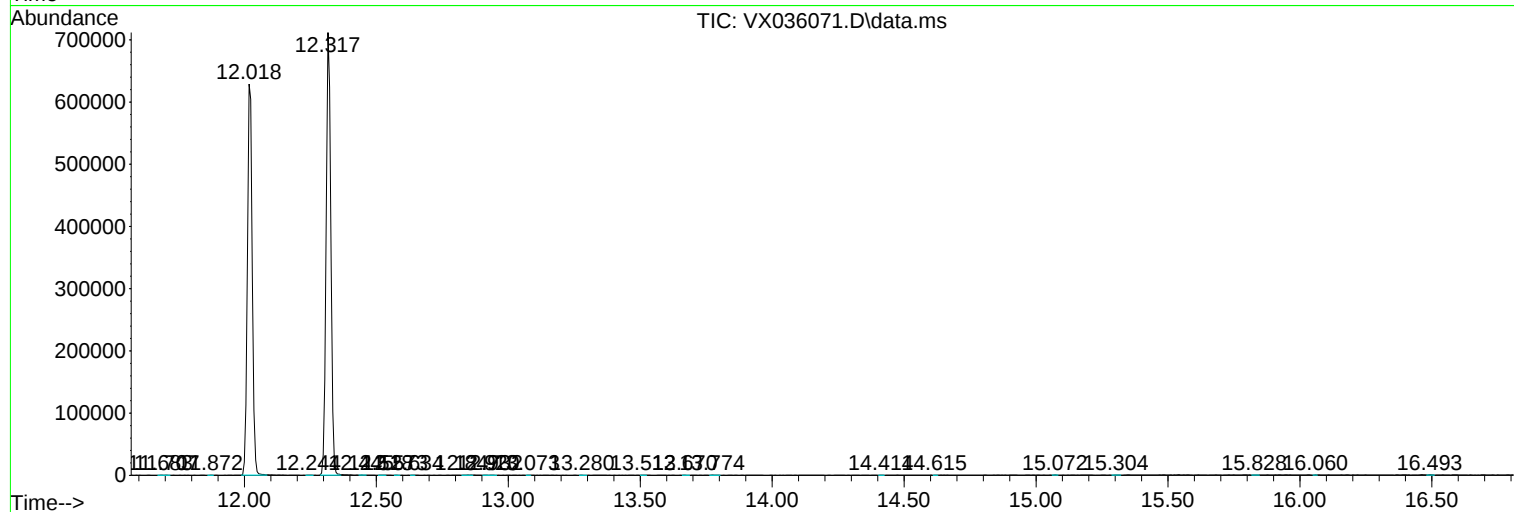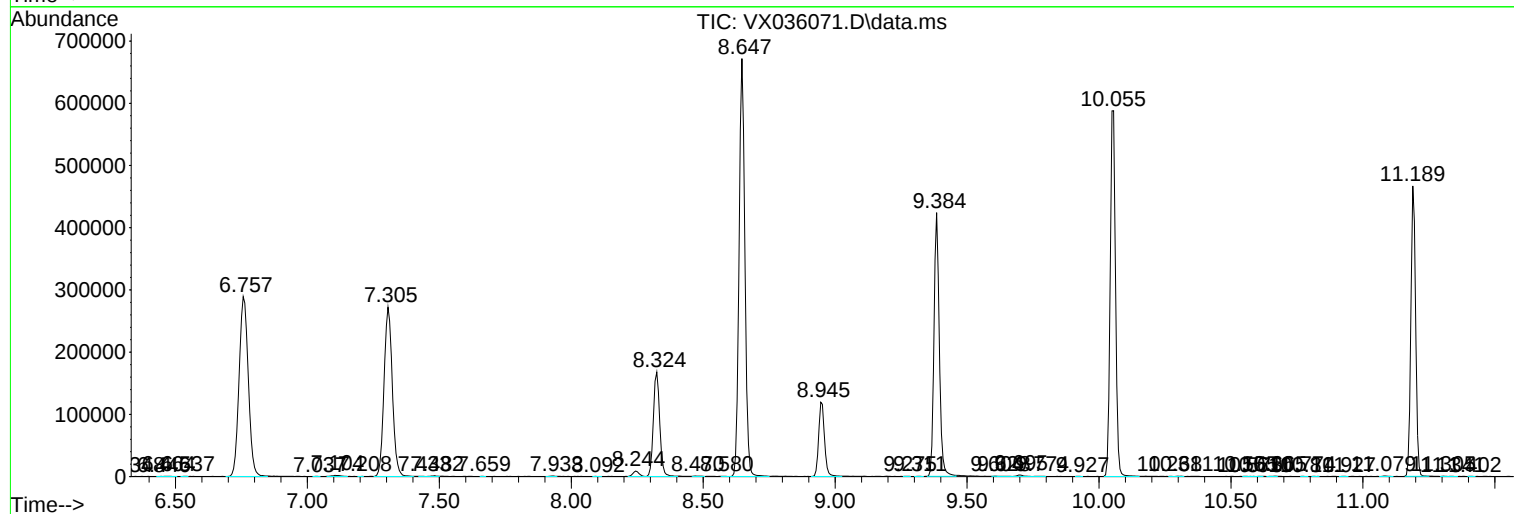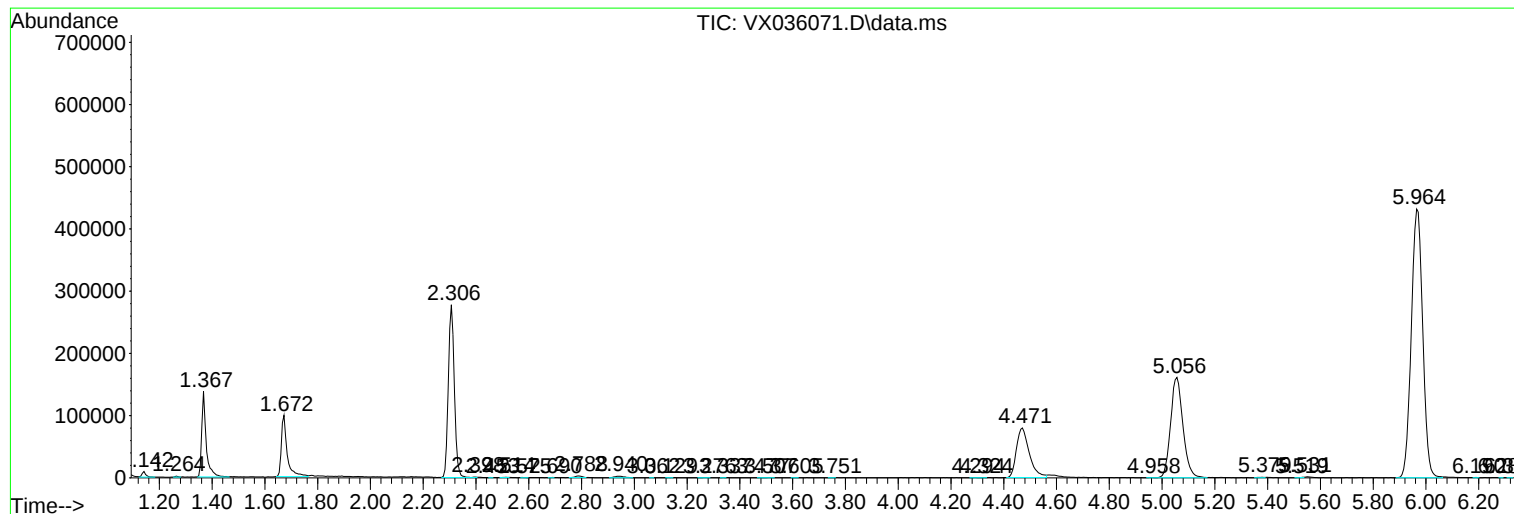

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036071.D
Acq On : 08 Jun 2023 15:32
Operator : JC/MD
Sample : 03097-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036071.D
Acq On : 08 Jun 2023 15:32
Operator : JC/MD
Sample : 03097-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------