

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036079.D
 Acq On : 08 Jun 2023 18:39
 Operator : JC/MD
 Sample : 03097-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rVB	9272	9792	0.74%	0.103%
2	1.264	26	29	32	rBV3	1495	1585	0.12%	0.017%
3	1.368	42	46	60	rVB	132994	161858	12.30%	1.705%
4	1.672	91	96	109	rBV	93688	147780	11.23%	1.556%
5	2.306	194	200	212	rVB	278484	440214	33.44%	4.636%
6	2.416	212	218	221	rBV3	1649	3762	0.29%	0.040%
7	2.794	274	280	283	rBV4	1547	2598	0.20%	0.027%
8	3.020	311	317	319	rBV4	906	1789	0.14%	0.019%
9	3.166	339	341	346	rVV3	294	311	0.02%	0.003%
10	3.532	398	401	402	rVB	240	203	0.02%	0.002%
11	3.587	407	410	412	rBV	165	215	0.02%	0.002%
12	3.672	421	424	427	rBV2	192	270	0.02%	0.003%
13	3.770	438	440	446	rBV2	189	376	0.03%	0.004%
14	4.087	490	492	494	rVB2	268	213	0.02%	0.002%
15	4.233	514	516	519	rBV	366	398	0.03%	0.004%
16	4.477	545	556	576	rBV	73291	267353	20.31%	2.816%
17	4.727	595	597	598	rBV	253	239	0.02%	0.003%
18	5.056	639	651	672	rBV2	164045	517341	39.30%	5.449%
19	5.196	672	674	677	rVB3	314	265	0.02%	0.003%
20	5.239	680	681	682	rBV	396	214	0.02%	0.002%
21	5.288	687	689	690	rBV2	264	217	0.02%	0.002%
22	5.385	700	705	706	rBV2	777	823	0.06%	0.009%
23	5.556	725	733	739	rVB4	1153	2879	0.22%	0.030%
24	5.647	746	748	752	rVB2	226	233	0.02%	0.002%
25	5.873	783	785	786	rBV	203	220	0.02%	0.002%
26	5.970	788	801	816	rBV2	442474	1316258	100.00%	13.863%
27	6.141	827	829	832	rVB2	314	327	0.02%	0.003%
28	6.172	832	834	836	rBV	259	222	0.02%	0.002%
29	6.214	839	841	843	rVB2	285	241	0.02%	0.003%
30	6.232	843	844	846	rBV2	267	223	0.02%	0.002%
31	6.275	849	851	854	rBV2	182	244	0.02%	0.003%
32	6.397	868	871	873	rVB2	239	263	0.02%	0.003%
33	6.470	882	883	887	rVB	352	354	0.03%	0.004%
34	6.537	890	894	896	rBV2	343	452	0.03%	0.005%
35	6.763	920	931	947	rVV	314171	754362	57.31%	7.945%
36	7.110	981	988	994	rBV4	4587	9906	0.75%	0.104%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036079.D
 Acq On : 08 Jun 2023 18:39
 Operator : JC/MD
 Sample : 03097-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.226	1004	1007	1009	rBV2	217	338	0.03%	0.004%
38	7.305	1011	1020	1033	rVV	276921	601630	45.71%	6.337%
39	7.476	1043	1048	1055	rBV3	795	1734	0.13%	0.018%
40	7.854	1106	1110	1112	rBV2	149	207	0.02%	0.002%
41	7.903	1112	1118	1125	rBV6	1017	3098	0.24%	0.033%
42	8.007	1134	1135	1138	rBV2	341	327	0.02%	0.003%
43	8.324	1180	1187	1204	rVV	168094	275342	20.92%	2.900%
44	8.513	1216	1218	1222	rVB2	268	251	0.02%	0.003%
45	8.592	1228	1231	1233	rBV2	268	253	0.02%	0.003%
46	8.647	1233	1240	1249	rBV	680527	1046864	79.53%	11.026%
47	8.903	1280	1282	1283	rBV	407	251	0.02%	0.003%
48	8.952	1283	1290	1307	rVV	117900	180998	13.75%	1.906%
49	9.128	1317	1319	1321	rVB2	366	280	0.02%	0.003%
50	9.220	1333	1334	1336	rBV	265	219	0.02%	0.002%
51	9.275	1341	1343	1347	rVB2	756	719	0.05%	0.008%
52	9.384	1356	1361	1377	rBV	414239	581697	44.19%	6.127%
53	9.525	1382	1384	1392	rVB3	1234	1796	0.14%	0.019%
54	9.738	1417	1419	1422	rVB	450	373	0.03%	0.004%
55	9.787	1425	1427	1430	rVB2	247	311	0.02%	0.003%
56	9.976	1457	1458	1461	rVB	214	210	0.02%	0.002%
57	10.055	1465	1471	1486	rVV	637850	891764	67.75%	9.392%
58	10.195	1490	1494	1499	rVB3	589	762	0.06%	0.008%
59	10.238	1499	1501	1503	rBV	438	327	0.02%	0.003%
60	10.305	1507	1512	1518	rVB3	1831	2401	0.18%	0.025%
61	10.445	1533	1535	1537	rBV2	275	240	0.02%	0.003%
62	10.585	1555	1558	1559	rBV2	223	202	0.02%	0.002%
63	10.640	1565	1567	1570	rBV2	629	590	0.04%	0.006%
64	10.762	1586	1587	1592	rVB	400	458	0.03%	0.005%
65	11.091	1637	1641	1644	rBV3	584	683	0.05%	0.007%
66	11.189	1652	1657	1670	rVB	435884	573183	43.55%	6.037%
67	11.311	1674	1677	1678	rVB2	375	350	0.03%	0.004%
68	11.390	1688	1690	1692	rVB2	229	204	0.02%	0.002%
69	11.414	1692	1694	1696	rBV2	362	287	0.02%	0.003%
70	11.671	1734	1736	1739	rBV	299	270	0.02%	0.003%
71	11.750	1746	1749	1754	rVB2	498	680	0.05%	0.007%
72	11.920	1775	1777	1780	rBV2	171	219	0.02%	0.002%
73	12.018	1788	1793	1804	rBV	636219	807534	61.35%	8.505%
74	12.152	1814	1815	1818	rBV2	295	278	0.02%	0.003%
75	12.280	1833	1836	1837	rBV2	263	311	0.02%	0.003%
76	12.317	1837	1842	1856	rVV	690509	863798	65.63%	9.098%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036079.D
 Acq On : 08 Jun 2023 18:39
 Operator : JC/MD
 Sample : 03097-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.457	1863	1865	1871	rVB3	269	375	0.03%	0.004%
78	12.756	1910	1914	1915	rBV2	405	421	0.03%	0.004%
79	12.774	1915	1917	1918	rVV2	311	226	0.02%	0.002%
80	12.811	1922	1923	1928	rVB2	333	424	0.03%	0.004%
81	12.859	1928	1931	1934	rBV	366	480	0.04%	0.005%
82	12.933	1940	1943	1945	rBV	249	261	0.02%	0.003%
83	13.030	1957	1959	1960	rBV	356	254	0.02%	0.003%
84	13.274	1997	1999	2001	rBV2	197	219	0.02%	0.002%
85	13.695	2065	2068	2070	rBV2	569	681	0.05%	0.007%
86	13.774	2079	2081	2082	rBV	443	305	0.02%	0.003%
87	14.091	2132	2133	2135	rBV	397	238	0.02%	0.003%
88	14.158	2142	2144	2147	rBV	205	216	0.02%	0.002%
89	14.469	2193	2195	2198	rVB2	297	252	0.02%	0.003%
90	14.499	2198	2200	2202	rBV2	286	211	0.02%	0.002%
91	14.548	2206	2208	2210	rVB	407	236	0.02%	0.002%
92	14.640	2220	2223	2225	rBV3	464	529	0.04%	0.006%
93	14.694	2230	2232	2233	rBV2	371	233	0.02%	0.002%
94	14.914	2266	2268	2271	rVB3	454	419	0.03%	0.004%
95	14.950	2271	2274	2276	rBV2	368	461	0.04%	0.005%
96	14.975	2276	2278	2280	rBV	333	285	0.02%	0.003%
97	15.408	2347	2349	2351	rBV2	487	335	0.03%	0.004%
98	15.755	2404	2406	2410	rBV2	567	877	0.07%	0.009%
99	16.371	2506	2507	2511	rBV2	598	606	0.05%	0.006%
100	16.651	2550	2553	2554	rBV2	555	632	0.05%	0.007%




Sum of corrected areas: 9494615

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036079.D
Acq On : 08 Jun 2023 18:39
Operator : JC/MD
Sample : 03097-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

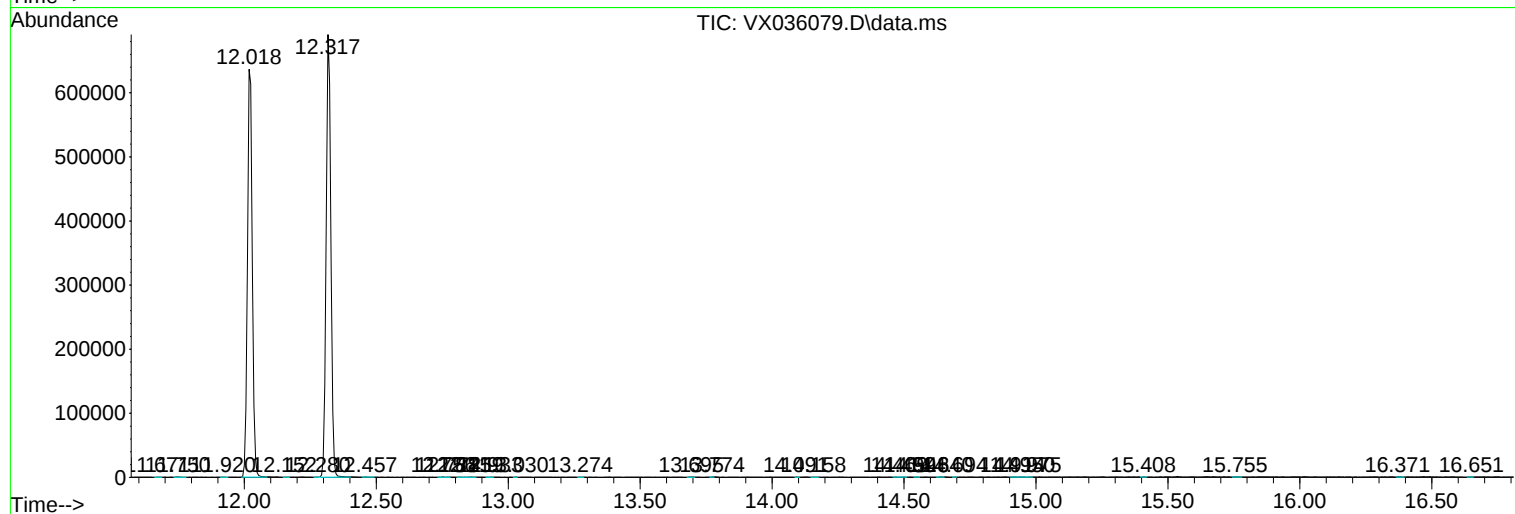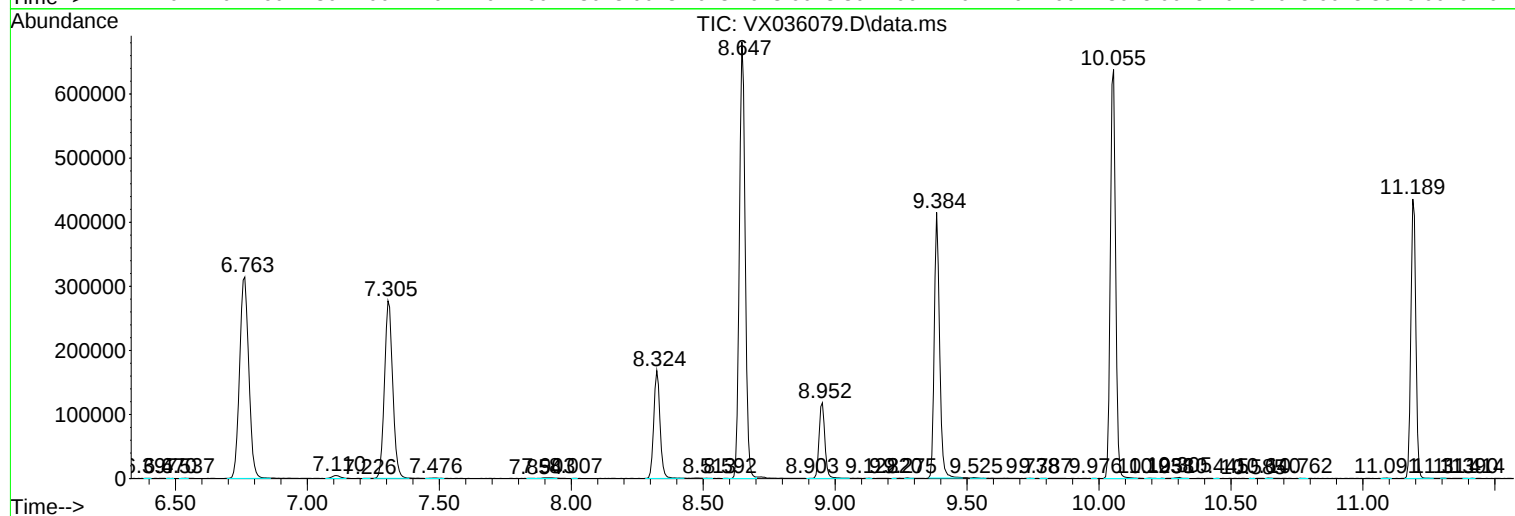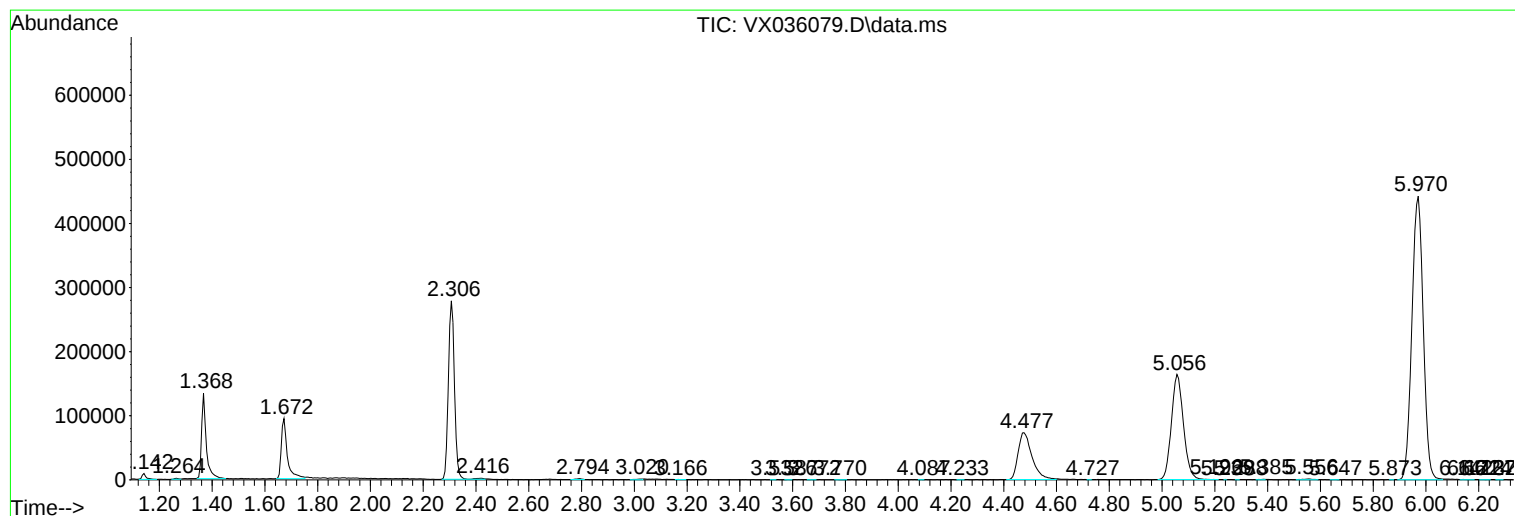

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036079.D
Acq On : 08 Jun 2023 18:39
Operator : JC/MD
Sample : 03097-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEPI

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036079.D
Acq On : 08 Jun 2023 18:39
Operator : JC/MD
Sample : 03097-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEPI

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------