

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036084.D
 Acq On : 08 Jun 2023 20:35
 Operator : JC/MD
 Sample : 03097-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	12989	14278	1.12%	0.143%
2	1.264	27	29	31	rBV2	1817	1102	0.09%	0.011%
3	1.368	42	46	57	rBV	128831	154583	12.09%	1.550%
4	1.672	91	96	111	rBV	102899	155094	12.13%	1.555%
5	2.306	194	200	210	rBV	273022	425738	33.31%	4.268%
6	2.684	260	262	264	rVB	259	184	0.01%	0.002%
7	2.788	273	279	283	rBV2	815	1386	0.11%	0.014%
8	2.934	299	303	306	rBV	328	547	0.04%	0.005%
9	3.099	324	330	336	rVB5	2469	4619	0.36%	0.046%
10	3.215	348	349	352	rBV2	188	209	0.02%	0.002%
11	3.288	358	361	362	rBV	219	186	0.01%	0.002%
12	3.379	373	376	377	rVV2	235	231	0.02%	0.002%
13	3.398	377	379	381	rVV	262	207	0.02%	0.002%
14	3.453	387	388	392	rVV	231	262	0.02%	0.003%
15	3.532	399	401	406	rBV2	235	327	0.03%	0.003%
16	3.568	406	407	410	rVB	252	193	0.02%	0.002%
17	3.599	410	412	413	rBV	289	262	0.02%	0.003%
18	3.617	413	415	417	rVV2	449	448	0.04%	0.004%
19	3.642	417	419	421	rVV2	180	184	0.01%	0.002%
20	3.702	426	429	433	rBV	193	232	0.02%	0.002%
21	3.776	438	441	445	rVB2	180	185	0.01%	0.002%
22	4.172	505	506	508	rBV	280	188	0.01%	0.002%
23	4.245	516	518	522	rBV2	277	389	0.03%	0.004%
24	4.355	533	536	537	rBV2	278	255	0.02%	0.003%
25	4.477	544	556	574	rBV2	105877	372941	29.18%	3.739%
26	4.769	603	604	606	rBV	366	228	0.02%	0.002%
27	4.897	623	625	629	rVB3	206	206	0.02%	0.002%
28	5.056	638	651	670	rBV	158789	505953	39.58%	5.072%
29	5.330	694	696	697	rBV	582	446	0.03%	0.004%
30	5.379	697	704	718	rVB3	6855	20165	1.58%	0.202%
31	5.531	728	729	730	rBV	391	212	0.02%	0.002%
32	5.818	775	776	780	rVB2	305	209	0.02%	0.002%
33	5.970	788	801	816	rBV2	424018	1278193	100.00%	12.814%
34	6.184	834	836	838	rBV	243	236	0.02%	0.002%
35	6.464	879	882	884	rVB3	401	397	0.03%	0.004%
36	6.763	919	931	944	rBV	308214	750034	58.68%	7.519%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036084.D
 Acq On : 08 Jun 2023 20:35
 Operator : JC/MD
 Sample : 03097-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.970	963	965	968	rBV	240	222	0.02%	0.002%
38	7.123	980	990	1004	rBV	210898	456714	35.73%	4.579%
39	7.305	1011	1020	1037	rBV	264496	587387	45.95%	5.889%
40	7.464	1045	1046	1048	rBV2	595	460	0.04%	0.005%
41	7.482	1048	1049	1053	rVB2	746	575	0.04%	0.006%
42	7.562	1061	1062	1067	rBV2	203	327	0.03%	0.003%
43	7.927	1118	1122	1123	rBV2	763	800	0.06%	0.008%
44	8.159	1158	1160	1166	rVB2	235	402	0.03%	0.004%
45	8.208	1166	1168	1169	rBV2	229	187	0.01%	0.002%
46	8.324	1180	1187	1200	rBV	160641	268162	20.98%	2.688%
47	8.470	1209	1211	1212	rBV	321	219	0.02%	0.002%
48	8.647	1233	1240	1255	rBV	640358	1010091	79.02%	10.126%
49	8.903	1281	1282	1284	rBV2	257	182	0.01%	0.002%
50	8.952	1284	1290	1298	rBV	113106	172693	13.51%	1.731%
51	9.104	1314	1315	1319	rBV2	288	230	0.02%	0.002%
52	9.275	1338	1343	1348	rVB3	935	1571	0.12%	0.016%
53	9.323	1348	1351	1354	rBV2	220	329	0.03%	0.003%
54	9.384	1355	1361	1374	rBV	406889	581677	45.51%	5.831%
55	9.628	1399	1401	1403	rVB	439	302	0.02%	0.003%
56	9.647	1403	1404	1406	rBV	440	248	0.02%	0.002%
57	9.927	1446	1450	1451	rBV2	325	261	0.02%	0.003%
58	10.055	1465	1471	1485	rBV	649586	884952	69.23%	8.872%
59	10.299	1509	1511	1514	rVB2	542	462	0.04%	0.005%
60	10.354	1517	1520	1521	rBV2	248	202	0.02%	0.002%
61	10.396	1525	1527	1529	rVB	276	215	0.02%	0.002%
62	10.628	1563	1565	1567	rBV	287	277	0.02%	0.003%
63	10.854	1598	1602	1603	rBV2	197	243	0.02%	0.002%
64	11.043	1631	1633	1636	rVV2	235	199	0.02%	0.002%
65	11.091	1637	1641	1644	rVB2	268	337	0.03%	0.003%
66	11.189	1652	1657	1671	rBV	460235	593806	46.46%	5.953%
67	11.311	1676	1677	1681	rVB3	654	625	0.05%	0.006%
68	11.354	1681	1684	1685	rBV2	270	241	0.02%	0.002%
69	11.402	1688	1692	1695	rBV3	235	378	0.03%	0.004%
70	11.573	1719	1720	1725	rVV	237	233	0.02%	0.002%
71	11.628	1725	1729	1732	rVB2	363	500	0.04%	0.005%
72	11.707	1740	1742	1746	rVB2	589	556	0.04%	0.006%
73	12.018	1788	1793	1803	rBV	677606	846605	66.23%	8.487%
74	12.225	1823	1827	1830	rBV5	1298	1803	0.14%	0.018%
75	12.268	1832	1834	1837	rBV2	334	357	0.03%	0.004%
76	12.317	1837	1842	1850	rBV	687460	862560	67.48%	8.647%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036084.D
 Acq On : 08 Jun 2023 20:35
 Operator : JC/MD
 Sample : 03097-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.524	1874	1876	1877	rBV	279	182	0.01%	0.002%
78	12.652	1894	1897	1898	rBV	224	296	0.02%	0.003%
79	12.853	1929	1930	1932	rBV2	322	235	0.02%	0.002%
80	12.981	1949	1951	1953	rBV2	220	257	0.02%	0.003%
81	13.079	1966	1967	1971	rBV2	247	247	0.02%	0.002%
82	13.408	2019	2021	2024	rBV2	287	203	0.02%	0.002%
83	13.567	2045	2047	2051	rVB2	279	378	0.03%	0.004%
84	13.725	2072	2073	2075	rBV	225	179	0.01%	0.002%
85	14.042	2123	2125	2129	rBV2	188	244	0.02%	0.002%
86	14.097	2132	2134	2136	rBV2	291	226	0.02%	0.002%
87	14.146	2141	2142	2143	rVV	313	179	0.01%	0.002%
88	14.188	2147	2149	2151	rBV	292	247	0.02%	0.002%
89	14.304	2166	2168	2172	rVV	206	201	0.02%	0.002%
90	14.359	2175	2177	2179	rBV2	337	330	0.03%	0.003%
91	14.377	2179	2180	2183	rVB2	328	227	0.02%	0.002%
92	14.402	2183	2184	2186	rBV	244	177	0.01%	0.002%
93	14.743	2237	2240	2242	rBV2	286	442	0.03%	0.004%
94	14.981	2277	2279	2281	rBV	339	225	0.02%	0.002%
95	15.042	2286	2289	2290	rBV2	378	364	0.03%	0.004%
96	15.194	2312	2314	2317	rVB	337	267	0.02%	0.003%
97	15.542	2370	2371	2375	rVB3	938	869	0.07%	0.009%
98	15.792	2410	2412	2415	rBV2	475	474	0.04%	0.005%
99	16.036	2451	2452	2454	rBV2	357	305	0.02%	0.003%
100	16.395	2510	2511	2512	rBV	435	198	0.02%	0.002%




Sum of corrected areas: 9975051

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036084.D
Acq On : 08 Jun 2023 20:35
Operator : JC/MD
Sample : 03097-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

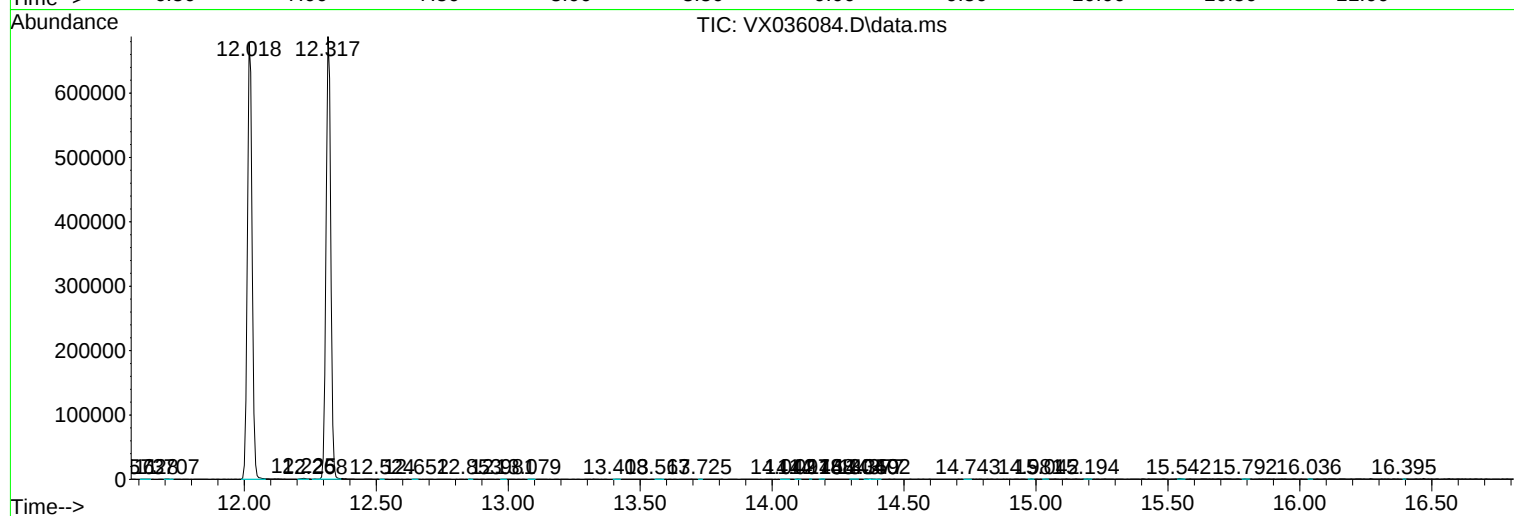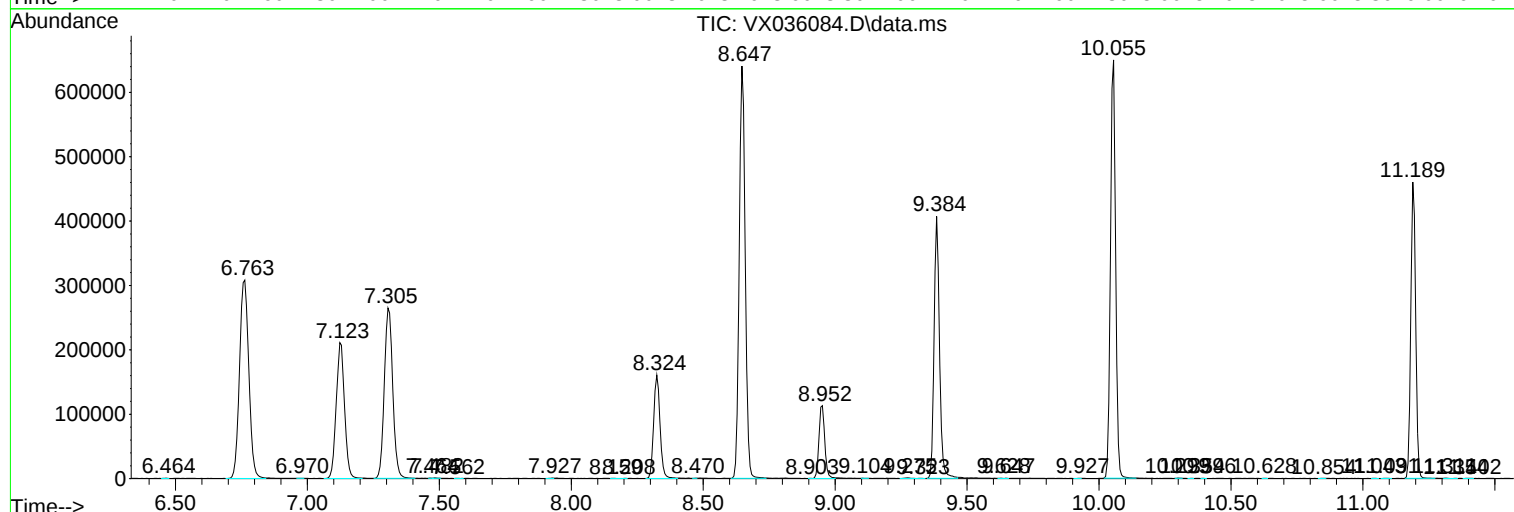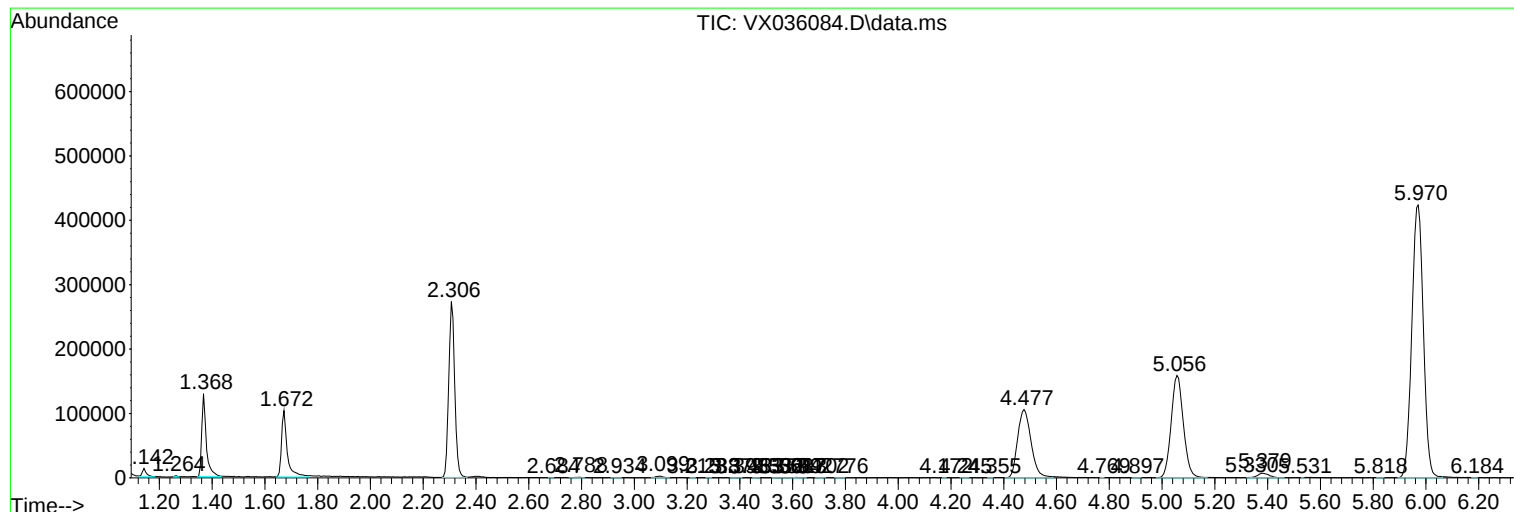

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036084.D
Acq On : 08 Jun 2023 20:35
Operator : JC/MD
Sample : 03097-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036084.D
Acq On : 08 Jun 2023 20:35
Operator : JC/MD
Sample : 03097-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc