

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036085.D
 Acq On : 08 Jun 2023 20:59
 Operator : JC/MD
 Sample : 03097-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	8361	9535	0.74%	0.098%
2	1.264	27	29	33	rVB2	1504	1201	0.09%	0.012%
3	1.368	42	46	60	rVB	130179	157360	12.15%	1.621%
4	1.672	91	96	110	rBV	103651	151178	11.68%	1.557%
5	2.306	194	200	212	rVB	280767	431876	33.35%	4.449%
6	2.508	231	233	236	rBV2	396	359	0.03%	0.004%
7	2.788	275	279	285	rVV2	1154	2119	0.16%	0.022%
8	2.947	304	305	307	rBV	409	254	0.02%	0.003%
9	2.995	310	313	314	rBV2	189	211	0.02%	0.002%
10	3.696	425	428	430	rBV	225	297	0.02%	0.003%
11	3.776	439	441	443	rBV	296	241	0.02%	0.002%
12	3.855	452	454	458	rVB2	187	232	0.02%	0.002%
13	3.898	458	461	463	rBV2	176	219	0.02%	0.002%
14	4.026	480	482	485	rVB2	263	263	0.02%	0.003%
15	4.288	524	525	529	rVB	244	288	0.02%	0.003%
16	4.318	529	530	533	rBB2	272	209	0.02%	0.002%
17	4.361	535	537	540	rVV	245	206	0.02%	0.002%
18	4.477	545	556	576	rBV	71909	255646	19.74%	2.634%
19	4.922	628	629	634	rVB	449	397	0.03%	0.004%
20	5.062	639	652	669	rBV3	180052	722113	55.77%	7.439%
21	5.251	680	683	684	rBV2	360	313	0.02%	0.003%
22	5.385	699	705	716	rVB5	1739	4735	0.37%	0.049%
23	5.550	726	732	740	rBV4	1185	3088	0.24%	0.032%
24	5.970	787	801	817	rBV2	427548	1294855	100.00%	13.339%
25	6.263	844	849	851	rBV2	229	338	0.03%	0.003%
26	6.318	857	858	862	rVB2	187	244	0.02%	0.003%
27	6.373	865	867	870	rVB	192	204	0.02%	0.002%
28	6.440	875	878	879	rBV2	257	286	0.02%	0.003%
29	6.592	901	903	907	rBV2	184	226	0.02%	0.002%
30	6.757	921	930	944	rBV	305732	744362	57.49%	7.668%
31	7.031	972	975	982	rVB3	299	505	0.04%	0.005%
32	7.123	982	990	1005	rBV2	66463	148569	11.47%	1.531%
33	7.306	1011	1020	1032	rBV	270628	595691	46.00%	6.137%
34	7.482	1044	1049	1054	rBV3	864	1880	0.15%	0.019%
35	7.623	1069	1072	1075	rBV2	245	182	0.01%	0.002%
36	7.647	1075	1076	1079	rBV2	202	184	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036085.D
 Acq On : 08 Jun 2023 20:59
 Operator : JC/MD
 Sample : 03097-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.824	1099	1105	1113	rBV	12049	21856	1.69%	0.225%
38	7.933	1117	1123	1129	rBV4	812	1494	0.12%	0.015%
39	8.031	1136	1139	1141	rVB	379	243	0.02%	0.003%
40	8.055	1141	1143	1146	rBV2	243	224	0.02%	0.002%
41	8.122	1152	1154	1159	rBV2	294	537	0.04%	0.006%
42	8.257	1175	1176	1178	rBV2	219	185	0.01%	0.002%
43	8.324	1180	1187	1200	rVV	167218	269528	20.82%	2.777%
44	8.580	1227	1229	1231	rBV	250	190	0.01%	0.002%
45	8.647	1233	1240	1258	rBV	670630	1031300	79.65%	10.624%
46	8.897	1280	1281	1283	rBV2	237	219	0.02%	0.002%
47	8.945	1284	1289	1298	rVV	114520	174266	13.46%	1.795%
48	9.074	1308	1310	1312	rBV	233	181	0.01%	0.002%
49	9.195	1327	1330	1333	rBV2	328	334	0.03%	0.003%
50	9.275	1341	1343	1347	rVB2	432	475	0.04%	0.005%
51	9.384	1355	1361	1378	rBV	387445	564802	43.62%	5.818%
52	9.659	1404	1406	1408	rBV2	252	291	0.02%	0.003%
53	9.799	1428	1429	1435	rVB2	440	578	0.04%	0.006%
54	10.055	1465	1471	1487	rVB	627463	880215	67.98%	9.068%
55	10.244	1498	1502	1506	rVB3	413	628	0.05%	0.006%
56	10.537	1548	1550	1553	rVB2	207	207	0.02%	0.002%
57	10.756	1583	1586	1587	rBV	182	180	0.01%	0.002%
58	10.939	1614	1616	1619	rVB	502	401	0.03%	0.004%
59	11.085	1635	1640	1644	rVB4	642	861	0.07%	0.009%
60	11.189	1652	1657	1665	rBV	448845	570799	44.08%	5.880%
61	11.378	1684	1688	1691	rBV2	257	380	0.03%	0.004%
62	11.433	1695	1697	1701	rBV2	259	417	0.03%	0.004%
63	11.707	1740	1742	1745	rBV2	324	323	0.02%	0.003%
64	11.793	1754	1756	1758	rBV	233	186	0.01%	0.002%
65	11.933	1777	1779	1781	rVB2	222	196	0.02%	0.002%
66	12.018	1788	1793	1803	rBV	630867	799305	61.73%	8.234%
67	12.177	1818	1819	1824	rBV	279	399	0.03%	0.004%
68	12.231	1824	1828	1829	rVV3	769	978	0.08%	0.010%
69	12.250	1829	1831	1833	rVB2	335	295	0.02%	0.003%
70	12.317	1837	1842	1852	rBV	681471	843856	65.17%	8.693%
71	12.494	1868	1871	1873	rBV	212	188	0.01%	0.002%
72	12.762	1913	1915	1917	rVB2	280	276	0.02%	0.003%
73	13.109	1969	1972	1973	rBV2	259	241	0.02%	0.002%
74	13.292	2001	2002	2005	rVB	304	238	0.02%	0.002%
75	13.317	2005	2006	2007	rBV	411	183	0.01%	0.002%
76	13.432	2024	2025	2029	rVB	241	188	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036085.D
 Acq On : 08 Jun 2023 20:59
 Operator : JC/MD
 Sample : 03097-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	13.469	2029	2031	2034	rBV	166	220	0.02%	0.002%
78	13.524	2039	2040	2042	rBV2	306	231	0.02%	0.002%
79	13.579	2047	2049	2052	rVB	301	258	0.02%	0.003%
80	13.615	2052	2055	2058	rBV3	274	384	0.03%	0.004%
81	13.774	2078	2081	2086	rVB2	531	584	0.05%	0.006%
82	13.829	2088	2090	2092	rBV2	296	311	0.02%	0.003%
83	13.926	2102	2106	2109	rBV2	315	463	0.04%	0.005%
84	13.975	2112	2114	2117	rVV2	331	232	0.02%	0.002%
85	14.030	2120	2123	2125	rBV2	429	408	0.03%	0.004%
86	14.109	2134	2136	2139	rBV2	299	383	0.03%	0.004%
87	14.225	2153	2155	2159	rBV2	297	211	0.02%	0.002%
88	14.298	2166	2167	2169	rBV	230	241	0.02%	0.002%
89	14.335	2172	2173	2175	rBV2	291	290	0.02%	0.003%
90	14.390	2180	2182	2185	rVV2	314	269	0.02%	0.003%
91	14.908	2264	2267	2268	rBV2	398	382	0.03%	0.004%
92	14.926	2268	2270	2272	rBV2	416	414	0.03%	0.004%
93	15.194	2310	2314	2317	rBV2	493	816	0.06%	0.008%
94	15.335	2336	2337	2338	rBV	419	214	0.02%	0.002%
95	15.377	2342	2344	2347	rBV	448	403	0.03%	0.004%
96	15.542	2369	2371	2374	rVB2	797	720	0.06%	0.007%
97	15.755	2403	2406	2408	rBV2	539	492	0.04%	0.005%
98	15.859	2421	2423	2424	rBV	444	248	0.02%	0.003%
99	16.469	2521	2523	2527	rBV2	753	733	0.06%	0.008%
100	16.664	2553	2555	2559	rBV3	420	596	0.05%	0.006%

Sum of corrected areas: 9707012




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036085.D
Acq On : 08 Jun 2023 20:59
Operator : JC/MD
Sample : 03097-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

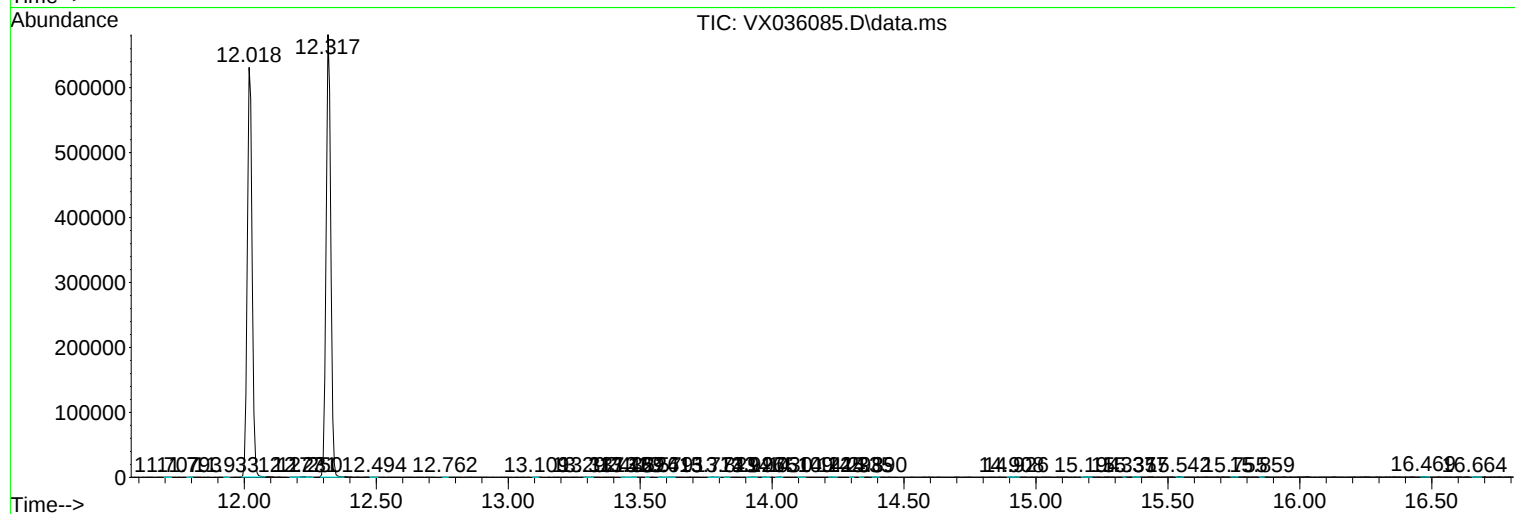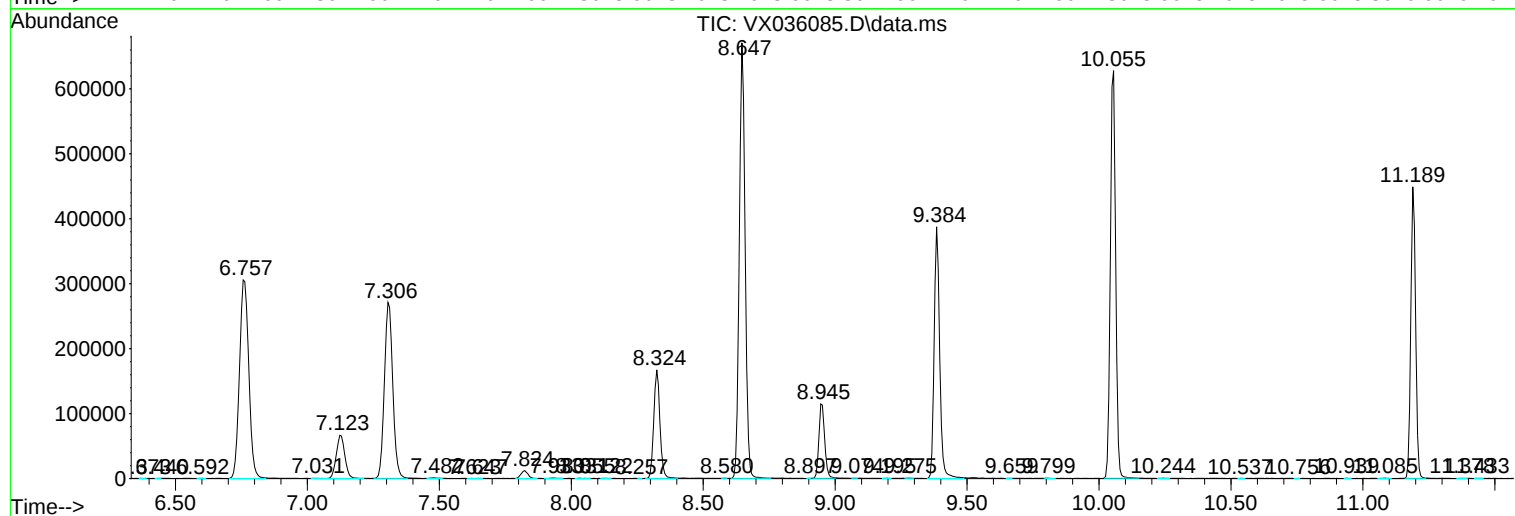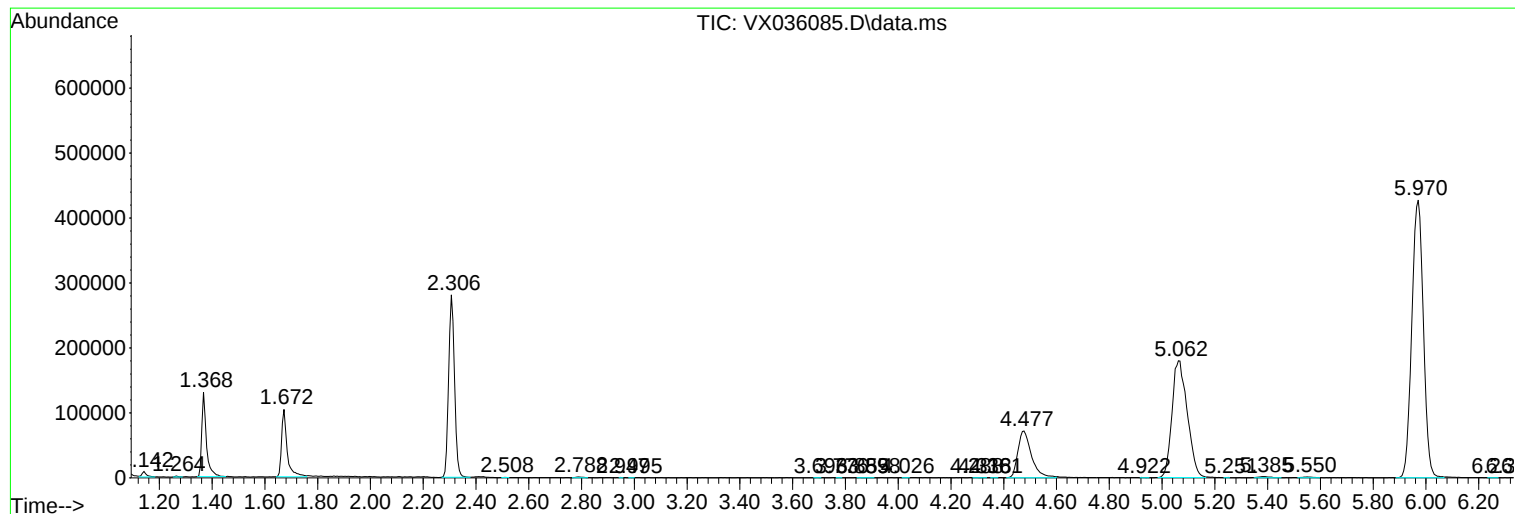

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036085.D
Acq On : 08 Jun 2023 20:59
Operator : JC/MD
Sample : 03097-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036085.D
Acq On : 08 Jun 2023 20:59
Operator : JC/MD
Sample : 03097-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------