

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036086.D
 Acq On : 08 Jun 2023 21:22
 Operator : JC/MD
 Sample : 03097-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	9677	10711	0.87%	0.118%
2	1.264	27	29	32	rVB3	1924	1806	0.15%	0.020%
3	1.368	42	46	57	rBV	123876	151155	12.23%	1.661%
4	1.672	91	96	106	rBV	99399	143514	11.62%	1.577%
5	2.306	193	200	211	rBV	264558	407060	32.95%	4.472%
6	2.514	230	234	235	rBV	326	321	0.03%	0.004%
7	2.550	238	240	242	rVV	332	233	0.02%	0.003%
8	2.599	246	248	250	rVB	331	199	0.02%	0.002%
9	2.715	265	267	270	rBV2	225	187	0.02%	0.002%
10	2.788	276	279	283	rVB3	709	820	0.07%	0.009%
11	2.916	298	300	305	rVB2	232	224	0.02%	0.002%
12	3.038	317	320	321	rBV	316	268	0.02%	0.003%
13	3.081	324	327	328	rBV2	303	298	0.02%	0.003%
14	3.148	337	338	342	rBV2	138	194	0.02%	0.002%
15	3.203	342	347	349	rBV2	280	318	0.03%	0.003%
16	3.258	353	356	357	rBV	293	250	0.02%	0.003%
17	3.501	392	396	398	rBV2	346	438	0.04%	0.005%
18	3.568	403	407	408	rBV2	207	240	0.02%	0.003%
19	3.636	417	418	421	rBV	151	179	0.01%	0.002%
20	3.898	459	461	464	rVV2	164	179	0.01%	0.002%
21	4.013	479	480	485	rBV2	188	292	0.02%	0.003%
22	4.081	489	491	493	rBV	217	191	0.02%	0.002%
23	4.471	545	555	580	rVV	73259	251099	20.32%	2.759%
24	4.721	594	596	598	rBV2	465	451	0.04%	0.005%
25	4.837	612	615	616	rBV2	203	237	0.02%	0.003%
26	5.062	639	652	669	rBV	156938	496692	40.20%	5.457%
27	5.282	685	688	690	rBV	268	249	0.02%	0.003%
28	5.373	701	703	705	rBV2	701	612	0.05%	0.007%
29	5.538	725	730	731	rBV2	815	901	0.07%	0.010%
30	5.794	770	772	775	rBV2	214	281	0.02%	0.003%
31	5.970	787	801	817	rBV3	415830	1235433	100.00%	13.573%
32	6.202	836	839	841	rBV2	237	342	0.03%	0.004%
33	6.428	874	876	878	rBV	190	182	0.01%	0.002%
34	6.519	889	891	893	rBV2	234	193	0.02%	0.002%
35	6.586	899	902	904	rBV2	262	275	0.02%	0.003%
36	6.757	919	930	943	rBV	306016	729715	59.07%	8.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036086.D
 Acq On : 08 Jun 2023 21:22
 Operator : JC/MD
 Sample : 03097-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.062	979	980	983	rBV	229	215	0.02%	0.002%
38	7.098	983	986	987	rBV2	1159	1275	0.10%	0.014%
39	7.306	1009	1020	1038	rBV	256654	562896	45.56%	6.184%
40	7.647	1073	1076	1077	rBV	202	189	0.02%	0.002%
41	7.708	1084	1086	1088	rVB2	329	206	0.02%	0.002%
42	7.751	1088	1093	1096	rBV2	155	276	0.02%	0.003%
43	7.787	1098	1099	1100	rBV	338	197	0.02%	0.002%
44	7.848	1106	1109	1112	rBV	280	327	0.03%	0.004%
45	7.927	1118	1122	1124	rBV2	714	805	0.07%	0.009%
46	8.159	1157	1160	1164	rVB	205	239	0.02%	0.003%
47	8.324	1180	1187	1197	rBV	158217	252415	20.43%	2.773%
48	8.476	1210	1212	1214	rVB2	535	379	0.03%	0.004%
49	8.519	1217	1219	1224	rVB2	338	322	0.03%	0.004%
50	8.647	1233	1240	1258	rBV	639346	985504	79.77%	10.827%
51	8.848	1272	1273	1277	rVB2	309	392	0.03%	0.004%
52	8.878	1277	1278	1280	rBV	239	216	0.02%	0.002%
53	8.952	1284	1290	1302	rBV	110760	169567	13.73%	1.863%
54	9.202	1330	1331	1336	rBV3	285	363	0.03%	0.004%
55	9.263	1340	1341	1342	rBV3	345	246	0.02%	0.003%
56	9.384	1355	1361	1374	rBV	392862	564212	45.67%	6.199%
57	9.738	1417	1419	1423	rVB2	392	424	0.03%	0.005%
58	9.945	1449	1453	1457	rVB2	226	396	0.03%	0.004%
59	10.012	1461	1464	1465	rBV2	181	194	0.02%	0.002%
60	10.055	1465	1471	1486	rVV	653223	872587	70.63%	9.586%
61	10.305	1506	1512	1515	rVB3	1004	1486	0.12%	0.016%
62	10.354	1519	1520	1524	rBV	262	294	0.02%	0.003%
63	10.628	1563	1565	1566	rBV	293	216	0.02%	0.002%
64	10.646	1566	1568	1571	rVB3	366	465	0.04%	0.005%
65	10.811	1593	1595	1599	rVB2	215	202	0.02%	0.002%
66	11.085	1637	1640	1643	rBV2	437	480	0.04%	0.005%
67	11.122	1643	1646	1647	rBV	232	226	0.02%	0.002%
68	11.189	1652	1657	1666	rBV	442322	570614	46.19%	6.269%
69	11.317	1674	1678	1684	rBV4	448	862	0.07%	0.009%
70	11.567	1717	1719	1724	rVB2	214	288	0.02%	0.003%
71	11.707	1740	1742	1745	rVB2	347	329	0.03%	0.004%
72	11.732	1745	1746	1749	rBV	284	229	0.02%	0.003%
73	11.884	1769	1771	1772	rVB2	299	179	0.01%	0.002%
74	11.902	1772	1774	1776	rBV	248	225	0.02%	0.002%
75	12.018	1788	1793	1804	rBV	640454	823189	66.63%	9.044%
76	12.177	1818	1819	1823	rVB	429	282	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036086.D
 Acq On : 08 Jun 2023 21:22
 Operator : JC/MD
 Sample : 03097-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.219	1823	1826	1833	rVB4	731	1048	0.08%	0.012%
78	12.317	1837	1842	1850	rBV	669848	844732	68.38%	9.280%
79	12.457	1863	1865	1869	rBV3	533	621	0.05%	0.007%
80	12.762	1914	1915	1917	rBV	335	240	0.02%	0.003%
81	12.933	1941	1943	1946	rVB2	295	307	0.02%	0.003%
82	12.963	1946	1948	1950	rBV	288	253	0.02%	0.003%
83	12.981	1950	1951	1955	rVB2	242	241	0.02%	0.003%
84	13.164	1977	1981	1984	rVB2	263	470	0.04%	0.005%
85	13.225	1989	1991	1994	rVB2	279	245	0.02%	0.003%
86	13.268	1996	1998	2000	rBV2	216	219	0.02%	0.002%
87	13.396	2016	2019	2021	rVV2	251	251	0.02%	0.003%
88	13.439	2024	2026	2029	rVB3	231	274	0.02%	0.003%
89	13.591	2049	2051	2053	rVB	247	192	0.02%	0.002%
90	13.615	2053	2055	2056	rBV	270	200	0.02%	0.002%
91	13.689	2064	2067	2071	rBV2	276	324	0.03%	0.004%
92	13.780	2080	2082	2084	rBV2	331	375	0.03%	0.004%
93	14.158	2143	2144	2148	rVB2	490	398	0.03%	0.004%
94	14.207	2148	2152	2153	rBV2	286	341	0.03%	0.004%
95	14.225	2153	2155	2159	rBV2	320	437	0.04%	0.005%
96	14.310	2168	2169	2172	rVB2	215	213	0.02%	0.002%
97	14.365	2175	2178	2181	rBV2	359	583	0.05%	0.006%
98	14.451	2190	2192	2194	rVB	338	236	0.02%	0.003%
99	14.646	2222	2224	2225	rBV	316	190	0.02%	0.002%
100	15.548	2368	2372	2374	rBV3	534	846	0.07%	0.009%




Sum of corrected areas: 9102383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036086.D
Acq On : 08 Jun 2023 21:22
Operator : JC/MD
Sample : 03097-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

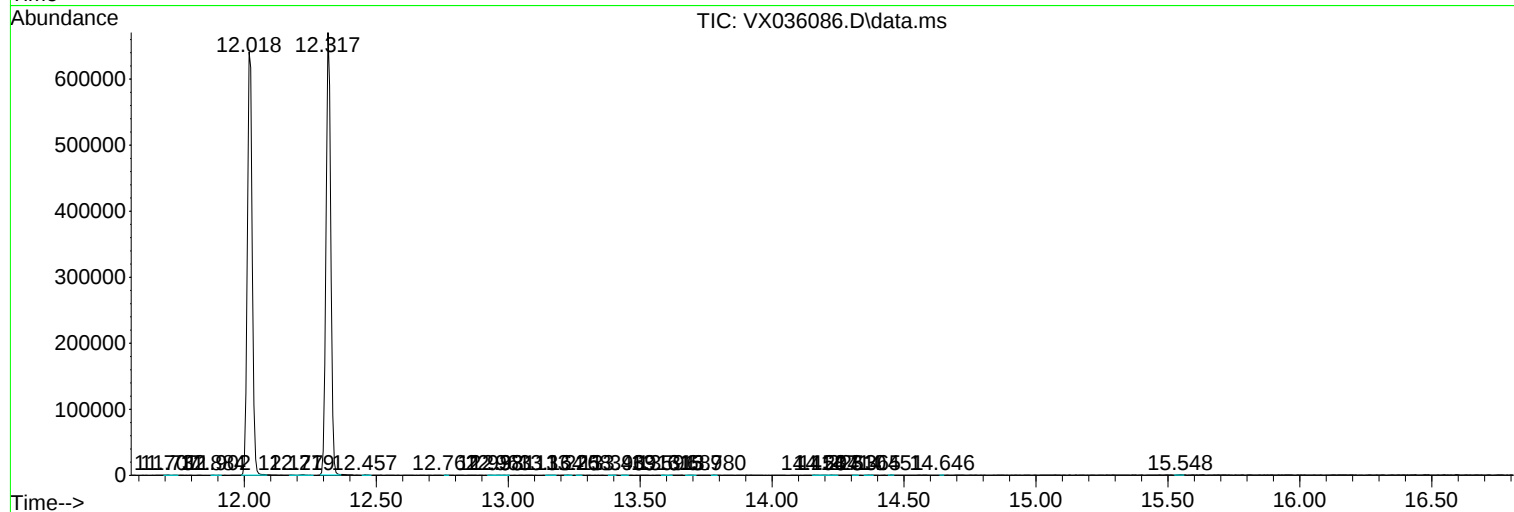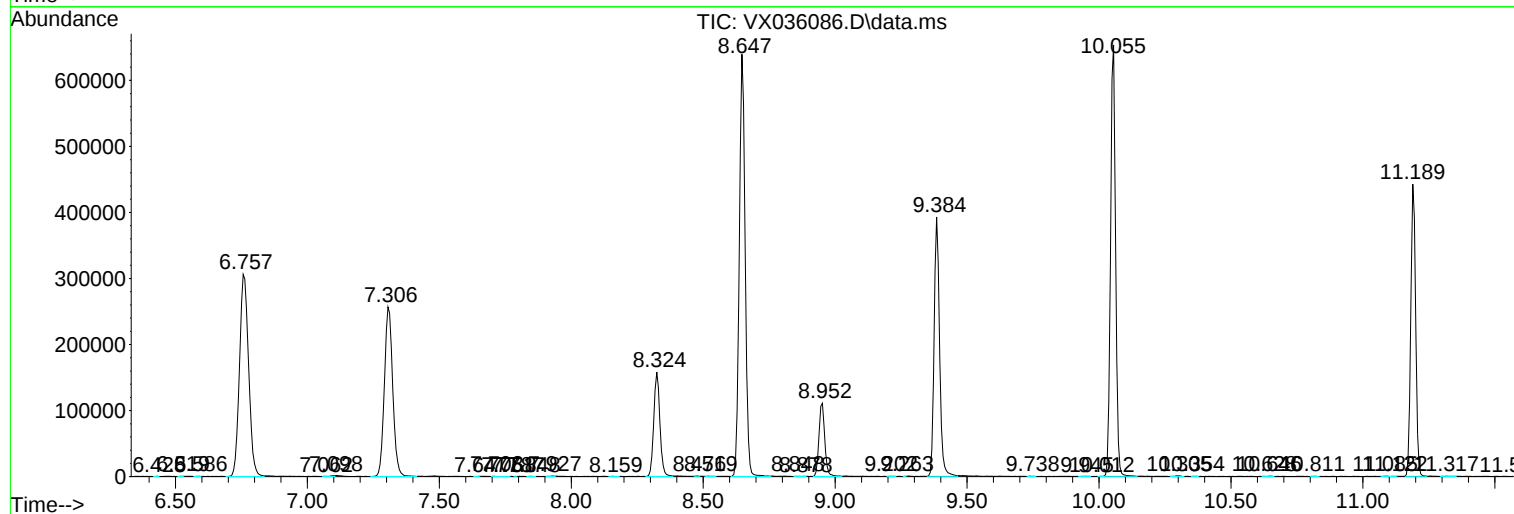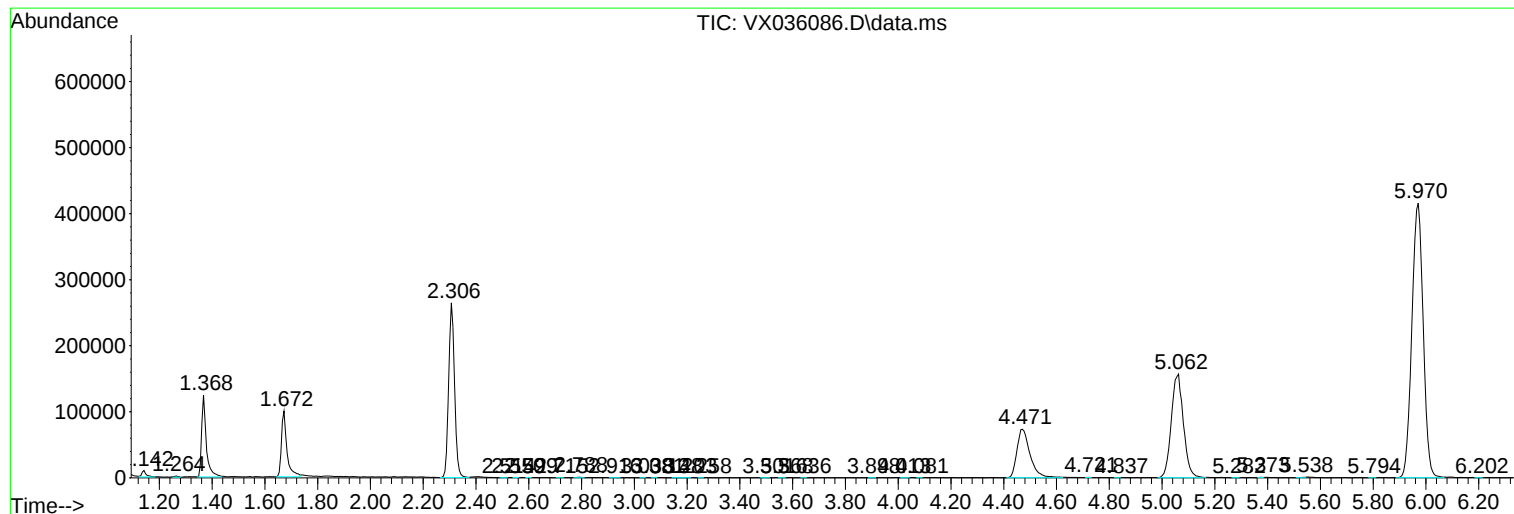

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036086.D
Acq On : 08 Jun 2023 21:22
Operator : JC/MD
Sample : 03097-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036086.D
Acq On : 08 Jun 2023 21:22
Operator : JC/MD
Sample : 03097-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc