

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036087.D
 Acq On : 08 Jun 2023 21:45
 Operator : JC/MD
 Sample : 03097-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZERO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	17	rVB	8877	10154	0.80%	0.109%
2	1.264	27	29	32	rBV2	1590	1365	0.11%	0.015%
3	1.368	42	46	58	rBV	129045	154635	12.16%	1.666%
4	1.672	91	96	113	rBV	98087	151867	11.95%	1.636%
5	2.306	194	200	210	rBV	267396	421445	33.15%	4.540%
6	2.794	276	280	284	rVB3	470	750	0.06%	0.008%
7	2.886	294	295	301	rBV2	288	399	0.03%	0.004%
8	2.995	312	313	316	rVB	289	180	0.01%	0.002%
9	3.038	318	320	323	rVV3	250	286	0.02%	0.003%
10	3.062	323	324	327	rVB2	335	294	0.02%	0.003%
11	3.111	330	332	333	rVB	337	169	0.01%	0.002%
12	3.197	345	346	349	rBV	217	213	0.02%	0.002%
13	3.361	371	373	374	rBV	233	167	0.01%	0.002%
14	3.434	382	385	386	rBV2	367	372	0.03%	0.004%
15	3.587	407	410	411	rBV	207	214	0.02%	0.002%
16	3.642	417	419	420	rBV2	194	170	0.01%	0.002%
17	3.660	420	422	425	rVB2	264	267	0.02%	0.003%
18	3.971	471	473	476	rVV2	194	193	0.02%	0.002%
19	4.172	503	506	507	rVB2	227	209	0.02%	0.002%
20	4.196	507	510	512	rBV2	291	285	0.02%	0.003%
21	4.471	546	555	576	rBV	73687	254139	19.99%	2.738%
22	4.727	596	597	600	rBV	262	180	0.01%	0.002%
23	4.873	619	621	623	rBV	277	247	0.02%	0.003%
24	5.056	638	651	670	rBV	168620	508660	40.01%	5.479%
25	5.562	726	734	737	rBV4	1006	2336	0.18%	0.025%
26	5.672	750	752	754	rVB2	325	199	0.02%	0.002%
27	5.970	788	801	815	rBV2	427361	1271281	100.00%	13.694%
28	6.214	839	841	843	rVB2	319	236	0.02%	0.003%
29	6.318	856	858	860	rBV2	260	246	0.02%	0.003%
30	6.604	903	905	908	rBV2	142	168	0.01%	0.002%
31	6.635	908	910	912	rBV	156	195	0.02%	0.002%
32	6.684	917	918	921	rBV	263	230	0.02%	0.002%
33	6.763	921	931	947	rBV	307757	739388	58.16%	7.965%
34	7.019	971	973	976	rBV3	242	226	0.02%	0.002%
35	7.117	982	989	993	rBV2	1378	2719	0.21%	0.029%
36	7.306	1010	1020	1038	rBV	262784	585080	46.02%	6.303%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036087.D
 Acq On : 08 Jun 2023 21:45
 Operator : JC/MD
 Sample : 03097-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZER0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	7.476	1046	1048	1051	rVB	574	484	0.04%	0.005%
38	7.842	1106	1108	1110	rVB2	252	173	0.01%	0.002%
39	7.879	1110	1114	1115	rBV	143	217	0.02%	0.002%
40	7.933	1118	1123	1124	rBV3	875	1016	0.08%	0.011%
41	8.019	1133	1137	1139	rBV	193	212	0.02%	0.002%
42	8.250	1173	1175	1176	rBV	267	171	0.01%	0.002%
43	8.324	1180	1187	1201	rBV	164239	263471	20.72%	2.838%
44	8.647	1231	1240	1254	rBV	652860	1014552	79.81%	10.929%
45	8.854	1272	1274	1278	rBV3	237	355	0.03%	0.004%
46	8.952	1284	1290	1302	rBV	113956	170709	13.43%	1.839%
47	9.208	1330	1332	1335	rVB2	291	216	0.02%	0.002%
48	9.275	1340	1343	1346	rBV3	402	535	0.04%	0.006%
49	9.384	1355	1361	1375	rBV	403034	572016	45.00%	6.162%
50	9.884	1441	1443	1445	rBV2	232	183	0.01%	0.002%
51	9.970	1455	1457	1460	rVB2	250	227	0.02%	0.002%
52	10.055	1465	1471	1485	rBV	636340	877498	69.02%	9.452%
53	10.305	1507	1512	1515	rBV2	883	1111	0.09%	0.012%
54	10.354	1518	1520	1524	rVV2	291	285	0.02%	0.003%
55	10.494	1541	1543	1545	rVV	273	177	0.01%	0.002%
56	10.537	1548	1550	1553	rVB2	282	199	0.02%	0.002%
57	10.573	1553	1556	1558	rBV2	232	276	0.02%	0.003%
58	10.604	1558	1561	1565	rBV2	213	260	0.02%	0.003%
59	10.793	1590	1592	1595	rVB2	214	184	0.01%	0.002%
60	10.909	1609	1611	1614	rBV2	179	210	0.02%	0.002%
61	11.000	1621	1626	1627	rBV2	178	250	0.02%	0.003%
62	11.085	1637	1640	1644	rVB3	437	534	0.04%	0.006%
63	11.122	1644	1646	1649	rVB2	238	274	0.02%	0.003%
64	11.189	1652	1657	1666	rBV	452895	579107	45.55%	6.238%
65	11.287	1671	1673	1675	rBV2	264	193	0.02%	0.002%
66	11.323	1675	1679	1680	rVV3	275	294	0.02%	0.003%
67	11.360	1683	1685	1690	rBV2	196	245	0.02%	0.003%
68	11.415	1693	1694	1697	rBV	191	222	0.02%	0.002%
69	11.469	1701	1703	1705	rBV	209	173	0.01%	0.002%
70	11.567	1717	1719	1721	rBV	163	174	0.01%	0.002%
71	11.677	1735	1737	1741	rVV2	323	370	0.03%	0.004%
72	11.707	1741	1742	1744	rVB	328	197	0.02%	0.002%
73	11.768	1750	1752	1755	rBV2	164	206	0.02%	0.002%
74	11.817	1759	1760	1762	rBV	272	201	0.02%	0.002%
75	12.018	1788	1793	1803	rBV	645424	826625	65.02%	8.904%
76	12.158	1815	1816	1820	rVB2	400	203	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036087.D
 Acq On : 08 Jun 2023 21:45
 Operator : JC/MD
 Sample : 03097-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZERO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.189	1820	1821	1824	rVB3	239	203	0.02%	0.002%
78	12.213	1824	1825	1829	rBV2	484	549	0.04%	0.006%
79	12.317	1837	1842	1854	rBV	682359	853803	67.16%	9.197%
80	12.768	1914	1916	1918	rBV	320	242	0.02%	0.003%
81	12.847	1927	1929	1930	rBV	306	267	0.02%	0.003%
82	12.981	1949	1951	1952	rBV	252	240	0.02%	0.003%
83	12.994	1952	1953	1956	rVV2	431	378	0.03%	0.004%
84	13.195	1983	1986	1989	rVB	194	204	0.02%	0.002%
85	13.225	1989	1991	1993	rBV	163	180	0.01%	0.002%
86	13.317	2003	2006	2007	rBV2	197	195	0.02%	0.002%
87	13.372	2013	2015	2017	rBV2	217	194	0.02%	0.002%
88	13.542	2039	2043	2044	rBV2	262	369	0.03%	0.004%
89	13.646	2058	2060	2062	rVB	339	199	0.02%	0.002%
90	13.689	2065	2067	2069	rVB2	268	202	0.02%	0.002%
91	13.780	2080	2082	2085	rBV3	281	285	0.02%	0.003%
92	14.115	2135	2137	2140	rBV	249	245	0.02%	0.003%
93	14.207	2150	2152	2154	rBV2	258	235	0.02%	0.003%
94	14.390	2181	2182	2186	rBV2	235	269	0.02%	0.003%
95	14.670	2225	2228	2229	rBV2	294	377	0.03%	0.004%
96	14.755	2240	2242	2246	rBV2	401	447	0.04%	0.005%
97	14.883	2261	2263	2266	rBV	314	189	0.01%	0.002%
98	14.938	2270	2272	2274	rVB2	394	218	0.02%	0.002%
99	15.920	2431	2433	2436	rVB2	556	397	0.03%	0.004%
100	16.706	2561	2562	2563	rBV	418	225	0.02%	0.002%




Sum of corrected areas: 9283281

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036087.D
Acq On : 08 Jun 2023 21:45
Operator : JC/MD
Sample : 03097-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZER0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

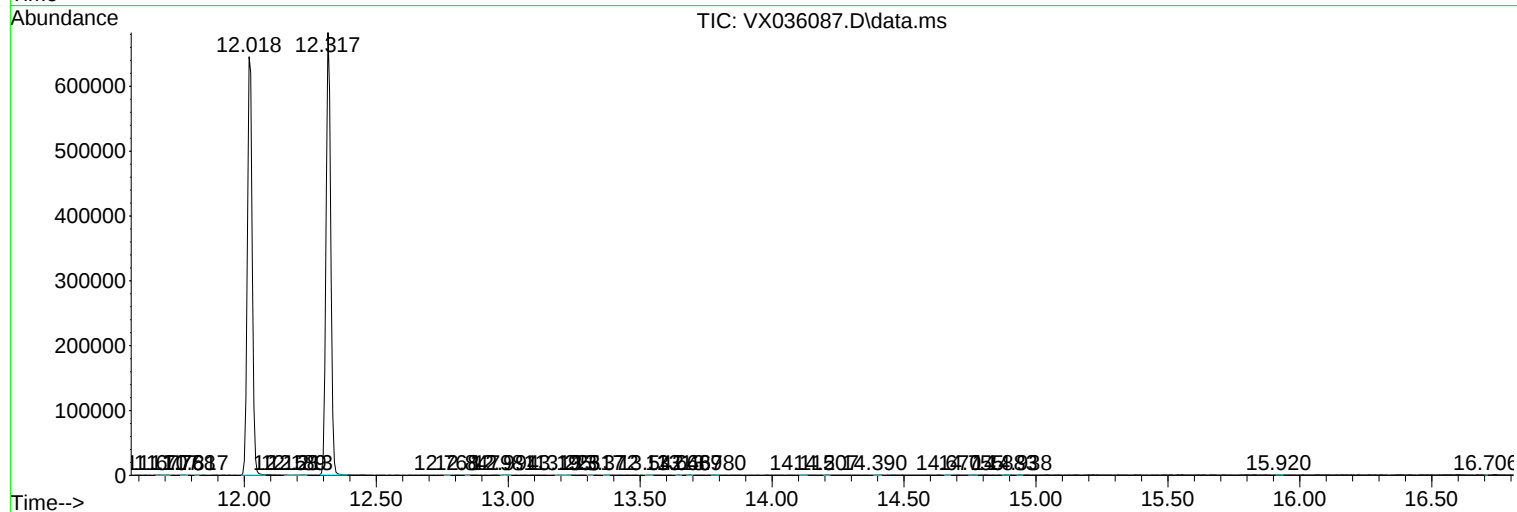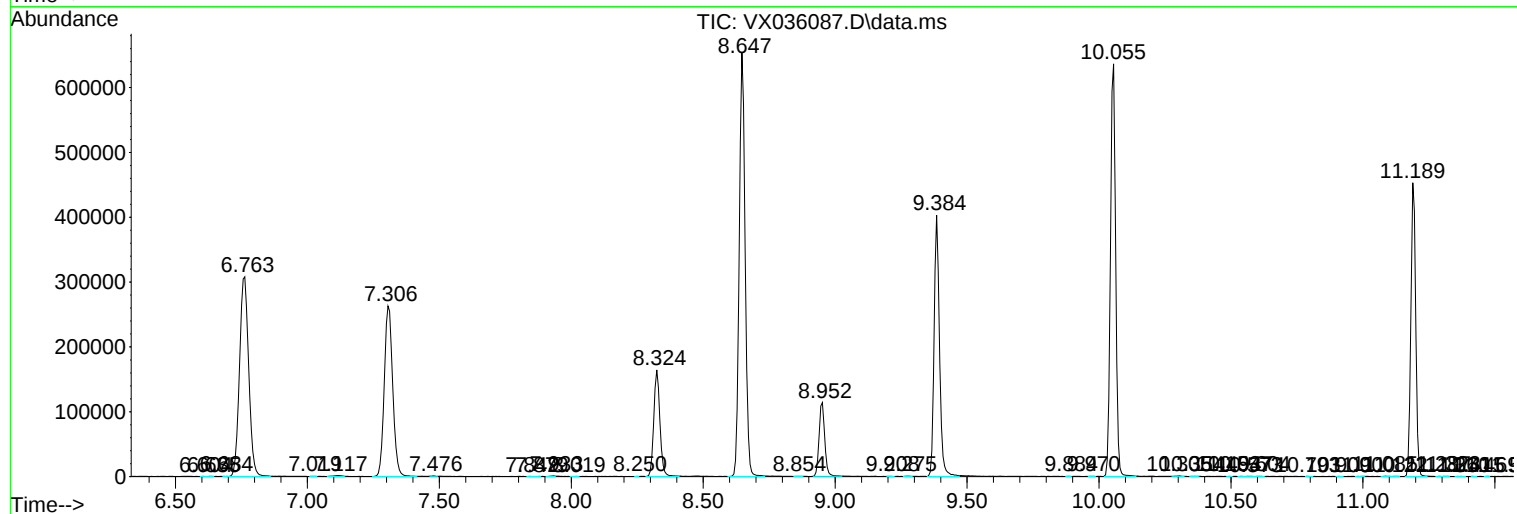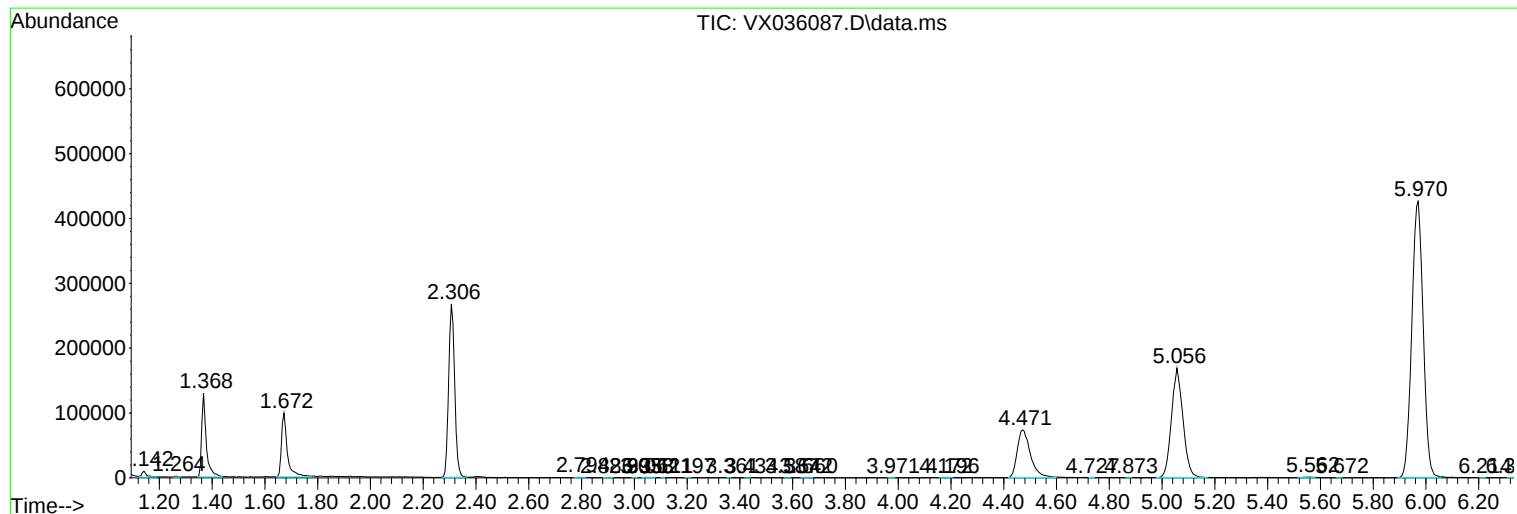

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036087.D
Acq On : 08 Jun 2023 21:45
Operator : JC/MD
Sample : 03097-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZERO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036087.D
Acq On : 08 Jun 2023 21:45
Operator : JC/MD
Sample : 03097-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZERO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc