

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036089.D
 Acq On : 08 Jun 2023 22:32
 Operator : JC/MD
 Sample : 03097-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	17178	18187	1.42%	0.194%
2	1.367	42	46	59	rBV	128319	157144	12.28%	1.674%
3	1.672	91	96	113	rBV	103045	153980	12.03%	1.640%
4	2.245	188	190	191	rBV2	424	235	0.02%	0.003%
5	2.306	193	200	210	rVV	266905	421298	32.91%	4.488%
6	2.459	224	225	228	rVB2	372	191	0.01%	0.002%
7	2.709	264	266	268	rBV	395	407	0.03%	0.004%
8	2.788	276	279	282	rBV3	587	922	0.07%	0.010%
9	2.843	286	288	290	rVB2	288	247	0.02%	0.003%
10	2.873	290	293	294	rBV2	281	184	0.01%	0.002%
11	2.892	294	296	299	rBV2	203	153	0.01%	0.002%
12	3.117	332	333	334	rVB	363	133	0.01%	0.001%
13	3.190	343	345	347	rBV	263	197	0.02%	0.002%
14	3.641	416	419	422	rBV	180	248	0.02%	0.003%
15	3.690	426	427	430	rVB	268	200	0.02%	0.002%
16	3.727	430	433	434	rBV	291	290	0.02%	0.003%
17	3.776	440	441	446	rBV2	209	258	0.02%	0.003%
18	3.818	446	448	452	rVB2	234	312	0.02%	0.003%
19	3.867	452	456	459	rBV2	397	555	0.04%	0.006%
20	3.964	468	472	475	rVV	198	288	0.02%	0.003%
21	4.013	478	480	481	rBV	220	133	0.01%	0.001%
22	4.141	499	501	504	rVB	312	256	0.02%	0.003%
23	4.471	545	555	581	rBV	74986	262257	20.49%	2.794%
24	4.788	605	607	608	rBV	281	217	0.02%	0.002%
25	4.891	623	624	626	rBV	295	250	0.02%	0.003%
26	5.056	637	651	671	rBV	169464	509133	39.78%	5.423%
27	5.324	694	695	697	rBV	226	190	0.01%	0.002%
28	5.367	699	702	703	rBV2	1177	1087	0.08%	0.012%
29	5.543	726	731	733	rBV2	1003	1676	0.13%	0.018%
30	5.653	746	749	751	rBV2	206	288	0.02%	0.003%
31	5.867	782	784	786	rVB	252	136	0.01%	0.001%
32	5.970	788	801	817	rBV2	426279	1280018	100.00%	13.635%
33	6.153	829	831	834	rBV	316	336	0.03%	0.004%
34	6.238	843	845	846	rBV2	279	134	0.01%	0.001%
35	6.367	864	866	869	rVB2	233	191	0.01%	0.002%
36	6.488	885	886	887	rBV	258	156	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036089.D
 Acq On : 08 Jun 2023 22:32
 Operator : JC/MD
 Sample : 03097-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.531	891	893	894	rBV2	245	169	0.01%	0.002%
38	6.616	905	907	908	rBV	300	160	0.01%	0.002%
39	6.757	920	930	944	rBV	305413	740767	57.87%	7.891%
40	6.976	963	966	969	rBV2	341	470	0.04%	0.005%
41	7.019	972	973	976	rVB2	407	273	0.02%	0.003%
42	7.122	982	990	999	rBV4	15564	34324	2.68%	0.366%
43	7.305	1010	1020	1033	rBV	264896	581200	45.41%	6.191%
44	7.433	1039	1041	1044	rVB2	256	189	0.01%	0.002%
45	7.647	1074	1076	1077	rBV	246	211	0.02%	0.002%
46	7.756	1092	1094	1097	rVB2	165	130	0.01%	0.001%
47	7.891	1113	1116	1119	rBV	194	278	0.02%	0.003%
48	7.927	1119	1122	1123	rBV2	590	557	0.04%	0.006%
49	8.086	1146	1148	1149	rVB	239	131	0.01%	0.001%
50	8.323	1180	1187	1204	rBV	161492	264900	20.70%	2.822%
51	8.482	1208	1213	1218	rVB5	665	1359	0.11%	0.014%
52	8.647	1233	1240	1263	rBV	644547	1015698	79.35%	10.819%
53	8.951	1284	1290	1300	rBV	111325	173288	13.54%	1.846%
54	9.275	1338	1343	1346	rBV3	679	1103	0.09%	0.012%
55	9.342	1352	1354	1355	rBV	225	149	0.01%	0.002%
56	9.384	1355	1361	1378	rVV	410189	580637	45.36%	6.185%
57	9.762	1420	1423	1424	rVB	347	223	0.02%	0.002%
58	9.848	1435	1437	1439	rVV	496	287	0.02%	0.003%
59	10.055	1465	1471	1482	rBV	630039	873056	68.21%	9.300%
60	10.152	1485	1487	1489	rVB	665	480	0.04%	0.005%
61	10.189	1491	1493	1498	rBV3	321	494	0.04%	0.005%
62	10.299	1509	1511	1516	rVB2	551	552	0.04%	0.006%
63	10.579	1554	1557	1561	rBV3	318	396	0.03%	0.004%
64	10.854	1598	1602	1605	rBV2	535	810	0.06%	0.009%
65	11.061	1633	1636	1638	rBV	259	281	0.02%	0.003%
66	11.085	1638	1640	1645	rVB3	676	728	0.06%	0.008%
67	11.189	1652	1657	1668	rBV	462475	585930	45.78%	6.241%
68	11.427	1694	1696	1698	rVB	261	169	0.01%	0.002%
69	11.664	1733	1735	1736	rVB	354	202	0.02%	0.002%
70	11.689	1736	1739	1741	rBV2	338	465	0.04%	0.005%
71	11.707	1741	1742	1746	rVB	297	298	0.02%	0.003%
72	11.853	1764	1766	1769	rBV2	232	195	0.02%	0.002%
73	12.018	1788	1793	1804	rBV	664751	828501	64.73%	8.825%
74	12.225	1822	1827	1832	rVB4	1659	2330	0.18%	0.025%
75	12.317	1837	1842	1851	rBV	701055	876736	68.49%	9.339%
76	12.621	1890	1892	1894	rVV	179	161	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036089.D
 Acq On : 08 Jun 2023 22:32
 Operator : JC/MD
 Sample : 03097-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	12.658	1897	1898	1900	rVB	349	154	0.01%	0.002%
78	12.682	1900	1902	1905	rBV	246	219	0.02%	0.002%
79	12.853	1927	1930	1934	rBV4	1634	2034	0.16%	0.022%
80	12.987	1950	1952	1953	rBV	273	192	0.01%	0.002%
81	13.018	1955	1957	1958	rBV	221	199	0.02%	0.002%
82	13.140	1976	1977	1980	rBV2	331	292	0.02%	0.003%
83	13.408	2018	2021	2022	rBV	295	287	0.02%	0.003%
84	13.463	2028	2030	2031	rBV	270	141	0.01%	0.002%
85	13.603	2051	2053	2056	rBV2	243	194	0.02%	0.002%
86	13.633	2056	2058	2059	rBV	249	166	0.01%	0.002%
87	13.743	2075	2076	2079	rVB2	326	194	0.02%	0.002%
88	13.774	2079	2081	2083	rBV	310	168	0.01%	0.002%
89	14.139	2138	2141	2142	rBV2	389	335	0.03%	0.004%
90	14.200	2149	2151	2152	rBV2	240	149	0.01%	0.002%
91	14.286	2163	2165	2168	rBV2	289	256	0.02%	0.003%
92	14.322	2169	2171	2174	rVV2	311	355	0.03%	0.004%
93	14.444	2190	2191	2193	rVB	468	250	0.02%	0.003%
94	14.475	2193	2196	2197	rBV2	352	388	0.03%	0.004%
95	14.493	2197	2199	2201	rVB2	326	224	0.02%	0.002%
96	14.554	2208	2209	2212	rBV2	356	260	0.02%	0.003%
97	14.895	2263	2265	2266	rBV2	349	311	0.02%	0.003%
98	15.036	2286	2288	2290	rVB	491	286	0.02%	0.003%
99	16.493	2525	2527	2529	rBV3	439	392	0.03%	0.004%
100	16.602	2543	2545	2546	rBV	618	361	0.03%	0.004%




Sum of corrected areas: 9387981

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036089.D
Acq On : 08 Jun 2023 22:32
Operator : JC/MD
Sample : 03097-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

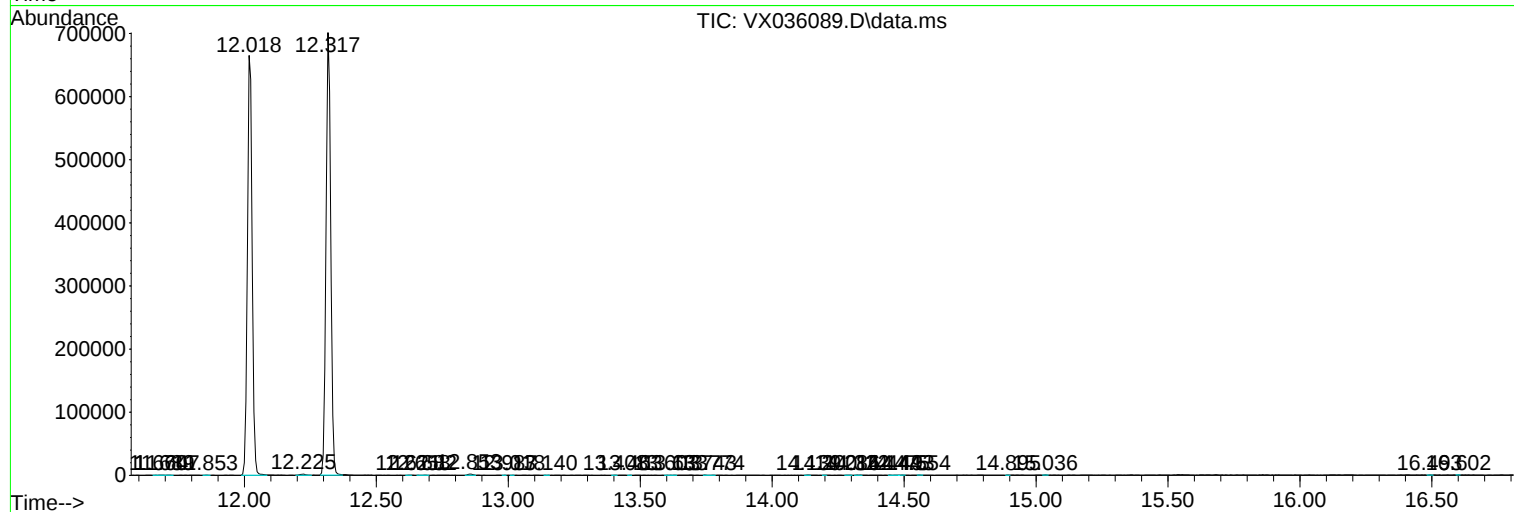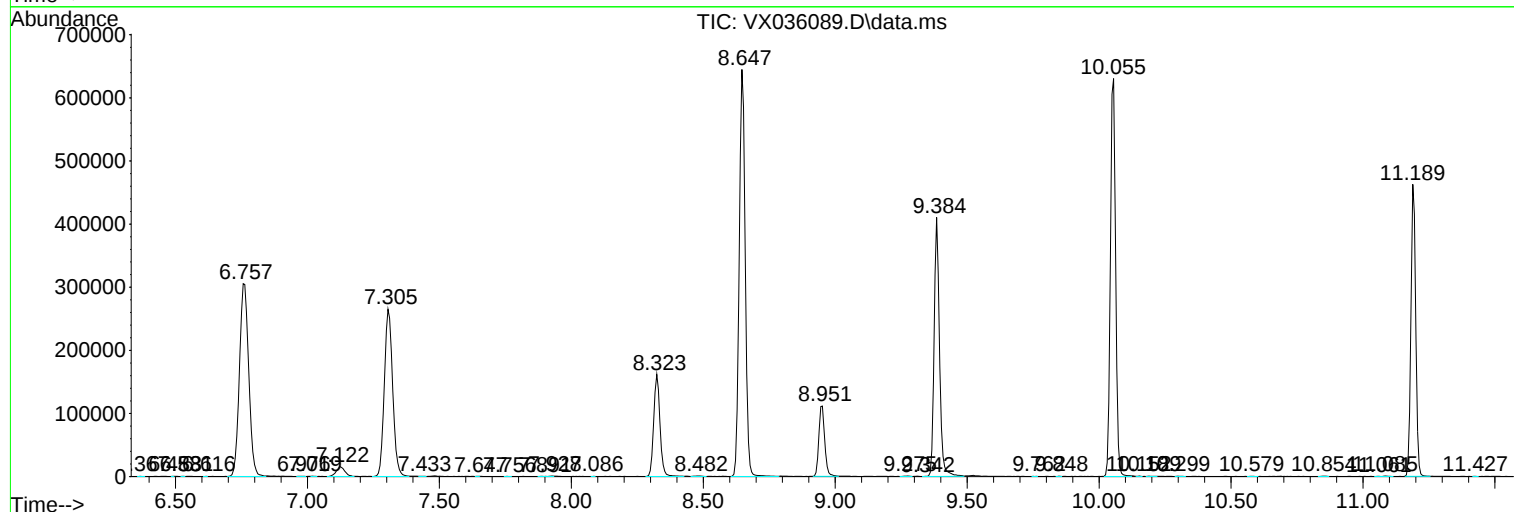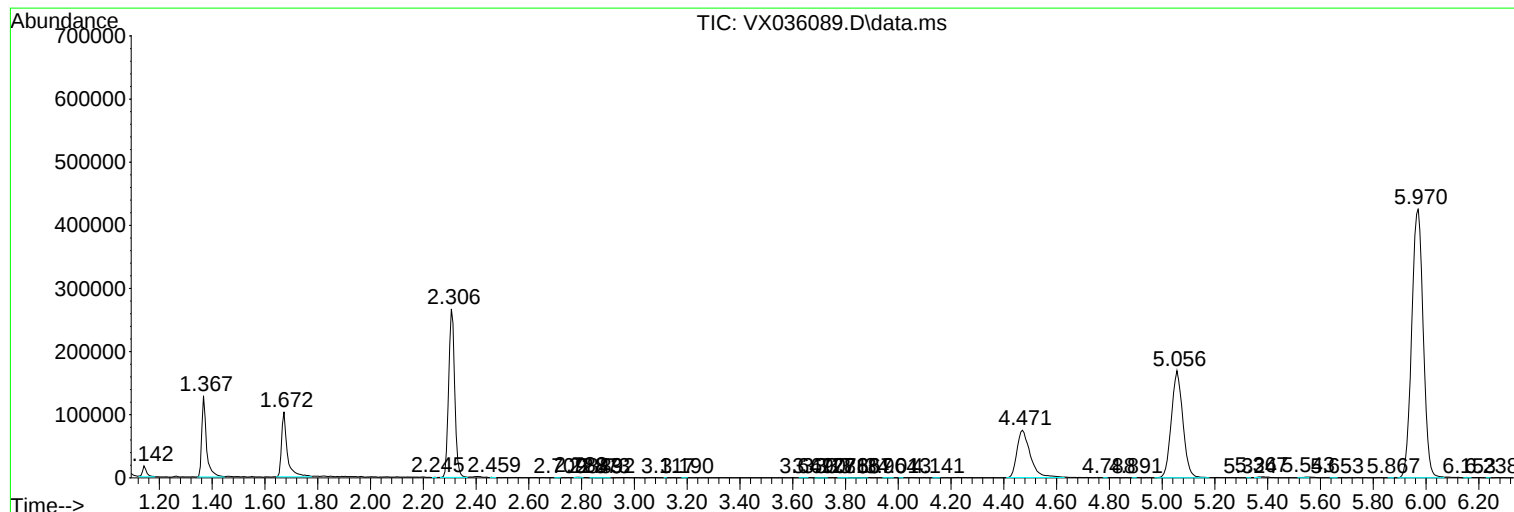

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036089.D
Acq On : 08 Jun 2023 22:32
Operator : JC/MD
Sample : 03097-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036089.D
Acq On : 08 Jun 2023 22:32
Operator : JC/MD
Sample : 03097-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc