

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036090.D
 Acq On : 08 Jun 2023 22:55
 Operator : JC/MD
 Sample : 03097-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

Signal : TIC: VX036090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	19	rVB2	19397	23503	1.85%	0.255%
2	1.368	42	46	57	rBV	126558	150836	11.85%	1.636%
3	1.672	91	96	106	rBV	100045	141745	11.14%	1.537%
4	2.160	174	176	178	rBV2	811	430	0.03%	0.005%
5	2.306	193	200	211	rBV	255704	401301	31.53%	4.352%
6	2.617	249	251	252	rVB	217	112	0.01%	0.001%
7	2.788	277	279	286	rVB2	996	1503	0.12%	0.016%
8	2.843	286	288	289	rVV	272	192	0.02%	0.002%
9	2.867	290	292	294	rVB	301	203	0.02%	0.002%
10	3.105	329	331	332	rVB	262	166	0.01%	0.002%
11	3.130	332	335	337	rBV2	210	222	0.02%	0.002%
12	3.184	343	344	346	rBV2	326	276	0.02%	0.003%
13	3.337	368	369	372	rBV	324	277	0.02%	0.003%
14	3.428	383	384	386	rVB	267	114	0.01%	0.001%
15	3.459	387	389	391	rVB2	229	129	0.01%	0.001%
16	3.477	391	392	394	rBV	219	115	0.01%	0.001%
17	3.507	396	397	398	rVV	257	120	0.01%	0.001%
18	3.550	402	404	405	rBV2	174	127	0.01%	0.001%
19	3.568	405	407	408	rVB2	257	145	0.01%	0.002%
20	3.764	438	439	440	rBV	252	174	0.01%	0.002%
21	3.879	456	458	460	rBV2	237	159	0.01%	0.002%
22	4.014	478	480	481	rBV	159	128	0.01%	0.001%
23	4.196	508	510	512	rBV2	178	131	0.01%	0.001%
24	4.215	512	513	515	rBV2	251	141	0.01%	0.002%
25	4.404	542	544	545	rBV2	232	142	0.01%	0.002%
26	4.471	545	555	576	rBV	72527	253918	19.95%	2.754%
27	4.861	617	619	621	rVB	320	220	0.02%	0.002%
28	4.885	621	623	624	rBV2	185	137	0.01%	0.001%
29	5.056	638	651	667	rBV	161785	509508	40.03%	5.526%
30	5.269	684	686	687	rVB2	308	160	0.01%	0.002%
31	5.294	689	690	692	rVV	220	124	0.01%	0.001%
32	5.385	698	705	713	rBV5	1471	3958	0.31%	0.043%
33	5.471	717	719	721	rBV	222	233	0.02%	0.003%
34	5.550	726	732	736	rBV3	975	2176	0.17%	0.024%
35	5.824	775	777	778	rBV	233	198	0.02%	0.002%
36	5.970	788	801	816	rBV2	425346	1272680	100.00%	13.802%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036090.D
 Acq On : 08 Jun 2023 22:55
 Operator : JC/MD
 Sample : 03097-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

37	6.184	834	836	838	rBV2	249	219	0.02%	0.002%
38	6.233	841	844	847	rBV2	213	188	0.01%	0.002%
39	6.257	847	848	851	rBV2	378	286	0.02%	0.003%
40	6.598	903	904	907	rVB2	230	184	0.01%	0.002%
41	6.629	907	909	911	rBV2	161	221	0.02%	0.002%
42	6.757	921	930	944	rBV	305323	735722	57.81%	7.979%
43	7.123	983	990	1001	rBV4	14629	33207	2.61%	0.360%
44	7.306	1011	1020	1035	rBV	269118	592631	46.57%	6.427%
45	7.482	1043	1049	1054	rVB6	768	1342	0.11%	0.015%
46	7.629	1071	1073	1075	rVB2	226	192	0.02%	0.002%
47	7.647	1075	1076	1079	rBV	275	210	0.02%	0.002%
48	7.732	1088	1090	1093	rBV2	240	270	0.02%	0.003%
49	7.757	1093	1094	1099	rVB2	271	292	0.02%	0.003%
50	7.873	1111	1113	1118	rVB	184	219	0.02%	0.002%
51	7.927	1118	1122	1123	rBV2	537	565	0.04%	0.006%
52	8.037	1139	1140	1144	rBV2	221	219	0.02%	0.002%
53	8.251	1174	1175	1177	rBV	245	200	0.02%	0.002%
54	8.324	1180	1187	1199	rBV	161042	261925	20.58%	2.841%
55	8.531	1219	1221	1222	rBV2	183	132	0.01%	0.001%
56	8.647	1233	1240	1251	rBV	631595	975416	76.64%	10.578%
57	8.842	1271	1272	1274	rBV	210	223	0.02%	0.002%
58	8.952	1283	1290	1302	rBV	113673	173997	13.67%	1.887%
59	9.159	1323	1324	1326	rVB	220	157	0.01%	0.002%
60	9.281	1337	1344	1346	rBV3	600	1074	0.08%	0.012%
61	9.384	1355	1361	1381	rBV	406891	576548	45.30%	6.253%
62	9.689	1409	1411	1412	rBV	243	166	0.01%	0.002%
63	10.055	1465	1471	1487	rBV	631929	865714	68.02%	9.389%
64	10.299	1506	1511	1516	rBV3	519	915	0.07%	0.010%
65	10.372	1521	1523	1526	rVV	455	403	0.03%	0.004%
66	10.403	1526	1528	1529	rVB	279	138	0.01%	0.001%
67	10.500	1542	1544	1545	rBV	178	179	0.01%	0.002%
68	10.518	1545	1547	1548	rVB2	400	213	0.02%	0.002%
69	10.829	1594	1598	1601	rBV2	284	541	0.04%	0.006%
70	10.860	1601	1603	1606	rVV2	169	183	0.01%	0.002%
71	11.189	1652	1657	1668	rVB	464229	582169	45.74%	6.314%
72	11.311	1674	1677	1681	rVB2	479	639	0.05%	0.007%
73	11.451	1696	1700	1703	rBV2	172	277	0.02%	0.003%
74	11.494	1705	1707	1711	rVB2	260	240	0.02%	0.003%
75	11.713	1739	1743	1744	rBV3	461	447	0.04%	0.005%
76	11.793	1754	1756	1757	rBV	261	171	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
 Data File : VX036090.D
 Acq On : 08 Jun 2023 22:55
 Operator : JC/MD
 Sample : 03097-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EZEN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
 Title : VOC Analysis

77	11.957	1781	1783	1785	rBV2	203	226	0.02%	0.002%
78	12.018	1788	1793	1805	rVV	618685	805320	63.28%	8.734%
79	12.116	1808	1809	1810	rVB	459	173	0.01%	0.002%
80	12.225	1823	1827	1833	rVB3	1132	1939	0.15%	0.021%
81	12.317	1837	1842	1853	rVB	672825	832537	65.42%	9.029%
82	12.463	1862	1866	1869	rBV2	559	606	0.05%	0.007%
83	12.646	1893	1896	1897	rBV2	227	187	0.01%	0.002%
84	12.786	1917	1919	1921	rBV	191	145	0.01%	0.002%
85	12.853	1927	1930	1937	rVB4	1504	1868	0.15%	0.020%
86	12.902	1937	1938	1939	rBV	274	115	0.01%	0.001%
87	13.030	1957	1959	1962	rBV	278	356	0.03%	0.004%
88	13.317	2005	2006	2009	rVB2	269	203	0.02%	0.002%
89	13.365	2012	2014	2016	rBV2	282	242	0.02%	0.003%
90	13.494	2033	2035	2036	rVB2	348	192	0.02%	0.002%
91	13.591	2049	2051	2054	rBV2	341	302	0.02%	0.003%
92	13.695	2066	2068	2071	rVB2	693	586	0.05%	0.006%
93	13.993	2116	2117	2120	rBV	229	201	0.02%	0.002%
94	14.018	2120	2121	2124	rBV	210	185	0.01%	0.002%
95	14.097	2130	2134	2136	rBV2	241	356	0.03%	0.004%
96	14.201	2148	2151	2153	rBV3	333	458	0.04%	0.005%
97	14.237	2156	2157	2158	rBV	289	134	0.01%	0.001%
98	14.317	2168	2170	2171	rBV	355	150	0.01%	0.002%
99	14.646	2222	2224	2226	rBV	396	310	0.02%	0.003%
100	15.060	2291	2292	2294	rVB	490	213	0.02%	0.002%




Sum of corrected areas: 9220741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036090.D
Acq On : 08 Jun 2023 22:55
Operator : JC/MD
Sample : 03097-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

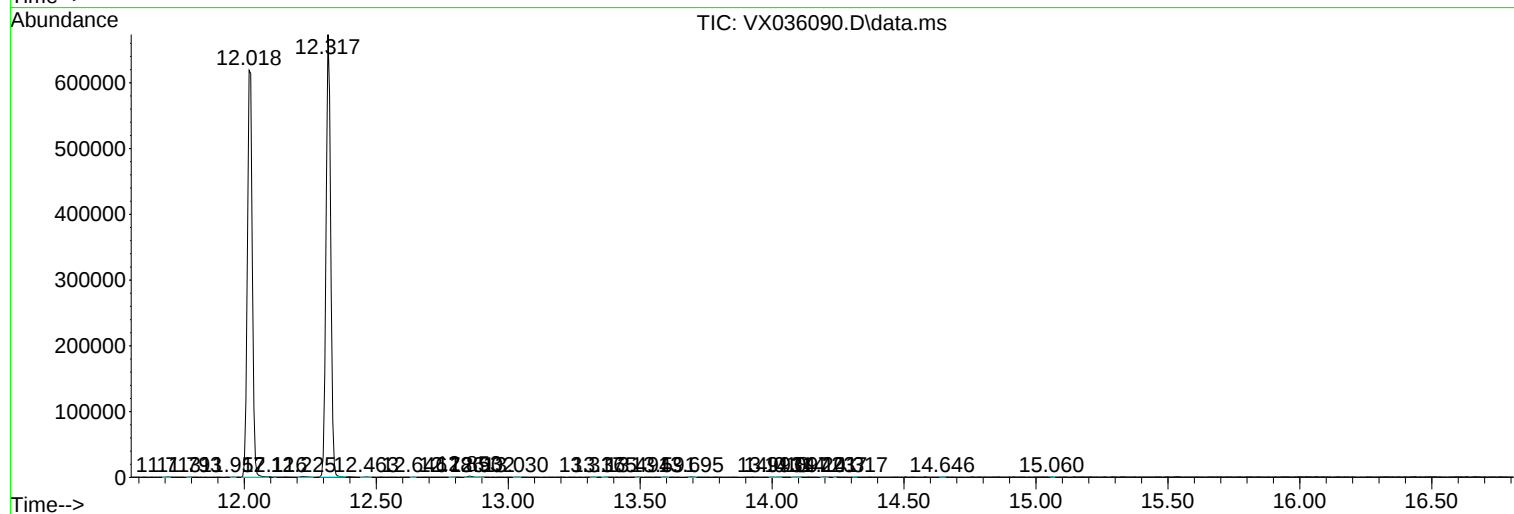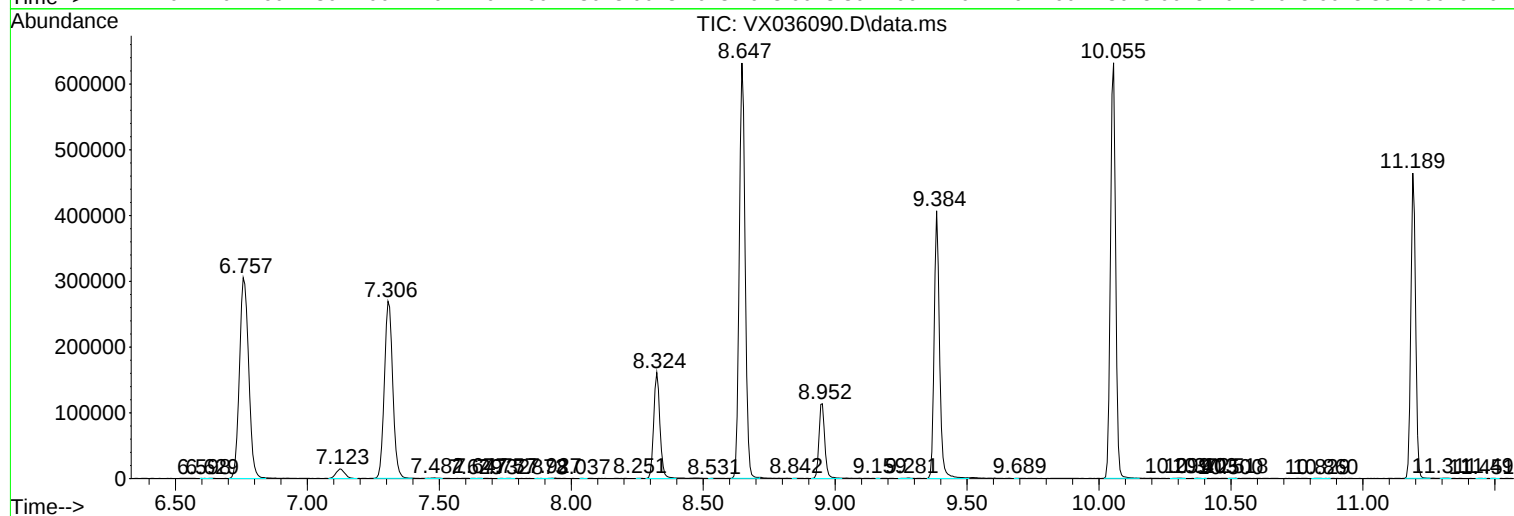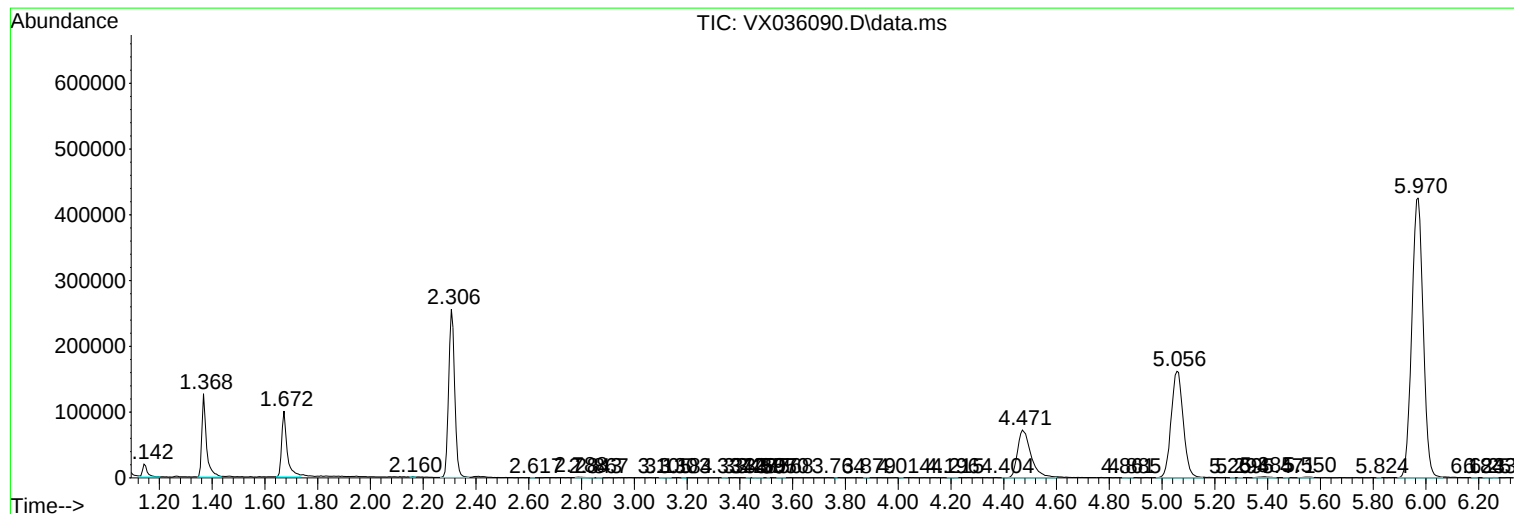

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036090.D
Acq On : 08 Jun 2023 22:55
Operator : JC/MD
Sample : 03097-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036090.D
Acq On : 08 Jun 2023 22:55
Operator : JC/MD
Sample : 03097-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EZEN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML060623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------