
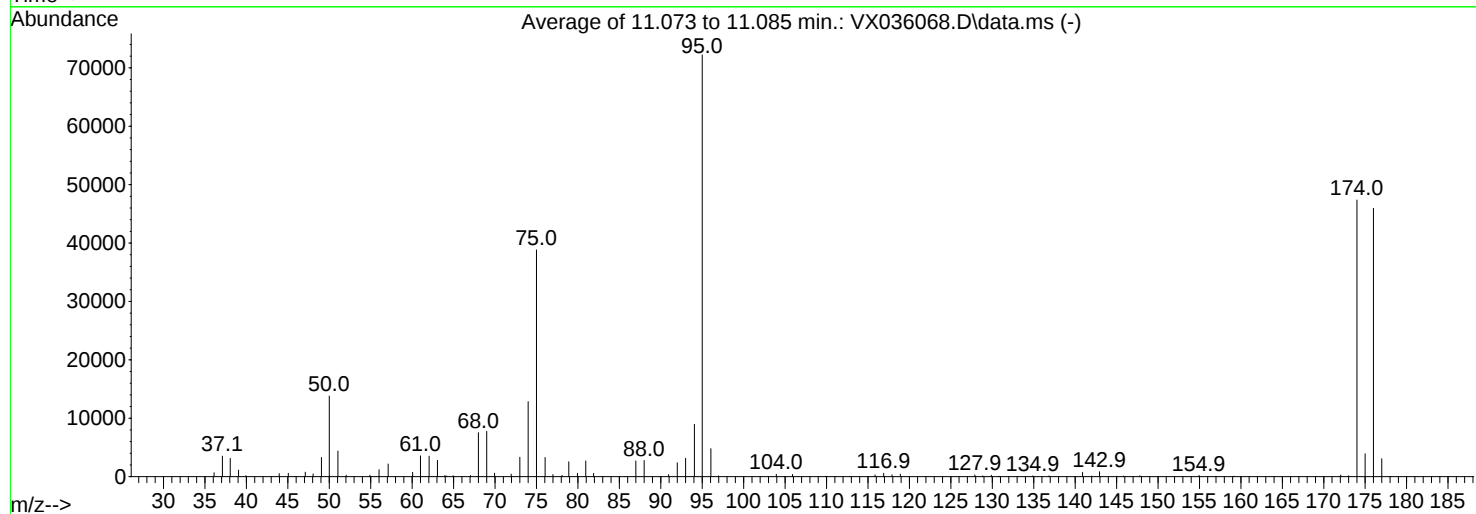


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060823\
Data File : VX036068.D
Acq On : 08 Jun 2023 13:42
Operator : JC/MD
Sample : BFB629
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB629

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM060623WMA.M
Title : VOC Analysis
Last Update : Wed Jun 07 05:37:48 2023

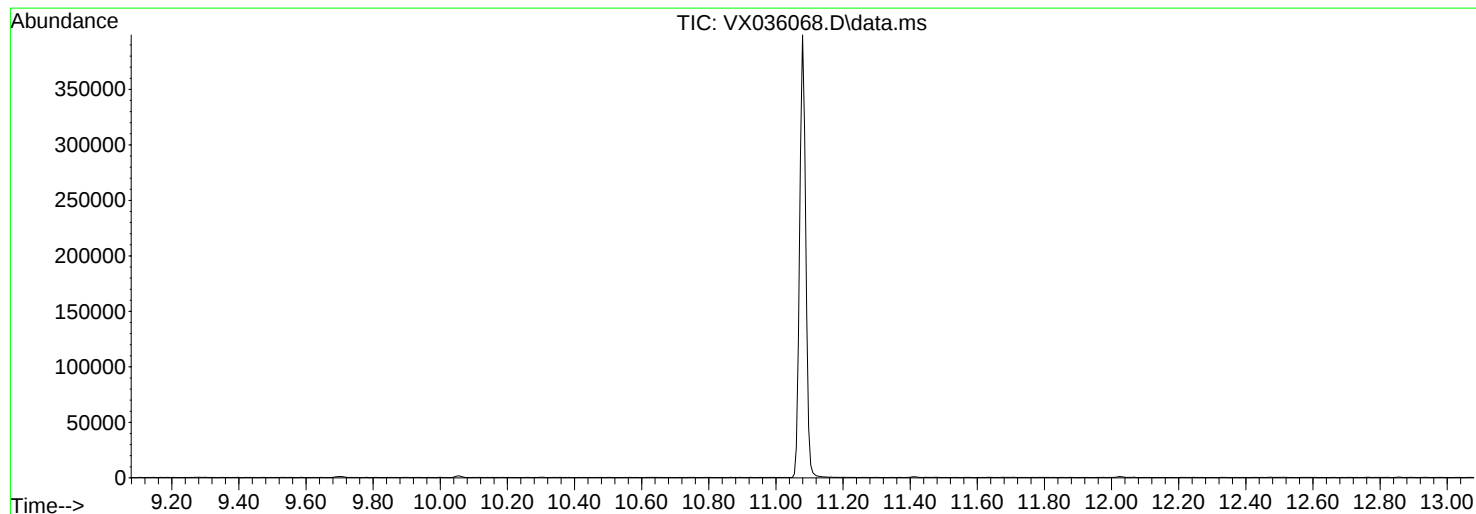

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	13815	PASS
75	95	30	80	53.7	38813	PASS
95	95	100	100	100.0	72219	PASS
96	95	5	9	6.6	4800	PASS
173	174	0.00	2	0.3	140	PASS
174	95	50	120	65.6	47357	PASS
175	174	5	9	8.3	3910	PASS
176	174	95	101	97.0	45936	PASS
177	176	5	9	6.7	3081	PASS

m/z	Abundance
39.00	66.0
40.10	134.0
43.90	76.0

Instrument :
MSVOA_X
ClientSampleId :
BFB629

m/z	Abundance
36.10	669.0
37.10	3579.0
38.00	3257.0
39.10	998.0
39.90	271.0
43.00	99.0
44.00	524.0
45.10	644.0
45.90	79.0
47.10	694.0
48.10	595.0
49.00	2924.0
50.00	13977.0
51.00	4158.0
52.10	235.0
55.00	343.0
56.00	1130.0
57.10	2304.0
58.00	79.0
60.10	701.0
61.00	3464.0
62.00	3134.0
63.10	2848.0
63.90	217.0
64.20	188.0
64.90	133.0
67.00	144.0
68.00	7413.0
69.00	6845.0
69.90	464.0
71.90	336.0
73.00	2828.0
74.00	12168.0
75.00	36208.0
76.10	3031.0
77.10	354.0
78.10	253.0
78.90	2343.0
79.90	512.0
81.00	2607.0
81.90	588.0
82.90	102.0
87.00	2594.0
88.00	2379.0
90.90	314.0
92.00	2129.0
93.00	2846.0
94.00	7735.0
95.00	64184.0
96.00	4481.0
96.90	159.0
104.00	345.0
104.90	67.0
105.90	302.0
109.90	58.0
111.10	60.0
115.90	275.0
116.90	406.0
117.90	290.0
118.80	344.0
127.90	301.0
128.80	105.0
129.90	158.0
130.70	71.0
134.90	106.0
136.80	128.0
140.90	616.0
141.90	55.0
142.90	658.0
145.10	54.0
145.80	86.0
147.80	176.0
154.90	326.0
159.20	91.0
172.00	222.0
173.00	421.0
174.00	36656.0
175.00	3285.0
176.00	33304.0
177.00	2612.0
178.10	83.0

Instrument :
MSVOA_X
ClientSampleId :
BFB629

m/z	Abundance
36.10	665.0
37.10	4007.0
38.10	3661.0
39.10	1455.0
40.00	187.0
43.10	73.0
44.00	746.0
45.00	701.0
45.80	65.0
47.10	917.0
48.00	493.0
49.10	4217.0
50.00	16688.0
51.00	5326.0
52.00	244.0
54.90	269.0
56.00	1432.0
57.10	2296.0
58.00	63.0
60.00	854.0
61.00	4141.0
62.10	4083.0
63.10	2954.0
64.00	420.0
65.00	140.0
67.10	215.0
68.00	8623.0
69.00	9055.0
70.00	786.0
71.90	621.0
73.00	3896.0
74.00	14746.0
75.00	46368.0
76.00	4062.0
76.90	482.0
78.10	440.0
78.90	3132.0
79.90	657.0
80.90	3131.0
81.90	561.0
83.10	64.0
87.00	3523.0
88.00	3597.0
91.00	383.0
92.00	3093.0
93.00	3684.0
94.10	10806.0
95.00	86776.0
96.10	5748.0
97.00	135.0
104.00	428.0
105.10	107.0
105.90	445.0
109.90	86.0
115.80	355.0
116.90	797.0
117.90	404.0
118.90	516.0
127.90	337.0
128.90	180.0
129.80	401.0
130.90	129.0
134.90	168.0
136.80	109.0
140.90	854.0
142.00	214.0
143.00	1185.0
145.00	104.0
145.90	131.0
146.70	60.0
147.80	133.0
150.00	92.0
155.00	199.0
156.90	109.0
159.20	54.0
172.10	423.0
174.00	57128.0
175.00	4313.0
176.00	55104.0
177.00	3629.0
178.10	110.0

Instrument :
MSVOA_X
ClientSampleId :
BFB629

m/z	Abundance
36.10	696.0
37.10	2976.0
38.00	2481.0
39.10	1100.0
40.20	136.0
44.00	551.0
45.10	394.0
47.10	673.0
48.00	327.0
49.00	2727.0
50.00	10781.0
51.10	3675.0
52.00	242.0
54.80	173.0
56.00	957.0
57.10	1886.0
60.00	683.0
61.00	3095.0
62.00	3315.0
63.00	2582.0
64.20	157.0
65.00	204.0
67.00	225.0
68.00	6551.0
69.00	7380.0
70.00	571.0
72.00	367.0
73.00	3225.0
74.00	11665.0
75.00	33864.0
76.00	2803.0
76.90	220.0
78.90	2136.0
80.00	600.0
80.90	2315.0
81.90	625.0
83.00	99.0
85.70	70.0
87.00	1949.0
88.00	2350.0
90.80	218.0
91.10	192.0
92.00	1910.0
93.00	2910.0
94.00	8308.0
95.00	65696.0
96.00	4171.0
96.90	91.0
103.90	427.0
105.90	408.0
112.80	65.0
115.10	57.0
115.90	273.0
116.90	555.0
117.90	301.0
119.00	487.0
127.90	270.0
128.90	147.0
130.00	201.0
130.90	58.0
134.90	156.0
136.90	173.0
140.90	766.0
141.90	82.0
142.90	721.0
145.00	90.0
145.90	104.0
147.80	192.0
155.00	126.0
156.90	91.0
159.10	81.0
172.00	216.0
174.00	48288.0
175.00	4131.0
176.00	49400.0
177.00	3002.0

Instrument :
MSVOA_X
ClientSampleId :
BFB629