

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060921\
 Data File : VX022628.D
 Acq On : 09 Jun 2021 20:49
 Operator : JC/MD
 Sample : M2610-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 W-8

Quant Time: Jun 10 05:46:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 07 14:27:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	55014	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	109090	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	97120	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	36555	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	47404	48.47	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	96.94%
35) Dibromofluoromethane	5.397	113	34031	49.86	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.72%
50) Toluene-d8	8.653	98	135745	49.84	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.68%
62) 4-Bromofluorobenzene	11.085	95	47028	46.46	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.92%


Target Compounds					Qvalue	
3) Chloromethane	1.294	50	187	0.24	ug/l #	42
6) Chloroethane	1.654	64	134	0.28	ug/l #	43
14) Allyl chloride	2.550	41	290	0.23	ug/l #	1
16) Acetone	2.392	43	842	1.92	ug/l	90
17) Carbon Disulfide	2.532	76	754	3.79	ug/l #	75
20) Methylene Chloride	2.800	84	364	0.40	ug/l #	67
27) cis-1,2-Dichloroethene	4.495	96	1343	1.46	ug/l	85
29) Tetrahydrofuran	5.032	42	87	0.20	ug/l #	27
31) Cyclohexane	5.471	56	1544	1.33	ug/l #	80
36) 1,1-Dichloropropene	5.562	75	5417	5.13	ug/l #	49
38) Carbon Tetrachloride	5.562	117	6520	8.45	ug/l #	15
39) Methylcyclohexane	7.385	83	2359	3.77	ug/l #	82
40) Benzene	6.044	78	945	0.29	ug/l #	84
47) Bromodichloromethane	7.891	83	64	2.50	ug/l #	25
52) Toluene	8.726	92	474	0.23	ug/l	95
55) 1,1,2-Trichloroethane	9.098	97	1044	1.31	ug/l #	15
56) Ethyl methacrylate	9.110	69	164	2.81	ug/l #	1
67) Ethyl Benzene	10.195	91	2026	0.55	ug/l #	83
68) m/p-Xylenes	10.305	106	959	0.71	ug/l	96
73) Isopropylbenzene	10.963	105	10226	3.43	ug/l	99
76) 1,2,3-Trichloropropane	11.085	75	25460	26.88	ug/l #	39
78) n-propylbenzene	11.305	91	13791	3.81	ug/l	98
79) 2-Chlorotoluene	11.305	91	13791	6.41	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.616	105	1980	0.78	ug/l	81
81) trans-1,4-Dichloro-2-b...	11.085	75	25460	66.09	ug/l #	12
82) 4-Chlorotoluene	11.305	91	13791	5.54	ug/l #	45
85) sec-Butylbenzene	11.890	105	2143	0.71	ug/l	90
86) p-Isopropyltoluene	12.183	119	881	0.35	ug/l #	77
89) n-Butylbenzene	12.329	91	2143	0.89	ug/l #	54
90) Hexachloroethane	12.646	117	3775	11.90	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.927	75	252	4.60	ug/l #	1
95) Naphthalene	13.780	128	663	0.23	ug/l #	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060921\
Data File : VX022628.D
Acq On : 09 Jun 2021 20:49
Operator : JC/MD
Sample : M2610-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
W-8

Quant Time: Jun 10 05:46:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060721W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 07 14:27:50 2021
Response via : Initial Calibration




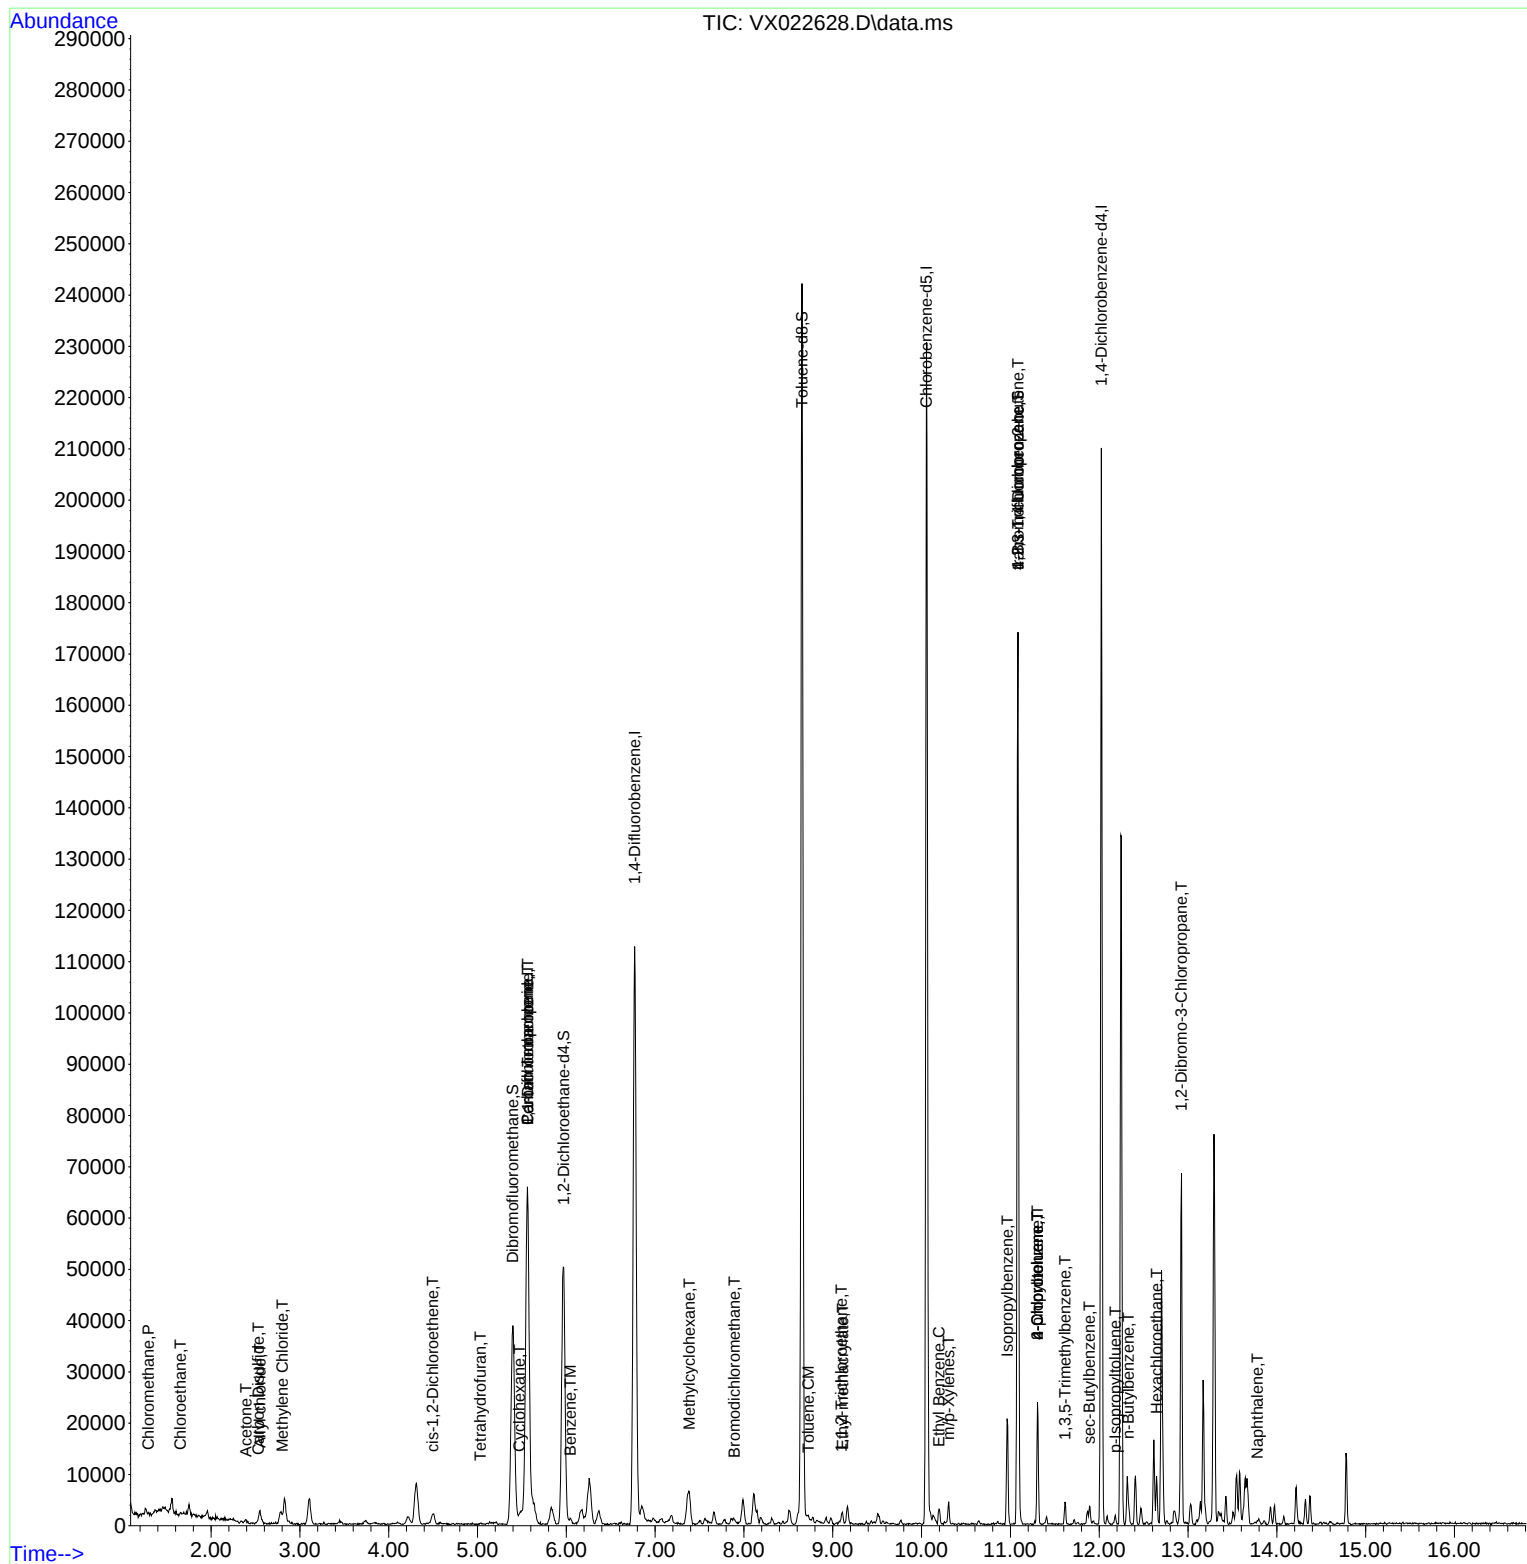


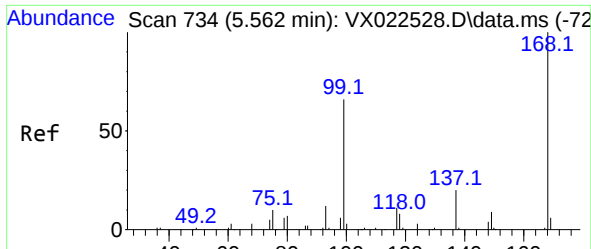

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion:168 Resp: 55014
Ion Ratio Lower Upper
168 100
99 67.4 45.8 68.6

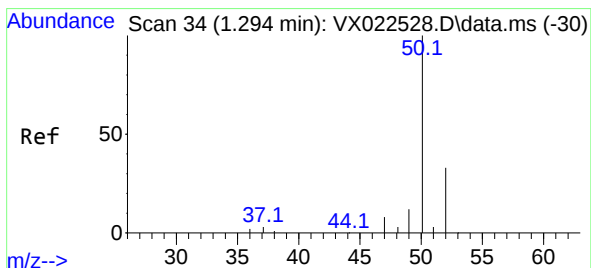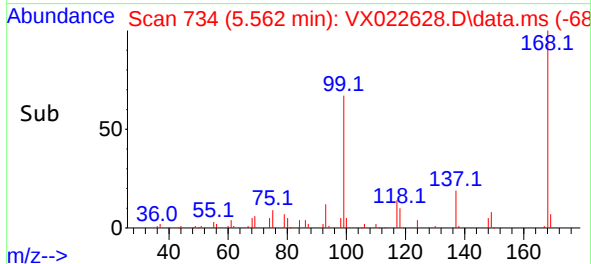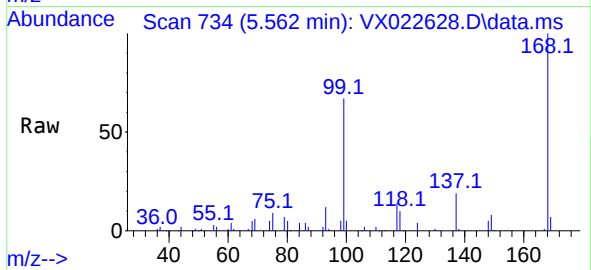

#3
Chloromethane
Concen: 0.24 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 50 Resp: 187
Ion Ratio Lower Upper
50 100
52 0.0 26.4 39.6#


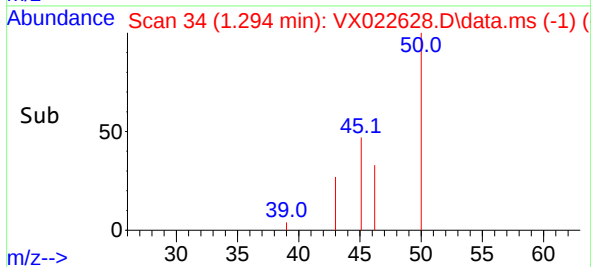

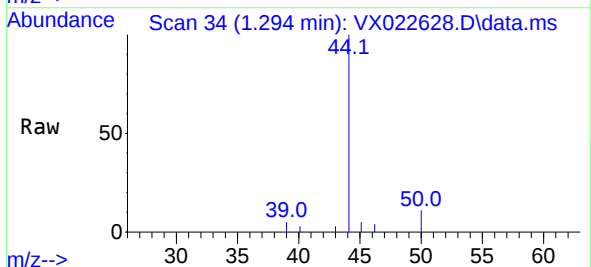


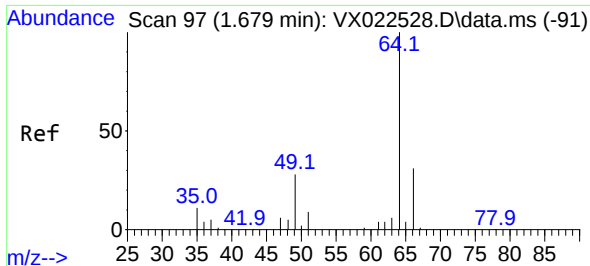

#6
Chloroethane
Concen: 0.28 ug/l
RT: 1.654 min Scan# 93
Delta R.T. -0.025 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion: 64 Resp: 134
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

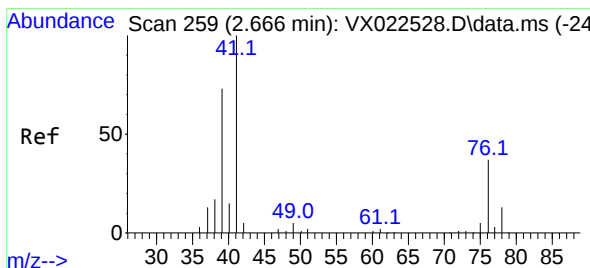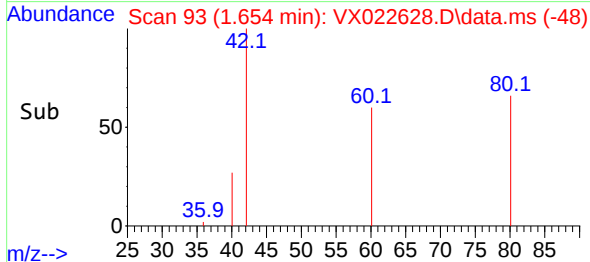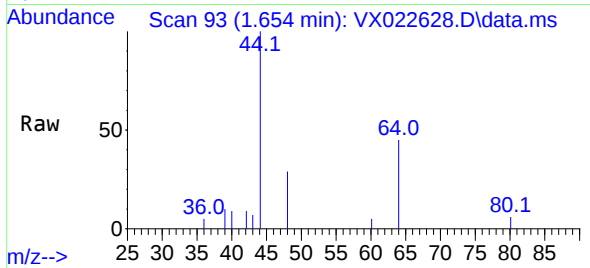

#14
Allyl chloride
Concen: 0.23 ug/l
RT: 2.550 min Scan# 240
Delta R.T. -0.116 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 41 Resp: 290
Ion Ratio Lower Upper
41 100
39 161.0 51.6 77.4#
76 119.7 30.5 45.7#


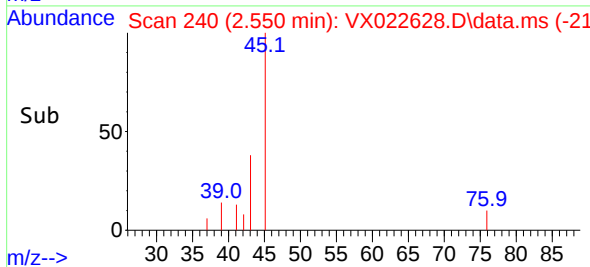

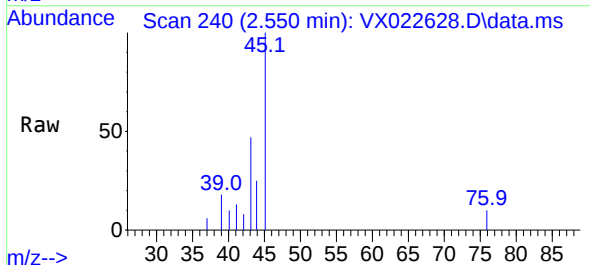




#16
Acetone
Concen: 1.92 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampleId :
W-8


Tgt Ion: 43 Resp: 842
Ion Ratio Lower Upper
43 100
58 40.9 27.8 41.8

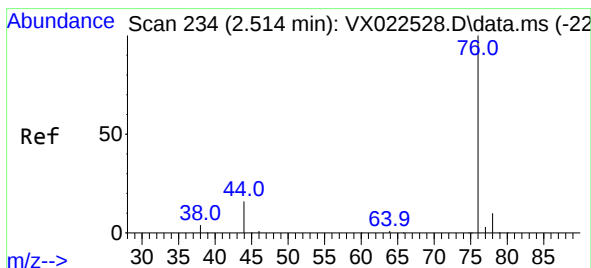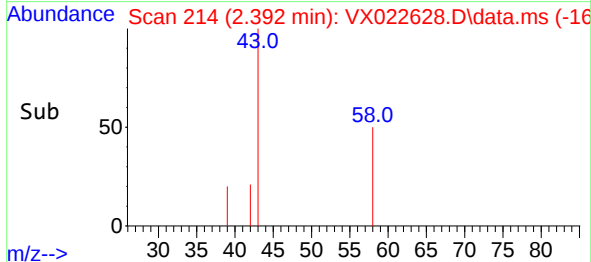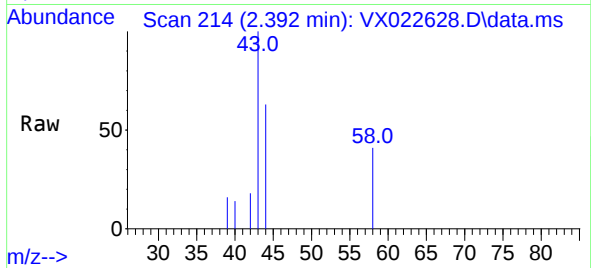

#17
Carbon Disulfide
Concen: 3.79 ug/l
RT: 2.532 min Scan# 237
Delta R.T. 0.018 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 76 Resp: 754
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

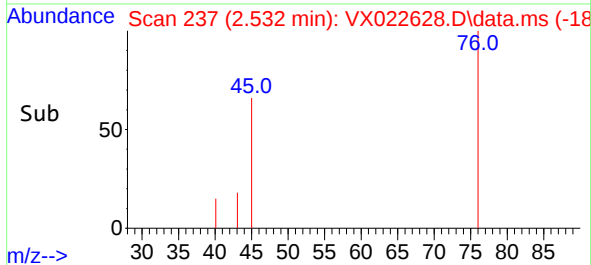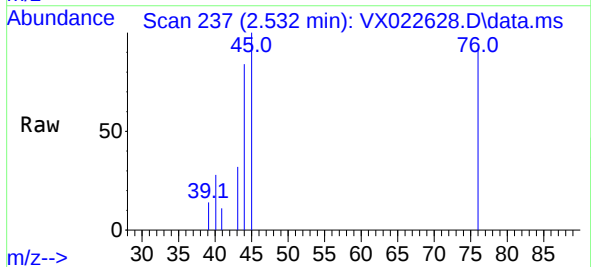







#20
Methylene Chloride
Concen: 0.40 ug/l
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Instrument :
MSVOA_X
ClientSampled :
W-8

Tgt Ion: 84 Resp: 364




Ion	Ratio	Lower	Upper
84	100		
49	67.9	88.6	132.8#
51	22.8	27.0	40.6#
86	42.3	50.3	75.5#




#27
cis-1,2-Dichloroethene
Concen: 1.46 ug/l
RT: 4.495 min Scan# 559
Delta R.T. 0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 96 Resp: 1343

Ion	Ratio	Lower	Upper
96	100		
61	120.3	0.0	285.6
98	59.3	0.0	129.6

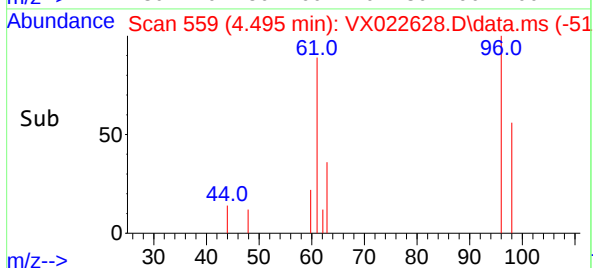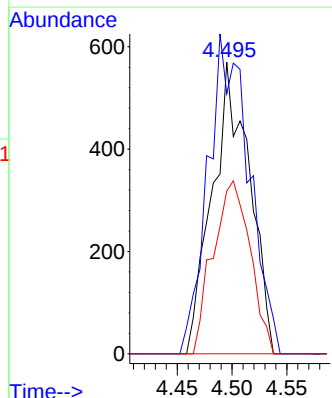



#29

Tetrahydrofuran

Concen: 0.20 ug/l

RT: 5.032 min Scan# 647

Delta R.T. 0.019 min

Lab File: VX022628.D

Acq: 09 Jun 2021 20:49





Tgt Ion: 42 Resp: 87

Ion Ratio Lower Upper

42 100

72 0.0 41.7 62.5#

71 0.0 38.4 57.6#

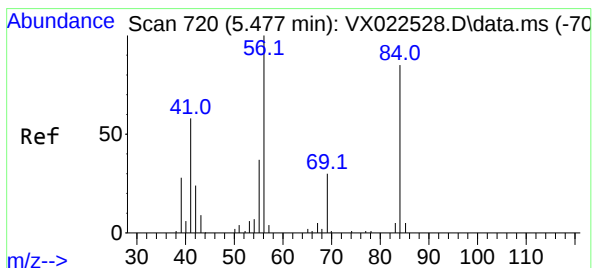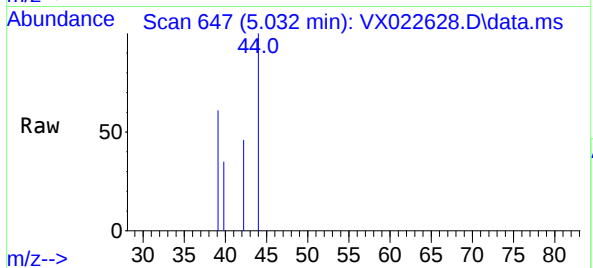

#31

Cyclohexane

Concen: 1.33 ug/l

RT: 5.471 min Scan# 719

Delta R.T. -0.006 min

Lab File: VX022628.D

Acq: 09 Jun 2021 20:49




Tgt Ion: 56 Resp: 1544


Ion Ratio Lower Upper

56 100

69 22.8 25.3 37.9#

84 68.8 71.4 107.0#

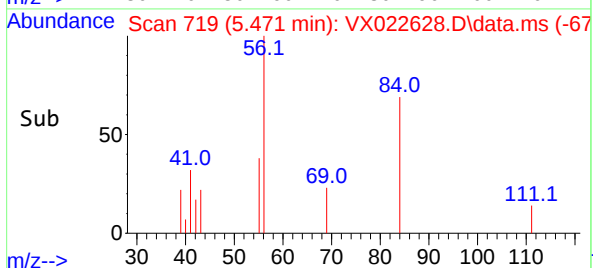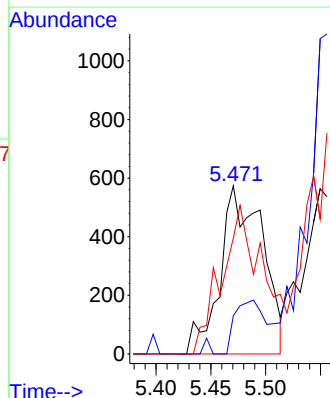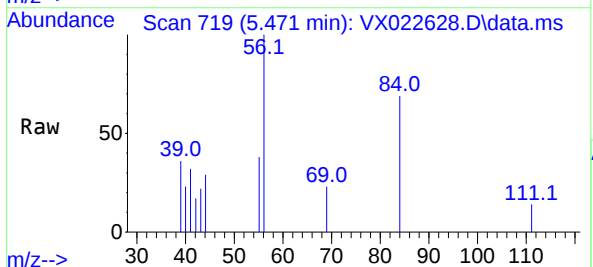







#33

1,2-Dichloroethane-d4
Concen: 48.47 ug/l
RT: 5.970 min Scan# 801
Delta R.T. 0.006 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Instrument :
MSVOA_X
ClientSampled :
W-8




Tgt Ion: 65 Resp: 47404
Ion Ratio Lower Upper
65 100
67 51.9 0.0 105.4




#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 114 Resp: 109090
Ion Ratio Lower Upper
114 100
63 22.4 0.0 40.8
88 18.8 0.0 32.8


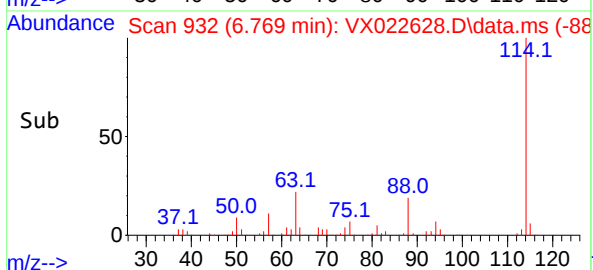




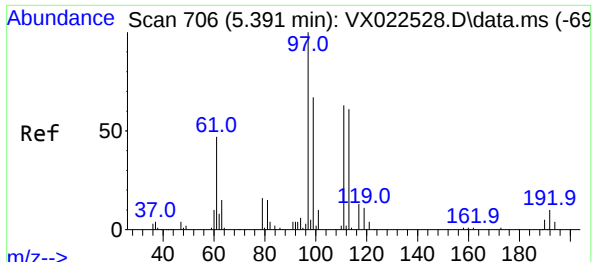

#35
Dibromofluoromethane
Concen: 49.86 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion:113 Resp: 34031
Ion Ratio Lower Upper
113 100
111 100.5 81.9 122.9
192 14.5 16.7 25.1#

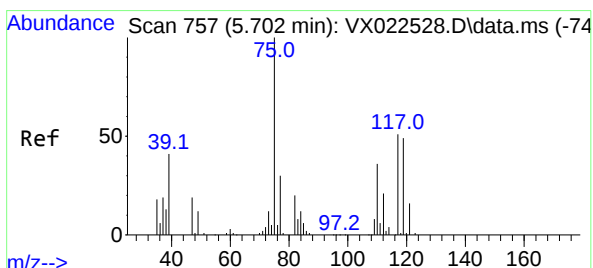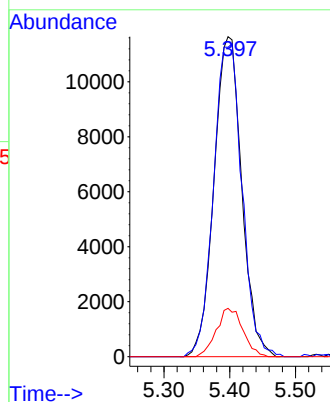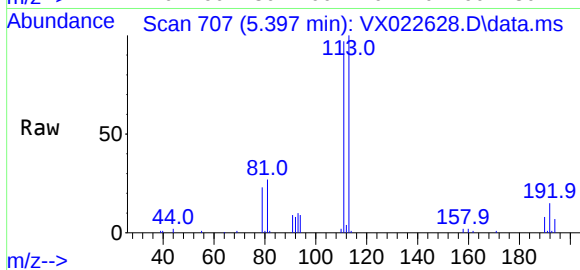

#36
1,1-Dichloropropene
Concen: 5.13 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49


Tgt Ion: 75 Resp: 5417
Ion Ratio Lower Upper
75 100
110 9.8 18.1 54.4#
77 0.0 25.3 37.9#

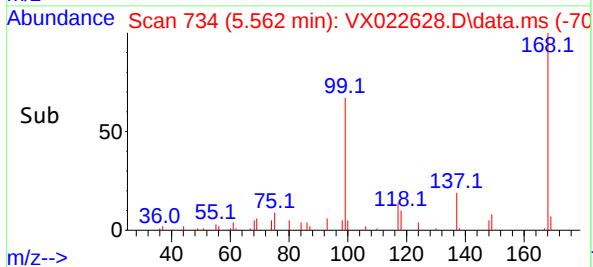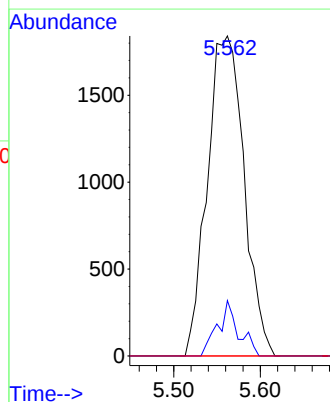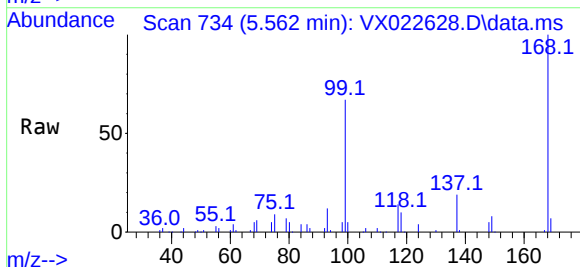






#38
Carbon Tetrachloride
Concen: 8.45 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.116 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Instrument :
MSVOA_X
ClientSampled :
W-8



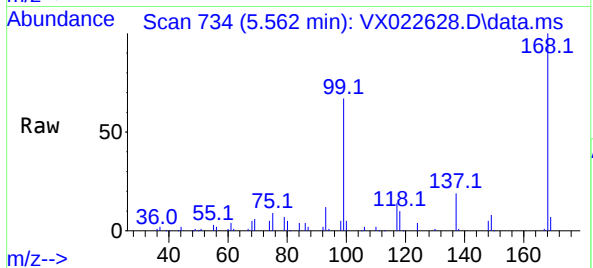



Tgt Ion:117 Resp: 6520
Ion Ratio Lower Upper
117 100
119 3.1 76.2 114.2#
121 0.0 24.8 37.2#

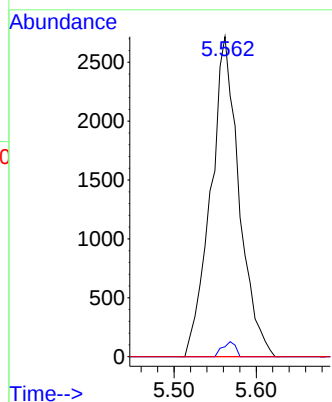

#39
Methylcyclohexane
Concen: 3.77 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 83 Resp: 2359
Ion Ratio Lower Upper
83 100
55 92.6 58.9 88.3#
98 41.1 38.1 57.1


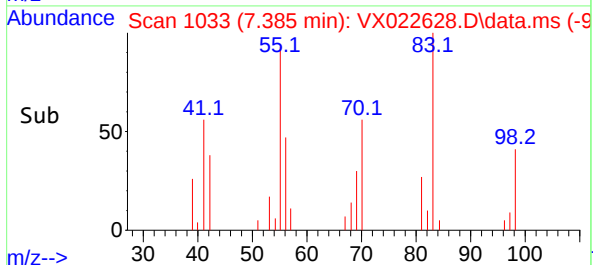

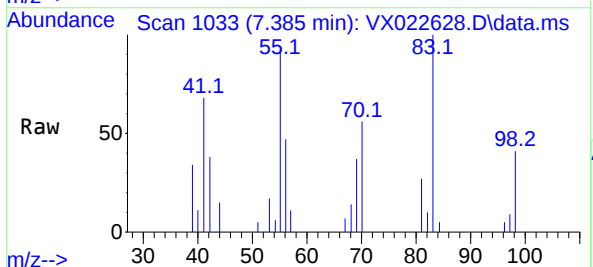




#40
Benzene
Concen: 0.29 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.006 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion: 78 Resp: 945
Ion Ratio Lower Upper
78 100
77 31.3 18.9 28.3#

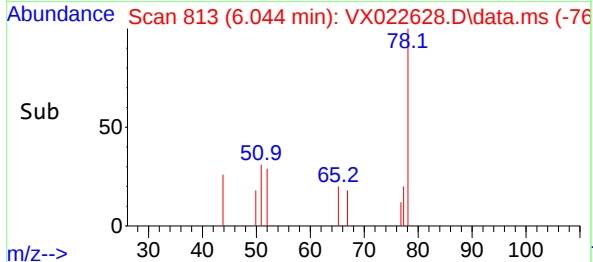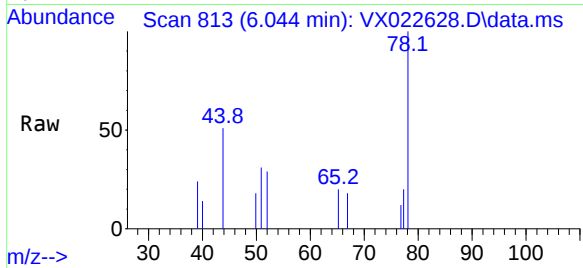

#47
Bromodichloromethane
Concen: 2.50 ug/l
RT: 7.891 min Scan# 1116
Delta R.T. 0.061 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 83 Resp: 64
Ion Ratio Lower Upper
83 100
85 0.0 51.4 77.0#
127 0.0 6.8 10.2#


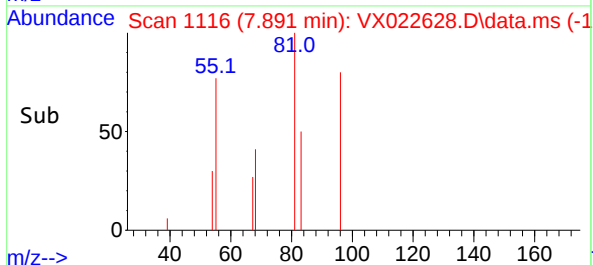
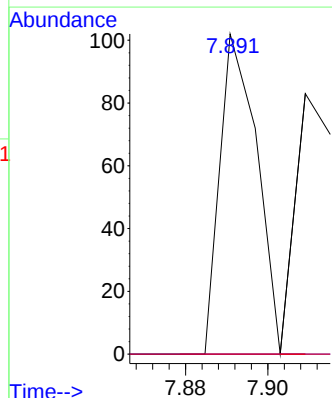
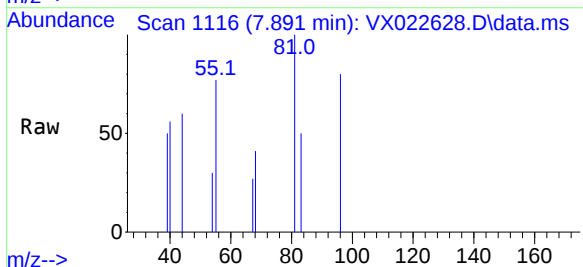




#50
Toluene-d8
Concen: 49.84 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion: 98 Resp: 135745
Ion Ratio Lower Upper
98 100
100 67.3 51.9 77.9

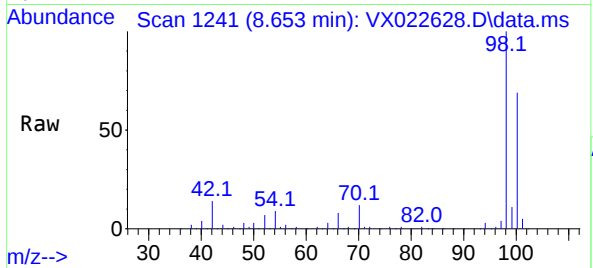

#52
Toluene
Concen: 0.23 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 92 Resp: 474
Ion Ratio Lower Upper
92 100
91 177.8 137.1 205.7


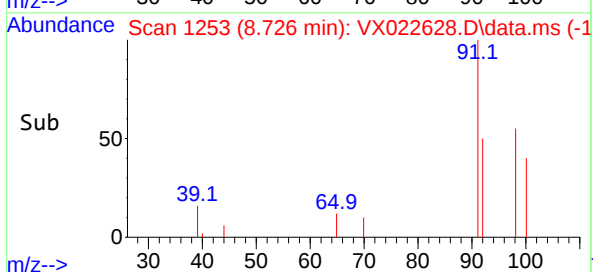






#55
1,1,2-Trichloroethane
Concen: 1.31 ug/l
RT: 9.098 min Scan# 1314
Delta R.T. -0.061 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion:	97	Resp:	1044
Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.3	103.9#
85	0.0	44.3	66.5#
99	0.0	50.3	75.5#

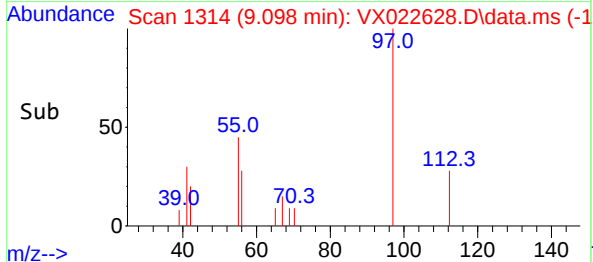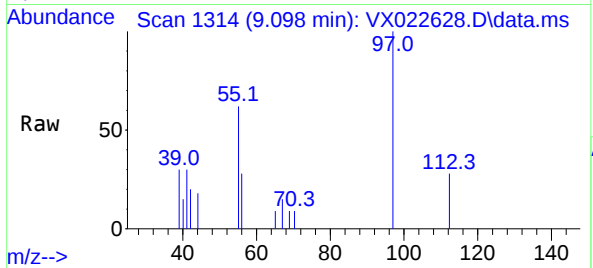

#56
Ethyl methacrylate
Concen: 2.81 ug/l
RT: 9.110 min Scan# 1316
Delta R.T. -0.012 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion:	69	Resp:	164
Ion	Ratio	Lower	Upper
69	100		
41	267.1	46.8	70.2#
39	225.0	24.7	37.1#


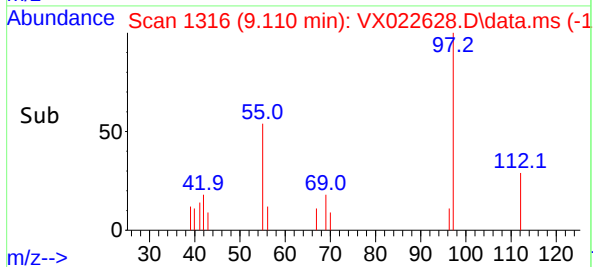

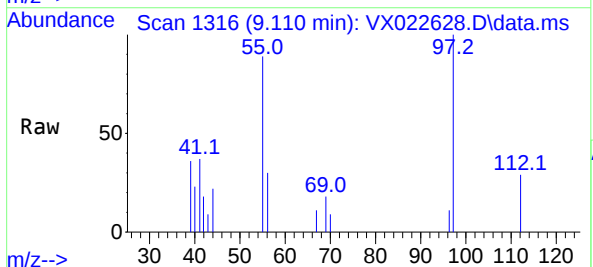




#62
4-Bromofluorobenzene
Concen: 46.46 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampleId :
W-8


Tgt Ion: 95 Resp: 47028
Ion Ratio Lower Upper
95 100
174 60.8 0.0 154.6
176 56.9 0.0 155.8

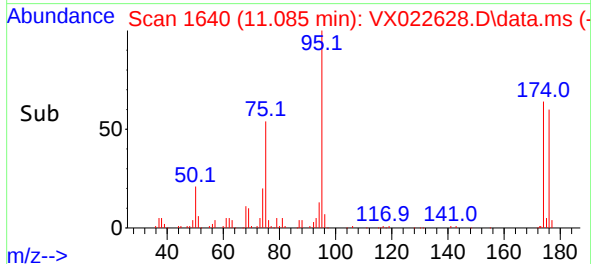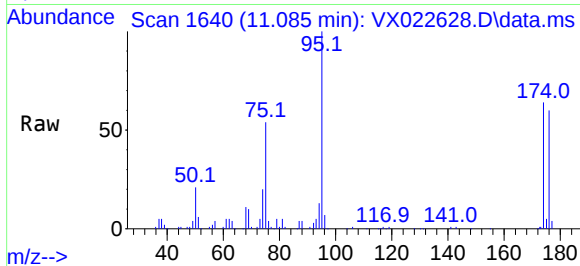

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 117 Resp: 97120
Ion Ratio Lower Upper
117 100
82 62.1 47.4 71.2
119 32.6 26.6 39.8


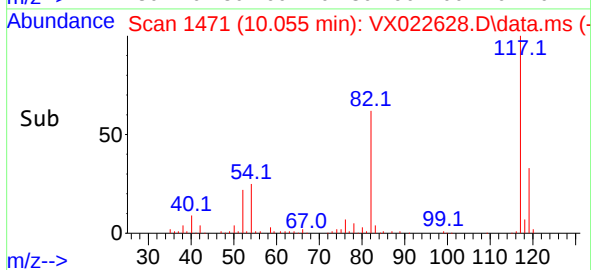

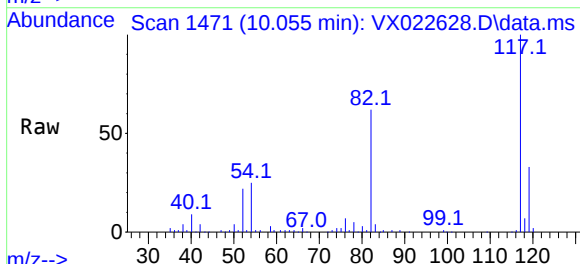




#67
Ethyl Benzene
Concen: 0.55 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion: 91 Resp: 2026
Ion Ratio Lower Upper
91 100
106 21.5 24.6 37.0#

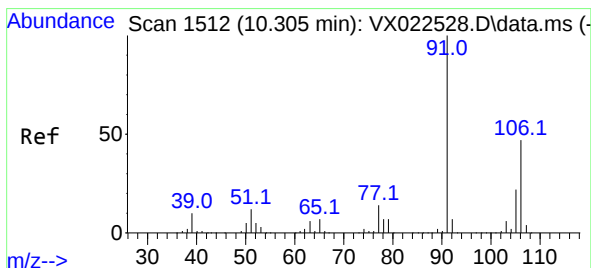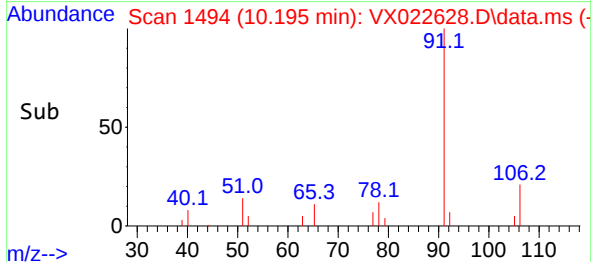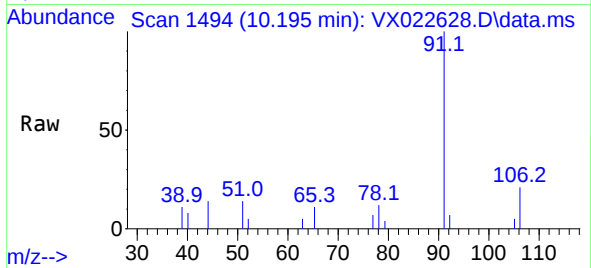

#68
m/p-Xylenes
Concen: 0.71 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion:106 Resp: 959
Ion Ratio Lower Upper
106 100
91 197.5 162.8 244.2


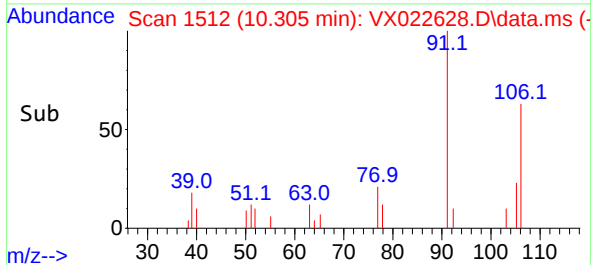

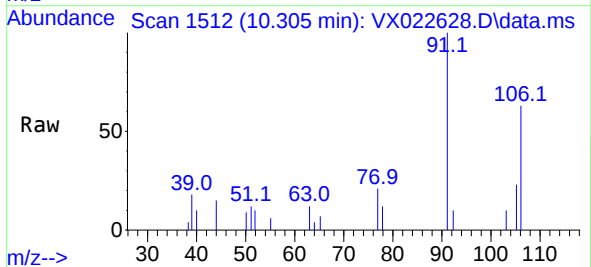




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion:152 Resp: 36555
Ion Ratio Lower Upper
152 100
115 67.4 41.1 123.3
150 158.9 0.0 349.0

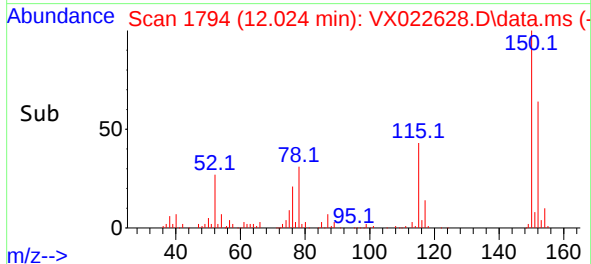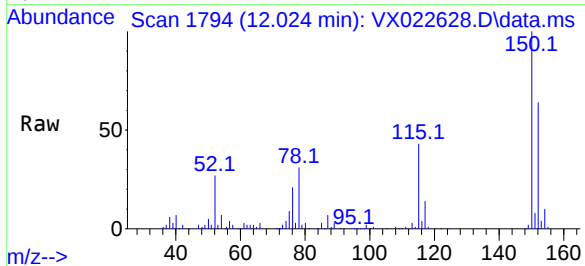

#73
Isopropylbenzene
Concen: 3.43 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion:105 Resp: 10226
Ion Ratio Lower Upper
105 100
120 26.9 13.2 39.6


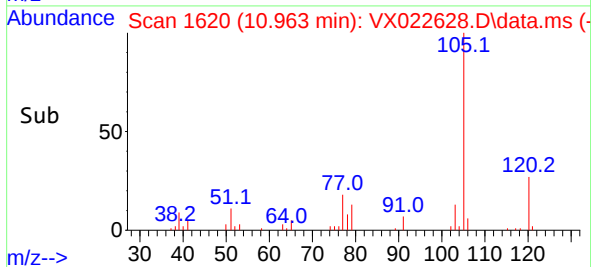

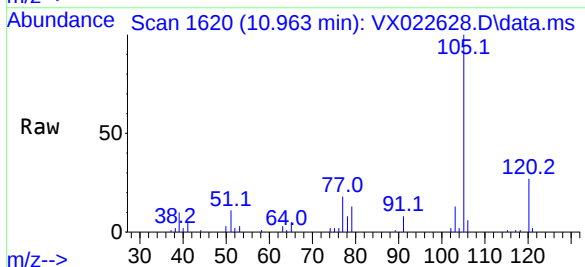




#76
1,2,3-Trichloropropane
Concen: 26.88 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion: 75 Resp: 25460
Ion Ratio Lower Upper
75 100
77 1.5 19.1 57.5#

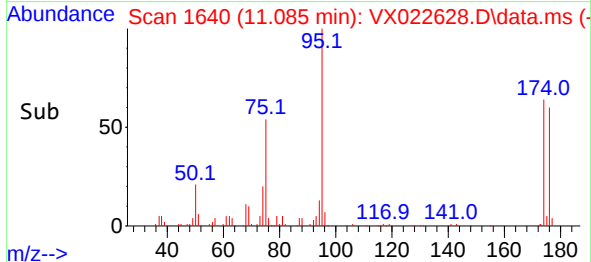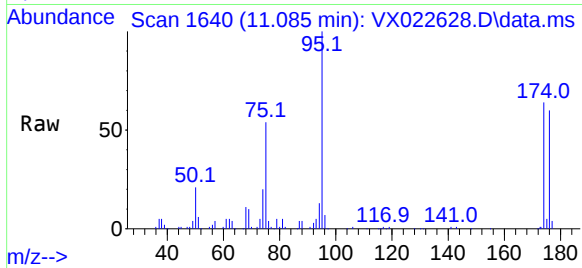

#78
n-propylbenzene
Concen: 3.81 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 91 Resp: 13791
Ion Ratio Lower Upper
91 100
120 22.0 11.5 34.5


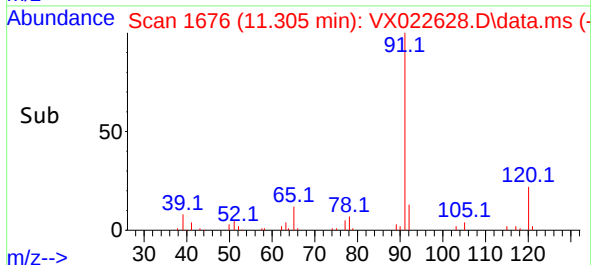
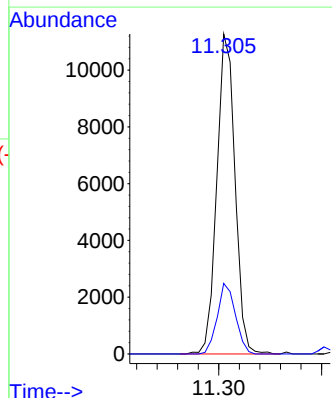
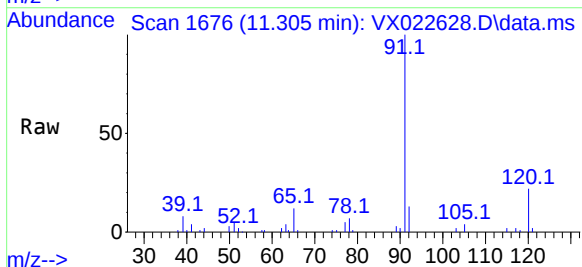




#79
2-Chlorotoluene
Concen: 6.41 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.061 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion: 91 Resp: 13791
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#

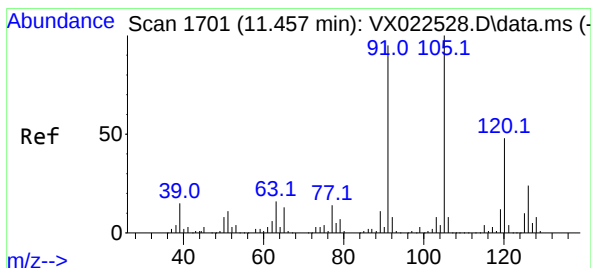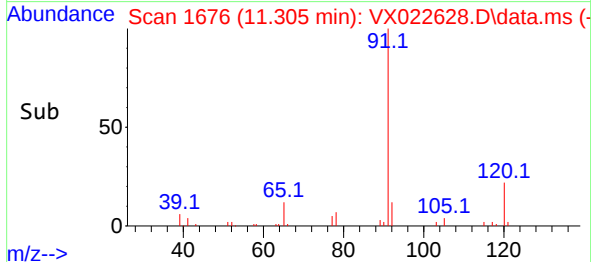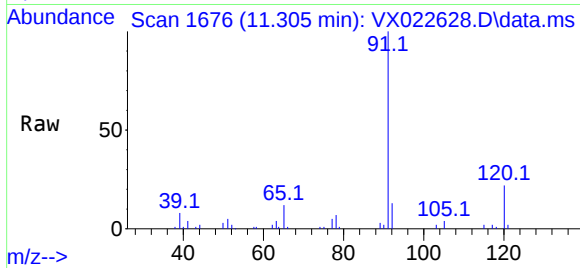

#80
1,3,5-Trimethylbenzene
Concen: 0.78 ug/l
RT: 11.616 min Scan# 1727
Delta R.T. 0.159 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 105 Resp: 1980
Ion Ratio Lower Upper
105 100
120 35.0 23.8 71.5


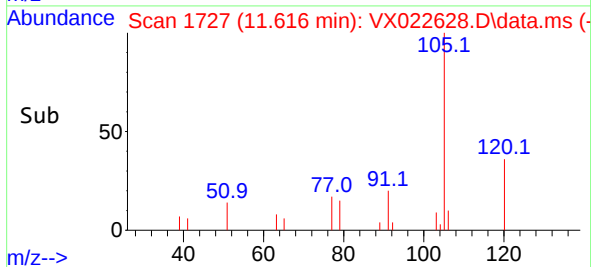

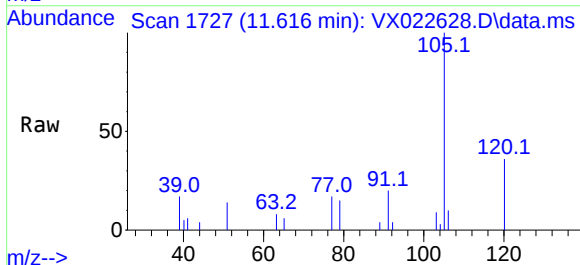




#81
trans-1,4-Dichloro-2-butene
Concen: 66.09 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion: 75 Resp: 25460
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

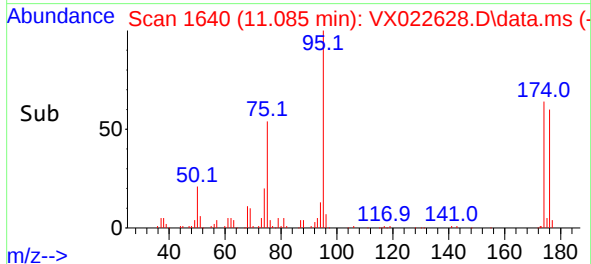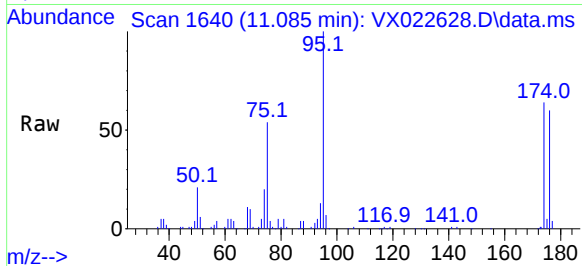

#82
4-Chlorotoluene
Concen: 5.54 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.152 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 91 Resp: 13791
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


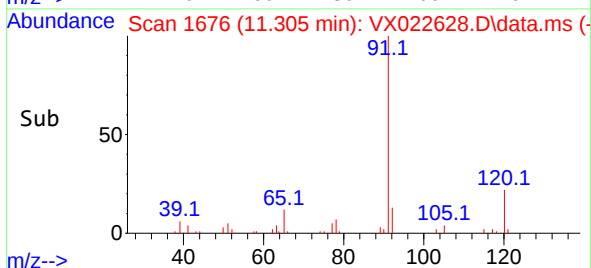
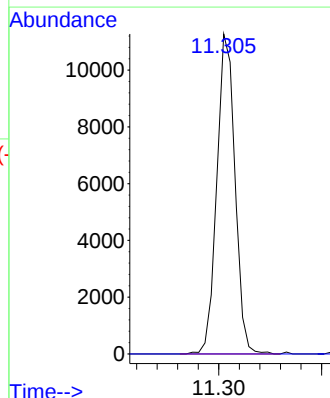
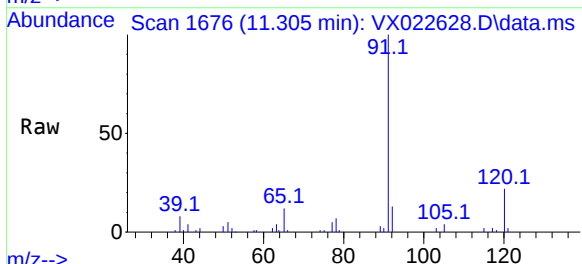




#85
sec-Butylbenzene
Concen: 0.71 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. -0.006 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion:105 Resp: 2143
Ion Ratio Lower Upper
105 100
134 15.2 10.0 29.8

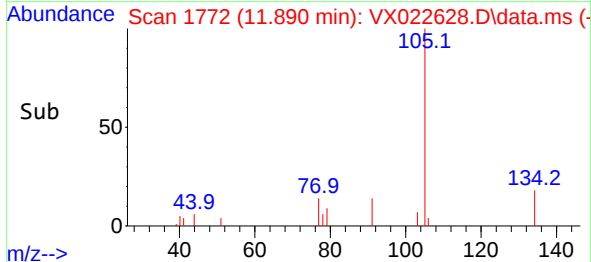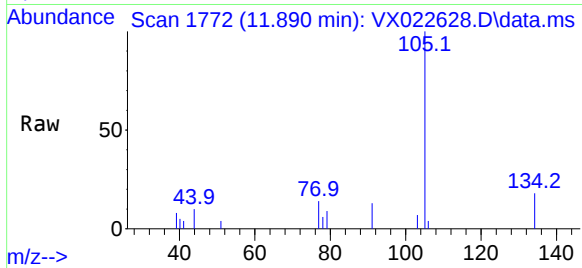

#86
p-Isopropyltoluene
Concen: 0.35 ug/l
RT: 12.183 min Scan# 1820
Delta R.T. 0.171 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion:119 Resp: 881
Ion Ratio Lower Upper
119 100
134 33.7 12.9 38.7
91 38.0 11.7 35.0#


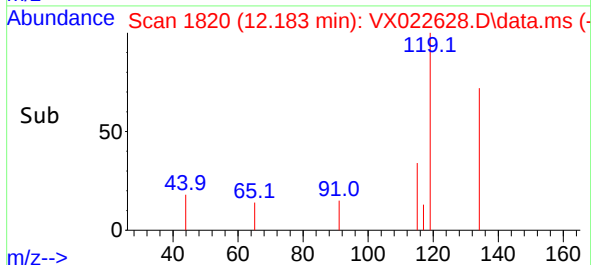
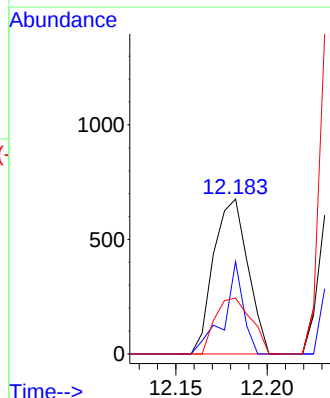
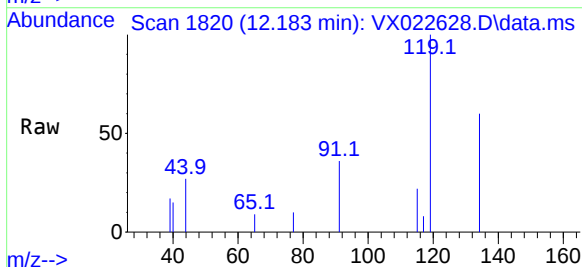


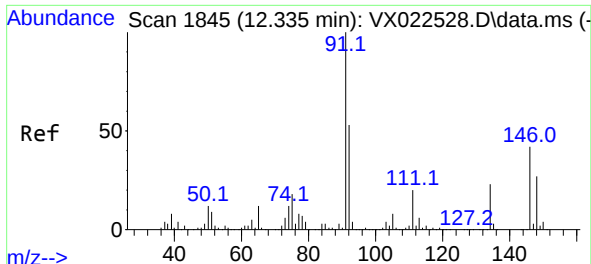

#89
n-Butylbenzene
Concen: 0.89 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49




Instrument :
MSVOA_X
ClientSampled :
W-8


Tgt Ion: 91 Resp: 2143
Ion Ratio Lower Upper
91 100
92 30.0 27.4 82.0
134 62.8 13.2 39.5#

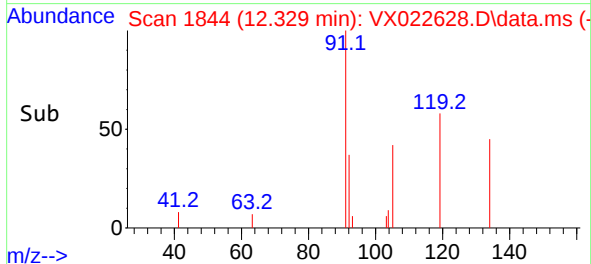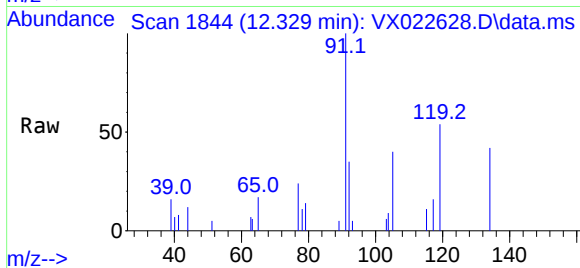

#90
Hexachloroethane
Concen: 11.90 ug/l
RT: 12.646 min Scan# 1896
Delta R.T. 0.104 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion: 117 Resp: 3775
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#


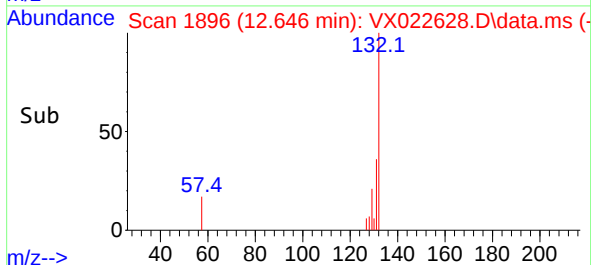
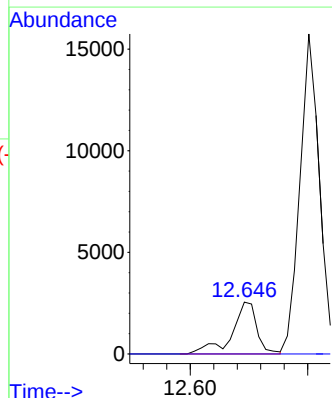
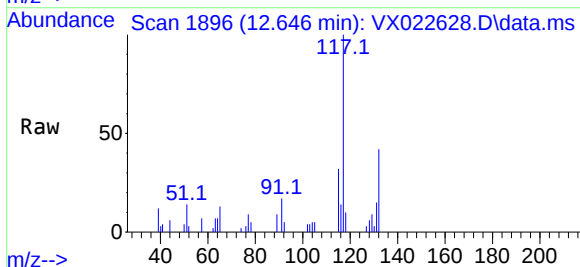


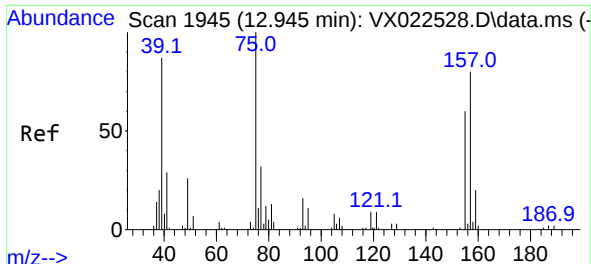

#92
1,2-Dibromo-3-Chloropropane
Concen: 4.60 ug/l
RT: 12.927 min Scan# 1942
Delta R.T. -0.018 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Instrument :
MSVOA_X
ClientSampled :
W-8

Tgt Ion: 75 Resp: 252
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

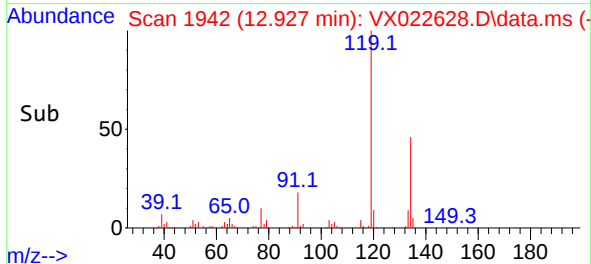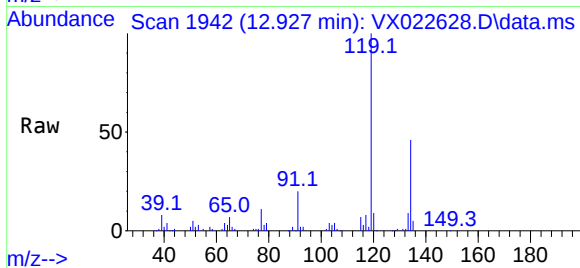

#95
Naphthalene
Concen: 0.23 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX022628.D
Acq: 09 Jun 2021 20:49

Tgt Ion:128 Resp: 663
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 6.8 8.8 13.2#

